

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071723\
 Data File : BP016274.D
 Acq On : 18 Jul 2023 02:54
 Operator : MA/JU
 Sample : 03477-06
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 HOA44

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP016274.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.240	4	9	18	rBV	1092732	1831445	7.31%	2.199%
2	3.311	18	21	41	rVB	699028	1136139	4.53%	1.364%
3	3.752	93	96	113	rBV	126559	341583	1.36%	0.410%
4	3.940	125	128	134	rVB2	19741	33433	0.13%	0.040%
5	4.581	231	237	265	rBV	13106635	25060190	100.00%	30.092%
6	7.205	676	683	693	rBV3	56665	199866	0.80%	0.240%
7	7.299	693	699	723	rVB	325990	977964	3.90%	1.174%
8	7.516	730	736	763	rVB	295071	919096	3.67%	1.104%
9	7.858	789	794	805	rVB6	12148	29913	0.12%	0.036%
10	7.963	805	812	837	rBV	315990	1011239	4.04%	1.214%
11	8.346	871	877	890	rVB5	23365	69802	0.28%	0.084%
12	8.728	936	942	969	rBV	184527	788828	3.15%	0.947%
13	9.163	1010	1016	1046	rBV	437294	1295773	5.17%	1.556%
14	9.899	1133	1141	1164	rBV	268526	1044609	4.17%	1.254%
15	10.487	1233	1241	1274	rBV2	266719	1445214	5.77%	1.735%
16	10.781	1284	1291	1311	rVB	698979	1704673	6.80%	2.047%
17	10.993	1319	1327	1367	rBV	264523	1325293	5.29%	1.591%
18	13.493	1746	1752	1759	rBV	19698	39057	0.16%	0.047%
19	14.034	1837	1844	1871	rBV	1221960	2703922	10.79%	3.247%
20	14.310	1884	1891	1912	rBV	1788313	3130969	12.49%	3.760%
21	14.610	1934	1942	1968	rBV	1514388	2527126	10.08%	3.035%
22	15.104	2019	2026	2030	rBV9	14524	42483	0.17%	0.051%
23	15.616	2107	2113	2135	rBV	1803170	4262371	17.01%	5.118%
24	15.816	2141	2147	2172	rBV2	276191	1138826	4.54%	1.368%
25	17.375	2406	2412	2424	rBV	2089828	3259490	13.01%	3.914%
26	17.481	2424	2430	2456	rVB2	2086503	4845576	19.34%	5.819%
27	18.239	2555	2559	2569	rBV9	28426	78124	0.31%	0.094%
28	18.316	2569	2572	2576	rVV	23701	27622	0.11%	0.033%
29	18.369	2576	2581	2600	rVV	283338	588469	2.35%	0.707%
30	19.292	2734	2738	2744	rBV3	50091	68965	0.28%	0.083%
31	19.375	2748	2752	2759	rVV	46881	76970	0.31%	0.092%
32	19.469	2765	2768	2774	rBV5	29307	47373	0.19%	0.057%
33	19.598	2787	2790	2795	rBV6	23270	30011	0.12%	0.036%
34	19.710	2803	2809	2835	rBV	3519951	6506899	25.97%	7.813%
35	21.480	3104	3110	3130	rBV2	1888099	4244368	16.94%	5.097%
36	23.792	3496	3503	3524	rVB2	2666066	6332899	25.27%	7.605%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071723\
Data File : BP016274.D
Acq On : 18 Jul 2023 02:54
Operator : MA/JU
Sample : 03477-06
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
HOA44

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
Title : SVOA CALIBRATION

37	23.963	3525	3532	3558	rVB	1360285	4111170	16.41%	4.937%
----	--------	------	------	------	-----	---------	---------	--------	--------




Sum of corrected areas: 83277750

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071723\
Data File : BP016274.D
Acq On : 18 Jul 2023 02:54
Operator : MA/JU
Sample : 03477-06
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
HOA44

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

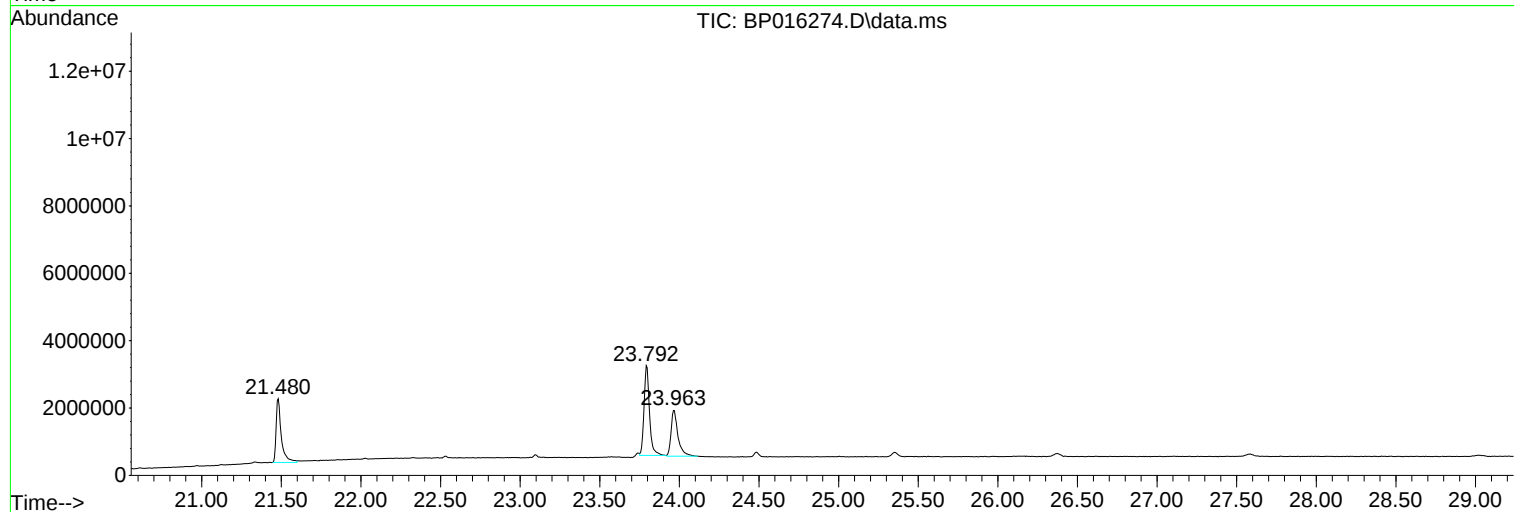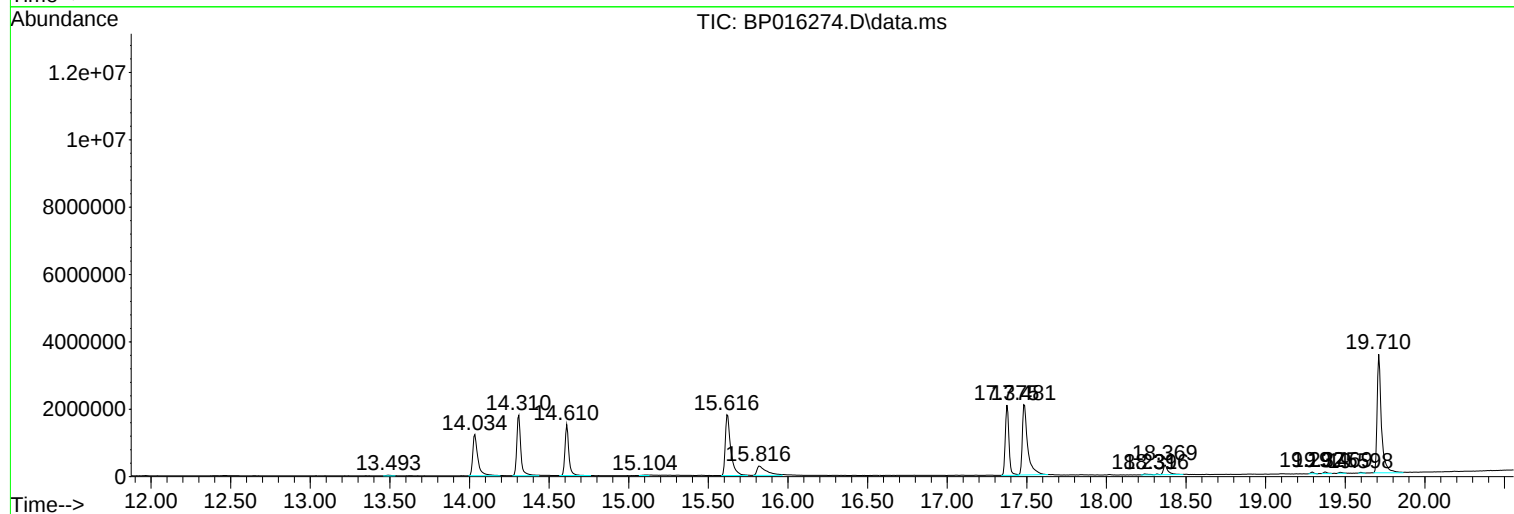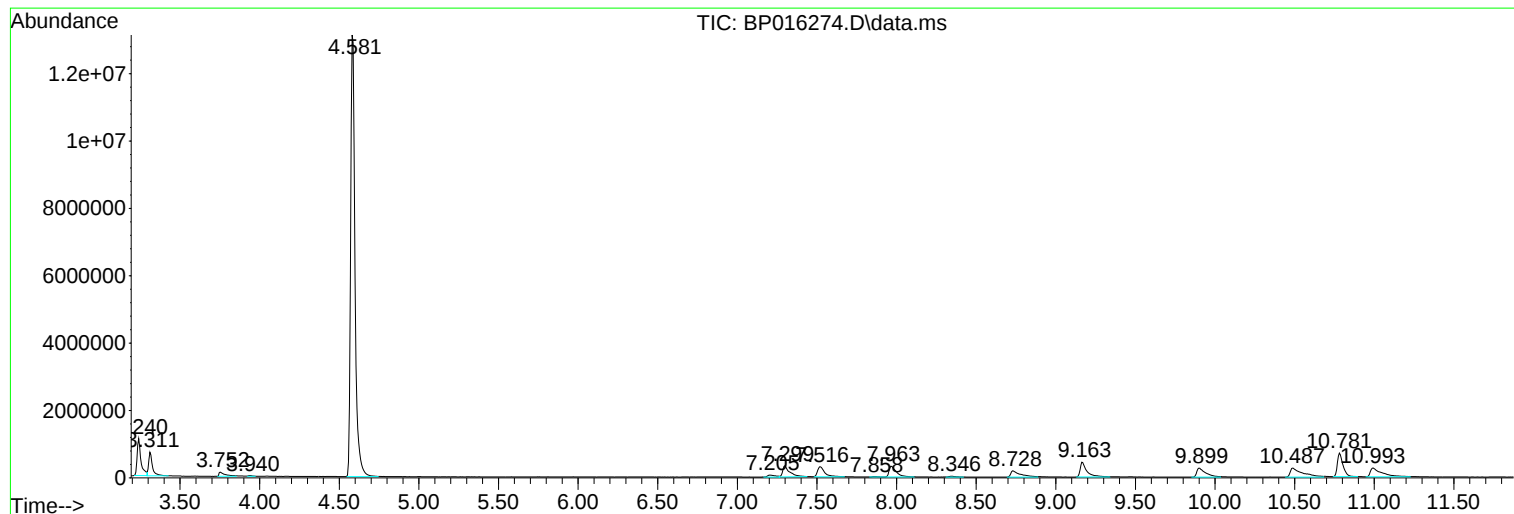

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071723\
Data File : BP016274.D
Acq On : 18 Jul 2023 02:54
Operator : MA/JU
Sample : 03477-06
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
HOA44










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Bromacil Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
18.369	3.61 ng/ul	588469	Phenanthrene-d10	17.375

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Bromacil	260	C9H13BrN2O2	000314-40-9	91
2			Bromacil	260	C9H13BrN2O2	000314-40-9	90
3			2-Amino-4-bromo-5-fluorophenol	205	C6H5BrFNO	1016234-89-1	50
4			5-Acetamido-2,4-dichlorobenzoic ...	247	C9H7Cl2NO3	050602-49-8	42
5			2-Amino-4-bromo-5-fluorophenol, ...	331	C12H11BrFN04	1000497-81-4	42

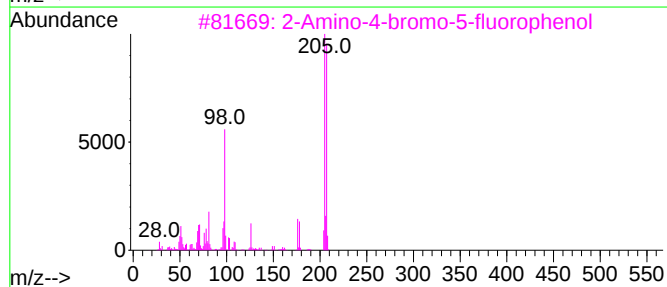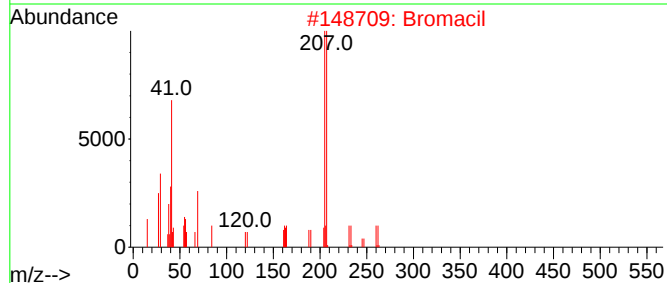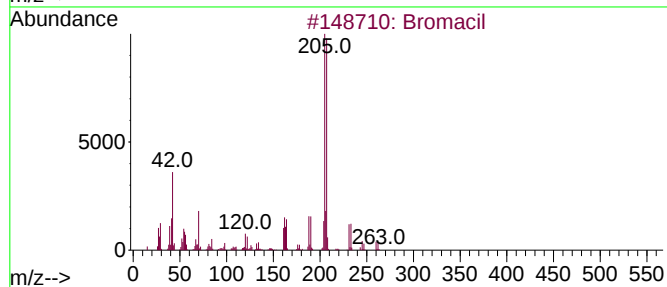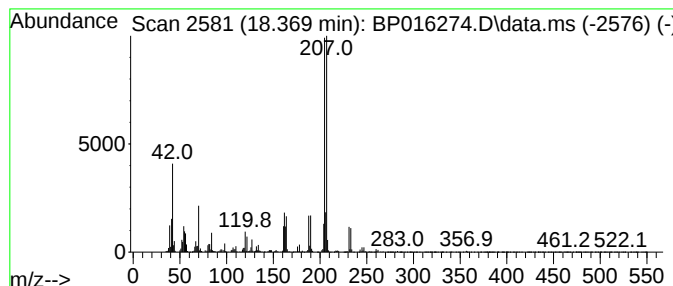

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071723\
Data File : BP016274.D
Acq On : 18 Jul 2023 02:54
Operator : MA/JU
Sample : 03477-06
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
HOA44

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Bromacil	18.369	3.6	ng/ul	588469	4	17.375	3259490	20.0