




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071822\
 Data File : BP010993.D
 Acq On : 18 Jul 2022 15:18
 Operator : CG/JU
 Sample : N3748-07
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH0E9

Manual IntegrationsAPPROVED

Quant Time: Jul 18 15:43:51 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jul 14 15:34:34 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/19/2022
 Supervised By :mohammad ahmed 07/20/2022

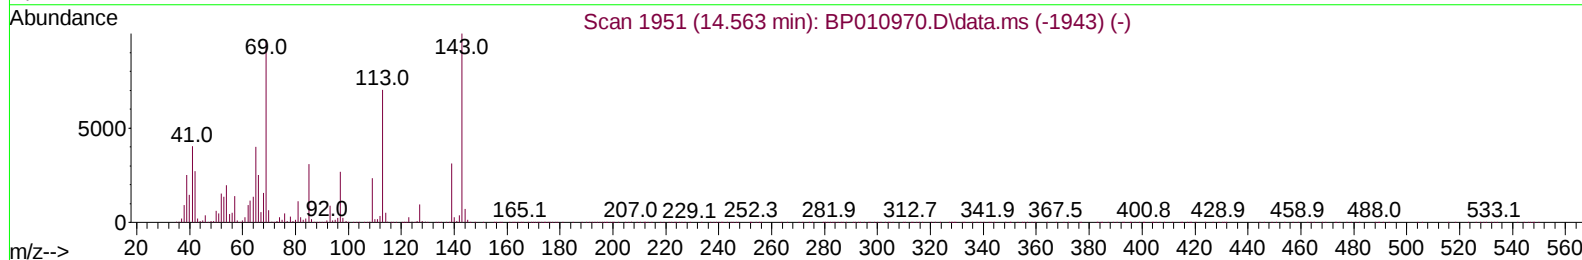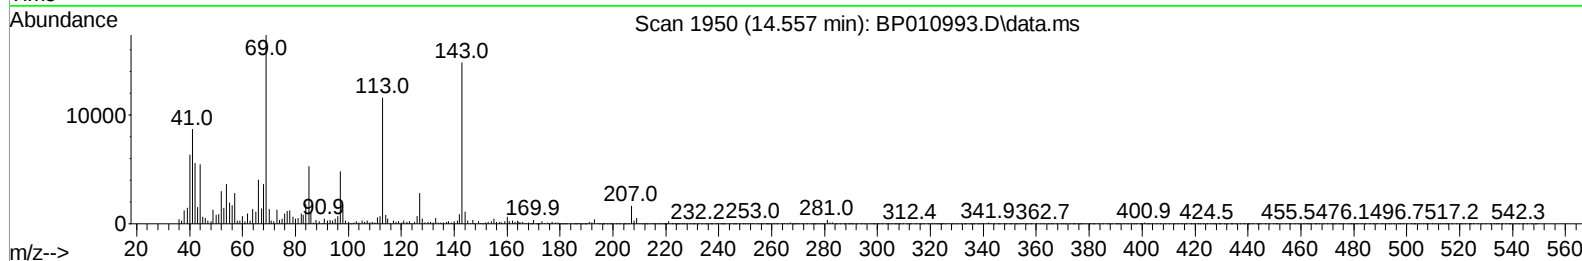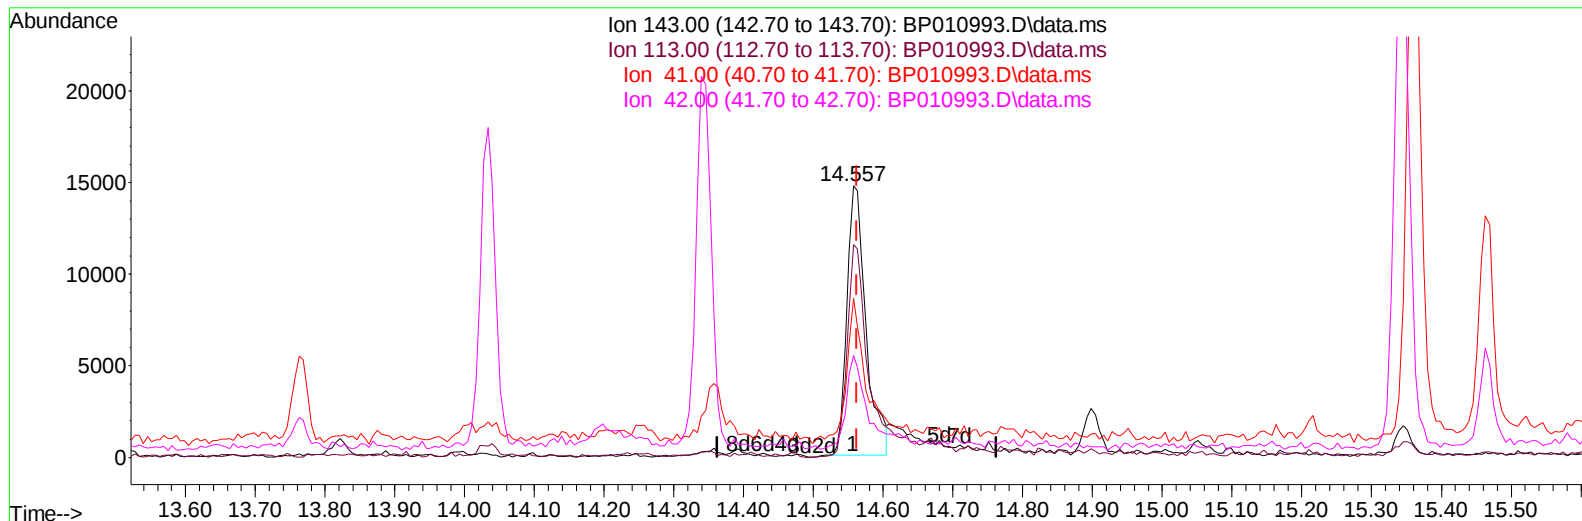

TIC: BP010993.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.557min (-0.006) 2.22 ng/u1

response 28109

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	94.50	78.29
41.00	59.00	58.66
42.00	41.10	37.72




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071822\
Data File : BP010993.D
Acq On : 18 Jul 2022 15:18
Operator : CG/JU
Sample : N3748-07
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH0E9

Manual IntegrationsAPPROVED

Quant Time: Jul 18 15:43:51 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jul 14 15:34:34 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/19/2022
Supervised By :mohammad ahmed 07/20/2022

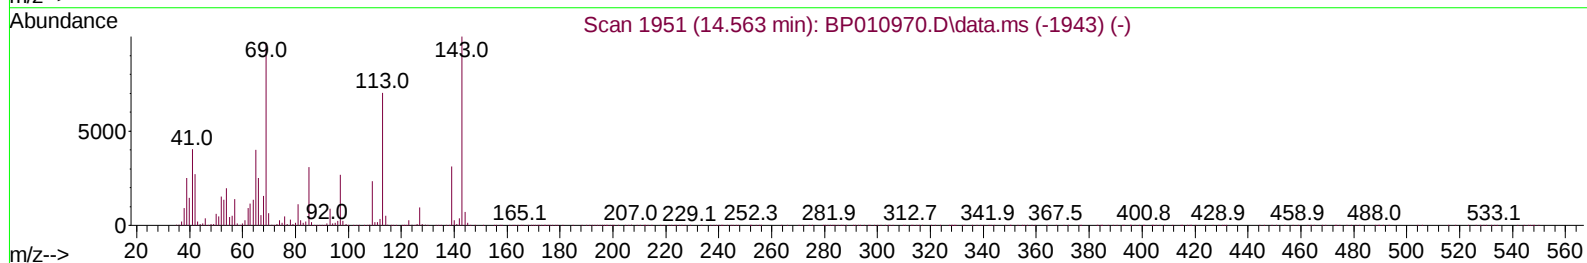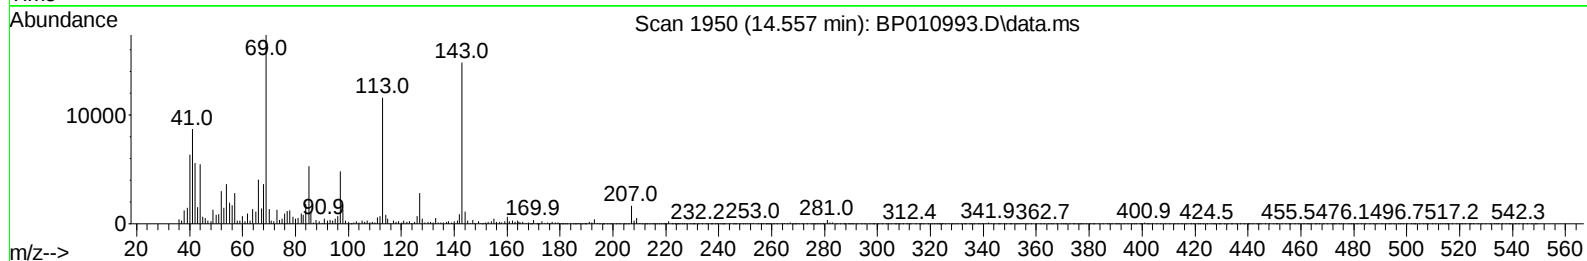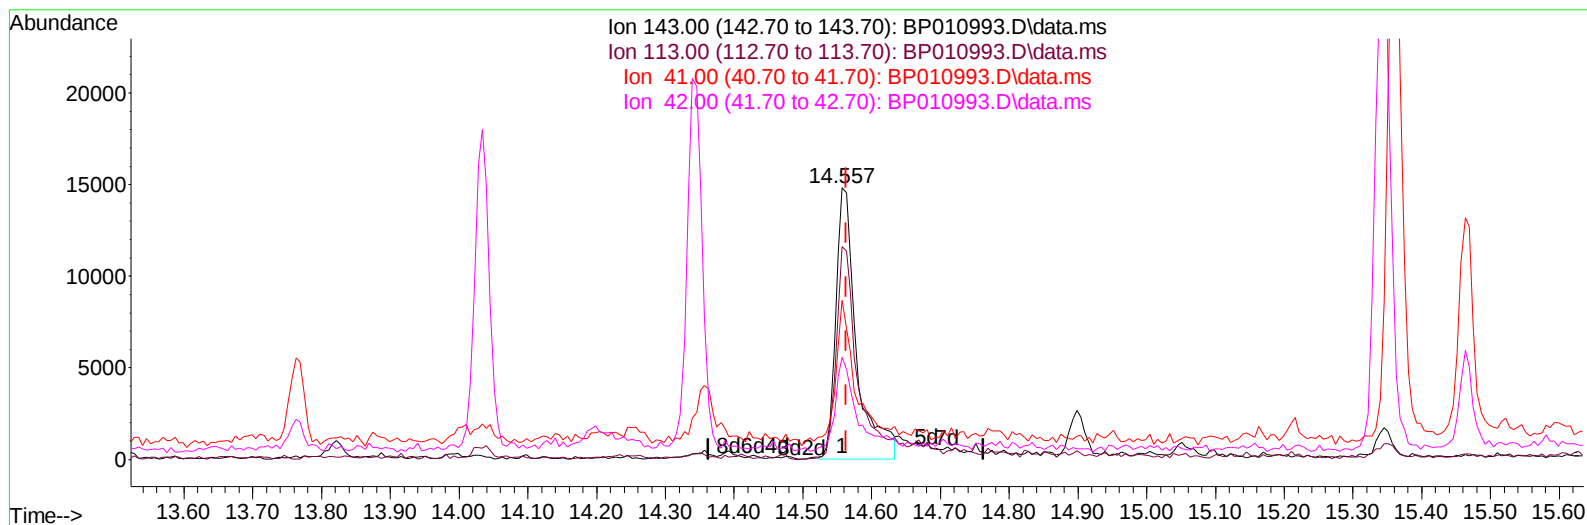

TIC: BP010993.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.557min (-0.006) 2.48 ng/ul m

response 31393

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	94.50	78.29
41.00	59.00	58.66
42.00	41.10	37.72

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071822\
 Data File : BP010993.D
 Acq On : 18 Jul 2022 15:18
 Operator : CG/JU
 Sample : N3748-07
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH0E9

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 07/19/2022
 Supervised By :mohammad ahmed 07/20/2022

Quant Time: Jul 18 15:43:51 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jul 14 15:34:34 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.681	152	428190	20.000	ng/ul	0.00
20) Naphthalene-d8	10.475	136	1801469	20.000	ng/ul	# 0.00
38) Acenaphthene-d10	14.345	164	916599	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.110	188	1547143	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.227	240	1481550	20.000	ng/ul	#-0.01
88) Perylene-d12	23.586	264	1681055	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.181	96	47978	4.039	ng/uL	0.00
4) Pyridine-d5	3.593	84	218742	7.125	ng/ul	0.00
7) Phenol-d5	6.857	99	181664	5.168	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.022	67	647653	28.655	ng/ul	0.00
11) 2-Chlorophenol-d4	7.216	132	612217	21.556	ng/ul	0.00
15) 4-Methylphenol-d8	8.399	113	345959	12.295	ng/ul	0.00
21) Nitrobenzene-d5	8.846	128	357173	27.207	ng/ul	0.00
24) 2-Nitrophenol-d4	9.563	143	328127	25.259	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.098	165	531828	22.387	ng/ul	0.00
31) 4-Chloroaniline-d4	10.622	131	400825	10.234	ng/ul	0.00
46) Dimethylphthalate-d6	13.763	166	1719406	27.446	ng/ul	0.00
49) Acenaphthylene-d8	14.034	160	2116260	28.631	ng/ul	0.00
54) 4-Nitrophenol-d4	14.557	143	31393m	2.476	ng/ul	0.00
60) Fluorene-d10	15.345	176	1451172	27.252	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.469	200	151138	19.742	ng/ul	0.00
73) Anthracene-d10	17.210	188	2031407	30.885	ng/ul	0.00
81) Pyrene-d10	19.463	212	2183614	28.063	ng/ul	-0.01
92) Benzo(a)pyrene-d12	23.433	264	2554460	31.638	ng/ul	-0.02

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071822\
Data File : BP010993.D
Acq On : 18 Jul 2022 15:18
Operator : CG/JU
Sample : N3748-07
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH0E9

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 07/19/2022
Supervised By :mohammad ahmed 07/20/2022

Quant Time: Jul 18 15:43:51 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jul 14 15:34:34 2022
Response via : Initial Calibration

