




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071822\
Data File : BP010999.D
Acq On : 18 Jul 2022 18:44
Operator : CG/JU
Sample : N3753-01
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBHP4

Manual IntegrationsAPPROVED

Quant Time: Jul 19 00:46:33 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jul 14 15:34:34 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/19/2022
Supervised By :mohammad ahmed 07/20/2022

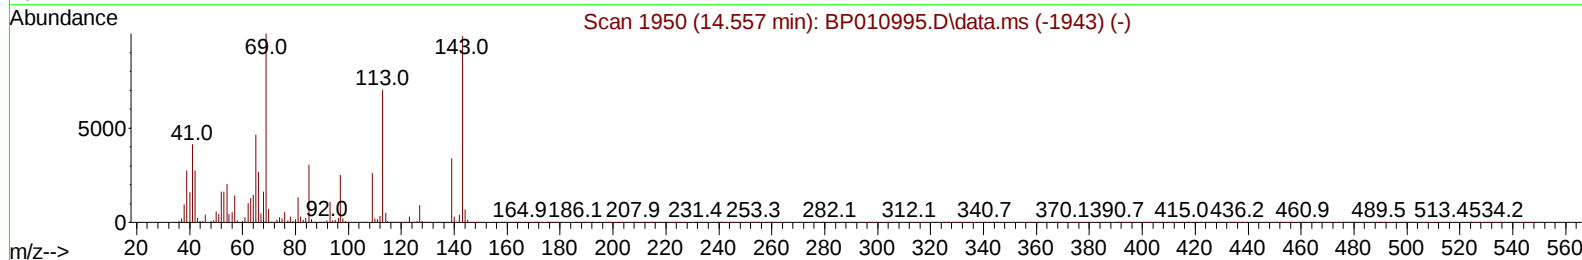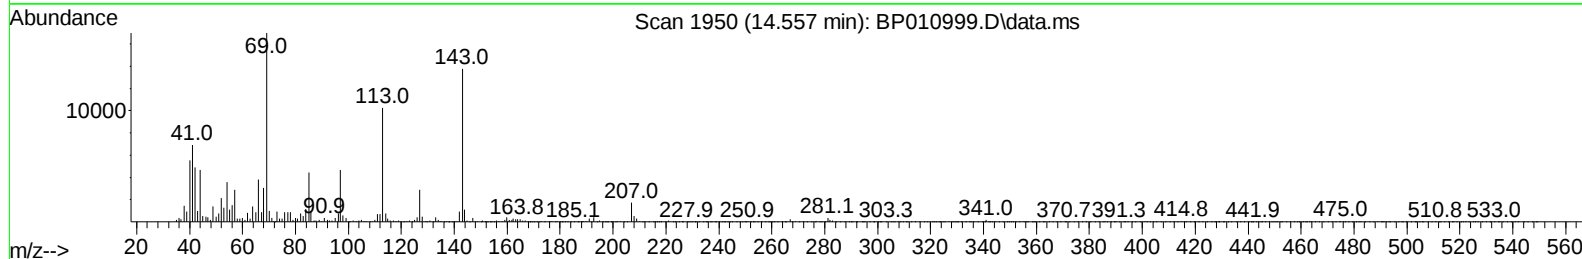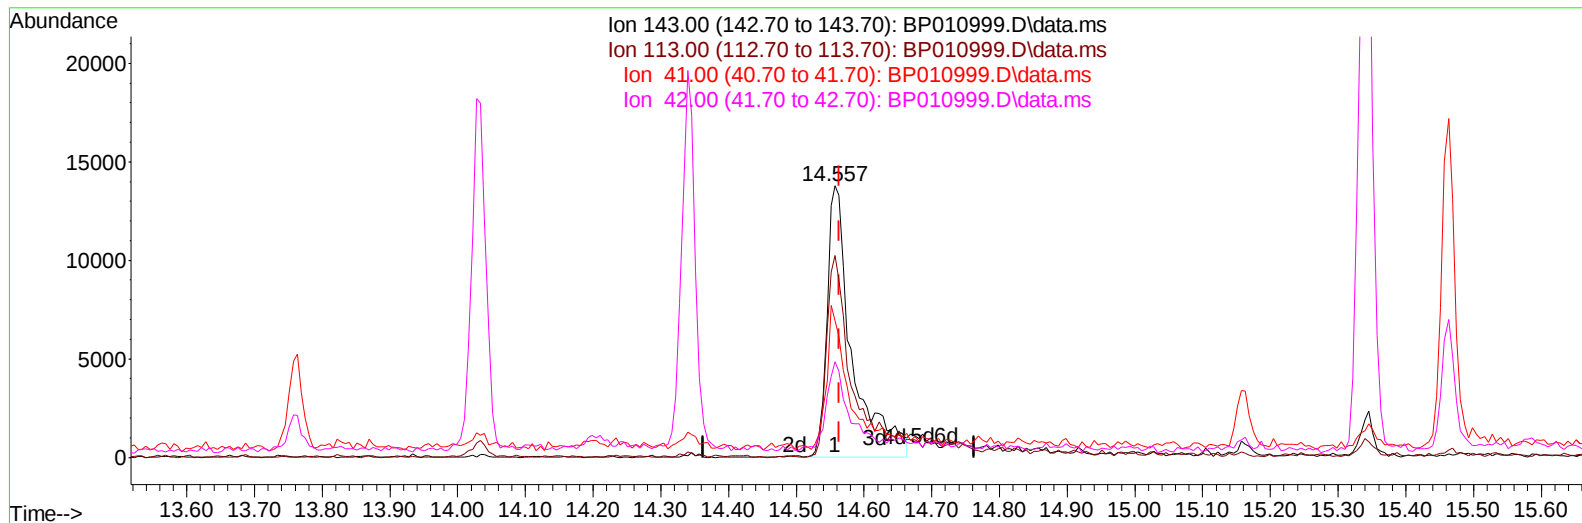

TIC: BP010999.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.557min (-0.006) 3.20 ng/ul m

response 35530

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	94.50	74.50#
41.00	59.00	50.34
42.00	41.10	35.36

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071822\
 Data File : BP010999.D
 Acq On : 18 Jul 2022 18:44
 Operator : CG/JU
 Sample : N3753-01
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GBHP4

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 07/19/2022
 Supervised By :mohammad ahmed 07/20/2022

Quant Time: Jul 19 00:46:33 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jul 14 15:34:34 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.681	152	346126	20.000	ng/ul	0.00
20) Naphthalene-d8	10.475	136	1455678	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.340	164	801743	20.000	ng/ul	-0.01
64) Phenanthrene-d10	17.110	188	1624171	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.227	240	1605403	20.000	ng/ul	#-0.01
88) Perylene-d12	23.580	264	1688516	20.000	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.181	96	48040	5.004	ng/uL	0.00
4) Pyridine-d5	3.593	84	224760	9.057	ng/ul	0.00
7) Phenol-d5	6.858	99	148788	5.237	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.022	67	562016	30.762	ng/ul	0.00
11) 2-Chlorophenol-d4	7.216	132	513262	22.357	ng/ul	0.00
15) 4-Methylphenol-d8	8.393	113	290455	12.770	ng/ul	-0.01
21) Nitrobenzene-d5	8.840	128	310521	29.272	ng/ul	0.00
24) 2-Nitrophenol-d4	9.563	143	273538	26.059	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.099	165	455070	23.706	ng/ul	0.00
31) 4-Chloroaniline-d4	10.622	131	716057	22.626	ng/ul	0.00
46) Dimethylphthalate-d6	13.763	166	1804915	32.939	ng/ul	0.00
49) Acenaphthylene-d8	14.034	160	2031866	31.427	ng/ul	0.00
54) 4-Nitrophenol-d4	14.557	143	35530m	3.204	ng/ul	0.00
60) Fluorene-d10	15.340	176	1539887	33.061	ng/ul	-0.01
65) 4,6-Dinitro-2-methylph...	15.463	200	204617	25.460	ng/ul	-0.01
73) Anthracene-d10	17.210	188	2623662	37.998	ng/ul	0.00
81) Pyrene-d10	19.463	212	3082029	36.553	ng/ul	-0.01
92) Benzo(a)pyrene-d12	23.427	264	3143787	38.765	ng/ul	-0.02

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071822\
Data File : BP010999.D
Acq On : 18 Jul 2022 18:44
Operator : CG/JU
Sample : N3753-01
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBHP4

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 07/19/2022
Supervised By :mohammad ahmed 07/20/2022

Quant Time: Jul 19 00:46:33 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jul 14 15:34:34 2022
Response via : Initial Calibration

