




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071822\
 Data File : BP011020.D
 Acq On : 19 Jul 2022 07:18
 Operator : CG/JU
 Sample : N3704-03
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AP8

Manual IntegrationsAPPROVED

Quant Time: Jul 19 07:45:14 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jul 19 03:25:54 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/19/2022
 Supervised By :mohammad ahmed 07/20/2022

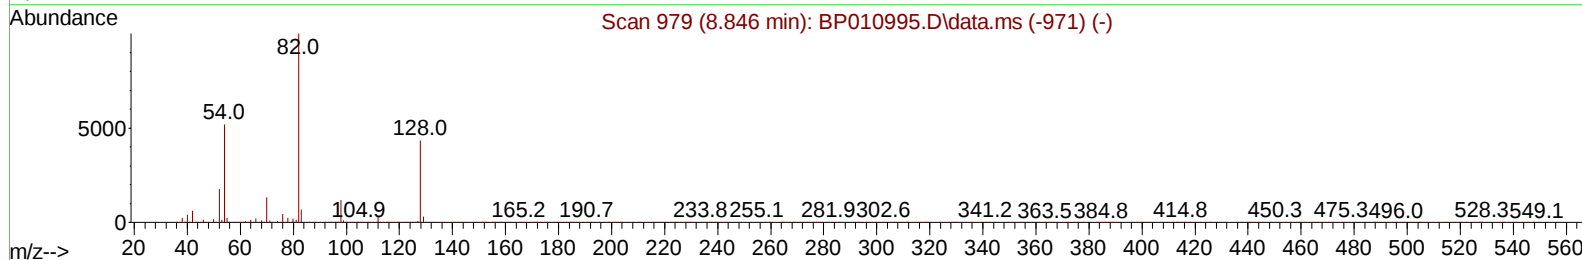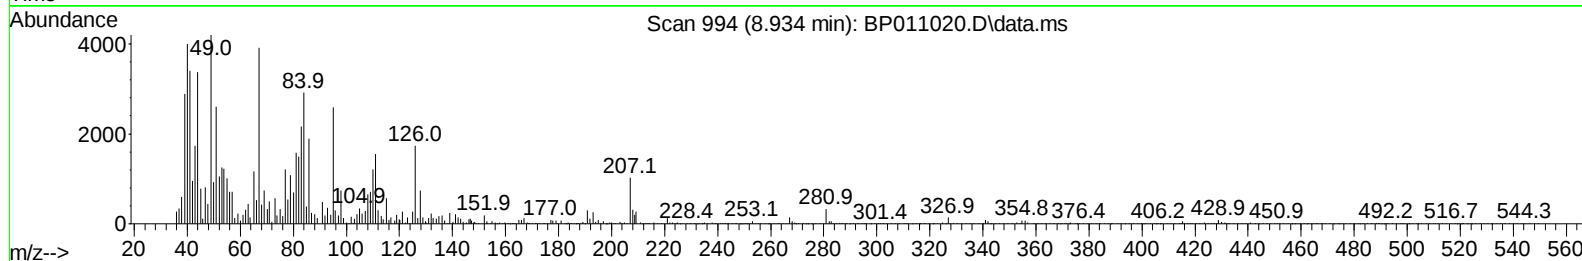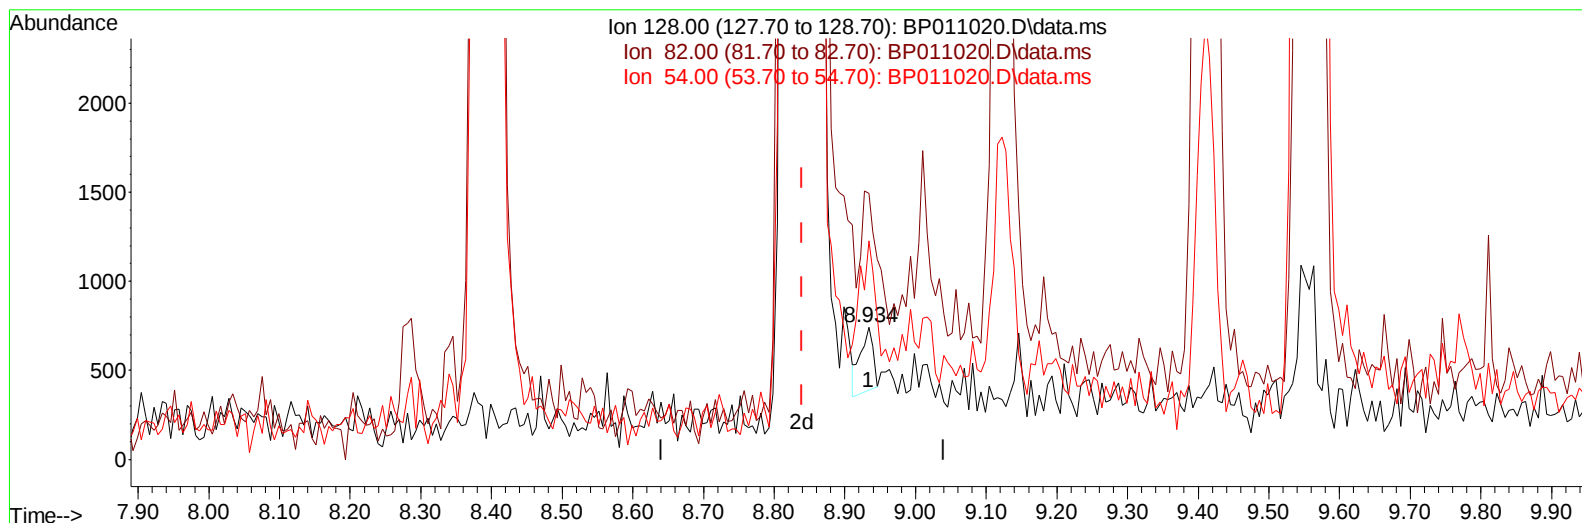

TIC: BP011020.D\data.ms

(21) Nitrobenzene-d5 (S)

8.934min (+ 0.094) 0.04 ng/u1

response 451

Ion	Exp%	Act%
128.00	100.00	100.00
82.00	249.70	200.67
54.00	155.90	165.05
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071822\
 Data File : BP011020.D
 Acq On : 19 Jul 2022 07:18
 Operator : CG/JU
 Sample : N3704-03
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AP8

Manual IntegrationsAPPROVED

Quant Time: Jul 19 07:45:14 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jul 19 03:25:54 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/19/2022
 Supervised By :mohammad ahmed 07/20/2022

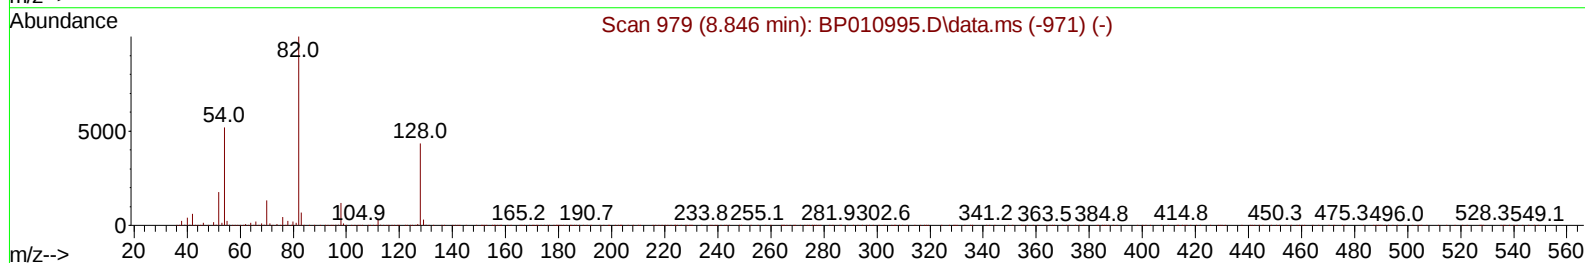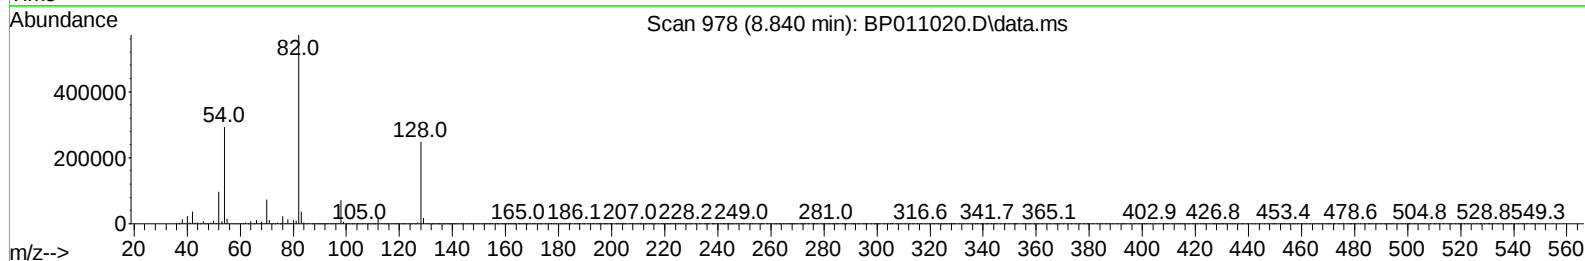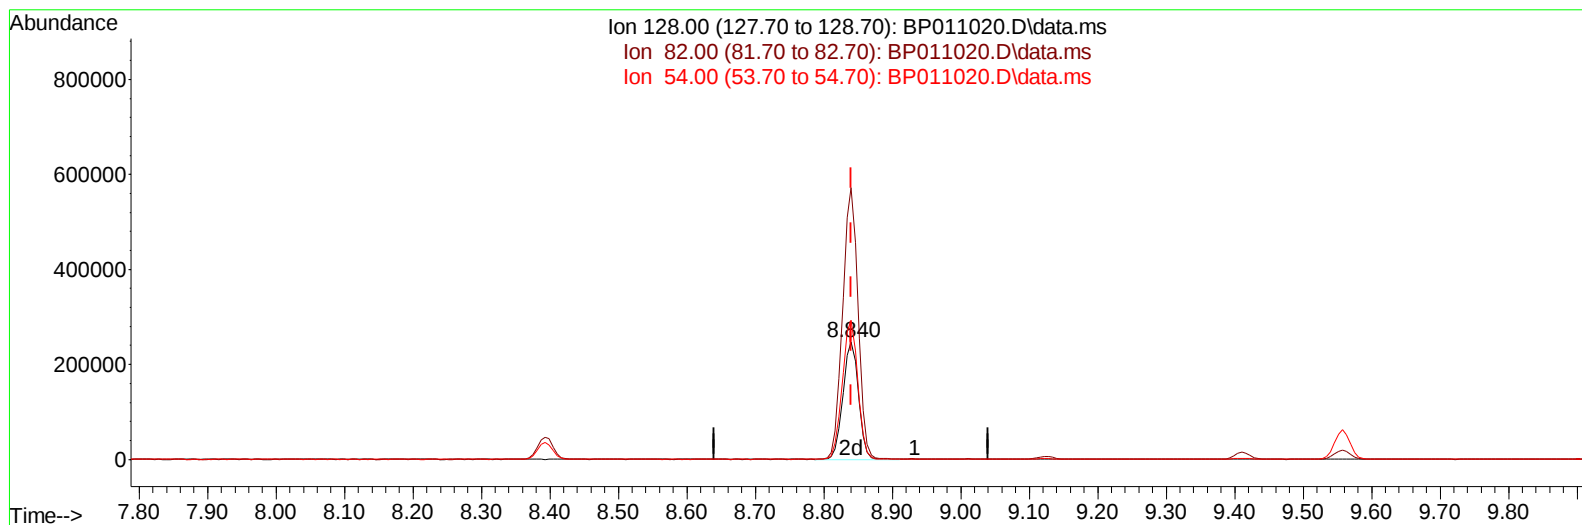

TIC: BP011020.D\data.ms

(21) Nitrobenzene-d5 (S)

8.840min (-0.000) 35.56 ng/ul m

response 387734

Ion	Exp%	Act%
128.00	100.00	100.00
82.00	249.70	230.78
54.00	155.90	118.37#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071822\
 Data File : BP011020.D
 Acq On : 19 Jul 2022 07:18
 Operator : CG/JU
 Sample : N3704-03
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AP8

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 07/19/2022
 Supervised By :mohammad ahmed 07/20/2022

Quant Time: Jul 19 07:45:14 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jul 19 03:25:54 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.675	152	376939	20.000	ng/ul	0.00
20) Naphthalene-d8	10.469	136	1496155	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.340	164	814976	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.104	188	1578458	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.227	240	1567133	20.000	ng/ul	# 0.00
88) Perylene-d12	23.586	264	1693268	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.181	96	58116	5.558	ng/uL	0.00
4) Pyridine-d5	3.593	84	189674	7.018	ng/ul	0.00
7) Phenol-d5	6.858	99	228720	7.392	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.022	67	654514	32.896	ng/ul	0.00
11) 2-Chlorophenol-d4	7.210	132	664942	26.596	ng/ul	0.00
15) 4-Methylphenol-d8	8.393	113	407471	16.450	ng/ul	0.00
21) Nitrobenzene-d5	8.840	128	387734m	35.561	ng/ul	0.00
24) 2-Nitrophenol-d4	9.557	143	372472	34.524	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.093	165	594995	30.156	ng/ul	0.00
31) 4-Chloroaniline-d4	10.616	131	397696	12.227	ng/ul	0.00
46) Dimethylphthalate-d6	13.757	166	2081545	37.370	ng/ul	0.00
49) Acenaphthylene-d8	14.028	160	2389795	36.363	ng/ul	0.00
54) 4-Nitrophenol-d4	14.557	143	64534	5.725	ng/ul	0.00
60) Fluorene-d10	15.339	176	1699388	35.893	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.463	200	231024	29.578	ng/ul	0.00
73) Anthracene-d10	17.204	188	2783152	41.475	ng/ul	0.00
81) Pyrene-d10	19.463	212	3215637	39.069	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.433	264	3380280	41.564	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071822\
Data File : BP011020.D
Acq On : 19 Jul 2022 07:18
Operator : CG/JU
Sample : N3704-03
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AP8

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 07/19/2022
Supervised By :mohammad ahmed 07/20/2022

Quant Time: Jul 19 07:45:14 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jul 19 03:25:54 2022
Response via : Initial Calibration

