

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071822\
 Data File : BP010988.D
 Acq On : 18 Jul 2022 12:26
 Operator : CG/JU
 Sample : N3748-01
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH0E3

Quant Time: Jul 18 12:54:20 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jul 14 15:34:34 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.681	152	549118	20.000	ng/ul	0.00
20) Naphthalene-d8	10.475	136	2474341	20.000	ng/ul	# 0.00
38) Acenaphthene-d10	14.345	164	1412592	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.110	188	2600947	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.227	240	2131176	20.000	ng/ul	#-0.01
88) Perylene-d12	23.580	264	1982358	20.000	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.181	96	56623	3.717	ng/uL	0.00
4) Pyridine-d5	3.593	84	289941	7.365	ng/ul	0.00
7) Phenol-d5	6.858	99	214170	4.751	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.022	67	726243	25.056	ng/ul	0.00
11) 2-Chlorophenol-d4	7.216	132	673180	18.483	ng/ul	0.00
15) 4-Methylphenol-d8	8.399	113	428736	11.881	ng/ul	0.00
21) Nitrobenzene-d5	8.846	128	429627	23.826	ng/ul	0.00
24) 2-Nitrophenol-d4	9.563	143	394362	22.102	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.099	165	661882	20.284	ng/ul	0.00
31) 4-Chloroaniline-d4	10.622	131	645676	12.003	ng/ul	0.00
46) Dimethylphthalate-d6	13.763	166	2584068	26.765	ng/ul	0.00
49) Acenaphthylene-d8	14.034	160	2903952	25.493	ng/ul	0.00
54) 4-Nitrophenol-d4	14.557	143	53017	2.713	ng/ul	0.00
60) Fluorene-d10	15.345	176	2086306	25.423	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.463	200	269869	20.968	ng/ul	-0.01
73) Anthracene-d10	17.210	188	3212468	29.053	ng/ul	0.00
81) Pyrene-d10	19.463	212	3242096	28.966	ng/ul	-0.01
92) Benzo(a)pyrene-d12	23.433	264	2922880	30.699	ng/ul	-0.02
Target Compounds						
					Qvalue	
34) Caprolactam	11.428	113	21101	1.783	ng/ul	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071822\
Data File : BP010988.D
Acq On : 18 Jul 2022 12:26
Operator : CG/JU
Sample : N3748-01
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH0E3

Quant Time: Jul 18 12:54:20 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jul 14 15:34:34 2022
Response via : Initial Calibration

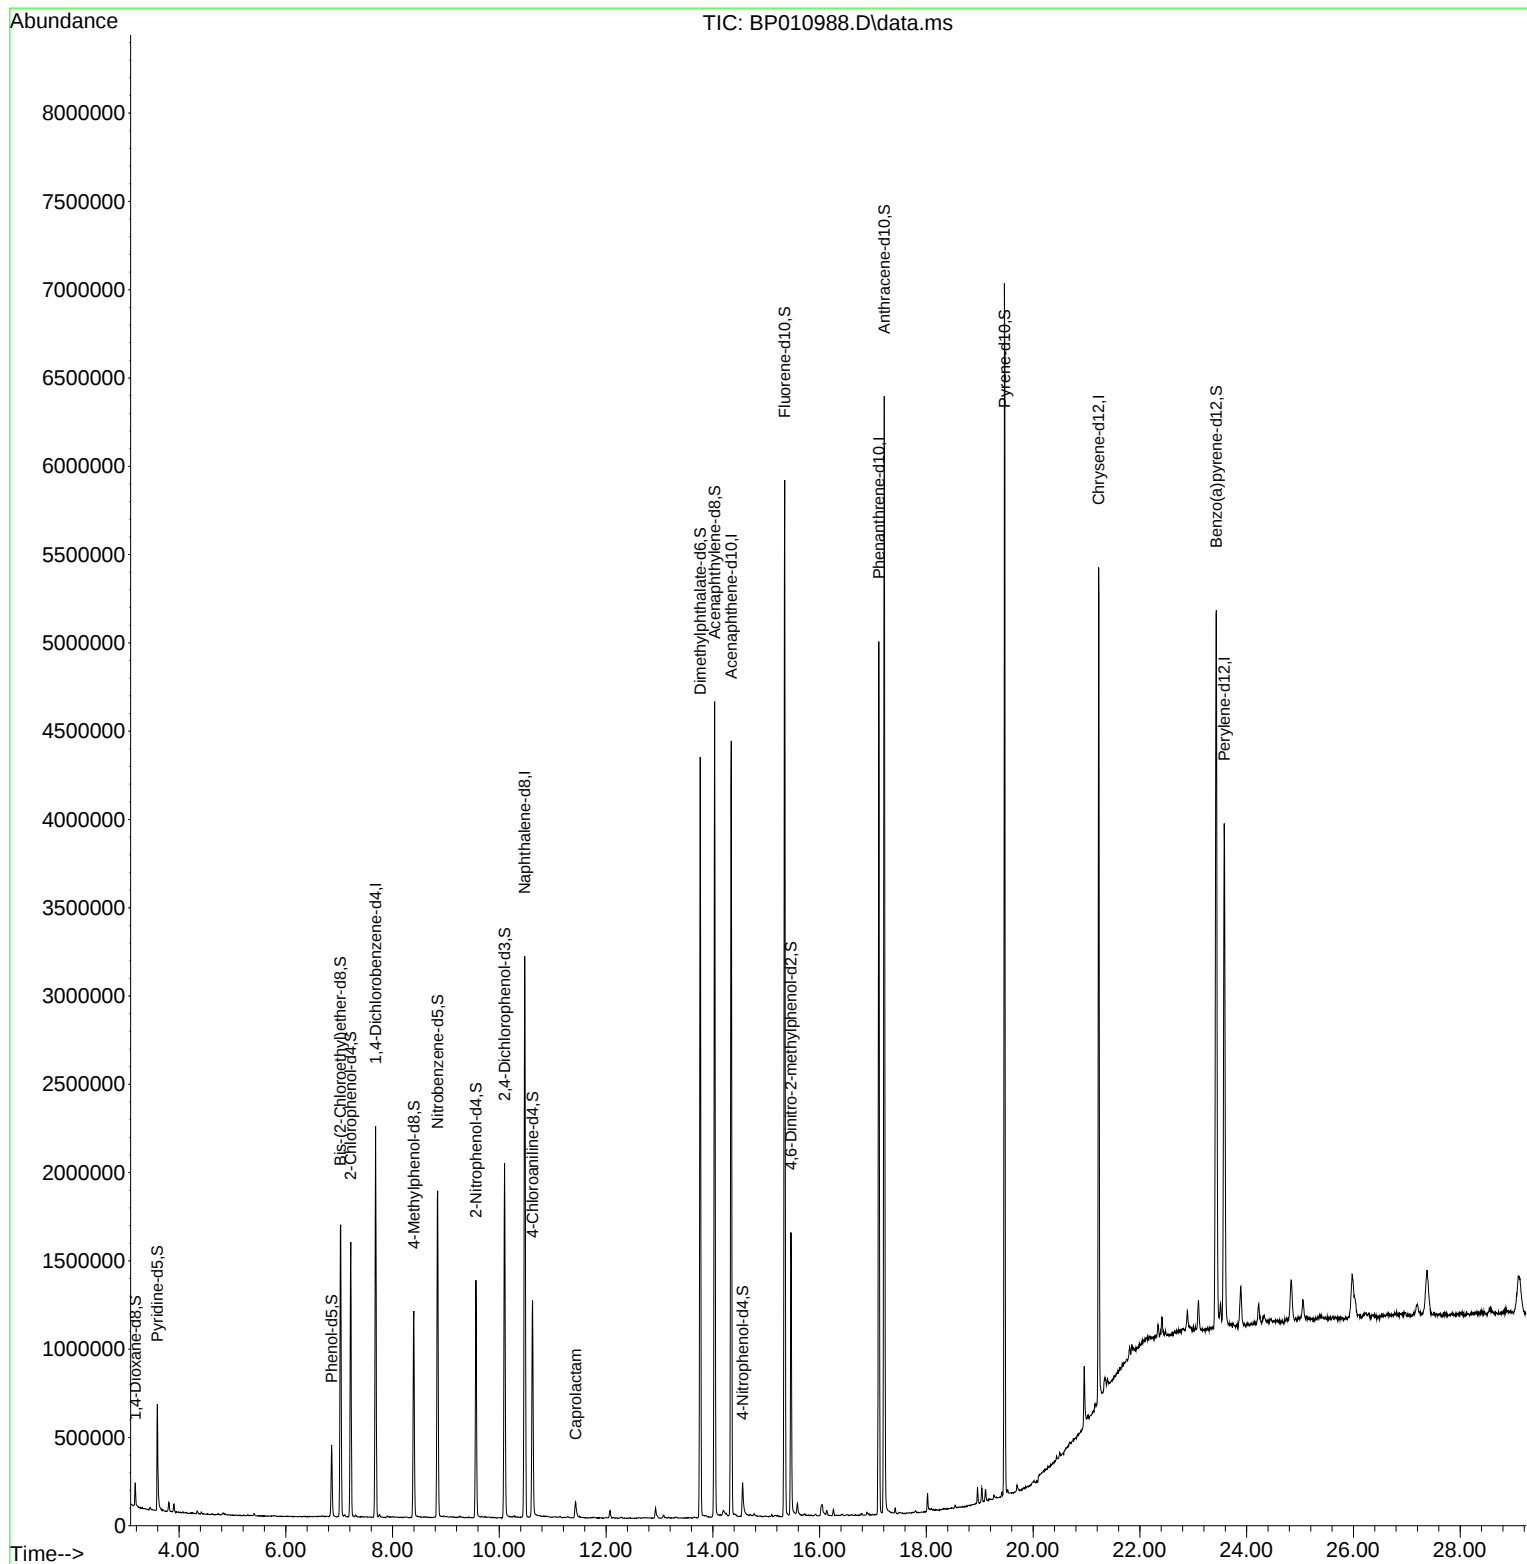

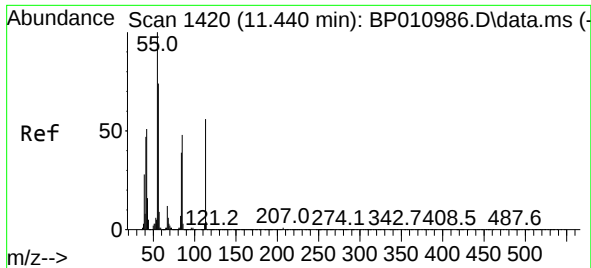

#34
 Caprolactam
 Concen: 1.783 ng/ul
 RT: 11.428 min Scan# 14
 Delta R.T. -0.018 min
 Lab File: BP010988.D
 Acq: 18 Jul 2022 12:26

Instrument :
 BNA_P
 ClientSampleId :
 BH0E3

Tgt Ion:113 Resp: 21101
 Ion Ratio Lower Upper
 113 100
 55 187.9 153.8 230.8
 56 132.1 110.2 165.4

