

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071822\
 Data File : BP010987.D
 Acq On : 18 Jul 2022 11:52
 Operator : CG/JU
 Sample : PB146256BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK256

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010987.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.181	12	16	21	rVB	172678	205893	2.35%	0.190%
2	3.587	82	85	104	rBV	1923832	2558373	29.23%	2.366%
3	3.905	134	139	144	rVB	40269	59204	0.68%	0.055%
4	6.857	635	641	651	rBV	2027464	3064636	35.01%	2.835%
5	7.028	662	670	681	rVB	1762663	2680126	30.62%	2.479%
6	7.216	695	702	709	rBV	2171396	3238377	36.99%	2.995%
7	7.681	775	781	792	rVB	1939702	2960421	33.82%	2.738%
8	7.998	830	835	839	rBV6	9128	17279	0.20%	0.016%
9	8.398	895	903	912	rBV	2485579	3862525	44.12%	3.573%
10	8.845	972	979	992	rBV	1969305	3120824	35.65%	2.887%
11	9.563	1093	1101	1111	rBV	1499476	2384277	27.24%	2.205%
12	10.098	1183	1192	1206	rBV	2250207	3576370	40.86%	3.308%
13	10.475	1246	1256	1265	rBV	2785589	4582546	52.35%	4.239%
14	10.622	1273	1281	1300	rBV	2469152	4148693	47.39%	3.837%
15	11.287	1390	1394	1402	rVB	4161	9472	0.11%	0.009%
16	12.075	1515	1528	1534	rBV	46575	83765	0.96%	0.077%
17	12.963	1673	1679	1687	rVB2	19729	36639	0.42%	0.034%
18	13.763	1807	1815	1827	rBV	4013427	5592480	63.89%	5.173%
19	14.033	1852	1861	1874	rBV	4470185	6555705	74.89%	6.064%
20	14.198	1881	1889	1904	rVB4	32997	93841	1.07%	0.087%
21	14.345	1907	1914	1924	rBV	4219281	5888013	67.26%	5.446%
22	14.557	1943	1950	1972	rBV	1451935	2557820	29.22%	2.366%
23	15.345	2077	2084	2096	rBV	5722616	8056092	92.03%	7.451%
24	15.469	2099	2105	2118	rVV	1608813	2283899	26.09%	2.112%
25	15.586	2121	2125	2136	rVB2	70632	113475	1.30%	0.105%
26	15.916	2177	2181	2184	rBV6	8177	13922	0.16%	0.013%
27	16.139	2214	2219	2226	rVB3	21851	34864	0.40%	0.032%
28	16.786	2325	2329	2335	rVB9	13909	25442	0.29%	0.024%
29	16.898	2343	2348	2353	rBV2	11837	20137	0.23%	0.019%
30	17.116	2378	2385	2395	rBV	4472785	6516770	74.45%	6.028%
31	17.216	2395	2402	2415	rBV2	5717993	8359903	95.50%	7.732%
32	17.416	2434	2436	2442	rVB6	9206	14679	0.17%	0.014%
33	18.021	2535	2539	2543	rBV6	21100	34733	0.40%	0.032%
34	18.545	2625	2628	2634	rBV8	10883	16804	0.19%	0.016%
35	19.045	2708	2713	2717	rBV3	74193	102154	1.17%	0.094%
36	19.110	2720	2724	2728	rVV	64455	88120	1.01%	0.082%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071822\
Data File : BP010987.D
Acq On : 18 Jul 2022 11:52
Operator : CG/JU
Sample : PB146256BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK256

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Title : SVOA CALIBRATION

37	19.468	2779	2785	2792	rBV	6867652	8753776	100.00%	8.097%
38	19.698	2822	2824	2828	rVB2	28608	31392	0.36%	0.029%
39	21.233	3080	3085	3094	rBV	4454355	5645656	64.49%	5.222%
40	23.433	3452	3459	3468	rBV2	3315462	6253344	71.44%	5.784%
41	23.586	3478	3485	3495	rVB	2215584	4472391	51.09%	4.137%




Sum of corrected areas: 108114832

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071822\
Data File : BP010987.D
Acq On : 18 Jul 2022 11:52
Operator : CG/JU
Sample : PB146256BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK256

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

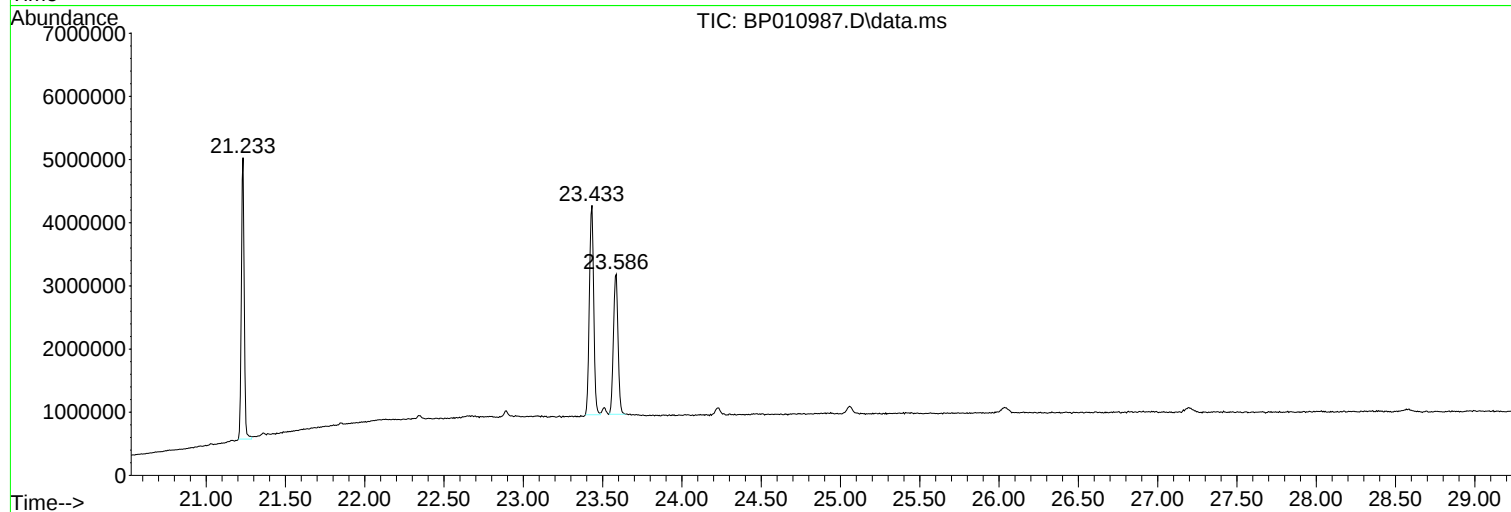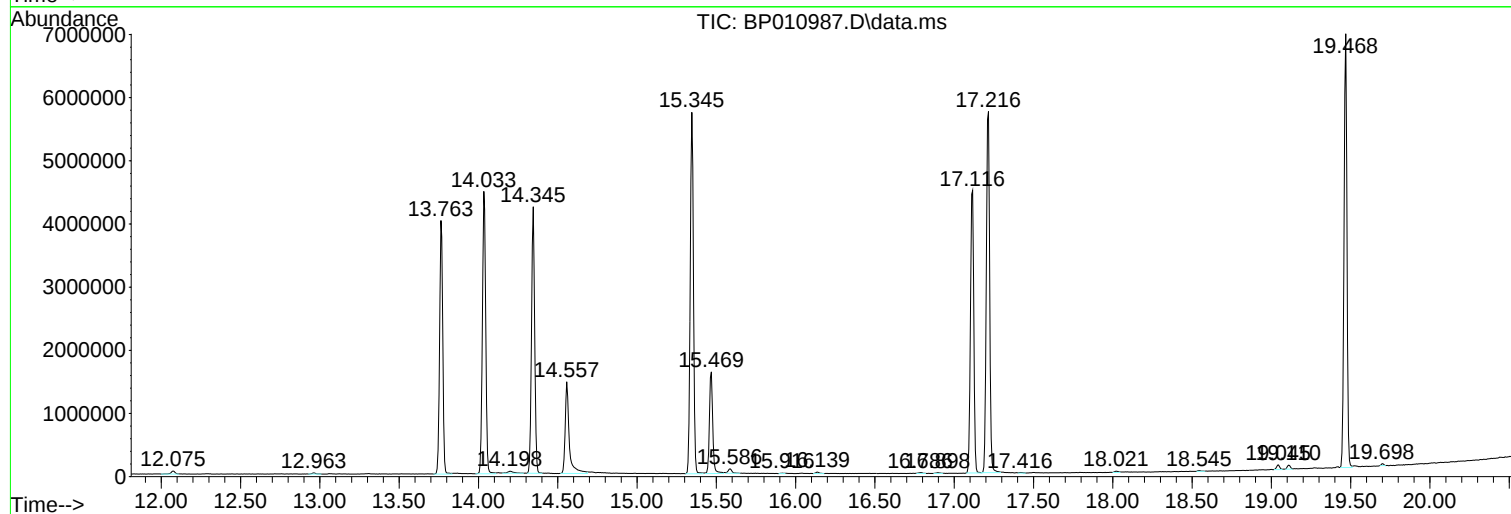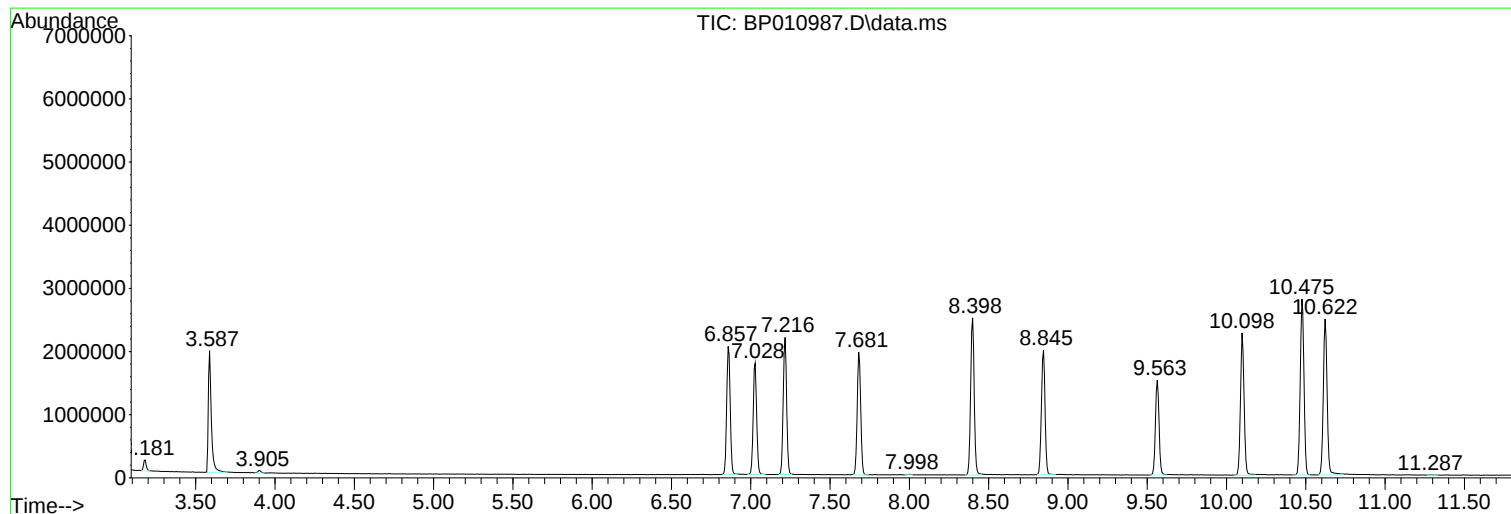

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071822\
Data File : BP010987.D
Acq On : 18 Jul 2022 11:52
Operator : CG/JU
Sample : PB146256BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK256

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071822\
Data File : BP010987.D
Acq On : 18 Jul 2022 11:52
Operator : CG/JU
Sample : PB146256BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK256

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------