

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071822\
 Data File : BP010988.D
 Acq On : 18 Jul 2022 12:26
 Operator : CG/JU
 Sample : N3748-01
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH0E3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010988.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.181	12	16	25	rVB	139305	182176	2.05%	0.177%
2	3.458	61	63	68	rVB	12445	15688	0.18%	0.015%
3	3.593	82	86	102	rVB	603425	831606	9.37%	0.810%
4	3.811	119	123	128	rVB	51656	71756	0.81%	0.070%
5	3.905	135	139	144	rVB	49073	65734	0.74%	0.064%
6	4.340	209	213	221	rVB6	16889	25371	0.29%	0.025%
7	4.417	223	226	230	rBV4	12255	15159	0.17%	0.015%
8	4.858	299	301	305	rVB3	6486	9128	0.10%	0.009%
9	5.405	390	394	399	rVB	13179	18641	0.21%	0.018%
10	6.858	632	641	648	rBV	406326	608832	6.86%	0.593%
11	7.028	662	670	679	rBV	1653141	2575201	29.02%	2.509%
12	7.111	679	684	691	rVB	12478	24897	0.28%	0.024%
13	7.216	695	702	713	rBV	1556718	2334109	26.30%	2.274%
14	7.305	713	717	720	rBV4	9625	13063	0.15%	0.013%
15	7.681	773	781	789	rBV	2217007	3326620	37.48%	3.241%
16	7.752	790	793	799	rVB3	15433	24172	0.27%	0.024%
17	7.910	815	820	822	rBV6	7416	10382	0.12%	0.010%
18	8.399	896	903	910	rBV	1167510	1810982	20.40%	1.764%
19	8.846	971	979	988	rBV	1849060	2979308	33.57%	2.902%
20	9.010	1005	1007	1015	rVB9	5727	9469	0.11%	0.009%
21	9.263	1047	1050	1054	rVB6	7351	9723	0.11%	0.009%
22	9.563	1090	1101	1114	rBV	1346481	2136878	24.08%	2.082%
23	9.805	1137	1142	1150	rVB	5913	15152	0.17%	0.015%
24	10.099	1183	1192	1203	rBV	2010513	3192230	35.97%	3.110%
25	10.475	1248	1256	1267	rVB	3175604	5102541	57.49%	4.971%
26	10.622	1272	1281	1291	rBV	1226194	2060600	23.22%	2.007%
27	11.140	1367	1369	1375	rVB7	8235	10400	0.12%	0.010%
28	11.428	1410	1418	1430	rBV	90763	212381	2.39%	0.207%
29	11.769	1471	1476	1481	rVB8	5303	9508	0.11%	0.009%
30	12.004	1506	1516	1518	rBV8	6664	12274	0.14%	0.012%
31	12.075	1521	1528	1534	rVB	43111	72034	0.81%	0.070%
32	12.287	1558	1564	1569	rVB8	5856	12026	0.14%	0.012%
33	12.928	1667	1673	1687	rVB2	58869	117175	1.32%	0.114%
34	13.081	1692	1699	1703	rBV4	17161	31097	0.35%	0.030%
35	13.310	1733	1738	1743	rVB7	6117	10030	0.11%	0.010%
36	13.645	1789	1795	1800	rBV10	5569	12623	0.14%	0.012%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071822\
 Data File : BP010988.D
 Acq On : 18 Jul 2022 12:26
 Operator : CG/JU
 Sample : N3748-01
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH0E3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
 Title : SVOA CALIBRATION

37	13.763	1806	1815	1829	rBV	4309656	5733093	64.60%	5.585%
38	14.034	1851	1861	1873	rBV	4619228	6456204	72.74%	6.290%
39	14.198	1884	1889	1897	rBV4	26622	65927	0.74%	0.064%
40	14.251	1897	1898	1904	rVB6	15116	15343	0.17%	0.015%
41	14.345	1907	1914	1921	rBV	4386047	6308320	71.08%	6.146%
42	14.557	1945	1950	1963	rBV	192078	389455	4.39%	0.379%
43	14.704	1972	1975	1980	rVB7	9427	14422	0.16%	0.014%
44	14.775	1981	1987	1992	rVB10	11904	19681	0.22%	0.019%
45	15.216	2059	2062	2066	rVB5	8859	9255	0.10%	0.009%
46	15.345	2077	2084	2097	rBV	5868885	8166512	92.01%	7.956%
47	15.463	2098	2104	2118	rVV	1604689	2229430	25.12%	2.172%
48	15.587	2120	2125	2136	rVB	68601	132994	1.50%	0.130%
49	15.716	2145	2147	2154	rVB7	9614	14702	0.17%	0.014%
50	15.928	2177	2183	2187	rBV9	8984	16070	0.18%	0.016%
51	16.045	2196	2203	2215	rBV2	63469	193183	2.18%	0.188%
52	16.134	2215	2218	2222	rVB5	26076	38169	0.43%	0.037%
53	16.257	2234	2239	2246	rBV2	36051	49747	0.56%	0.048%
54	16.886	2343	2346	2350	rBV4	14234	18975	0.21%	0.018%
55	17.110	2377	2384	2394	rBV	4944908	6636968	74.78%	6.466%
56	17.210	2395	2401	2421	rVV	6325886	8720537	98.26%	8.496%
57	17.416	2432	2436	2442	rVB	32083	46893	0.53%	0.046%
58	18.022	2535	2539	2544	rBV	104615	139045	1.57%	0.135%
59	18.957	2695	2698	2705	rBV	92765	106504	1.20%	0.104%
60	19.039	2708	2712	2717	rBV2	80726	104964	1.18%	0.102%
61	19.104	2720	2723	2728	rBV	65082	91199	1.03%	0.089%
62	19.463	2779	2784	2792	rBV	6857039	8875288	100.00%	8.646%
63	20.957	3034	3038	3047	rBV2	344868	575025	6.48%	0.560%
64	21.227	3079	3084	3093	rBV	4738200	6166318	69.48%	6.007%
65	23.433	3452	3459	3467	rBV2	4014172	7794884	87.83%	7.594%
66	23.580	3478	3484	3496	rVB2	2836396	5550126	62.53%	5.407%


Sum of corrected areas: 102648199

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071822\
Data File : BP010988.D
Acq On : 18 Jul 2022 12:26
Operator : CG/JU
Sample : N3748-01
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH0E3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

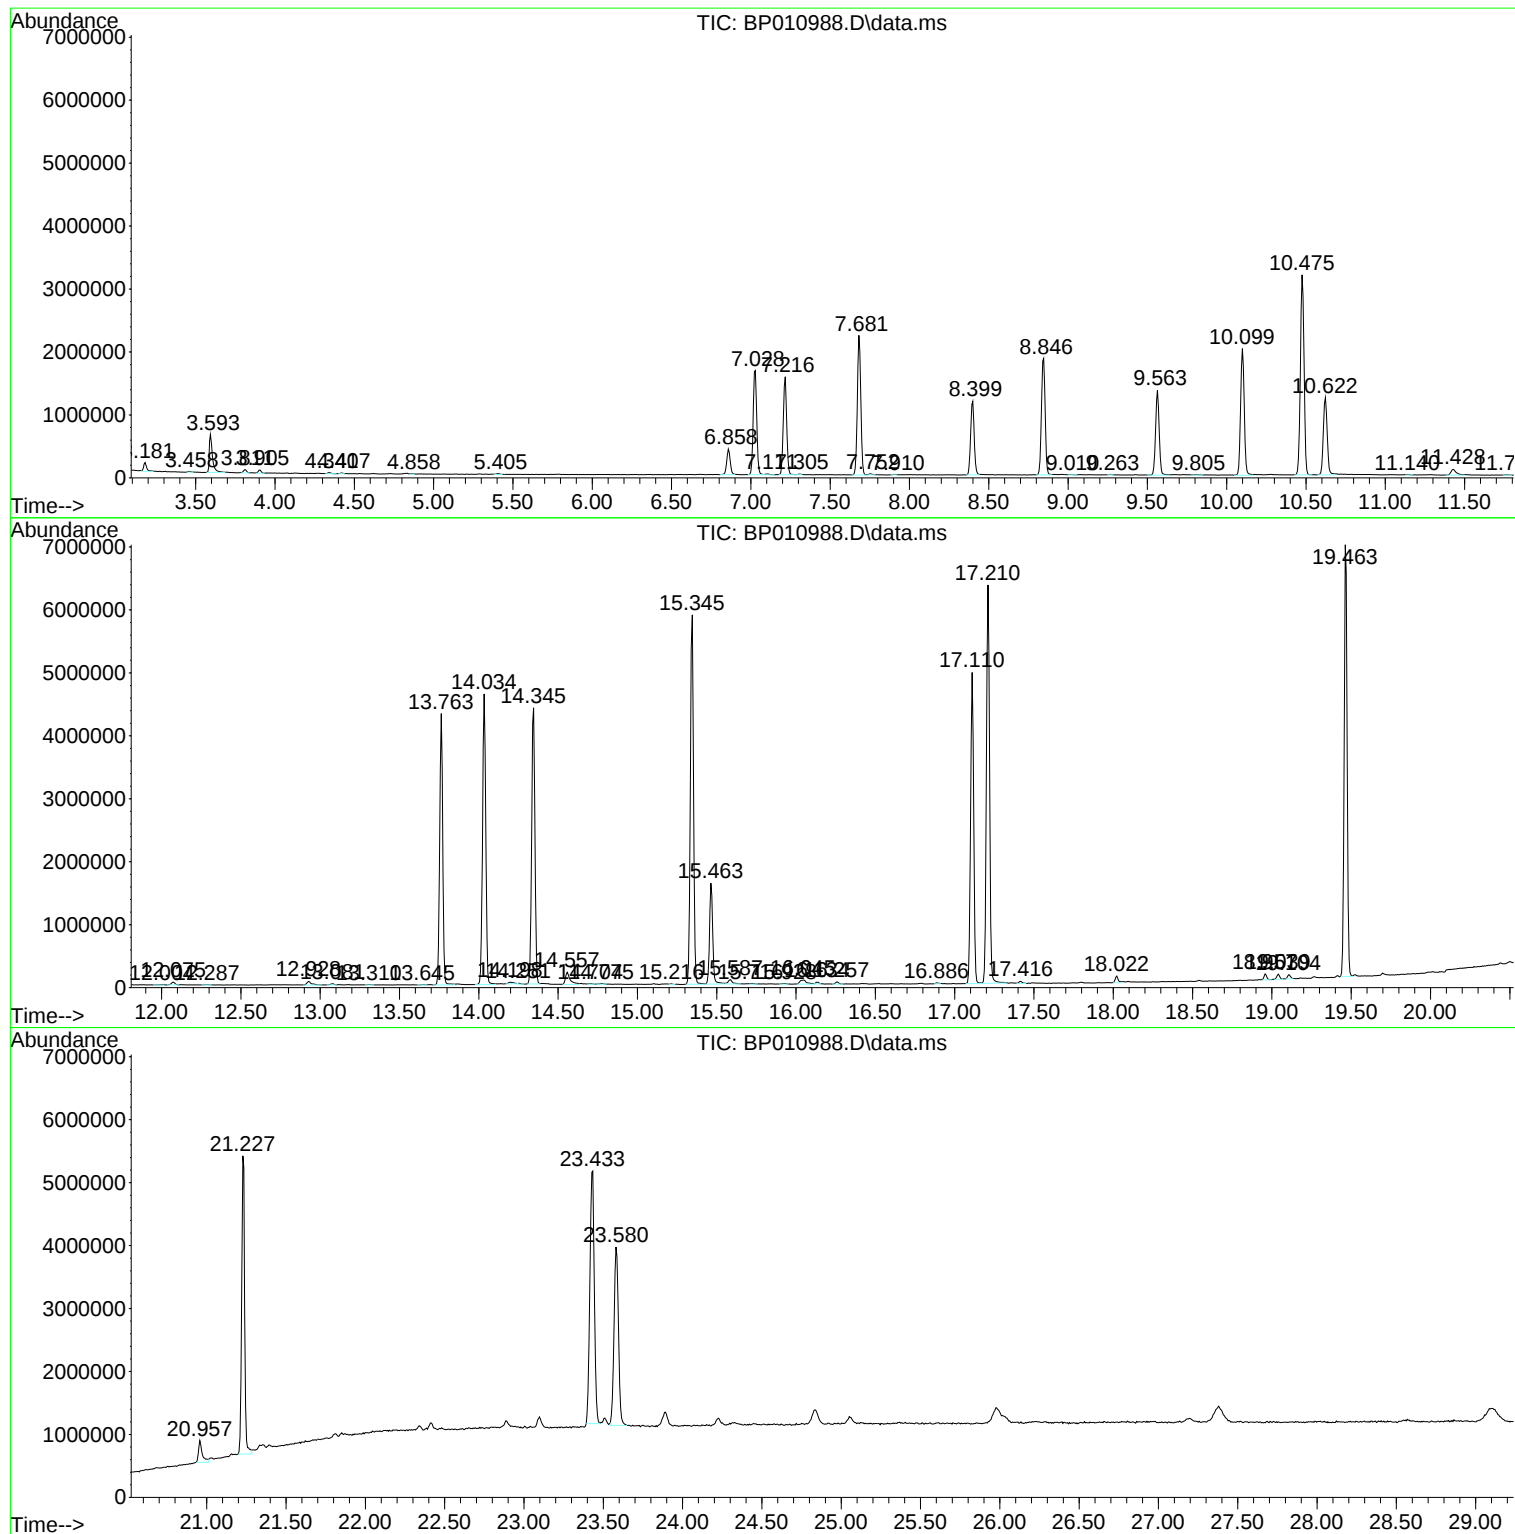

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071822\
Data File : BP010988.D
Acq On : 18 Jul 2022 12:26
Operator : CG/JU
Sample : N3748-01
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH0E3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071822\
Data File : BP010988.D
Acq On : 18 Jul 2022 12:26
Operator : CG/JU
Sample : N3748-01
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH0E3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc