

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071822\
 Data File : BP010989.D
 Acq On : 18 Jul 2022 13:00
 Operator : CG/JU
 Sample : N3748-02
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH0E4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010989.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.181	12	16	20	rBV	120147	142893	1.25%	0.128%
2	3.593	83	86	99	rBV	327434	462079	4.05%	0.414%
3	3.811	118	123	128	rBV	54816	73497	0.64%	0.066%
4	3.899	135	138	143	rBV	40695	50886	0.45%	0.046%
5	5.405	391	394	398	rVB	13046	15392	0.13%	0.014%
6	6.858	634	641	650	rBV	435274	648397	5.68%	0.581%
7	7.022	659	669	678	rBV	1850818	2892766	25.33%	2.593%
8	7.216	694	702	714	rBV	1718639	2621144	22.95%	2.350%
9	7.311	714	718	724	rVB7	10675	19011	0.17%	0.017%
10	7.681	774	781	789	rBV	2117144	3198935	28.01%	2.868%
11	7.752	791	793	801	rVB5	12116	19297	0.17%	0.017%
12	8.399	896	903	915	rBV	1253293	1986085	17.39%	1.780%
13	8.846	971	979	993	rBV	2104137	3380443	29.60%	3.030%
14	9.263	1046	1050	1058	rVB6	9100	20246	0.18%	0.018%
15	9.563	1092	1101	1114	rBV	1548231	2437760	21.35%	2.185%
16	10.099	1184	1192	1205	rBV	2199535	3504547	30.69%	3.142%
17	10.475	1248	1256	1264	rBV	3033045	4968204	43.51%	4.454%
18	10.622	1272	1281	1297	rBV	1107587	1887503	16.53%	1.692%
19	11.134	1365	1368	1374	rVB8	7390	14029	0.12%	0.013%
20	12.075	1522	1528	1537	rBV2	49421	85295	0.75%	0.076%
21	12.957	1673	1678	1684	rVB5	12774	20644	0.18%	0.019%
22	13.063	1693	1696	1702	rBV7	6512	11566	0.10%	0.010%
23	13.310	1734	1738	1746	rVB9	9219	16553	0.14%	0.015%
24	13.763	1808	1815	1825	rBV	4752125	6536370	57.24%	5.859%
25	13.851	1828	1830	1839	rVB10	10310	25387	0.22%	0.023%
26	14.034	1851	1861	1872	rBV	5073526	7282639	63.77%	6.528%
27	14.198	1884	1889	1895	rBV2	26216	59503	0.52%	0.053%
28	14.346	1907	1914	1924	rBV	4383416	6410387	56.14%	5.746%
29	14.557	1943	1950	1966	rBV	241131	515076	4.51%	0.462%
30	14.775	1983	1987	1991	rVB5	23525	30774	0.27%	0.028%
31	15.216	2059	2062	2067	rVB5	12829	17345	0.15%	0.016%
32	15.345	2077	2084	2091	rBV	6741181	9371756	82.07%	8.401%
33	15.463	2098	2104	2120	rBV	2074183	2871118	25.14%	2.574%
34	15.587	2120	2125	2136	rVB	85385	133512	1.17%	0.120%
35	15.722	2144	2148	2154	rVB3	17788	25557	0.22%	0.023%
36	16.034	2196	2201	2202	rBV3	28536	37058	0.32%	0.033%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071822\
 Data File : BP010989.D
 Acq On : 18 Jul 2022 13:00
 Operator : CG/JU
 Sample : N3748-02
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH0E4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
 Title : SVOA CALIBRATION

37	16.134	2214	2218	2226	rVB4	30980	44628	0.39%	0.040%
38	16.257	2235	2239	2244	rVB2	18727	27506	0.24%	0.025%
39	16.787	2324	2329	2335	rVB8	14076	24220	0.21%	0.022%
40	16.892	2342	2347	2349	rBV3	16666	27816	0.24%	0.025%
41	16.922	2349	2352	2358	rVB	37211	52813	0.46%	0.047%
42	17.110	2378	2384	2394	rBV	5234802	7189208	62.96%	6.445%
43	17.210	2394	2401	2422	rVV2	7775179	10854505	95.05%	9.730%
44	17.416	2432	2436	2441	rVB3	17156	25856	0.23%	0.023%
45	17.798	2497	2501	2505	rVB6	13959	22819	0.20%	0.020%
46	18.022	2534	2539	2544	rBV2	105587	143125	1.25%	0.128%
47	18.957	2694	2698	2702	rBV	133439	156598	1.37%	0.140%
48	19.039	2708	2712	2717	rBV2	101128	128236	1.12%	0.115%
49	19.110	2720	2724	2728	rVV	87347	111792	0.98%	0.100%
50	19.263	2748	2750	2754	rBV4	22711	21563	0.19%	0.019%
51	19.416	2773	2776	2778	rBV2	36526	37180	0.33%	0.033%
52	19.469	2778	2785	2792	rVV	8625774	11419347	100.00%	10.237%
53	20.957	3034	3038	3046	rBV	461137	728238	6.38%	0.653%
54	21.228	3079	3084	3094	rBV	4716085	6144337	53.81%	5.508%
55	23.433	3452	3459	3467	rBV2	4145639	7782073	68.15%	6.976%
56	23.586	3479	3485	3498	rVB2	2509132	4817830	42.19%	4.319%




Sum of corrected areas: 111553344

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071822\
Data File : BP010989.D
Acq On : 18 Jul 2022 13:00
Operator : CG/JU
Sample : N3748-02
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH0E4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

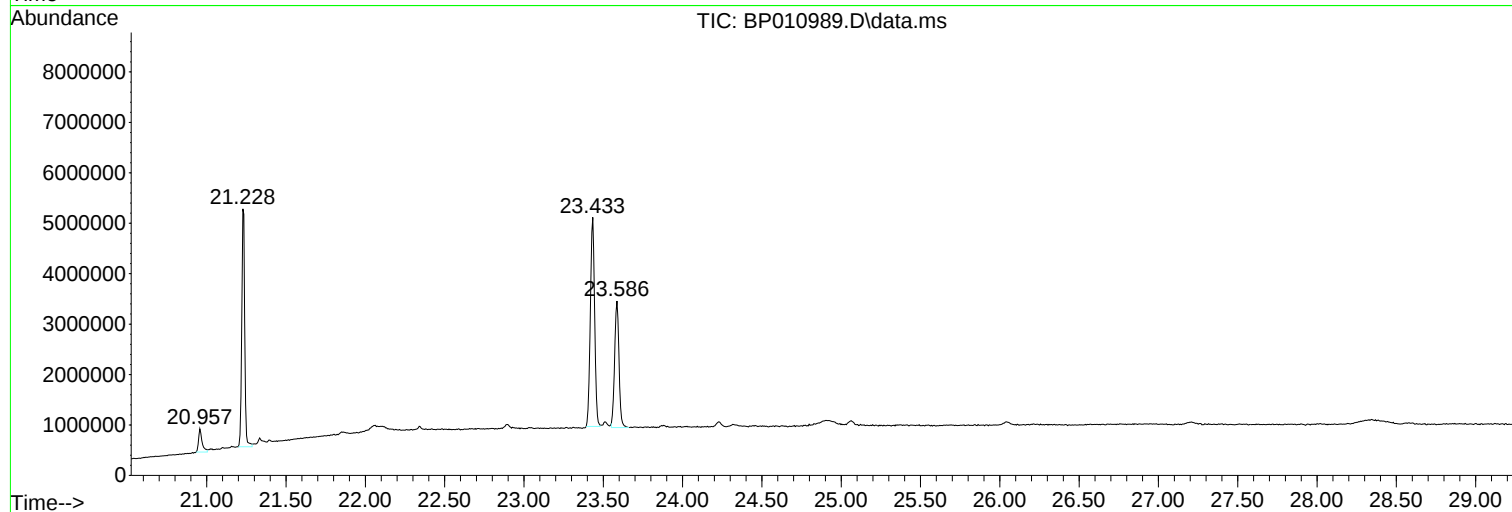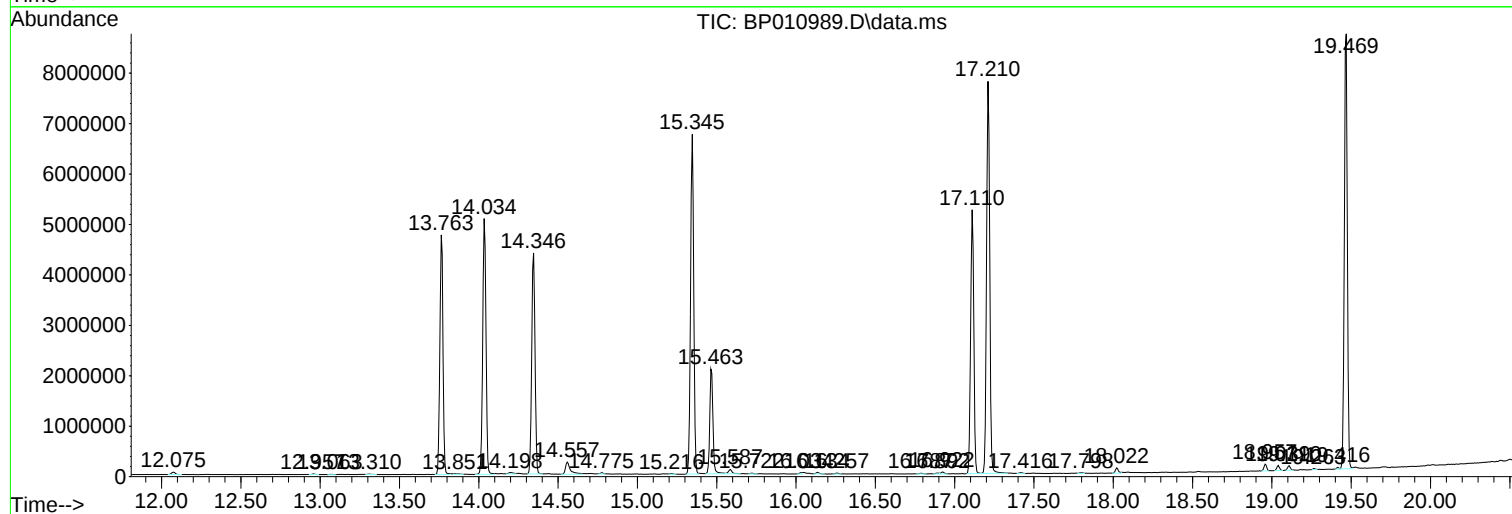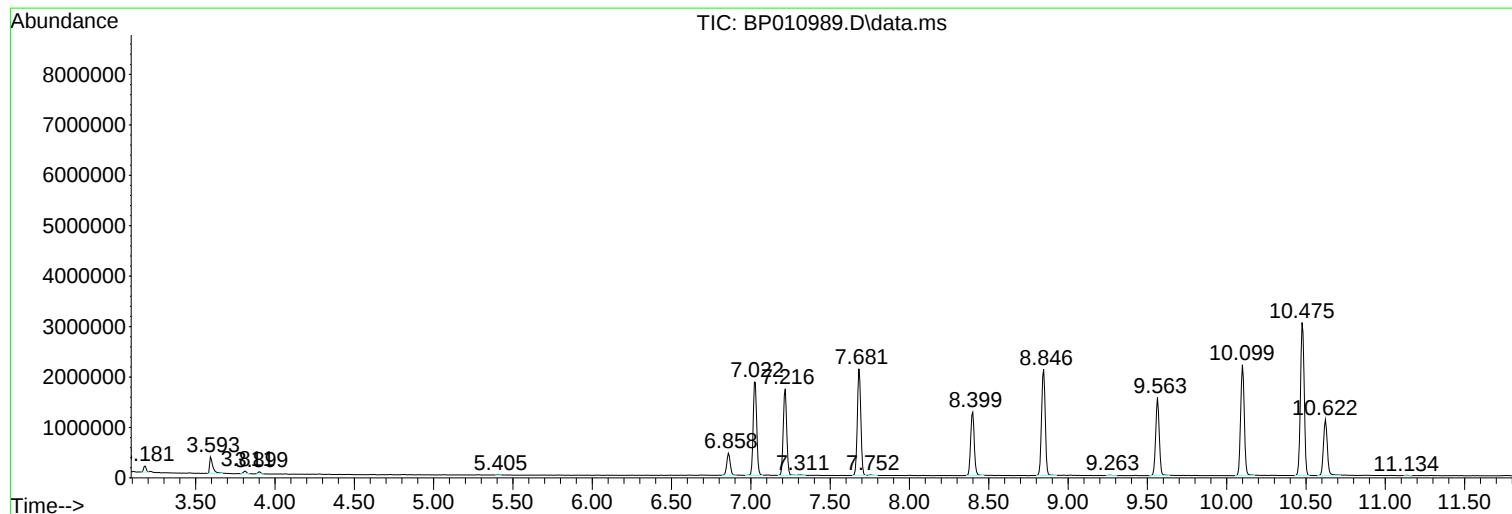

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071822\
Data File : BP010989.D
Acq On : 18 Jul 2022 13:00
Operator : CG/JU
Sample : N3748-02
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH0E4










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Cyclic20.957 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
20.957	2.37 ng/ul	728238	Chrysene-d12	21.233

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Cyclotetracosane	336	C24H48	000297-03-0	95
2			Cyclotetracosane	336	C24H48	000297-03-0	94
3			1-Hexacosene	364	C26H52	018835-33-1	94
4			Octacosanol	410	C28H58O	000557-61-9	94
5			Pentacos-1-ene	350	C25H50	016980-85-1	94

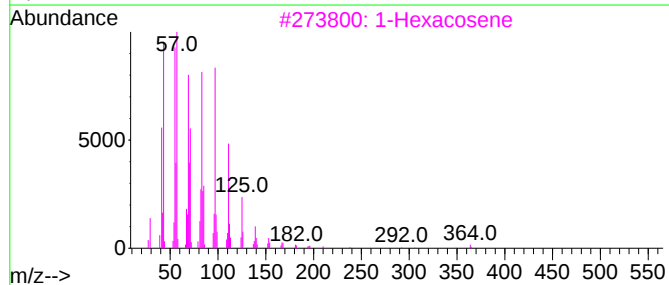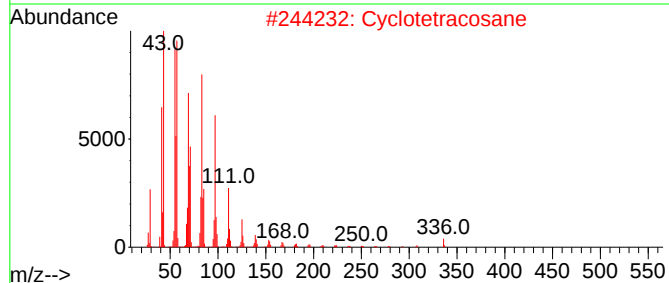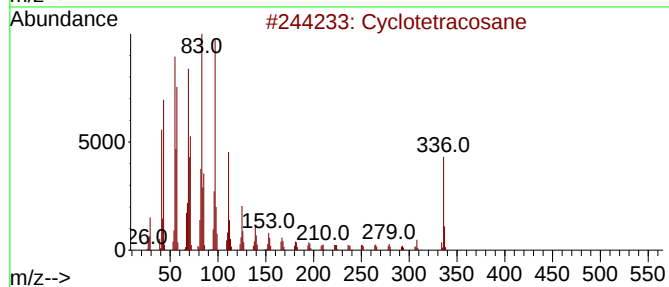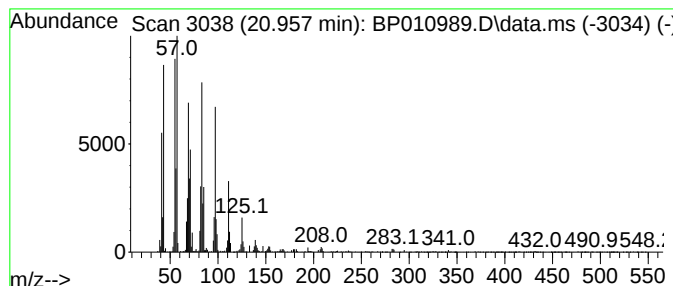

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071822\
Data File : BP010989.D
Acq On : 18 Jul 2022 13:00
Operator : CG/JU
Sample : N3748-02
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH0E4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: C...	20.957	2.4	ng/u1	728238	5	21.233	6144340	20.0