

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071822\
 Data File : BP010990.D
 Acq On : 18 Jul 2022 13:35
 Operator : CG/JU
 Sample : N3748-03
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH0E5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010990.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.181	12	16	19	rBV	109307	122287	1.42%	0.154%
2	3.593	84	86	101	rBV	373333	518450	6.03%	0.654%
3	3.811	118	123	128	rVB	48950	69497	0.81%	0.088%
4	3.899	135	138	143	rVB	37171	50998	0.59%	0.064%
5	4.340	207	213	223	rVB	470583	647993	7.53%	0.818%
6	4.811	289	293	295	rBV5	6841	9236	0.11%	0.012%
7	5.011	323	327	332	rVB	45411	62504	0.73%	0.079%
8	5.281	370	373	378	rVB6	6758	10570	0.12%	0.013%
9	5.405	389	394	399	rBV3	12681	21687	0.25%	0.027%
10	6.681	603	611	613	rBV9	5814	12557	0.15%	0.016%
11	6.858	631	641	651	rVB	335520	527189	6.13%	0.665%
12	7.028	662	670	680	rBV	1392109	2172565	25.25%	2.742%
13	7.099	680	682	689	rVB2	7294	12574	0.15%	0.016%
14	7.216	696	702	710	rBV	1361788	2020590	23.48%	2.550%
15	7.558	756	760	767	rVB9	9380	18679	0.22%	0.024%
16	7.681	773	781	791	rBV	1578812	2424169	28.17%	3.060%
17	7.758	791	794	799	rVB6	6824	11462	0.13%	0.014%
18	8.028	837	840	849	rVB10	10332	24551	0.29%	0.031%
19	8.399	896	903	911	rBV	904886	1416122	16.46%	1.787%
20	8.787	962	969	972	rBV4	17354	29323	0.34%	0.037%
21	8.846	972	979	988	rVV	1465762	2350131	27.31%	2.966%
22	8.934	991	994	997	rVV5	9304	15377	0.18%	0.019%
23	9.028	1003	1010	1014	rBV10	7673	17105	0.20%	0.022%
24	9.128	1022	1027	1032	rBV3	9635	14979	0.17%	0.019%
25	9.199	1034	1039	1040	rBV5	6655	9307	0.11%	0.012%
26	9.263	1046	1050	1054	rBV7	10626	16896	0.20%	0.021%
27	9.305	1054	1057	1062	rVB4	11139	16802	0.20%	0.021%
28	9.563	1093	1101	1113	rBV	1029571	1647777	19.15%	2.080%
29	9.675	1116	1120	1125	rVB8	8013	14298	0.17%	0.018%
30	9.752	1132	1133	1139	rVB6	7131	8959	0.10%	0.011%
31	9.869	1146	1153	1164	rVB6	11277	34307	0.40%	0.043%
32	10.099	1183	1192	1204	rBV	1487950	2341627	27.21%	2.956%
33	10.175	1204	1205	1213	rVB8	7103	10225	0.12%	0.013%
34	10.352	1232	1235	1238	rVB5	6301	9301	0.11%	0.012%
35	10.475	1248	1256	1264	rBV	2001793	3272209	38.03%	4.130%
36	10.622	1272	1281	1288	rBV	982297	1644885	19.12%	2.076%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071822\
 Data File : BP010990.D
 Acq On : 18 Jul 2022 13:35
 Operator : CG/JU
 Sample : N3748-03
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH0E5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
 Title : SVOA CALIBRATION

37	10.781	1305	1308	1314	rVB8	5879	9624	0.11%	0.012%
38	10.851	1314	1320	1323	rVV8	6828	12926	0.15%	0.016%
39	11.140	1366	1369	1372	rBV4	8218	10209	0.12%	0.013%
40	11.281	1386	1393	1394	rBV7	5281	10040	0.12%	0.013%

41	11.510	1425	1432	1437	rVB6	9539	13363	0.16%	0.017%
42	11.763	1471	1475	1480	rBV5	6918	10098	0.12%	0.013%
43	11.840	1482	1488	1493	rVB3	14669	23381	0.27%	0.030%
44	11.998	1509	1515	1518	rBV6	10436	19397	0.23%	0.024%
45	12.075	1523	1528	1533	rVB	28343	45857	0.53%	0.058%

46	12.587	1611	1615	1619	rBV7	7657	9790	0.11%	0.012%
47	12.928	1668	1673	1682	rVB4	33279	65942	0.77%	0.083%
48	13.187	1710	1717	1721	rVB6	11202	20672	0.24%	0.026%
49	13.516	1768	1773	1778	rVB	25410	37216	0.43%	0.047%
50	13.675	1791	1800	1802	rBV9	9230	19070	0.22%	0.024%

51	13.763	1808	1815	1821	rBV	2604106	3531997	41.05%	4.458%
52	13.822	1821	1825	1832	rVV	33949	58523	0.68%	0.074%
53	13.893	1835	1837	1842	rVB6	7703	9400	0.11%	0.012%
54	14.034	1853	1861	1871	rBV	3043983	4308948	50.08%	5.439%
55	14.204	1883	1890	1897	rBV4	25336	64013	0.74%	0.081%

56	14.345	1907	1914	1922	rBV	2472498	3620463	42.08%	4.570%
57	14.410	1922	1925	1932	rVB2	53628	83531	0.97%	0.105%
58	14.475	1932	1936	1942	rVB	31611	46319	0.54%	0.058%
59	14.557	1944	1950	1962	rBV	141823	304336	3.54%	0.384%
60	14.892	2005	2007	2013	rVB4	11476	14796	0.17%	0.019%

61	14.975	2015	2021	2025	rBV9	7338	14928	0.17%	0.019%
62	15.116	2040	2045	2048	rBV7	6331	11614	0.13%	0.015%
63	15.216	2059	2062	2067	rVB6	10552	14058	0.16%	0.018%
64	15.345	2077	2084	2098	rBV2	3906436	6187372	71.91%	7.810%
65	15.463	2098	2104	2111	rBV	958915	1342098	15.60%	1.694%

66	15.587	2121	2125	2128	rBV2	44263	63525	0.74%	0.080%
67	15.834	2164	2167	2171	rBV5	9066	12978	0.15%	0.016%
68	15.875	2171	2174	2177	rVV	20716	26980	0.31%	0.034%
69	15.910	2177	2180	2186	rVB	40221	55152	0.64%	0.070%
70	16.039	2197	2202	2211	rBV2	165178	316319	3.68%	0.399%

71	16.139	2217	2219	2225	rVB7	20107	22782	0.26%	0.029%
72	16.198	2225	2229	2233	rBV	41313	55657	0.65%	0.070%
73	16.257	2235	2239	2245	rVB3	65446	116415	1.35%	0.147%
74	16.322	2245	2250	2254	rBV2	49225	73234	0.85%	0.092%
75	16.363	2254	2257	2261	rVB2	21117	26763	0.31%	0.034%

76	16.416	2262	2266	2272	rBV2	61180	96397	1.12%	0.122%
----	--------	------	------	------	------	-------	-------	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071822\
 Data File : BP010990.D
 Acq On : 18 Jul 2022 13:35
 Operator : CG/JU
 Sample : N3748-03
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH0E5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
 Title : SVOA CALIBRATION

77	16.486	2275	2278	2281	rVV	35604	50441	0.59%	0.064%
78	16.516	2281	2283	2291	rVB4	37568	58804	0.68%	0.074%
79	16.592	2291	2296	2299	rBV	33810	49383	0.57%	0.062%
80	16.663	2305	2308	2314	rVB3	26593	38811	0.45%	0.049%
81	16.892	2343	2347	2350	rBV6	11528	16948	0.20%	0.021%
82	17.110	2376	2384	2391	rBV	2732000	3812740	44.31%	4.812%
83	17.210	2395	2401	2413	rBV2	4098014	5763891	66.99%	7.275%
84	17.498	2446	2450	2458	rBV6	16216	29909	0.35%	0.038%
85	18.022	2535	2539	2543	rBV2	82821	108638	1.26%	0.137%
86	18.086	2547	2550	2558	rVB3	51954	81962	0.95%	0.103%
87	19.045	2709	2713	2718	rVB4	54670	75274	0.87%	0.095%
88	19.110	2721	2724	2727	rVV	51229	57578	0.67%	0.073%
89	19.269	2748	2751	2757	rBV8	30838	41870	0.49%	0.053%
90	19.469	2779	2785	2791	rBV	5541079	7120562	82.76%	8.988%
91	19.522	2791	2794	2801	rVB	97786	149791	1.74%	0.189%
92	20.963	3036	3039	3044	rBV	175244	213565	2.48%	0.270%
93	21.233	3080	3085	3094	rBV	4141683	5140517	59.74%	6.488%
94	23.433	3453	3459	3468	rVB2	4605461	8604294	100.00%	10.860%
95	23.586	3479	3485	3495	rVB2	2684960	5417686	62.96%	6.838%




Sum of corrected areas: 79226035

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071822\
Data File : BP010990.D
Acq On : 18 Jul 2022 13:35
Operator : CG/JU
Sample : N3748-03
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH0E5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

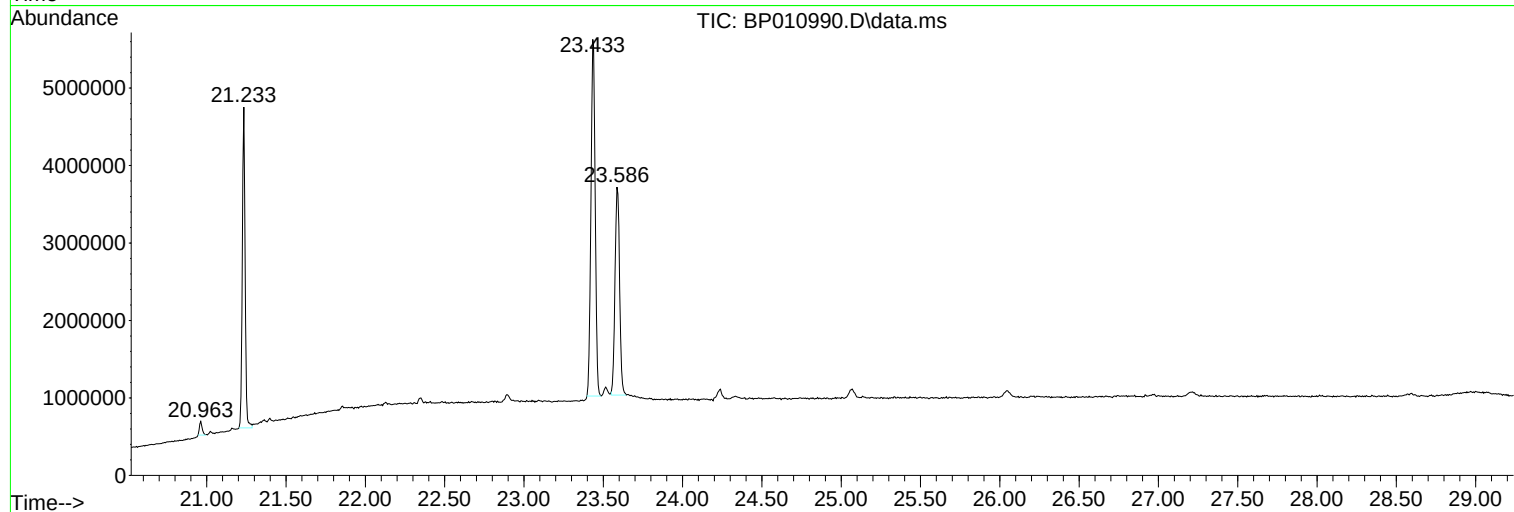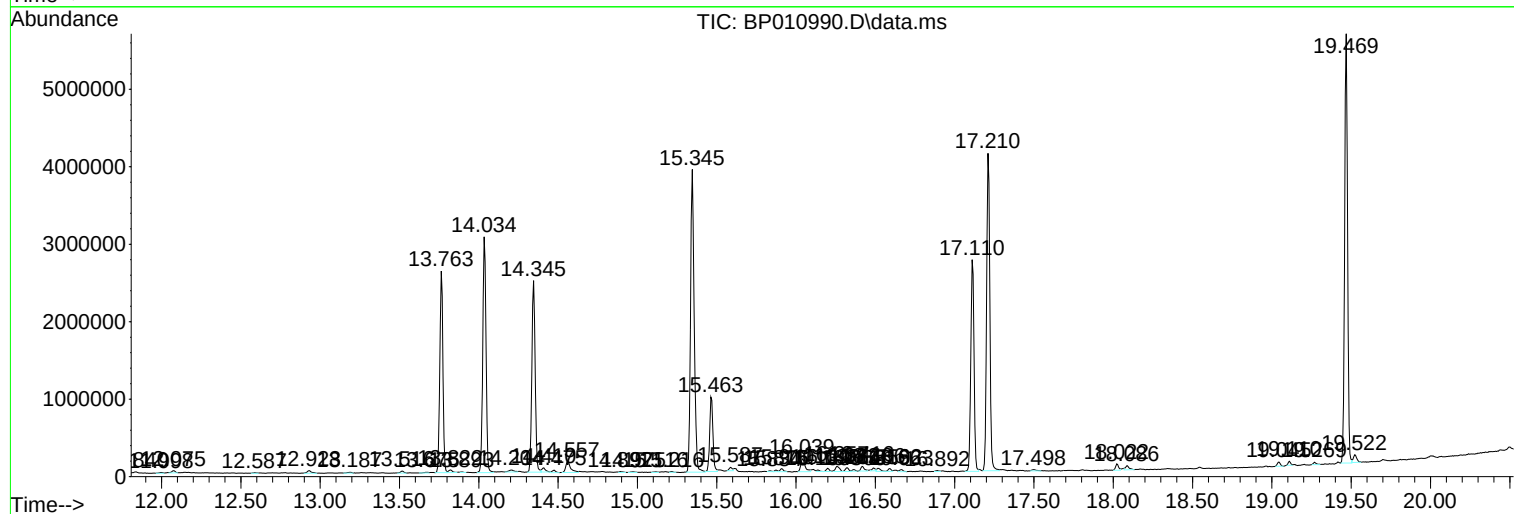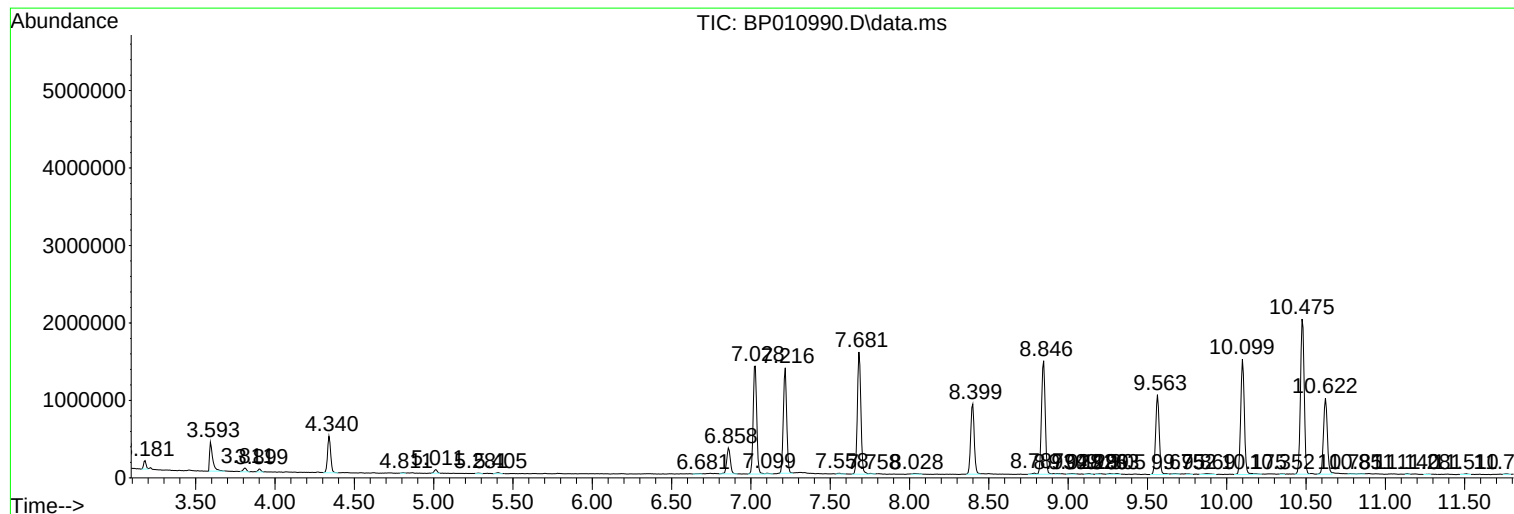

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071822\
Data File : BP010990.D
Acq On : 18 Jul 2022 13:35
Operator : CG/JU
Sample : N3748-03
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH0E5










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 1,3-Oxathiolane Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.340	5.35 ng/ul	647993	1,4-Dichlorobenzene-d4	7.681

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			1,3-Oxathiolane	90	C3H6OS	002094-97-5	91
2			1,3-Oxathiolane	90	C3H6OS	002094-97-5	56
3			Thiourea, methyl-	90	C2H6N2S	000598-52-7	50
4			Hydrazinecarboxylic acid, methyl...	90	C2H6N2O2	006294-89-9	45
5			Acrolein, 2-chloro-	90	C3H3ClO	000683-51-2	36

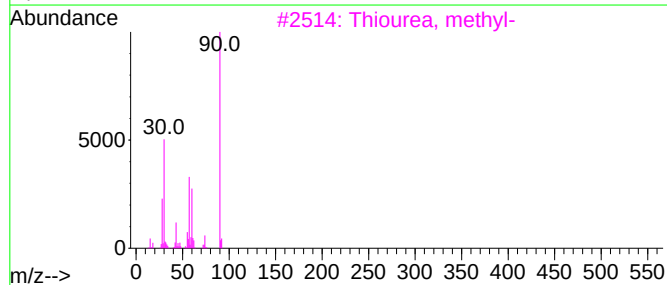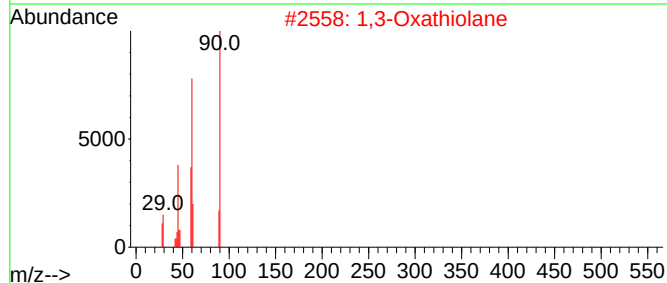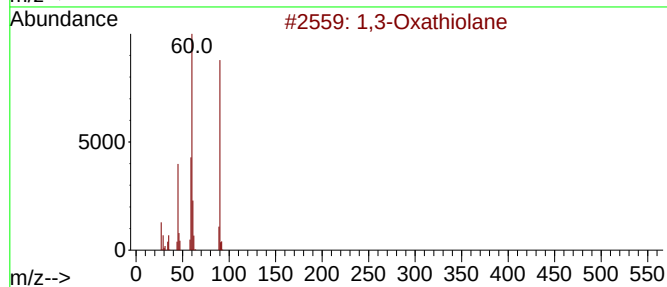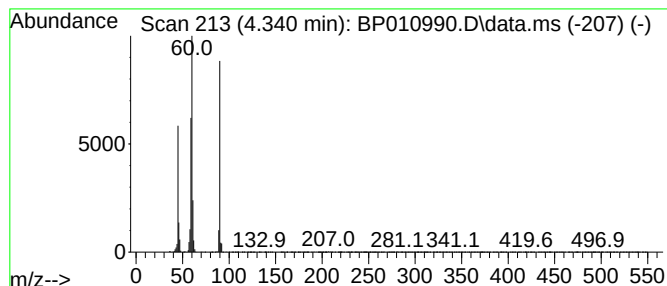

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071822\
Data File : BP010990.D
Acq On : 18 Jul 2022 13:35
Operator : CG/JU
Sample : N3748-03
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH0E5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
1,3-Oxathiolane	4.340	5.3	ng/ul	647993	1	7.681	2424170	20.0