

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071822\
 Data File : BP010993.D
 Acq On : 18 Jul 2022 15:18
 Operator : CG/JU
 Sample : N3748-07
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH0E9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
 Title : SVOA CALIBRATION

Signal : TIC: BP010993.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.181	12	16	19	rBV	111231	132654	1.82%	0.169%
2	3.211	19	21	25	rVB2	23901	25009	0.34%	0.032%
3	3.593	83	86	99	rBV	468560	631466	8.66%	0.802%
4	3.811	118	123	127	rVB	50070	69923	0.96%	0.089%
5	3.899	134	138	148	rVB	285748	387904	5.32%	0.493%
6	4.340	207	213	220	rBV	498286	667155	9.15%	0.847%
7	4.728	275	279	283	rVB7	5195	8396	0.12%	0.011%
8	5.011	323	327	332	rBV	65661	92293	1.27%	0.117%
9	5.275	370	372	378	rVB4	5544	8364	0.11%	0.011%
10	5.399	390	393	398	rBV2	14113	19962	0.27%	0.025%
11	5.699	441	444	448	rVB6	8338	10753	0.15%	0.014%
12	6.734	615	620	628	rVB6	6935	15055	0.21%	0.019%
13	6.857	635	641	654	rVB	341120	521912	7.16%	0.663%
14	7.022	662	669	680	rBV	1475842	2299184	31.53%	2.920%
15	7.099	680	682	690	rVB2	7726	12809	0.18%	0.016%
16	7.216	695	702	709	rBV	1405650	2106272	28.89%	2.675%
17	7.552	755	759	764	rBV2	9662	17761	0.24%	0.023%
18	7.681	773	781	792	rBV	1715006	2628581	36.05%	3.339%
19	7.752	792	793	798	rVB3	11559	11918	0.16%	0.015%
20	8.034	838	841	849	rVB8	9768	19229	0.26%	0.024%
21	8.399	895	903	911	rBV	939295	1475021	20.23%	1.874%
22	8.787	962	969	972	rBV4	17784	30420	0.42%	0.039%
23	8.846	972	979	987	rVV	1558290	2518704	34.54%	3.199%
24	8.928	991	993	997	rVB5	7869	9365	0.13%	0.012%
25	9.022	1004	1009	1018	rVB5	8437	21908	0.30%	0.028%
26	9.128	1023	1027	1030	rBV4	10820	14308	0.20%	0.018%
27	9.204	1035	1040	1044	rVV8	10168	19877	0.27%	0.025%
28	9.263	1046	1050	1055	rVV3	12307	24966	0.34%	0.032%
29	9.310	1055	1058	1063	rVB2	12330	19761	0.27%	0.025%
30	9.487	1083	1088	1091	rBV7	4427	8013	0.11%	0.010%
31	9.563	1093	1101	1109	rBV	1125711	1776233	24.36%	2.256%
32	9.875	1147	1154	1164	rVB10	13480	32423	0.44%	0.041%
33	10.098	1184	1192	1203	rBV	1601677	2545124	34.91%	3.233%
34	10.475	1248	1256	1263	rBV	2252824	3708370	50.86%	4.710%
35	10.528	1263	1265	1272	rVB8	12889	19695	0.27%	0.025%
36	10.622	1272	1281	1291	rBV	755273	1297668	17.80%	1.648%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071822\
 Data File : BP010993.D
 Acq On : 18 Jul 2022 15:18
 Operator : CG/JU
 Sample : N3748-07
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH0E9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
 Title : SVOA CALIBRATION

37	10.793	1307	1310	1314	rVB6	6893	10458	0.14%	0.013%
38	10.851	1317	1320	1324	rBV6	5409	8335	0.11%	0.011%
39	11.140	1363	1369	1373	rVB7	10005	15301	0.21%	0.019%
40	11.510	1425	1432	1437	rBV9	11942	24740	0.34%	0.031%

41	11.769	1469	1476	1480	rBV6	9192	14504	0.20%	0.018%
42	11.816	1480	1484	1485	rBV4	7405	8426	0.12%	0.011%
43	11.840	1485	1488	1491	rVB2	16882	20228	0.28%	0.026%
44	11.998	1508	1515	1519	rBV5	10761	20905	0.29%	0.027%
45	12.075	1523	1528	1533	rVV	30928	49078	0.67%	0.062%

46	12.592	1610	1616	1618	rBV7	6738	11220	0.15%	0.014%
47	12.928	1667	1673	1684	rVB6	39457	77994	1.07%	0.099%
48	13.181	1711	1716	1723	rVB6	16323	32285	0.44%	0.041%
49	13.251	1723	1728	1729	rBV5	6154	8715	0.12%	0.011%
50	13.398	1749	1753	1758	rVB7	7585	13077	0.18%	0.017%

51	13.516	1769	1773	1779	rBV2	26429	38742	0.53%	0.049%
52	13.663	1795	1798	1799	rBV3	8500	9222	0.13%	0.012%
53	13.763	1809	1815	1822	rBV	2770035	3777823	51.81%	4.799%
54	13.822	1822	1825	1829	rVB	31496	44153	0.61%	0.056%
55	13.928	1842	1843	1851	rVB8	9025	12913	0.18%	0.016%

56	14.034	1851	1861	1873	rBV	3229148	4735228	64.94%	6.015%
57	14.198	1885	1889	1896	rBV6	16261	35103	0.48%	0.045%
58	14.345	1907	1914	1921	rBV	2851054	4222710	57.92%	5.364%
59	14.404	1921	1924	1932	rVB	61620	96470	1.32%	0.123%
60	14.475	1932	1936	1942	rVB2	32409	49679	0.68%	0.063%

61	14.557	1944	1950	1962	rBV2	114124	249022	3.42%	0.316%
62	14.892	2006	2007	2012	rVB5	13226	14930	0.20%	0.019%
63	14.969	2012	2020	2024	rBV5	9799	24316	0.33%	0.031%
64	15.169	2048	2054	2055	rBV6	5865	10333	0.14%	0.013%
65	15.216	2059	2062	2066	rVB5	12995	15167	0.21%	0.019%

66	15.345	2072	2084	2097	rBV2	4091369	6639503	91.06%	8.434%
67	15.463	2098	2104	2118	rVV	921500	1353544	18.56%	1.719%
68	15.586	2121	2125	2127	rVV2	57907	87531	1.20%	0.111%
69	15.616	2127	2130	2136	rVB2	48375	71182	0.98%	0.090%
70	15.833	2164	2167	2170	rVV5	14116	17820	0.24%	0.023%

71	15.875	2170	2174	2177	rVV2	21115	30099	0.41%	0.038%
72	15.910	2177	2180	2186	rVB	47489	64558	0.89%	0.082%
73	16.039	2196	2202	2211	rBV2	161253	327556	4.49%	0.416%
74	16.104	2211	2213	2216	rVB2	18725	21764	0.30%	0.028%
75	16.198	2225	2229	2234	rBV	43125	58177	0.80%	0.074%

76	16.257	2235	2239	2245	rVB2	67452	115569	1.59%	0.147%
----	--------	------	------	------	------	-------	--------	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071822\
 Data File : BP010993.D
 Acq On : 18 Jul 2022 15:18
 Operator : CG/JU
 Sample : N3748-07
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BH0E9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
 Title : SVOA CALIBRATION

77	16.322	2245	2250	2254	rBV2	51220	77218	1.06%	0.098%
78	16.363	2254	2257	2261	rVV3	25374	30103	0.41%	0.038%
79	16.416	2262	2266	2272	rVV2	59748	96715	1.33%	0.123%
80	16.486	2275	2278	2281	rVV	37715	54459	0.75%	0.069%
81	16.516	2281	2283	2289	rVB4	41808	59914	0.82%	0.076%
82	16.586	2291	2295	2300	rBV	35978	53354	0.73%	0.068%
83	16.663	2305	2308	2312	rVB2	26326	34919	0.48%	0.044%
84	16.886	2342	2346	2350	rBV7	17279	30407	0.42%	0.039%
85	16.986	2360	2363	2367	rBV6	6311	8457	0.12%	0.011%
86	17.110	2376	2384	2390	rBV	2866735	3947208	54.14%	5.014%
87	17.210	2395	2401	2418	rVV2	3894045	5453878	74.80%	6.928%
88	17.498	2445	2450	2453	rBV6	16208	25118	0.34%	0.032%
89	17.804	2499	2502	2505	rBV4	8293	8269	0.11%	0.011%
90	18.022	2535	2539	2542	rBV3	48632	61632	0.85%	0.078%
91	18.086	2547	2550	2557	rVB3	46514	74235	1.02%	0.094%
92	18.539	2624	2627	2632	rBV7	16254	26752	0.37%	0.034%
93	19.039	2709	2712	2717	rVB4	45280	58432	0.80%	0.074%
94	19.110	2720	2724	2727	rBV	46909	61899	0.85%	0.079%
95	19.463	2779	2784	2791	rBV	4510133	6047967	82.95%	7.682%
96	19.522	2791	2794	2799	rVB	79606	113118	1.55%	0.144%
97	20.957	3035	3038	3044	rBV2	131123	205082	2.81%	0.261%
98	21.227	3080	3084	3090	rBV2	3437818	4372110	59.96%	5.554%
99	23.433	3452	3459	3469	rBV	3917724	7291208	100.00%	9.261%
100	23.586	3479	3485	3496	rVB2	2522880	4886759	67.02%	6.207%




Sum of corrected areas: 78726049

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071822\
Data File : BP010993.D
Acq On : 18 Jul 2022 15:18
Operator : CG/JU
Sample : N3748-07
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH0E9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

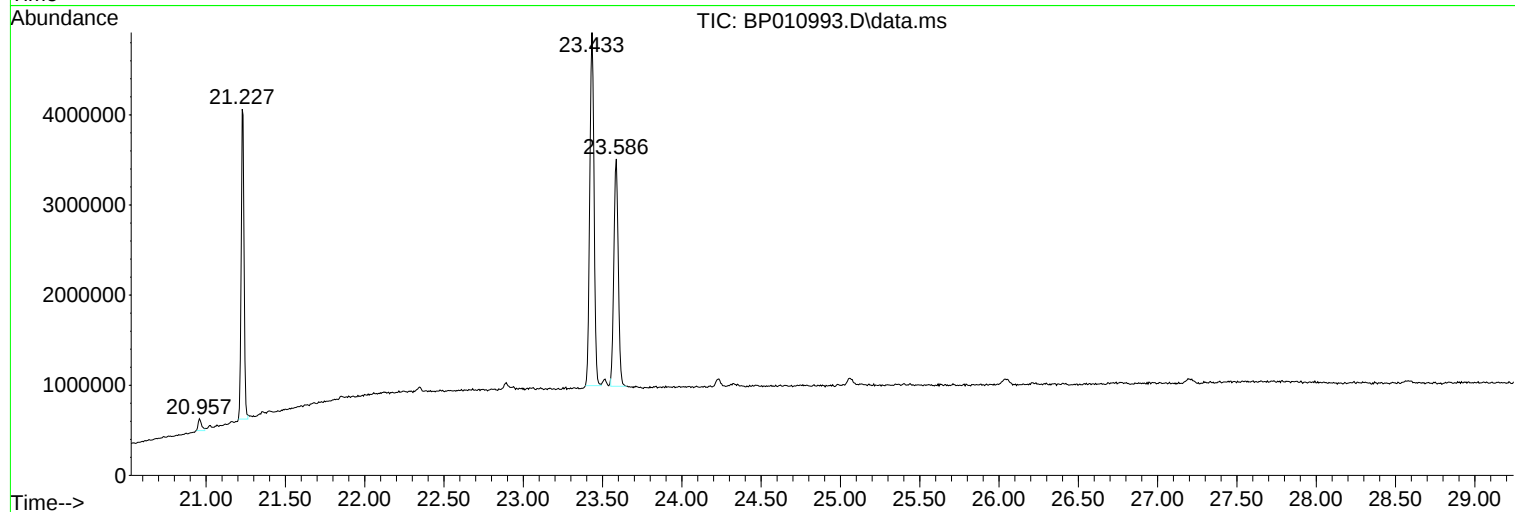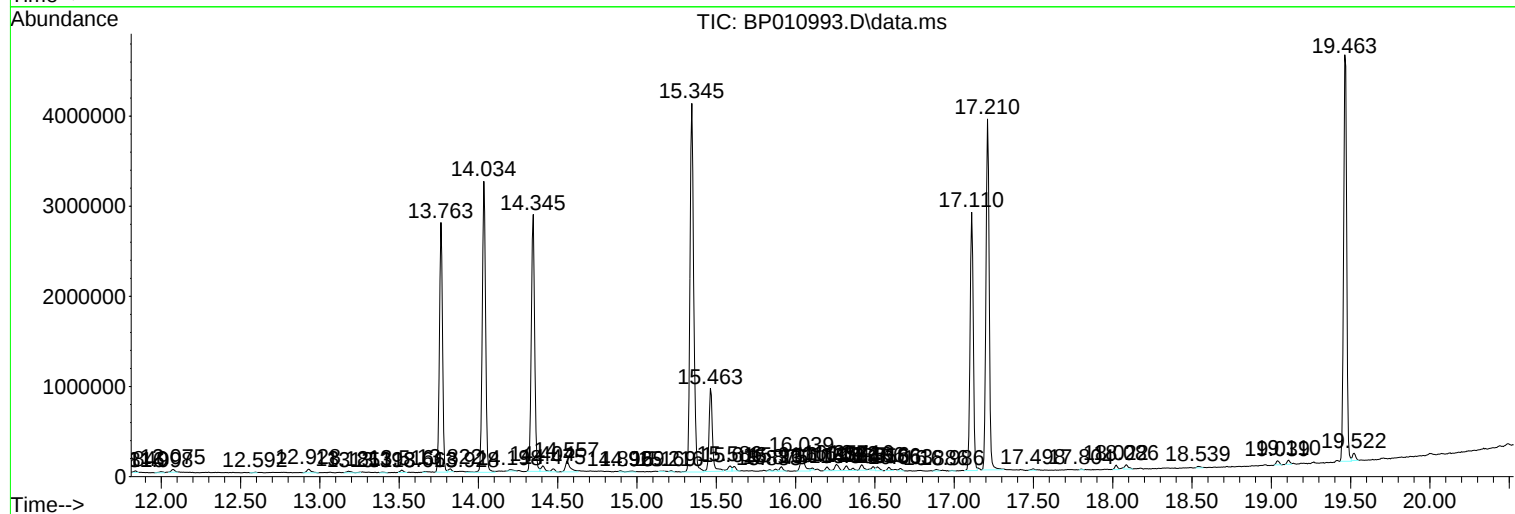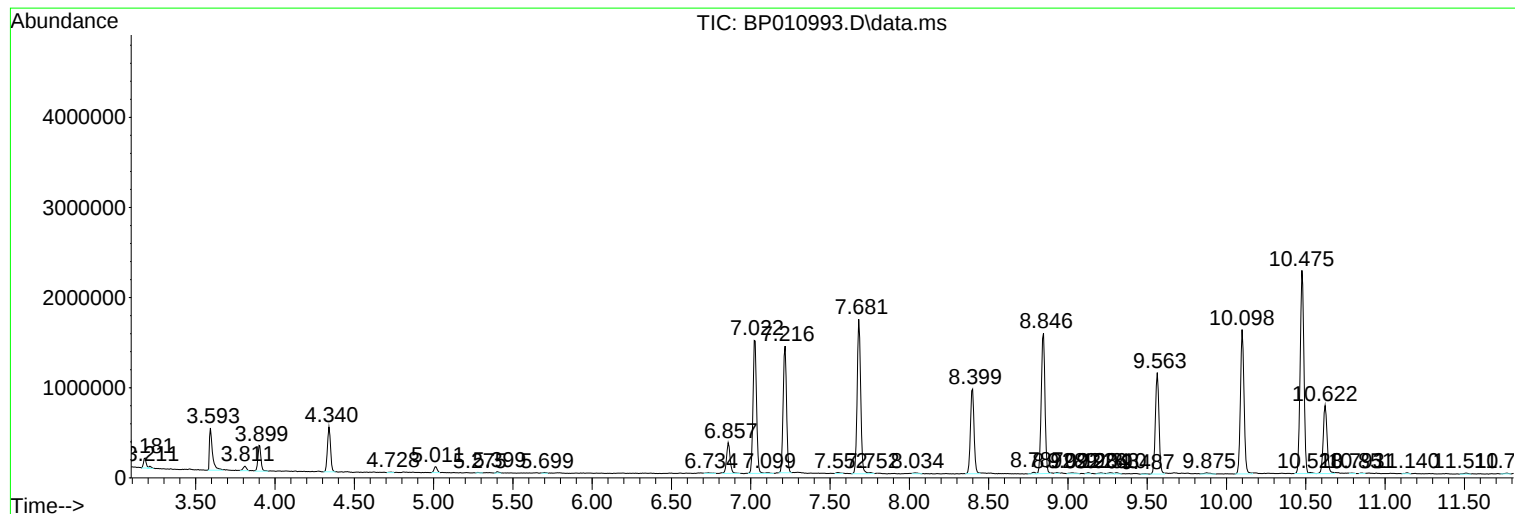

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071822\
Data File : BP010993.D
Acq On : 18 Jul 2022 15:18
Operator : CG/JU
Sample : N3748-07
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH0E9










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 1,3-Oxathiolane Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.340	5.08 ng/ul	667155	1,4-Dichlorobenzene-d4	7.681

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			1,3-Oxathiolane	90	C3H6OS	002094-97-5	90
2			1,3-Oxathiolane	90	C3H6OS	002094-97-5	64
3			Hydrazinecarboxylic acid, methyl...	90	C2H6N2O2	006294-89-9	45
4			Acrolein, 2-chloro-	90	C3H3ClO	000683-51-2	36
5			3-Thietanol	90	C3H6OS	010304-16-2	33

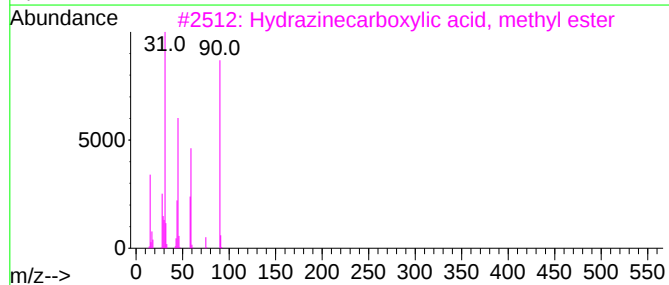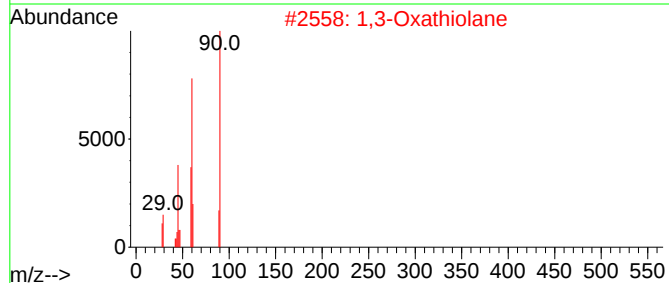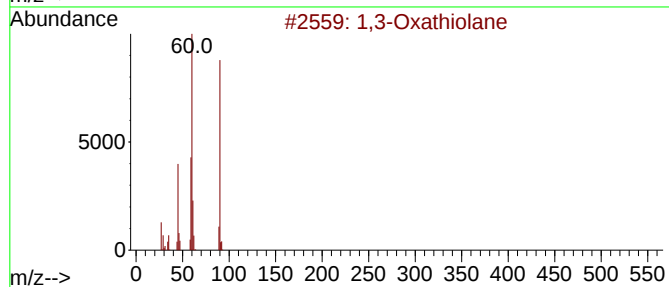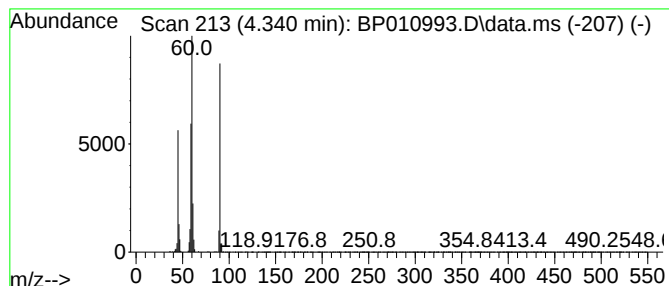

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071822\
Data File : BP010993.D
Acq On : 18 Jul 2022 15:18
Operator : CG/JU
Sample : N3748-07
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BH0E9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
1,3-Oxathiolane	4.340	5.1	ng/ul	667155	1	7.681	2628580	20.0