

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071822\
 Data File : BP011015.D
 Acq On : 19 Jul 2022 04:27
 Operator : CG/JU
 Sample : PB146234BL
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK234

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011015.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.181	12	16	21	rBV	161341	183277	2.28%	0.205%
2	3.587	82	85	102	rBV	1594134	2284224	28.43%	2.552%
3	3.905	135	139	143	rVB	39968	54639	0.68%	0.061%
4	6.857	634	641	655	rBV	1790039	2702540	33.63%	3.019%
5	7.022	663	669	682	rVB	1560157	2358026	29.35%	2.634%
6	7.210	694	701	715	rBV	1911298	2915503	36.28%	3.257%
7	7.675	774	780	788	rVB	1616948	2535844	31.56%	2.833%
8	8.393	895	902	917	rBV	2125300	3283755	40.87%	3.669%
9	8.840	970	978	987	rBV	1631426	2583180	32.15%	2.886%
10	9.557	1093	1100	1111	rBV	1235851	1929242	24.01%	2.155%
11	10.092	1184	1191	1205	rBV	1804083	2987424	37.18%	3.338%
12	10.469	1247	1255	1264	rBV	2039681	3380414	42.07%	3.777%
13	10.616	1270	1280	1296	rBV	1953275	3349229	41.68%	3.742%
14	12.069	1522	1527	1533	rBV2	36336	61362	0.76%	0.069%
15	13.063	1689	1696	1699	rBV9	4136	8700	0.11%	0.010%
16	13.298	1733	1736	1742	rVB7	6737	9738	0.12%	0.011%
17	13.757	1808	1814	1824	rBV	2999670	4082995	50.81%	4.562%
18	14.028	1851	1860	1870	rBV	3447527	4945146	61.54%	5.525%
19	14.339	1905	1913	1922	rBV	2780874	3877950	48.26%	4.333%
20	14.557	1943	1950	1973	rBV	990972	1891853	23.54%	2.114%
21	15.339	2076	2083	2093	rBV	4249747	6072475	75.57%	6.784%
22	15.463	2098	2104	2116	rVV	1124375	1579405	19.66%	1.765%
23	15.580	2120	2124	2133	rVB2	55949	88990	1.11%	0.099%
24	16.127	2213	2217	2225	rVB6	17609	30366	0.38%	0.034%
25	16.786	2324	2329	2332	rVB6	10419	14895	0.19%	0.017%
26	16.892	2343	2347	2348	rBV3	7107	8095	0.10%	0.009%
27	17.104	2377	2383	2390	rBV	3009968	4263300	53.06%	4.763%
28	17.204	2394	2400	2416	rBV2	4616074	6423507	79.94%	7.177%
29	19.033	2708	2711	2717	rVB3	55945	71641	0.89%	0.080%
30	19.104	2719	2723	2727	rBV	56080	77133	0.96%	0.086%
31	19.463	2778	2784	2793	rBV	5641470	7419159	92.33%	8.289%
32	21.227	3079	3084	3093	rBV	3895621	4925755	61.30%	5.503%
33	23.427	3451	3458	3467	rBV2	4250038	8035242	100.00%	8.977%
34	23.580	3478	3484	3493	rVB2	2584875	5072384	63.13%	5.667%

Sum of corrected areas: 89507388




Instrument :
BNA_P
ClientSampleId :
SBLK234

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071822\
Data File : BP011015.D
Acq On : 19 Jul 2022 04:27
Operator : CG/JU
Sample : PB146234BL
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK234

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

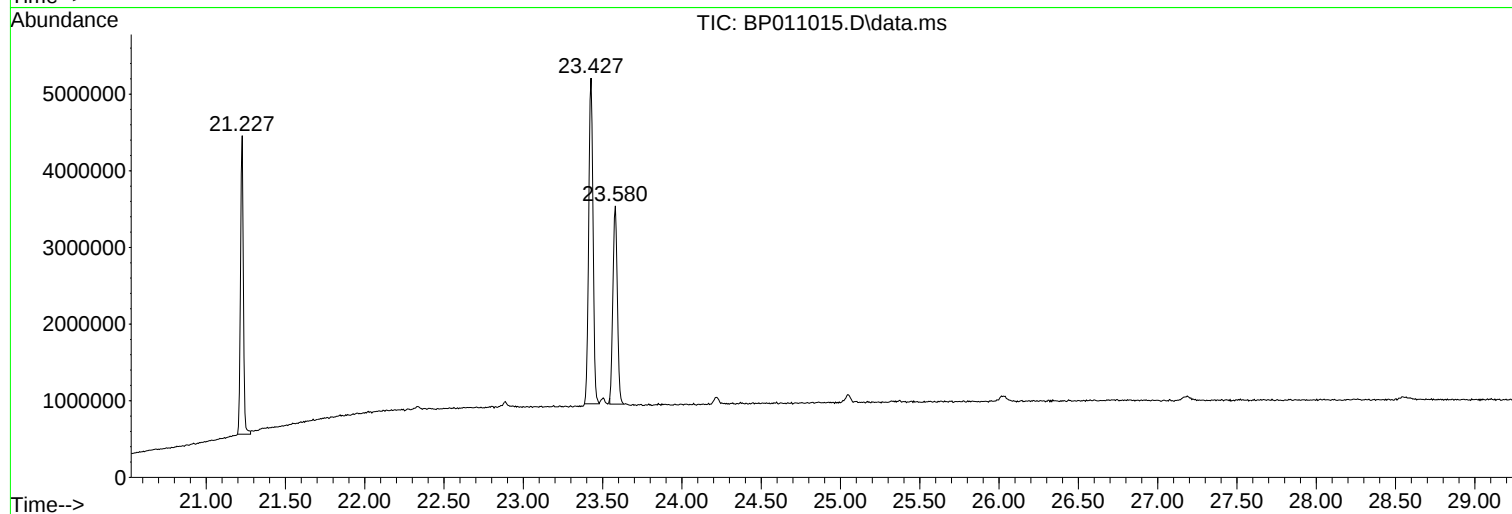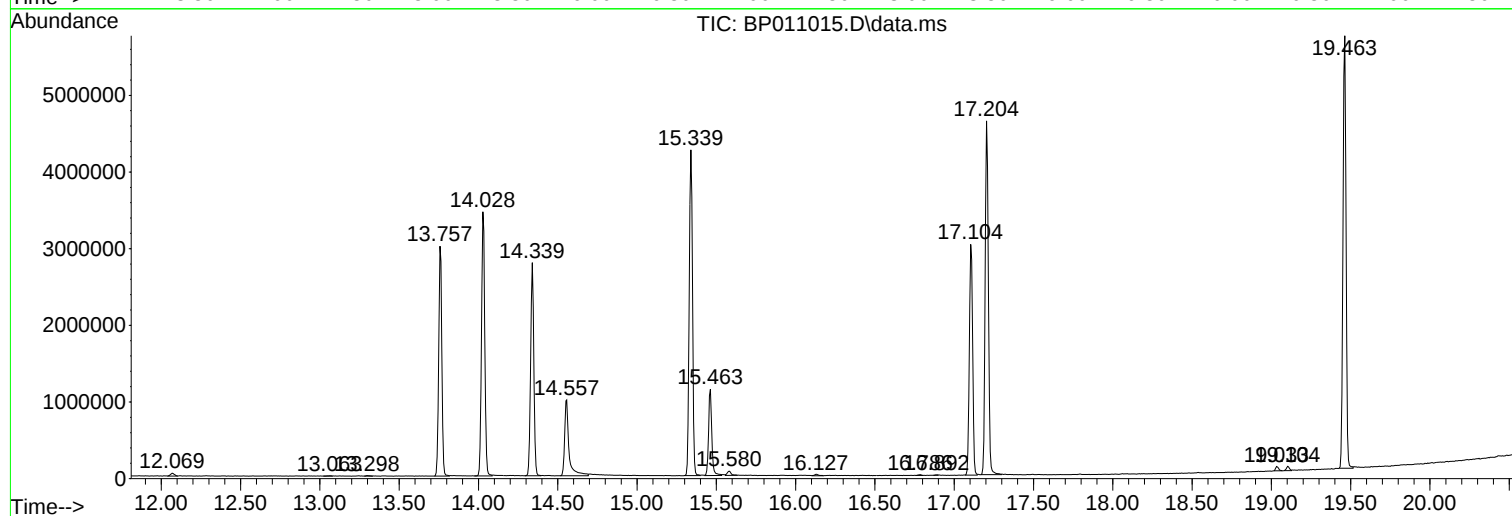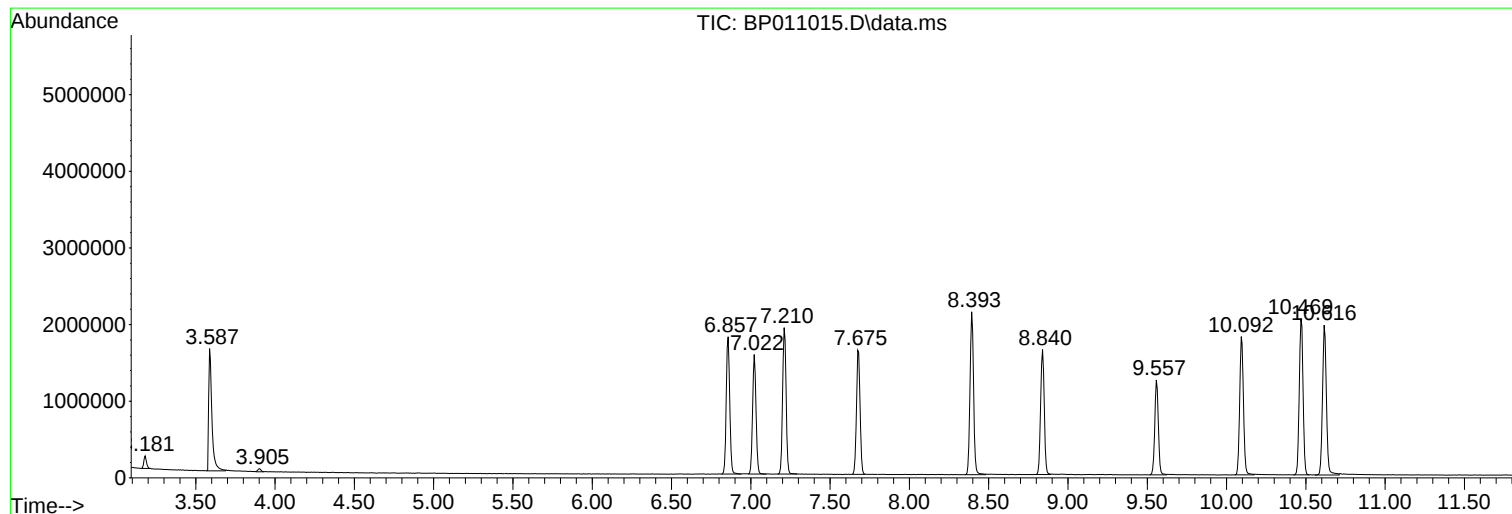

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071822\
Data File : BP011015.D
Acq On : 19 Jul 2022 04:27
Operator : CG/JU
Sample : PB146234BL
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK234

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071822\
Data File : BP011015.D
Acq On : 19 Jul 2022 04:27
Operator : CG/JU
Sample : PB146234BL
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK234

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc