

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071822\
 Data File : BP011016.D
 Acq On : 19 Jul 2022 05:01
 Operator : CG/JU
 Sample : N3710-01
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 H0B38

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011016.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.181	12	16	22	rVB	136218	163501	1.60%	0.176%
2	3.452	60	62	71	rVB	40962	65679	0.64%	0.071%
3	3.593	83	86	101	rBV	643671	898230	8.78%	0.964%
4	3.811	118	123	132	rVB	57078	96003	0.94%	0.103%
5	3.899	134	138	144	rVB	56244	73101	0.71%	0.078%
6	5.281	370	373	379	rVB5	9492	16070	0.16%	0.017%
7	5.405	390	394	399	rVB2	14785	20630	0.20%	0.022%
8	6.857	631	641	650	rBV	396542	610388	5.97%	0.655%
9	7.022	662	669	679	rBV	1737359	2590037	25.33%	2.781%
10	7.105	679	683	689	rVB3	10380	16597	0.16%	0.018%
11	7.210	694	701	710	rBV	1597873	2405101	23.52%	2.582%
12	7.305	712	717	722	rVB6	10606	16495	0.16%	0.018%
13	7.675	773	780	789	rBV	1855823	2911922	28.48%	3.126%
14	8.393	895	902	917	rBV	1126053	1719695	16.82%	1.846%
15	8.840	971	978	987	rBV	1796790	2848426	27.86%	3.058%
16	8.963	994	999	1003	rBV2	16063	25708	0.25%	0.028%
17	9.004	1003	1006	1014	rVB10	8887	19927	0.19%	0.021%
18	9.557	1092	1100	1108	rBV	1283294	1988819	19.45%	2.135%
19	10.093	1184	1191	1203	rBV	1780660	2869792	28.07%	3.081%
20	10.469	1247	1255	1265	rVB	2373467	3860217	37.75%	4.144%
21	10.616	1270	1280	1299	rBV	1297483	2233849	21.85%	2.398%
22	11.287	1387	1394	1398	rBV9	7406	14811	0.14%	0.016%
23	12.069	1522	1527	1534	rVB	40246	65368	0.64%	0.070%
24	12.287	1558	1564	1568	rVB9	6544	11508	0.11%	0.012%
25	12.687	1630	1632	1640	rBV9	8237	15252	0.15%	0.016%
26	12.951	1670	1677	1682	rVB9	11903	20168	0.20%	0.022%
27	13.245	1721	1727	1730	rVV2	14714	21756	0.21%	0.023%
28	13.304	1730	1737	1745	rVB2	7061	15357	0.15%	0.016%
29	13.557	1776	1780	1783	rBV4	14796	17794	0.17%	0.019%
30	13.757	1806	1814	1827	rBV	3352513	4516489	44.17%	4.849%
31	14.028	1851	1860	1876	rBV	3699830	5355078	52.37%	5.749%
32	14.339	1905	1913	1923	rBV	2990041	4272830	41.79%	4.587%
33	14.557	1944	1950	1959	rBV3	149839	317991	3.11%	0.341%
34	14.639	1959	1964	1974	rVB	76164	150329	1.47%	0.161%
35	14.769	1984	1986	1993	rVB8	8112	11816	0.12%	0.013%
36	15.122	2041	2046	2050	rBV	16221	32085	0.31%	0.034%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071822\
 Data File : BP011016.D
 Acq On : 19 Jul 2022 05:01
 Operator : CG/JU
 Sample : N3710-01
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 H0B38

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
 Title : SVOA CALIBRATION

37	15.157	2050	2052	2057	rVB2	12258	15084	0.15%	0.016%
38	15.339	2076	2083	2097	rBV	4941511	6779817	66.31%	7.279%
39	15.463	2097	2104	2118	rVV	1341929	1850210	18.10%	1.986%
40	15.581	2119	2124	2131	rVB	56295	88037	0.86%	0.095%
41	15.910	2177	2180	2185	rVB7	6735	10436	0.10%	0.011%
42	16.128	2214	2217	2223	rVB6	19742	29051	0.28%	0.031%
43	16.257	2234	2239	2245	rVB9	9782	18594	0.18%	0.020%
44	16.780	2324	2328	2333	rVB8	11043	16040	0.16%	0.017%
45	16.886	2341	2346	2351	rBV6	14307	25318	0.25%	0.027%
46	17.039	2368	2372	2376	rBV7	6249	11833	0.12%	0.013%
47	17.104	2377	2383	2390	rVV	3318222	4618276	45.17%	4.958%
48	17.204	2394	2400	2414	rVB2	5385521	7644598	74.77%	8.207%
49	17.516	2450	2453	2458	rVB4	30647	45242	0.44%	0.049%
50	17.798	2497	2501	2508	rVB	249311	301049	2.94%	0.323%
51	18.016	2534	2538	2542	rBV4	37508	53657	0.52%	0.058%
52	18.304	2584	2587	2591	rBV5	21952	32000	0.31%	0.034%
53	18.945	2693	2696	2700	rVB3	36049	36837	0.36%	0.040%
54	19.033	2708	2711	2715	rBV	69069	88602	0.87%	0.095%
55	19.074	2715	2718	2720	rVV	95263	101430	0.99%	0.109%
56	19.104	2720	2723	2726	rVB	64936	80368	0.79%	0.086%
57	19.463	2778	2784	2792	rBV	7055966	9289104	90.85%	9.972%
58	20.957	3034	3038	3043	rBV2	197507	301997	2.95%	0.324%
59	21.227	3079	3084	3093	rBV	4509402	5490432	53.70%	5.894%
60	23.427	3451	3458	3467	rBV2	5291809	10224771	100.00%	10.977%
61	23.580	3478	3484	3493	rVB2	3006011	5706747	55.81%	6.127%




Sum of corrected areas: 93148349

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071822\
Data File : BP011016.D
Acq On : 19 Jul 2022 05:01
Operator : CG/JU
Sample : N3710-01
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0B38

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

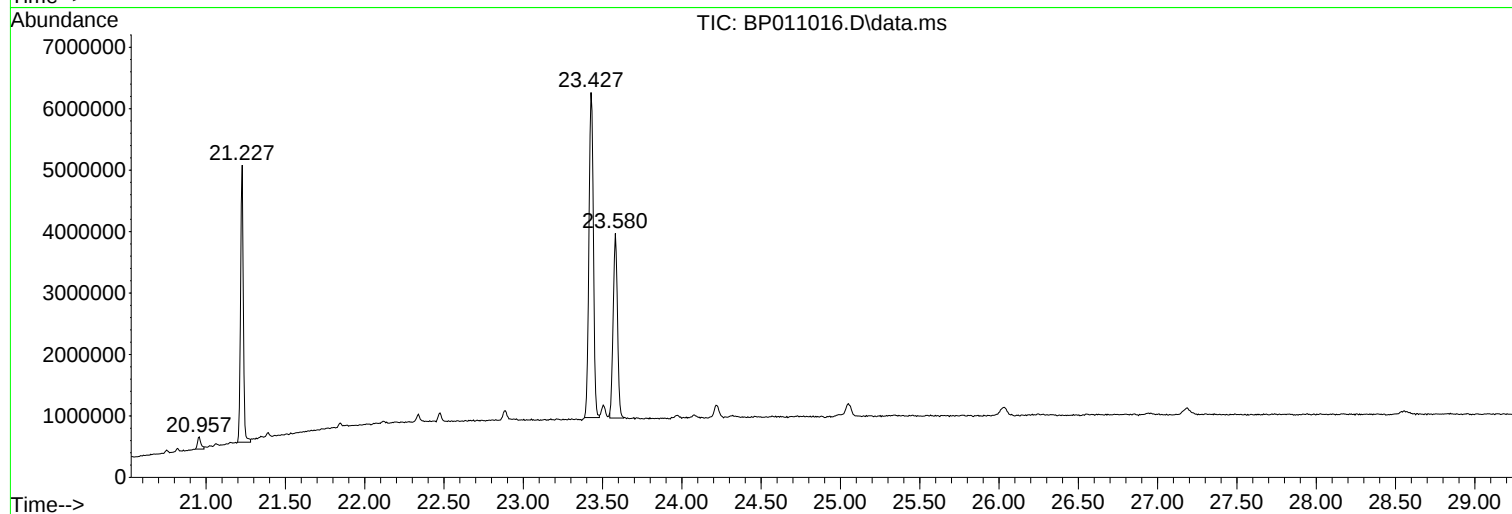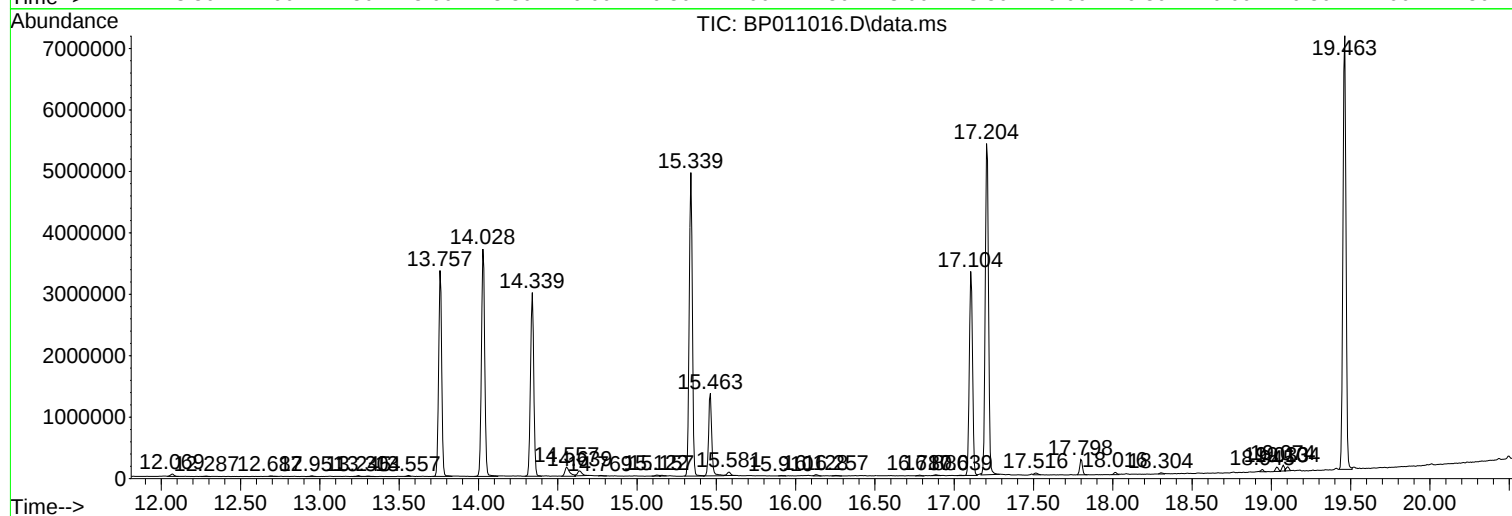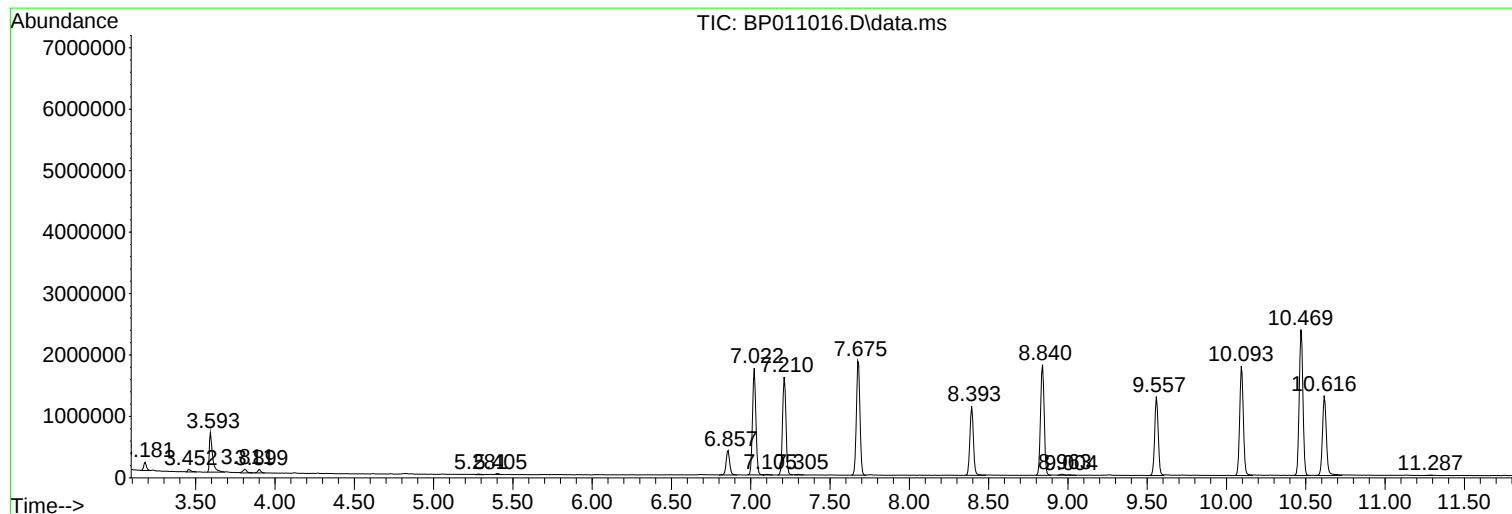

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071822\
Data File : BP011016.D
Acq On : 19 Jul 2022 05:01
Operator : CG/JU
Sample : N3710-01
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0B38

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071822\
Data File : BP011016.D
Acq On : 19 Jul 2022 05:01
Operator : CG/JU
Sample : N3710-01
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0B38

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc