

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071822\
 Data File : BP011021.D
 Acq On : 19 Jul 2022 07:52
 Operator : CG/JU
 Sample : N3704-07
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AQ1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011021.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.146	7	10	13	rBV	34660	46834	0.53%	0.049%
2	3.181	13	16	26	rVB	129182	178222	2.04%	0.187%
3	3.275	28	32	37	rVB	51660	72290	0.83%	0.076%
4	3.452	60	62	71	rBV	53241	75684	0.86%	0.079%
5	3.593	82	86	103	rBV	680236	1098019	12.54%	1.153%
6	3.810	115	123	131	rVB2	57528	122488	1.40%	0.129%
7	3.899	134	138	144	rVB	80473	109355	1.25%	0.115%
8	4.363	212	217	221	rBV2	54978	78269	0.89%	0.082%
9	4.416	221	226	237	rVB	726514	1061774	12.13%	1.115%
10	4.828	289	296	299	rBV5	15016	30659	0.35%	0.032%
11	5.198	355	359	369	rVB	99557	143713	1.64%	0.151%
12	5.328	376	381	390	rBV	116391	203246	2.32%	0.213%
13	5.404	390	394	397	rBV	13172	16866	0.19%	0.018%
14	5.540	413	417	422	rBV6	9181	13749	0.16%	0.014%
15	5.598	425	427	435	rVB9	8008	11314	0.13%	0.012%
16	5.698	439	444	447	rVV	71512	113507	1.30%	0.119%
17	5.728	447	449	456	rVV3	42185	70565	0.81%	0.074%
18	5.787	456	459	464	rVB4	9327	11883	0.14%	0.012%
19	6.687	610	612	616	rVB3	12146	13305	0.15%	0.014%
20	6.769	621	626	630	rBV2	18317	31385	0.36%	0.033%
21	6.828	630	636	638	rVV	194346	309835	3.54%	0.325%
22	6.857	638	641	654	rVB	402426	610274	6.97%	0.641%
23	7.022	662	669	678	rBV	1486173	2255721	25.76%	2.369%
24	7.098	678	682	689	rVB	41035	62754	0.72%	0.066%
25	7.210	694	701	713	rBV	1438341	2171894	24.81%	2.281%
26	7.322	713	720	725	rVV2	33475	59801	0.68%	0.063%
27	7.375	725	729	733	rVV7	11512	17367	0.20%	0.018%
28	7.675	772	780	787	rBV	1500059	2327943	26.59%	2.445%
29	7.745	787	792	799	rBV	165520	270862	3.09%	0.284%
30	7.928	817	823	832	rBV2	90957	156489	1.79%	0.164%
31	8.257	876	879	884	rVB6	7750	12109	0.14%	0.013%
32	8.392	895	902	914	rBV	1087945	1735180	19.82%	1.822%
33	8.504	917	921	927	rVV6	13263	28029	0.32%	0.029%
34	8.575	929	933	938	rVB6	8009	15344	0.18%	0.016%
35	8.775	962	967	971	rBV7	13226	25017	0.29%	0.026%
36	8.839	971	978	987	rVB	1609245	2559417	29.23%	2.688%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071822\
 Data File : BP011021.D
 Acq On : 19 Jul 2022 07:52
 Operator : CG/JU
 Sample : N3704-07
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AQ1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
 Title : SVOA CALIBRATION

37	8.963	996	999	1003	rVV3	17622	19666	0.22%	0.021%
38	9.010	1003	1007	1013	rVB4	19604	31645	0.36%	0.033%
39	9.210	1036	1041	1042	rBV5	8349	11947	0.14%	0.013%
40	9.257	1045	1049	1055	rVB	19403	34802	0.40%	0.037%
41	9.410	1069	1075	1081	rBV	42177	71964	0.82%	0.076%
42	9.557	1092	1100	1108	rBV	1174759	1861556	21.26%	1.955%
43	9.728	1123	1129	1137	rBV	131786	264790	3.02%	0.278%
44	9.804	1138	1142	1152	rVB5	21305	42572	0.49%	0.045%
45	10.004	1171	1176	1184	rVB5	8204	18001	0.21%	0.019%
46	10.092	1184	1191	1205	rBV	1661950	2726286	31.14%	2.863%
47	10.469	1246	1255	1270	rVB	1931799	3215464	36.73%	3.377%
48	10.616	1270	1280	1293	rBV	682515	1226144	14.01%	1.288%
49	11.133	1360	1368	1373	rBV2	17381	33383	0.38%	0.035%
50	11.281	1388	1393	1401	rBV6	24024	43993	0.50%	0.046%
51	11.986	1511	1513	1517	rBV5	7168	9160	0.10%	0.010%
52	12.069	1520	1527	1533	rVB	40114	67423	0.77%	0.071%
53	12.263	1554	1560	1568	rBV	39289	77026	0.88%	0.081%
54	12.616	1617	1620	1625	rBV6	7911	10813	0.12%	0.011%
55	12.951	1673	1677	1679	rBV5	11270	16028	0.18%	0.017%
56	12.975	1679	1681	1687	rVV5	8687	13051	0.15%	0.014%
57	13.057	1691	1695	1699	rBV7	5856	9002	0.10%	0.009%
58	13.169	1709	1714	1723	rBV3	31844	56395	0.64%	0.059%
59	13.245	1723	1727	1731	rBV7	5685	9385	0.11%	0.010%
60	13.304	1733	1737	1742	rVB7	10408	16744	0.19%	0.018%
61	13.757	1807	1814	1823	rBV	3292902	4510511	51.52%	4.737%
62	13.827	1823	1826	1830	rVV4	15981	25160	0.29%	0.026%
63	13.863	1830	1832	1838	rVB7	6840	11048	0.13%	0.012%
64	14.027	1852	1860	1870	rBV	3684297	5284140	60.36%	5.549%
65	14.251	1894	1898	1901	rVB4	20175	25248	0.29%	0.027%
66	14.339	1906	1913	1926	rBV	2707432	3878821	44.30%	4.073%
67	14.557	1945	1950	1960	rBV	194413	365446	4.17%	0.384%
68	14.774	1982	1987	1992	rVB9	11724	19160	0.22%	0.020%
69	15.157	2047	2052	2055	rBV	16167	24266	0.28%	0.025%
70	15.210	2058	2061	2066	rVB6	14838	16913	0.19%	0.018%
71	15.339	2076	2083	2090	rBV	4899178	6627812	75.70%	6.960%
72	15.463	2097	2104	2117	rBV	1242638	1763106	20.14%	1.851%
73	15.580	2118	2124	2129	rVB2	57691	102482	1.17%	0.108%
74	15.910	2178	2180	2184	rVB5	7605	9439	0.11%	0.010%
75	16.045	2197	2203	2206	rBV8	17222	33016	0.38%	0.035%
76	16.133	2215	2218	2222	rVB5	23488	32016	0.37%	0.034%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071822\
 Data File : BP011021.D
 Acq On : 19 Jul 2022 07:52
 Operator : CG/JU
 Sample : N3704-07
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AQ1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
 Title : SVOA CALIBRATION

77	16.580	2291	2294	2300	rVB7	14515	25947	0.30%	0.027%
78	16.786	2325	2329	2331	rVB5	7519	9130	0.10%	0.010%
79	16.880	2341	2345	2349	rBV6	14811	27289	0.31%	0.029%
80	17.104	2377	2383	2394	rBV	3111266	4429677	50.60%	4.652%
81	17.204	2394	2400	2415	rBV2	5170420	7326386	83.68%	7.694%
82	17.492	2445	2449	2456	rBV2	41982	58638	0.67%	0.062%
83	17.663	2475	2478	2480	rBV4	9472	13605	0.16%	0.014%
84	17.757	2491	2494	2497	rBV2	15977	19069	0.22%	0.020%
85	17.798	2498	2501	2505	rVB	29784	36133	0.41%	0.038%
86	18.015	2535	2538	2543	rBV5	31374	48631	0.56%	0.051%
87	18.092	2545	2551	2556	rVV	5083924	6092625	69.59%	6.398%
88	18.286	2581	2584	2589	rBV6	14900	25498	0.29%	0.027%
89	18.762	2662	2665	2674	rVB	71388	103886	1.19%	0.109%
90	19.039	2708	2712	2719	rBV3	70292	113839	1.30%	0.120%
91	19.104	2720	2723	2726	rBV	63892	86685	0.99%	0.091%
92	19.239	2743	2746	2753	rBV	80436	105620	1.21%	0.111%
93	19.462	2778	2784	2791	rBV	6670601	8690897	99.27%	9.126%
94	20.951	3034	3037	3043	rBV	323805	403744	4.61%	0.424%
95	21.227	3079	3084	3090	rBV	4171452	5006657	57.19%	5.258%
96	23.427	3452	3458	3466	rVB2	4561318	8754990	100.00%	9.194%
97	23.580	3478	3484	3495	rVB2	2622651	5111383	58.38%	5.368%




Sum of corrected areas: 95227316

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071822\
Data File : BP011021.D
Acq On : 19 Jul 2022 07:52
Operator : CG/JU
Sample : N3704-07
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AQ1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

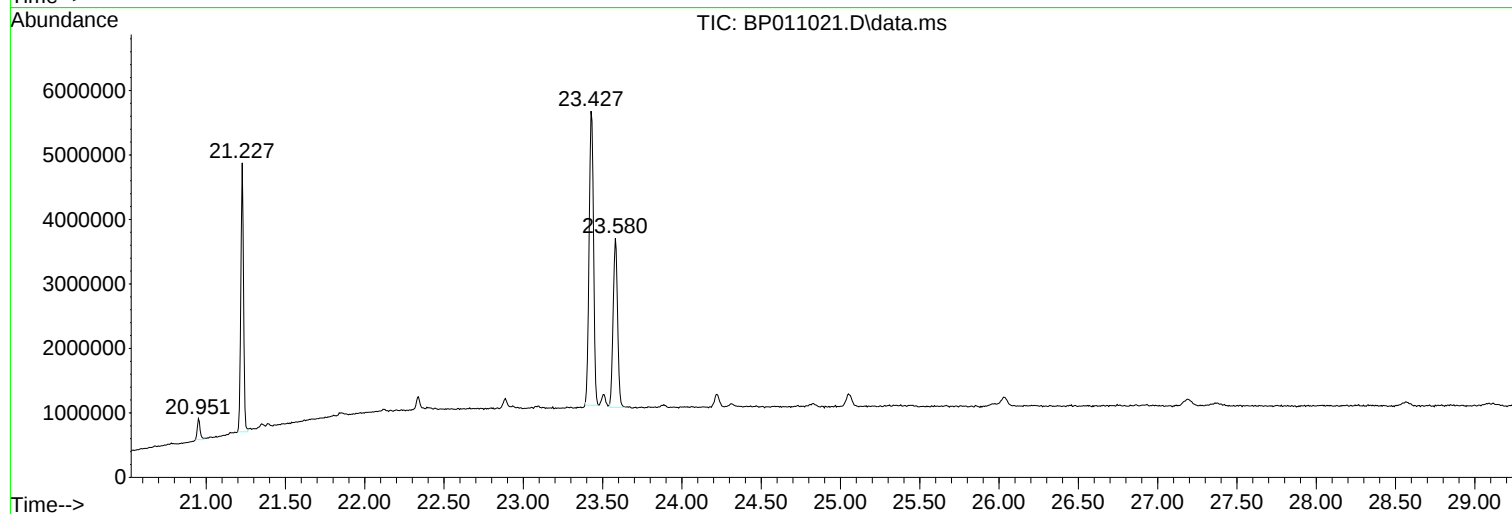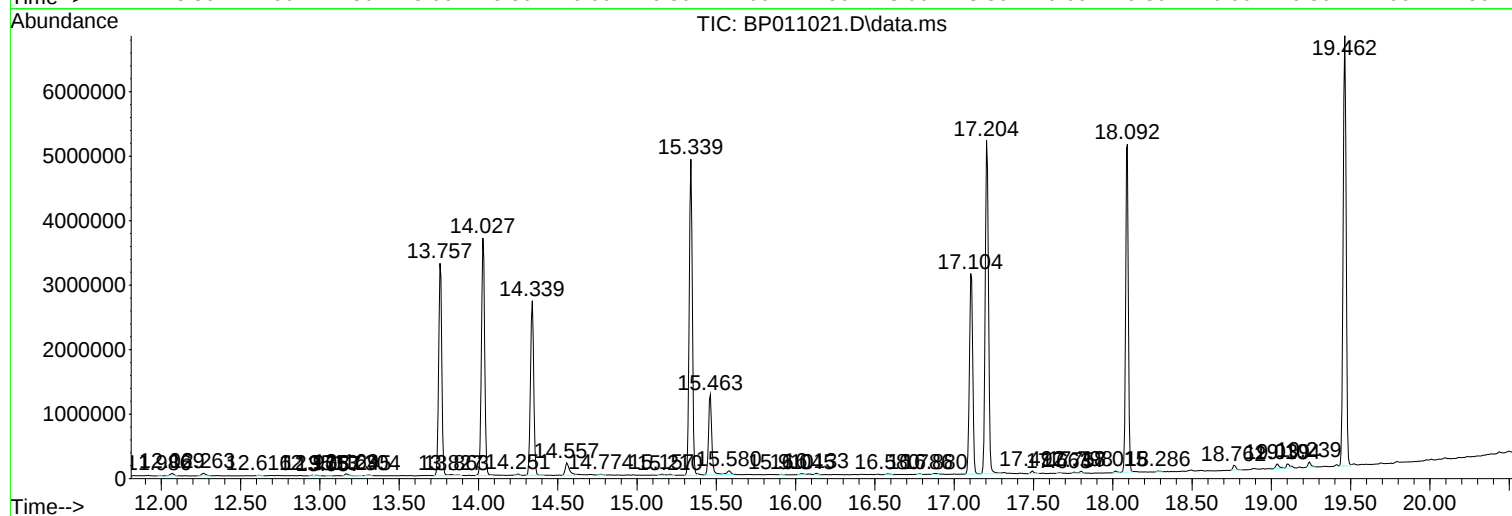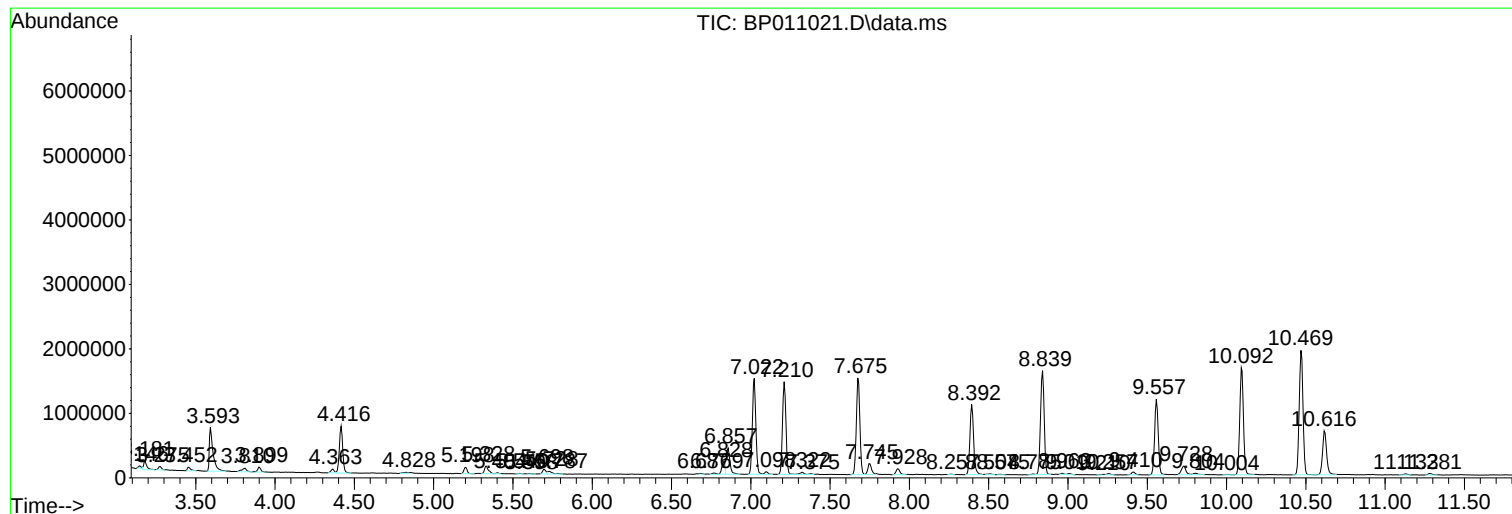

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071822\
Data File : BP011021.D
Acq On : 19 Jul 2022 07:52
Operator : CG/JU
Sample : N3704-07
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AQ1










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 1-Hexanol, 2-ethyl- Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.745	2.33 ng/ul	270862	1,4-Dichlorobenzene-d4	7.675

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	1-Hexanol, 2-ethyl-			130	C8H18O	000104-76-7	78
2	1-Hexanol, 2-ethyl-			130	C8H18O	000104-76-7	78
3	1-Hexanol, 2-ethyl-			130	C8H18O	000104-76-7	64
4	Carbonic acid, isobutyl 2-ethylh...			230	C13H26O3	1000383-13-3	59
5	Heptane, 1,1'-oxybis-			214	C14H30O	000629-64-1	59

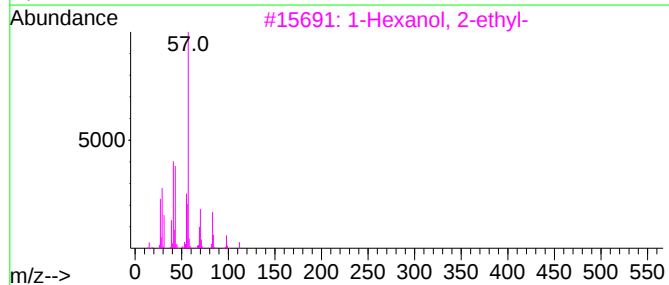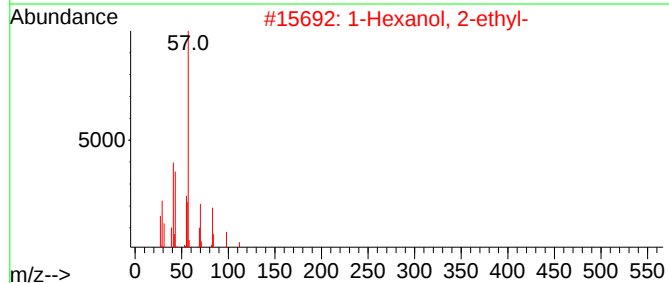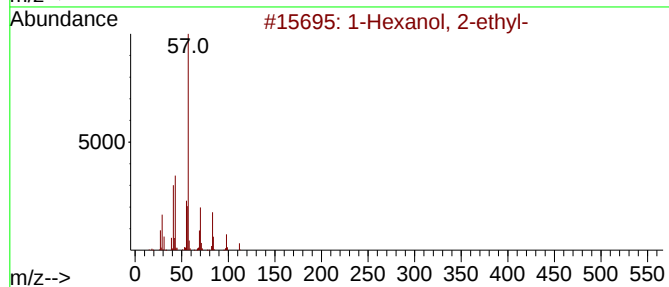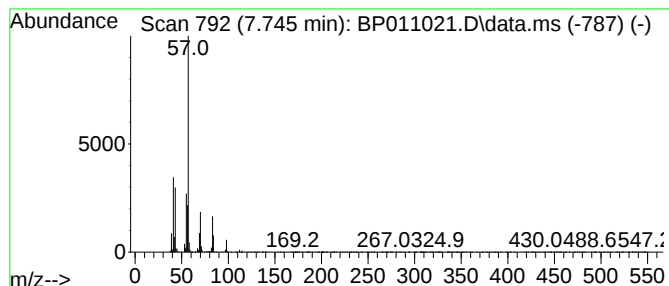

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071822\
Data File : BP011021.D
Acq On : 19 Jul 2022 07:52
Operator : CG/JU
Sample : N3704-07
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AQ1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
1-Hexanol, 2-et...	7.745	2.3	ng/u1	270862	1	7.675	2327940	20.0