

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071822\
 Data File : BP011022.D
 Acq On : 19 Jul 2022 08:26
 Operator : CG/JU
 Sample : N3704-06
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AJ5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011022.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.146	6	10	13	rBV	138208	189126	1.73%	0.177%
2	3.181	13	16	27	rVB	148577	218179	2.00%	0.204%
3	3.458	60	63	69	rBV	43161	58712	0.54%	0.055%
4	3.593	83	86	104	rBV	563718	897559	8.21%	0.840%
5	3.811	115	123	128	rVB3	55804	114657	1.05%	0.107%
6	3.905	135	139	148	rVB	54554	78188	0.72%	0.073%
7	4.416	220	226	242	rVB	2367128	3453582	31.61%	3.233%
8	4.811	289	293	299	rBV3	10209	19683	0.18%	0.018%
9	4.863	299	302	306	rVB3	10891	12757	0.12%	0.012%
10	5.205	355	360	366	rVB	55677	81387	0.74%	0.076%
11	5.334	377	382	390	rBV	65435	121916	1.12%	0.114%
12	5.405	390	394	401	rVB3	13626	26675	0.24%	0.025%
13	5.699	439	444	449	rBV	42445	61008	0.56%	0.057%
14	5.781	456	458	466	rVB6	12084	23159	0.21%	0.022%
15	6.687	605	612	617	rVB8	9369	21643	0.20%	0.020%
16	6.769	622	626	631	rVV3	9532	14916	0.14%	0.014%
17	6.857	631	641	652	rVB	556183	1008103	9.23%	0.944%
18	7.022	662	669	679	rBV	1661143	2480879	22.71%	2.323%
19	7.099	679	682	690	rVB	34269	50117	0.46%	0.047%
20	7.210	694	701	710	rBV	1677538	2549359	23.33%	2.387%
21	7.322	718	720	725	rVB2	19244	27105	0.25%	0.025%
22	7.681	772	781	788	rBV	1458529	2317961	21.21%	2.170%
23	7.752	788	793	799	rVV	93011	144247	1.32%	0.135%
24	7.928	817	823	830	rBV2	49322	84647	0.77%	0.079%
25	8.393	895	902	916	rBV	1400849	2205102	20.18%	2.064%
26	8.510	919	922	928	rVV6	9462	16570	0.15%	0.016%
27	8.581	930	934	938	rVB7	8062	11181	0.10%	0.010%
28	8.781	961	968	970	rBV8	7208	12030	0.11%	0.011%
29	8.840	970	978	986	rVV	1815771	2844884	26.04%	2.663%
30	8.963	993	999	1003	rBV5	13906	22366	0.20%	0.021%
31	9.010	1004	1007	1012	rVB6	12202	16700	0.15%	0.016%
32	9.257	1045	1049	1053	rVB3	11607	16731	0.15%	0.016%
33	9.416	1070	1076	1080	rBV2	22740	38352	0.35%	0.036%
34	9.557	1093	1100	1114	rBV	1344739	2155417	19.73%	2.018%
35	9.728	1121	1129	1138	rBV	78459	164174	1.50%	0.154%
36	9.799	1138	1141	1147	rVB6	10280	17576	0.16%	0.016%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071822\
 Data File : BP011022.D
 Acq On : 19 Jul 2022 08:26
 Operator : CG/JU
 Sample : N3704-06
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AJ5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
 Title : SVOA CALIBRATION

37	10.098	1183	1192	1204	rBV	1915203	3184917	29.15%	2.982%
38	10.469	1248	1255	1263	rBV	1893777	3187850	29.18%	2.984%
39	10.522	1263	1264	1270	rVB6	8170	11710	0.11%	0.011%
40	10.616	1270	1280	1292	rBV	979262	1694409	15.51%	1.586%
41	11.128	1363	1367	1374	rVB3	13181	23211	0.21%	0.022%
42	11.281	1387	1393	1401	rBV10	12334	26340	0.24%	0.025%
43	12.069	1522	1527	1533	rBV2	39153	65916	0.60%	0.062%
44	12.269	1554	1561	1568	rBV3	19753	45256	0.41%	0.042%
45	13.169	1710	1714	1719	rVV4	25106	39060	0.36%	0.037%
46	13.304	1732	1737	1741	rBV8	7909	11709	0.11%	0.011%
47	13.763	1808	1815	1824	rBV	3874703	5301982	48.53%	4.964%
48	13.828	1824	1826	1832	rVV7	12027	23212	0.21%	0.022%
49	14.034	1852	1861	1872	rBV	4139807	6135966	56.16%	5.745%
50	14.251	1895	1898	1904	rVB2	19011	26070	0.24%	0.024%
51	14.339	1906	1913	1922	rBV	2744053	3871762	35.44%	3.625%
52	14.557	1944	1950	1966	rBV	327748	650443	5.95%	0.609%
53	14.710	1972	1976	1982	rVB10	11375	15741	0.14%	0.015%
54	14.775	1984	1987	2000	rVV10	14664	34489	0.32%	0.032%
55	14.881	2000	2005	2011	rVB10	7683	16159	0.15%	0.015%
56	15.163	2048	2053	2055	rBV4	11016	17897	0.16%	0.017%
57	15.204	2058	2060	2065	rVB5	13133	17052	0.16%	0.016%
58	15.339	2077	2083	2091	rBV	5411110	7787058	71.27%	7.290%
59	15.463	2098	2104	2118	rBV	1675147	2272067	20.79%	2.127%
60	15.581	2120	2124	2129	rVB2	61770	94547	0.87%	0.089%
61	15.916	2176	2181	2189	rVB2	9626	19688	0.18%	0.018%
62	16.045	2198	2203	2207	rBV7	11920	26314	0.24%	0.025%
63	16.133	2214	2218	2221	rVB4	20863	26230	0.24%	0.025%
64	16.410	2263	2265	2271	rBV7	6164	13688	0.13%	0.013%
65	16.592	2291	2296	2297	rBV5	8508	12416	0.11%	0.012%
66	16.786	2325	2329	2333	rVB7	8828	13307	0.12%	0.012%
67	16.886	2342	2346	2349	rBV6	14565	24450	0.22%	0.023%
68	17.110	2377	2384	2391	rBV	3113530	4375204	40.04%	4.096%
69	17.210	2394	2401	2415	rBV	6409669	8824051	80.76%	8.261%
70	17.498	2446	2450	2456	rVB2	24420	35300	0.32%	0.033%
71	17.757	2492	2494	2498	rBV3	14873	19397	0.18%	0.018%
72	17.804	2499	2502	2506	rVB2	25205	26508	0.24%	0.025%
73	18.022	2535	2539	2545	rBV2	52889	75225	0.69%	0.070%
74	18.092	2546	2551	2556	rVV	3845653	4299164	39.35%	4.025%
75	18.769	2662	2666	2674	rBV2	46815	85584	0.78%	0.080%
76	19.039	2708	2712	2719	rBV2	88429	144335	1.32%	0.135%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071822\
Data File : BP011022.D
Acq On : 19 Jul 2022 08:26
Operator : CG/JU
Sample : N3704-06
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AJ5

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Title : SVOA CALIBRATION

77	19.110	2720	2724	2726	rBV	75174	108113	0.99%	0.101%
78	19.245	2743	2747	2753	rBV	68337	104305	0.95%	0.098%
79	19.469	2779	2785	2792	rBV	7964720	10489172	96.00%	9.820%
80	20.957	3034	3038	3045	rBV	771792	1008583	9.23%	0.944%
81	21.233	3080	3085	3090	rBV	3978810	4923403	45.06%	4.609%
82	23.439	3453	3460	3469	rBV2	5818790	10926263	100.00%	10.229%
83	23.592	3479	3486	3499	rVB2	2537233	5101559	46.69%	4.776%




Sum of corrected areas: 106813730

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071822\
Data File : BP011022.D
Acq On : 19 Jul 2022 08:26
Operator : CG/JU
Sample : N3704-06
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AJ5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

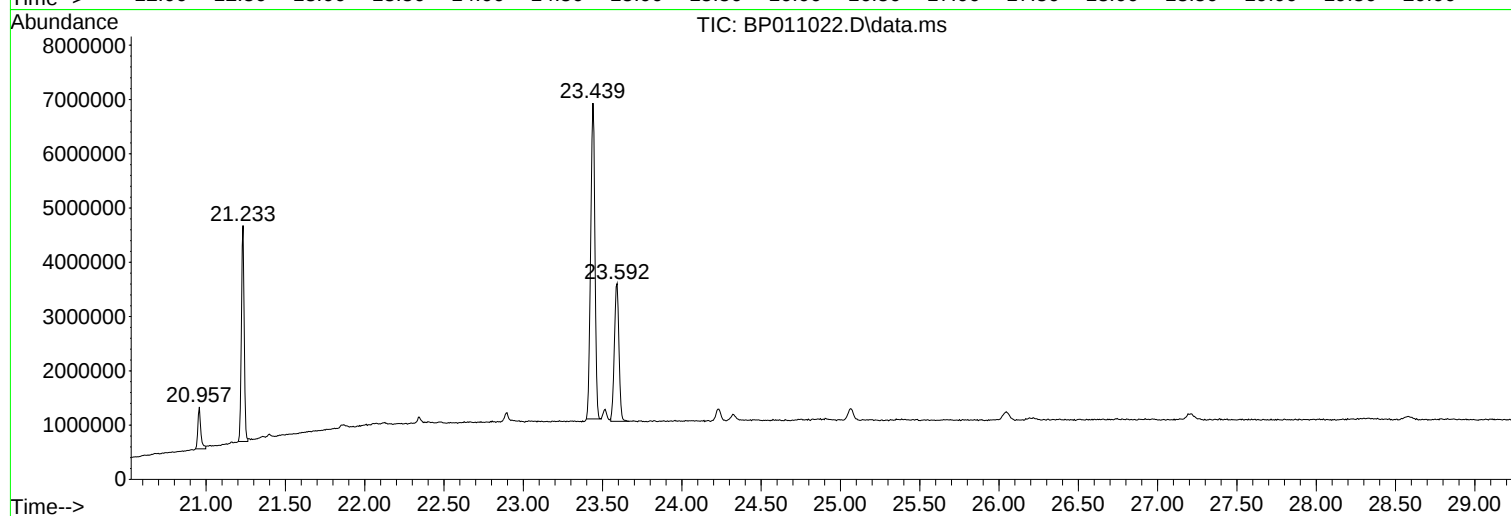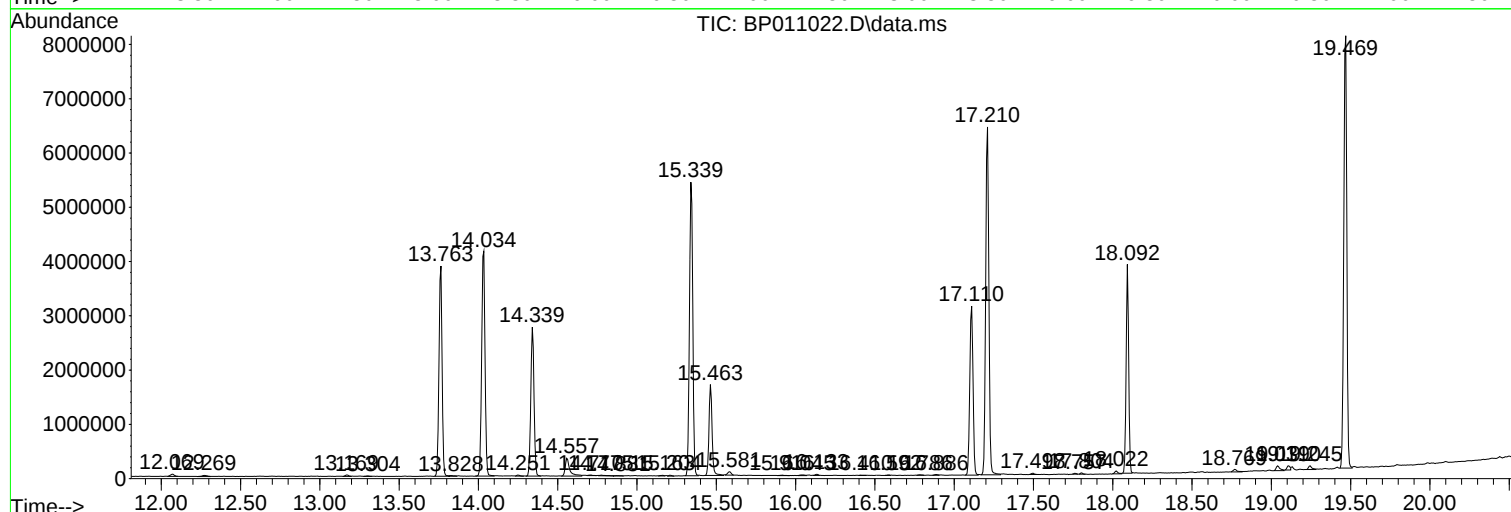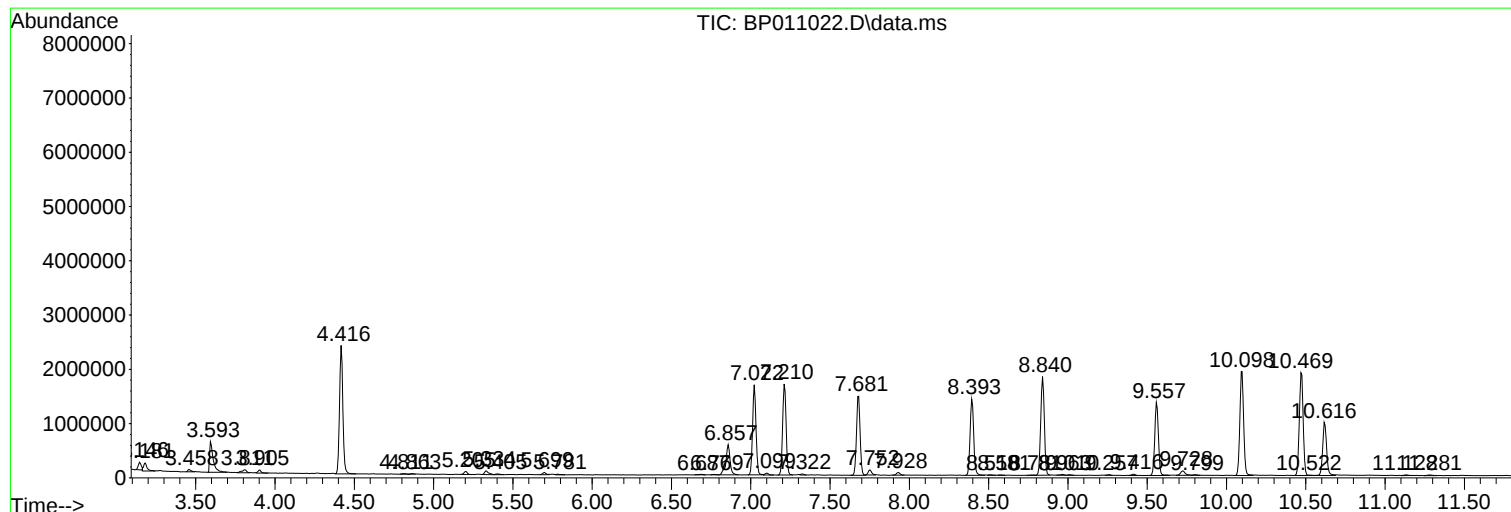

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071822\
Data File : BP011022.D
Acq On : 19 Jul 2022 08:26
Operator : CG/JU
Sample : N3704-06
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AJ5










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 (DEL) Alkane: Straight-Chai... Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
20.957	4.10 ng/ul	1008580	Chrysene-d12	21.233

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			1-Hexacosene	364	C26H52	018835-33-1	94
2			Pentacos-1-ene	350	C25H50	016980-85-1	94
3			n-Tetracosanol-1	354	C24H50O	000506-51-4	94
4			Behenic alcohol	326	C22H46O	000661-19-8	94
5			E-14-Hexadecenal	238	C16H30O	330207-53-9	93

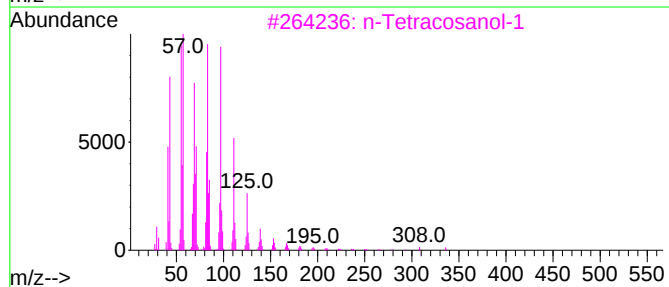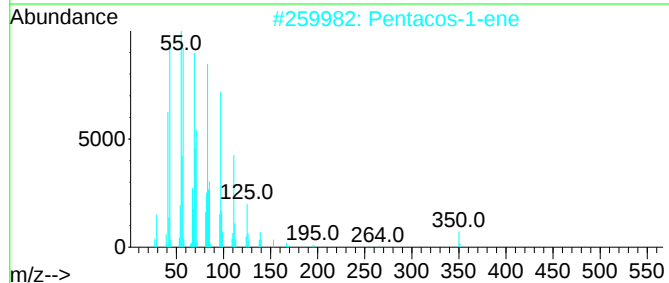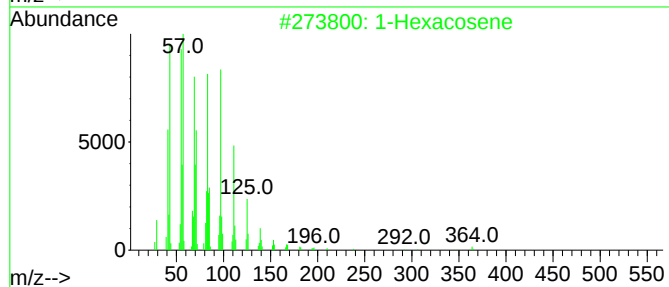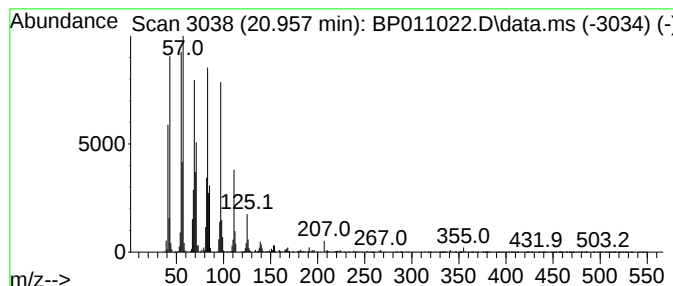

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071822\
Data File : BP011022.D
Acq On : 19 Jul 2022 08:26
Operator : CG/JU
Sample : N3704-06
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AJ5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: S...	20.957	4.1	ng/u1	1008580	5	21.233	4923400	20.0