

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071823\
 Data File : BP016299.D
 Acq On : 18 Jul 2023 18:39
 Operator : MA/JU
 Sample : PB153940BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK940

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP016299.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.281	12	16	27	rVB	67354	107487	1.83%	0.173%
2	3.729	90	92	121	rBV	605095	1328297	22.57%	2.139%
3	4.040	143	145	156	rVB4	13088	24311	0.41%	0.039%
4	6.093	490	494	498	rVB6	6700	8571	0.15%	0.014%
5	7.146	667	673	691	rBV	464140	1544287	26.23%	2.486%
6	7.281	691	696	723	rVV	550277	1387581	23.57%	2.234%
7	7.481	724	730	758	rVB	684410	1613108	27.40%	2.597%
8	7.952	802	810	835	rBV	531274	1424416	24.20%	2.293%
9	8.699	931	937	974	rBV	557151	1769537	30.06%	2.849%
10	9.152	1007	1014	1044	rBV	480472	1284070	21.81%	2.067%
11	9.887	1131	1139	1166	rBV	394854	1368675	23.25%	2.204%
12	10.469	1230	1238	1277	rBV2	349337	1840083	31.26%	2.963%
13	10.775	1283	1290	1316	rVB	940075	2173295	36.92%	3.499%
14	10.975	1317	1324	1362	rBV2	387229	1769706	30.06%	2.849%
15	12.452	1569	1575	1577	rBV6	7430	12373	0.21%	0.020%
16	12.652	1603	1609	1611	rBV7	3771	6095	0.10%	0.010%
17	13.499	1746	1753	1757	rBV8	6710	15836	0.27%	0.025%
18	14.028	1836	1843	1872	rBV	1361549	3106095	52.77%	5.001%
19	14.304	1883	1890	1920	rBV2	2003271	3530690	59.98%	5.685%
20	14.604	1935	1941	1962	rBV	1673488	2905354	49.36%	4.678%
21	14.957	1995	2001	2026	rBV2	147317	935374	15.89%	1.506%
22	15.616	2106	2113	2134	rBV	1978595	4420226	75.09%	7.117%
23	15.798	2139	2144	2170	rBV	343465	1284973	21.83%	2.069%
24	16.545	2267	2271	2277	rVB4	8462	12553	0.21%	0.020%
25	17.175	2375	2378	2384	rVB4	7159	11762	0.20%	0.019%
26	17.369	2405	2411	2423	rBV	2106815	3341500	56.77%	5.380%
27	17.481	2423	2430	2463	rVB	1941507	4810544	81.72%	7.745%
28	18.257	2557	2562	2570	rBV6	20992	54824	0.93%	0.088%
29	19.292	2734	2738	2744	rBV	40287	61195	1.04%	0.099%
30	19.375	2748	2752	2756	rBV	34360	56607	0.96%	0.091%
31	19.475	2766	2769	2779	rVB9	24211	47347	0.80%	0.076%
32	19.716	2803	2810	2833	rBV	2748169	5872667	99.77%	9.456%
33	21.481	3104	3110	3128	rBV	1705129	3846414	65.34%	6.193%
34	23.792	3496	3503	3523	rVB2	2472435	5886412	100.00%	9.478%
35	23.963	3525	3532	3556	rVB	1329256	4245977	72.13%	6.836%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071823\
Data File : BP016299.D
Acq On : 18 Jul 2023 18:39
Operator : MA/JU
Sample : PB153940BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK940

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 62108242

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071823\
Data File : BP016299.D
Acq On : 18 Jul 2023 18:39
Operator : MA/JU
Sample : PB153940BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK940

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

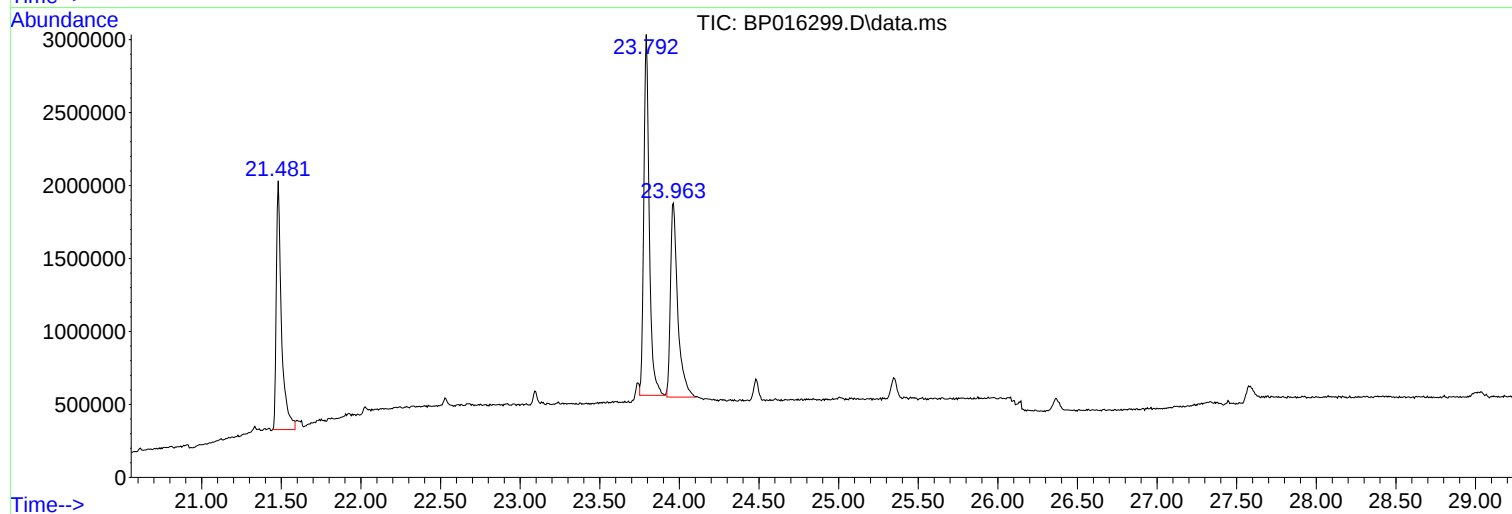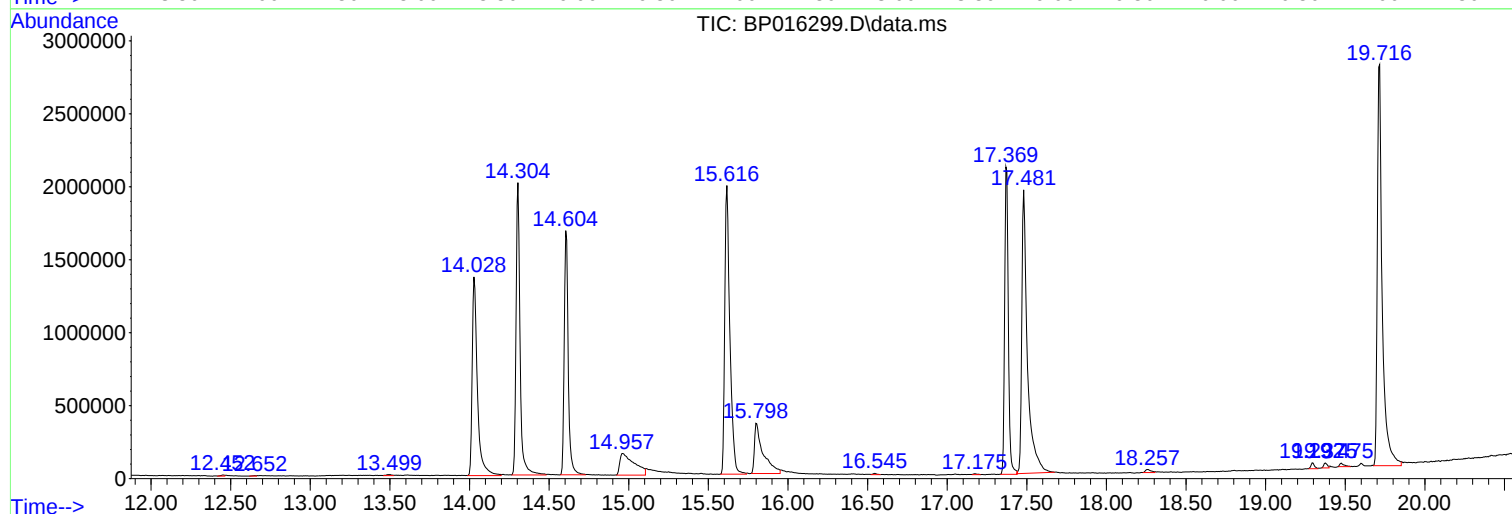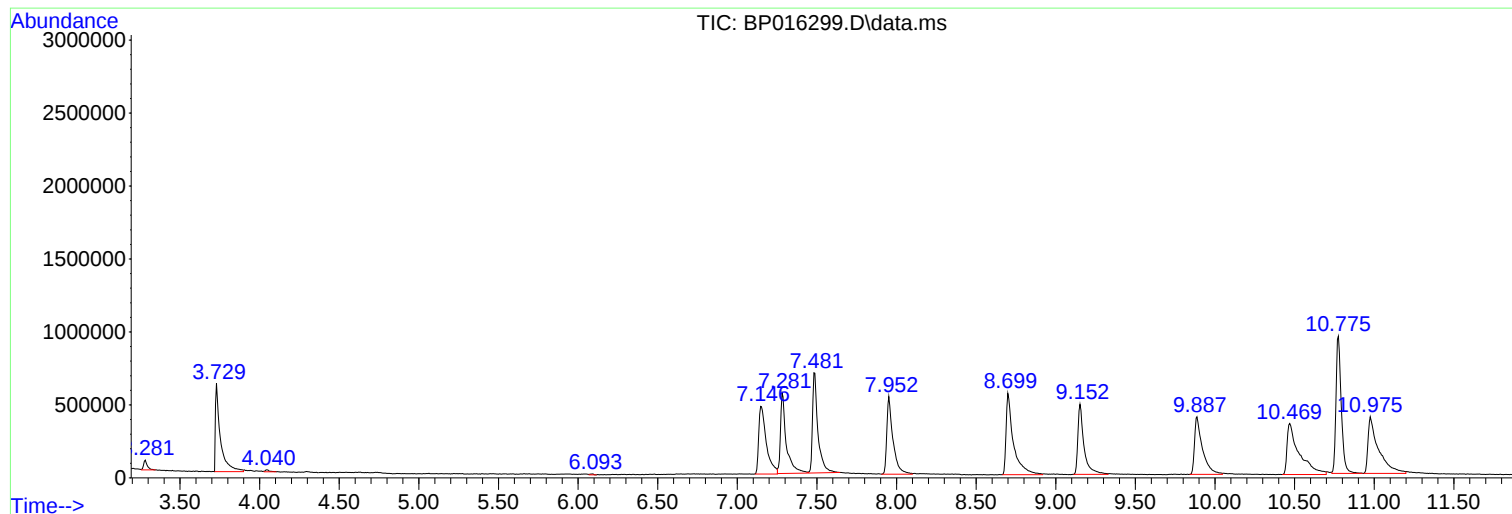

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071823\
Data File : BP016299.D
Acq On : 18 Jul 2023 18:39
Operator : MA/JU
Sample : PB153940BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK940

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071823\
Data File : BP016299.D
Acq On : 18 Jul 2023 18:39
Operator : MA/JU
Sample : PB153940BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK940

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------