

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071823\
 Data File : BP016301.D
 Acq On : 18 Jul 2023 19:48
 Operator : MA/JU
 Sample : 03477-05DL 5X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 HOA43DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP016301.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.240	4	9	18	rBV	490636	745535	6.43%	1.807%
2	3.310	18	21	33	rVB	327926	453745	3.92%	1.100%
3	3.793	101	103	108	rBV4	24364	44657	0.39%	0.108%
4	4.046	143	146	154	rVB2	13013	23162	0.20%	0.056%
5	4.581	230	237	266	rBV	7293274	11587136	100.00%	28.090%
6	5.199	337	342	350	rBV8	8258	20831	0.18%	0.050%
7	7.281	688	696	697	rBV7	12335	25577	0.22%	0.062%
8	7.322	697	703	725	rVV2	69988	333518	2.88%	0.809%
9	7.569	737	745	767	rVB2	77328	300375	2.59%	0.728%
10	7.963	805	812	843	rBV	400802	1555162	13.42%	3.770%
11	8.357	872	879	880	rBV6	9643	16982	0.15%	0.041%
12	8.834	951	960	962	rBV6	22826	59134	0.51%	0.143%
13	9.210	1018	1024	1043	rBV	79998	341511	2.95%	0.828%
14	9.986	1144	1156	1178	rBV7	44863	329539	2.84%	0.799%
15	10.586	1251	1258	1261	rBV3	66168	153426	1.32%	0.372%
16	10.786	1284	1292	1329	rVB	717848	2360873	20.37%	5.723%
17	11.110	1340	1347	1358	rBV6	19460	75443	0.65%	0.183%
18	11.810	1456	1466	1467	rBV9	9330	17659	0.15%	0.043%
19	13.504	1748	1754	1765	rBV3	23678	60913	0.53%	0.148%
20	14.051	1839	1847	1872	rBV	378363	1081686	9.34%	2.622%
21	14.310	1885	1891	1915	rBV	522488	1078507	9.31%	2.615%
22	14.610	1935	1942	1979	rVB	1582602	3222448	27.81%	7.812%
23	15.392	2069	2075	2084	rBV	43957	96983	0.84%	0.235%
24	15.633	2109	2116	2139	rBV	591497	1583529	13.67%	3.839%
25	15.804	2140	2145	2146	rBV5	15223	22969	0.20%	0.056%
26	15.874	2151	2157	2173	rBV8	57277	247866	2.14%	0.601%
27	16.021	2178	2182	2199	rVB	52259	140158	1.21%	0.340%
28	16.557	2268	2273	2281	rBV5	11633	24452	0.21%	0.059%
29	17.374	2406	2412	2427	rBV	1730796	3104103	26.79%	7.525%
30	17.504	2427	2434	2459	rVB2	378891	1252702	10.81%	3.037%
31	18.245	2555	2560	2569	rBV3	50955	119777	1.03%	0.290%
32	18.404	2582	2587	2594	rBV5	19943	49913	0.43%	0.121%
33	19.468	2764	2768	2775	rBV4	39443	77444	0.67%	0.188%
34	19.727	2806	2812	2831	rBV	890900	2064123	17.81%	5.004%
35	20.633	2963	2966	2970	rVB2	87661	90384	0.78%	0.219%
36	21.480	3104	3110	3128	rBV2	1671609	3943826	34.04%	9.561%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071823\
Data File : BP016301.D
Acq On : 18 Jul 2023 19:48
Operator : MA/JU
Sample : 03477-05DL 5X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
HOA43DL

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
Title : SVOA CALIBRATION

37	23.092	3381	3384	3390	rVB	158616	225415	1.95%	0.546%
38	23.803	3500	3505	3523	rVB2	447917	1072517	9.26%	2.600%
39	23.962	3525	3532	3554	rVB	865008	2855711	24.65%	6.923%
40	24.480	3615	3620	3627	rVB	193504	391000	3.37%	0.948%




Sum of corrected areas: 41250691

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071823\
Data File : BP016301.D
Acq On : 18 Jul 2023 19:48
Operator : MA/JU
Sample : 03477-05DL 5X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
HOA43DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

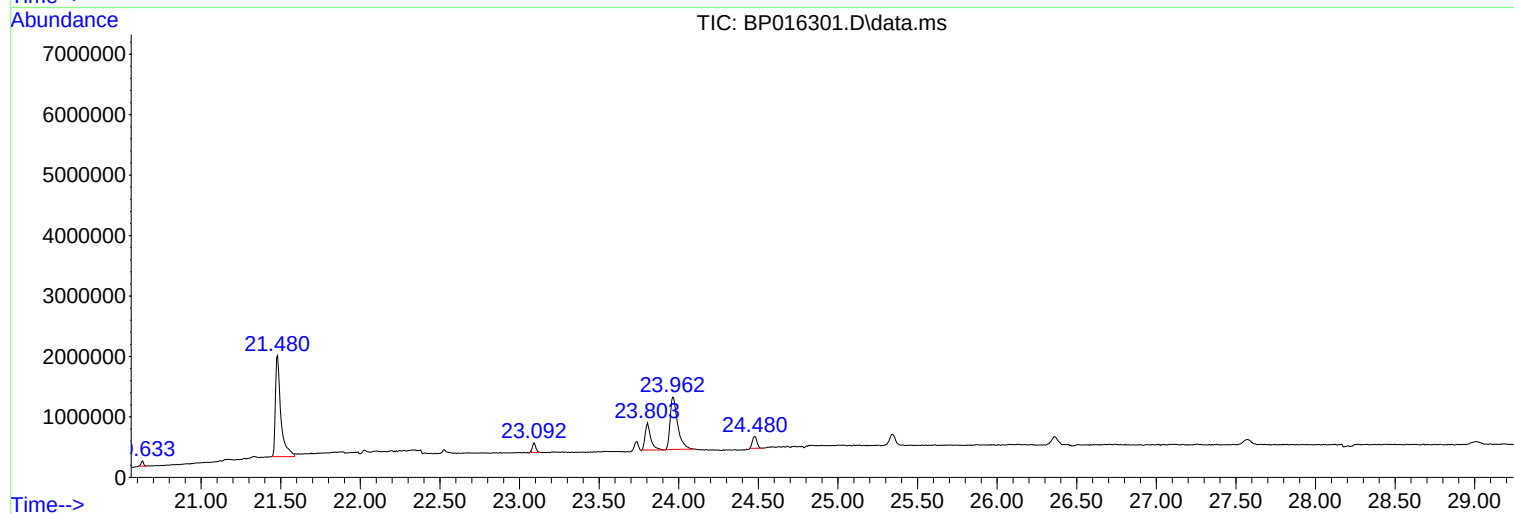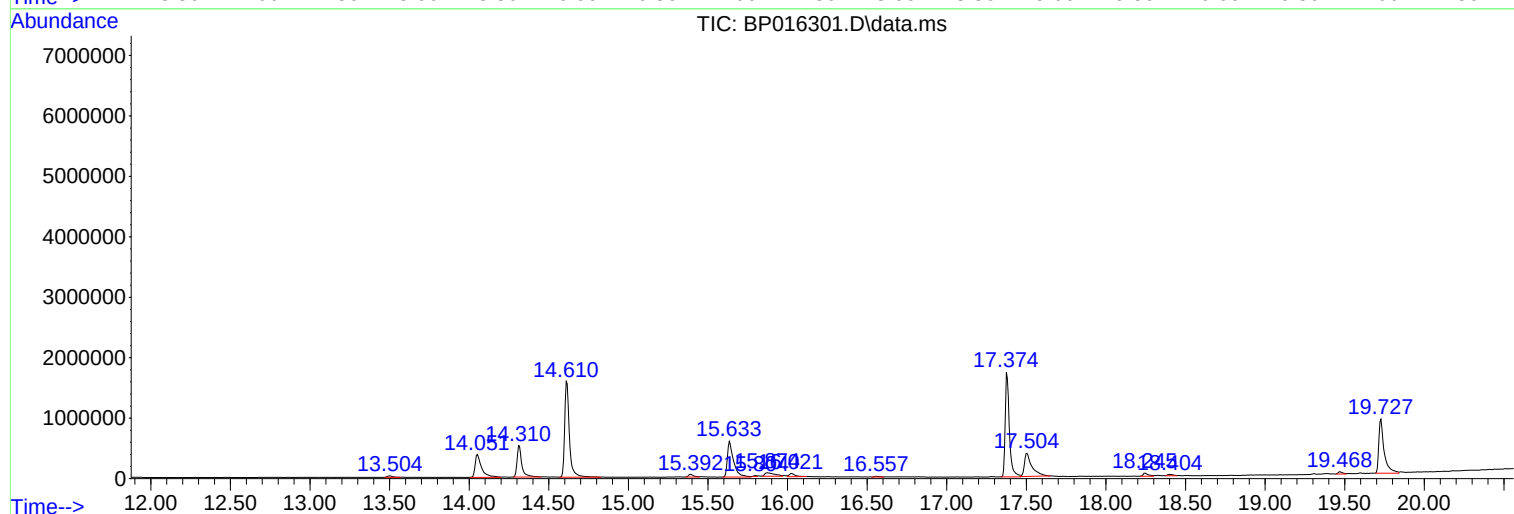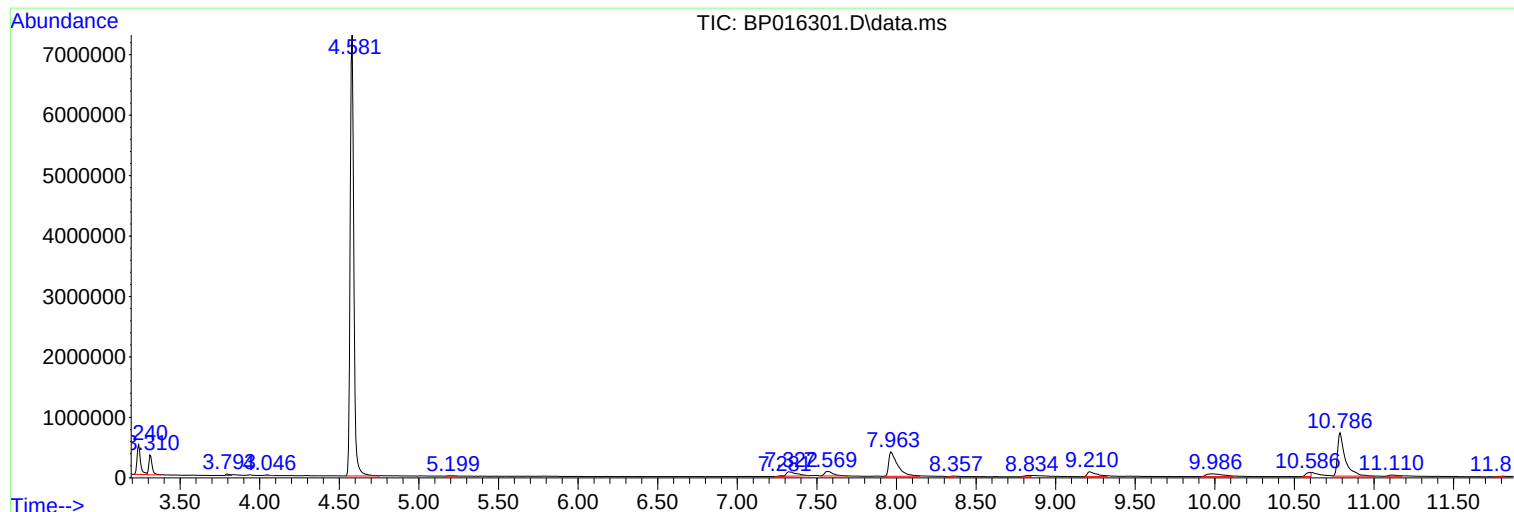

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071823\
Data File : BP016301.D
Acq On : 18 Jul 2023 19:48
Operator : MA/JU
Sample : 03477-05DL 5X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
HOA43DL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 (DEL) Alkane: Straight-Chai... Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
24.480	2.74 ng/ul	391000	Perylene-d12	23.962

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Heptadecane	240	C17H36	000629-78-7	93
2			Pentadecane, 8-hexyl-	296	C21H44	013475-75-7	90
3			Hexadecane	226	C16H34	000544-76-3	90
4			Octacosane	394	C28H58	000630-02-4	90
5			Eicosane, 10-methyl-	296	C21H44	054833-23-7	90

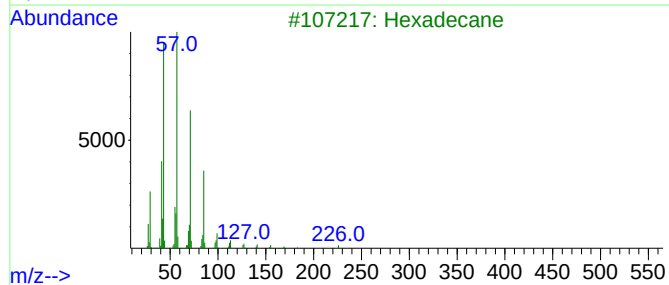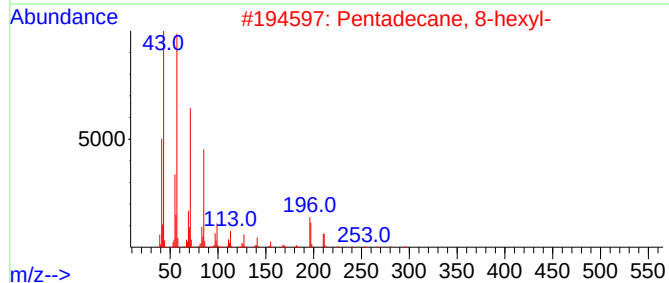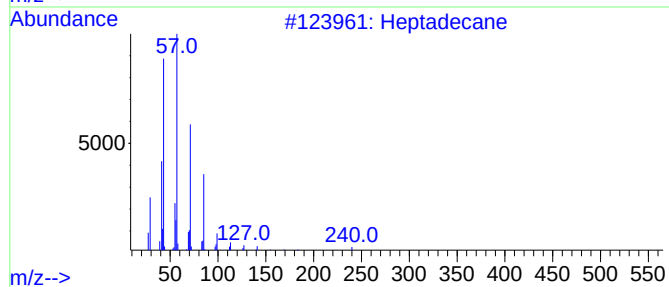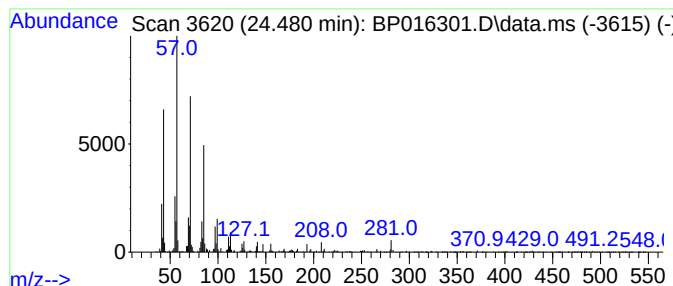

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071823\
Data File : BP016301.D
Acq On : 18 Jul 2023 19:48
Operator : MA/JU
Sample : 03477-05DL 5X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
HOA43DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: S...	24.480	2.7	ng/u1	391000	6	23.962	2855710	20.0