

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071823\
 Data File : BP016303.D
 Acq On : 18 Jul 2023 20:56
 Operator : MA/JU
 Sample : 03477-01DL 5X
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 HOA41DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP016303.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.240	4	9	18	rBV	289123	490887	4.76%	1.210%
2	3.311	18	21	31	rVB	260715	379149	3.68%	0.935%
3	3.805	102	105	111	rBV2	17558	45772	0.44%	0.113%
4	4.046	142	146	152	rBV2	11132	18449	0.18%	0.045%
5	4.581	230	237	261	rBV	6142282	10308373	100.00%	25.417%
6	7.299	693	699	701	rBV6	8805	17063	0.17%	0.042%
7	7.357	701	709	722	rVV4	39375	193080	1.87%	0.476%
8	7.581	740	747	763	rBV3	50248	174249	1.69%	0.430%
9	7.975	806	814	843	rBV	354756	1519263	14.74%	3.746%
10	8.840	954	961	962	rBV3	23996	46608	0.45%	0.115%
11	9.234	1022	1028	1051	rBV2	60496	295233	2.86%	0.728%
12	10.004	1145	1159	1170	rBV10	36278	207756	2.02%	0.512%
13	10.622	1250	1264	1285	rBV3	44941	282863	2.74%	0.697%
14	10.787	1285	1292	1317	rBV	572500	1936043	18.78%	4.774%
15	11.087	1335	1343	1366	rBV3	42097	238162	2.31%	0.587%
16	13.504	1748	1754	1762	rBV2	21798	52121	0.51%	0.129%
17	14.063	1840	1849	1879	rBV	247712	806141	7.82%	1.988%
18	14.316	1885	1892	1911	rBV	365278	799674	7.76%	1.972%
19	14.616	1936	1943	1972	rBV	1481901	3196604	31.01%	7.882%
20	15.645	2111	2118	2138	rBV	424920	1252868	12.15%	3.089%
21	15.898	2155	2161	2162	rBV3	36231	51605	0.50%	0.127%
22	16.039	2183	2185	2194	rVB5	16547	33983	0.33%	0.084%
23	16.563	2269	2274	2280	rBV4	13476	26835	0.26%	0.066%
24	17.186	2376	2380	2387	rVB8	6059	12288	0.12%	0.030%
25	17.380	2406	2413	2428	rBV	1894694	3777304	36.64%	9.314%
26	17.510	2429	2435	2459	rVB	380855	1270239	12.32%	3.132%
27	18.245	2555	2560	2569	rBV3	57006	113767	1.10%	0.281%
28	18.392	2580	2585	2595	rBV	38814	90449	0.88%	0.223%
29	19.304	2738	2740	2746	rBV7	11304	21598	0.21%	0.053%
30	19.363	2748	2750	2753	rBV3	16058	18997	0.18%	0.047%
31	19.463	2764	2767	2781	rBV7	54911	115182	1.12%	0.284%
32	19.592	2786	2789	2795	rVV2	55274	63486	0.62%	0.157%
33	19.727	2806	2812	2831	rBV	724284	1696424	16.46%	4.183%
34	20.610	2959	2962	2967	rBV4	44066	46491	0.45%	0.115%
35	21.333	3080	3085	3094	rVB	510490	1125354	10.92%	2.775%
36	21.474	3104	3109	3126	rBV2	1896346	4272496	41.45%	10.535%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071823\
Data File : BP016303.D
Acq On : 18 Jul 2023 20:56
Operator : MA/JU
Sample : 03477-01DL 5X
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
HOA41DL

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
Title : SVOA CALIBRATION

37	23.798	3499	3504	3518	rVB2	533632	1228133	11.91%	3.028%
38	23.957	3525	3531	3556	rVB	1442833	4331680	42.02%	10.681%




Sum of corrected areas: 40556669

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071823\
Data File : BP016303.D
Acq On : 18 Jul 2023 20:56
Operator : MA/JU
Sample : 03477-01DL 5X
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
HOA41DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

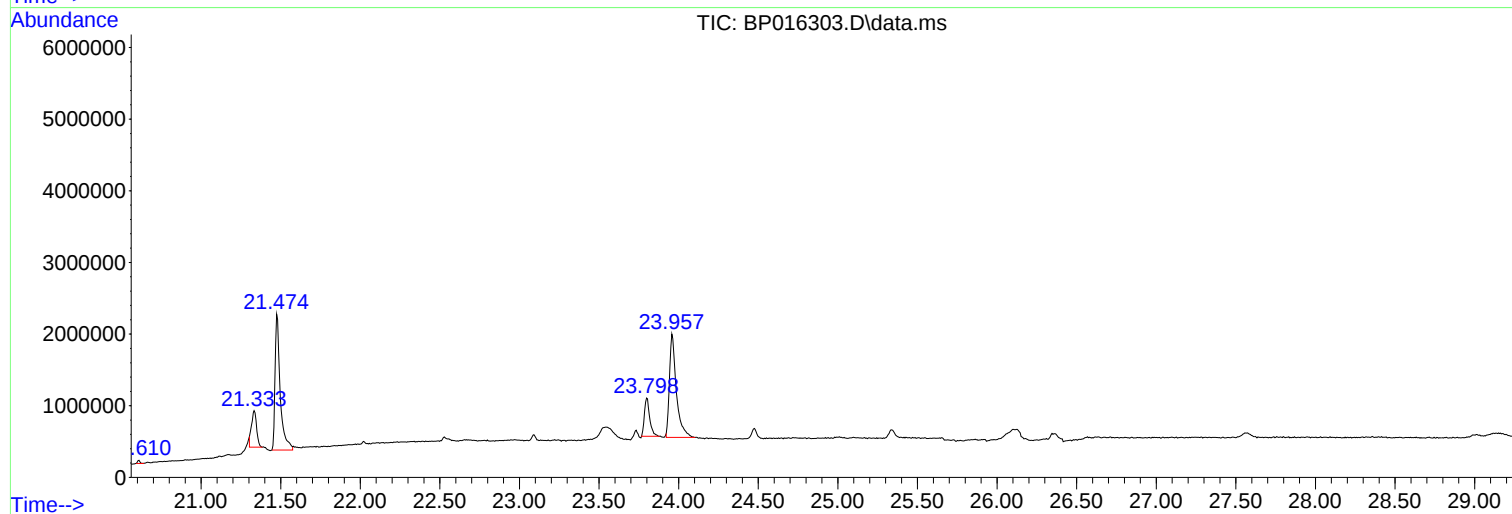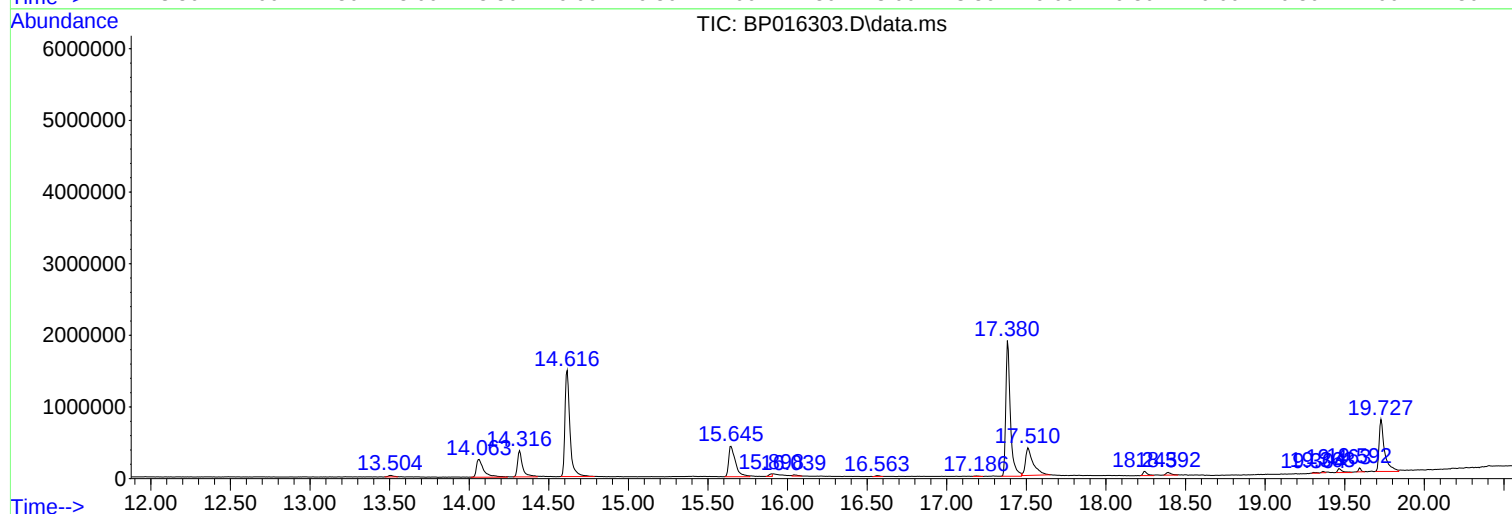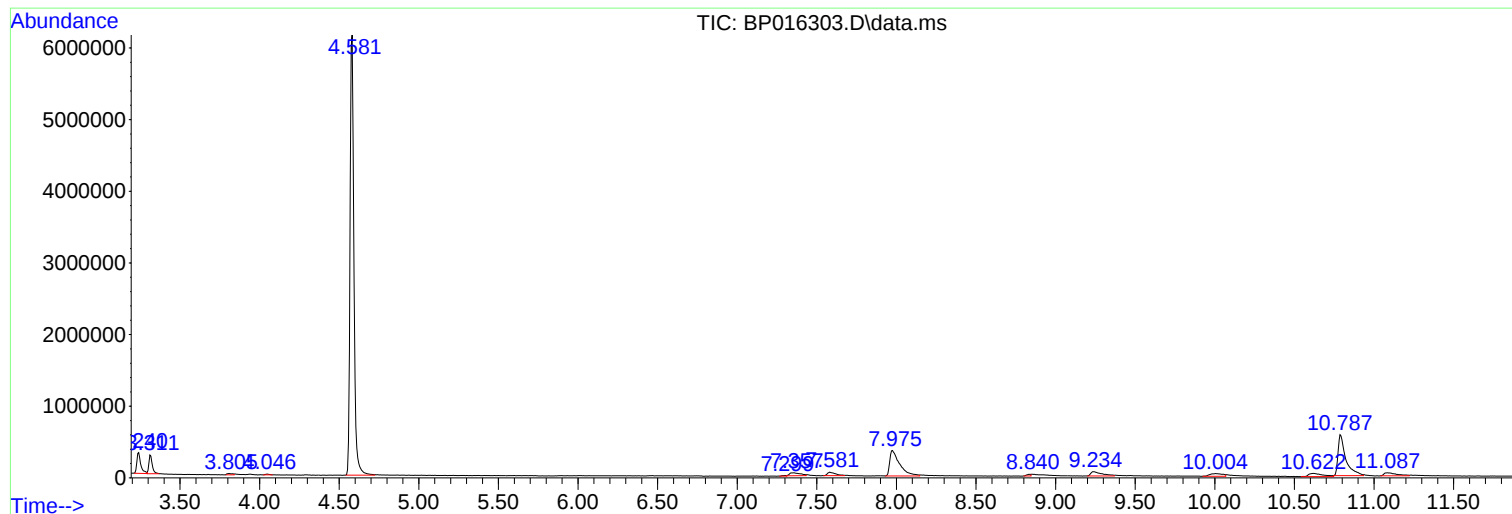

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071823\
Data File : BP016303.D
Acq On : 18 Jul 2023 20:56
Operator : MA/JU
Sample : 03477-01DL 5X
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
HOA41DL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 (DEL) Alkane: Straight-Chai... Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
21.333	5.27 ng/ul	1125350	Chrysene-d12	21.474

Hit#	of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	Eicosane		282	C20H42	000112-95-8	95
2	Hexacosane		366	C26H54	000630-01-3	90
3	Hexadecane		226	C16H34	000544-76-3	87
4	Heneicosane		296	C21H44	000629-94-7	87
5	Nonadecane		268	C19H40	000629-92-5	87

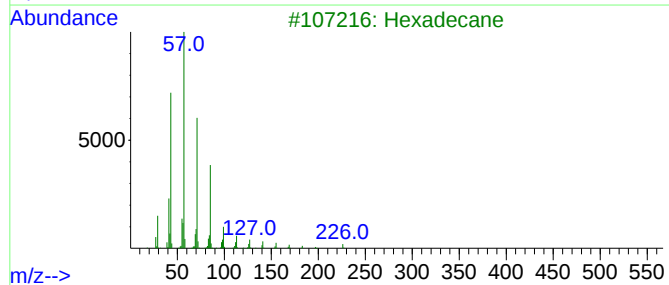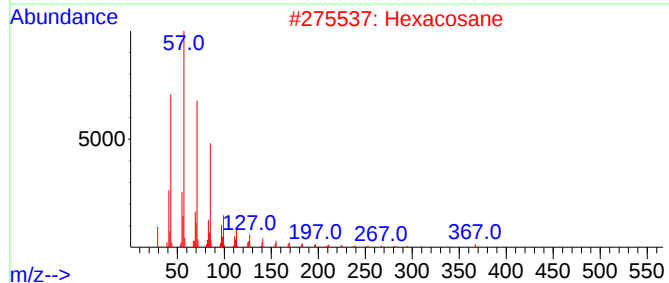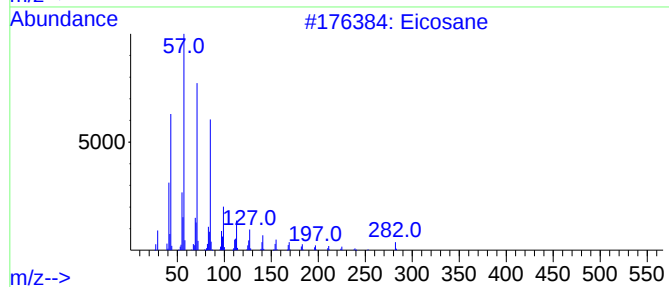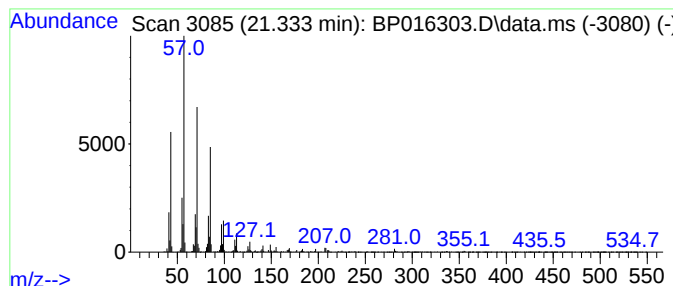

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071823\
Data File : BP016303.D
Acq On : 18 Jul 2023 20:56
Operator : MA/JU
Sample : 03477-01DL 5X
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
HOA41DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: S...	21.333	5.3	ng/u1	1125350	5	21.474	4272500	20.0