




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071824\
Data File : BP021053.D
Acq On : 18 Jul 2024 19:47
Operator : MA/JU
Sample : P3260-07
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E08F9

Manual IntegrationsAPPROVED

Quant Time: Jul 18 22:56:14 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jul 18 14:23:21 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/19/2024
Supervised By :mohammad ahmed 07/20/2024

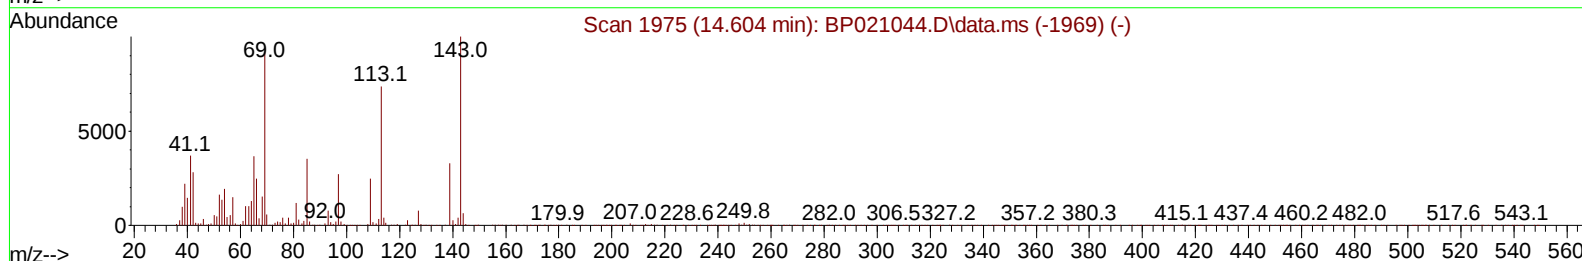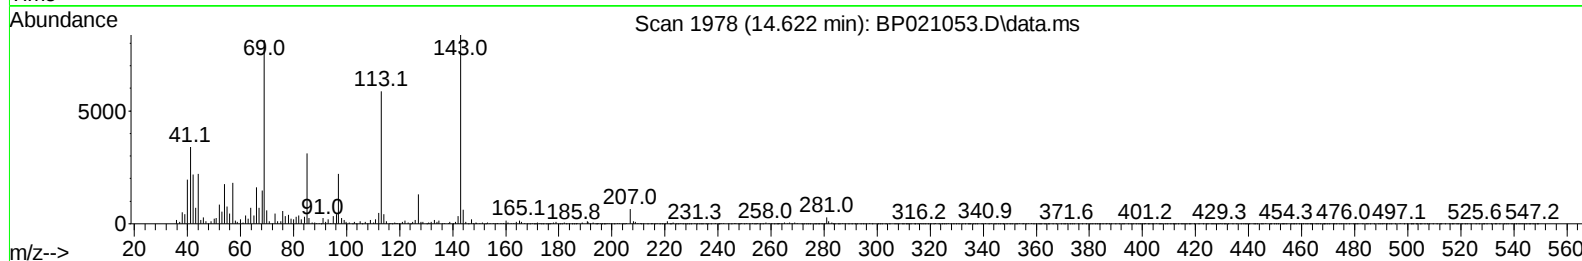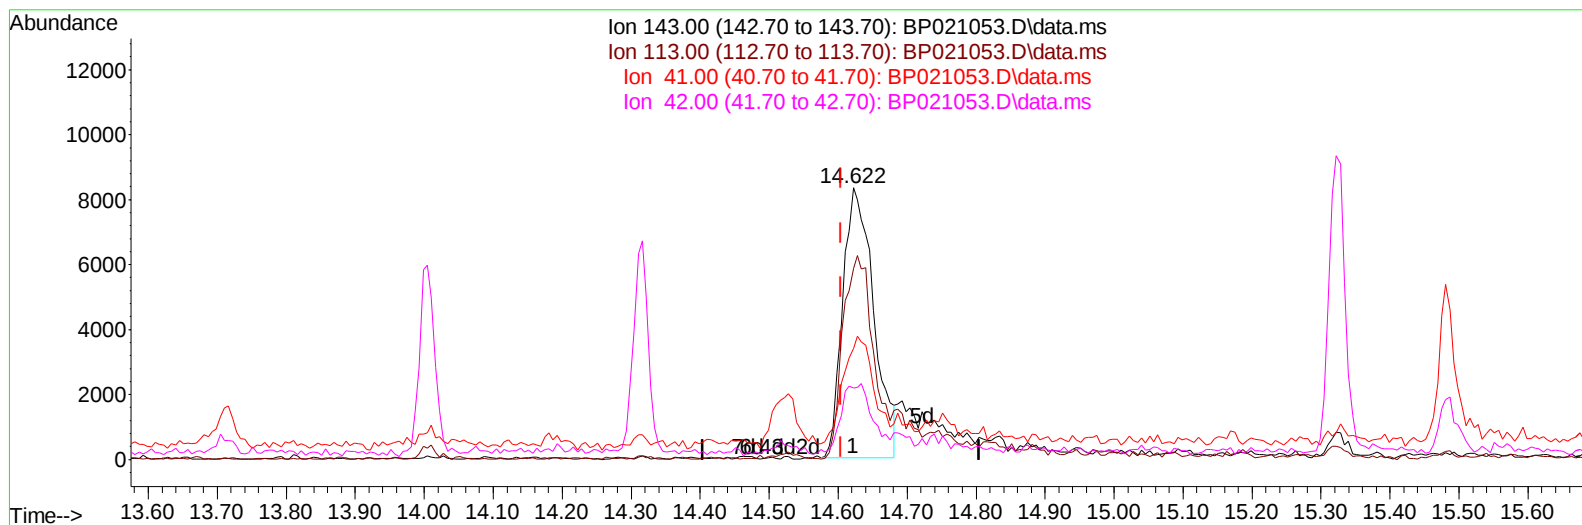

TIC: BP021053.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.622min (+ 0.018) 7.54 ng/u1

response 25953

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	74.70	70.34
41.00	37.90	40.82
42.00	27.10	26.22




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071824\
Data File : BP021053.D
Acq On : 18 Jul 2024 19:47
Operator : MA/JU
Sample : P3260-07
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E08F9

Manual IntegrationsAPPROVED

Quant Time: Jul 18 22:56:14 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jul 18 14:23:21 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/19/2024
Supervised By :mohammad ahmed 07/20/2024

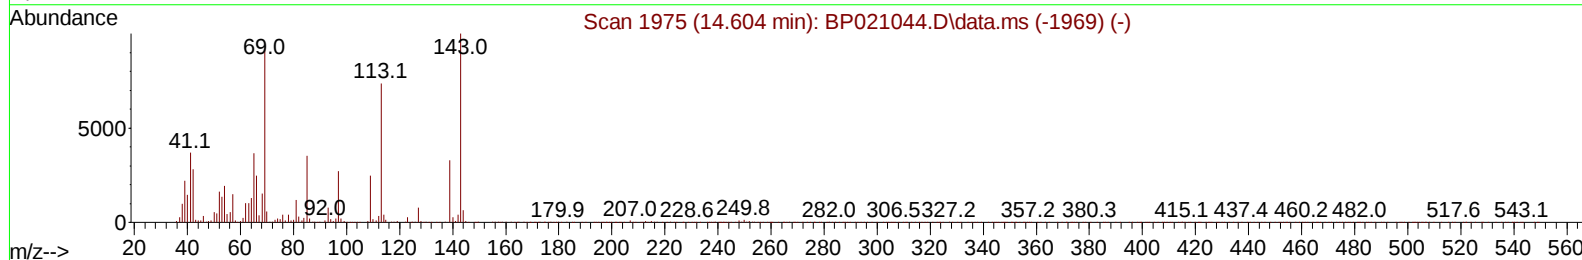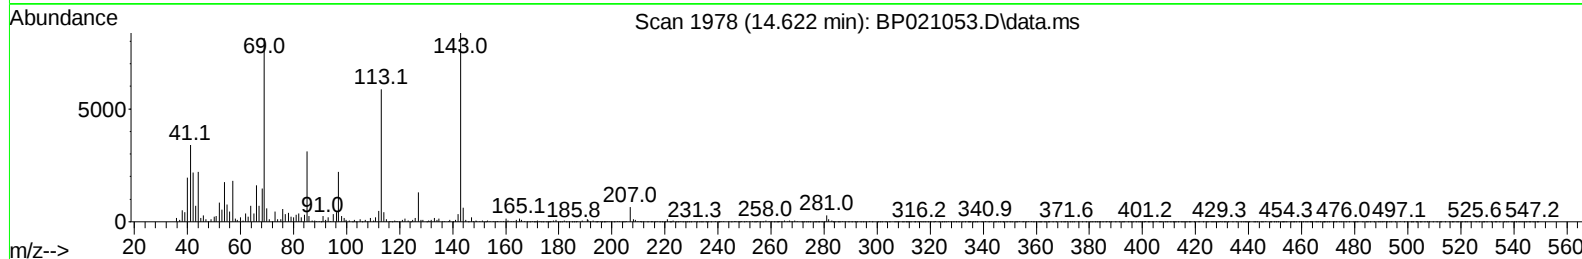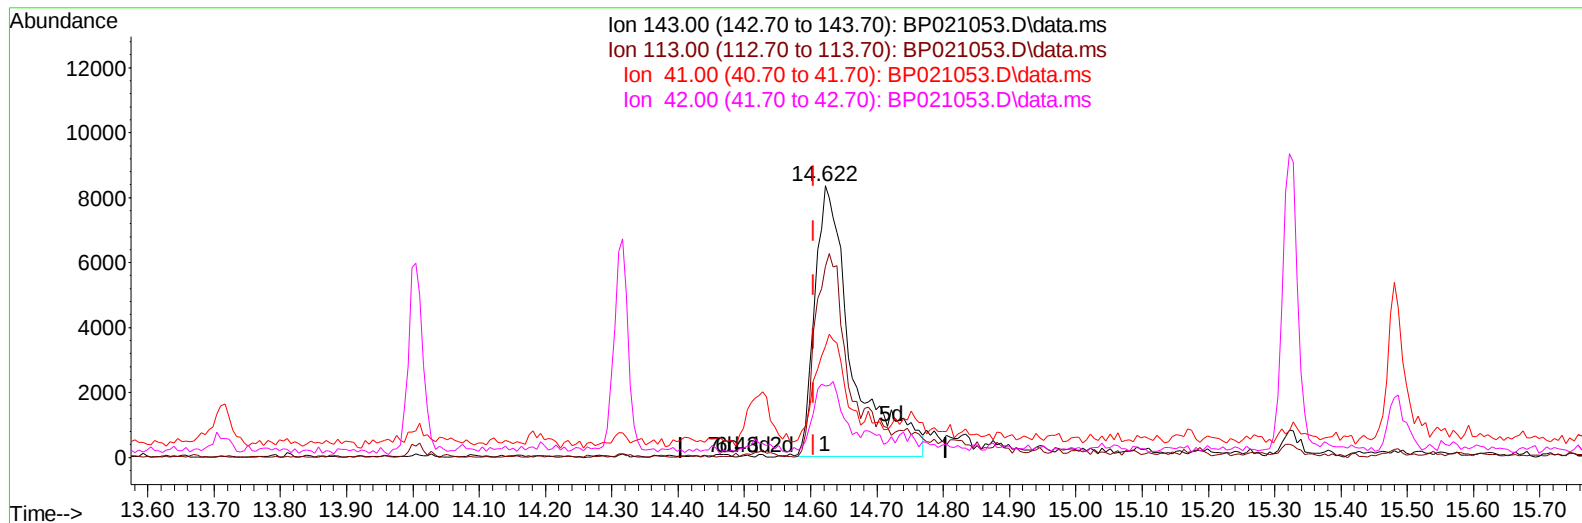

TIC: BP021053.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.622min (+ 0.018) 9.41 ng/ul m

response 32410

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	74.70	70.34
41.00	37.90	40.82
42.00	27.10	26.22

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071824\
 Data File : BP021053.D
 Acq On : 18 Jul 2024 19:47
 Operator : MA/JU
 Sample : P3260-07
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 E08F9

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 07/19/2024
 Supervised By :mohammad ahmed 07/20/2024

Quant Time: Jul 18 23:00:53 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jul 18 14:23:21 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.681	152	129779	20.000	ng/ul	-0.01
20) Naphthalene-d8	10.446	136	515053	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.316	164	332870	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.122	188	712350	20.000	ng/ul	0.00
79) Chrysene-d12	21.580	240	708132	20.000	ng/ul	0.00
88) Perylene-d12	24.886	264	884867	20.000	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.234	96	12636	4.431	ng/uL	0.00
4) Pyridine-d5	3.658	84	59731	7.234	ng/ul	0.00
7) Phenol-d5	6.899	99	92494	8.742	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.028	67	169692	26.465	ng/ul	-0.01
11) 2-Chlorophenol-d4	7.240	132	225624	25.882	ng/ul	0.00
15) 4-Methylphenol-d8	8.411	113	157318	17.902	ng/ul	0.00
21) Nitrobenzene-d5	8.834	128	113512	28.375	ng/ul	-0.01
24) 2-Nitrophenol-d4	9.552	143	130739	28.553	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.099	165	219595	26.523	ng/ul	0.00
31) 4-Chloroaniline-d4	10.605	131	261704	23.860	ng/ul	0.00
46) Dimethylphthalate-d6	13.716	166	709492	29.320	ng/ul	0.00
49) Acenaphthylene-d8	14.004	160	793857	29.217	ng/ul	0.00
54) 4-Nitrophenol-d4	14.622	143	32410m	9.414	ng/ul	0.02
60) Fluorene-d10	15.328	176	629941	31.732	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.481	200	101804	23.620	ng/ul	0.00
73) Anthracene-d10	17.234	188	1115836	35.268	ng/ul	0.00
81) Pyrene-d10	19.616	212	1380650	31.536	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.657	264	1548938	35.492	ng/ul	-0.03

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071824\
Data File : BP021053.D
Acq On : 18 Jul 2024 19:47
Operator : MA/JU
Sample : P3260-07
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E08F9

Manual IntegrationsAPPROVED

Quant Time: Jul 18 23:00:53 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jul 18 14:23:21 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/19/2024
Supervised By :mohammad ahmed 07/20/2024

