




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071824\
 Data File : BP021066.D
 Acq On : 19 Jul 2024 05:45
 Operator : MA/JU
 Sample : P3201-18
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A4CJ9

Manual IntegrationsAPPROVED

Quant Time: Jul 19 06:11:37 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jul 18 14:23:21 2024
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/19/2024
 Supervised By :mohammad ahmed 07/20/2024

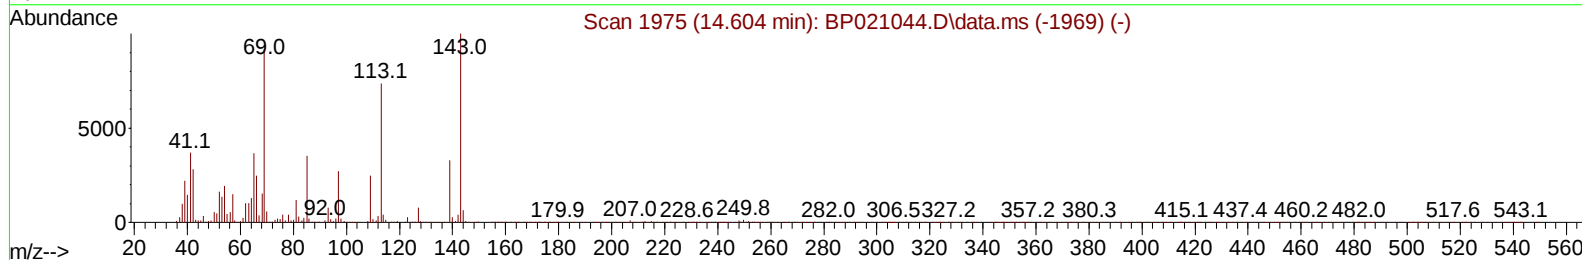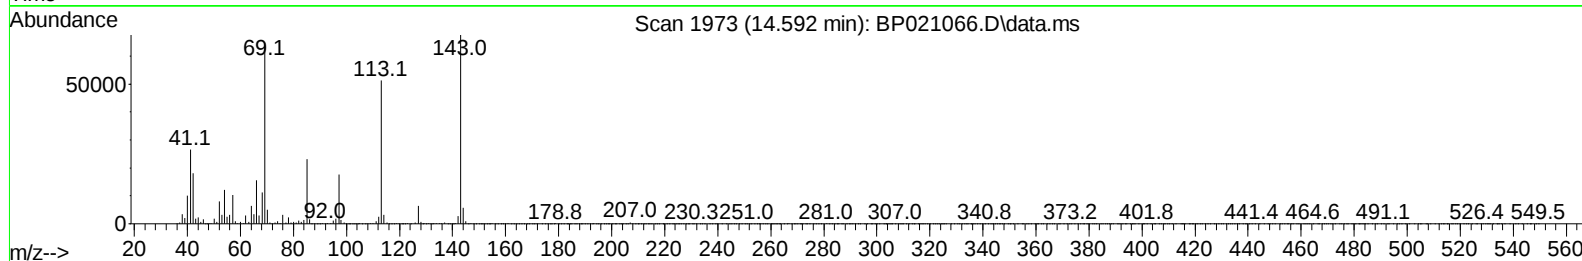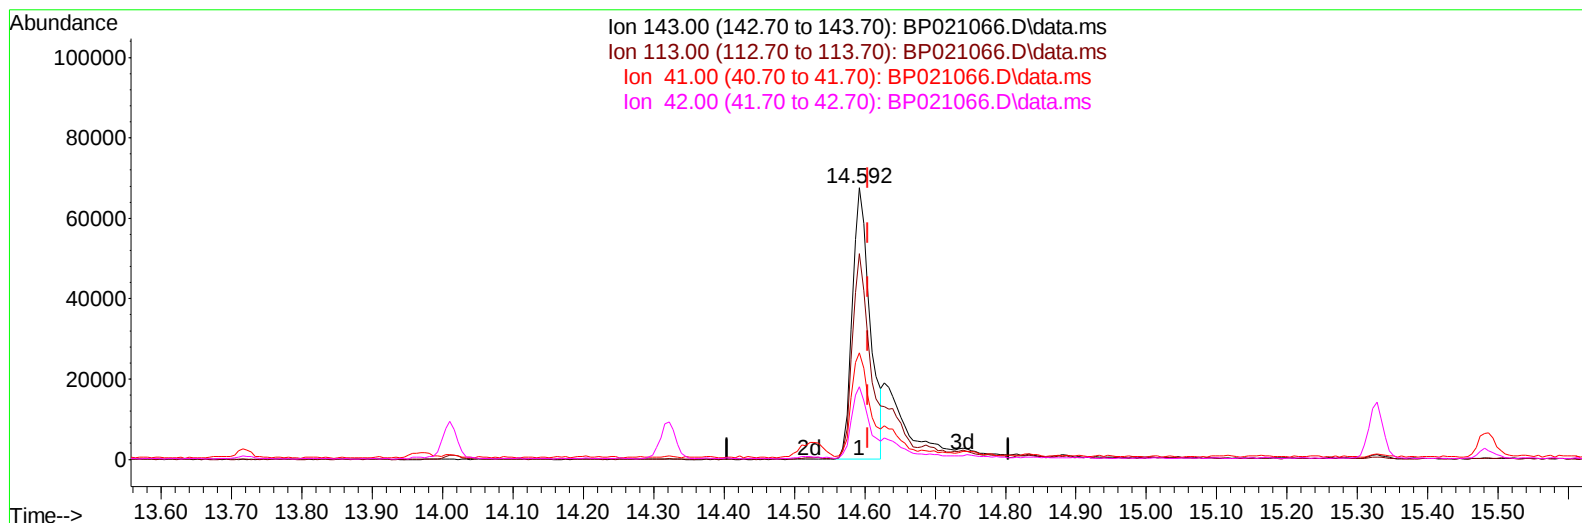

TIC: BP021066.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.592min (-0.012) 23.30 ng/u1

response 117695

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	74.70	75.86
41.00	37.90	39.23
42.00	27.10	26.78




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071824\
Data File : BP021066.D
Acq On : 19 Jul 2024 05:45
Operator : MA/JU
Sample : P3201-18
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A4CJ9

Manual IntegrationsAPPROVED

Quant Time: Jul 19 06:11:37 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jul 18 14:23:21 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/19/2024
Supervised By :mohammad ahmed 07/20/2024

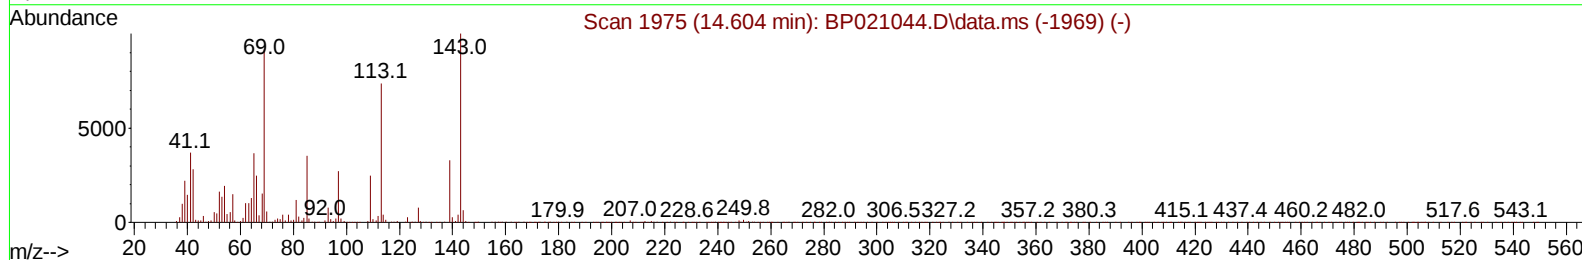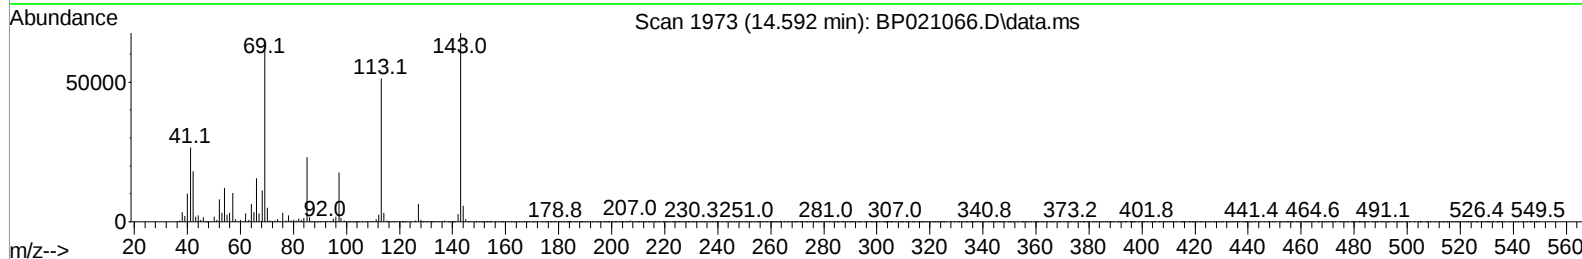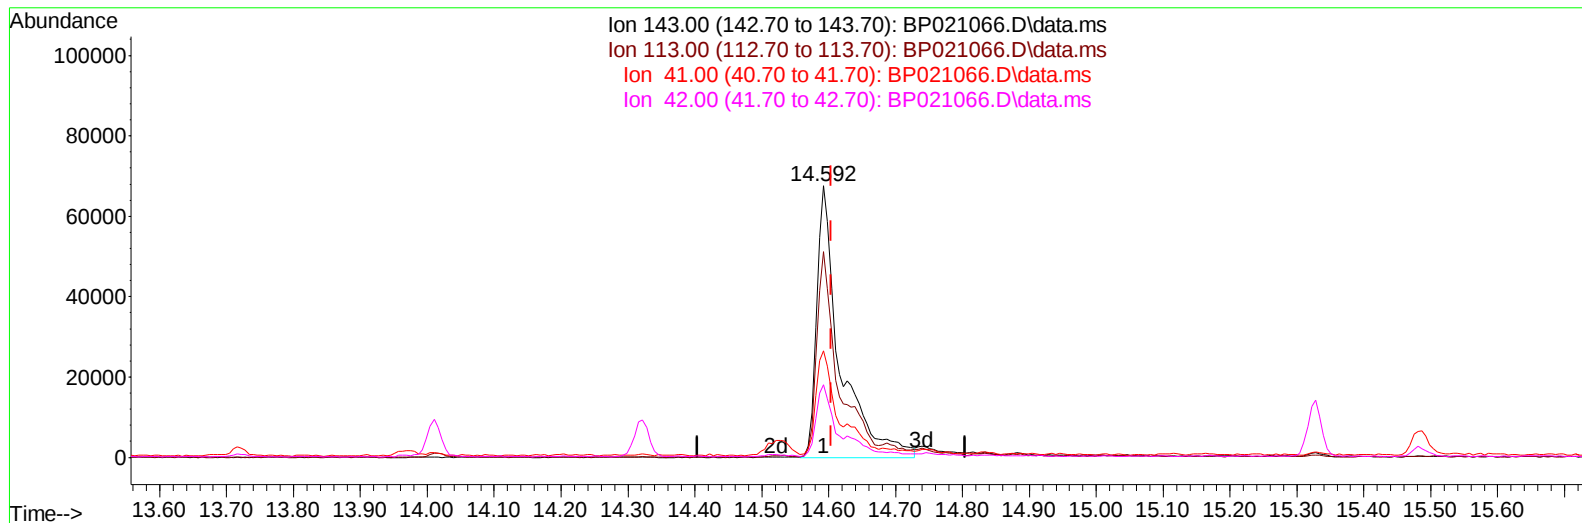

TIC: BP021066.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.592min (-0.012) 32.50 ng/ul m

response 164189

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	74.70	75.86
41.00	37.90	39.23
42.00	27.10	26.78

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071824\
 Data File : BP021066.D
 Acq On : 19 Jul 2024 05:45
 Operator : MA/JU
 Sample : P3201-18
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A4CJ9

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 07/19/2024
 Supervised By :mohammad ahmed 07/20/2024

Quant Time: Jul 19 06:17:29 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jul 18 14:23:21 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.687	152	186388	20.000	ng/ul	0.00
20) Naphthalene-d8	10.446	136	758467	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.322	164	488403	20.000	ng/ul	0.01
64) Phenanthrene-d10	17.122	188	1103784	20.000	ng/ul	0.00
79) Chrysene-d12	21.574	240	1254984	20.000	ng/ul	0.00
88) Perylene-d12	24.886	264	1558071	20.000	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.234	96	20498	5.005	ng/uL	0.00
4) Pyridine-d5	3.646	84	260065	21.932	ng/ul	-0.01
7) Phenol-d5	6.899	99	416753	27.426	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.034	67	238965	25.949	ng/ul	0.00
11) 2-Chlorophenol-d4	7.234	132	342342	27.344	ng/ul	0.00
15) 4-Methylphenol-d8	8.405	113	342018	27.100	ng/ul	-0.01
21) Nitrobenzene-d5	8.834	128	162860	27.645	ng/ul	-0.01
24) 2-Nitrophenol-d4	9.546	143	190396	28.237	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.087	165	327516	26.862	ng/ul	-0.02
31) 4-Chloroaniline-d4	10.599	131	404625	25.051	ng/ul	0.00
46) Dimethylphthalate-d6	13.716	166	965805	27.202	ng/ul	0.00
49) Acenaphthylene-d8	14.010	160	1154569	28.961	ng/ul	0.01
54) 4-Nitrophenol-d4	14.592	143	164189m	32.503	ng/ul	-0.01
60) Fluorene-d10	15.328	176	871822	29.931	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.486	200	133106	19.931	ng/ul	0.00
73) Anthracene-d10	17.233	188	1366783	27.880	ng/ul	0.00
81) Pyrene-d10	19.616	212	1925247	24.814	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.662	264	2212903	28.797	ng/ul	-0.02

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071824\
Data File : BP021066.D
Acq On : 19 Jul 2024 05:45
Operator : MA/JU
Sample : P3201-18
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A4CJ9

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 07/19/2024
Supervised By :mohammad ahmed 07/20/2024

Quant Time: Jul 19 06:17:29 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jul 18 14:23:21 2024
Response via : Initial Calibration

