

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071824\
 Data File : BP021045.D
 Acq On : 18 Jul 2024 14:02
 Operator : MA/JU
 Sample : PB162120BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK120

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP021045.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.240	39	43	54	rVB	42210	64734	1.59%	0.158%
2	3.652	111	113	130	rBV	503752	789392	19.35%	1.925%
3	3.958	162	165	170	rVB	11509	15280	0.37%	0.037%
4	6.793	643	647	651	rBV7	2873	4615	0.11%	0.011%
5	6.910	658	667	682	rBV	560106	994590	24.38%	2.426%
6	7.034	682	688	702	rVB	473171	756513	18.54%	1.845%
7	7.246	717	724	733	rBV	608475	1002522	24.57%	2.445%
8	7.687	791	799	810	rBV	576605	918486	22.51%	2.240%
9	8.416	915	923	937	rBV	693178	1222924	29.98%	2.983%
10	8.840	987	995	1008	rBV	575495	972834	23.85%	2.373%
11	9.552	1108	1116	1126	rBV	522263	858508	21.04%	2.094%
12	10.093	1201	1208	1231	rBV	632130	1263300	30.96%	3.081%
13	10.240	1231	1233	1238	rVB6	3243	5402	0.13%	0.013%
14	10.446	1260	1268	1281	rBV	729765	1279328	31.36%	3.120%
15	10.599	1285	1294	1317	rBV	594607	1291458	31.66%	3.150%
16	12.051	1535	1541	1551	rBV5	8916	21435	0.53%	0.052%
17	13.716	1818	1824	1836	rBV	1392858	1998127	48.98%	4.873%
18	14.010	1866	1874	1886	rBV	1494281	2339668	57.35%	5.706%
19	14.310	1917	1925	1938	rVB	1065452	1817622	44.55%	4.433%
20	14.592	1967	1973	1994	rBV	331472	805149	19.74%	1.964%
21	14.828	2011	2013	2020	rVB8	3886	5237	0.13%	0.013%
22	15.322	2090	2097	2111	rBV	2086413	2904185	71.18%	7.083%
23	15.475	2117	2123	2133	rBV	580108	898799	22.03%	2.192%
24	17.116	2396	2402	2413	rBV	1443698	2258023	55.35%	5.507%
25	17.222	2413	2420	2433	rVV2	2097319	3271053	80.18%	7.978%
26	18.057	2558	2562	2569	rBV4	43776	69409	1.70%	0.169%
27	19.610	2820	2826	2832	rBV	2748622	3942047	96.62%	9.614%
28	21.574	3154	3160	3171	rBV	1460959	2464621	60.41%	6.011%
29	24.674	3679	3687	3700	rVB	1502043	4079784	100.00%	9.950%
30	24.874	3716	3721	3740	rVB	977200	2687930	65.88%	6.555%




Sum of corrected areas: 41002975

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071824\
Data File : BP021045.D
Acq On : 18 Jul 2024 14:02
Operator : MA/JU
Sample : PB162120BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK120

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

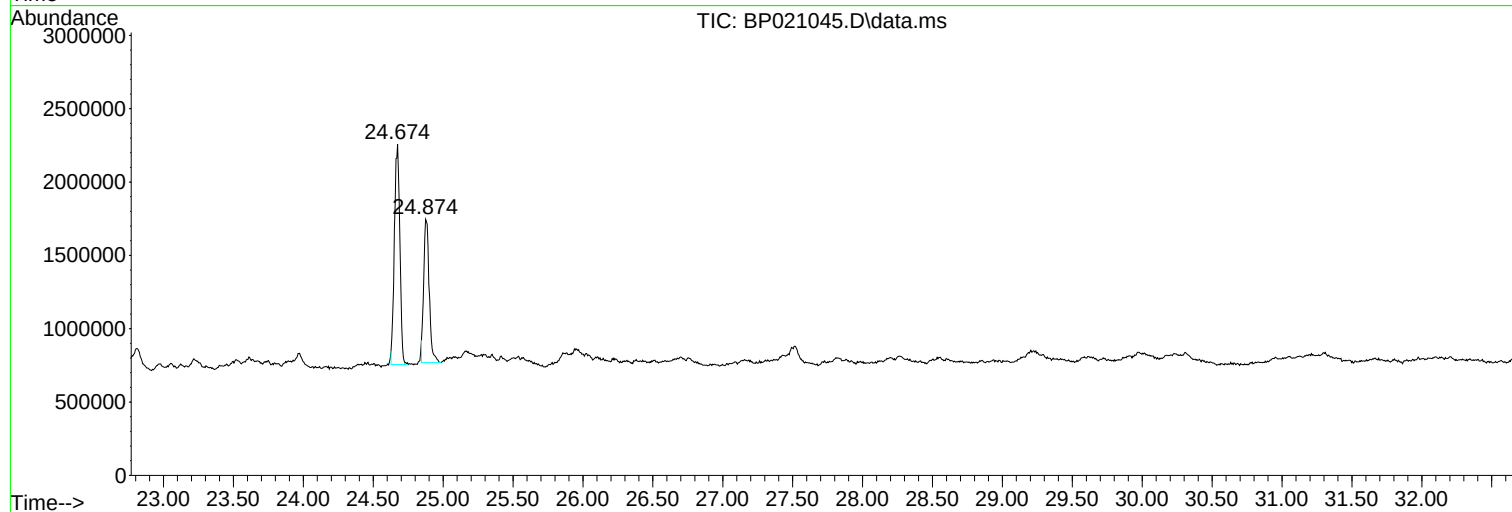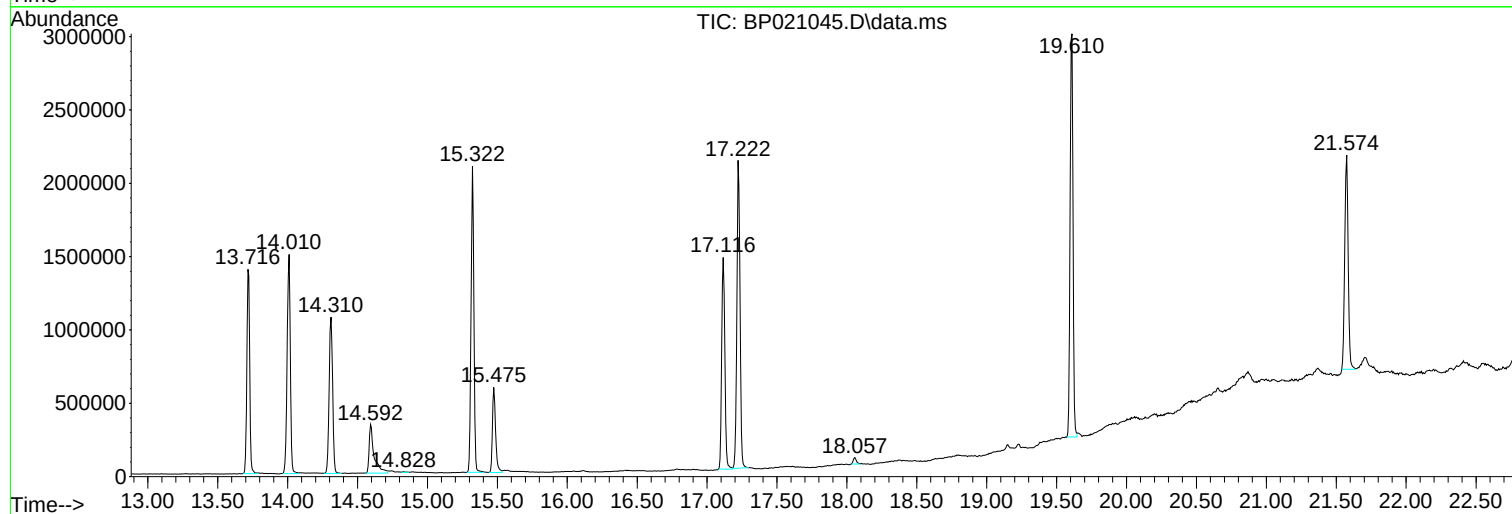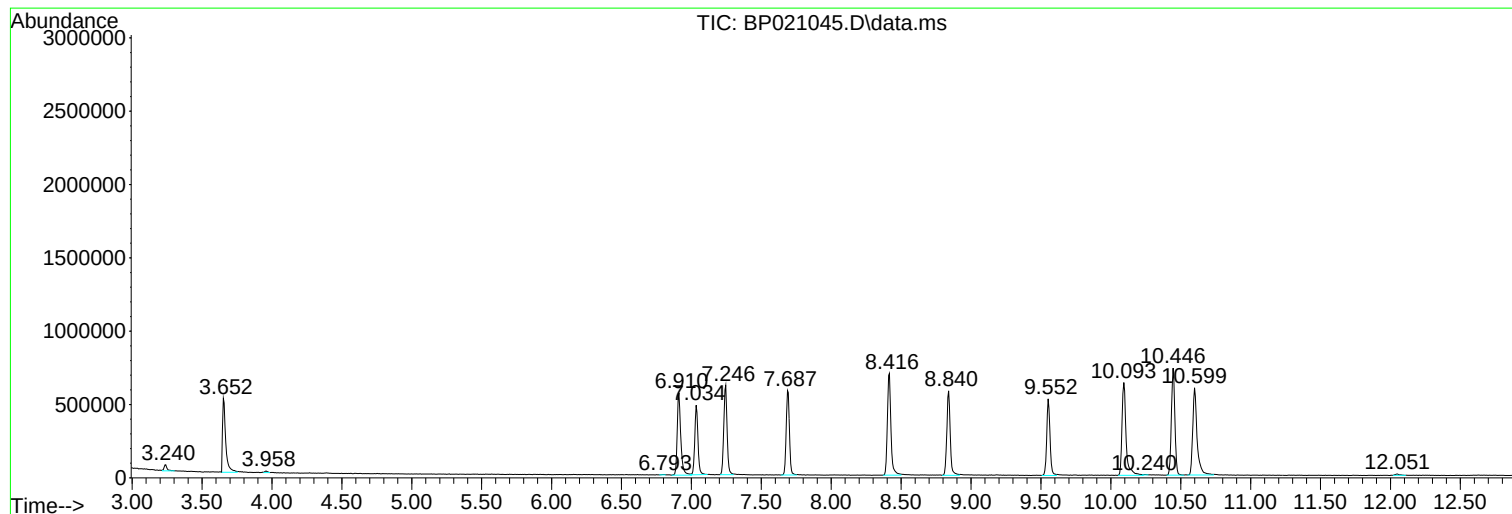

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071824\
Data File : BP021045.D
Acq On : 18 Jul 2024 14:02
Operator : MA/JU
Sample : PB162120BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK120

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071824\
Data File : BP021045.D
Acq On : 18 Jul 2024 14:02
Operator : MA/JU
Sample : PB162120BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK120

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------