

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071824\
 Data File : BP021059.D
 Acq On : 19 Jul 2024 00:47
 Operator : MA/JU
 Sample : PB162066BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK066

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP021059.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.234	39	42	47	rVB	48535	53512	1.33%	0.133%
2	3.652	110	113	132	rBV	474144	788356	19.64%	1.959%
3	3.958	161	165	171	rVB2	10580	16278	0.41%	0.040%
4	6.799	645	648	652	rBV5	4365	6946	0.17%	0.017%
5	6.899	658	665	681	rBV	614218	1031883	25.70%	2.564%
6	7.034	681	688	702	rVB	447697	767540	19.12%	1.907%
7	7.240	715	723	737	rBV	600241	1043105	25.98%	2.592%
8	7.687	792	799	810	rBV	620584	968150	24.12%	2.406%
9	7.981	847	849	856	rVB8	2259	4240	0.11%	0.011%
10	8.405	914	921	941	rBV	632496	1258789	31.36%	3.128%
11	8.834	987	994	1005	rBV	520623	972768	24.23%	2.417%
12	9.546	1106	1115	1124	rBV	507980	855272	21.30%	2.125%
13	10.099	1199	1209	1222	rBV	520482	1244012	30.99%	3.091%
14	10.446	1260	1268	1278	rBV	769527	1338413	33.34%	3.326%
15	10.604	1287	1295	1315	rBV	572479	1175595	29.28%	2.921%
16	12.051	1537	1541	1542	rBV3	6664	8318	0.21%	0.021%
17	12.069	1542	1544	1550	rVB6	7187	10179	0.25%	0.025%
18	13.269	1744	1748	1752	rBV6	4133	7776	0.19%	0.019%
19	13.716	1817	1824	1833	rBV	1198736	1801839	44.88%	4.477%
20	14.004	1866	1873	1892	rBV	1644570	2220232	55.31%	5.517%
21	14.310	1919	1925	1936	rBV	1217469	1784169	44.44%	4.433%
22	14.587	1965	1972	1993	rBV	241531	785432	19.56%	1.952%
23	14.728	1994	1996	2002	rVB7	14867	23818	0.59%	0.059%
24	15.322	2090	2097	2117	rBV	1847628	2760767	68.77%	6.860%
25	15.481	2117	2124	2136	rBV	433874	833366	20.76%	2.071%
26	15.851	2183	2187	2190	rVV6	5689	7845	0.20%	0.019%
27	16.128	2229	2234	2241	rBV6	5964	12393	0.31%	0.031%
28	16.792	2344	2347	2352	rVB7	4528	5530	0.14%	0.014%
29	17.128	2396	2404	2415	rBV	1259085	2169261	54.04%	5.390%
30	17.233	2415	2422	2433	rBV	1974519	3040611	75.74%	7.555%
31	17.810	2517	2520	2525	rVB6	9256	14476	0.36%	0.036%
32	18.063	2559	2563	2566	rBV4	15654	23067	0.57%	0.057%
33	19.163	2747	2750	2755	rBV5	20095	25516	0.64%	0.063%
34	19.616	2821	2827	2839	rBV	2537053	3845741	95.80%	9.556%
35	21.574	3154	3160	3178	rVB	1525504	2478121	61.73%	6.158%
36	24.657	3675	3684	3701	rVB2	1517508	4014491	100.00%	9.975%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071824\
Data File : BP021059.D
Acq On : 19 Jul 2024 00:47
Operator : MA/JU
Sample : PB162066BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK066

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Title : SVOA CALIBRATION

37	24.886	3716	3723	3740	rVB	992483	2846756	70.91%	7.074%
----	--------	------	------	------	-----	--------	---------	--------	--------




Sum of corrected areas: 40244563

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071824\
Data File : BP021059.D
Acq On : 19 Jul 2024 00:47
Operator : MA/JU
Sample : PB162066BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK066

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

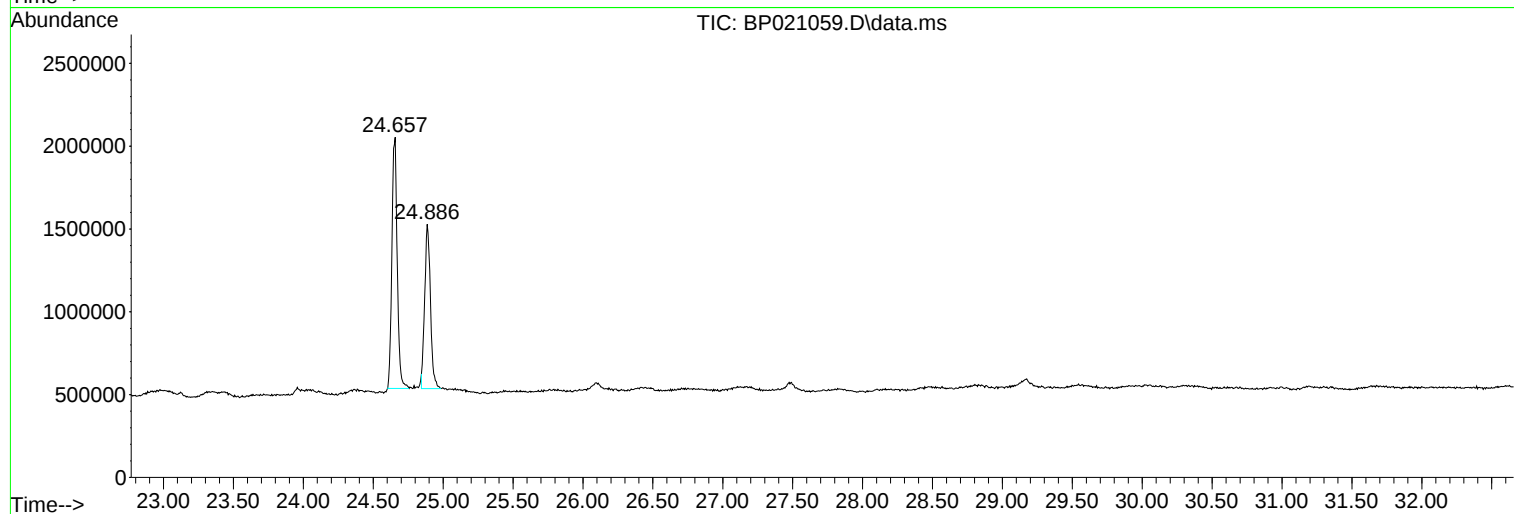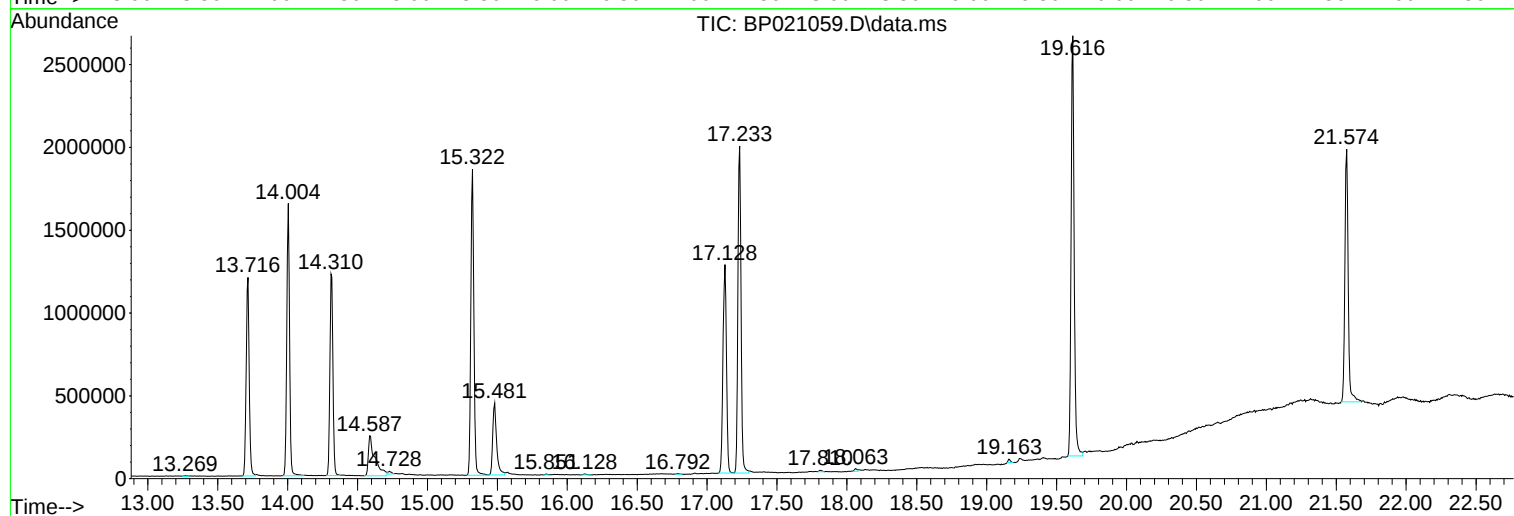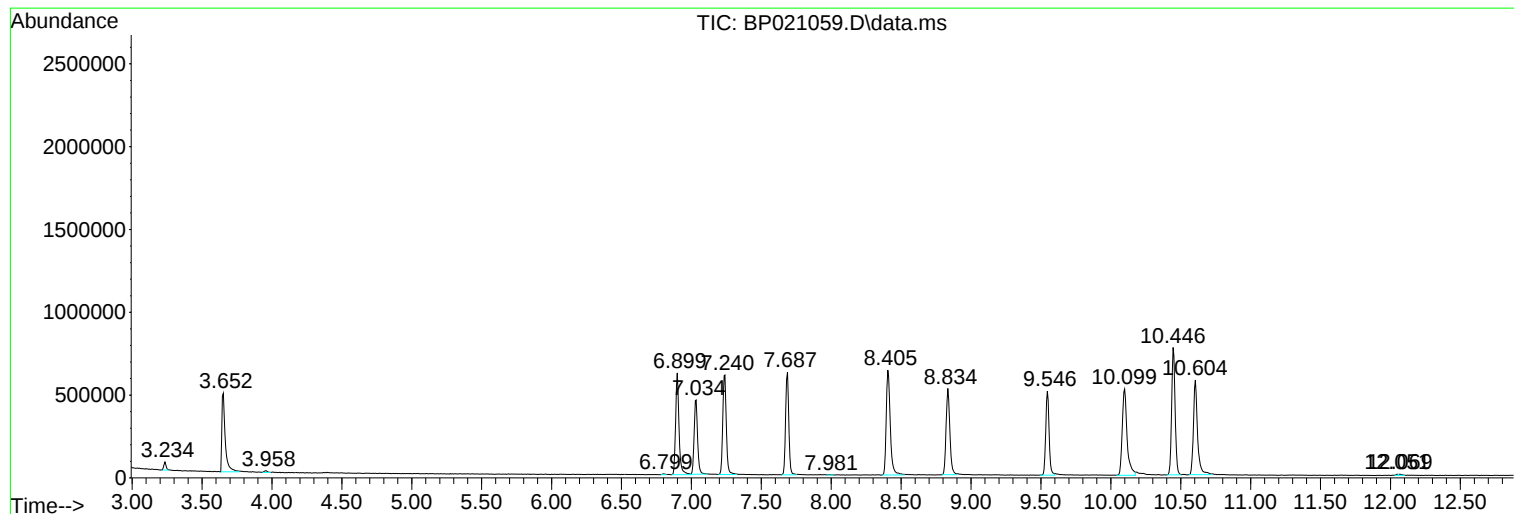

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071824\
Data File : BP021059.D
Acq On : 19 Jul 2024 00:47
Operator : MA/JU
Sample : PB162066BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK066

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071824\
Data File : BP021059.D
Acq On : 19 Jul 2024 00:47
Operator : MA/JU
Sample : PB162066BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK066

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------