




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071923\
 Data File : BP016324.D
 Acq On : 19 Jul 2023 14:47
 Operator : MA/JU
 Sample : 03501-09
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A46X4

Manual IntegrationsAPPROVED

Quant Time: Jul 19 23:35:12 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jul 19 14:47:57 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/20/2023
 Supervised By :mohammad ahmed 07/20/2023

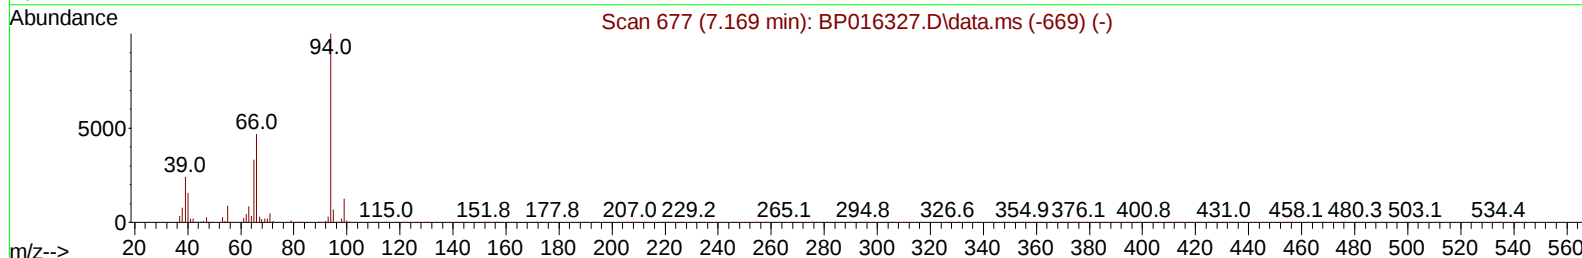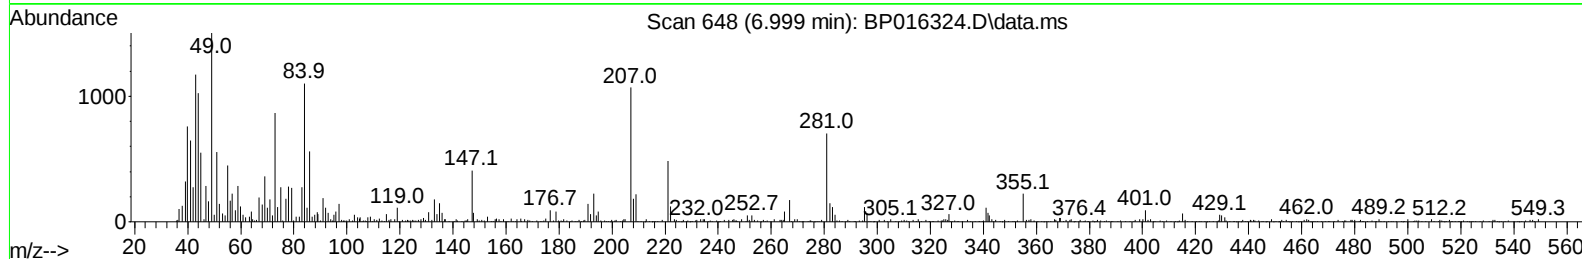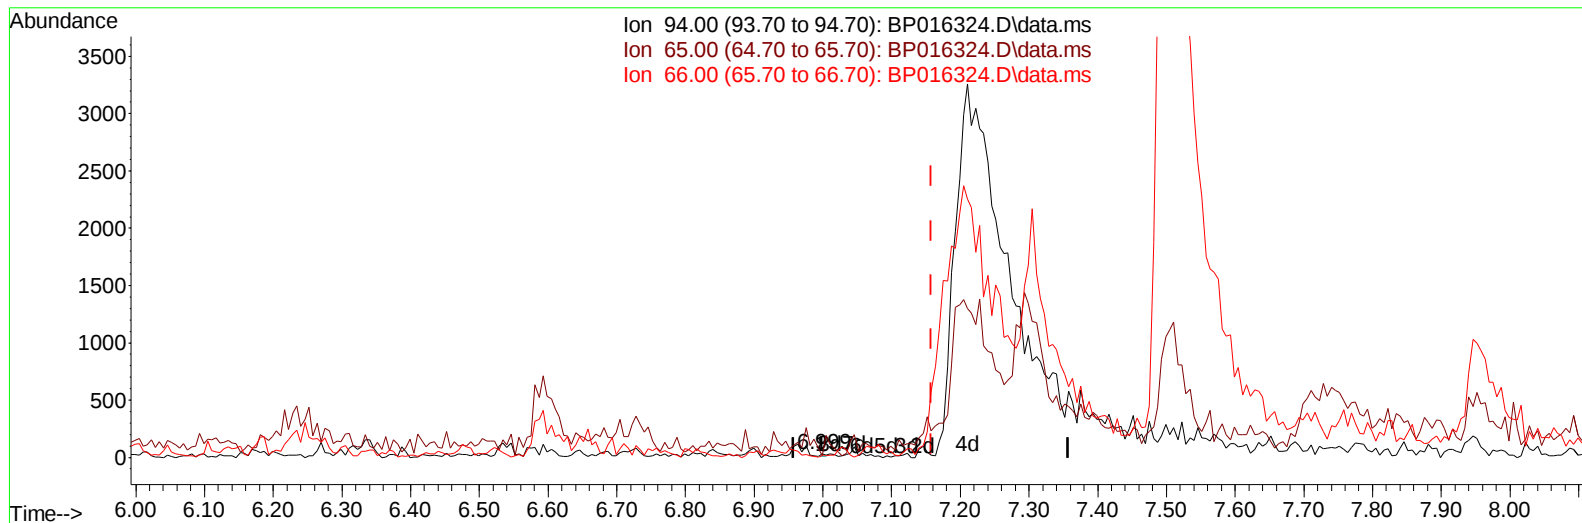

TIC: BP016324.D\data.ms

(8) Phenol

6.999min (-0.159) 0.00 ng/u1

response 12

Ion	Exp%	Act%
94.00	100.00	100.00
65.00	31.90	37.50
66.00	40.90	46.88
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071923\
 Data File : BP016324.D
 Acq On : 19 Jul 2023 14:47
 Operator : MA/JU
 Sample : 03501-09
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A46X4

Manual IntegrationsAPPROVED

Quant Time: Jul 19 23:35:12 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jul 19 14:47:57 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/20/2023
 Supervised By :mohammad ahmed 07/20/2023

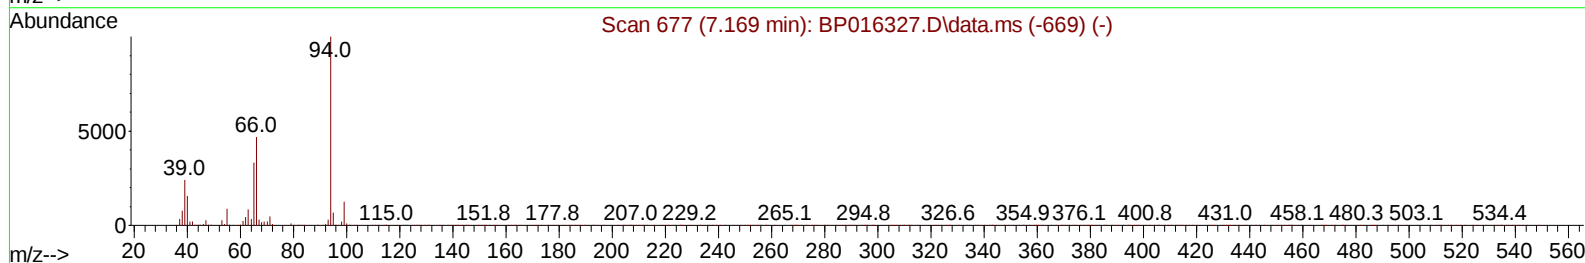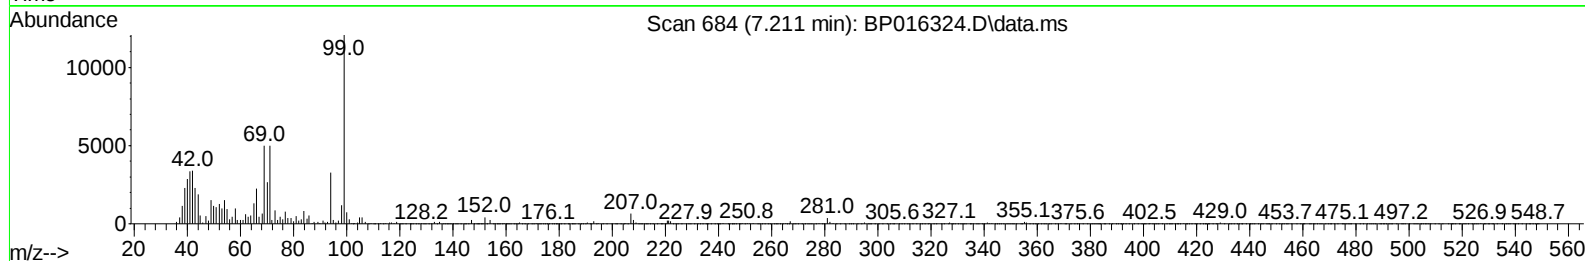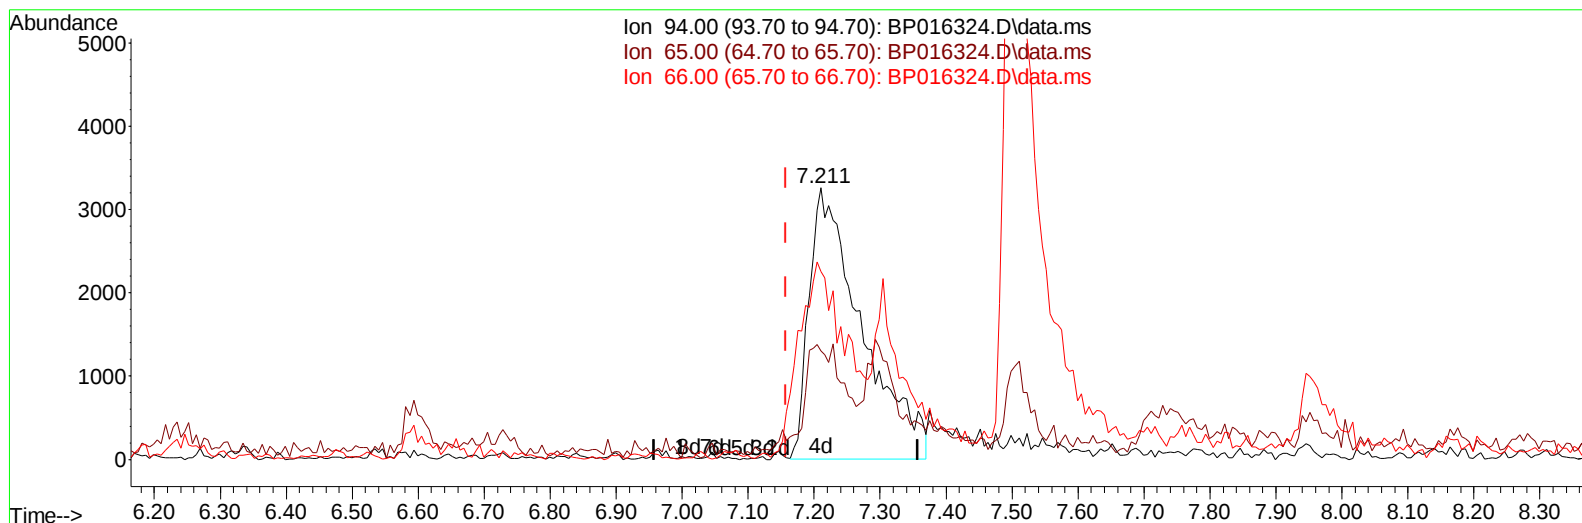

TIC: BP016324.D\data.ms

(8) Phenol

7.211min (+ 0.053) 2.10 ng/ul m

response 17960

Ion	Exp%	Act%
94.00	100.00	100.00
65.00	31.90	39.92#
66.00	40.90	69.22#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071923\
 Data File : BP016324.D
 Acq On : 19 Jul 2023 14:47
 Operator : MA/JU
 Sample : 03501-09
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A46X4

Manual IntegrationsAPPROVED

Quant Time: Jul 19 23:35:12 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jul 19 14:47:57 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/20/2023
 Supervised By :mohammad ahmed 07/20/2023

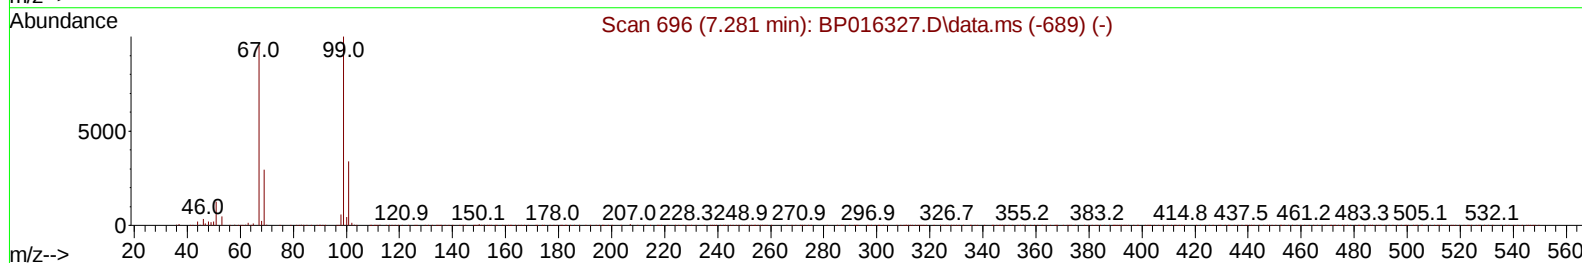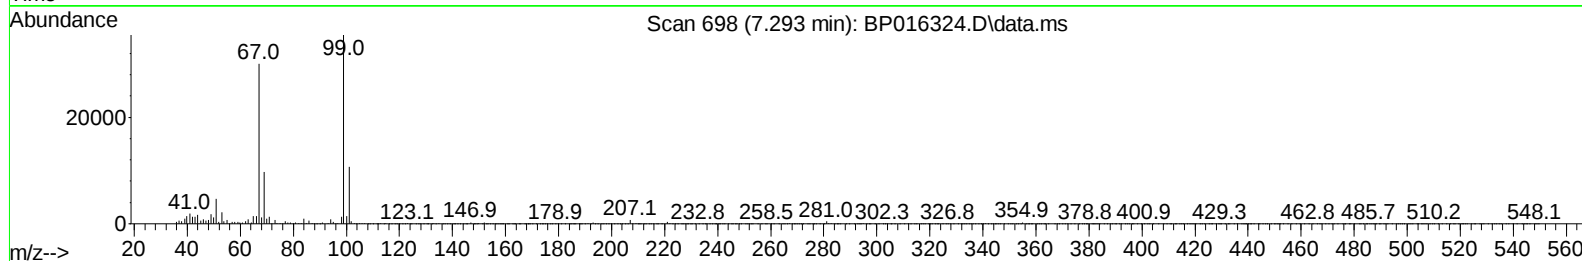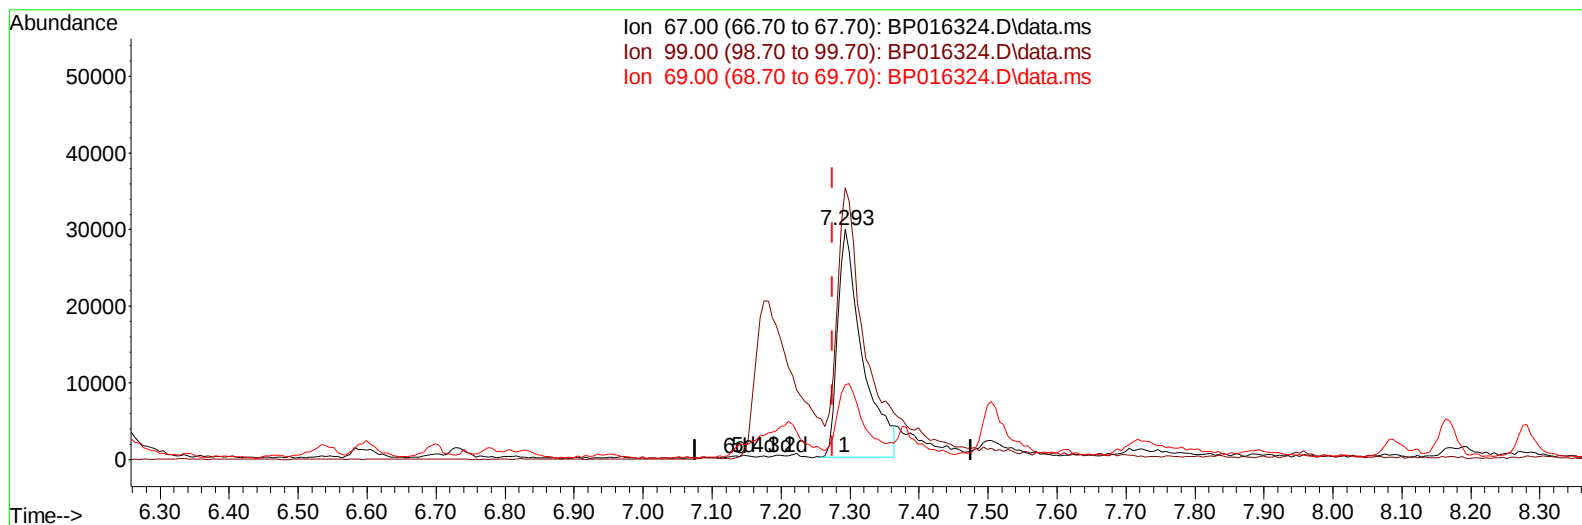

TIC: BP016324.D\data.ms

(9) Bis-(2-Chloroethyl)ether-d8 (S)

7.293min (+ 0.018) 13.73 ng/u1

response 74068

Ion	Exp%	Act%
67.00	100.00	100.00
99.00	117.30	118.07
69.00	33.10	32.50
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071923\
 Data File : BP016324.D
 Acq On : 19 Jul 2023 14:47
 Operator : MA/JU
 Sample : 03501-09
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A46X4

Manual IntegrationsAPPROVED

Quant Time: Jul 19 23:35:12 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jul 19 14:47:57 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/20/2023
 Supervised By :mohammad ahmed 07/20/2023

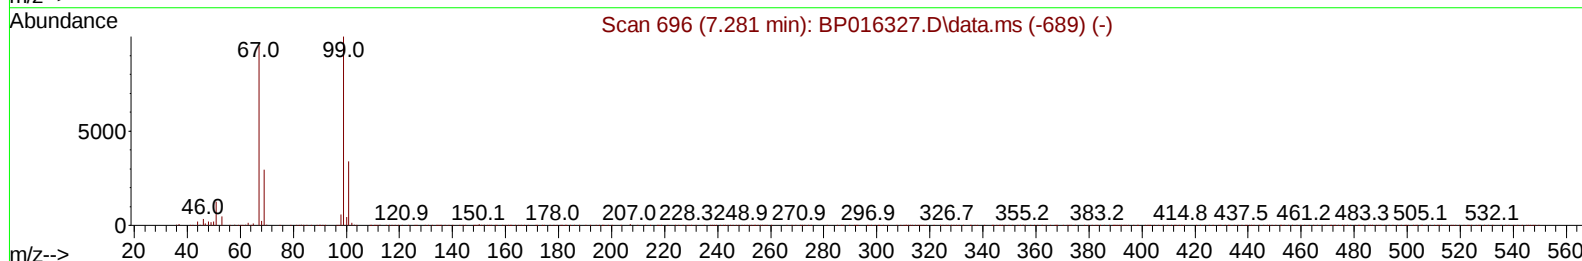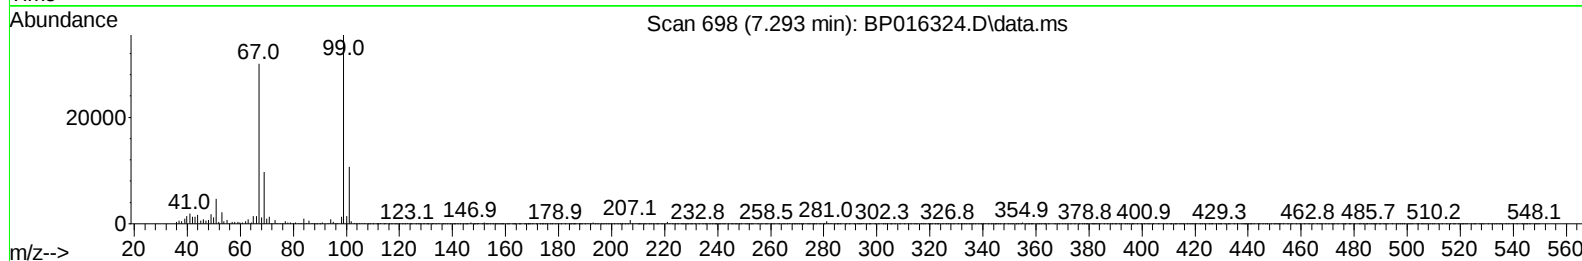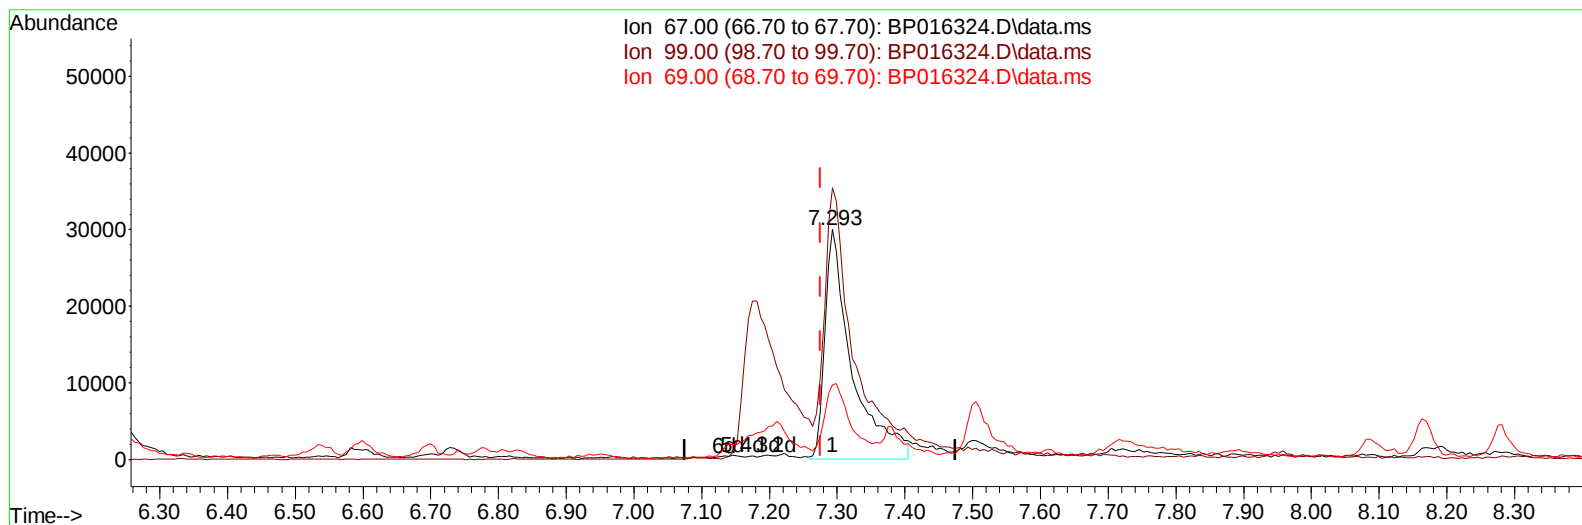

TIC: BP016324.D\data.ms

(9) Bis-(2-Chloroethyl)ether-d8 (S)

7.293min (+ 0.018) 15.41 ng/ul m

response 83167

Ion	Exp%	Act%
67.00	100.00	100.00
99.00	117.30	118.07
69.00	33.10	32.50
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071923\
 Data File : BP016324.D
 Acq On : 19 Jul 2023 14:47
 Operator : MA/JU
 Sample : 03501-09
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A46X4

Manual IntegrationsAPPROVED

Quant Time: Jul 19 23:35:12 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jul 19 14:47:57 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/20/2023
 Supervised By :mohammad ahmed 07/20/2023

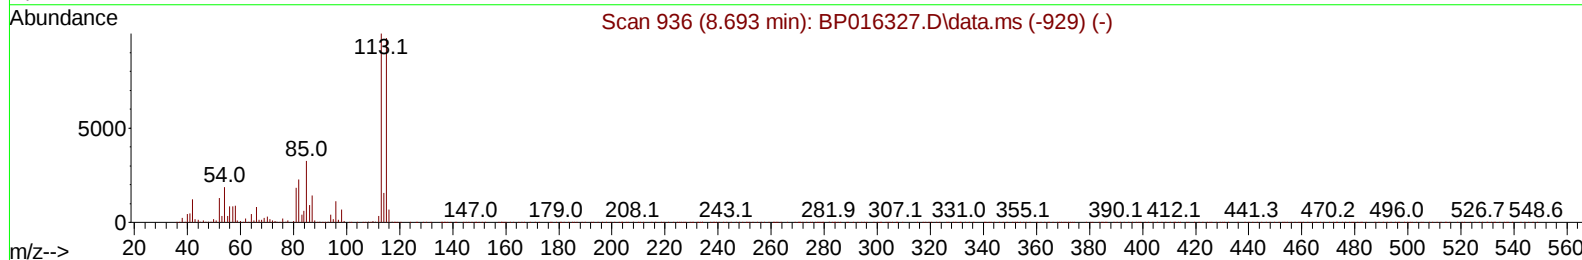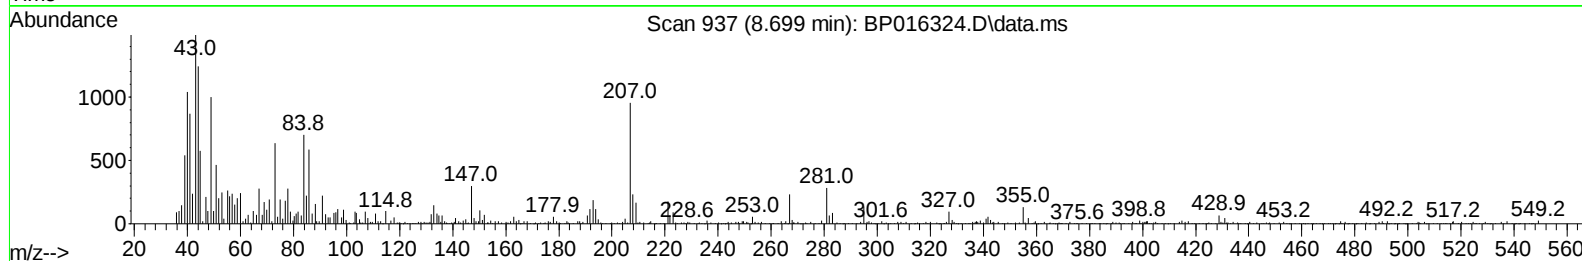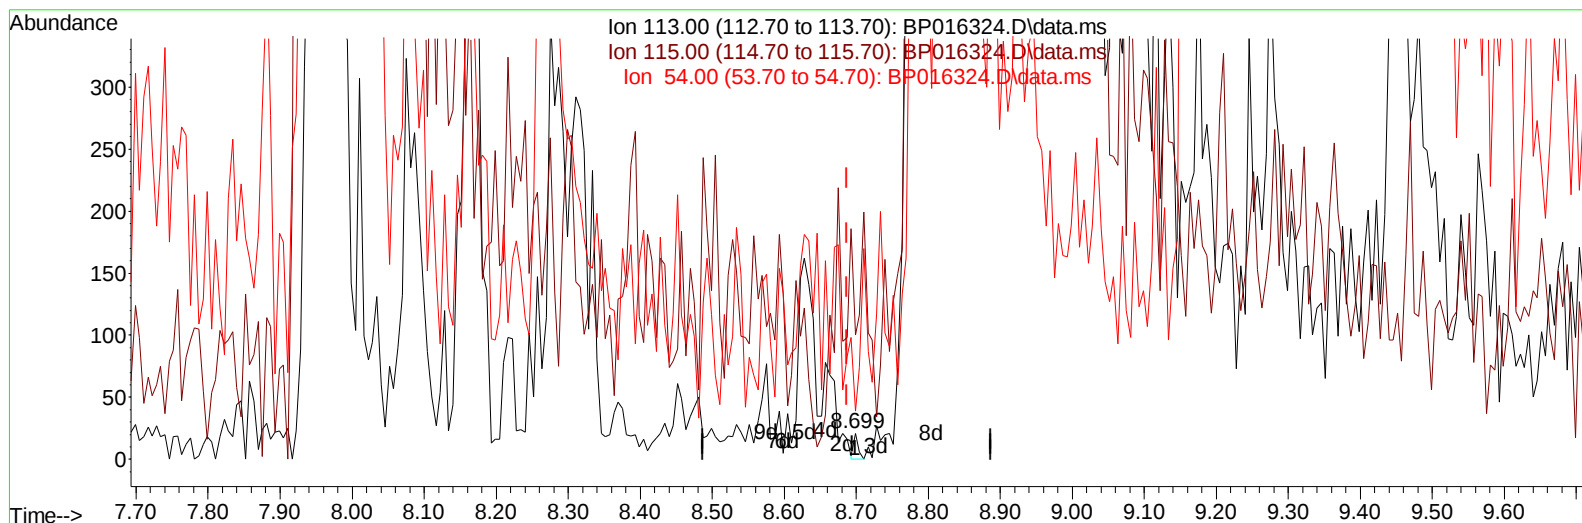

TIC: BP016324.D\data.ms

(15) 4-Methylphenol-d8 (S)

8.699min (+ 0.012) 0.00 ng/u1

response 10

Ion	Exp%	Act%
113.00	100.00	100.00
115.00	90.20	476.19#
54.00	16.30	185.71#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071923\
 Data File : BP016324.D
 Acq On : 19 Jul 2023 14:47
 Operator : MA/JU
 Sample : 03501-09
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A46X4

Manual IntegrationsAPPROVED

Quant Time: Jul 19 23:35:12 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jul 19 14:47:57 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/20/2023
 Supervised By :mohammad ahmed 07/20/2023

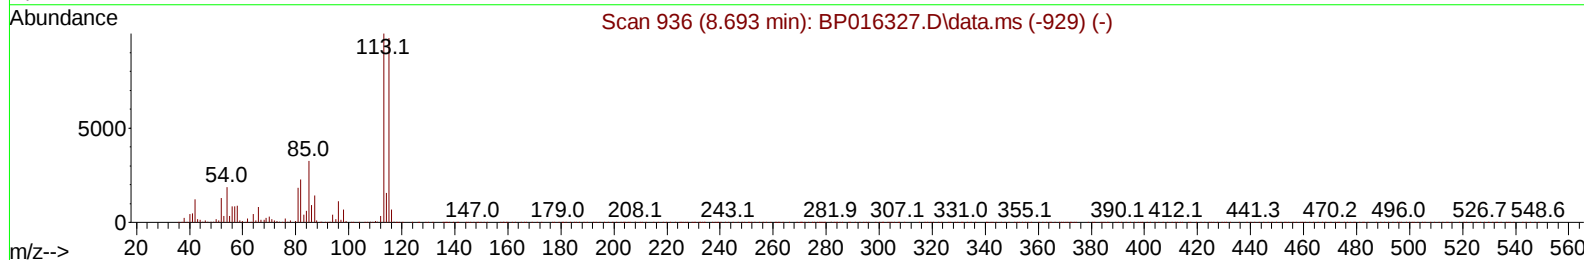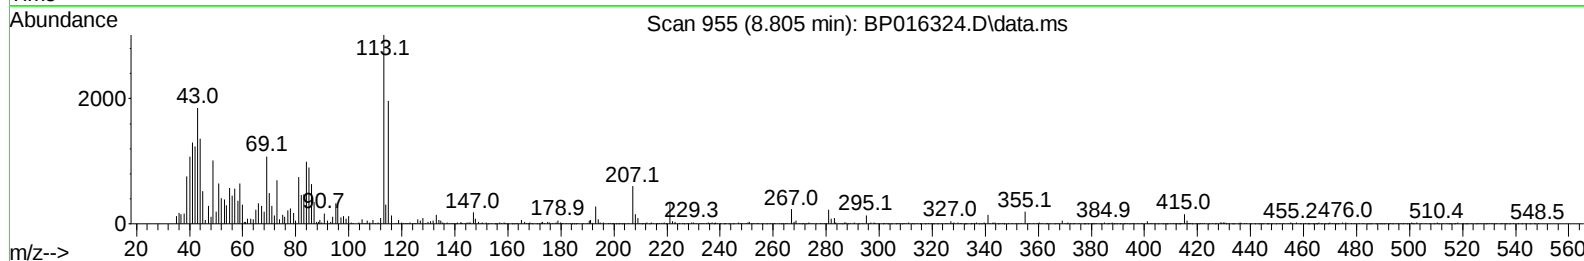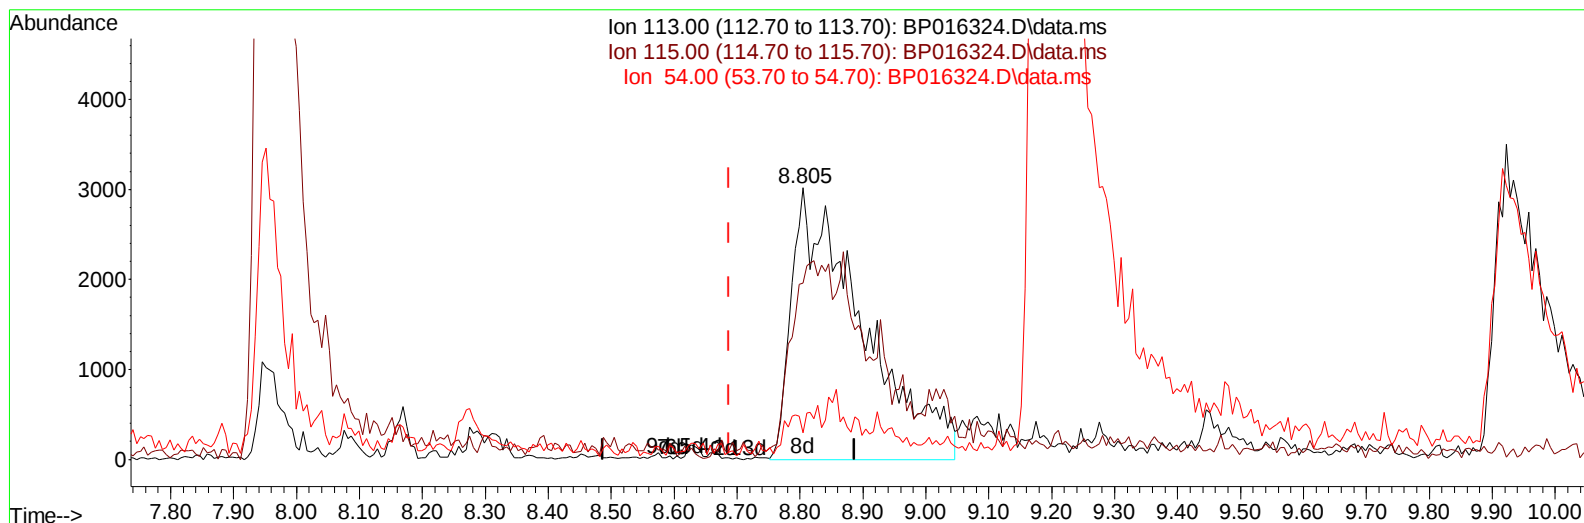

TIC: BP016324.D\data.ms

(15) 4-Methylphenol-d8 (S)

8.805min (+ 0.118) 3.65 ng/ul m

response 23440

Ion	Exp%	Act%
113.00	100.00	100.00
115.00	90.20	65.06#
54.00	16.30	9.91#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071923\
 Data File : BP016324.D
 Acq On : 19 Jul 2023 14:47
 Operator : MA/JU
 Sample : 03501-09
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A46X4

Manual IntegrationsAPPROVED

Quant Time: Jul 19 23:35:12 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jul 19 14:47:57 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/20/2023
 Supervised By :mohammad ahmed 07/20/2023

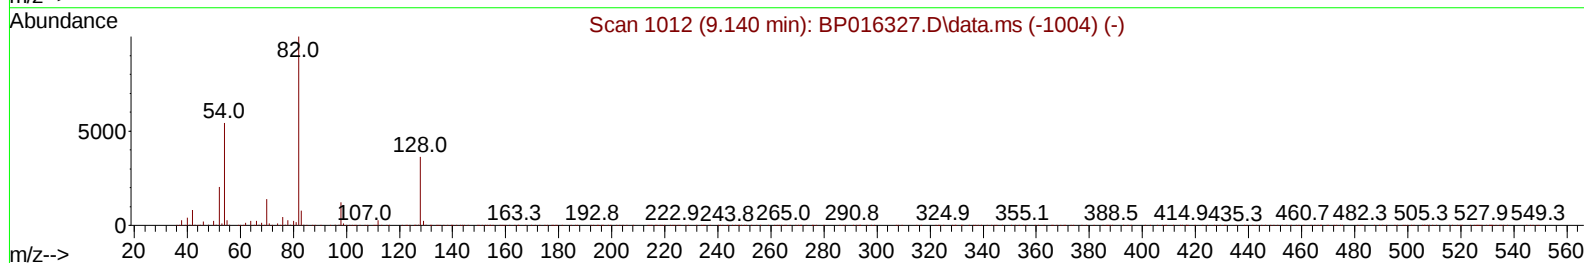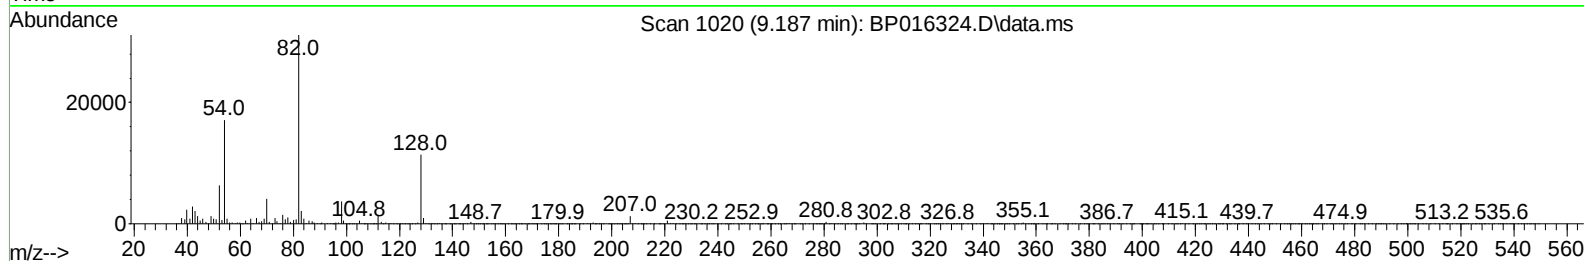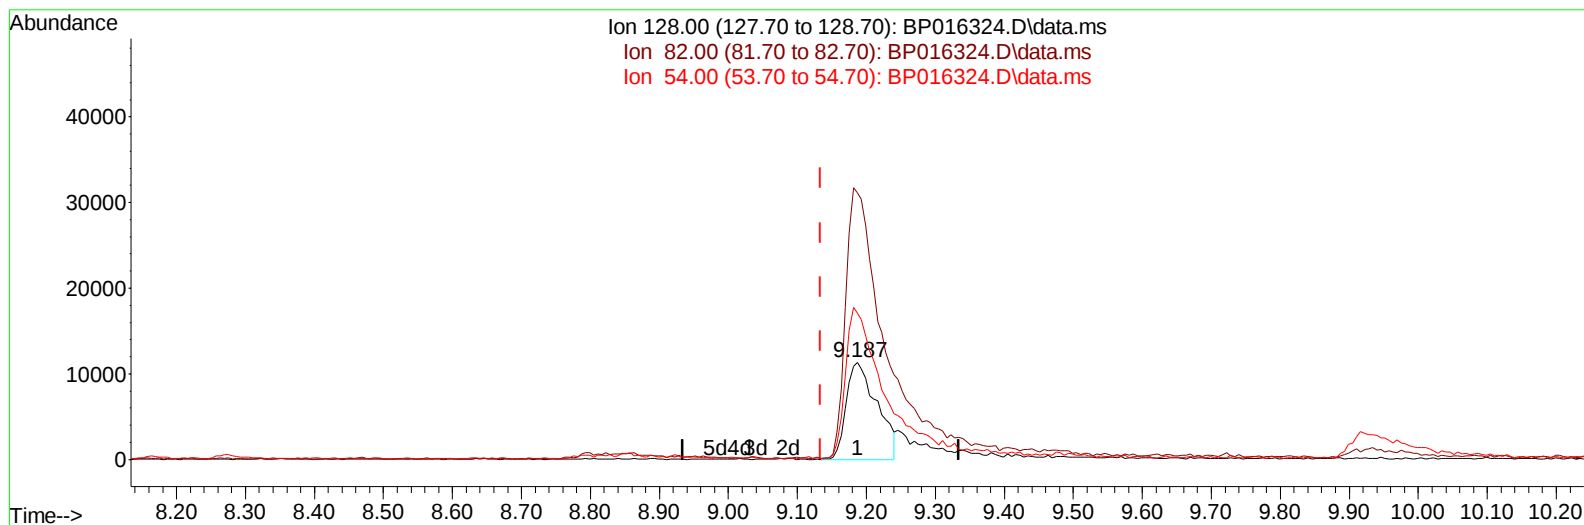

TIC: BP016324.D\data.ms

(21) Nitrobenzene-d5 (S)

9.187min (+ 0.053) 12.69 ng/u1

response 35316

Ion	Exp%	Act%
128.00	100.00	100.00
82.00	261.40	274.33
54.00	136.80	150.88
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071923\
 Data File : BP016324.D
 Acq On : 19 Jul 2023 14:47
 Operator : MA/JU
 Sample : 03501-09
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A46X4

Manual IntegrationsAPPROVED

Quant Time: Jul 19 23:35:12 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jul 19 14:47:57 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/20/2023
 Supervised By :mohammad ahmed 07/20/2023

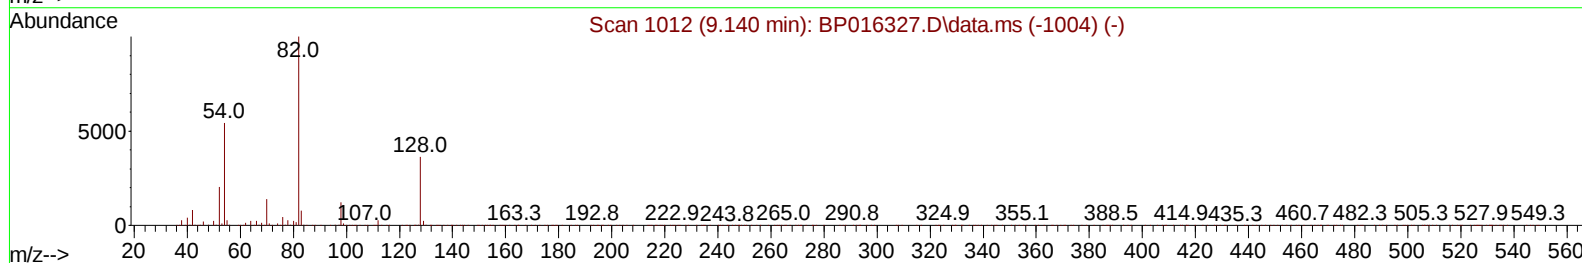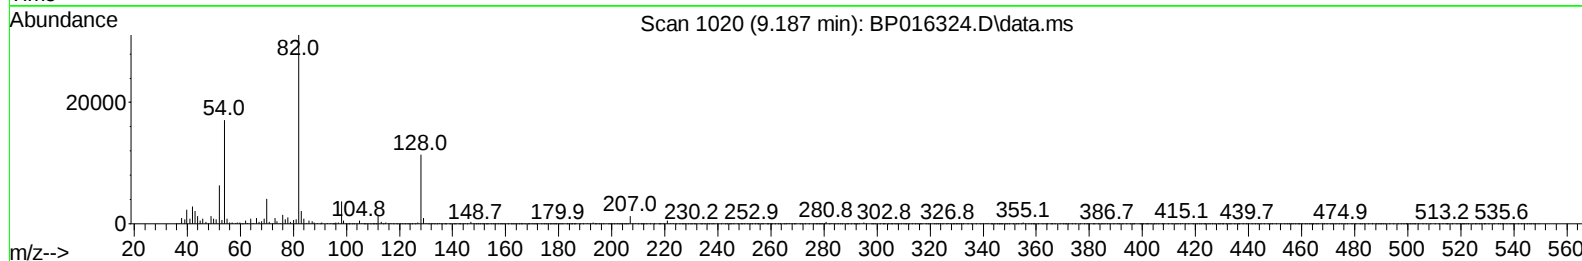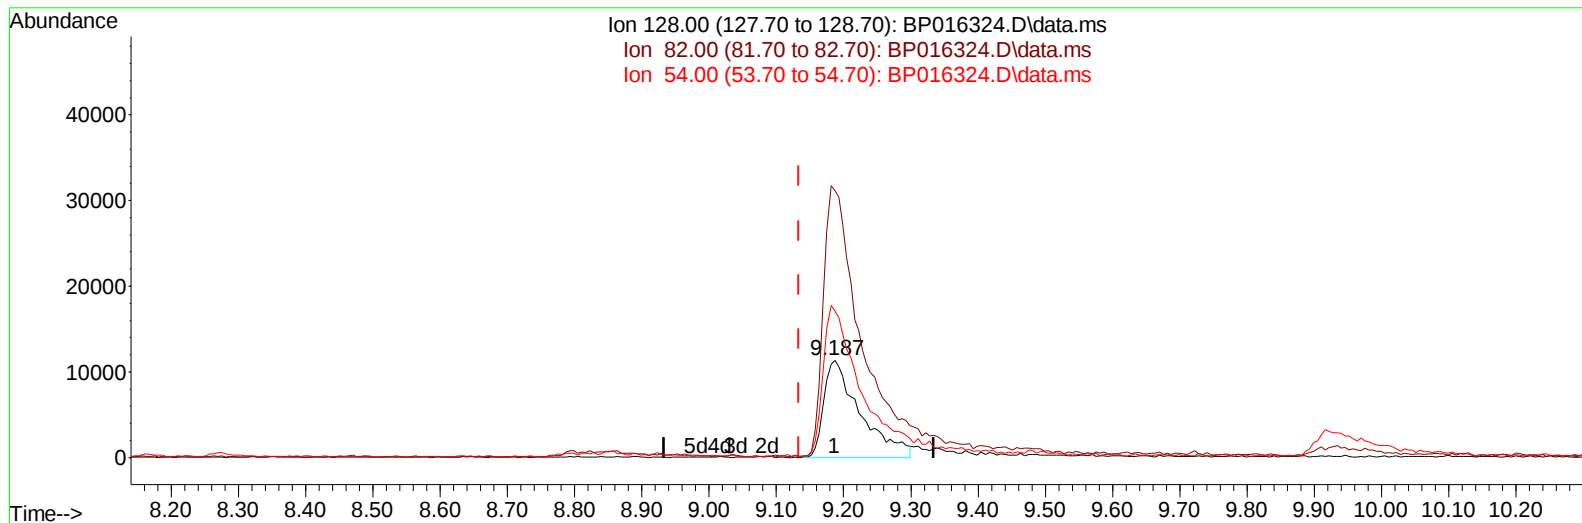

TIC: BP016324.D\data.ms

(21) Nitrobenzene-d5 (S)

9.187min (+ 0.053) 15.35 ng/ul m

response 42722

Ion	Exp%	Act%
128.00	100.00	100.00
82.00	261.40	274.33
54.00	136.80	150.88
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071923\
Data File : BP016324.D
Acq On : 19 Jul 2023 14:47
Operator : MA/JU
Sample : 03501-09
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A46X4

Manual IntegrationsAPPROVED

Quant Time: Jul 19 23:35:12 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jul 19 14:47:57 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/20/2023
Supervised By :mohammad ahmed 07/20/2023

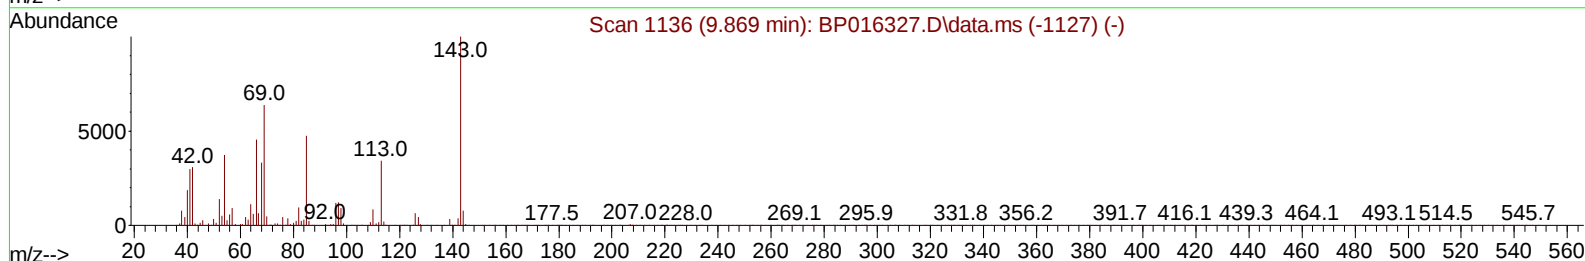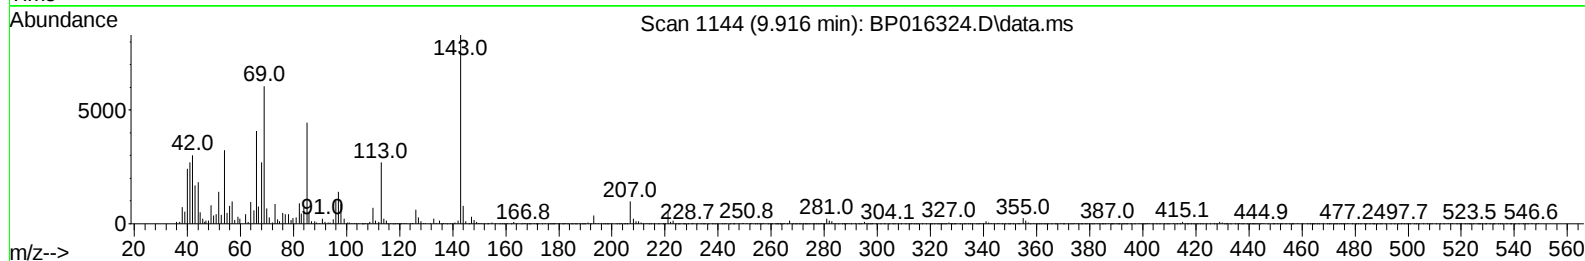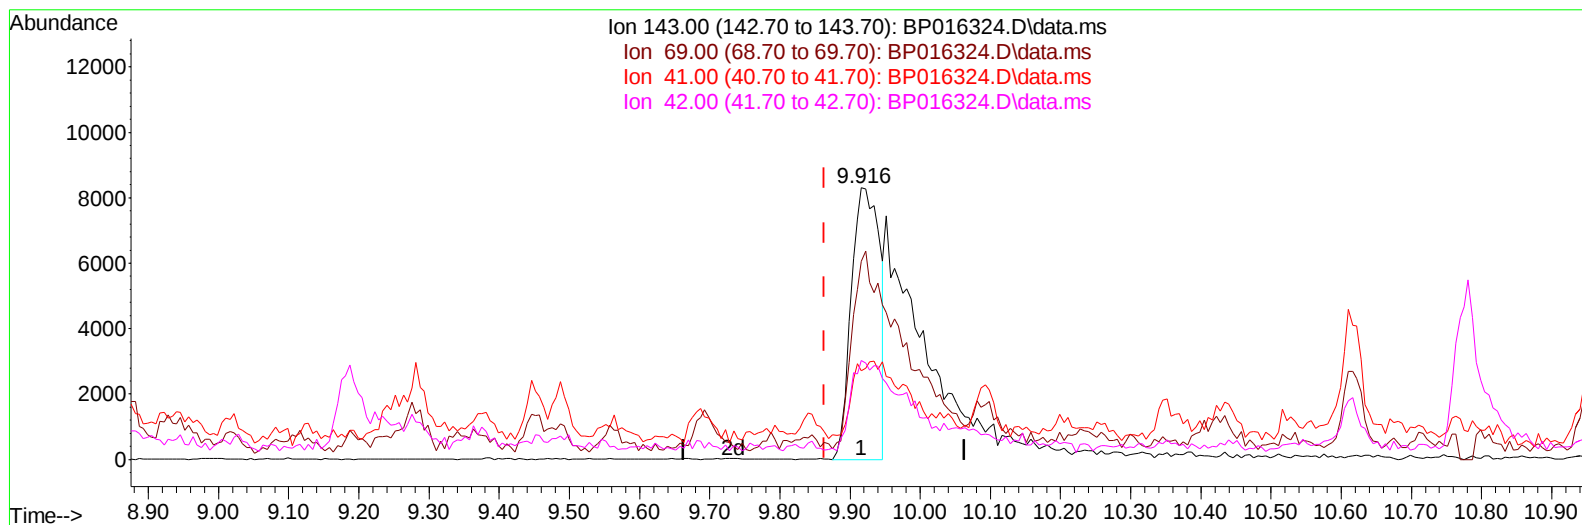

TIC: BP016324.D\data.ms

(24) 2-Nitrophenol-d4 (S)

9.916min (+ 0.053) 7.31 ng/u1

response 23196

Ion	Exp%	Act%
143.00	100.00	100.00
69.00	62.00	73.03
41.00	28.60	32.66
42.00	29.20	36.37#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071923\
Data File : BP016324.D
Acq On : 19 Jul 2023 14:47
Operator : MA/JU
Sample : 03501-09
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A46X4

Manual IntegrationsAPPROVED

Quant Time: Jul 19 23:35:12 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jul 19 14:47:57 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/20/2023
Supervised By :mohammad ahmed 07/20/2023

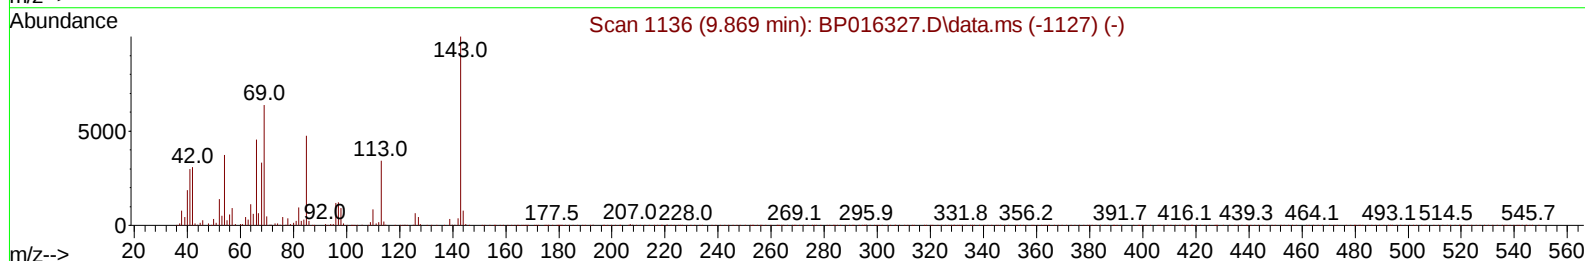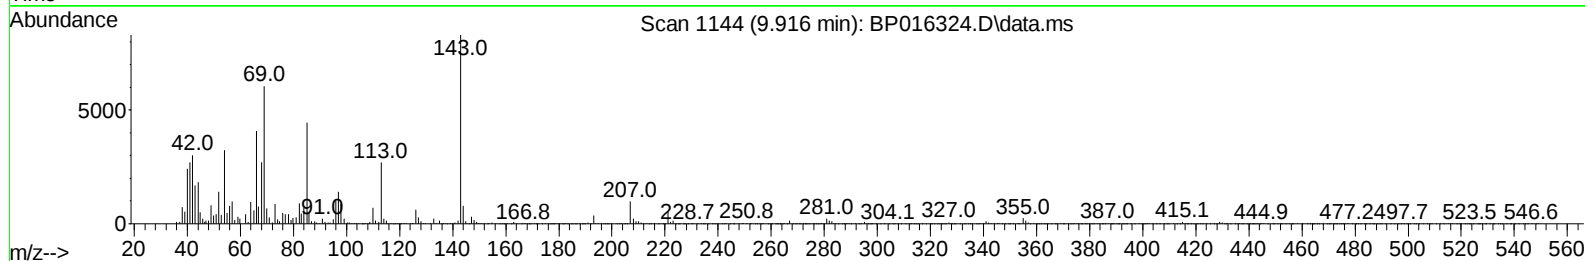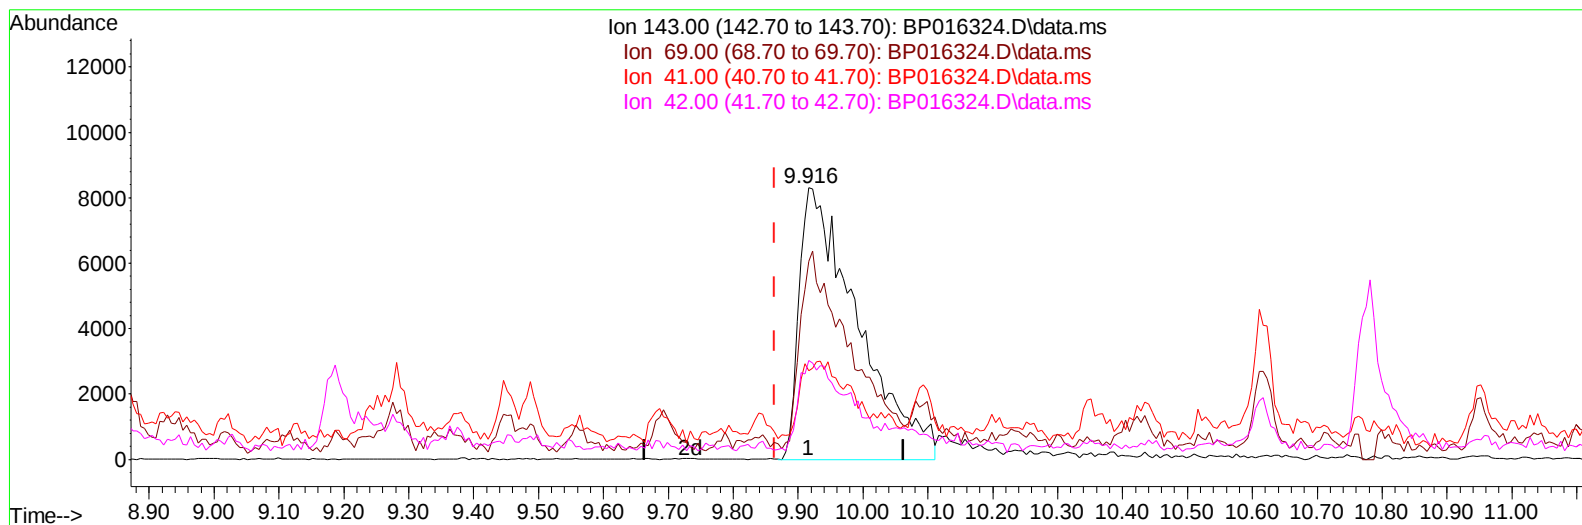

TIC: BP016324.D\data.ms

(24) 2-Nitrophenol-d4 (S)

9.916min (+ 0.053) 16.27 ng/ul m

response 51607

Ion	Exp%	Act%
143.00	100.00	100.00
69.00	62.00	73.03
41.00	28.60	32.66
42.00	29.20	36.37#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071923\
Data File : BP016324.D
Acq On : 19 Jul 2023 14:47
Operator : MA/JU
Sample : 03501-09
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A46X4

Manual IntegrationsAPPROVED

Quant Time: Jul 19 23:35:12 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jul 19 14:47:57 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/20/2023
Supervised By :mohammad ahmed 07/20/2023

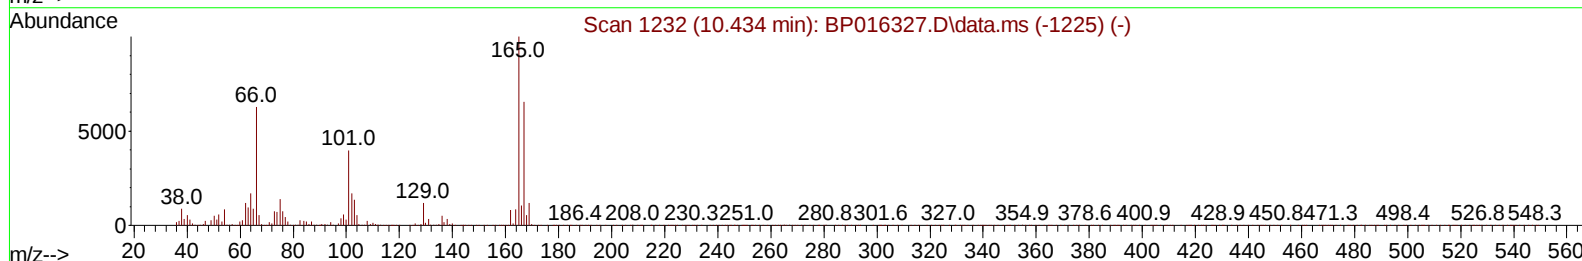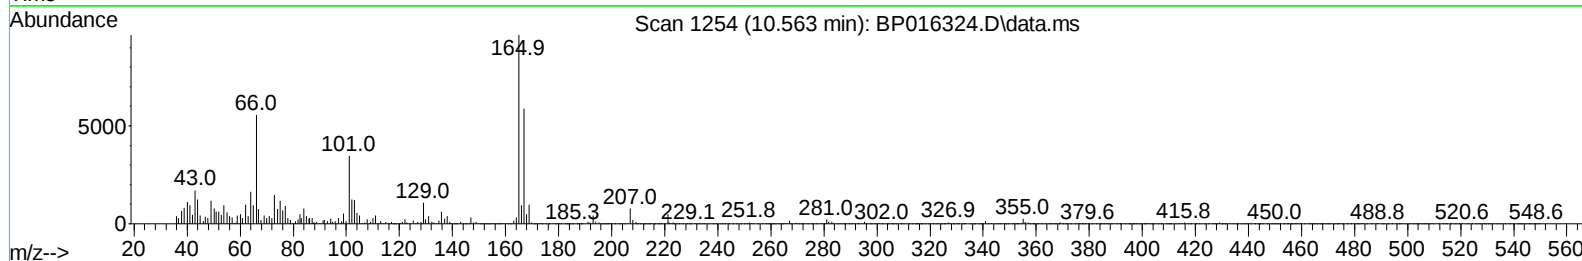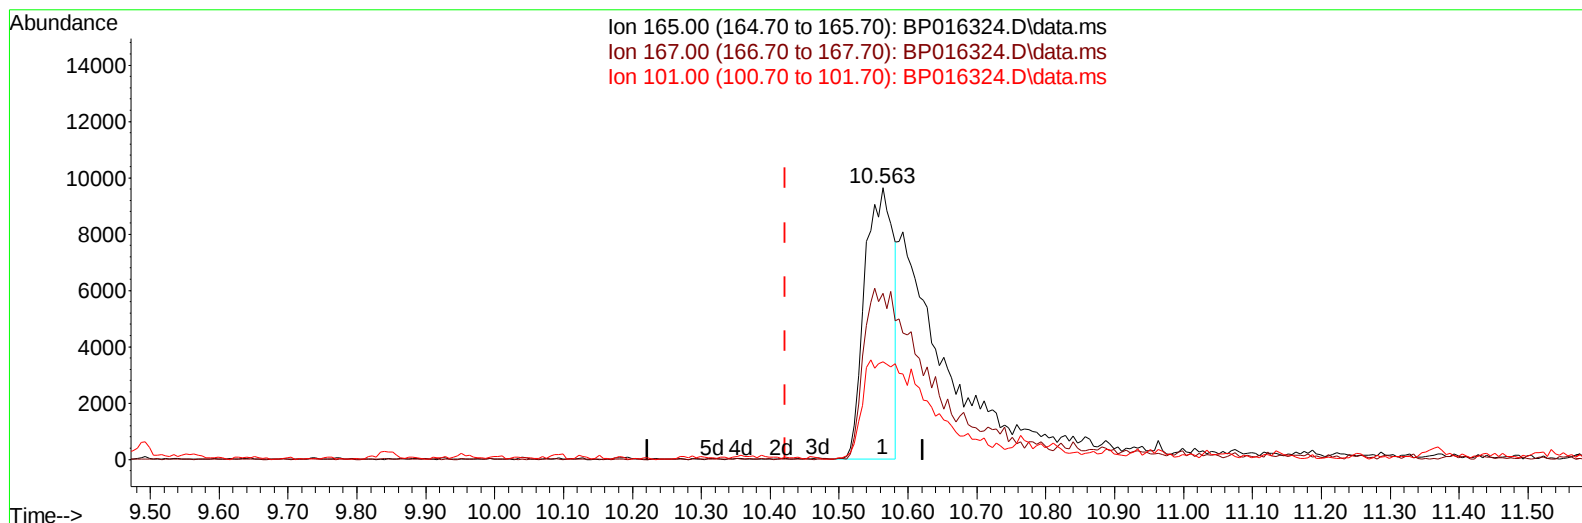

TIC: BP016324.D\data.ms

(28) 2,4-Dichlorophenol-d3 (S)

10.563min (+ 0.141) 5.01 ng/u1

response 27494

Ion	Exp%	Act%
165.00	100.00	100.00
167.00	65.20	61.10
101.00	38.50	35.99
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071923\
Data File : BP016324.D
Acq On : 19 Jul 2023 14:47
Operator : MA/JU
Sample : 03501-09
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A46X4

Manual IntegrationsAPPROVED

Quant Time: Jul 19 23:35:12 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jul 19 14:47:57 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/20/2023
Supervised By :mohammad ahmed 07/20/2023

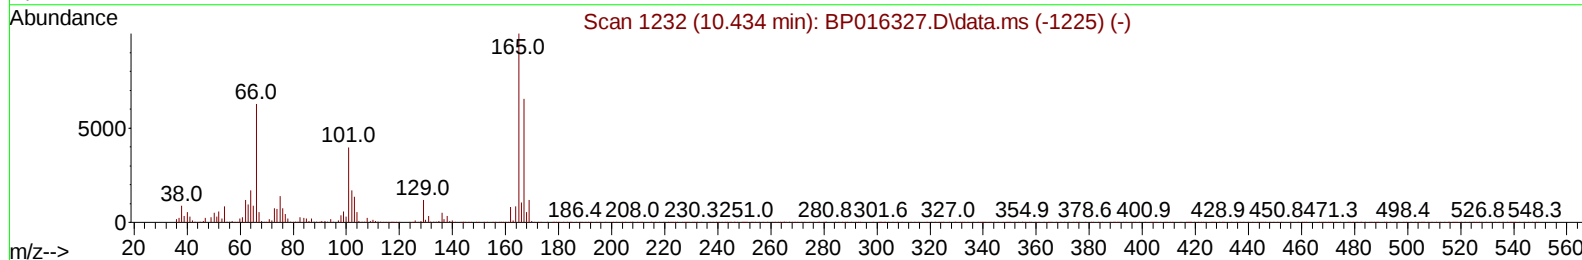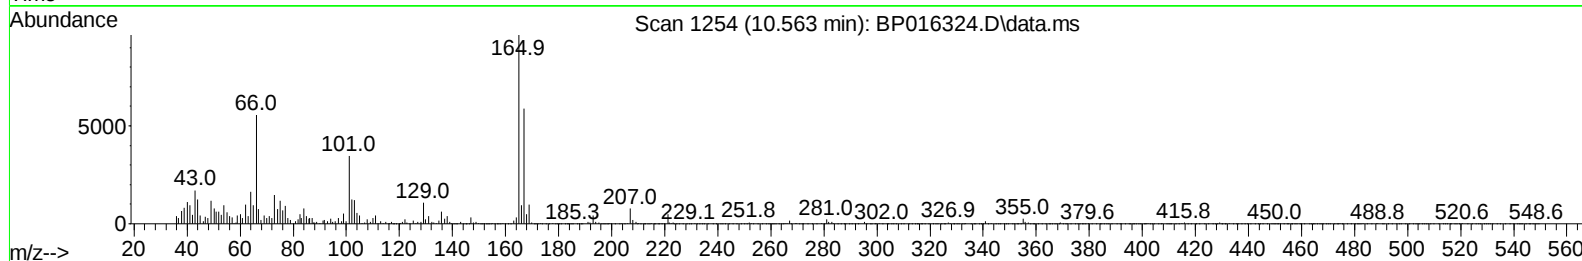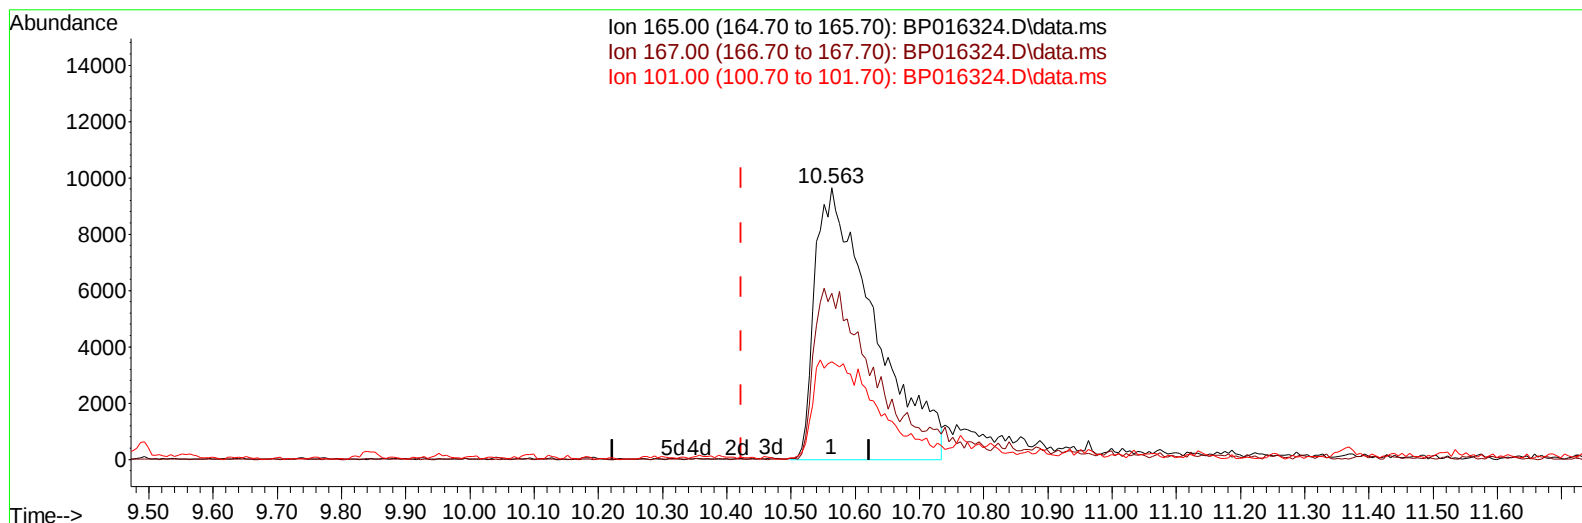

TIC: BP016324.D\data.ms

(28) 2,4-Dichlorophenol-d3 (S)

10.563min (+ 0.141) 11.29 ng/ul m

response 62006

Ion	Exp%	Act%
165.00	100.00	100.00
167.00	65.20	61.10
101.00	38.50	35.99
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071923\
 Data File : BP016324.D
 Acq On : 19 Jul 2023 14:47
 Operator : MA/JU
 Sample : 03501-09
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A46X4

Manual IntegrationsAPPROVED

Quant Time: Jul 19 23:35:12 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jul 19 14:47:57 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/20/2023
 Supervised By :mohammad ahmed 07/20/2023

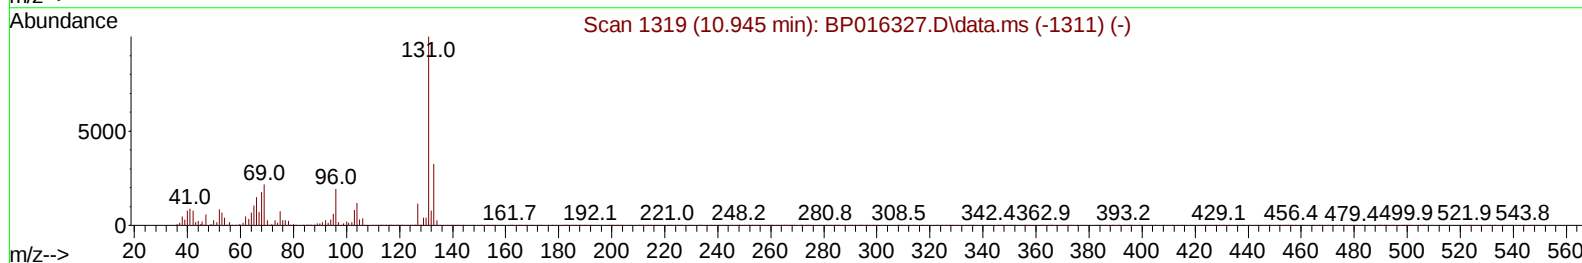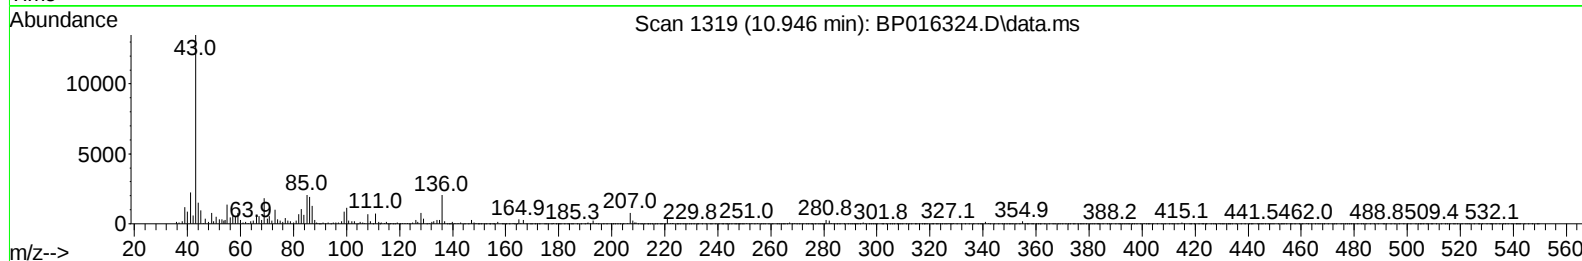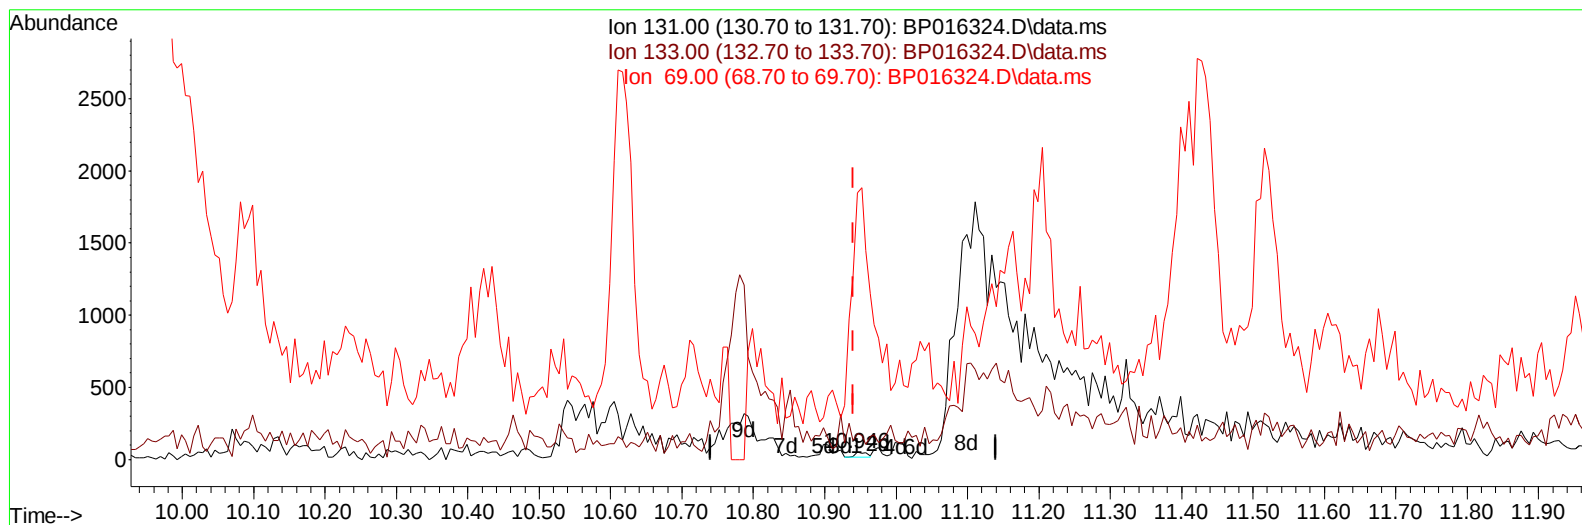

TIC: BP016324.D\data.ms

(31) 4-Chloroaniline-d4 (S)

10.946min (+ 0.006) 0.00 ng/ul

response 41

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	31.50	356.86#
69.00	21.00	3623.53#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071923\
 Data File : BP016324.D
 Acq On : 19 Jul 2023 14:47
 Operator : MA/JU
 Sample : 03501-09
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A46X4

Manual IntegrationsAPPROVED

Quant Time: Jul 19 23:35:12 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jul 19 14:47:57 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/20/2023
 Supervised By :mohammad ahmed 07/20/2023

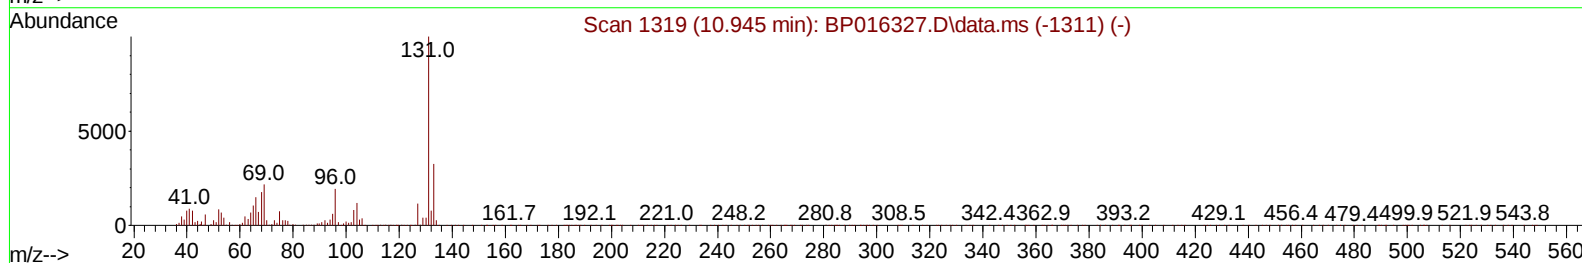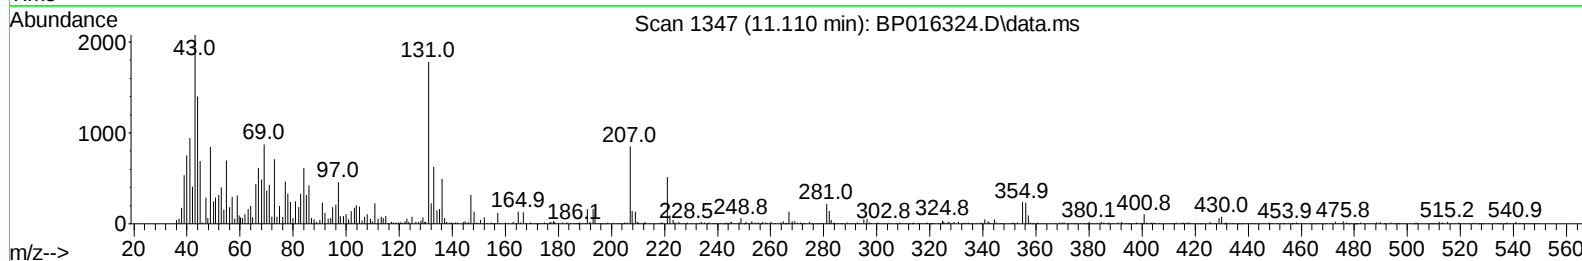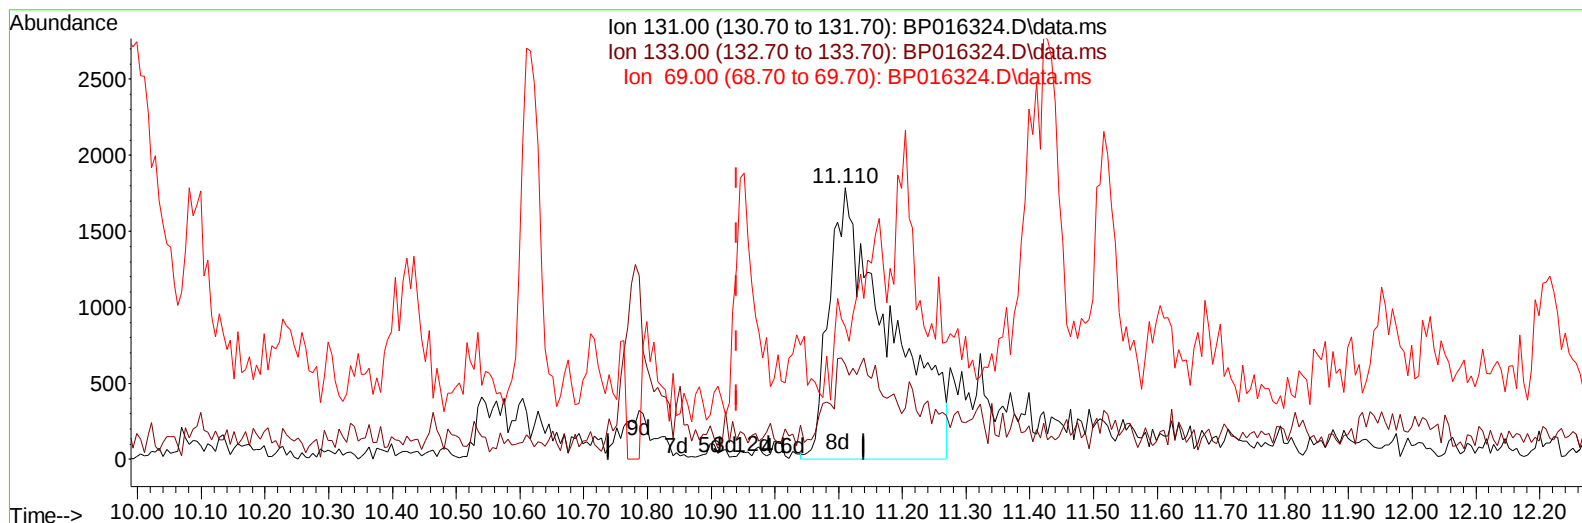

TIC: BP016324.D\data.ms

(31) 4-Chloroaniline-d4 (S)

11.110min (+ 0.171) 1.33 ng/ul m

response 11712

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	31.50	35.01
69.00	21.00	48.96#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071923\
Data File : BP016324.D
Acq On : 19 Jul 2023 14:47
Operator : MA/JU
Sample : 03501-09
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A46X4

Manual IntegrationsAPPROVED

Quant Time: Jul 19 23:35:12 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jul 19 14:47:57 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/20/2023
Supervised By :mohammad ahmed 07/20/2023

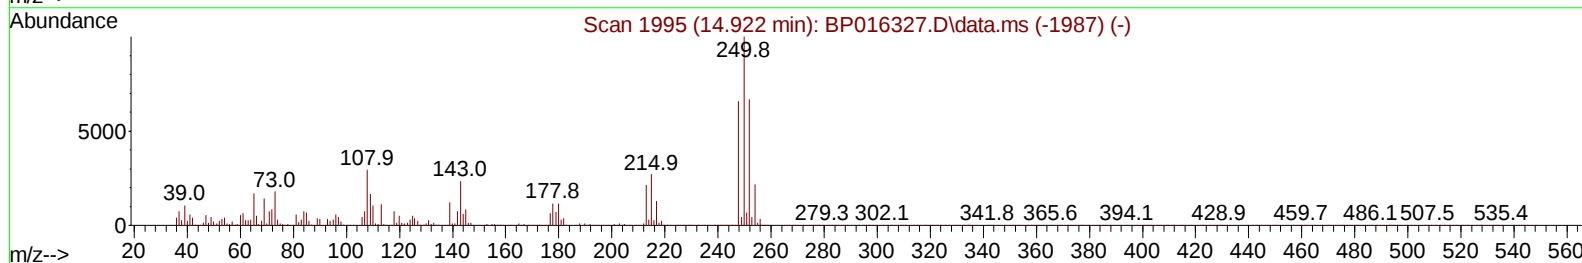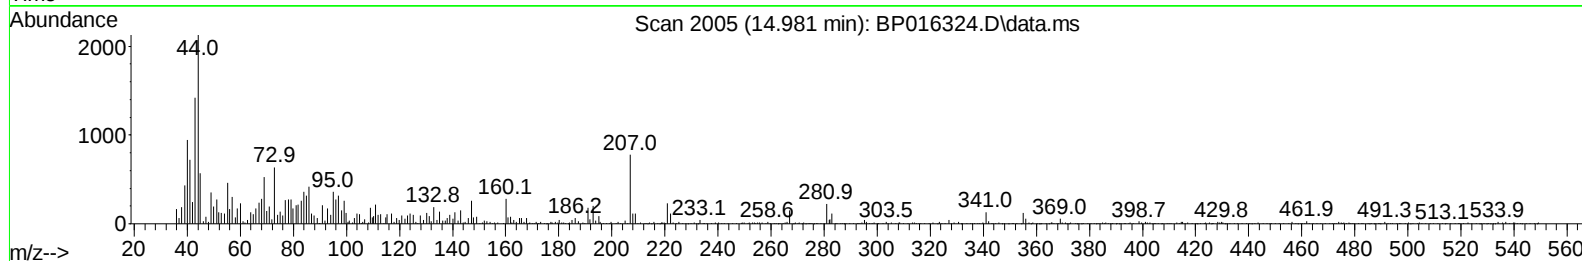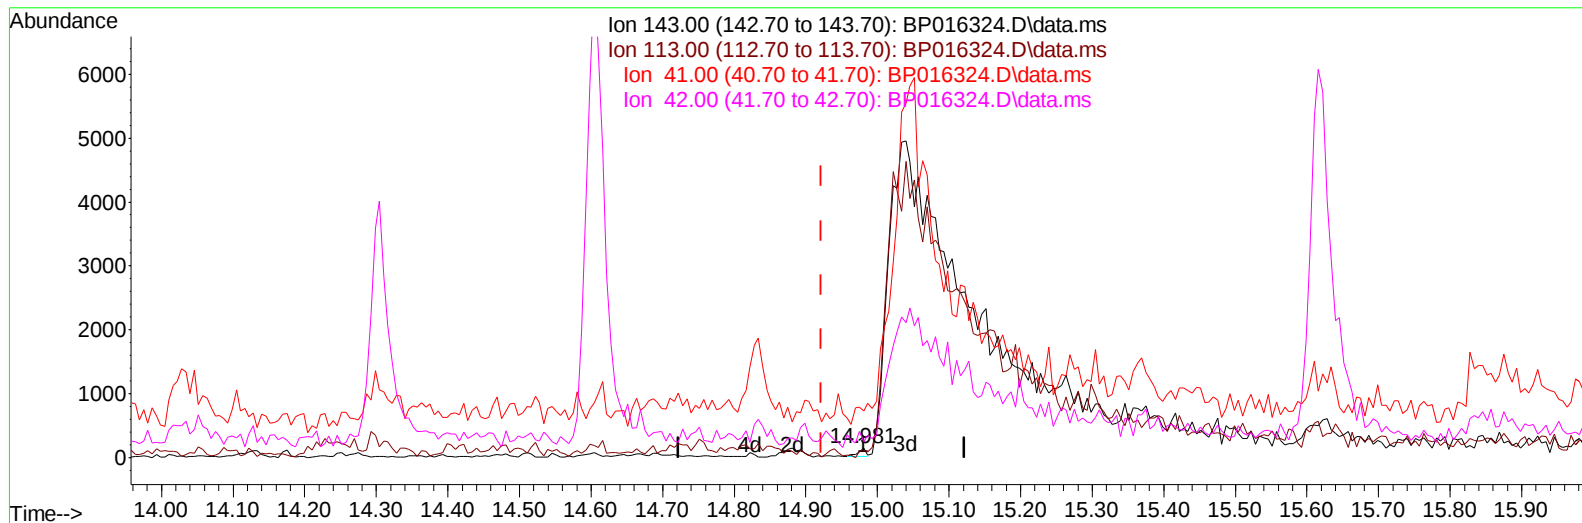

TIC: BP016324.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.981min (+ 0.059) 0.02 ng/u1

response 103

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	79.50	70.47
41.00	49.30	485.91#
42.00	32.70	162.42#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071923\
Data File : BP016324.D
Acq On : 19 Jul 2023 14:47
Operator : MA/JU
Sample : 03501-09
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A46X4

Manual IntegrationsAPPROVED

Quant Time: Jul 19 23:35:12 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jul 19 14:47:57 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/20/2023
Supervised By :mohammad ahmed 07/20/2023

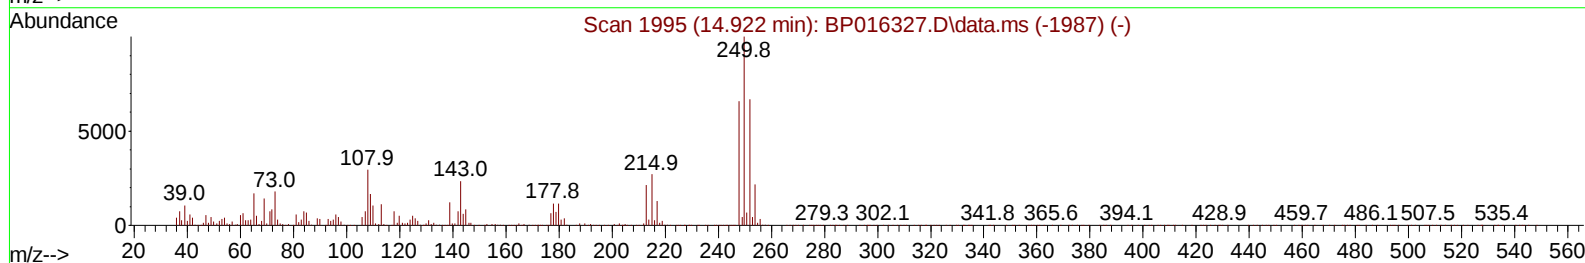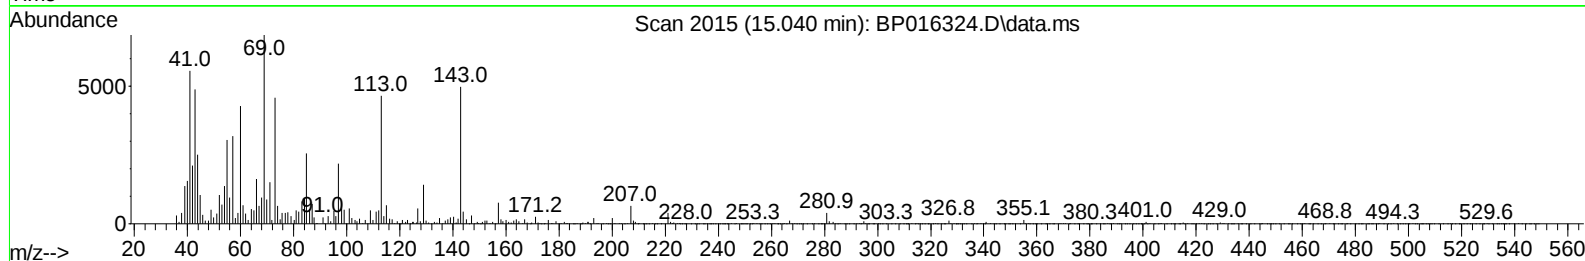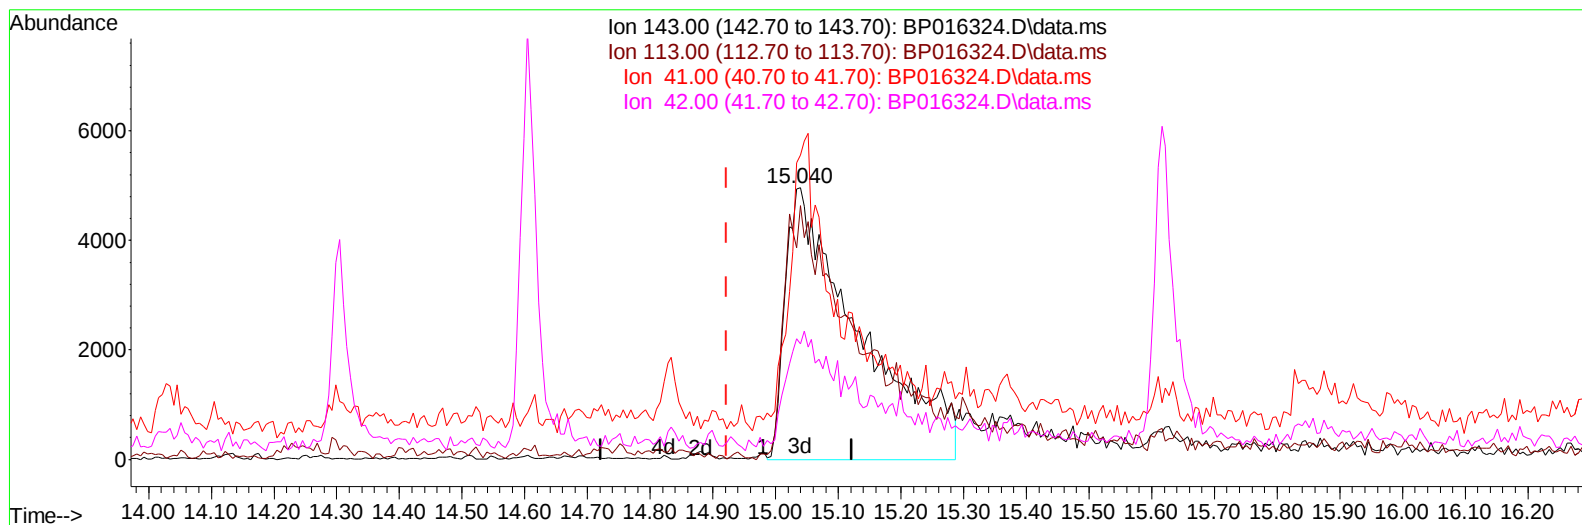

TIC: BP016324.D\data.ms

(54) 4-Nitrophenol-d4 (S)

15.040min (+ 0.118) 9.16 ng/ul m

response 40499

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	79.50	93.53
41.00	49.30	112.00#
42.00	32.70	42.64#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071923\
Data File : BP016324.D
Acq On : 19 Jul 2023 14:47
Operator : MA/JU
Sample : 03501-09
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A46X4

Manual IntegrationsAPPROVED

Quant Time: Jul 19 23:35:12 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jul 19 14:47:57 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/20/2023
Supervised By :mohammad ahmed 07/20/2023

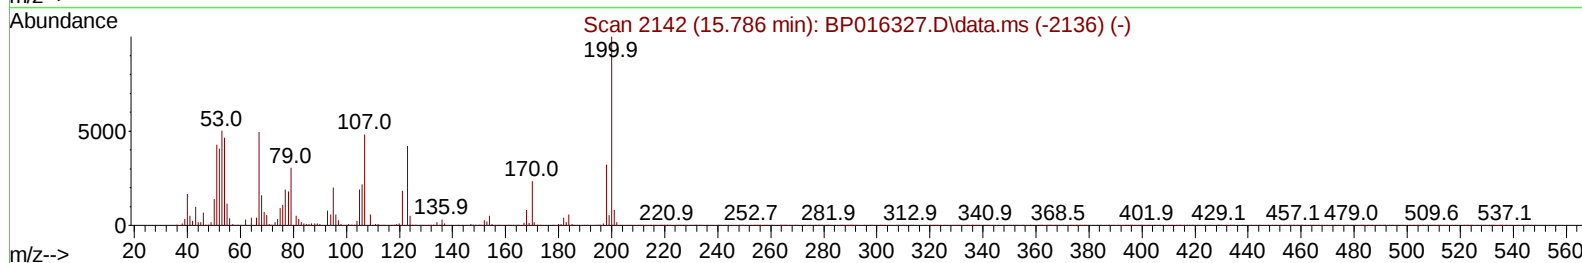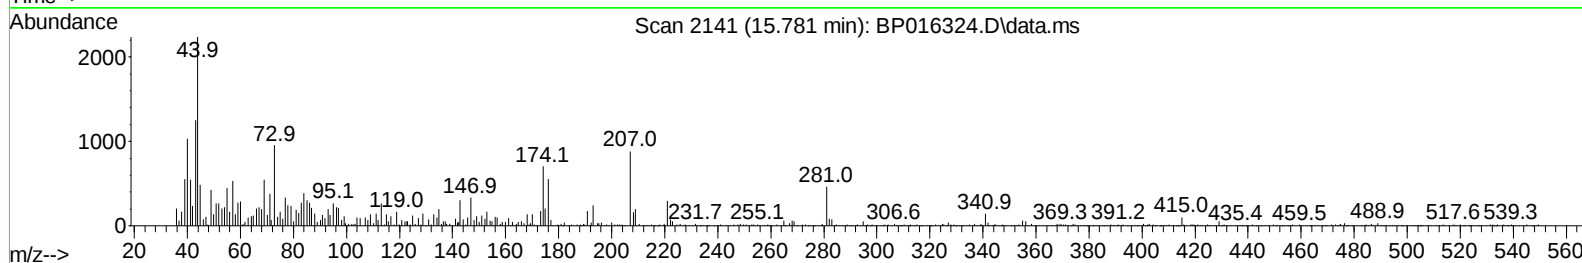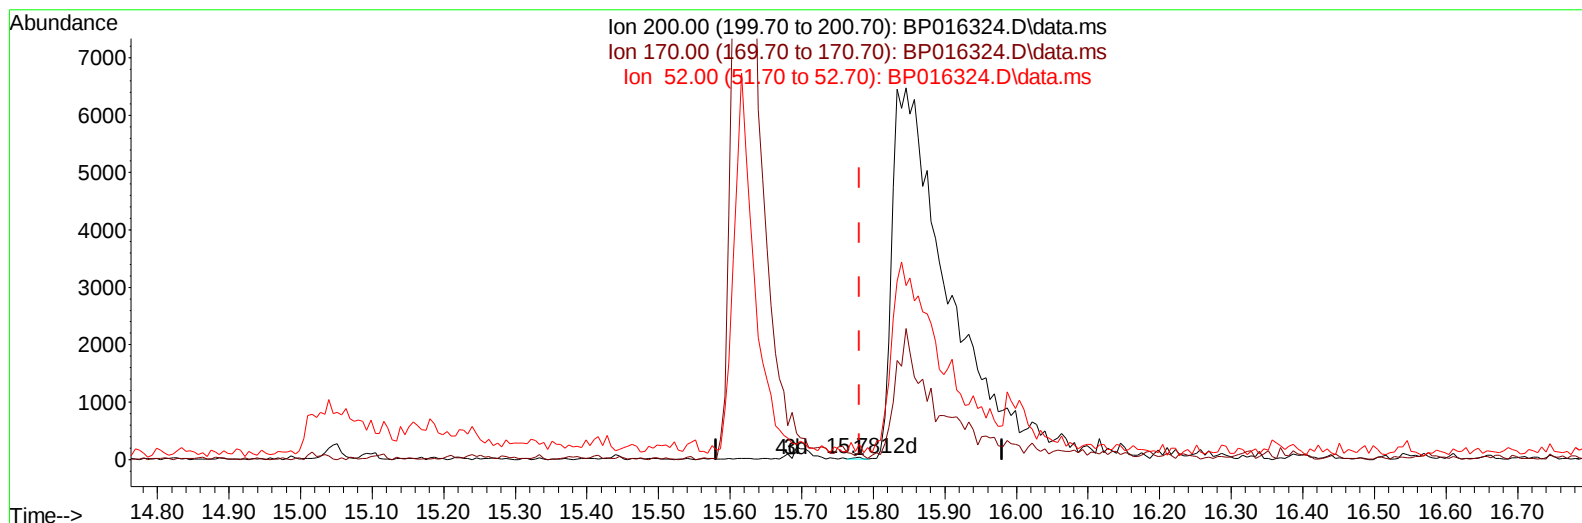

TIC: BP016324.D\data.ms

(65) 4,6-Dinitro-2-methylphenol-d2 (S)

15.781min (+ 0.000) 0.01 ng/ul

response 26

Ion	Exp%	Act%
200.00	100.00	100.00
170.00	21.90	362.16#
52.00	58.00	727.03#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071923\
Data File : BP016324.D
Acq On : 19 Jul 2023 14:47
Operator : MA/JU
Sample : 03501-09
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A46X4

Manual IntegrationsAPPROVED

Quant Time: Jul 19 23:35:12 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jul 19 14:47:57 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/20/2023
Supervised By :mohammad ahmed 07/20/2023

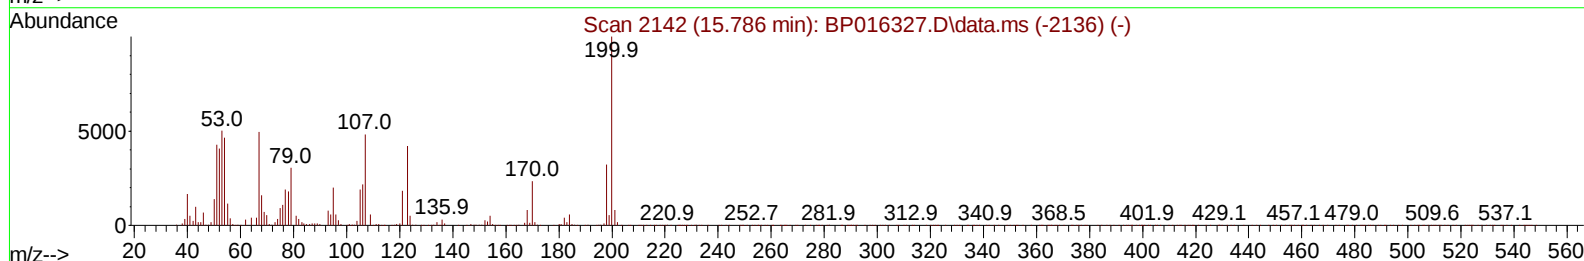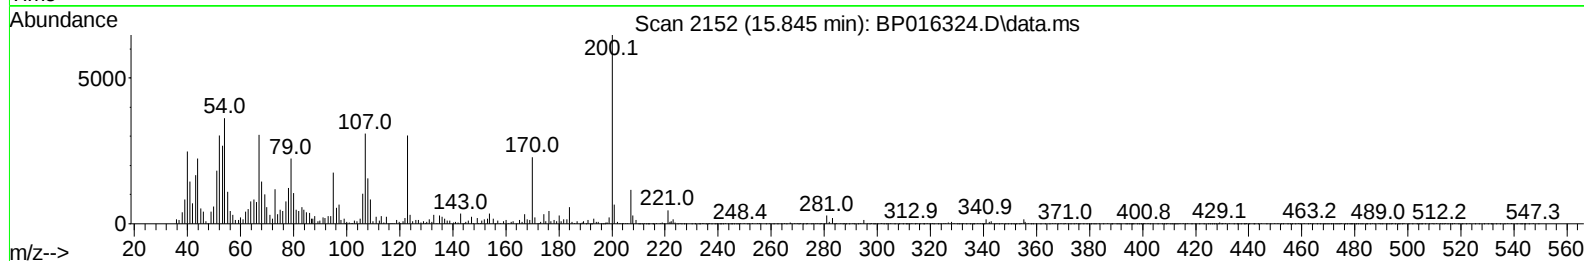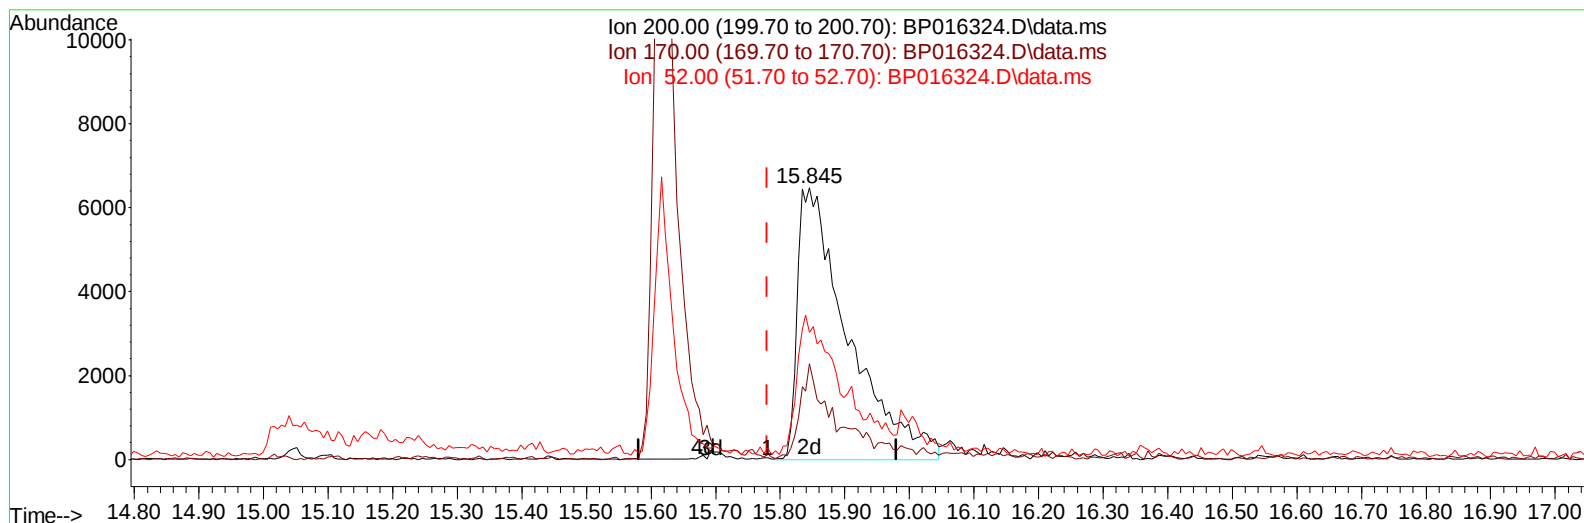

TIC: BP016324.D\data.ms

(65) 4,6-Dinitro-2-methylphenol-d2 (S)

15.845min (+ 0.065) 9.22 ng/ul m

response 35364

Ion	Exp%	Act%
200.00	100.00	100.00
170.00	21.90	35.29#
52.00	58.00	46.74
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071923\
 Data File : BP016324.D
 Acq On : 19 Jul 2023 14:47
 Operator : MA/JU
 Sample : 03501-09
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A46X4

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 07/20/2023
 Supervised By :mohammad ahmed 07/20/2023

Quant Time: Jul 19 23:46:58 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jul 19 14:47:57 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.952	152	88335	20.000	ng/ul	0.00
20) Naphthalene-d8	10.775	136	403304	20.000	ng/ul	0.02
38) Acenaphthene-d10	14.604	164	283852	20.000	ng/ul	0.01
64) Phenanthrene-d10	17.375	188	664327	20.000	ng/ul	0.01
79) Chrysene-d12	21.469	240	760272	20.000	ng/ul	0.00
88) Perylene-d12	23.957	264	790983	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.276	96	6657	2.667	ng/uL	0.00
4) Pyridine-d5	3.705	84	26227	4.213	ng/ul	-0.02
7) Phenol-d5	7.181	99	79538	9.969	ng/ul	0.05
9) Bis-(2-Chloroethyl)eth...	7.293	67	83167m	15.415	ng/ul	0.02
11) 2-Chlorophenol-d4	7.505	132	81883	14.216	ng/ul	0.03
15) 4-Methylphenol-d8	8.805	113	23440m	3.647	ng/ul	0.12
21) Nitrobenzene-d5	9.187	128	42722m	15.354	ng/ul	0.05
24) 2-Nitrophenol-d4	9.916	143	51607m	16.274	ng/ul	0.05
28) 2,4-Dichlorophenol-d3	10.563	165	62006m	11.291	ng/ul	0.14
31) 4-Chloroaniline-d4	11.110	131	11712m	1.331	ng/ul	0.17
46) Dimethylphthalate-d6	14.034	166	380968	17.595	ng/ul	0.02
49) Acenaphthylene-d8	14.304	160	349720	14.738	ng/ul	0.01
54) 4-Nitrophenol-d4	15.040	143	40499m	9.165	ng/ul	0.12
60) Fluorene-d10	15.616	176	331777	18.309	ng/ul	0.02
65) 4,6-Dinitro-2-methylph...	15.845	200	35364m	9.221	ng/ul	0.06
73) Anthracene-d10	17.487	188	363534	12.510	ng/ul	0.02
81) Pyrene-d10	19.710	212	335834	8.513	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.804	264	144354	3.800	ng/ul	0.02
Target Compounds						
						Qvalue
8) Phenol	7.211	94	17960m	2.100	ng/ul	
16) Acetophenone	8.863	105	35639	3.363	ng/ul	95
80) Fluoranthene	19.398	202	53380	1.157	ng/ul#	96
86) Bis(2-ethylhexyl)phtha...	21.322	149	37483	1.181	ng/ul#	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071923\
Data File : BP016324.D
Acq On : 19 Jul 2023 14:47
Operator : MA/JU
Sample : 03501-09
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A46X4

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 07/20/2023
Supervised By :mohammad ahmed 07/20/2023

Quant Time: Jul 19 23:46:58 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jul 19 14:47:57 2023
Response via : Initial Calibration

