




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071923\
 Data File : BP016335.D
 Acq On : 19 Jul 2023 21:36
 Operator : MA/JU
 Sample : 03472-21
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A46R2

Manual IntegrationsAPPROVED

Quant Time: Jul 19 22:44:06 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jul 19 14:47:57 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/20/2023
 Supervised By :mohammad ahmed 07/20/2023

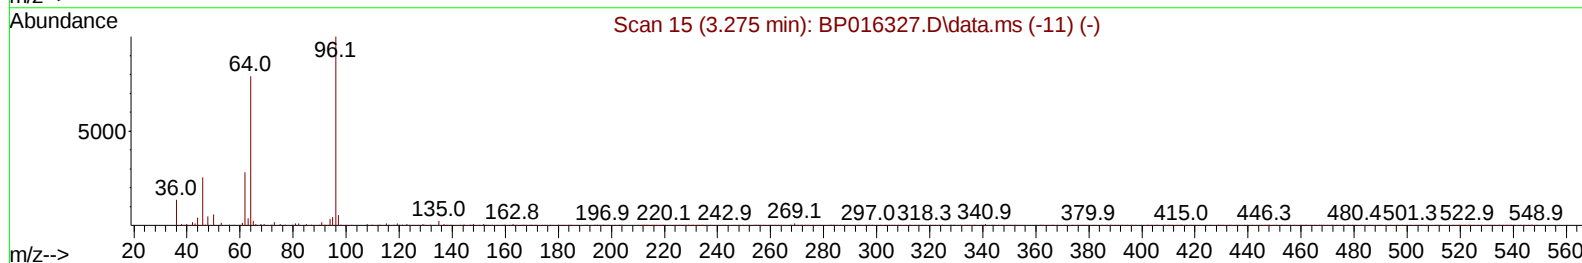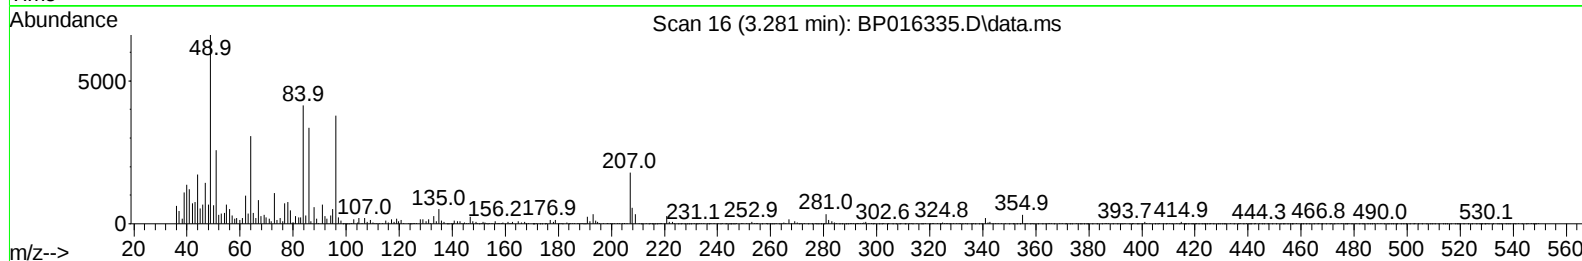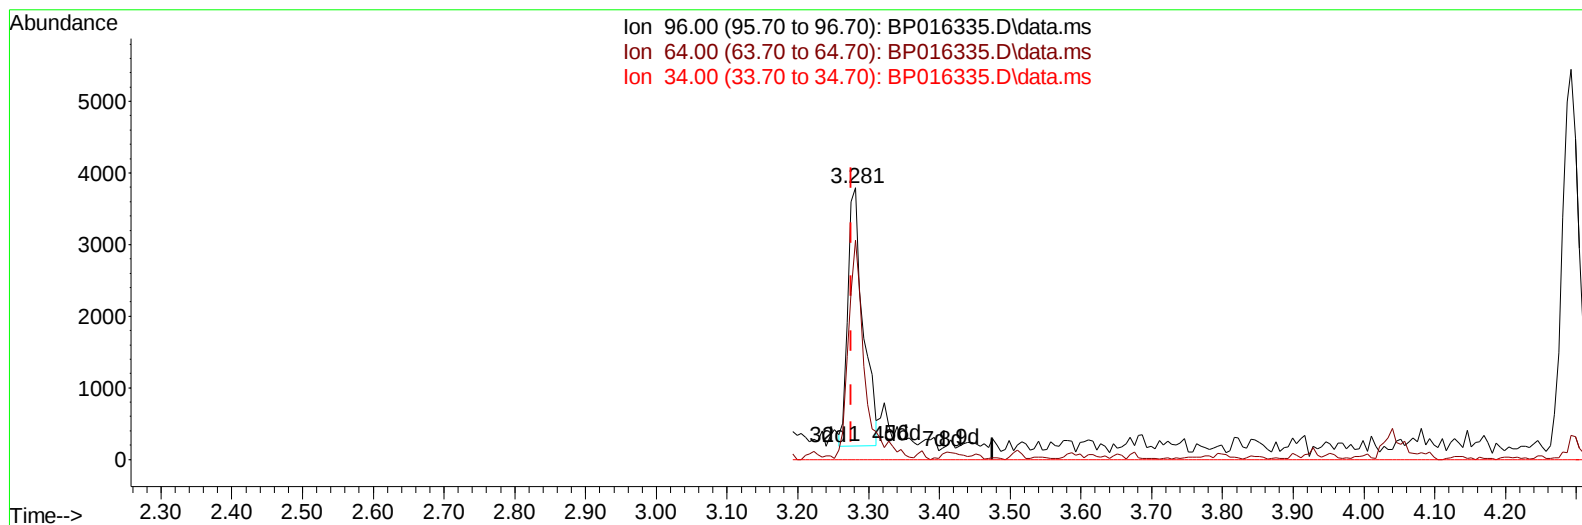

TIC: BP016335.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.281min (+ 0.006) 1.70 ng/uL

response 5395

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	75.90	80.80
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071923\
 Data File : BP016335.D
 Acq On : 19 Jul 2023 21:36
 Operator : MA/JU
 Sample : 03472-21
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A46R2

Manual IntegrationsAPPROVED

Quant Time: Jul 19 22:44:06 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jul 19 14:47:57 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/20/2023
 Supervised By :mohammad ahmed 07/20/2023

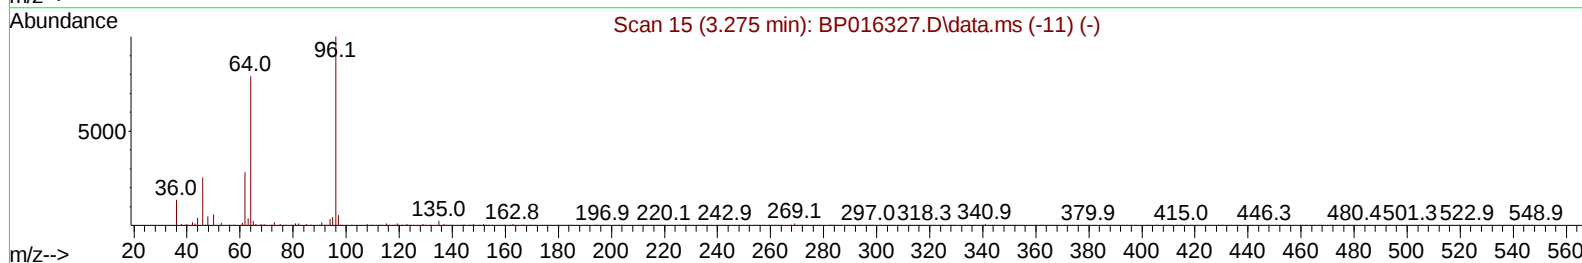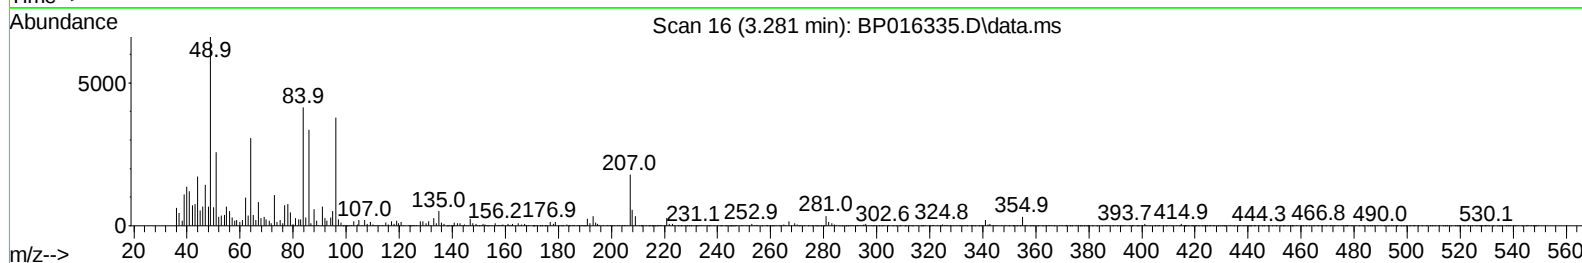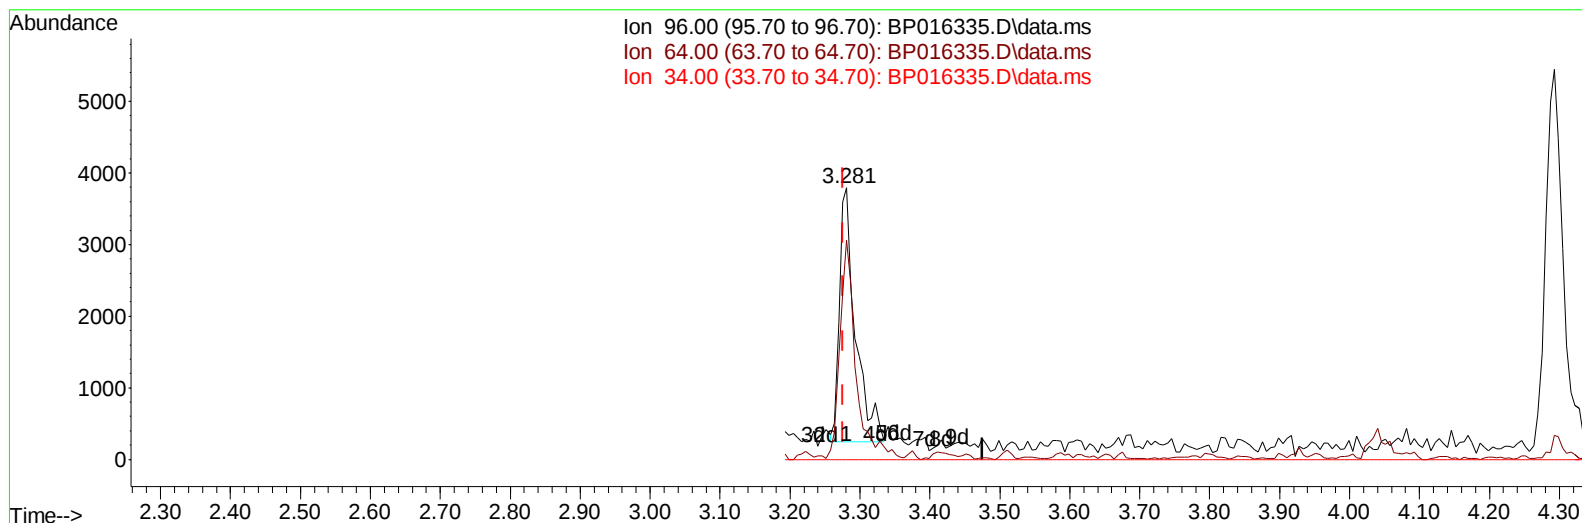

TIC: BP016335.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.281min (+ 0.006) 1.78 ng/uL m

response 5640

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	75.90	80.80
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071923\
 Data File : BP016335.D
 Acq On : 19 Jul 2023 21:36
 Operator : MA/JU
 Sample : 03472-21
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A46R2

Manual IntegrationsAPPROVED

Quant Time: Jul 19 22:44:06 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jul 19 14:47:57 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/20/2023
 Supervised By :mohammad ahmed 07/20/2023

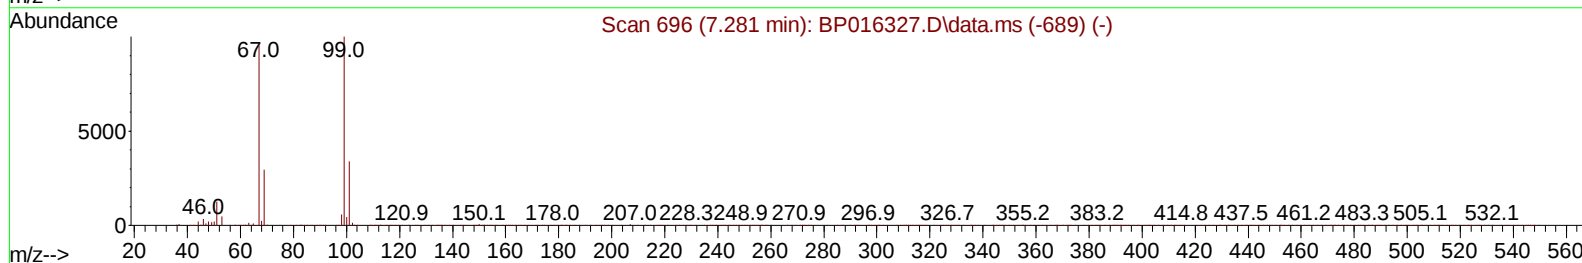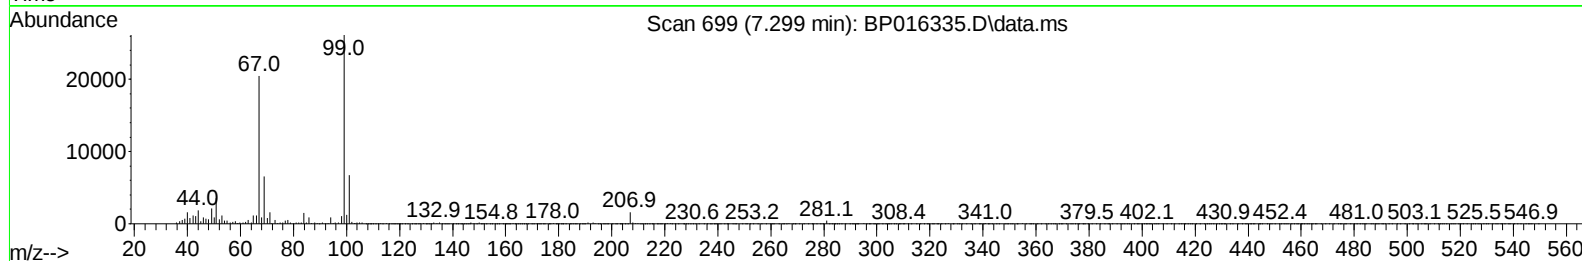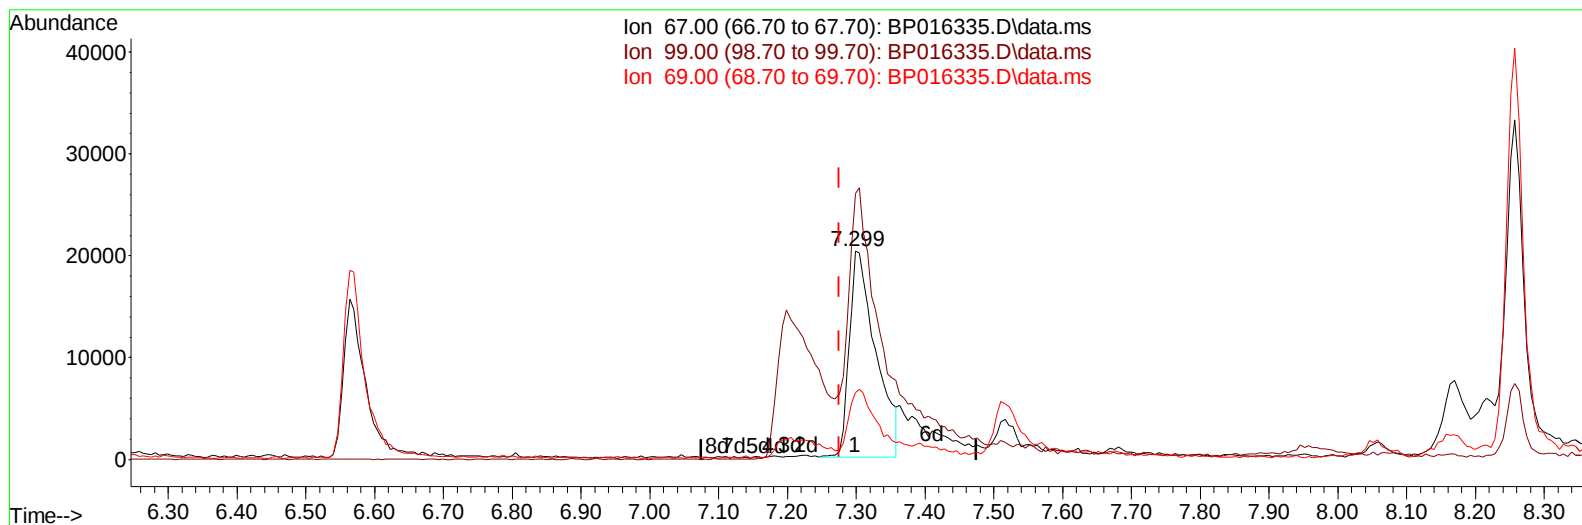

TIC: BP016335.D\data.ms

(9) Bis-(2-Chloroethyl)ether-d8 (S)

7.299min (+ 0.023) 7.92 ng/u1

response 54291

Ion	Exp%	Act%
67.00	100.00	100.00
99.00	117.30	127.66
69.00	33.10	32.07
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071923\
 Data File : BP016335.D
 Acq On : 19 Jul 2023 21:36
 Operator : MA/JU
 Sample : 03472-21
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A46R2

Manual IntegrationsAPPROVED

Quant Time: Jul 19 22:44:06 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jul 19 14:47:57 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/20/2023
 Supervised By :mohammad ahmed 07/20/2023

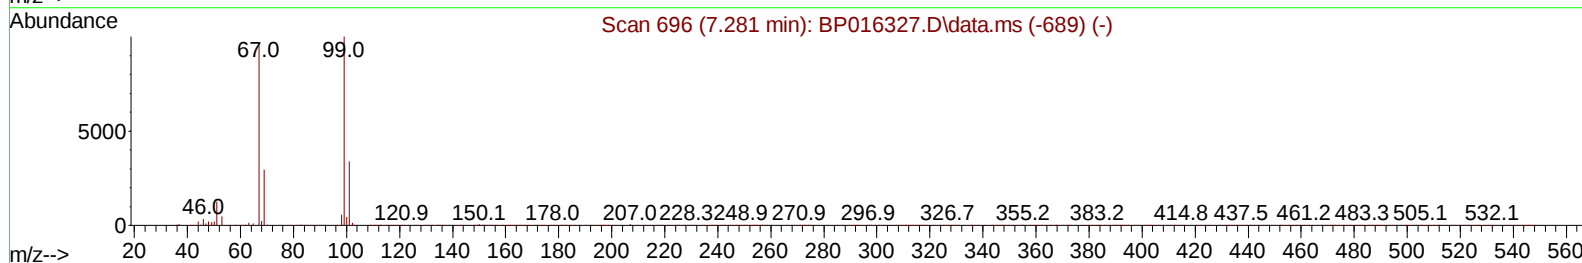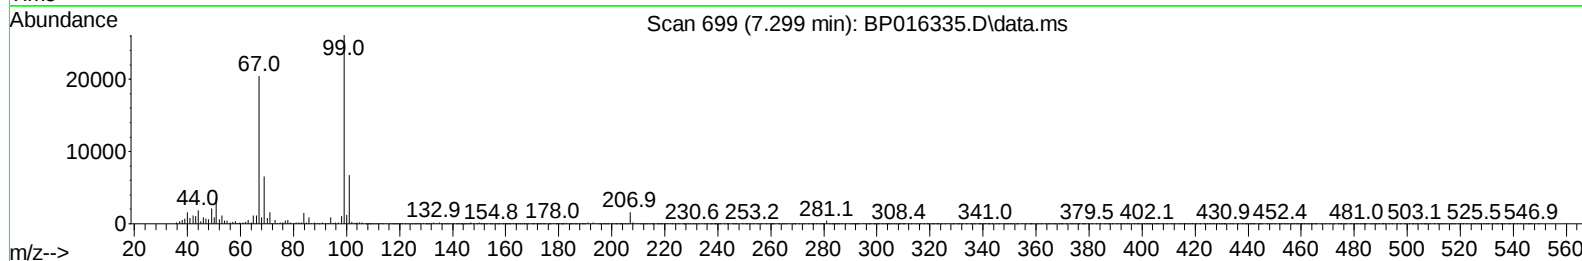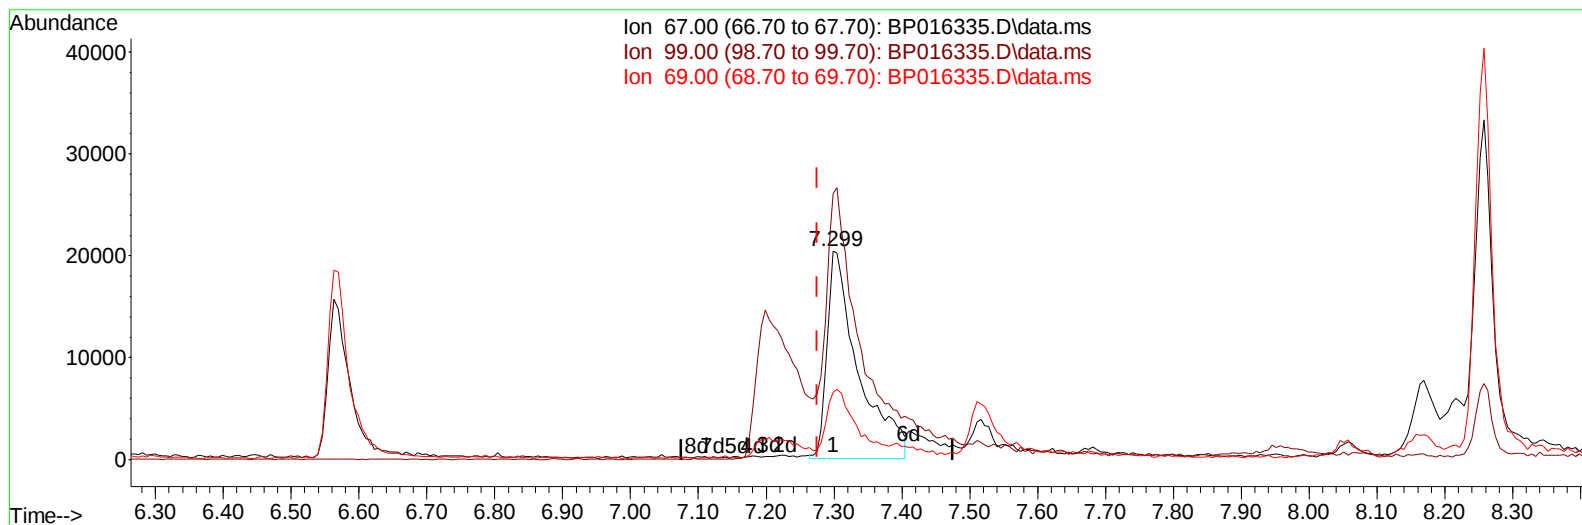

TIC: BP016335.D\data.ms

(9) Bis-(2-Chloroethyl)ether-d8 (S)

7.299min (+ 0.023) 9.51 ng/ul m

response 65145

Ion	Exp%	Act%
67.00	100.00	100.00
99.00	117.30	127.66
69.00	33.10	32.07
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071923\
Data File : BP016335.D
Acq On : 19 Jul 2023 21:36
Operator : MA/JU
Sample : 03472-21
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A46R2

Manual IntegrationsAPPROVED

Quant Time: Jul 19 23:28:43 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jul 19 14:47:57 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/20/2023
Supervised By :mohammad ahmed 07/20/2023

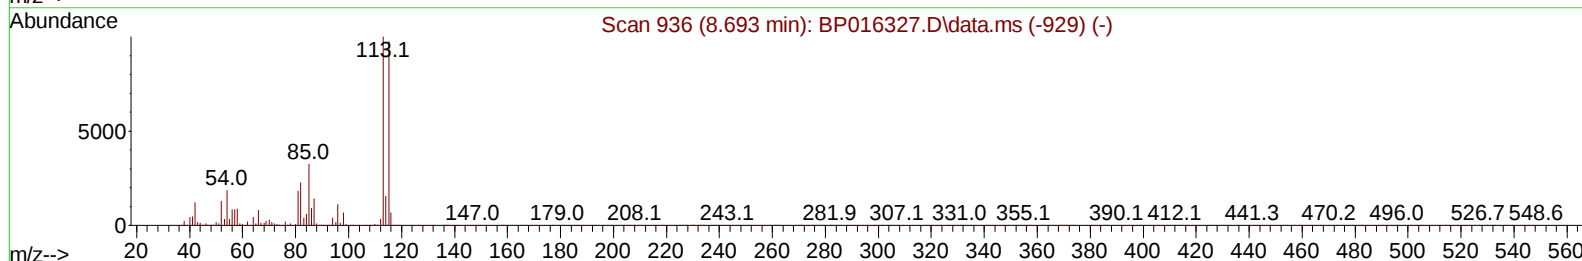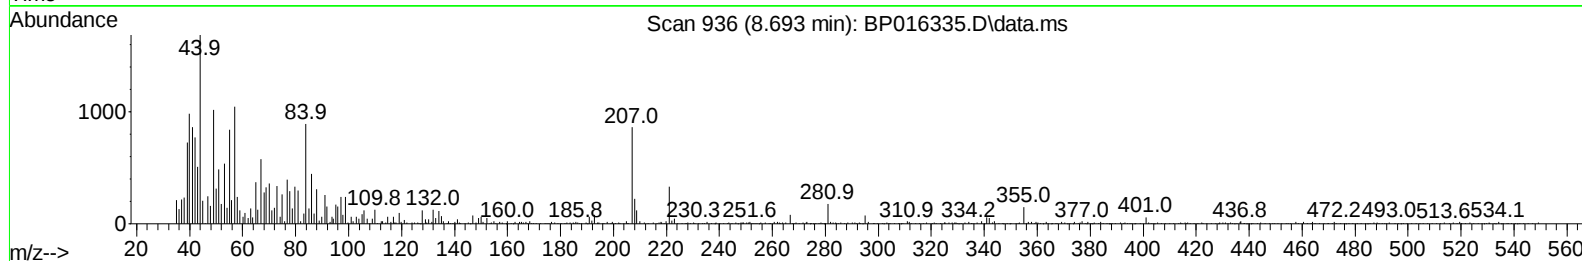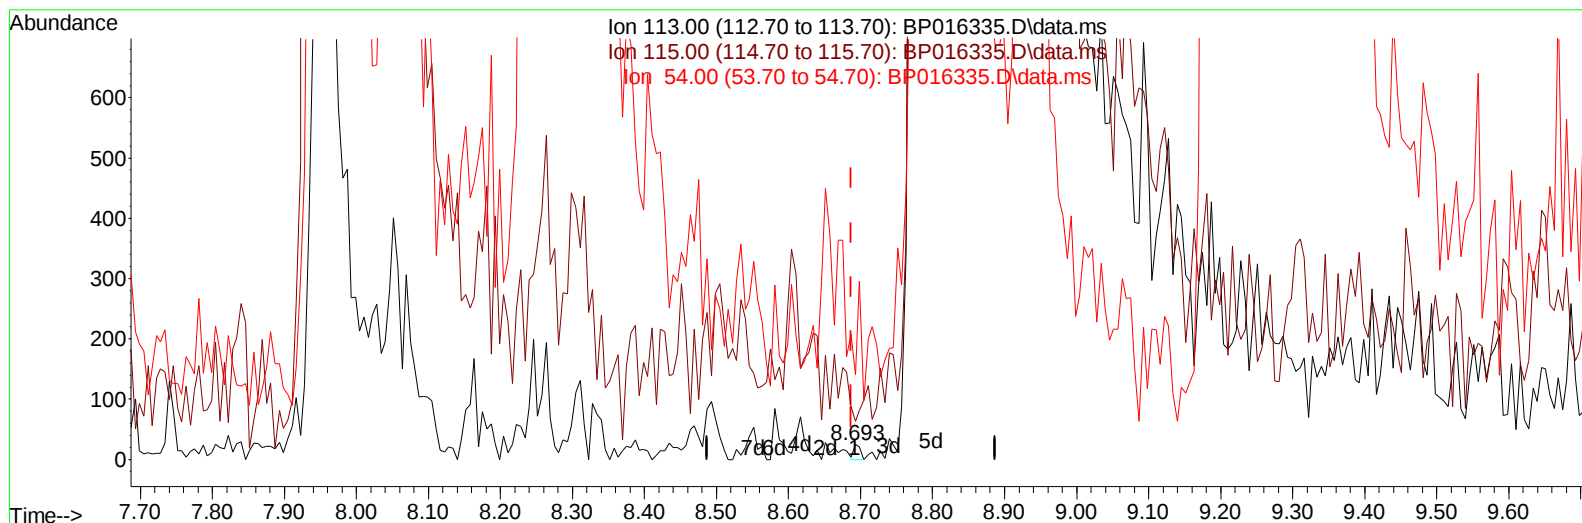

TIC: BP016335.D\data.ms

(15) 4-Methylphenol-d8 (S)

8.693min (+ 0.006) 0.00 ng/u1

response 16

Ion	Exp%	Act%
113.00	100.00	100.00
115.00	90.20	252.00#
54.00	16.30	564.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071923\
 Data File : BP016335.D
 Acq On : 19 Jul 2023 21:36
 Operator : MA/JU
 Sample : 03472-21
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A46R2

Manual IntegrationsAPPROVED

Quant Time: Jul 19 23:28:43 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jul 19 14:47:57 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/20/2023
 Supervised By :mohammad ahmed 07/20/2023

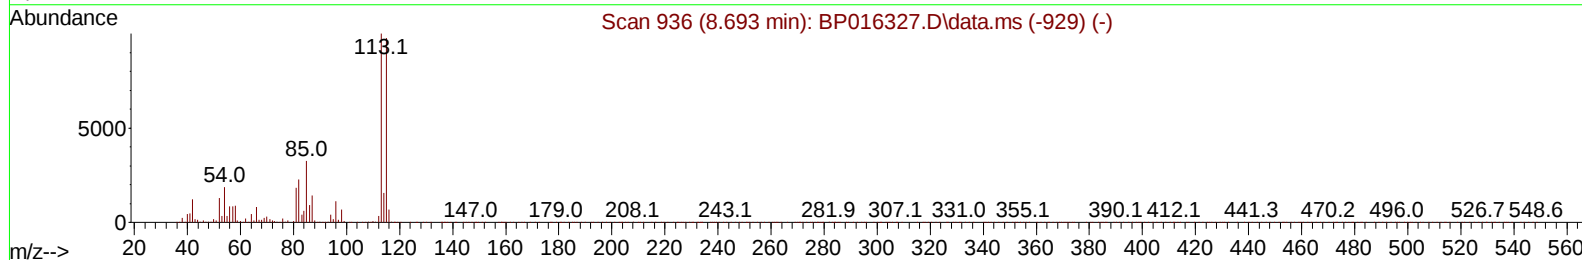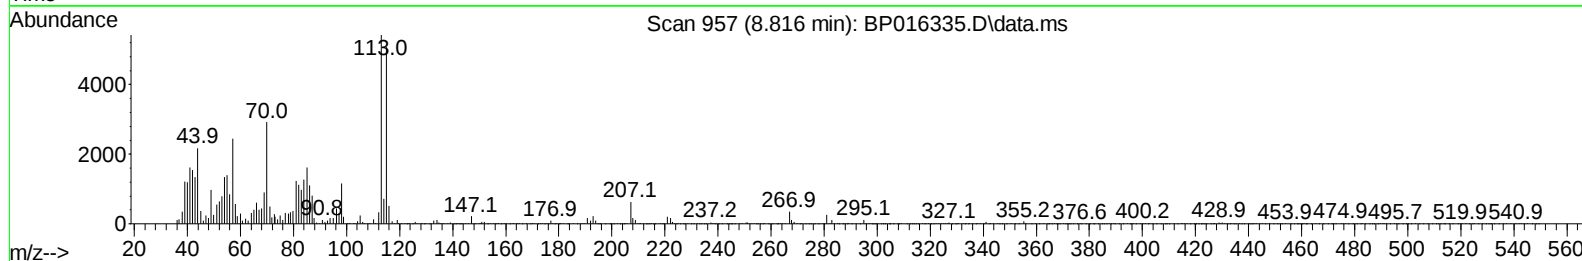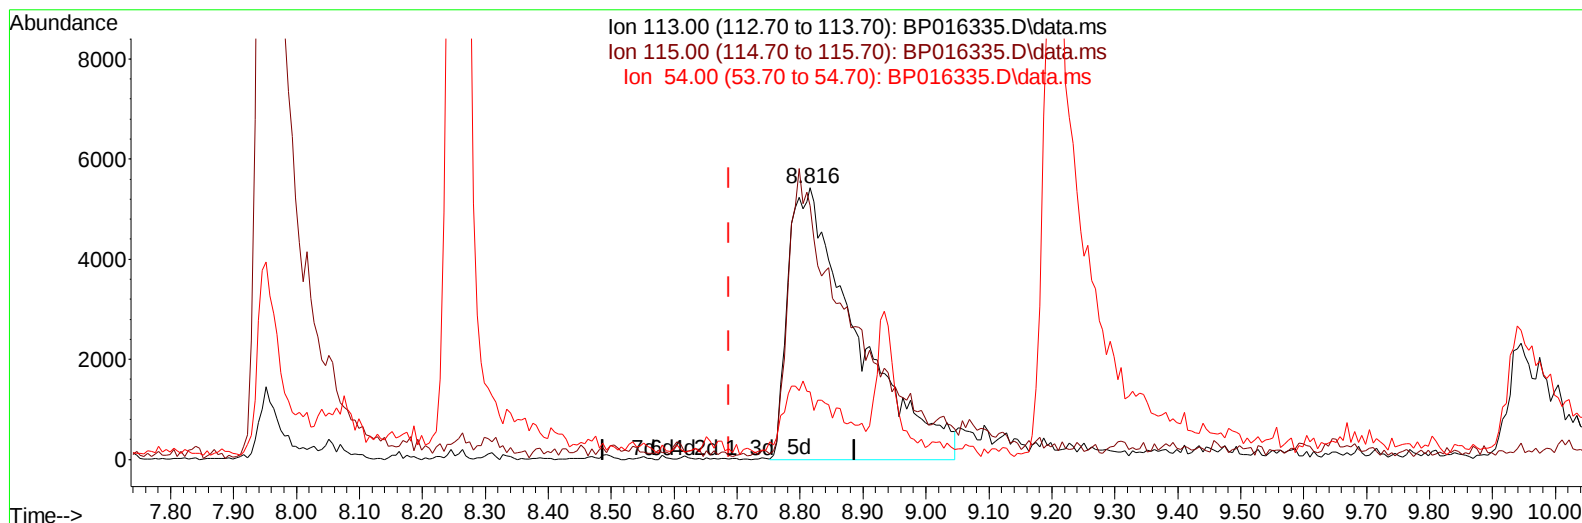

TIC: BP016335.D\data.ms

(15) 4-Methylphenol-d8 (S)

8.816min (+ 0.129) 5.04 ng/u1 m

response 41164

Ion	Exp%	Act%
113.00	100.00	100.00
115.00	90.20	93.49
54.00	16.30	24.91#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071923\
Data File : BP016335.D
Acq On : 19 Jul 2023 21:36
Operator : MA/JU
Sample : 03472-21
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A46R2

Manual IntegrationsAPPROVED

Quant Time: Jul 19 23:28:43 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jul 19 14:47:57 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/20/2023
Supervised By :mohammad ahmed 07/20/2023

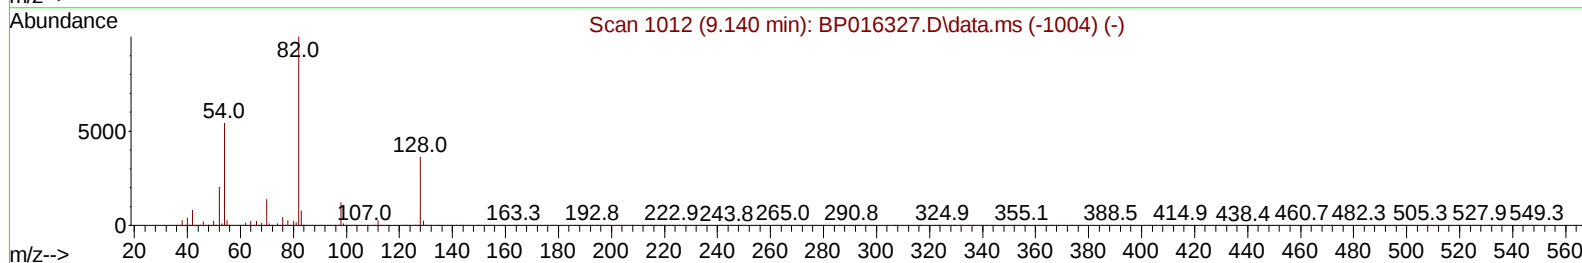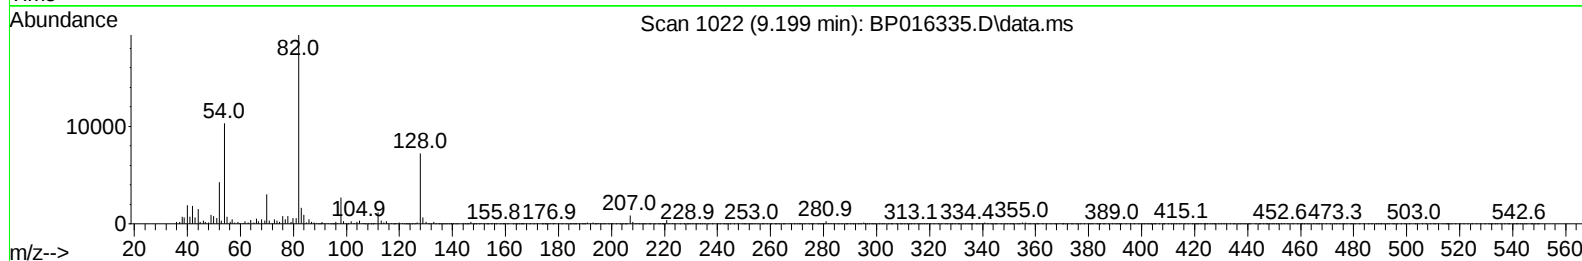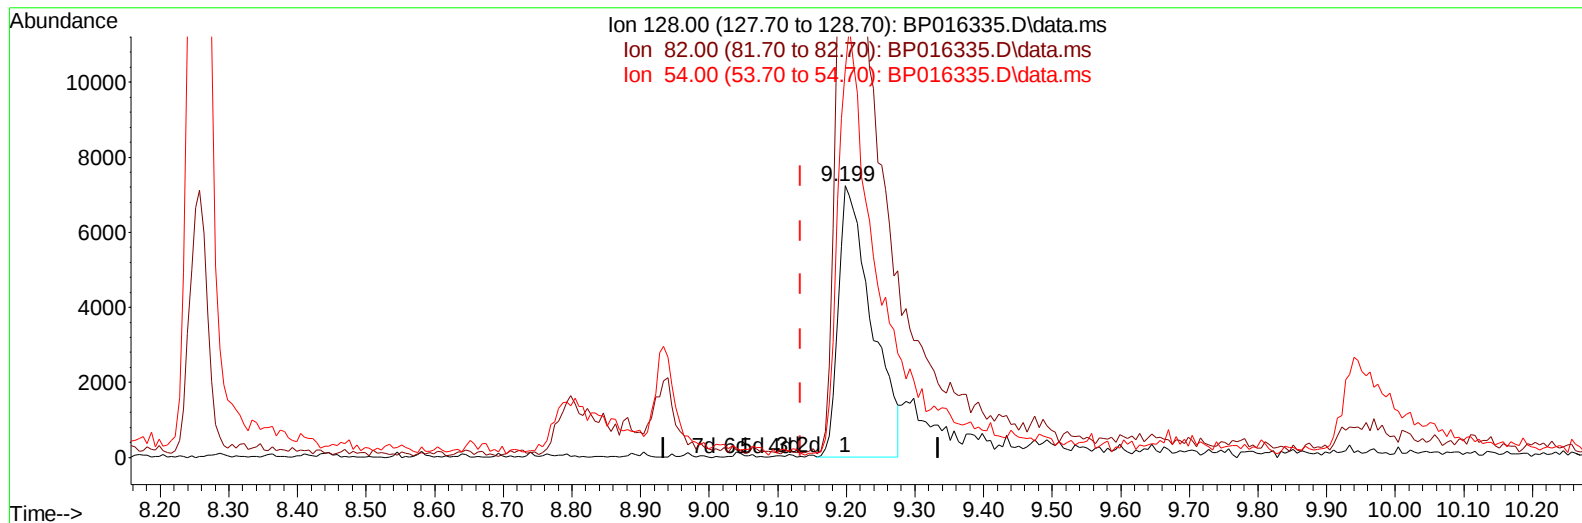

TIC: BP016335.D\data.ms

(21) Nitrobenzene-d5 (S)

9.199min (+ 0.065) 6.88 ng/u1

response 24302

Ion	Exp%	Act%
128.00	100.00	100.00
82.00	261.40	267.44
54.00	136.80	142.73
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071923\
 Data File : BP016335.D
 Acq On : 19 Jul 2023 21:36
 Operator : MA/JU
 Sample : 03472-21
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A46R2

Manual IntegrationsAPPROVED

Quant Time: Jul 19 23:28:43 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jul 19 14:47:57 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/20/2023
 Supervised By :mohammad ahmed 07/20/2023

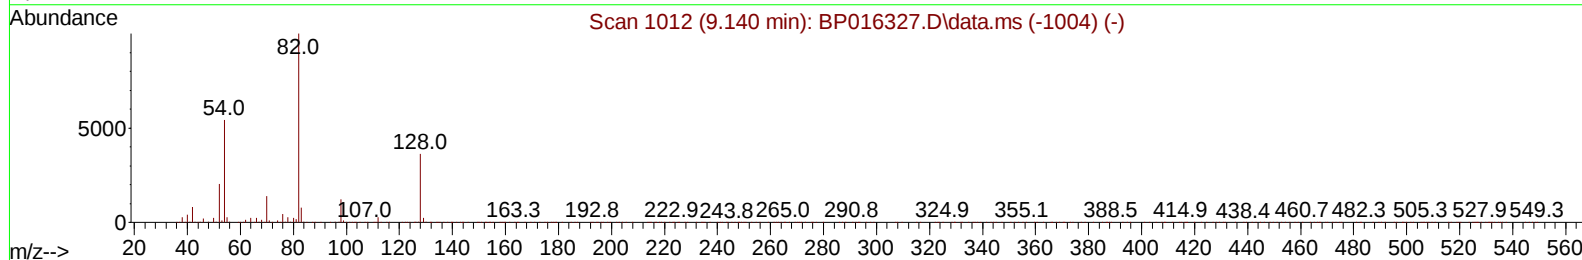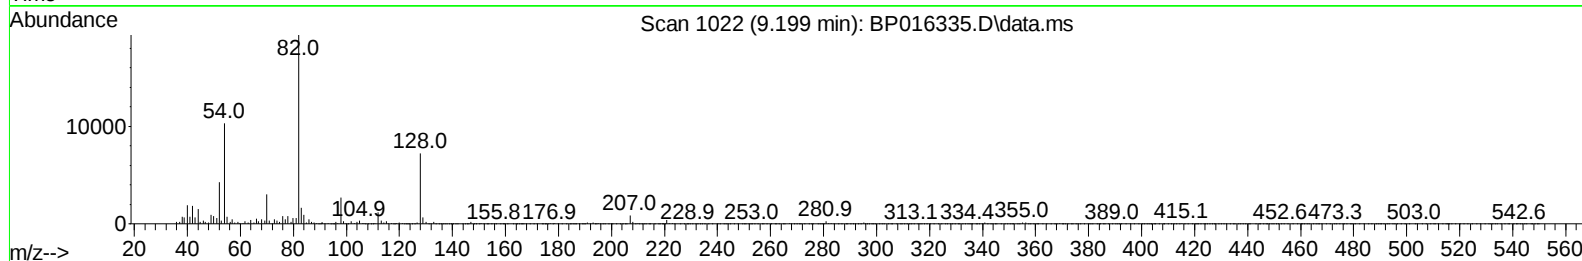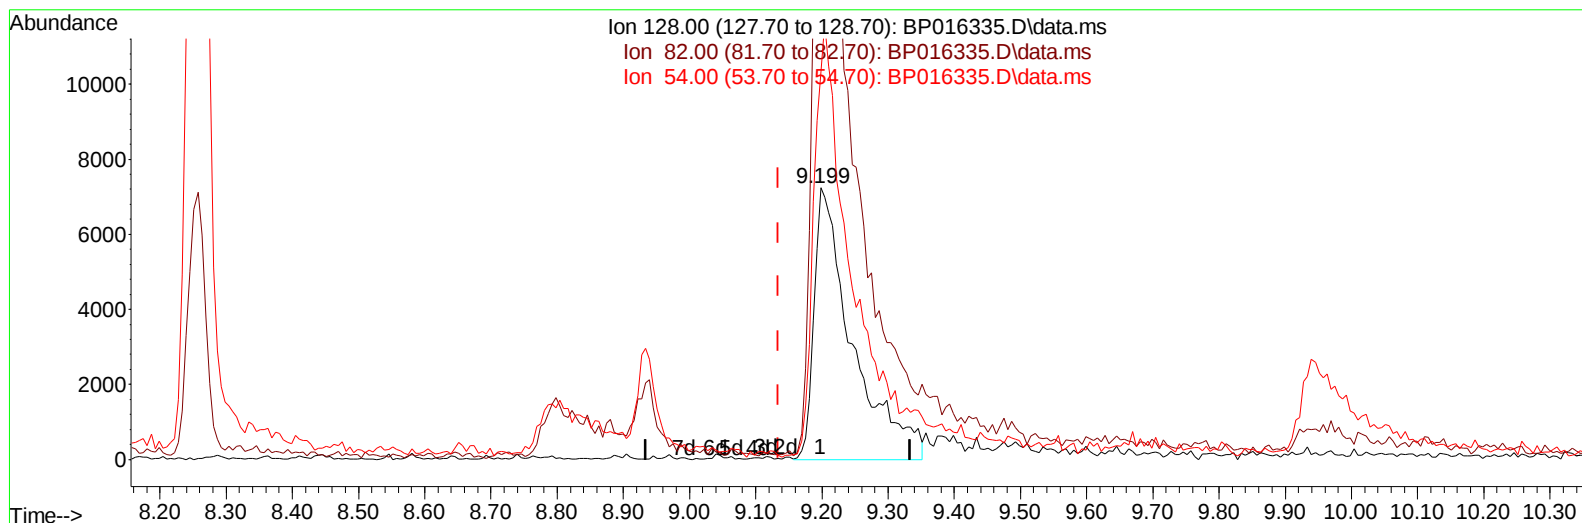

TIC: BP016335.D\data.ms

(21) Nitrobenzene-d5 (S)

9.199min (+ 0.065) 8.25 ng/ul m

response 29119

Ion	Exp%	Act%
128.00	100.00	100.00
82.00	261.40	267.44
54.00	136.80	142.73
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071923\
 Data File : BP016335.D
 Acq On : 19 Jul 2023 21:36
 Operator : MA/JU
 Sample : 03472-21
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A46R2

Manual IntegrationsAPPROVED

Quant Time: Jul 19 23:28:43 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jul 19 14:47:57 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/20/2023
 Supervised By :mohammad ahmed 07/20/2023

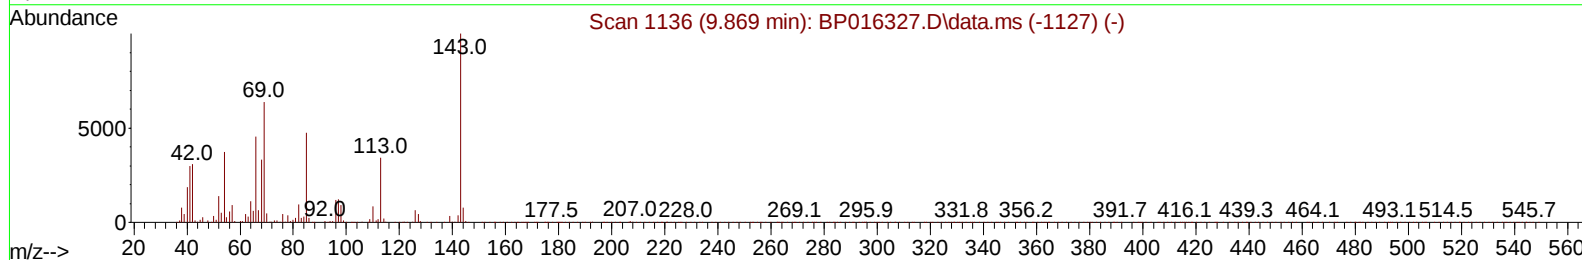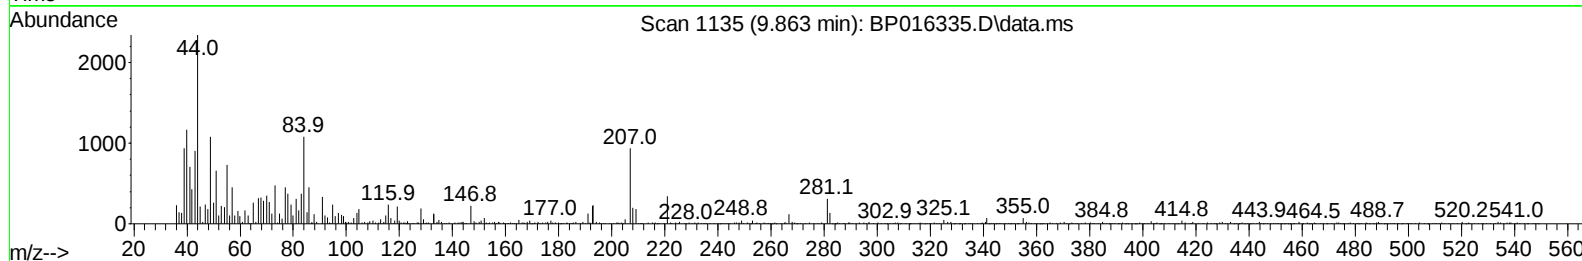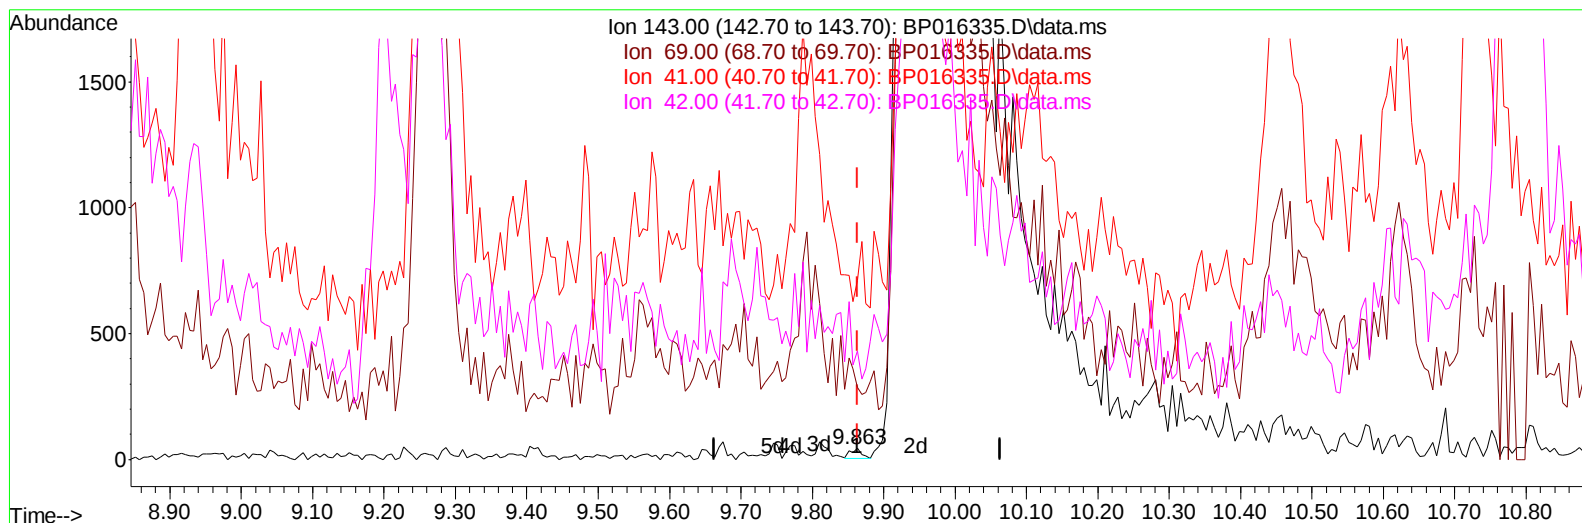

TIC: BP016335.D\data.ms

(24) 2-Nitrophenol-d4 (S)

9.863min (-0.000) 0.01 ng/u1

response 42

Ion	Exp%	Act%
143.00	100.00	100.00
69.00	62.00	650.00#
41.00	28.60	1613.64#
42.00	29.20	979.55#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071923\
Data File : BP016335.D
Acq On : 19 Jul 2023 21:36
Operator : MA/JU
Sample : 03472-21
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A46R2

Manual IntegrationsAPPROVED

Quant Time: Jul 19 23:28:43 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jul 19 14:47:57 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/20/2023
Supervised By :mohammad ahmed 07/20/2023

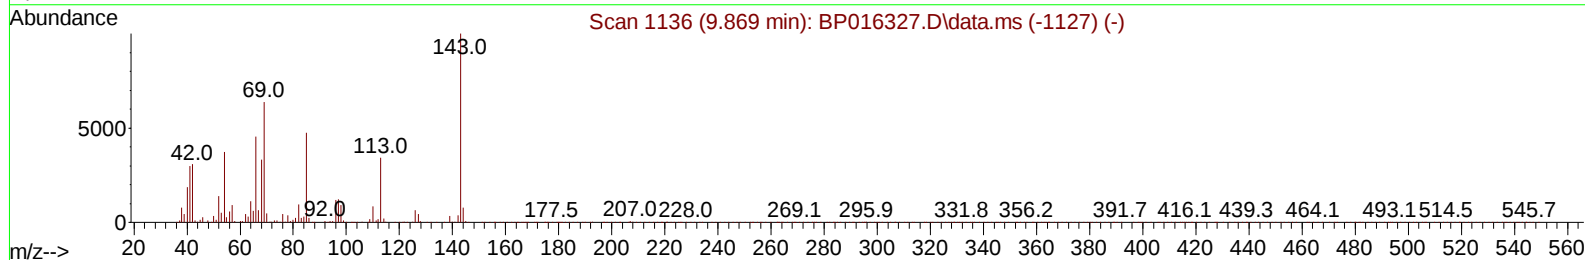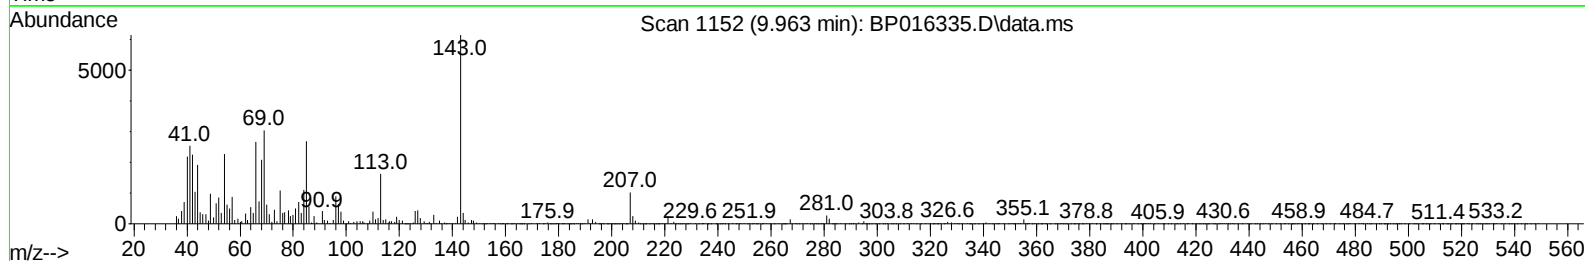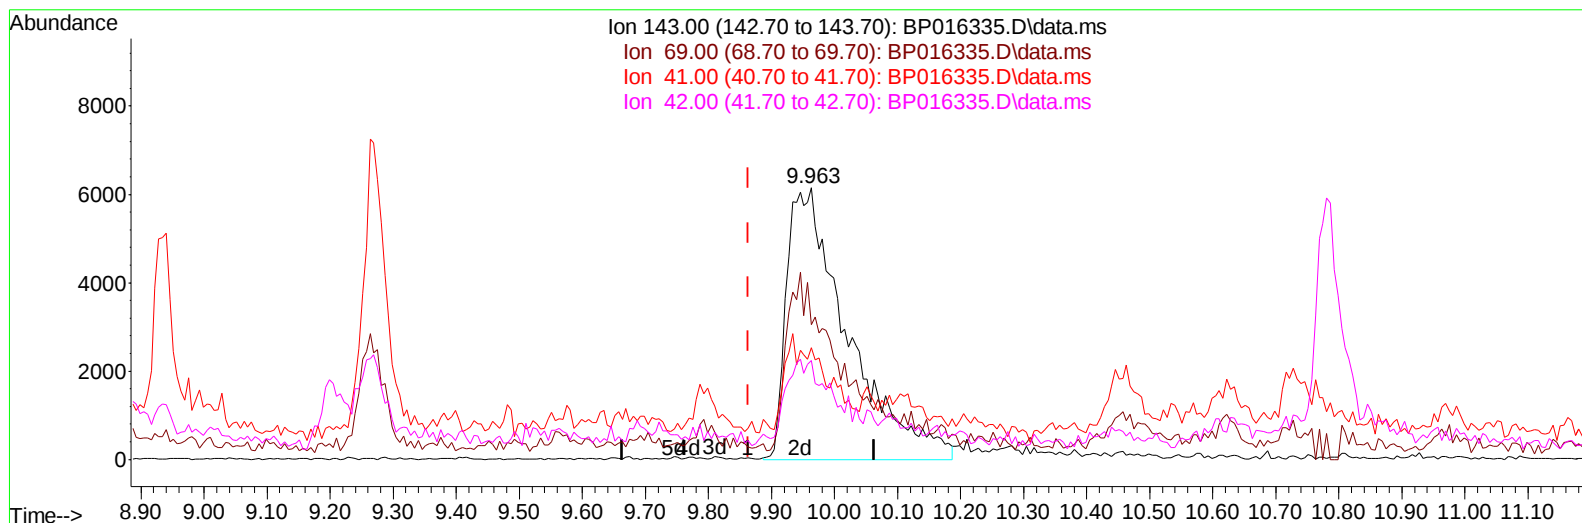

TIC: BP016335.D\data.ms

(24) 2-Nitrophenol-d4 (S)

9.963min (+ 0.100) 10.22 ng/ul m

response 41142

Ion	Exp%	Act%
143.00	100.00	100.00
69.00	62.00	49.59#
41.00	28.60	41.24#
42.00	29.20	36.46#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071923\
 Data File : BP016335.D
 Acq On : 19 Jul 2023 21:36
 Operator : MA/JU
 Sample : 03472-21
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A46R2

Manual IntegrationsAPPROVED

Quant Time: Jul 19 23:28:43 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jul 19 14:47:57 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/20/2023
 Supervised By :mohammad ahmed 07/20/2023

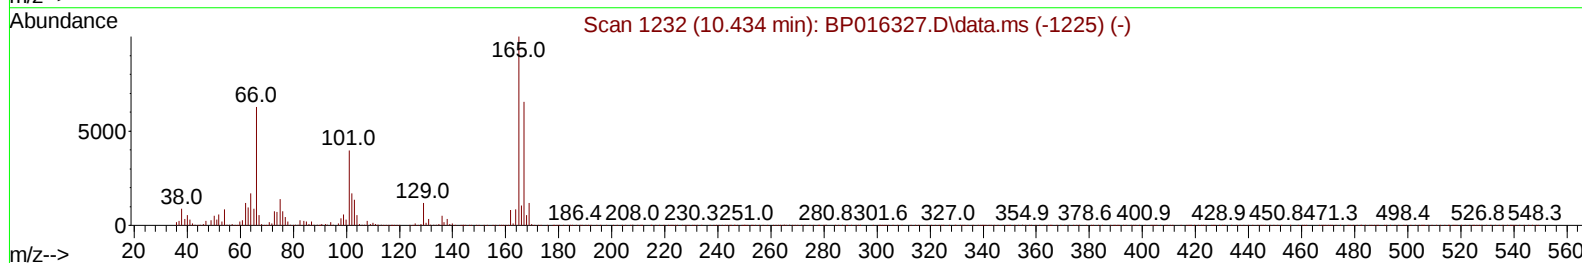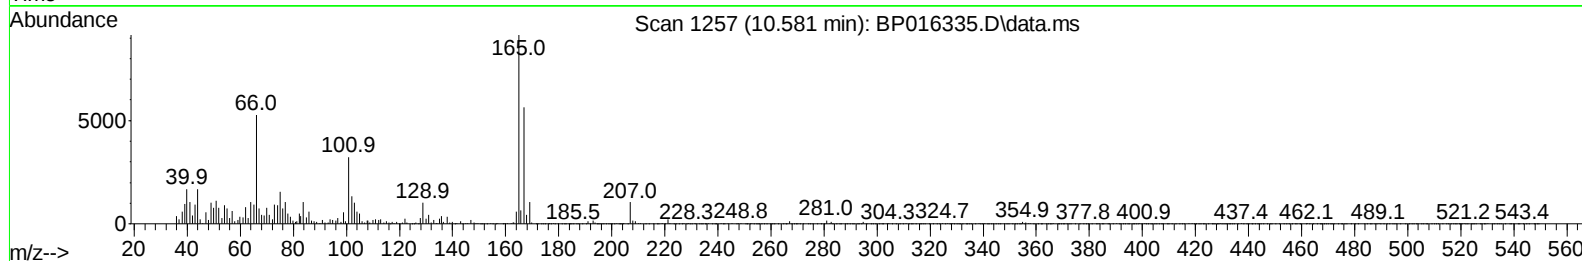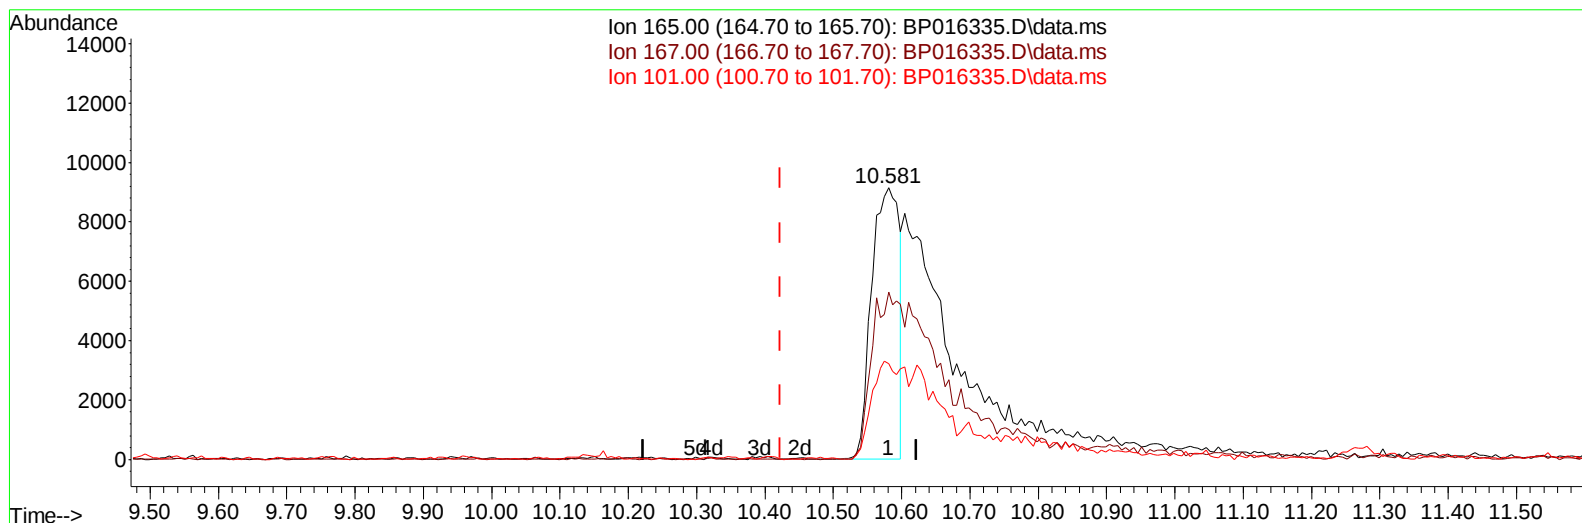

TIC: BP016335.D\data.ms

(28) 2,4-Dichlorophenol-d3 (S)

10.581min (+ 0.159) 3.72 ng/u1

response 25907

Ion	Exp%	Act%
165.00	100.00	100.00
167.00	65.20	61.71
101.00	38.50	35.38
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071923\
 Data File : BP016335.D
 Acq On : 19 Jul 2023 21:36
 Operator : MA/JU
 Sample : 03472-21
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A46R2

Manual IntegrationsAPPROVED

Quant Time: Jul 19 23:28:43 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jul 19 14:47:57 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/20/2023
 Supervised By :mohammad ahmed 07/20/2023

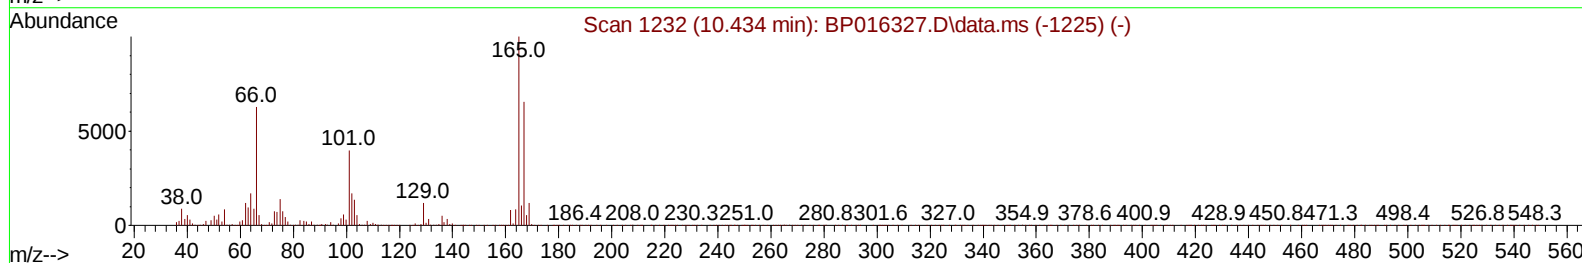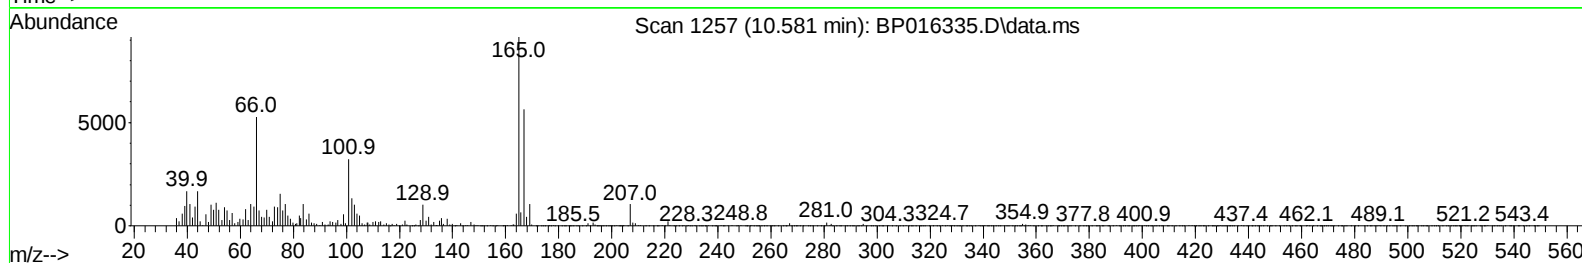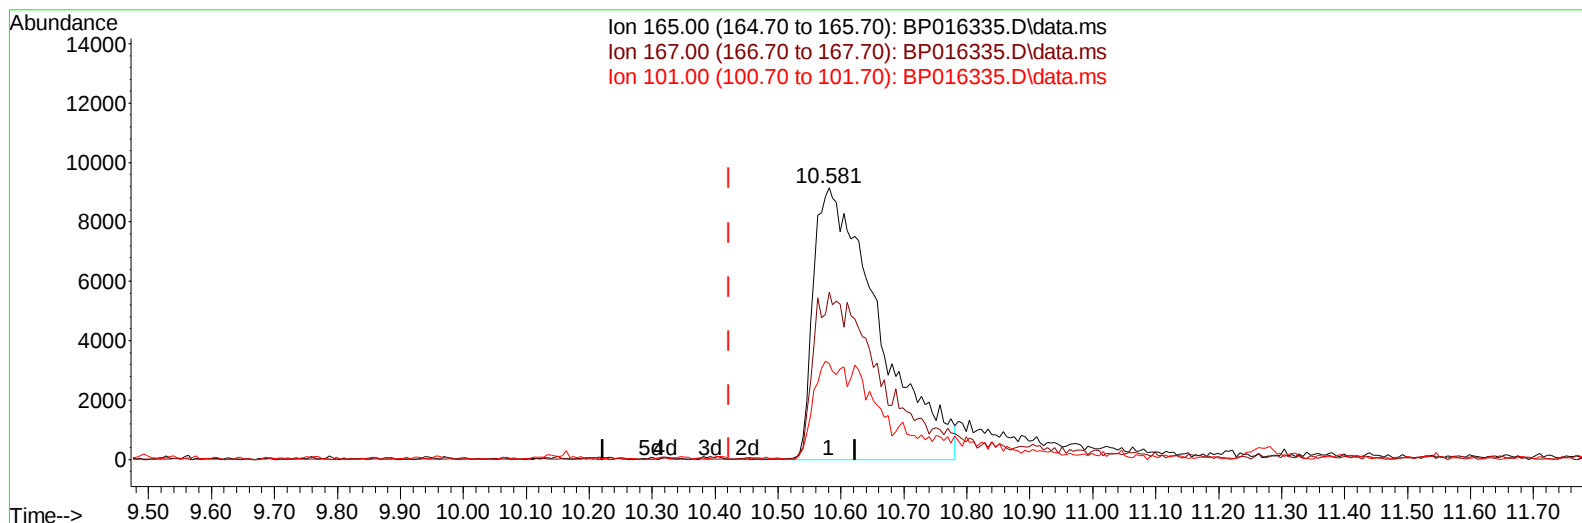

TIC: BP016335.D\data.ms

(28) 2,4-Dichlorophenol-d3 (S)

10.581min (+ 0.159) 9.49 ng/ul m

response 66132

Ion	Exp%	Act%
165.00	100.00	100.00
167.00	65.20	61.71
101.00	38.50	35.38
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071923\
Data File : BP016335.D
Acq On : 19 Jul 2023 21:36
Operator : MA/JU
Sample : 03472-21
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A46R2

Manual IntegrationsAPPROVED

Quant Time: Jul 19 23:28:43 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jul 19 14:47:57 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/20/2023
Supervised By :mohammad ahmed 07/20/2023

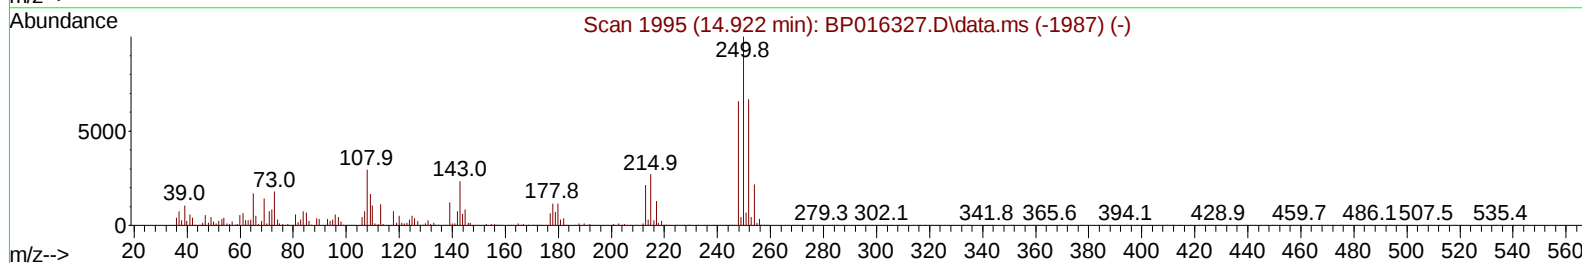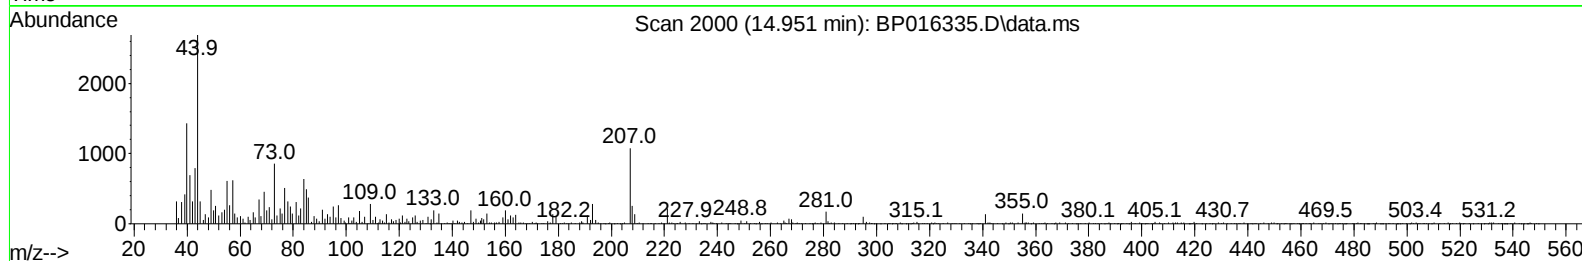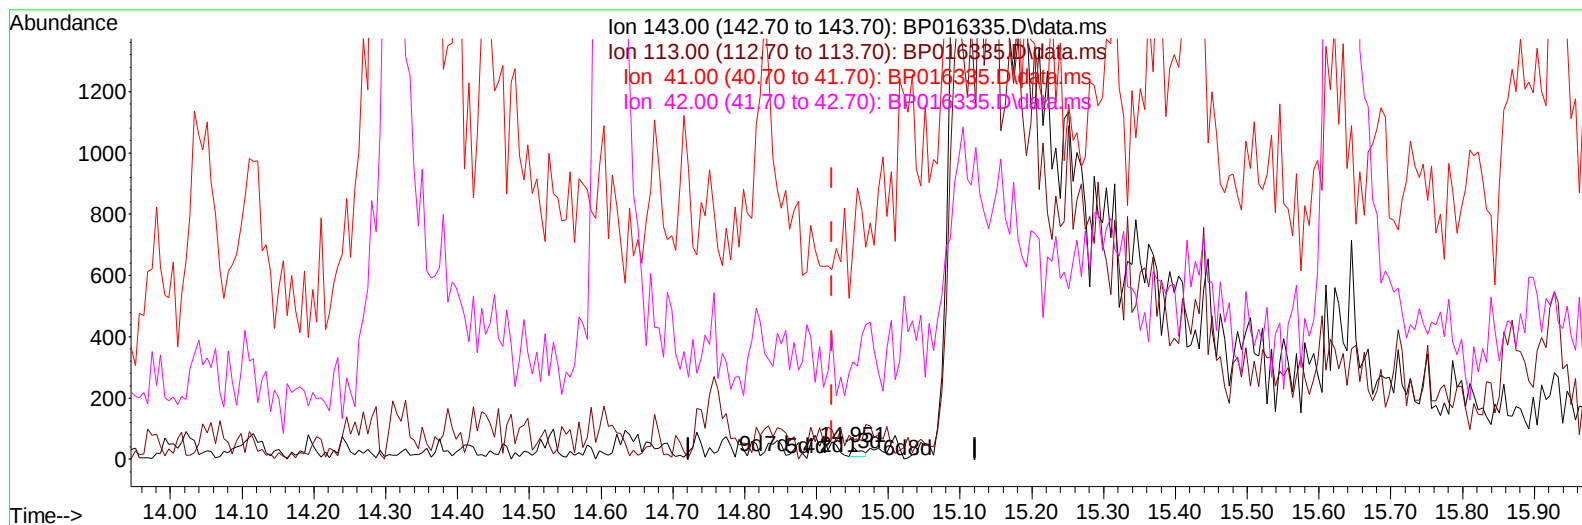

TIC: BP016335.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.951min (+ 0.029) 0.01 ng/u1

response 28

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	79.50	273.17#
41.00	49.30	1682.93#
42.00	32.70	778.05#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071923\
Data File : BP016335.D
Acq On : 19 Jul 2023 21:36
Operator : MA/JU
Sample : 03472-21
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A46R2

Manual IntegrationsAPPROVED

Quant Time: Jul 19 23:28:43 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jul 19 14:47:57 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/20/2023
Supervised By :mohammad ahmed 07/20/2023

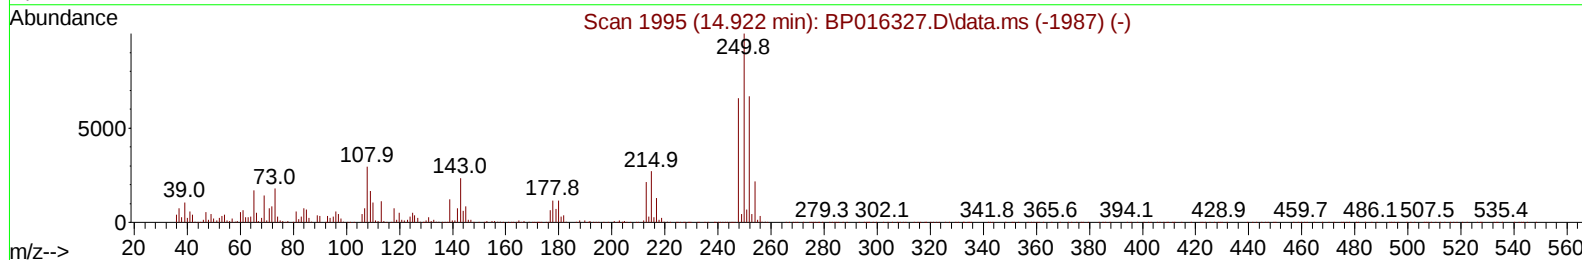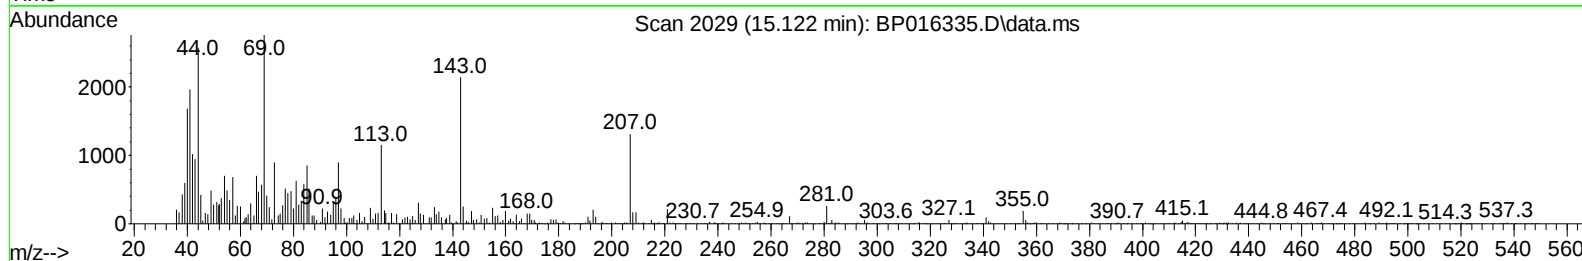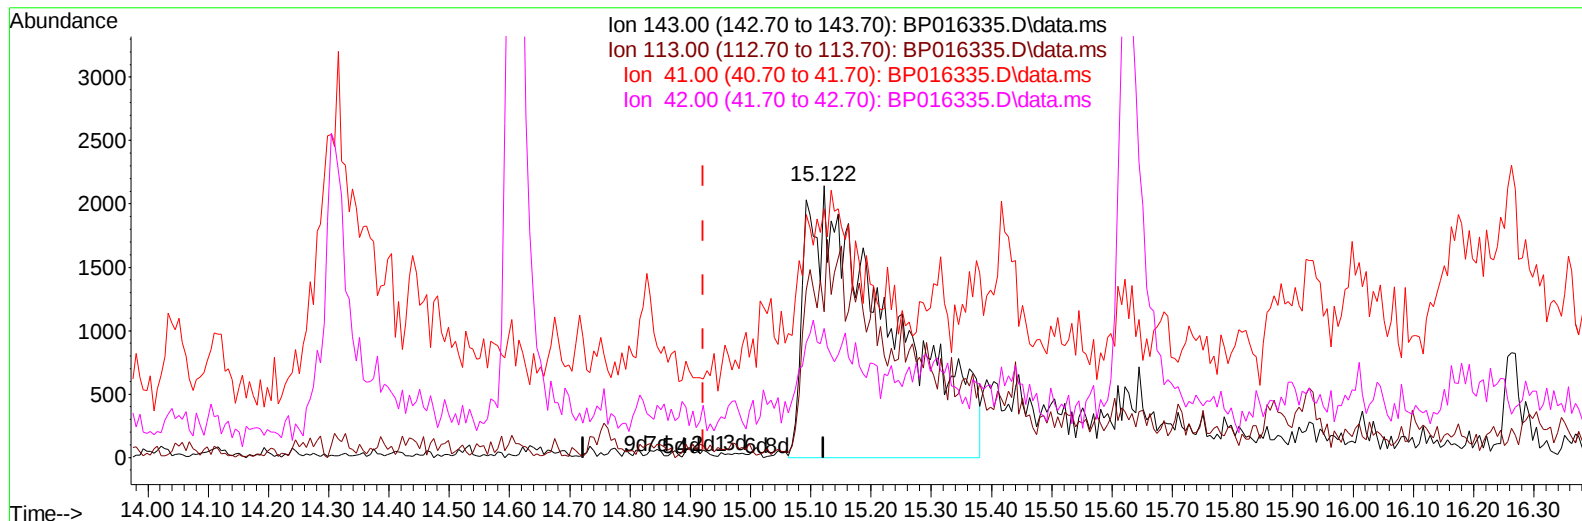

TIC: BP016335.D\data.ms

(54) 4-Nitrophenol-d4 (S)

15.122min (+ 0.200) 4.01 ng/ul m

response 21114

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	79.50	53.55#
41.00	49.30	91.64#
42.00	32.70	47.53#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071923\
 Data File : BP016335.D
 Acq On : 19 Jul 2023 21:36
 Operator : MA/JU
 Sample : 03472-21
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A46R2

Manual IntegrationsAPPROVED

Quant Time: Jul 19 23:28:43 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jul 19 14:47:57 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/20/2023
 Supervised By :mohammad ahmed 07/20/2023

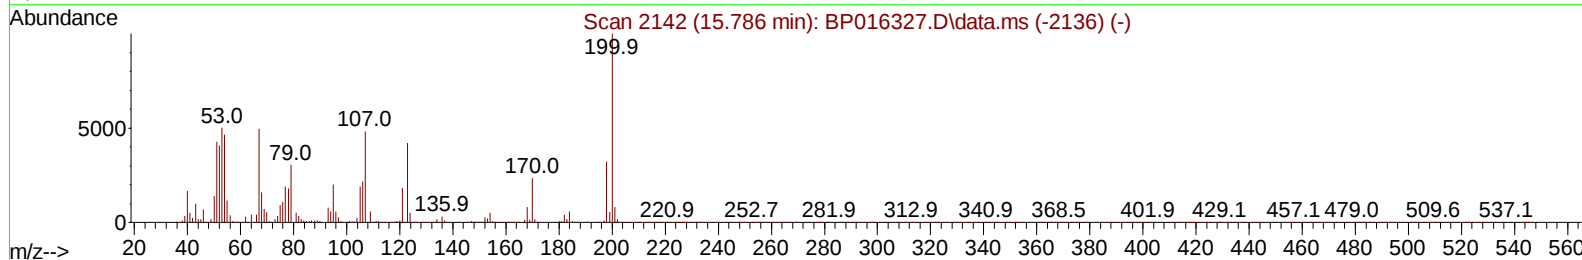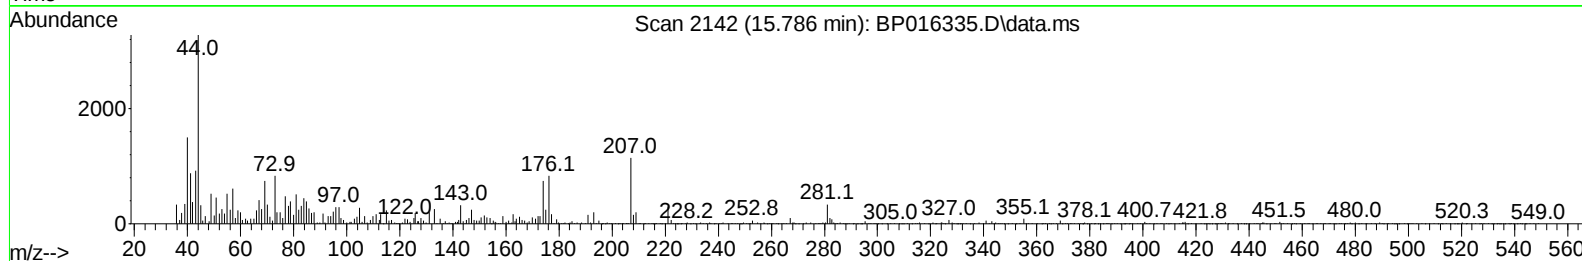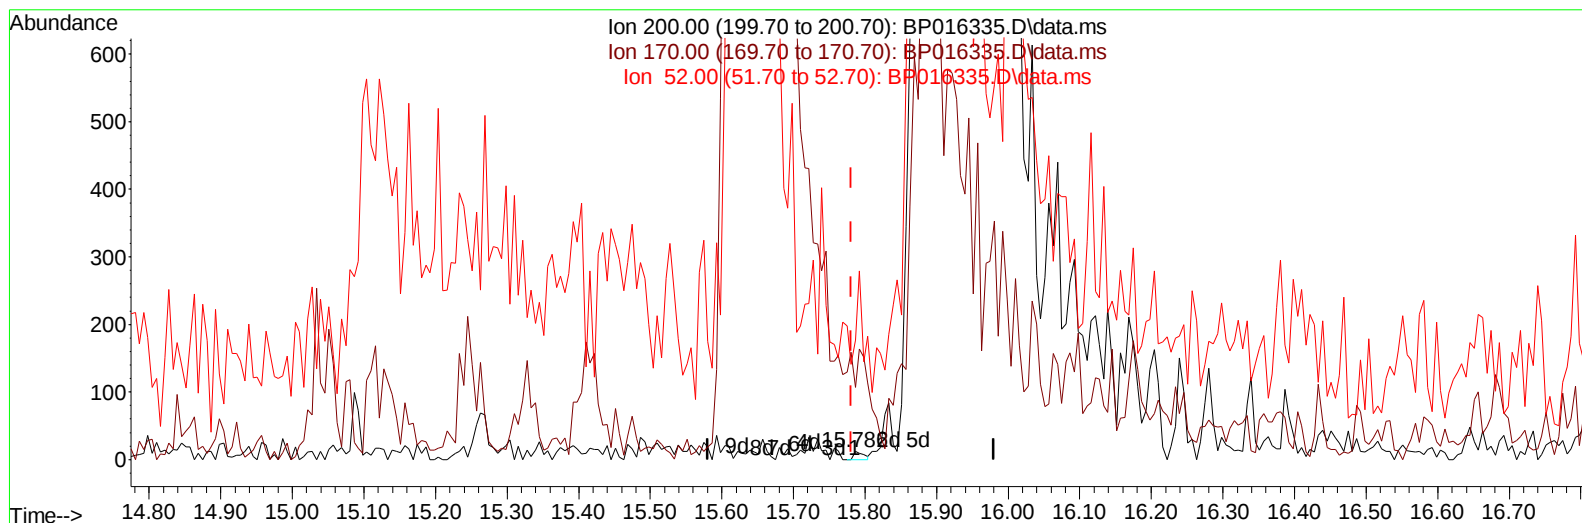

TIC: BP016335.D\data.ms

(65) 4,6-Dinitro-2-methylphenol-d2 (S)

15.786min (+ 0.006) 0.00 ng/u1

response 12

Ion	Exp%	Act%
200.00	100.00	100.00
170.00	21.90	891.67#
52.00	58.00	1475.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071923\
 Data File : BP016335.D
 Acq On : 19 Jul 2023 21:36
 Operator : MA/JU
 Sample : 03472-21
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A46R2

Manual IntegrationsAPPROVED

Quant Time: Jul 19 23:28:43 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jul 19 14:47:57 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/20/2023
 Supervised By :mohammad ahmed 07/20/2023

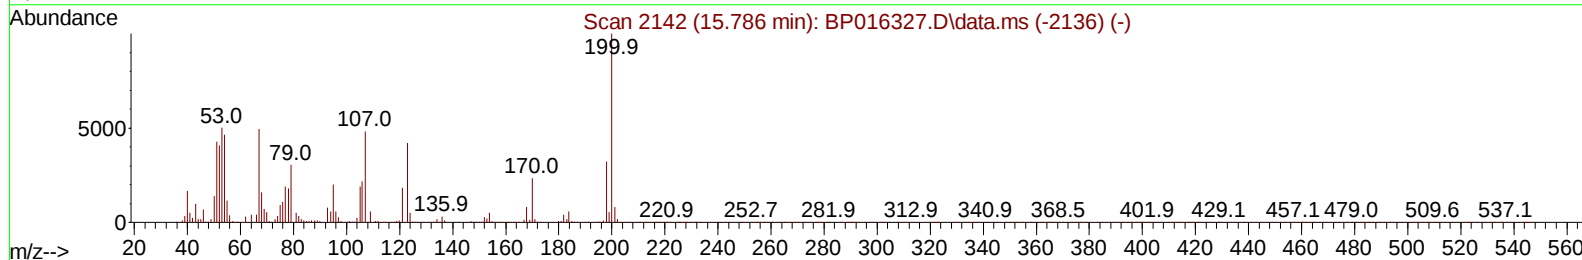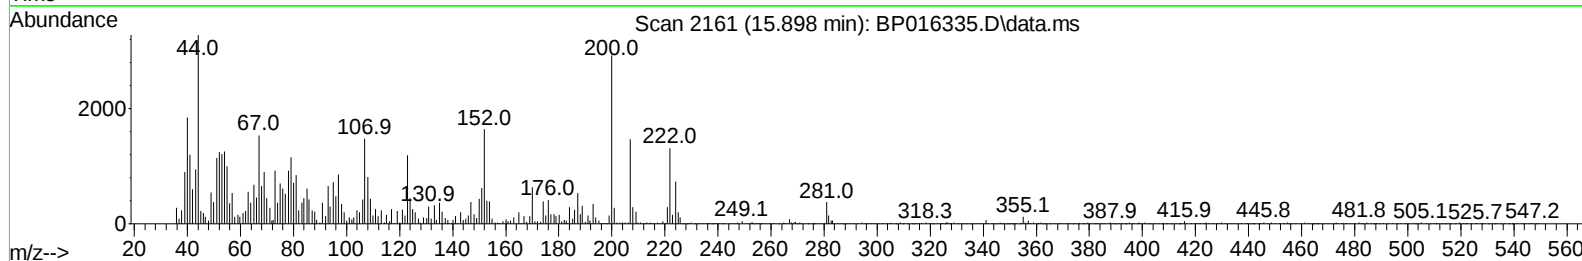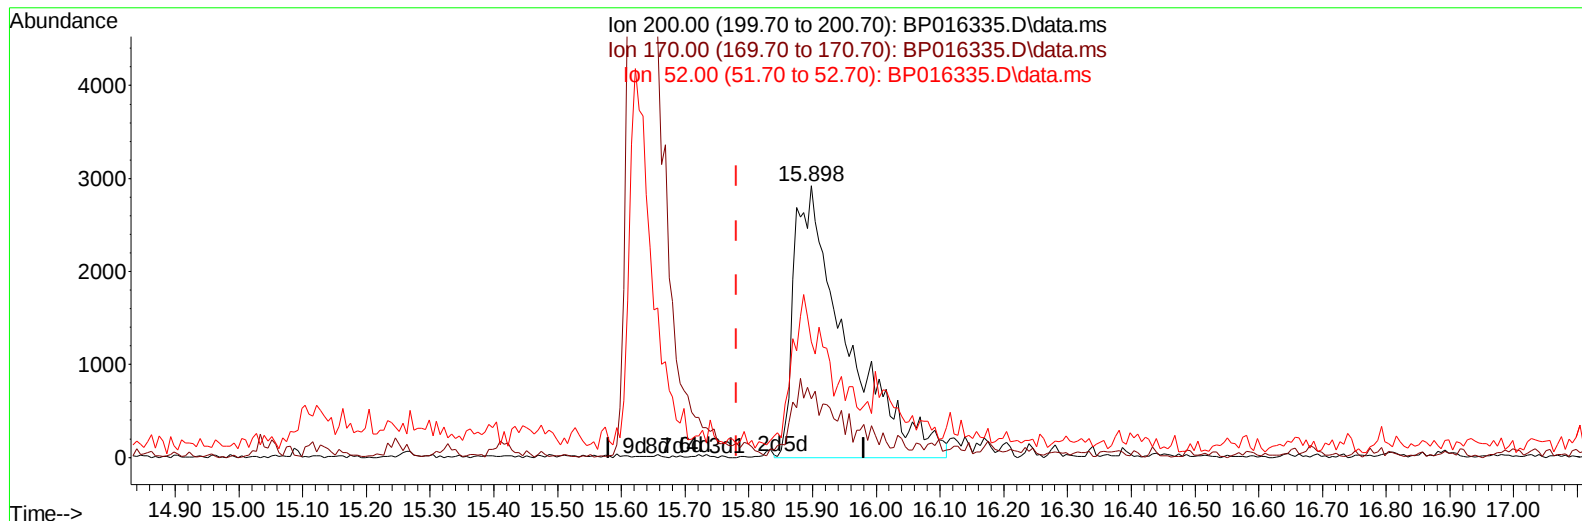

TIC: BP016335.D\data.ms

(65) 4,6-Dinitro-2-methylphenol-d2 (S)

15.898min (+ 0.118) 3.65 ng/ul m

response 16638

Ion	Exp%	Act%
200.00	100.00	100.00
170.00	21.90	21.58
52.00	58.00	42.60#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071923\
 Data File : BP016335.D
 Acq On : 19 Jul 2023 21:36
 Operator : MA/JU
 Sample : 03472-21
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A46R2

Manual IntegrationsAPPROVED

Quant Time: Jul 19 23:31:13 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jul 19 14:47:57 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/20/2023
 Supervised By :mohammad ahmed 07/20/2023

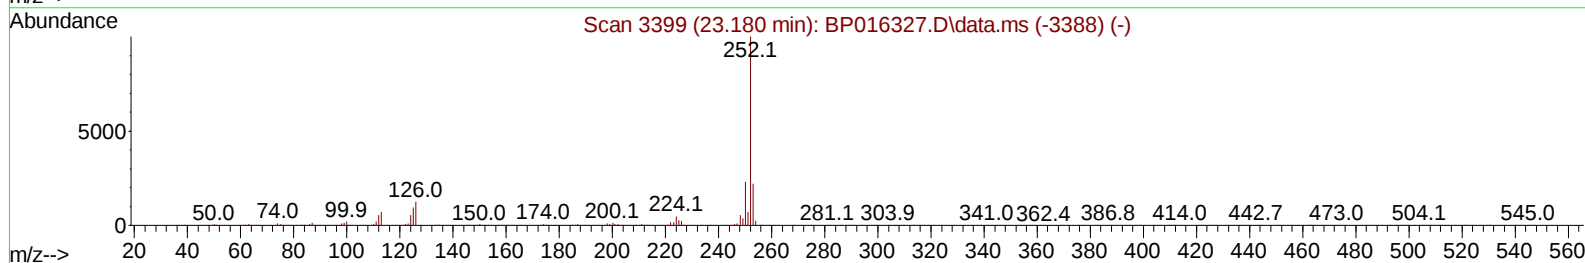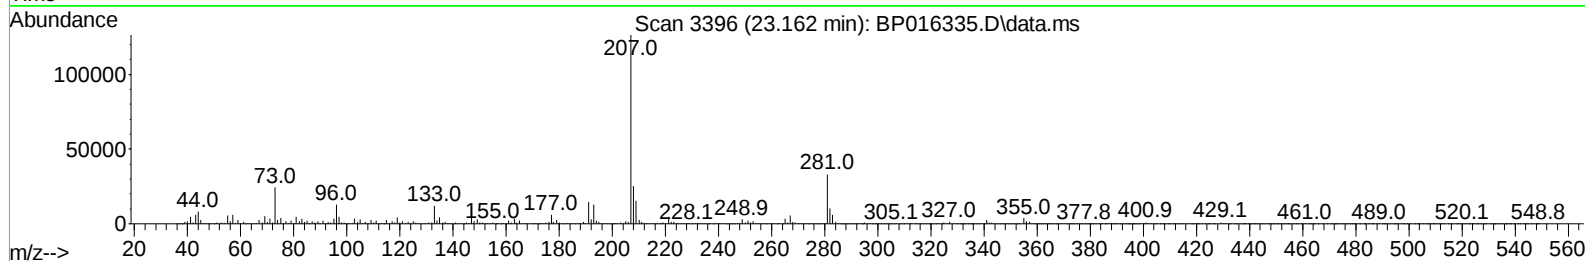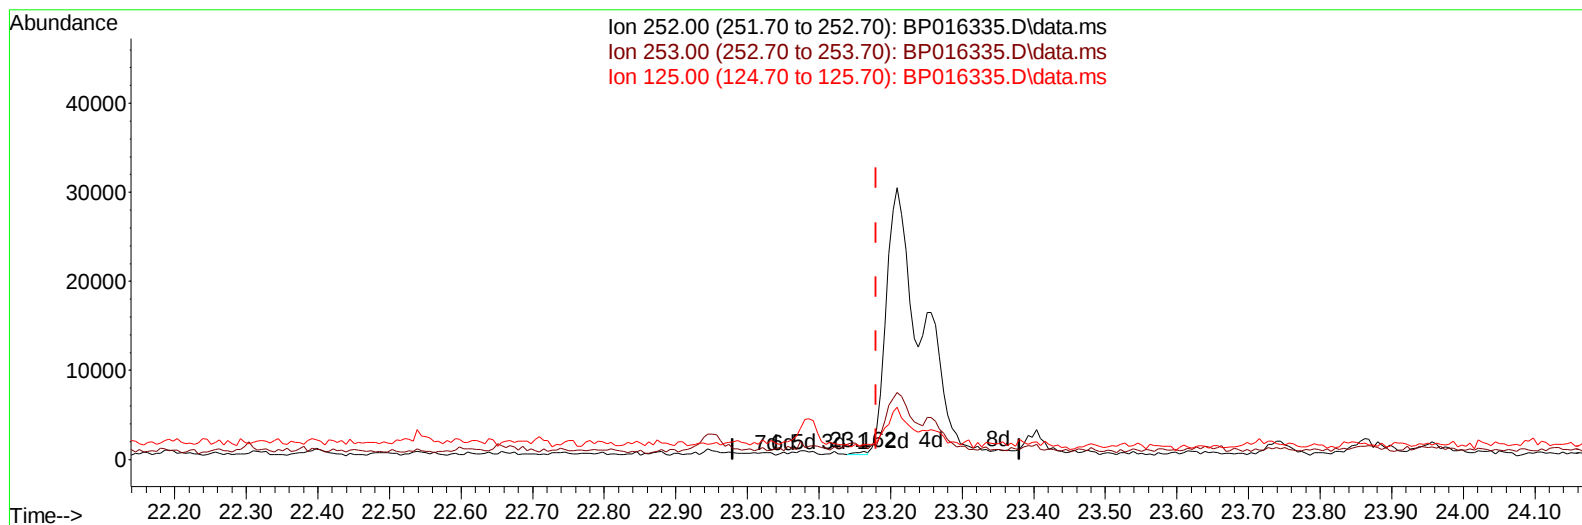

TIC: BP016335.D\data.ms

(90) Benzo(b)fluoranthene

23.162min (-0.018) 0.01 ng/u1

response 372

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	21.60	188.61#
125.00	11.70	192.37#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071923\
 Data File : BP016335.D
 Acq On : 19 Jul 2023 21:36
 Operator : MA/JU
 Sample : 03472-21
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A46R2

Manual IntegrationsAPPROVED

Quant Time: Jul 19 23:31:13 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jul 19 14:47:57 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/20/2023
 Supervised By :mohammad ahmed 07/20/2023

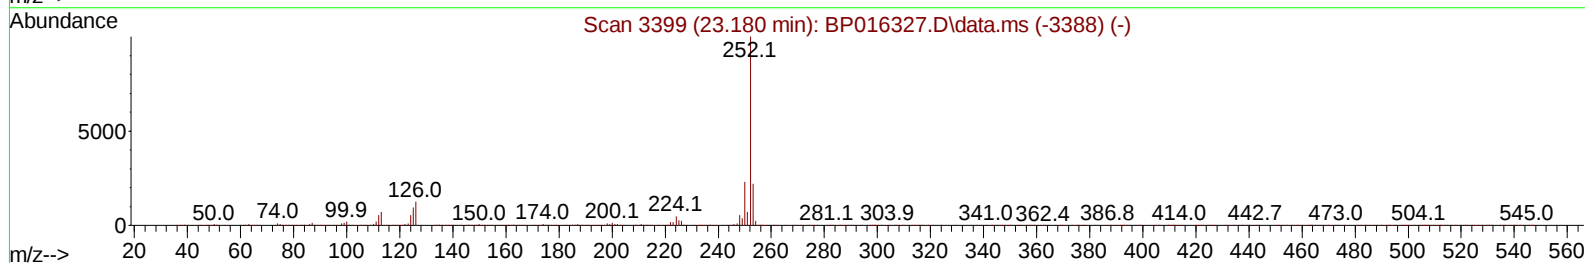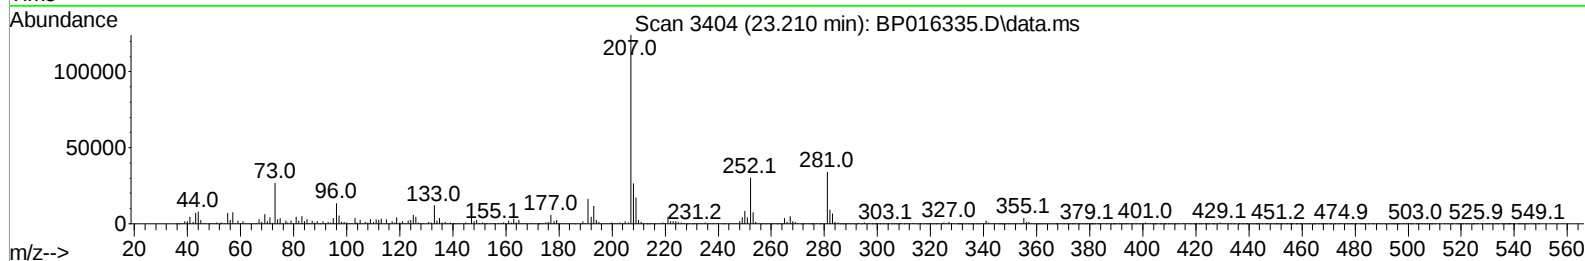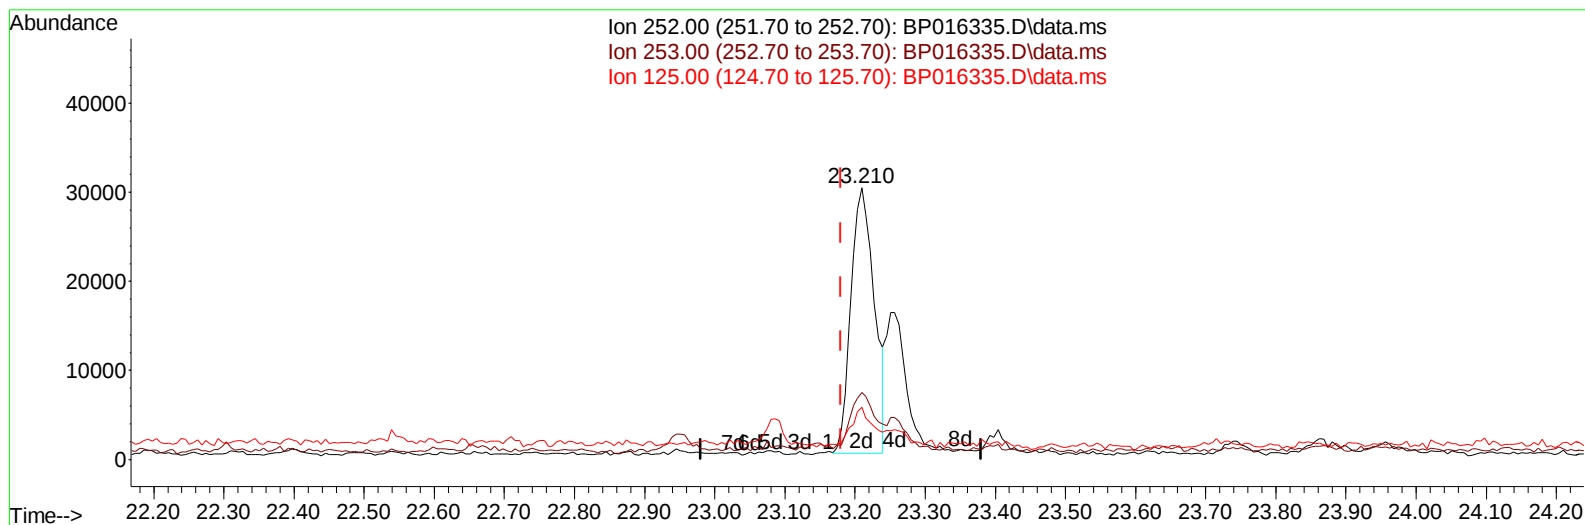

TIC: BP016335.D\data.ms

(90) Benzo(b)fluoranthene

23.210min (+ 0.029) 1.33 ng/u1 m

response 69025

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	21.60	24.70
125.00	11.70	19.18#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071923\
 Data File : BP016335.D
 Acq On : 19 Jul 2023 21:36
 Operator : MA/JU
 Sample : 03472-21
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A46R2

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 07/20/2023
 Supervised By :mohammad ahmed 07/20/2023

Quant Time: Jul 19 23:32:06 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jul 19 14:47:57 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.952	152	112163	20.000	ng/ul	0.00
20) Naphthalene-d8	10.781	136	511825	20.000	ng/ul	0.02
38) Acenaphthene-d10	14.610	164	338343	20.000	ng/ul	0.02
64) Phenanthrene-d10	17.380	188	789747	20.000	ng/ul	0.02
79) Chrysene-d12	21.468	240	889034	20.000	ng/ul	0.00
88) Perylene-d12	23.957	264	905359	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.281	96	5640m	1.779	ng/uL	0.00
4) Pyridine-d5	0.000	84	0d	0.000	ng/ul	
7) Phenol-d5	7.199	99	57344	5.660	ng/ul	0.06
9) Bis-(2-Chloroethyl)eth...	7.299	67	65145m	9.509	ng/ul	0.02
11) 2-Chlorophenol-d4	7.516	132	77741	10.630	ng/ul	0.04
15) 4-Methylphenol-d8	8.816	113	41164m	5.044	ng/ul	0.13
21) Nitrobenzene-d5	9.199	128	29119m	8.247	ng/ul	0.06
24) 2-Nitrophenol-d4	9.963	143	41142m	10.223	ng/ul	0.10
28) 2,4-Dichlorophenol-d3	10.581	165	66132m	9.489	ng/ul	0.16
31) 4-Chloroaniline-d4	10.975	131	26	0.002	ng/ul	0.04
46) Dimethylphthalate-d6	14.045	166	241198	9.345	ng/ul	0.04
49) Acenaphthylene-d8	14.310	160	213474	7.547	ng/ul	0.02
54) 4-Nitrophenol-d4	15.122	143	21114m	4.009	ng/ul	0.20
60) Fluorene-d10	15.628	176	278784	12.907	ng/ul	0.04
65) 4,6-Dinitro-2-methylph...	15.898	200	16638m	3.649	ng/ul	0.12
73) Anthracene-d10	17.492	188	307447	8.900	ng/ul	0.02
81) Pyrene-d10	19.721	212	138462	3.001	ng/ul	0.02
92) Benzo(a)pyrene-d12	23.804	264	54746	1.259	ng/ul	0.02
Target Compounds						
						Qvalue
16) Acetophenone	8.869	105	34405	2.556	ng/ul	95
80) Fluoranthene	19.398	202	104914	1.945	ng/ul	100
86) Bis(2-ethylhexyl)phtha...	21.316	149	125525	3.383	ng/ul	97
87) Chrysene	21.510	228	71323	1.216	ng/ul	96
90) Benzo(b)fluoranthene	23.210	252	69025m	1.335	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071923\
Data File : BP016335.D
Acq On : 19 Jul 2023 21:36
Operator : MA/JU
Sample : 03472-21
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A46R2

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 07/20/2023
Supervised By :mohammad ahmed 07/20/2023

Quant Time: Jul 19 23:32:06 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jul 19 14:47:57 2023
Response via : Initial Calibration

