




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071923\
Data File : BP016337.D
Acq On : 19 Jul 2023 22:44
Operator : MA/JU
Sample : 03472-23
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A46R4

Manual IntegrationsAPPROVED

Quant Time: Jul 20 00:12:17 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jul 19 14:47:57 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/20/2023
Supervised By :mohammad ahmed 07/20/2023

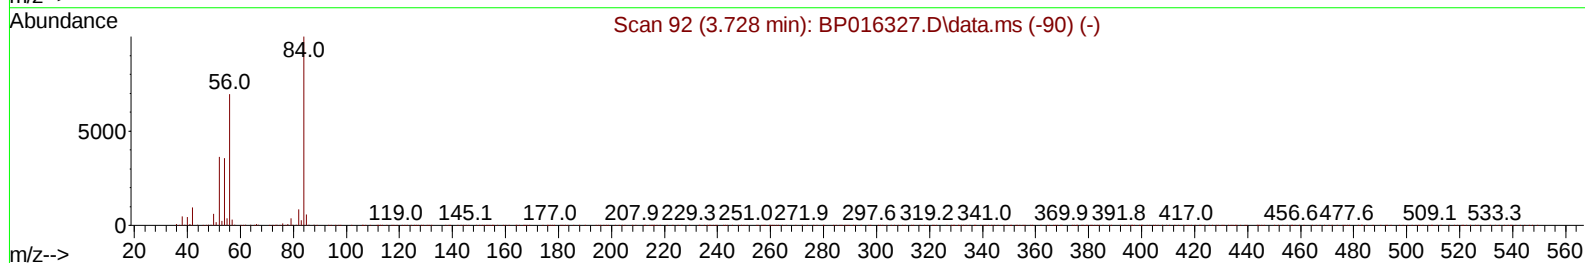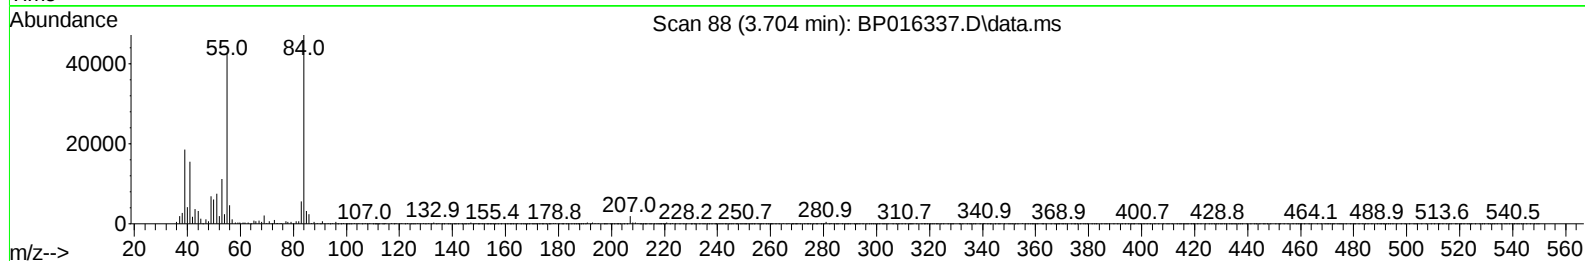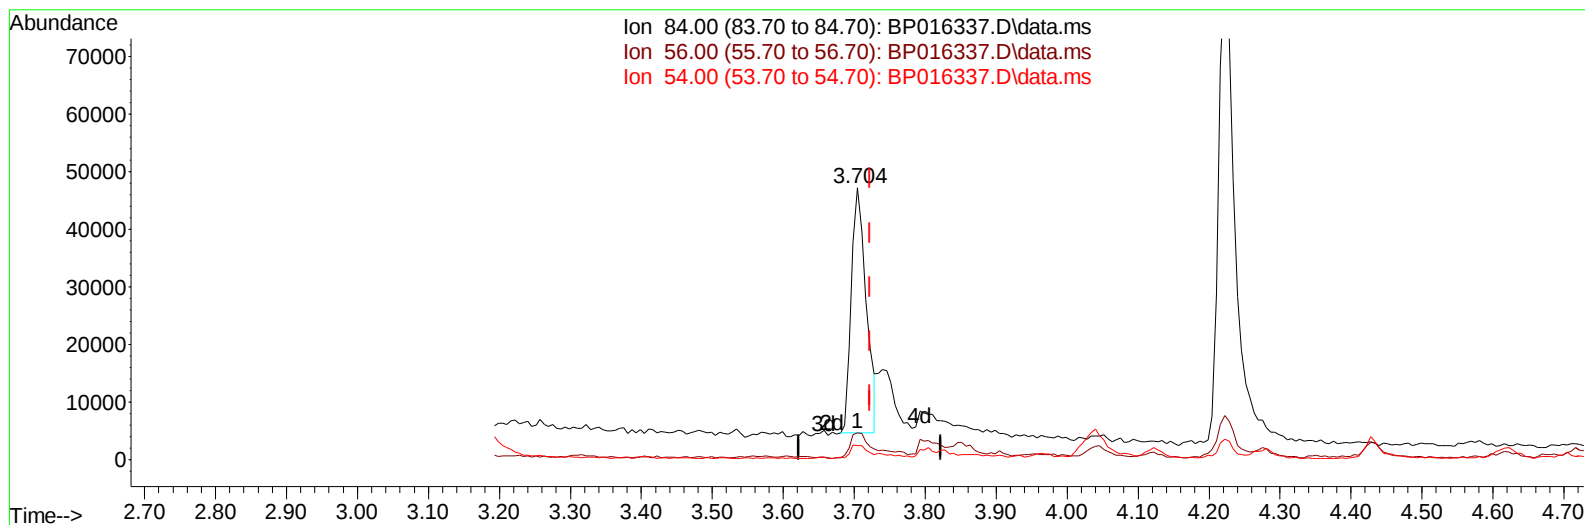

TIC: BP016337.D\data.ms

(4) Pyridine-d5 (S)

3.704min (-0.018) 8.02 ng/u1

response 61362

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	64.90	9.89#
54.00	32.50	5.10#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071923\
 Data File : BP016337.D
 Acq On : 19 Jul 2023 22:44
 Operator : MA/JU
 Sample : 03472-23
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A46R4

Manual IntegrationsAPPROVED

Quant Time: Jul 20 00:12:17 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jul 19 14:47:57 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/20/2023
 Supervised By :mohammad ahmed 07/20/2023

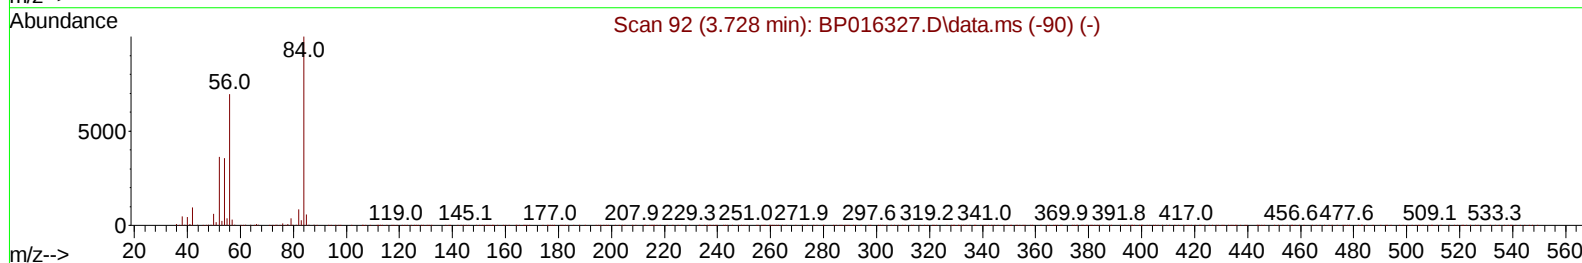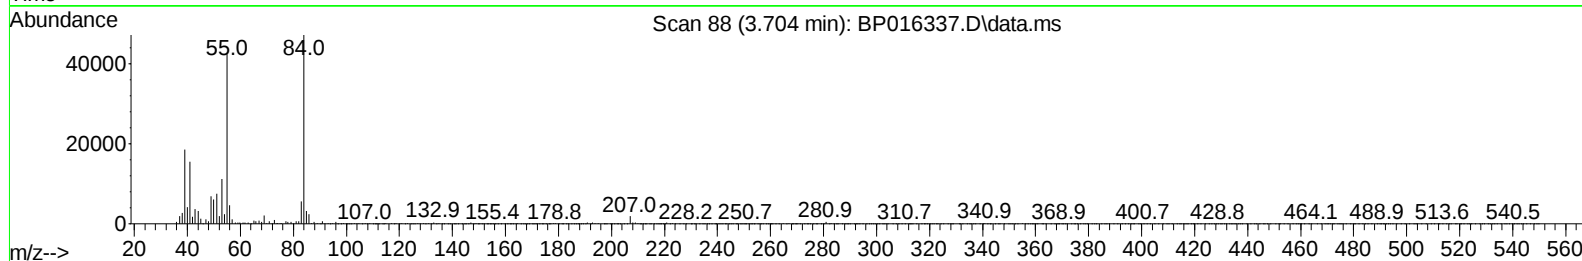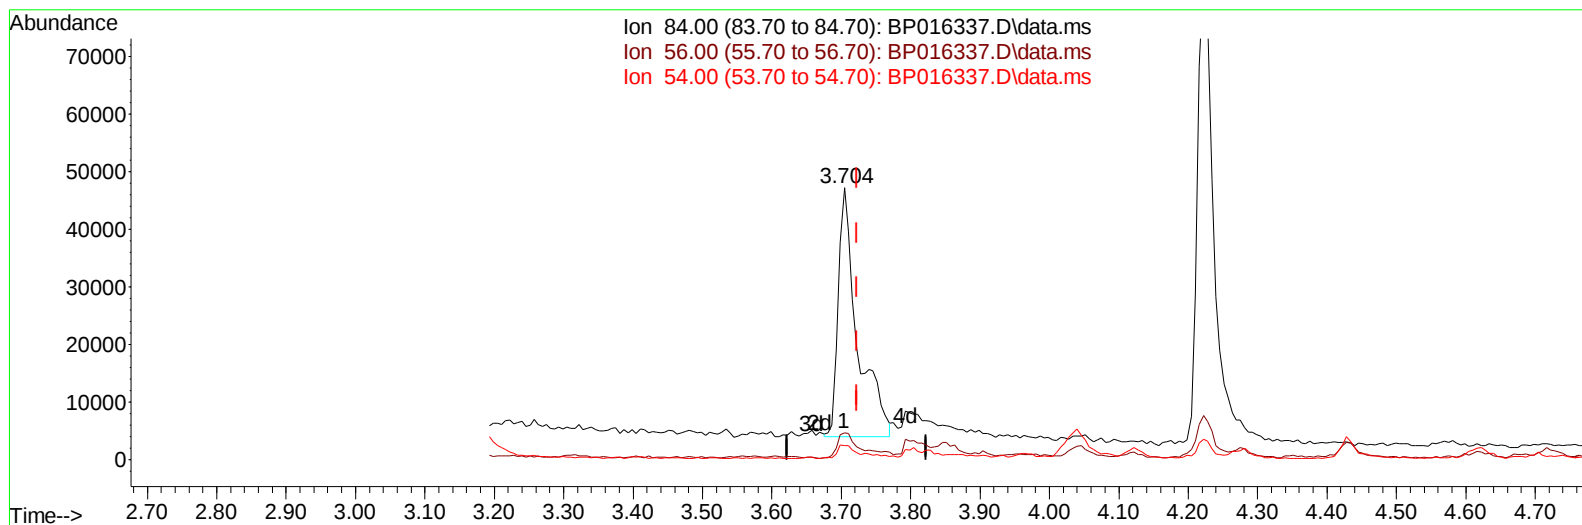

TIC: BP016337.D\data.ms

(4) Pyridine-d5 (S)

3.704min (-0.018) 10.90 ng/ul m

response 83357

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	64.90	9.89#
54.00	32.50	5.10#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071923\
 Data File : BP016337.D
 Acq On : 19 Jul 2023 22:44
 Operator : MA/JU
 Sample : 03472-23
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A46R4

Manual IntegrationsAPPROVED

Quant Time: Jul 20 00:12:17 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jul 19 14:47:57 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/20/2023
 Supervised By :mohammad ahmed 07/20/2023

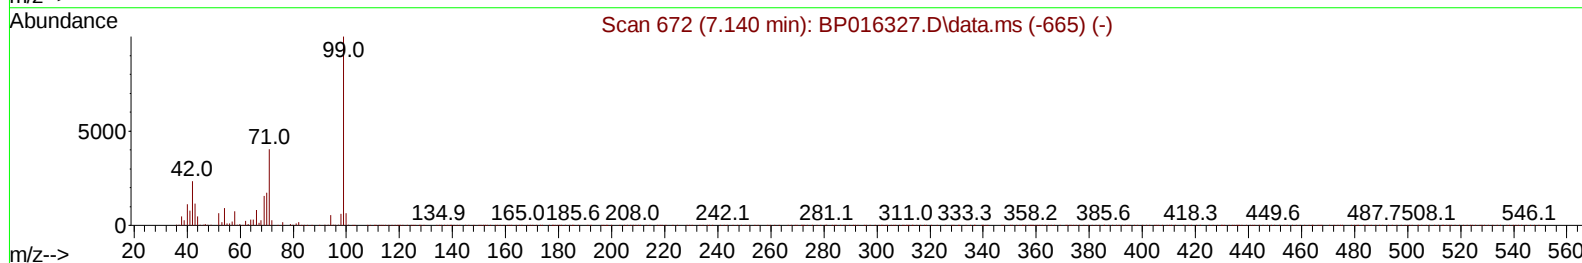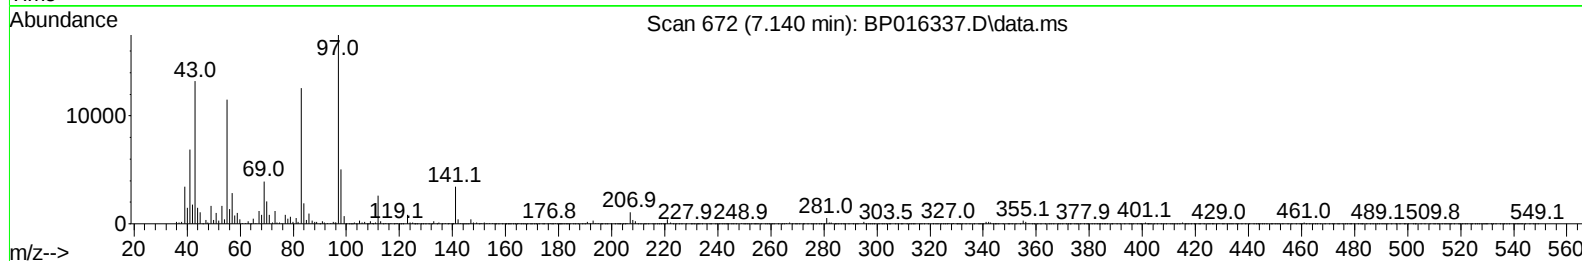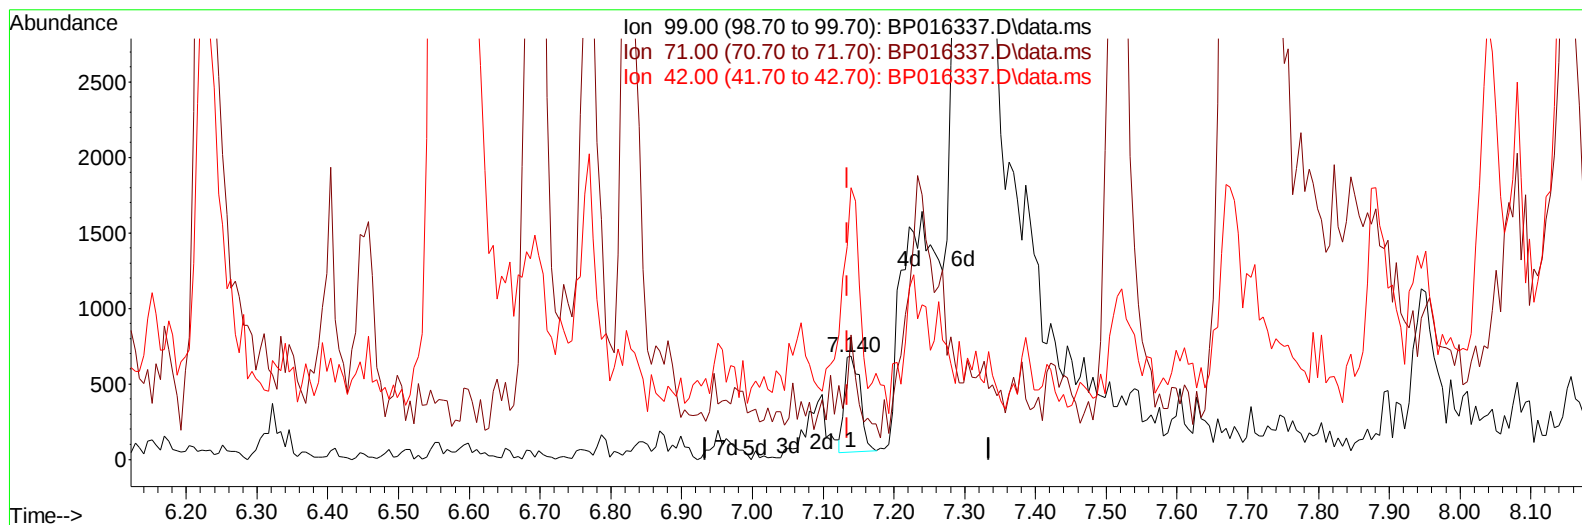

TIC: BP016337.D\data.ms

(7) Phenol-d5 (S)

7.140min (+ 0.006) 0.10 ng/u1

response 978

Ion	Exp%	Act%
99.00	100.00	100.00
71.00	35.20	120.47#
42.00	21.40	262.87#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071923\
 Data File : BP016337.D
 Acq On : 19 Jul 2023 22:44
 Operator : MA/JU
 Sample : 03472-23
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A46R4

Manual IntegrationsAPPROVED

Quant Time: Jul 20 00:12:17 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jul 19 14:47:57 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/20/2023
 Supervised By :mohammad ahmed 07/20/2023

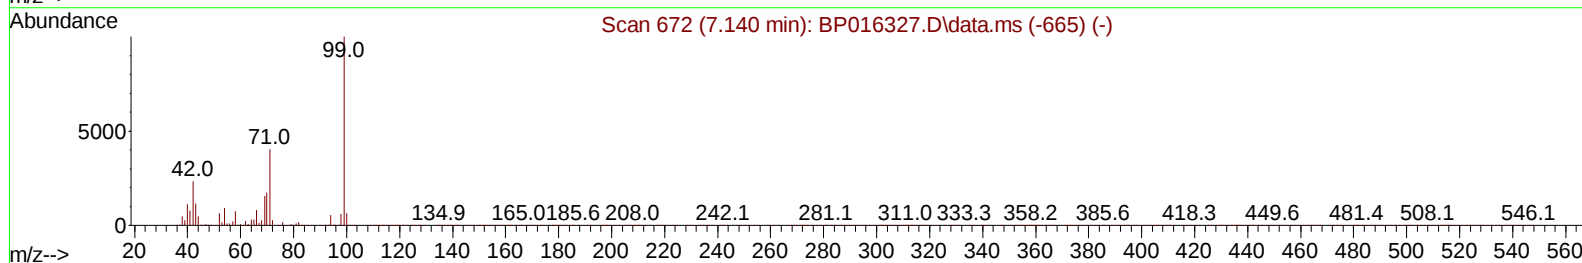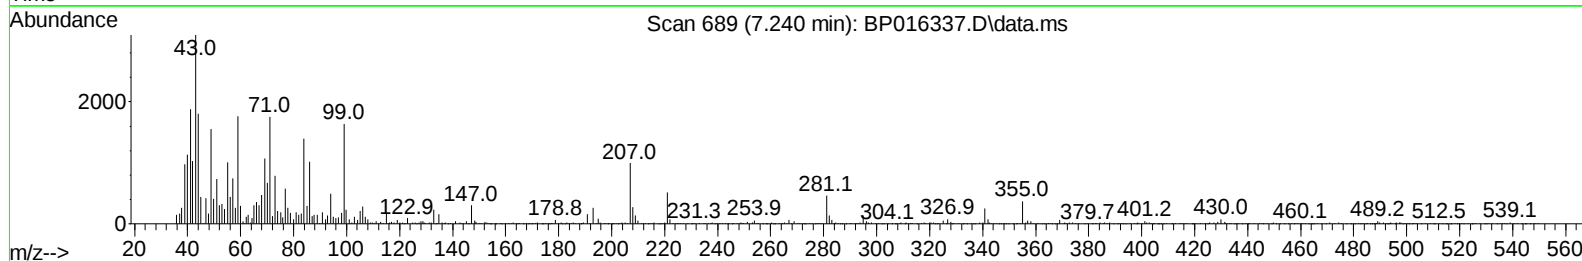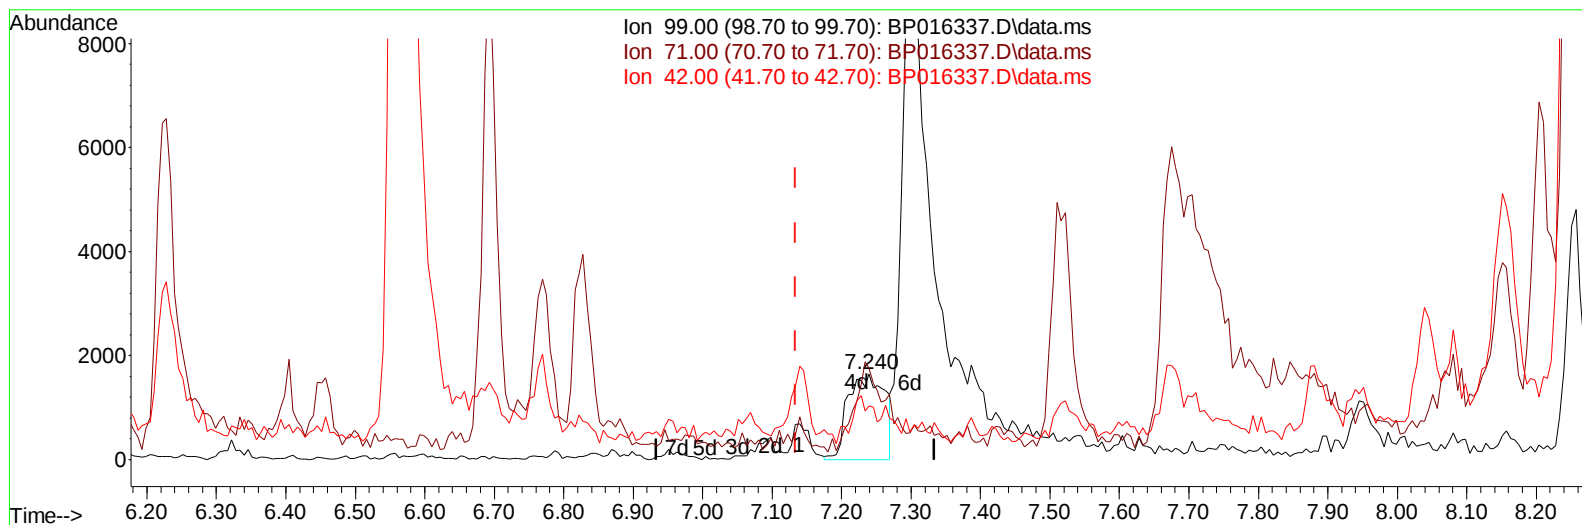

TIC: BP016337.D\data.ms

(7) Phenol-d5 (S)

7.240min (+ 0.106) 0.61 ng/u1 m

response 6007

Ion	Exp%	Act%
99.00	100.00	100.00
71.00	35.20	106.88#
42.00	21.40	62.48#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071923\
 Data File : BP016337.D
 Acq On : 19 Jul 2023 22:44
 Operator : MA/JU
 Sample : 03472-23
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A46R4

Manual IntegrationsAPPROVED

Quant Time: Jul 20 00:12:17 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jul 19 14:47:57 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/20/2023
 Supervised By :mohammad ahmed 07/20/2023

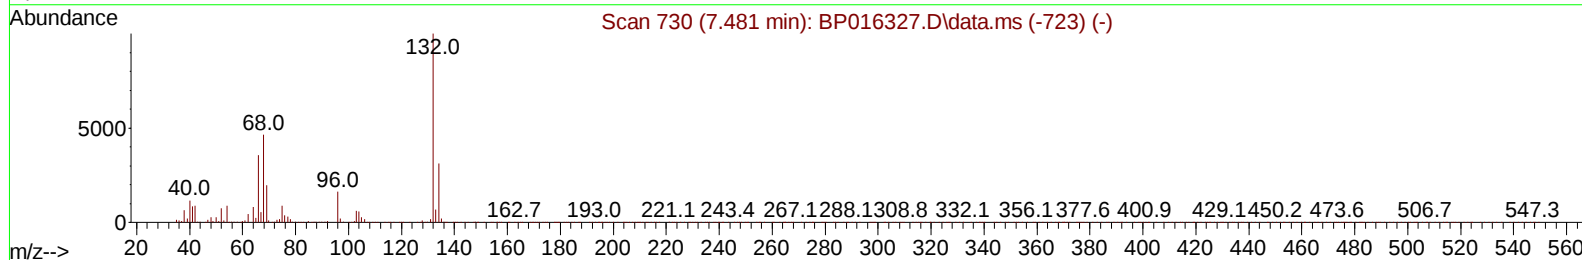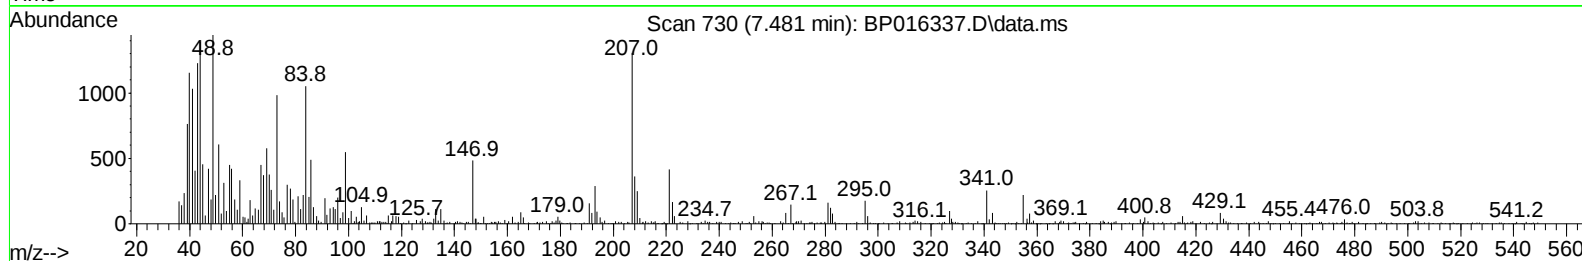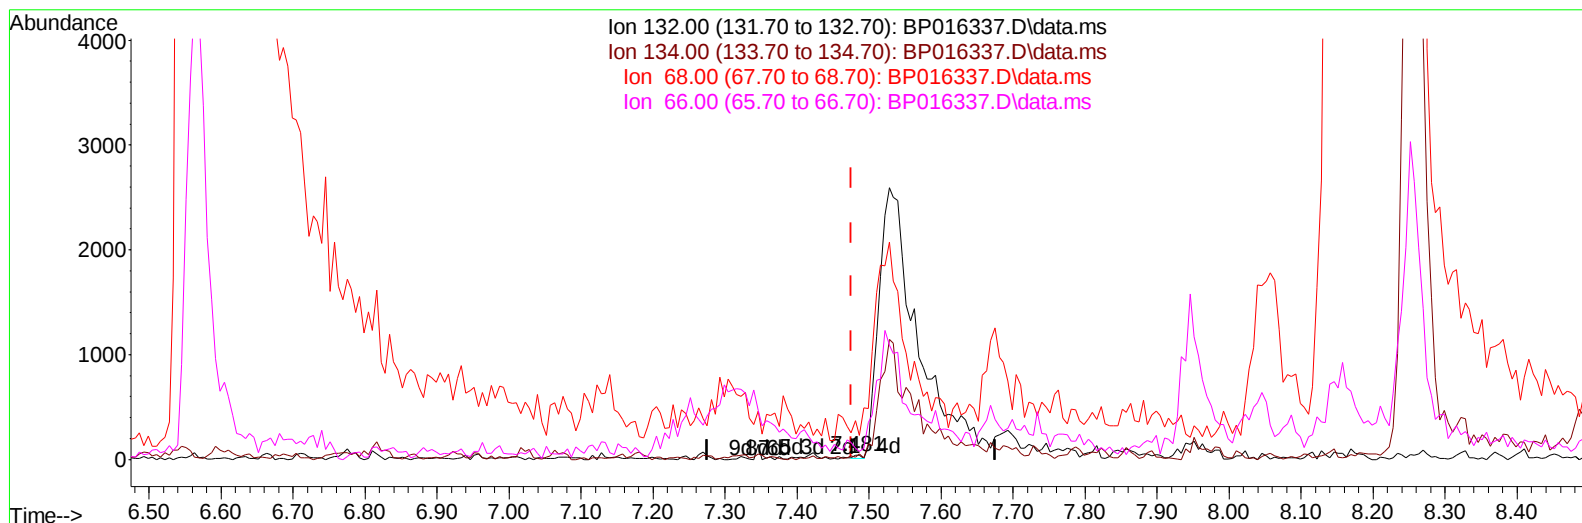

TIC: BP016337.D\data.ms

(11) 2-Chlorophenol-d4 (S)

7.481min (+ 0.006) 0.00 ng/u1

response 19

Ion	Exp%	Act%
132.00	100.00	100.00
134.00	31.50	60.00#
68.00	47.30	925.00#
66.00	33.60	270.00#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071923\
 Data File : BP016337.D
 Acq On : 19 Jul 2023 22:44
 Operator : MA/JU
 Sample : 03472-23
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A46R4

Manual IntegrationsAPPROVED

Quant Time: Jul 20 00:12:17 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jul 19 14:47:57 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/20/2023
 Supervised By :mohammad ahmed 07/20/2023

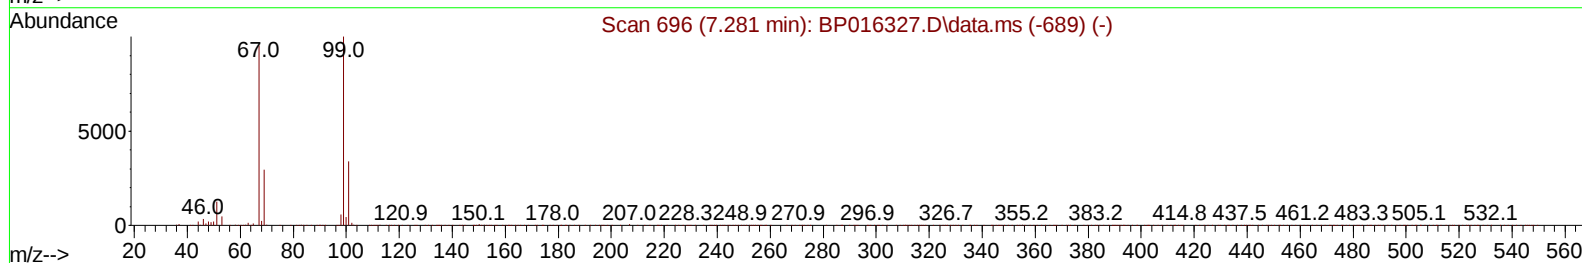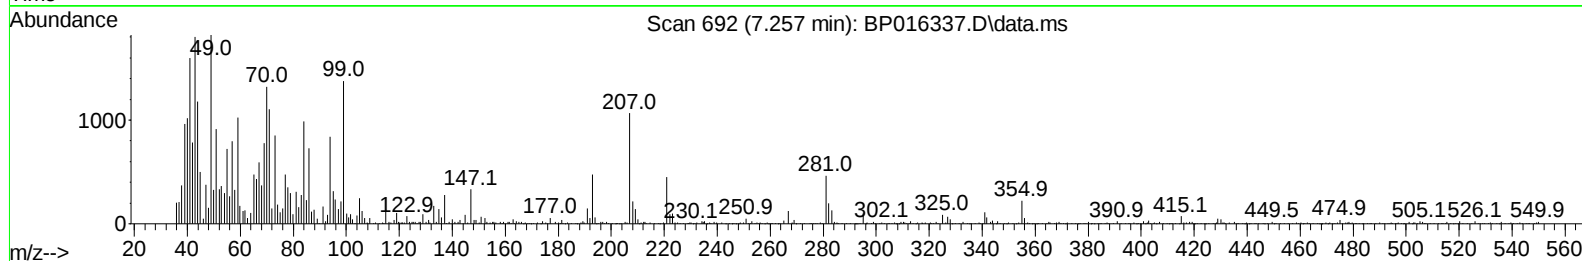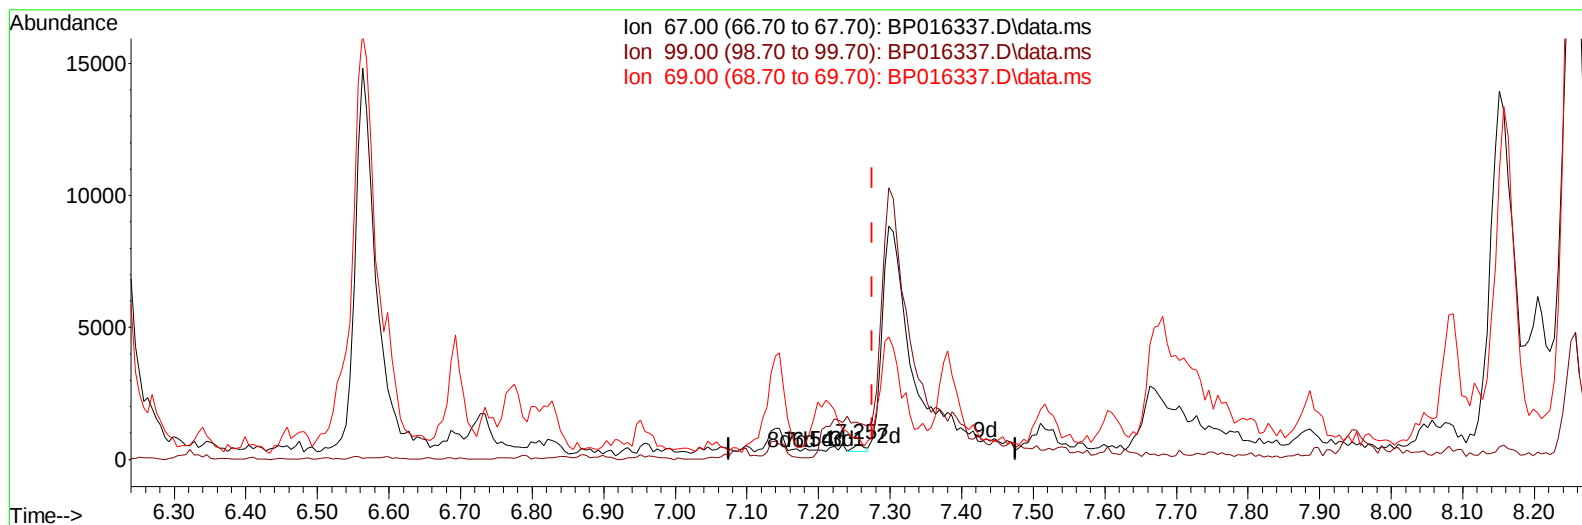

TIC: BP016337.D\data.ms

(9) Bis-(2-Chloroethyl)ether-d8 (S)

7.257min (-0.018) 0.05 ng/u1

response 303

Ion	Exp%	Act%
67.00	100.00	100.00
99.00	117.30	231.43#
69.00	33.10	131.26#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071923\
 Data File : BP016337.D
 Acq On : 19 Jul 2023 22:44
 Operator : MA/JU
 Sample : 03472-23
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A46R4

Manual IntegrationsAPPROVED

Quant Time: Jul 20 00:12:17 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jul 19 14:47:57 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/20/2023
 Supervised By :mohammad ahmed 07/20/2023

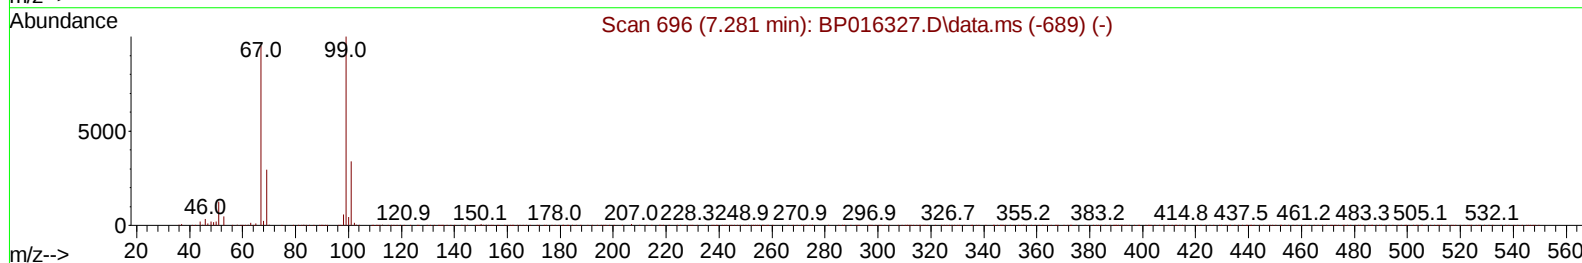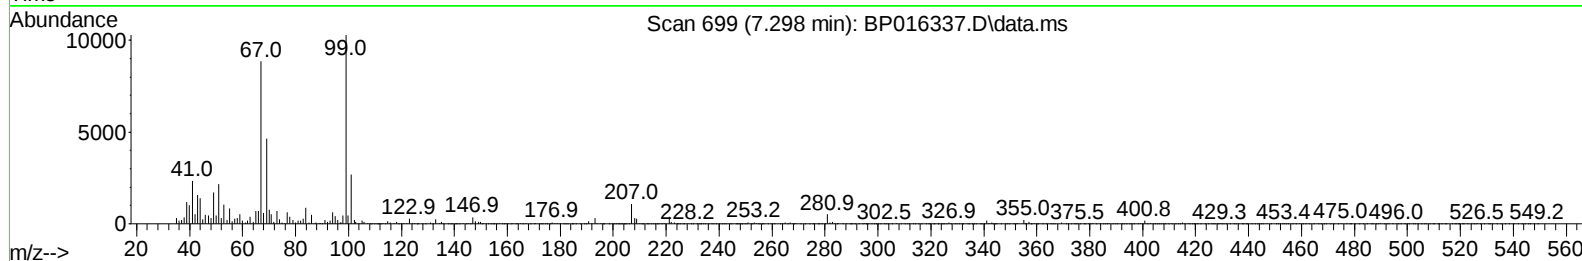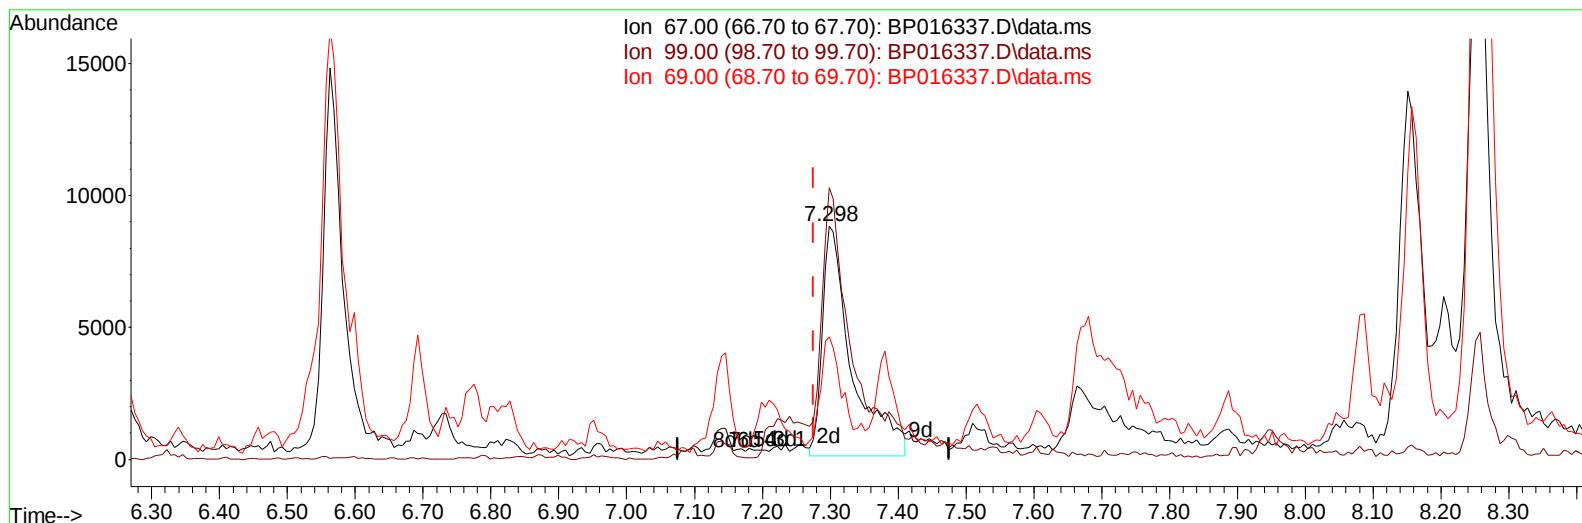

TIC: BP016337.D\data.ms

(9) Bis-(2-Chloroethyl)ether-d8 (S)

7.298min (+ 0.023) 3.98 ng/u1 m

response 26360

Ion	Exp%	Act%
67.00	100.00	100.00
99.00	117.30	116.31
69.00	33.10	52.40#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071923\
 Data File : BP016337.D
 Acq On : 19 Jul 2023 22:44
 Operator : MA/JU
 Sample : 03472-23
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A46R4

Manual IntegrationsAPPROVED

Quant Time: Jul 20 00:12:17 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jul 19 14:47:57 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/20/2023
 Supervised By :mohammad ahmed 07/20/2023

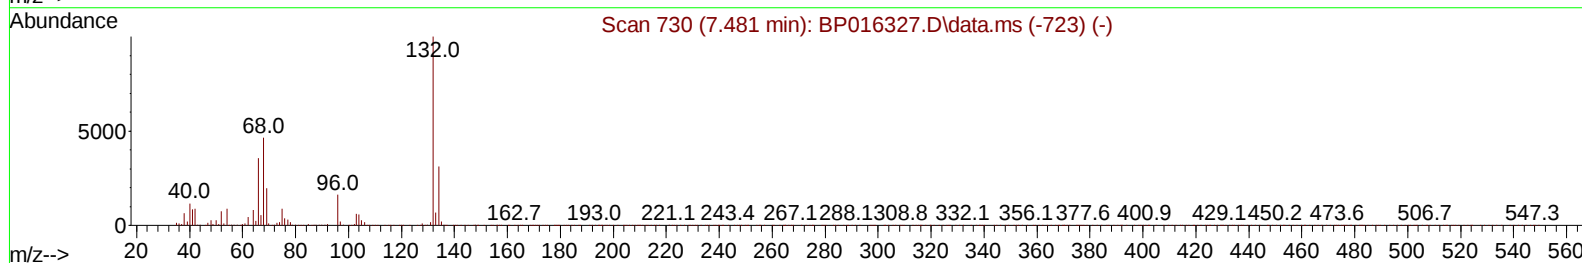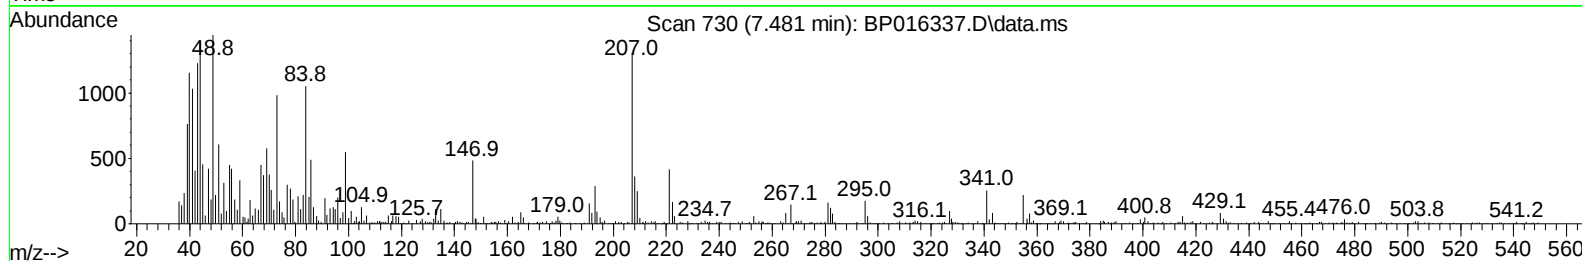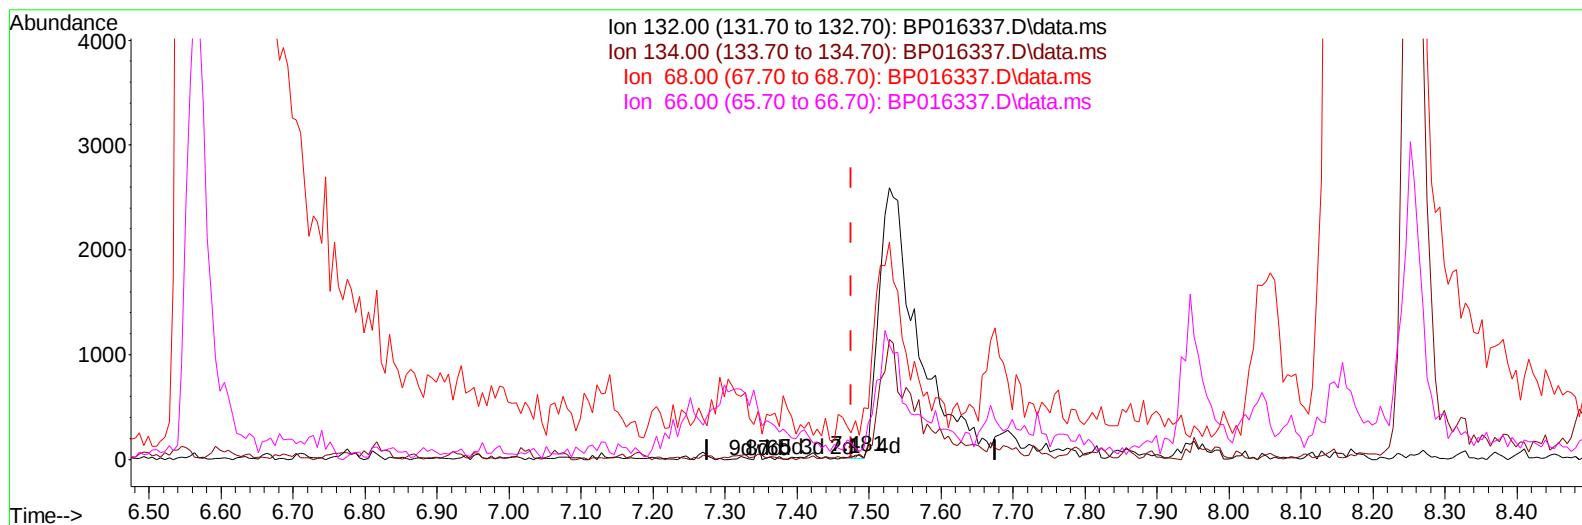

TIC: BP016337.D\data.ms

(11) 2-Chlorophenol-d4 (S)

7.481min (+ 0.006) 0.00 ng/u1

response 19

Ion	Exp%	Act%
132.00	100.00	100.00
134.00	31.50	60.00#
68.00	47.30	925.00#
66.00	33.60	270.00#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071923\
Data File : BP016337.D
Acq On : 19 Jul 2023 22:44
Operator : MA/JU
Sample : 03472-23
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A46R4

Manual IntegrationsAPPROVED

Quant Time: Jul 20 00:12:17 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jul 19 14:47:57 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/20/2023
Supervised By :mohammad ahmed 07/20/2023

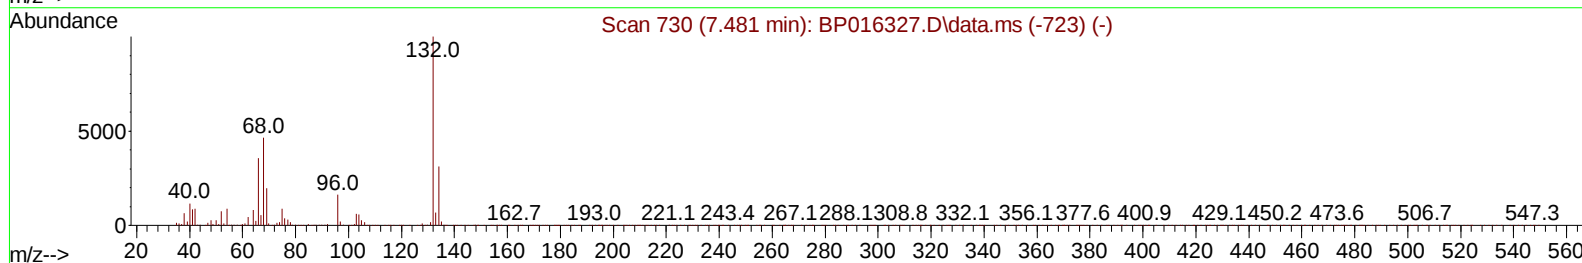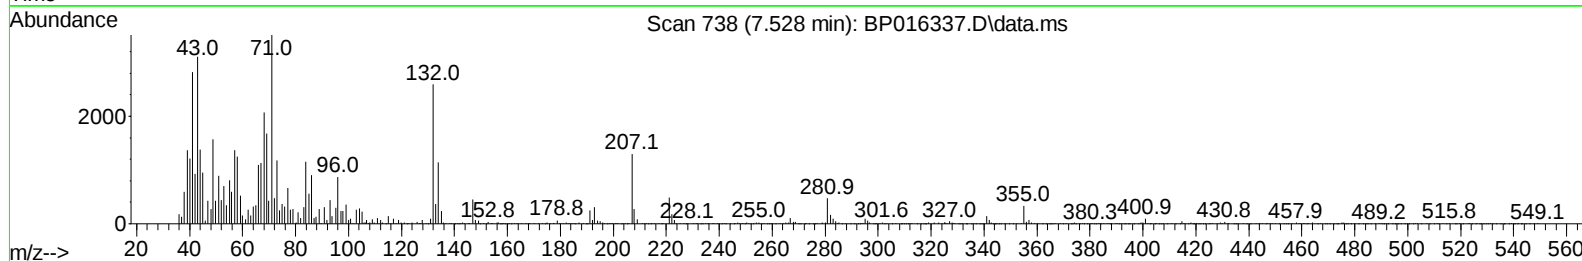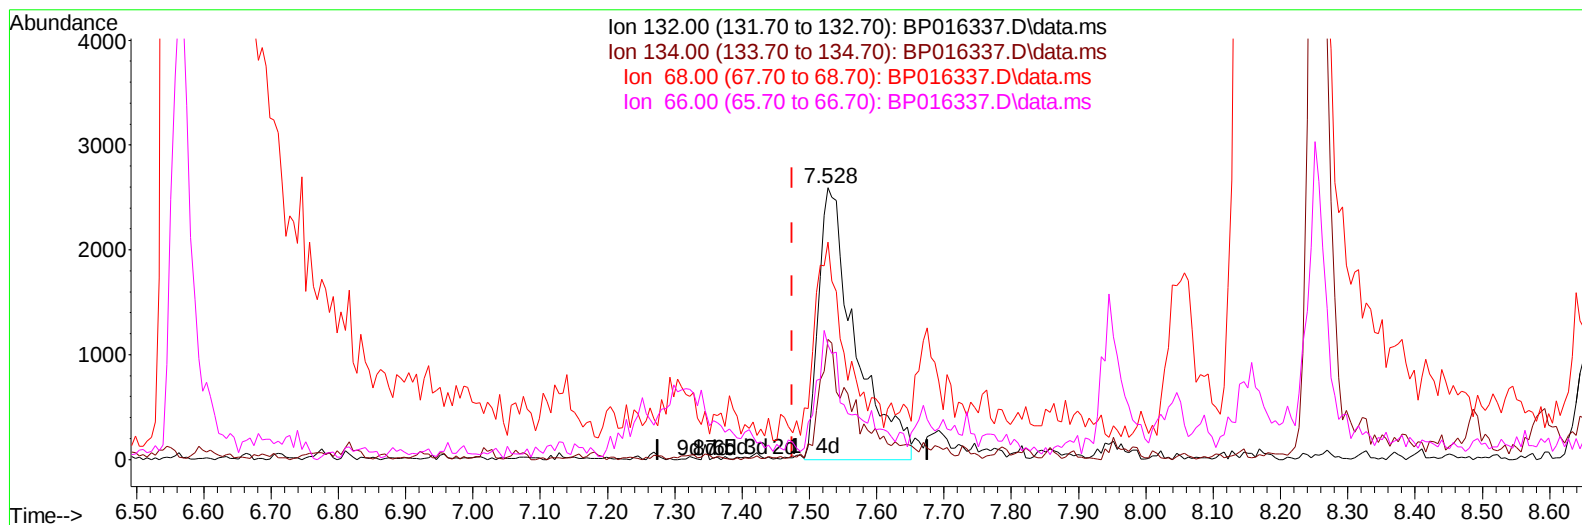

TIC: BP016337.D\data.ms

(11) 2-Chlorophenol-d4 (S)

7.528min (+ 0.053) 1.38 ng/u1 m

response 9740

Ion	Exp%	Act%
132.00	100.00	100.00
134.00	31.50	44.15#
68.00	47.30	80.01#
66.00	33.60	42.07#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071923\
 Data File : BP016337.D
 Acq On : 19 Jul 2023 22:44
 Operator : MA/JU
 Sample : 03472-23
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A46R4

Manual IntegrationsAPPROVED

Quant Time: Jul 20 00:12:17 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jul 19 14:47:57 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/20/2023
 Supervised By :mohammad ahmed 07/20/2023

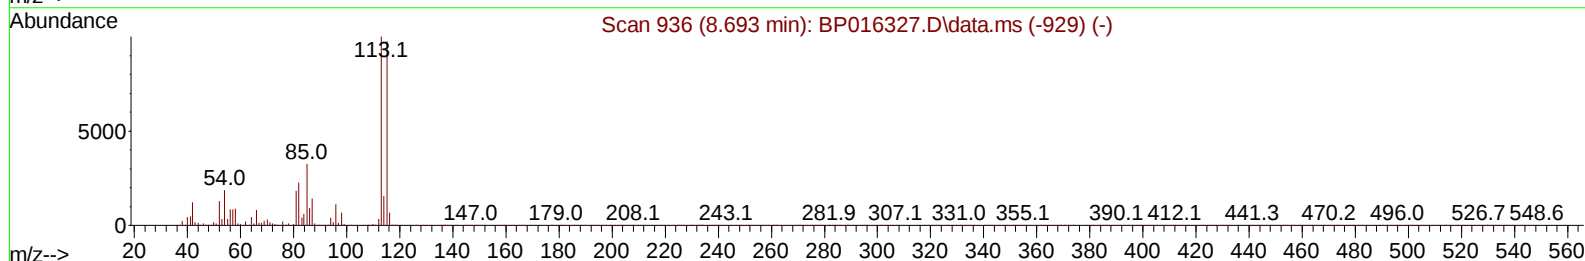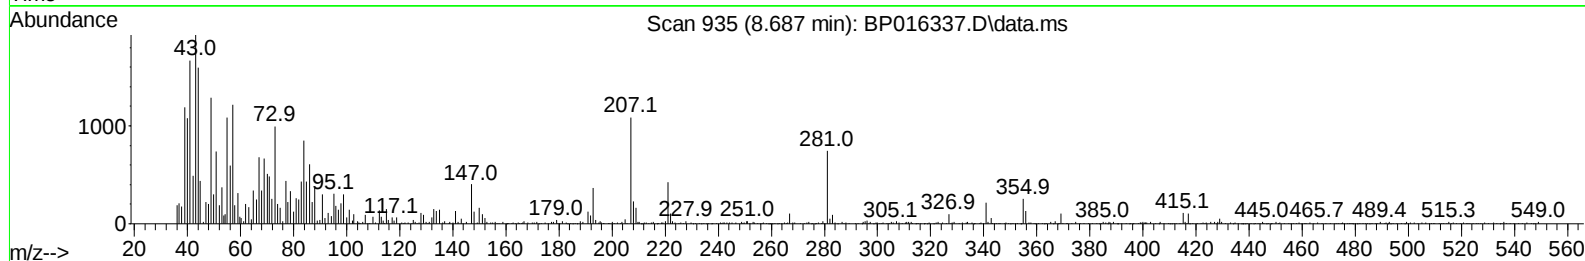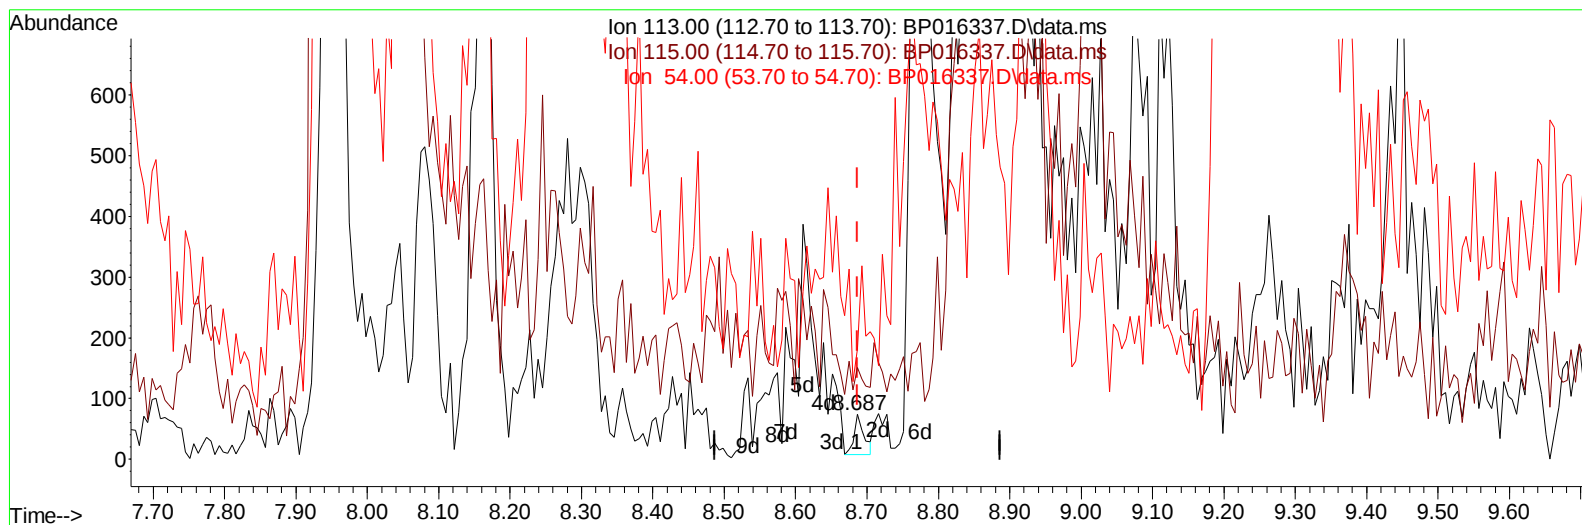

TIC: BP016337.D\data.ms

(15) 4-Methylphenol-d8 (S)

8.687min (-0.000) 0.01 ng/u1

response 62

Ion	Exp%	Act%
113.00	100.00	100.00
115.00	90.20	175.93#
54.00	16.30	168.52#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071923\
Data File : BP016337.D
Acq On : 19 Jul 2023 22:44
Operator : MA/JU
Sample : 03472-23
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A46R4

Manual IntegrationsAPPROVED

Quant Time: Jul 20 00:12:17 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jul 19 14:47:57 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/20/2023
Supervised By :mohammad ahmed 07/20/2023

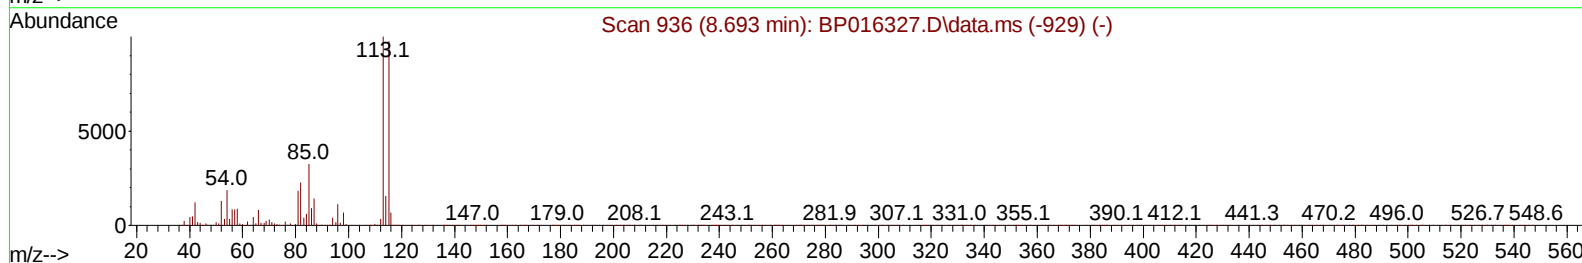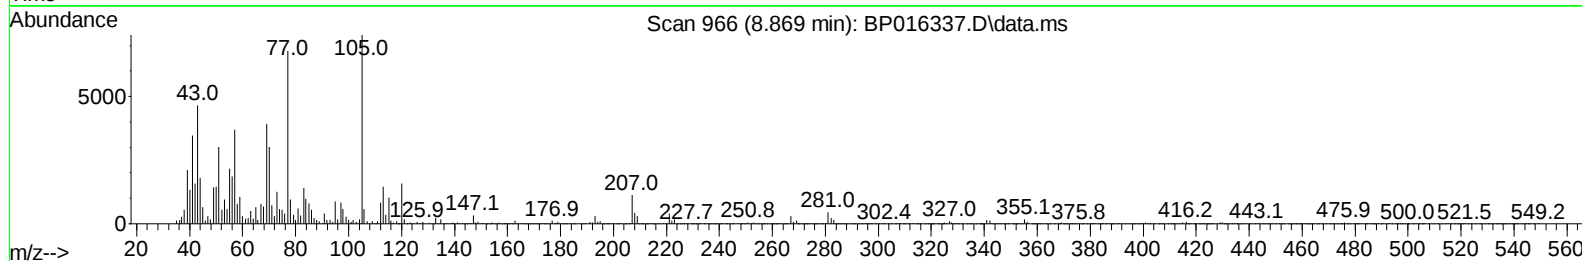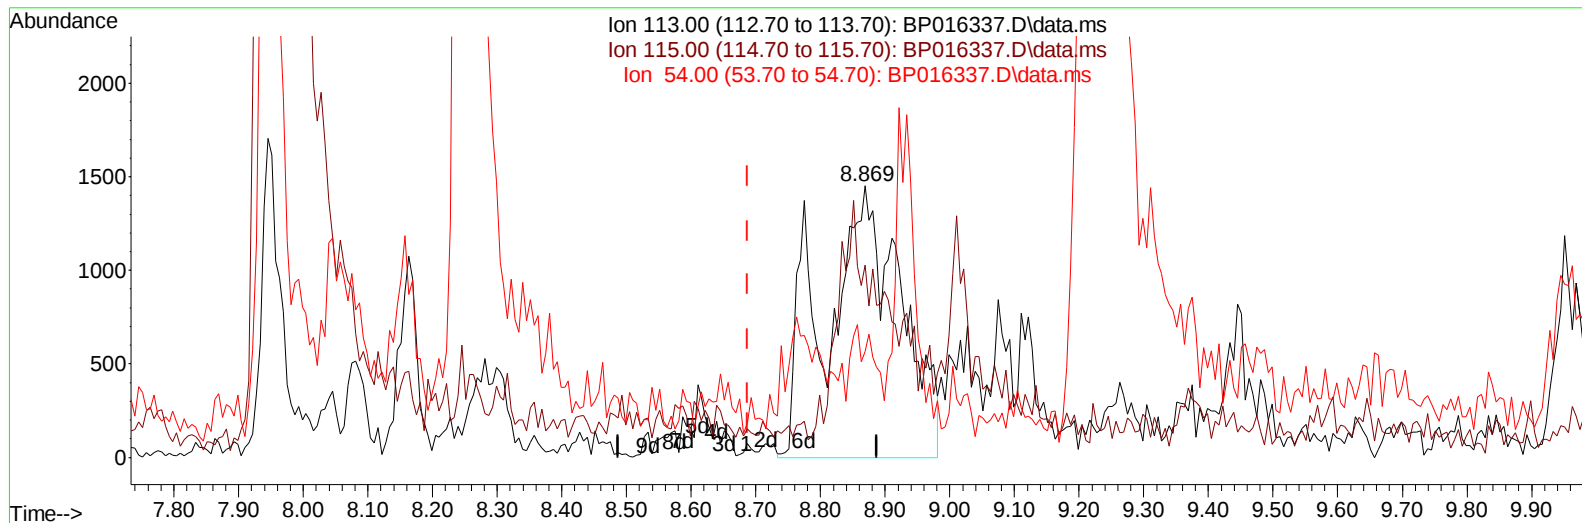

TIC: BP016337.D\data.ms

(15) 4-Methylphenol-d8 (S)

8.869min (+ 0.182) 1.49 ng/ul m

response 11763

Ion	Exp%	Act%
113.00	100.00	100.00
115.00	90.20	70.78#
54.00	16.30	39.15#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071923\
 Data File : BP016337.D
 Acq On : 19 Jul 2023 22:44
 Operator : MA/JU
 Sample : 03472-23
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A46R4

Manual IntegrationsAPPROVED

Quant Time: Jul 20 00:12:17 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jul 19 14:47:57 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/20/2023
 Supervised By :mohammad ahmed 07/20/2023

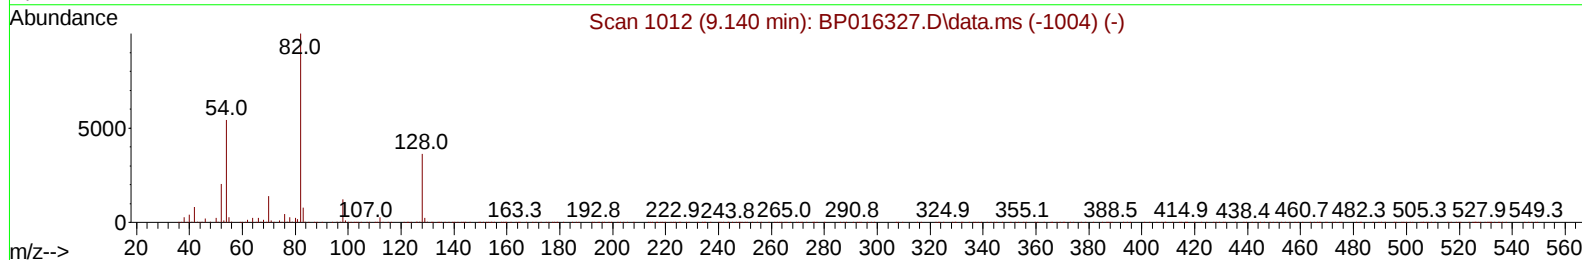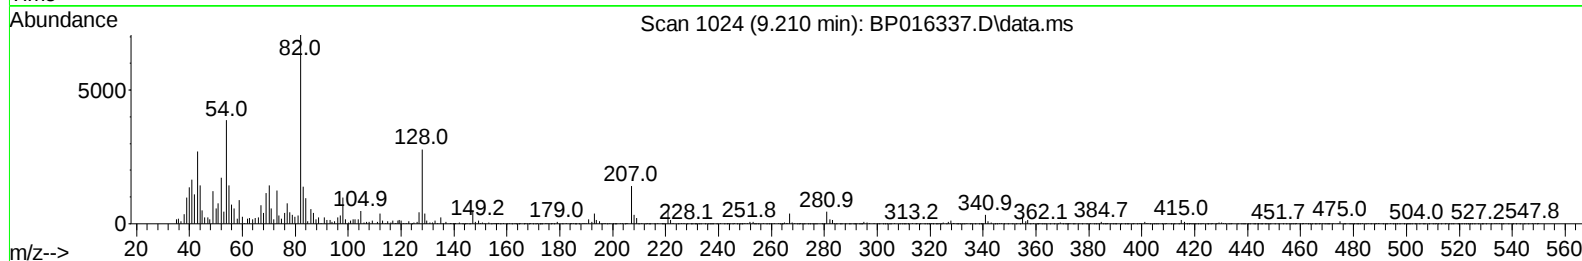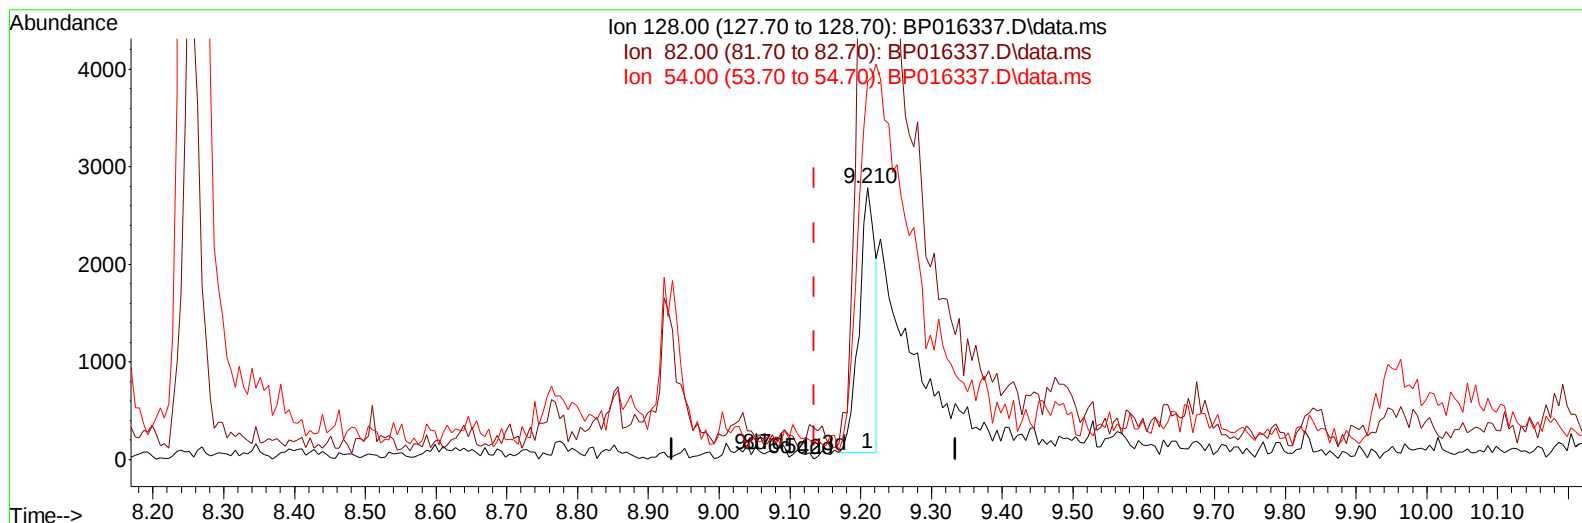

TIC: BP016337.D\data.ms

(21) Nitrobenzene-d5 (S)

9.210min (+ 0.076) 1.24 ng/u1

response 4317

Ion	Exp%	Act%
128.00	100.00	100.00
82.00	261.40	253.79
54.00	136.80	139.24
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071923\
Data File : BP016337.D
Acq On : 19 Jul 2023 22:44
Operator : MA/JU
Sample : 03472-23
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A46R4

Manual IntegrationsAPPROVED

Quant Time: Jul 20 00:12:17 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jul 19 14:47:57 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/20/2023
Supervised By :mohammad ahmed 07/20/2023

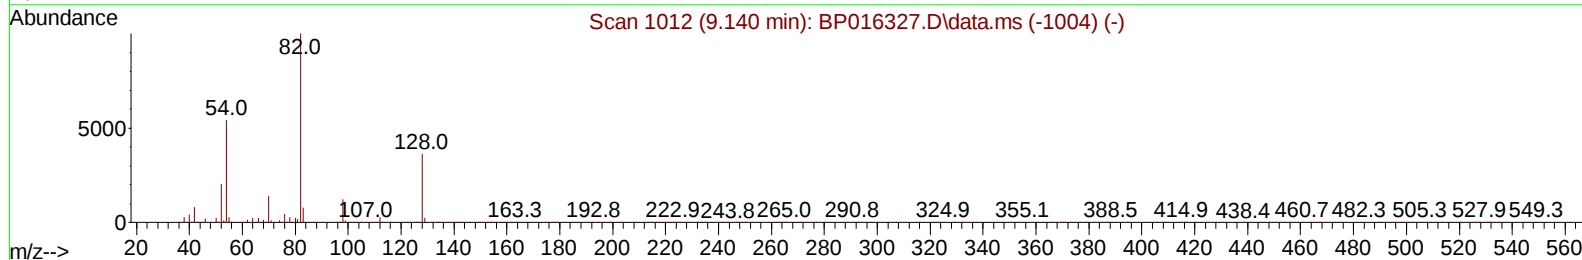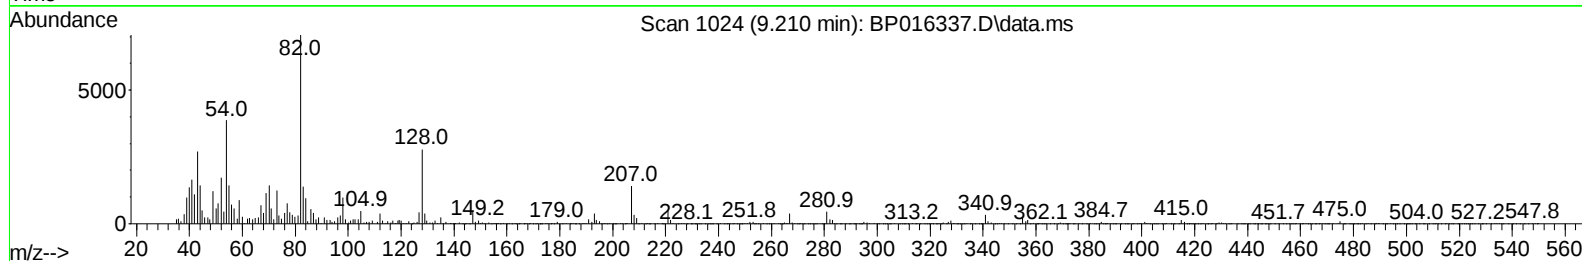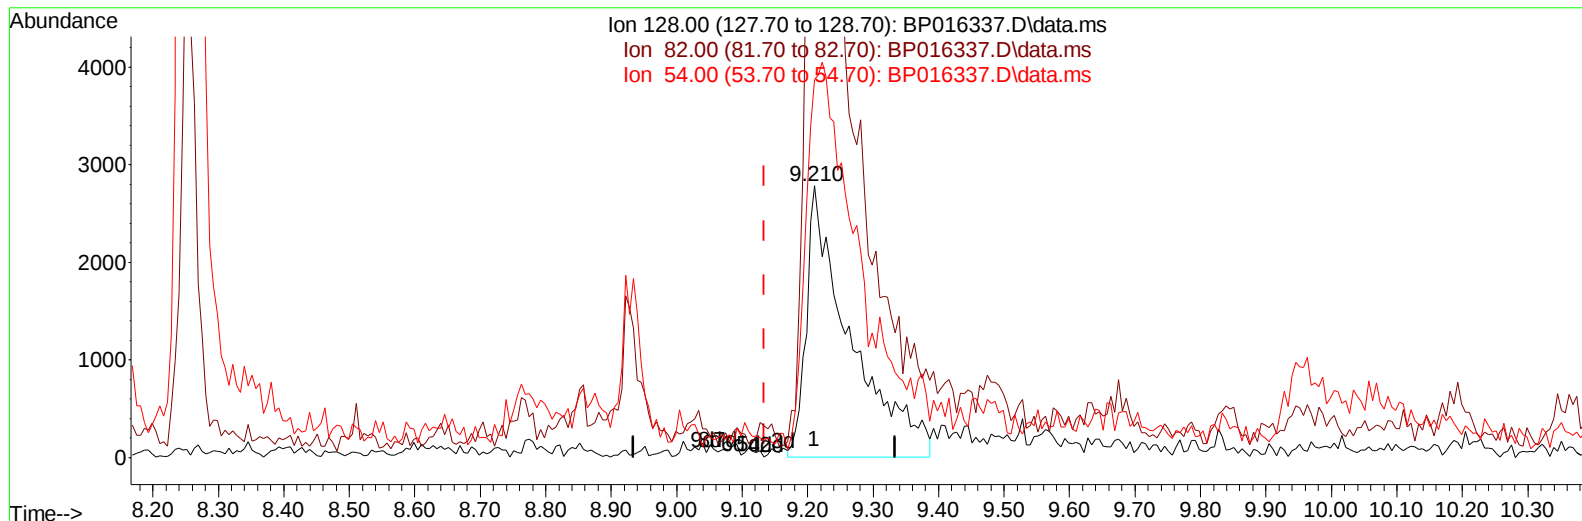

TIC: BP016337.D\data.ms

(21) Nitrobenzene-d5 (S)

9.210min (+ 0.076) 3.70 ng/u1 m

response 12892

Ion	Exp%	Act%
128.00	100.00	100.00
82.00	261.40	253.79
54.00	136.80	139.24
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071923\
Data File : BP016337.D
Acq On : 19 Jul 2023 22:44
Operator : MA/JU
Sample : 03472-23
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A46R4

Manual IntegrationsAPPROVED

Quant Time: Jul 20 00:12:17 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jul 19 14:47:57 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/20/2023
Supervised By :mohammad ahmed 07/20/2023

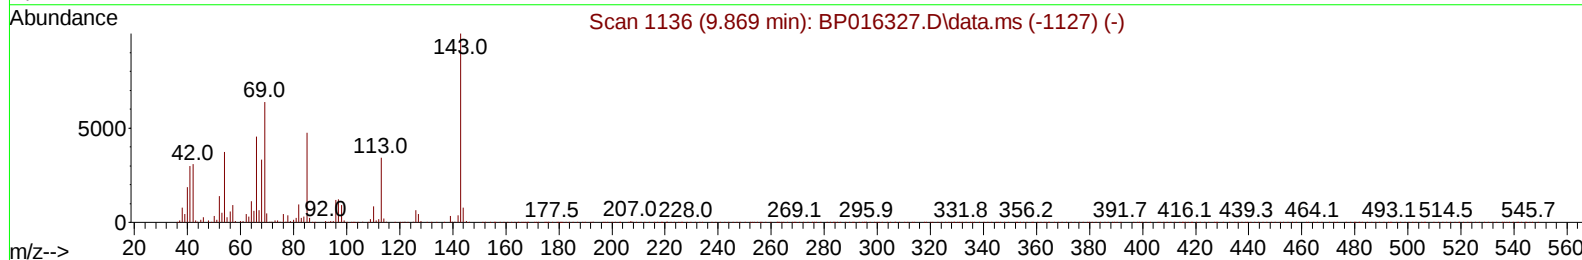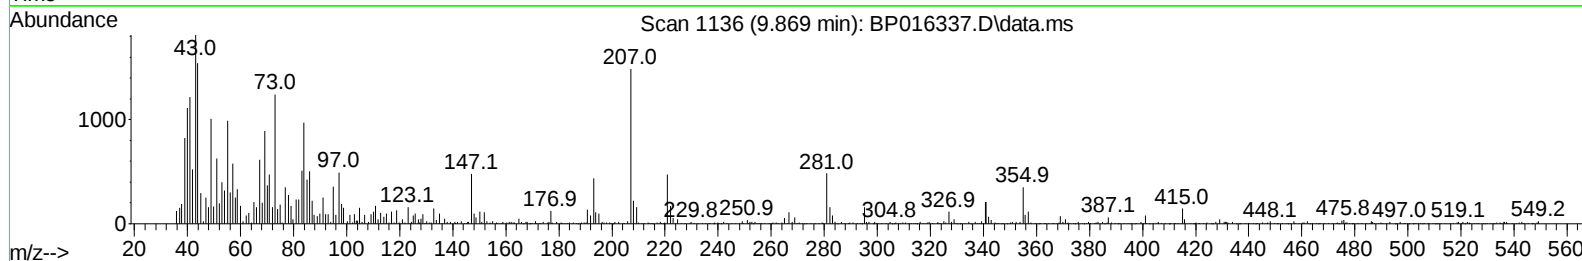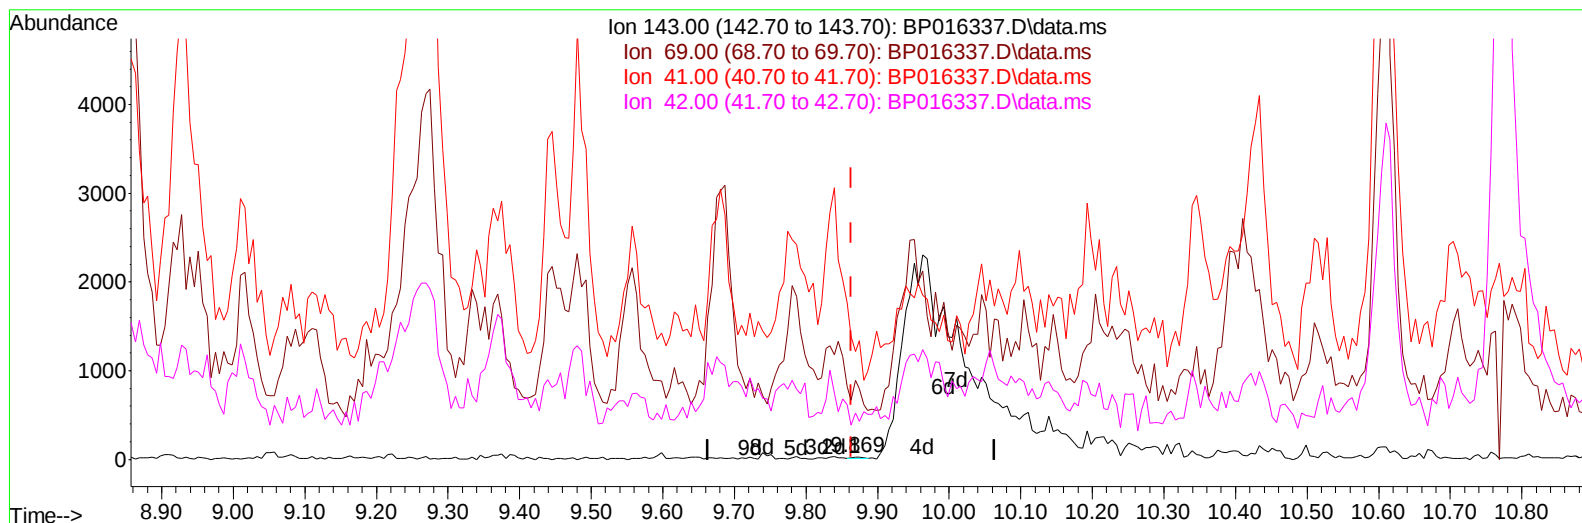

TIC: BP016337.D\data.ms

(24) 2-Nitrophenol-d4 (S)

9.869min (+ 0.006) 0.00 ng/u1

response 8

Ion	Exp%	Act%
143.00	100.00	100.00
69.00	62.00	3415.38#
41.00	28.60	4676.92#
42.00	29.20	2015.38#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071923\
 Data File : BP016337.D
 Acq On : 19 Jul 2023 22:44
 Operator : MA/JU
 Sample : 03472-23
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A46R4

Manual IntegrationsAPPROVED

Quant Time: Jul 20 00:12:17 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jul 19 14:47:57 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/20/2023
 Supervised By :mohammad ahmed 07/20/2023

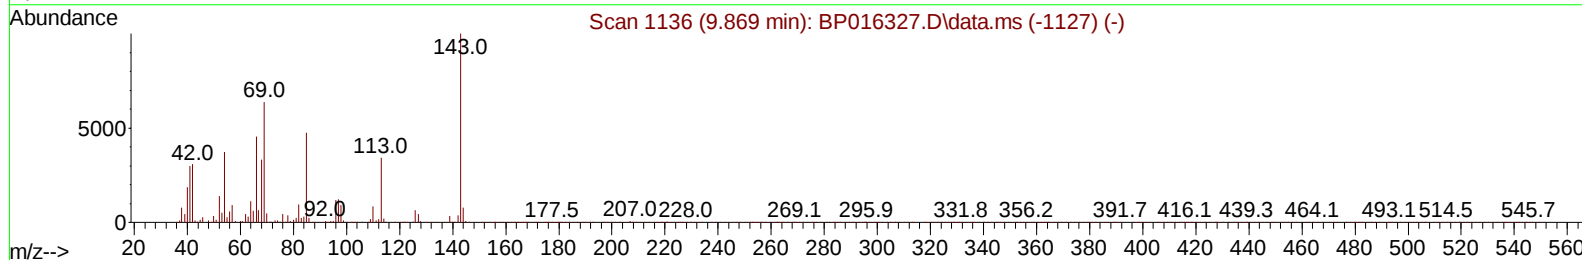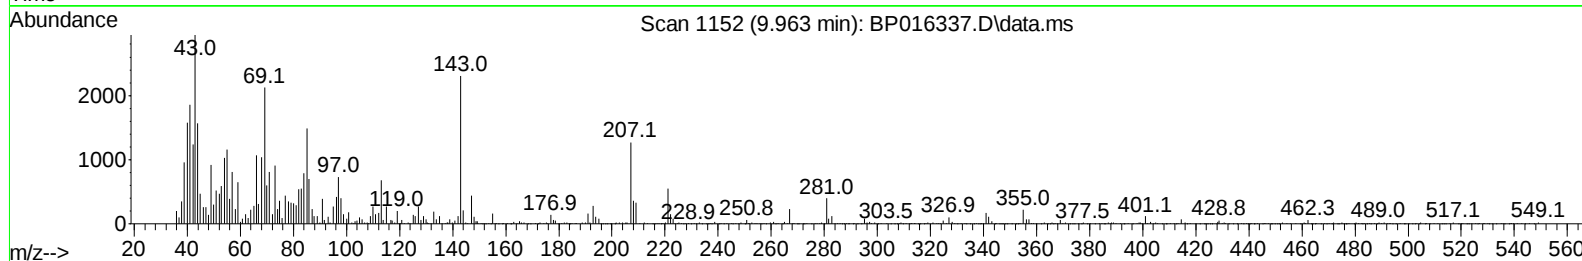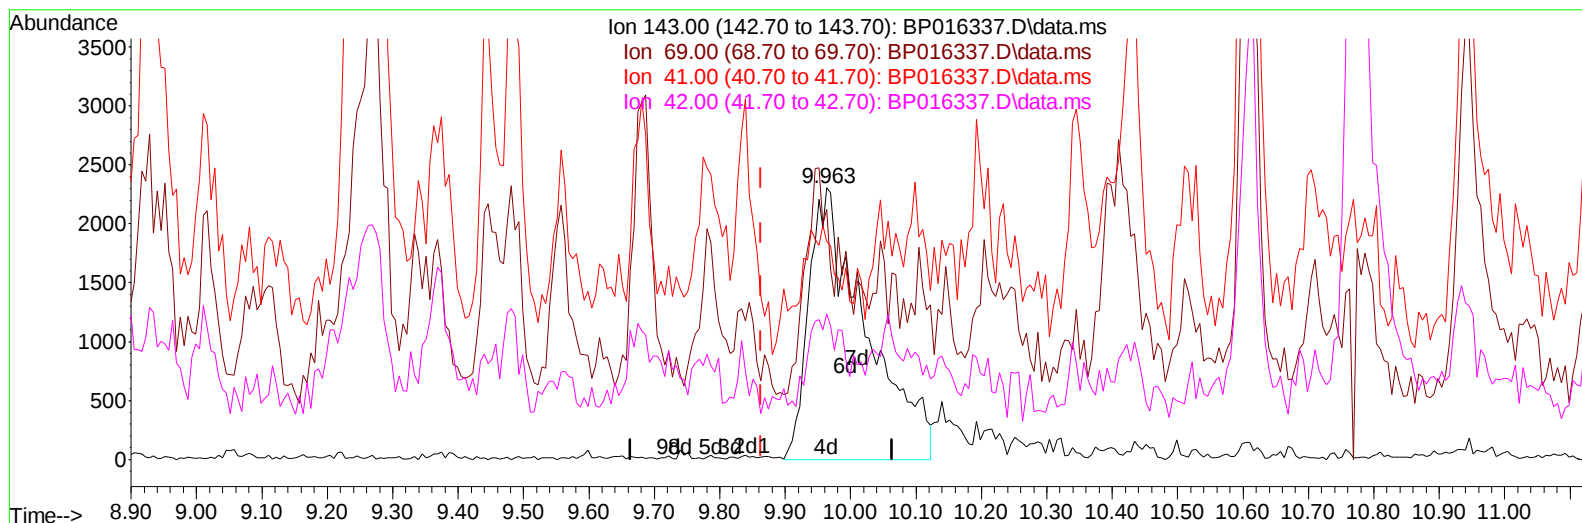

TIC: BP016337.D\data.ms

(24) 2-Nitrophenol-d4 (S)

9.963min (+ 0.100) 3.50 ng/u1 m

response 13934

Ion	Exp%	Act%
143.00	100.00	100.00
69.00	62.00	92.06#
41.00	28.60	80.39#
42.00	29.20	53.75#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071923\
 Data File : BP016337.D
 Acq On : 19 Jul 2023 22:44
 Operator : MA/JU
 Sample : 03472-23
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A46R4

Manual IntegrationsAPPROVED

Quant Time: Jul 20 00:12:17 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jul 19 14:47:57 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/20/2023
 Supervised By :mohammad ahmed 07/20/2023

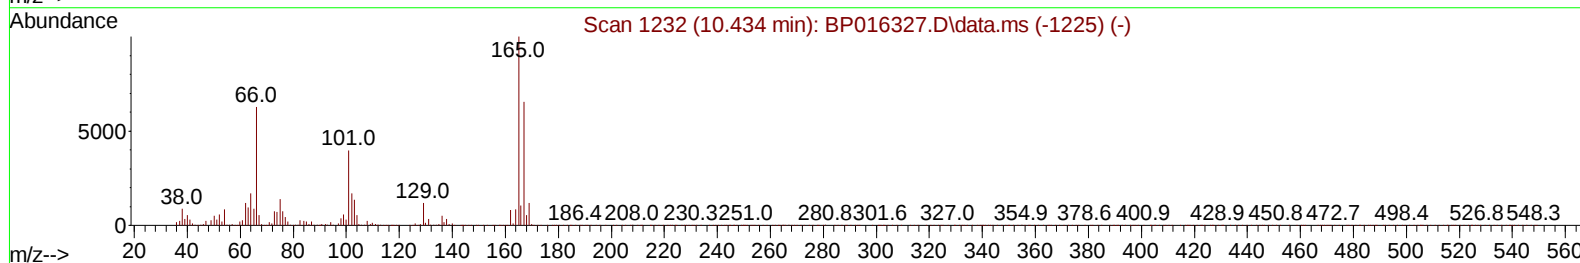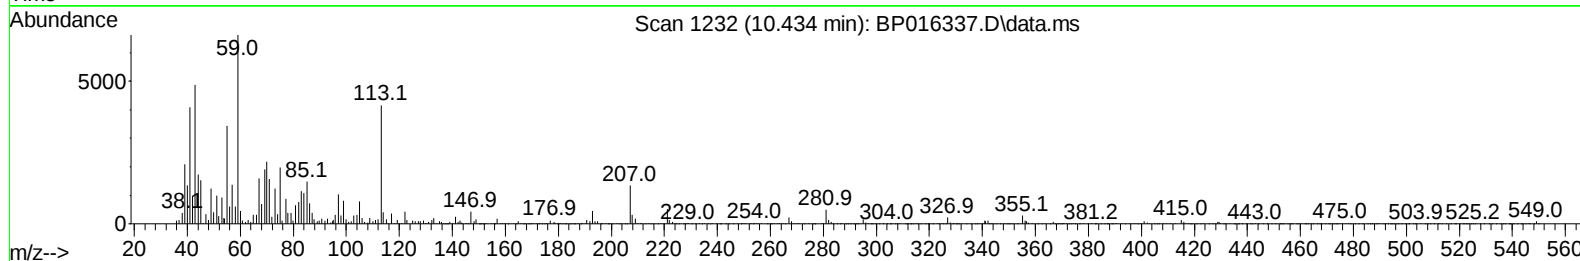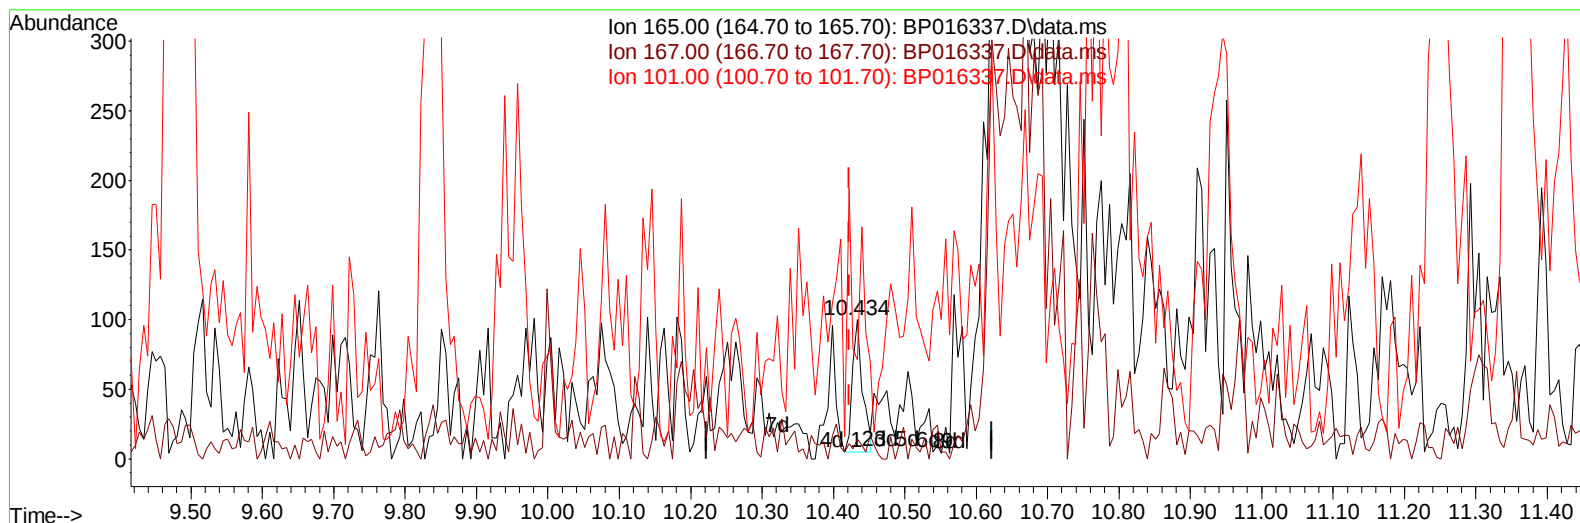

TIC: BP016337.D\data.ms

(28) 2,4-Dichlorophenol-d3 (S)

10.434min (+ 0.011) 0.01 ng/ul

response 91

Ion	Exp%	Act%
165.00	100.00	100.00
167.00	65.20	11.57#
101.00	38.50	58.68#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071923\
 Data File : BP016337.D
 Acq On : 19 Jul 2023 22:44
 Operator : MA/JU
 Sample : 03472-23
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A46R4

Manual IntegrationsAPPROVED

Quant Time: Jul 20 00:20:07 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jul 19 14:47:57 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/20/2023
 Supervised By :mohammad ahmed 07/20/2023

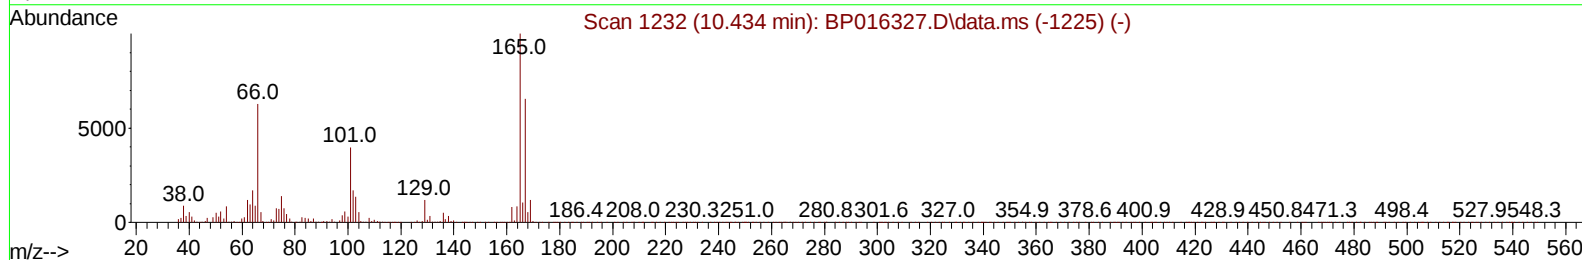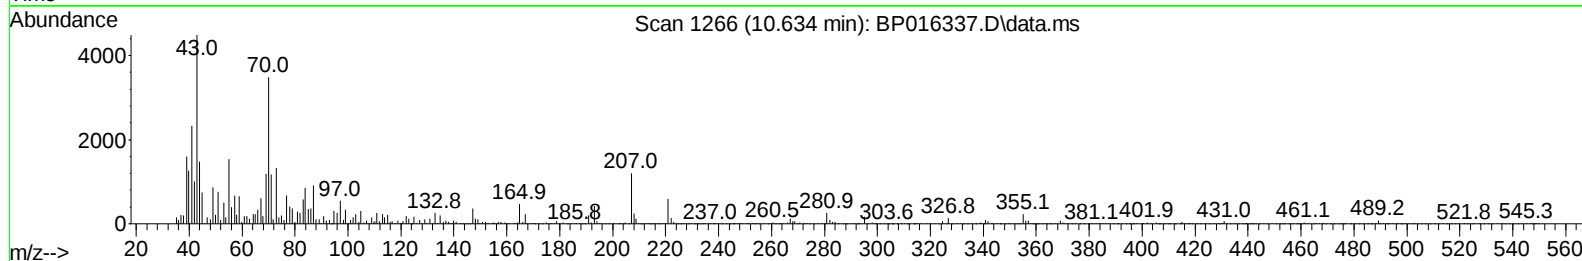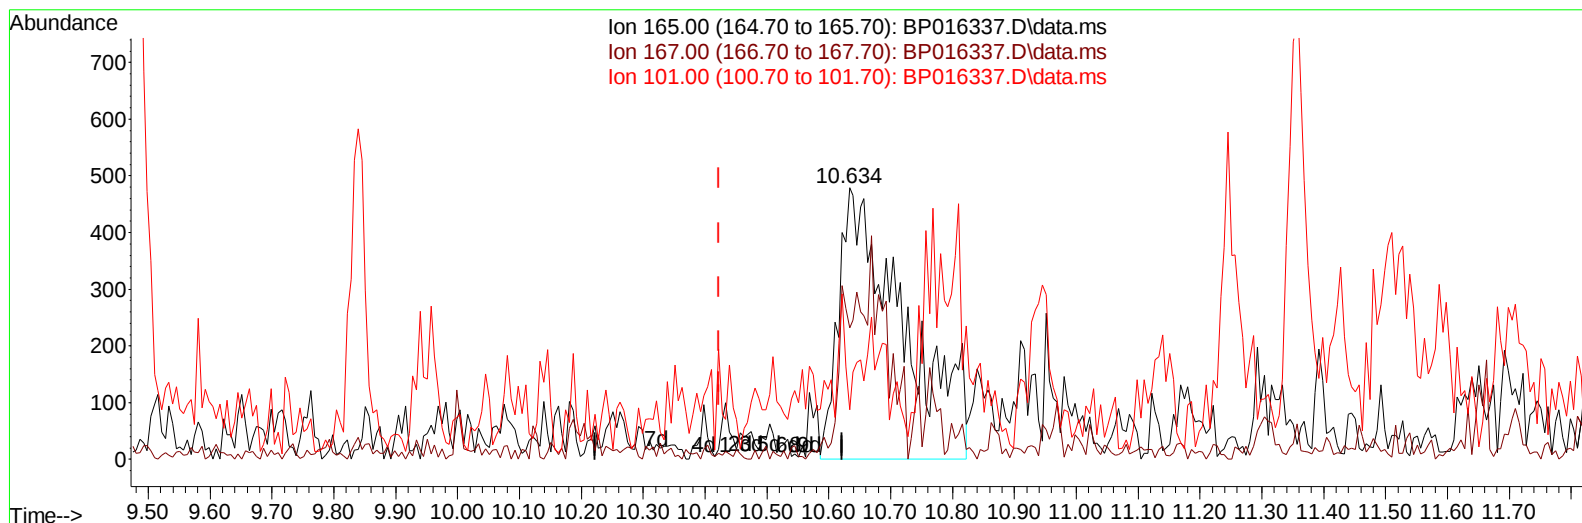

TIC: BP016337.D\data.ms

(28) 2,4-Dichlorophenol-d3 (S)

10.634min (+ 0.211) 0.50 ng/ul m

response 3418

Ion	Exp%	Act%
165.00	100.00	100.00
167.00	65.20	48.43#
101.00	38.50	18.37#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071923\
Data File : BP016337.D
Acq On : 19 Jul 2023 22:44
Operator : MA/JU
Sample : 03472-23
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A46R4

Manual IntegrationsAPPROVED

Quant Time: Jul 20 00:20:36 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jul 19 14:47:57 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/20/2023
Supervised By :mohammad ahmed 07/20/2023

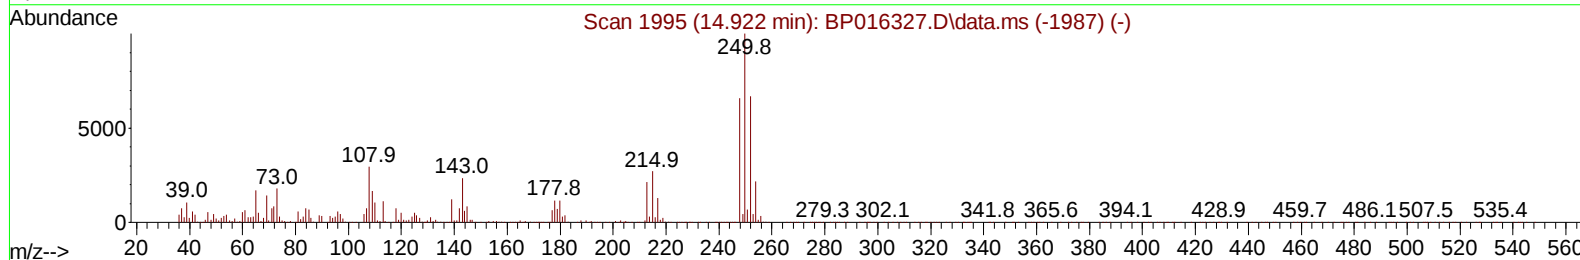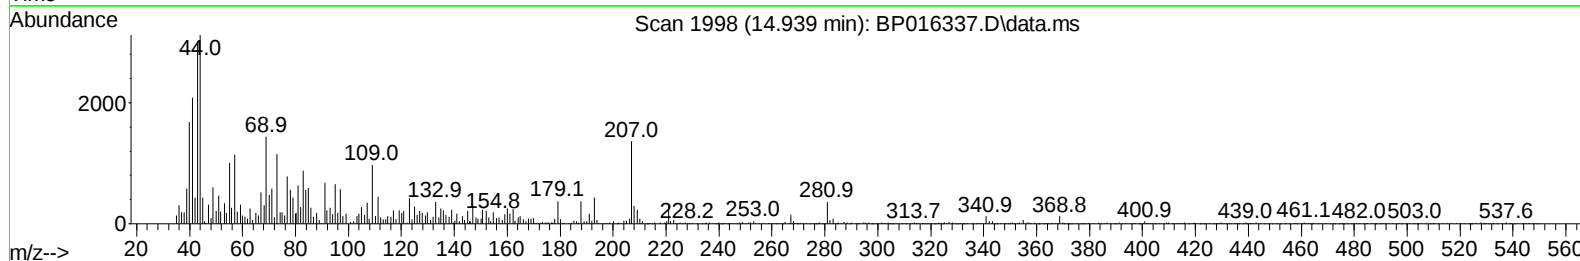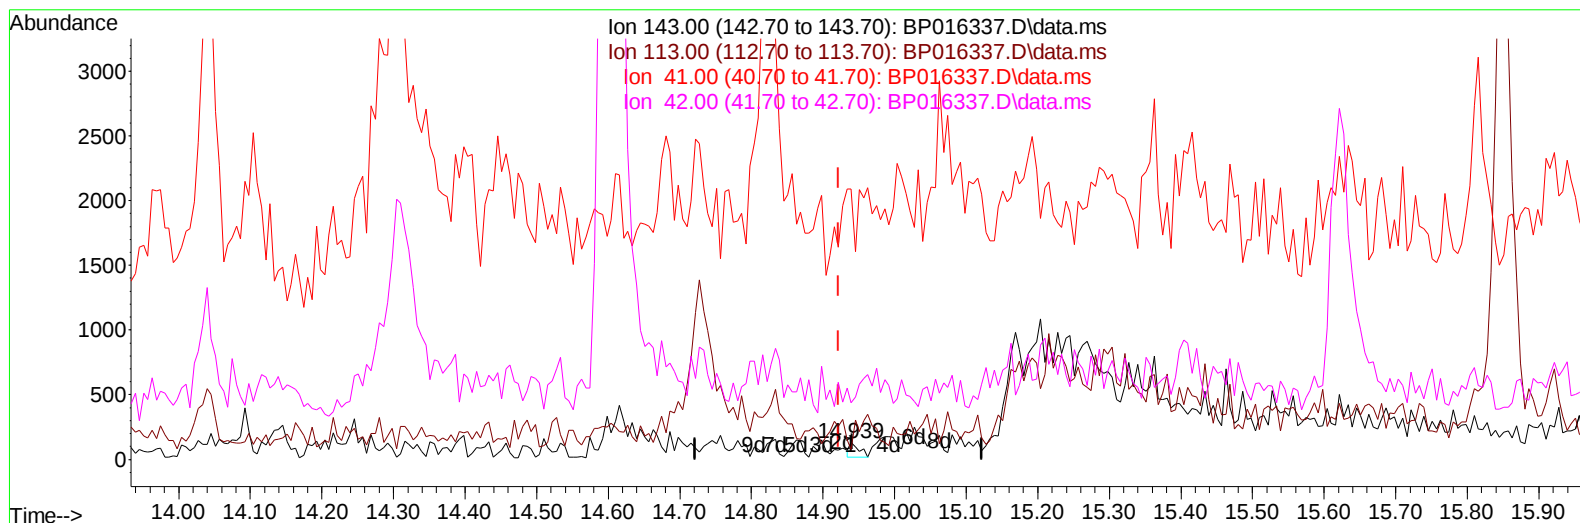

TIC: BP016337.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.939min (+ 0.017) 0.01 ng/u1

response 103

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	79.50	58.78#
41.00	49.30	1593.89#
42.00	32.70	334.35#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071923\
Data File : BP016337.D
Acq On : 19 Jul 2023 22:44
Operator : MA/JU
Sample : 03472-23
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A46R4

Manual IntegrationsAPPROVED

Quant Time: Jul 20 00:20:36 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jul 19 14:47:57 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/20/2023
Supervised By :mohammad ahmed 07/20/2023

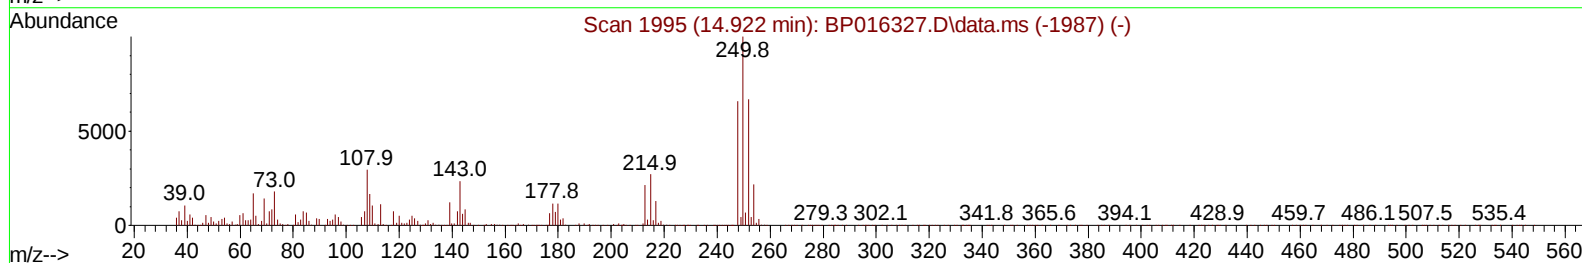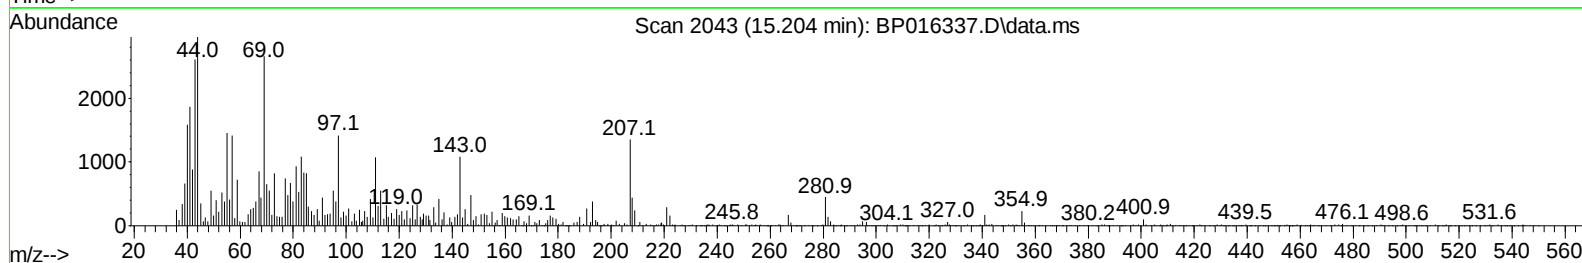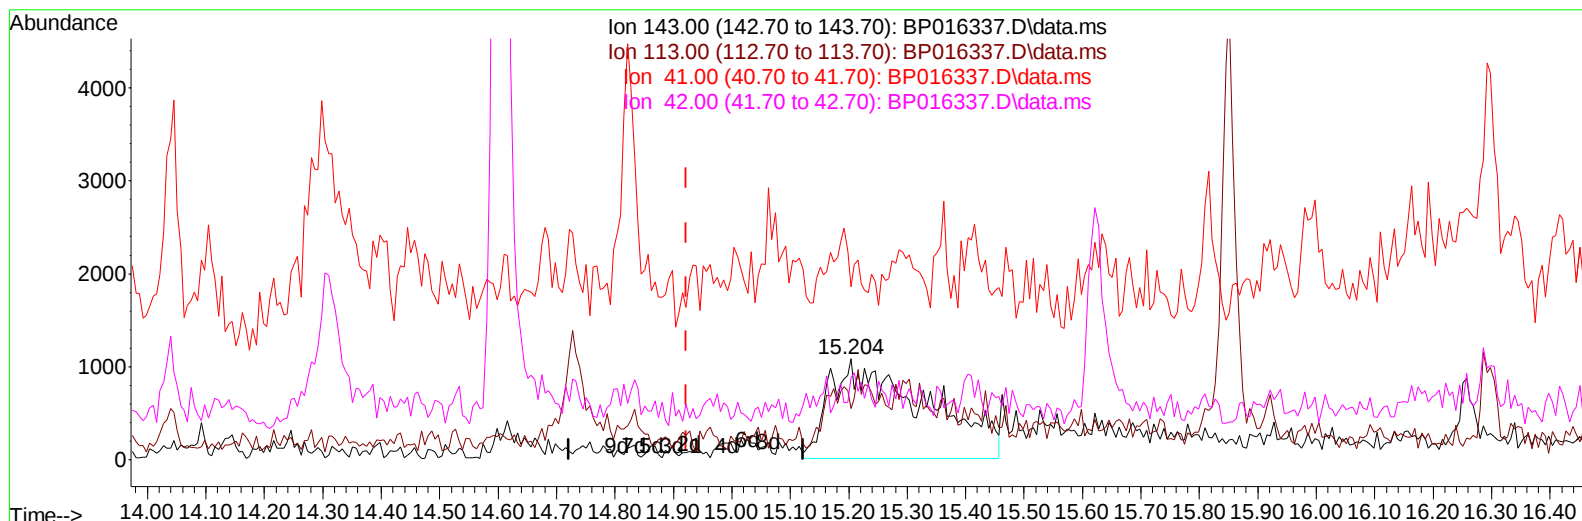

TIC: BP016337.D\data.ms

(54) 4-Nitrophenol-d4 (S)

15.204min (+ 0.282) 1.66 ng/ul m

response 11934

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	79.50	50.46#
41.00	49.30	171.36#
42.00	32.70	81.22#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071923\
 Data File : BP016337.D
 Acq On : 19 Jul 2023 22:44
 Operator : MA/JU
 Sample : 03472-23
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A46R4

Manual IntegrationsAPPROVED

Quant Time: Jul 20 00:20:36 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jul 19 14:47:57 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/20/2023
 Supervised By :mohammad ahmed 07/20/2023

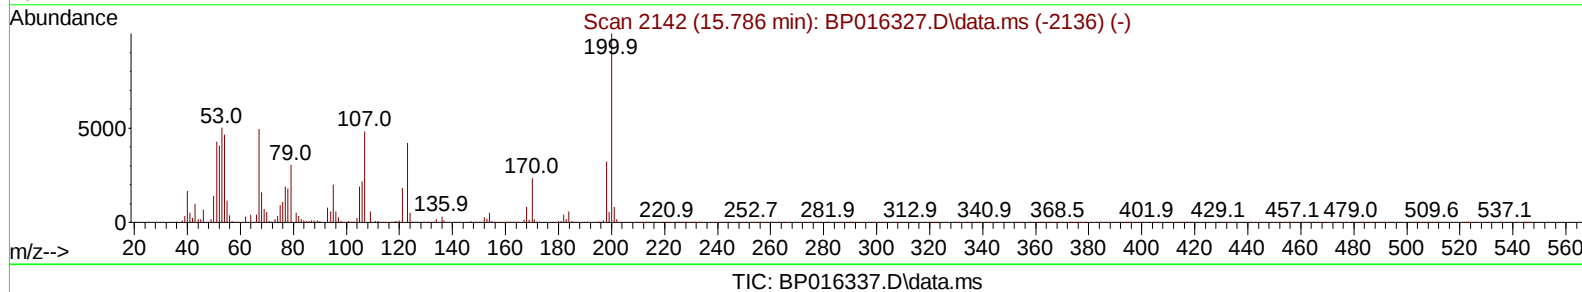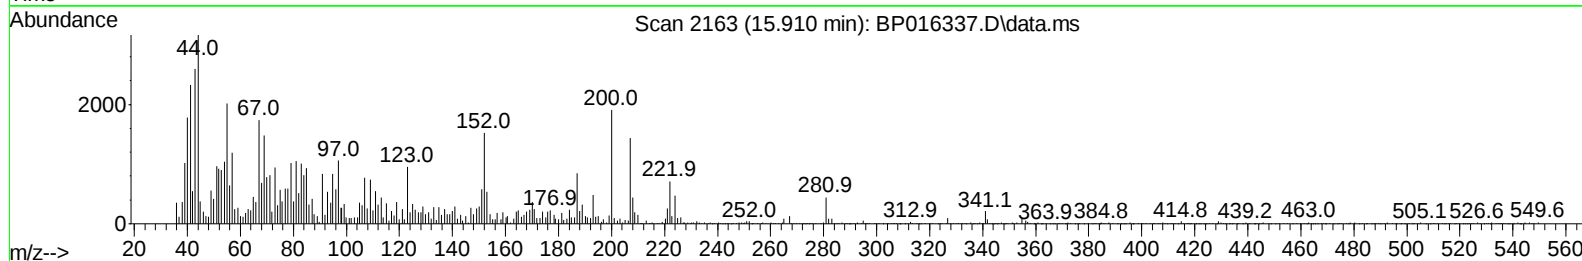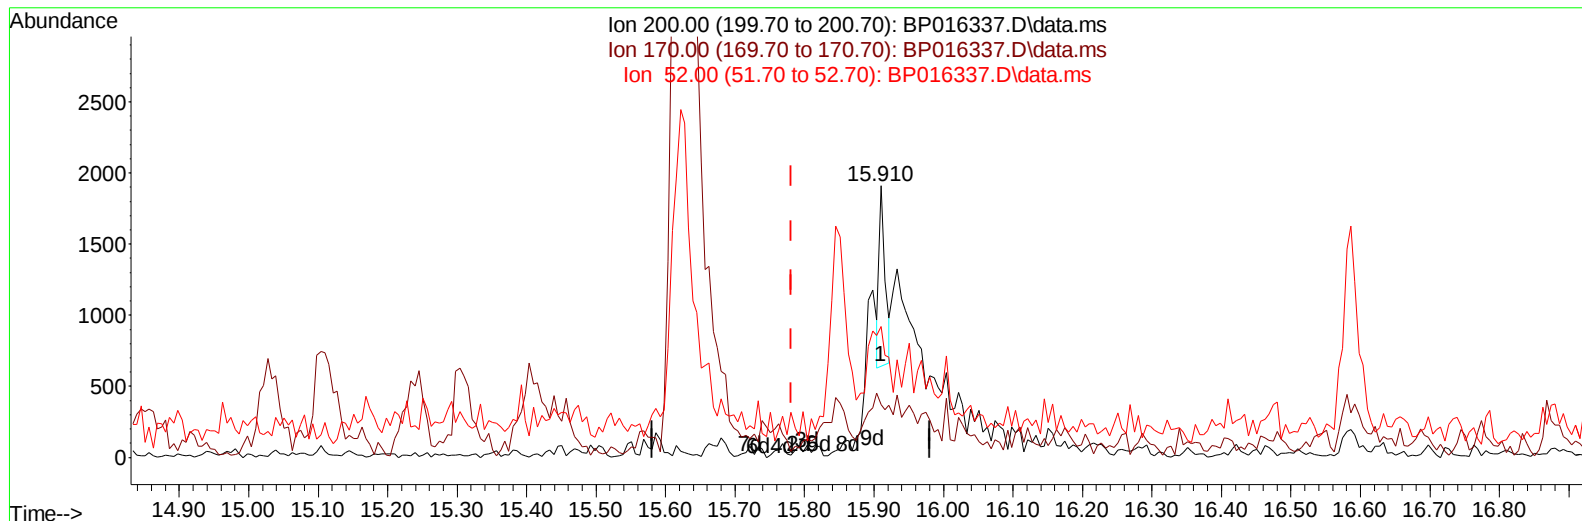

(65) 4,6-Dinitro-2-methylphenol-d2 (S)

15.910min (+ 0.129) 0.13 ng/u1

response 774

Ion	Exp%	Act%
200.00	100.00	100.00
170.00	21.90	19.38
52.00	58.00	48.19
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071923\
Data File : BP016337.D
Acq On : 19 Jul 2023 22:44
Operator : MA/JU
Sample : 03472-23
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A46R4

Manual IntegrationsAPPROVED

Quant Time: Jul 20 00:20:36 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jul 19 14:47:57 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/20/2023
Supervised By :mohammad ahmed 07/20/2023

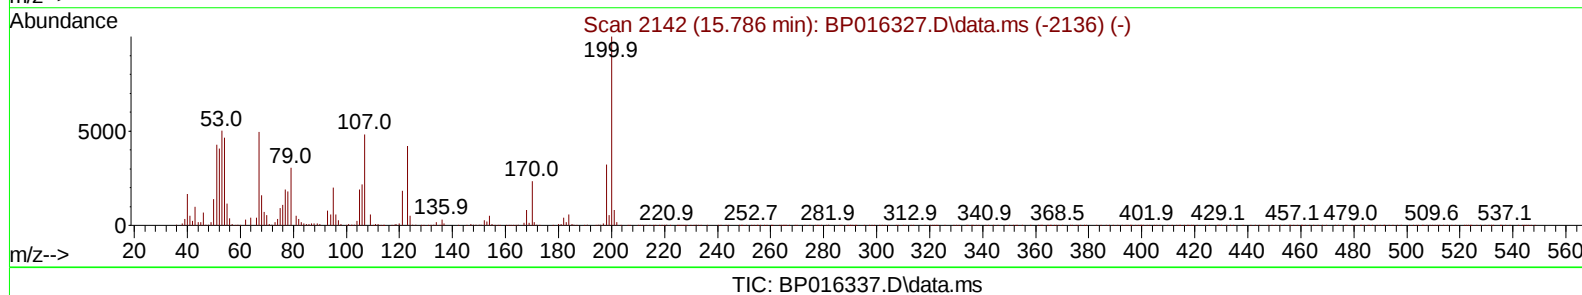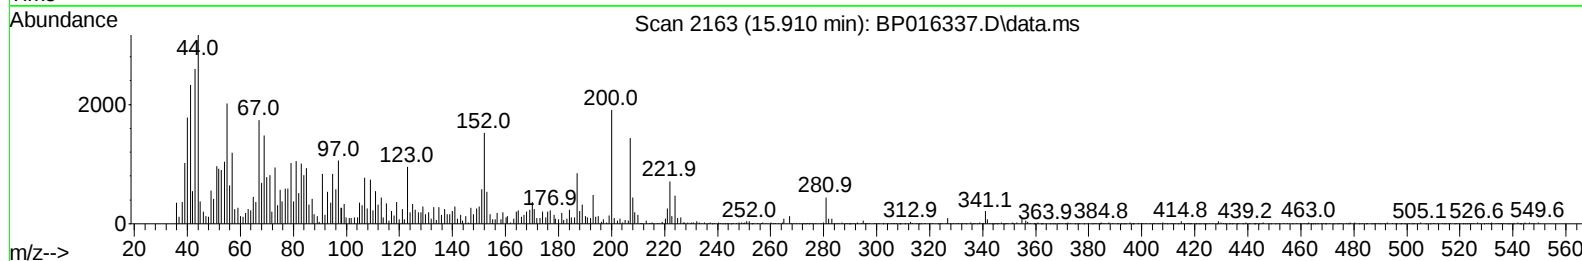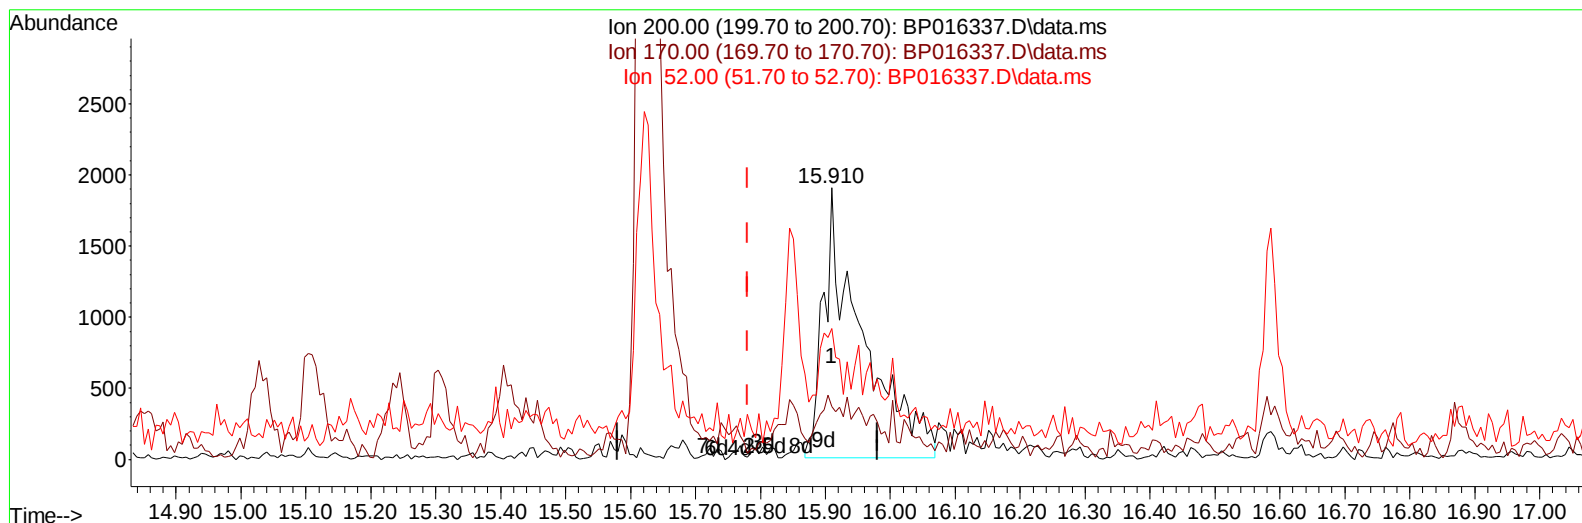

(65) 4,6-Dinitro-2-methylphenol-d2 (S)

15.910min (+ 0.129) 1.27 ng/ul m

response 7786

Ion	Exp%	Act%
200.00	100.00	100.00
170.00	21.90	19.38
52.00	58.00	48.19
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071923\
 Data File : BP016337.D
 Acq On : 19 Jul 2023 22:44
 Operator : MA/JU
 Sample : 03472-23
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A46R4

Manual IntegrationsAPPROVED

Quant Time: Jul 20 00:21:45 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jul 19 14:47:57 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/20/2023
 Supervised By :mohammad ahmed 07/20/2023

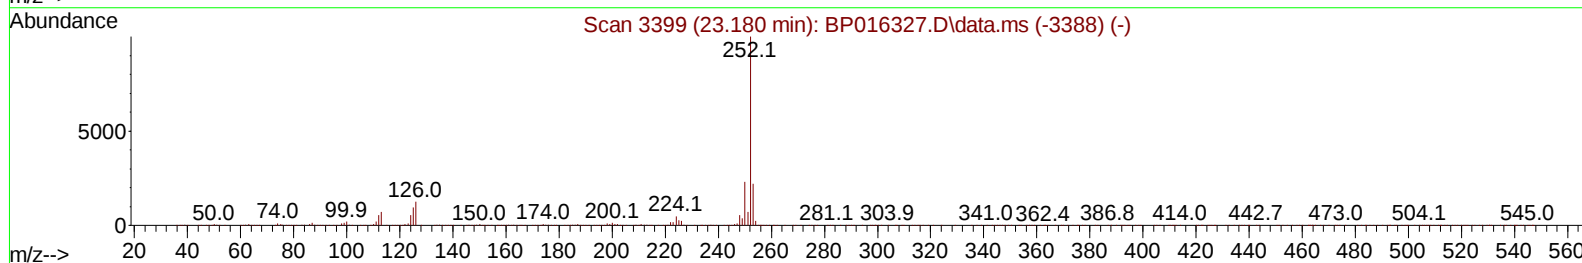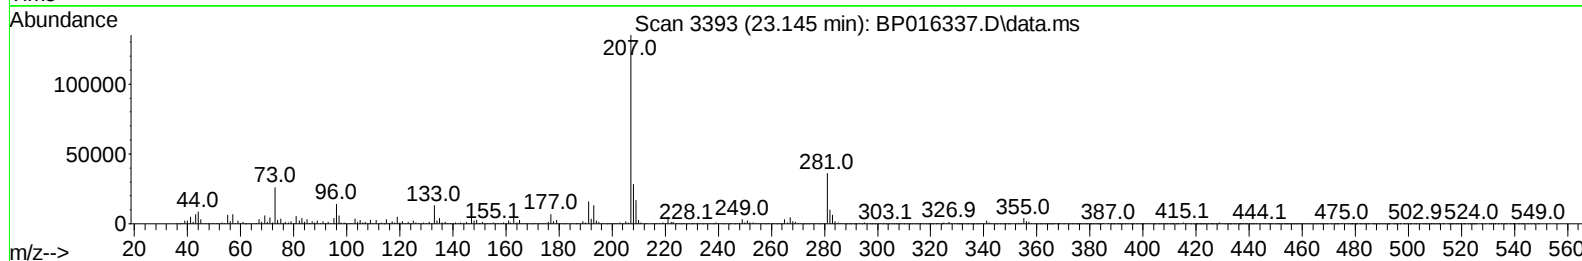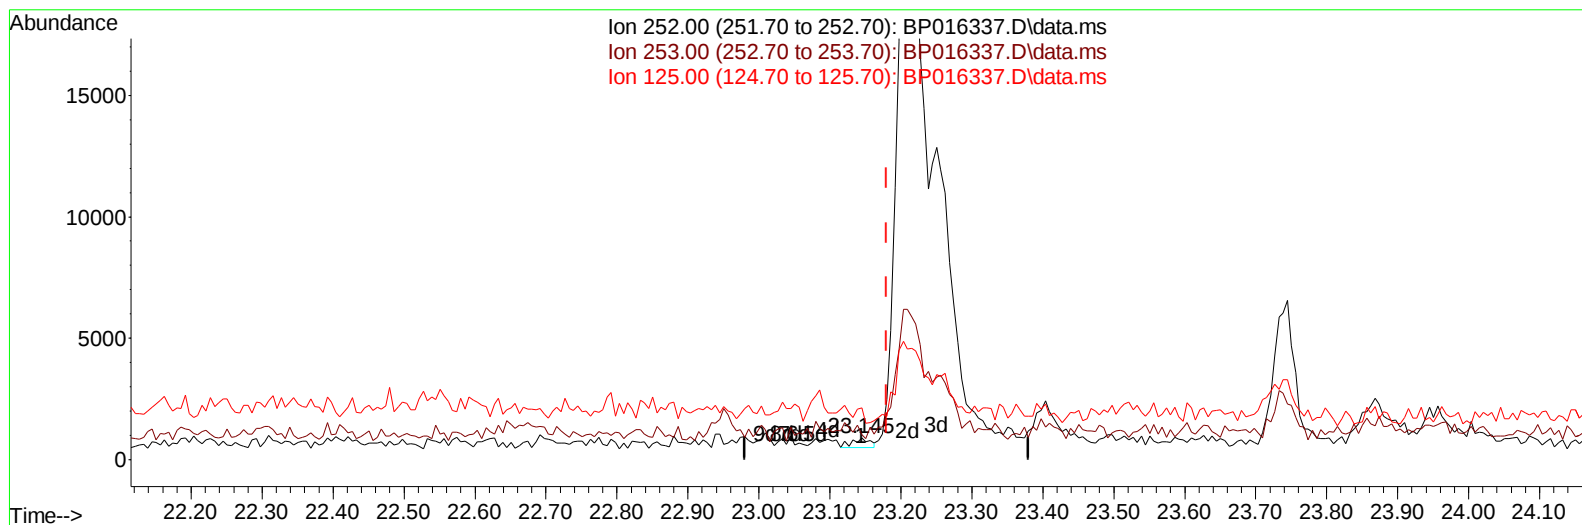

TIC: BP016337.D\data.ms

(90) Benzo(b)fluoranthene

23.145min (-0.036) 0.01 ng/u1

response 695

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	21.60	113.37#
125.00	11.70	238.54#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071923\
 Data File : BP016337.D
 Acq On : 19 Jul 2023 22:44
 Operator : MA/JU
 Sample : 03472-23
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A46R4

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 07/20/2023
 Supervised By :mohammad ahmed 07/20/2023

Quant Time: Jul 20 00:22:24 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jul 19 14:47:57 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.945	152	108539	20.000	ng/ul	0.00
20) Naphthalene-d8	10.775	136	505716	20.000	ng/ul	0.02
38) Acenaphthene-d10	14.604	164	461169	20.000	ng/ul	0.01
64) Phenanthrene-d10	17.374	188	1062692	20.000	ng/ul	0.01
79) Chrysene-d12	21.462	240	1092527	20.000	ng/ul	0.00
88) Perylene-d12	23.950	264	1057307	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.275	96	3148	1.026	ng/uL	0.00
4) Pyridine-d5	3.704	84	83357m	10.897	ng/ul	-0.02
7) Phenol-d5	7.240	99	6007m	0.613	ng/ul	0.11
9) Bis-(2-Chloroethyl)eth...	7.298	67	26360m	3.976	ng/ul	0.02
11) 2-Chlorophenol-d4	7.528	132	9740m	1.376	ng/ul	0.05
15) 4-Methylphenol-d8	8.869	113	11763m	1.489	ng/ul	0.18
21) Nitrobenzene-d5	9.210	128	12892m	3.695	ng/ul	0.08
24) 2-Nitrophenol-d4	9.963	143	13934m	3.504	ng/ul	0.10
28) 2,4-Dichlorophenol-d3	10.634	165	3418m	0.496	ng/ul	0.21
31) 4-Chloroaniline-d4	10.957	131	96	0.009	ng/ul	0.02
46) Dimethylphthalate-d6	14.039	166	143864	4.090	ng/ul	0.03
49) Acenaphthylene-d8	14.310	160	122952	3.189	ng/ul	0.02
54) 4-Nitrophenol-d4	15.204	143	11934m	1.662	ng/ul	0.28
60) Fluorene-d10	15.621	176	129260	4.390	ng/ul	0.03
65) 4,6-Dinitro-2-methylph...	15.910	200	7786m	1.269	ng/ul	0.13
73) Anthracene-d10	17.504	188	76214	1.640	ng/ul	0.04
81) Pyrene-d10	19.715	212	239624	4.227	ng/ul	0.01
92) Benzo(a)pyrene-d12	23.803	264	39159	0.771	ng/ul	0.02
Target Compounds						
						Qvalue
72) Phenanthrene	17.421	178	58961	1.065	ng/ul	98
80) Fluoranthene	19.392	202	113952	1.719	ng/ul	99
82) Pyrene	19.745	202	85132	1.203	ng/ul	98
86) Bis(2-ethylhexyl)phtha...	21.315	149	100283	2.199	ng/ul	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071923\
Data File : BP016337.D
Acq On : 19 Jul 2023 22:44
Operator : MA/JU
Sample : 03472-23
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A46R4

Manual IntegrationsAPPROVED

Quant Time: Jul 20 00:22:24 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jul 19 14:47:57 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/20/2023
Supervised By :mohammad ahmed 07/20/2023

