




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071923\
 Data File : BP016338.D
 Acq On : 19 Jul 2023 23:17
 Operator : MA/JU
 Sample : 03472-24
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A46R5

Manual IntegrationsAPPROVED

Quant Time: Jul 20 00:12:34 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jul 19 14:47:57 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/20/2023
 Supervised By :mohammad ahmed 07/20/2023

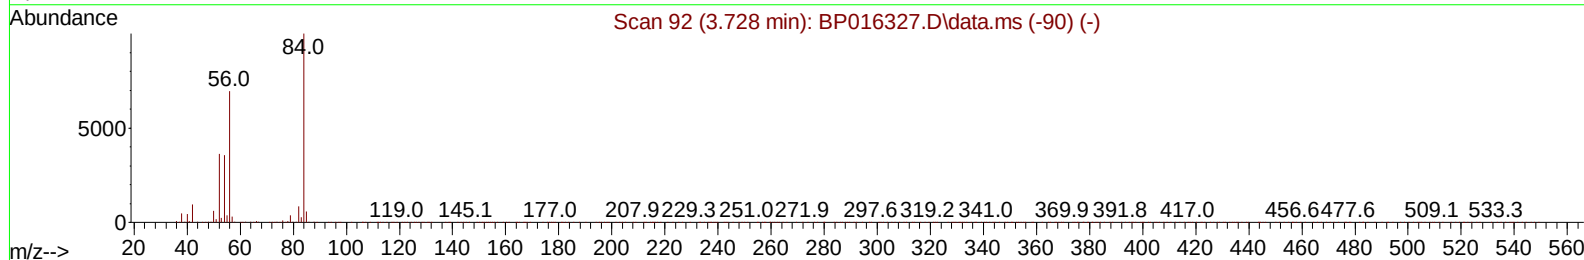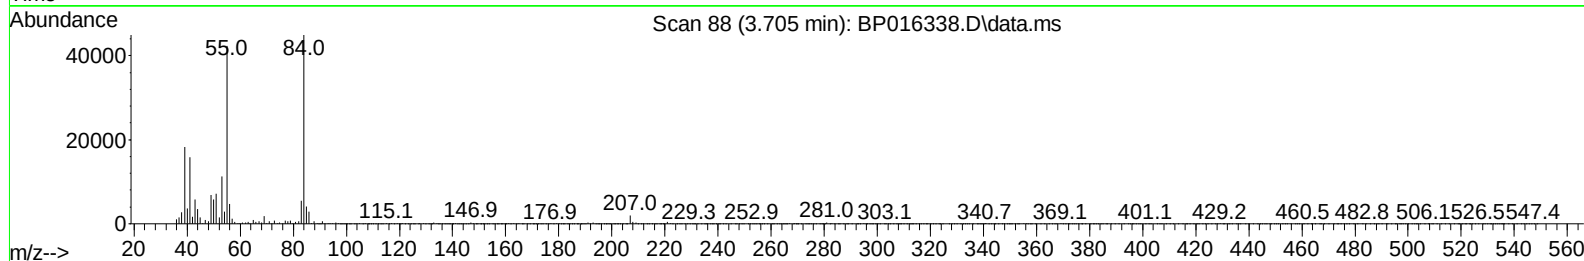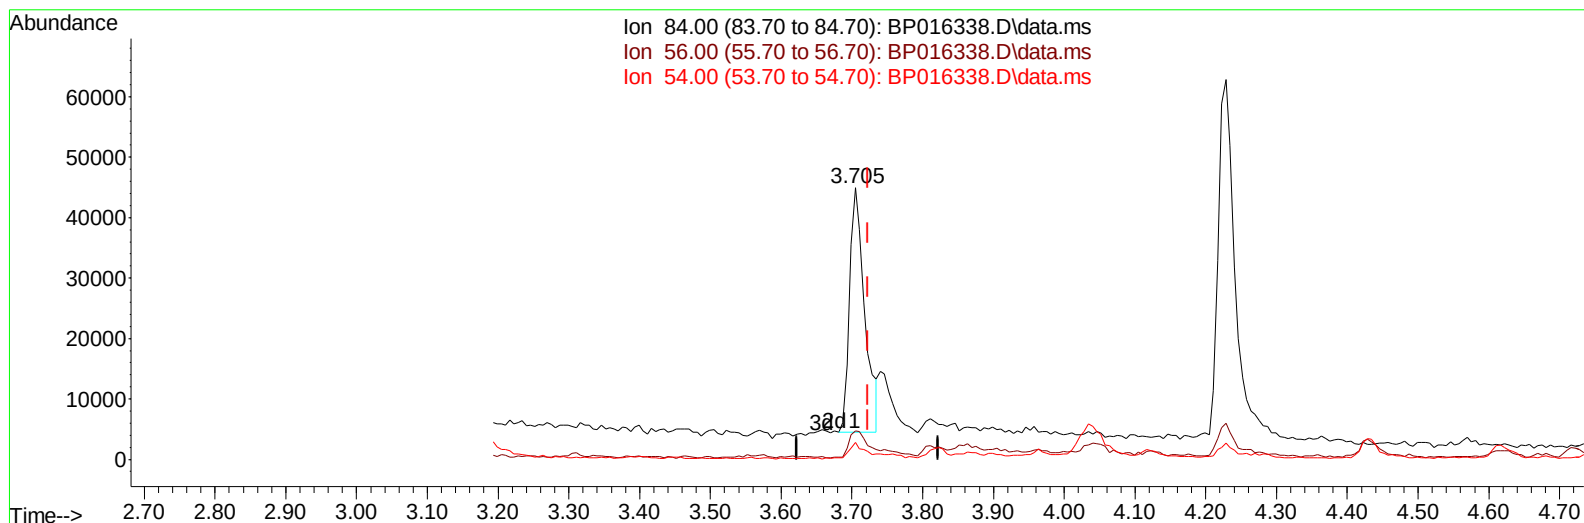

TIC: BP016338.D\data.ms

(4) Pyridine-d5 (S)

3.705min (-0.018) 7.15 ng/uI

response 60179

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	64.90	10.50#
54.00	32.50	6.31#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071923\
Data File : BP016338.D
Acq On : 19 Jul 2023 23:17
Operator : MA/JU
Sample : 03472-24
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A46R5

Manual IntegrationsAPPROVED

Quant Time: Jul 20 00:12:34 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jul 19 14:47:57 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/20/2023
Supervised By :mohammad ahmed 07/20/2023

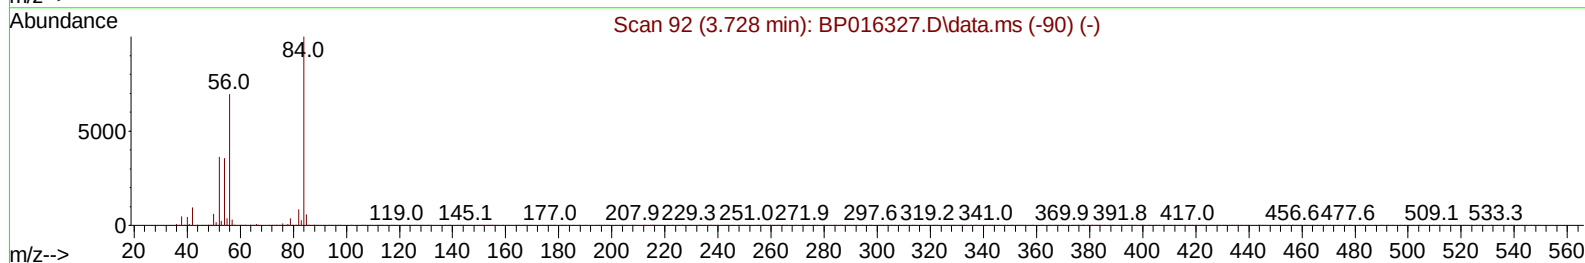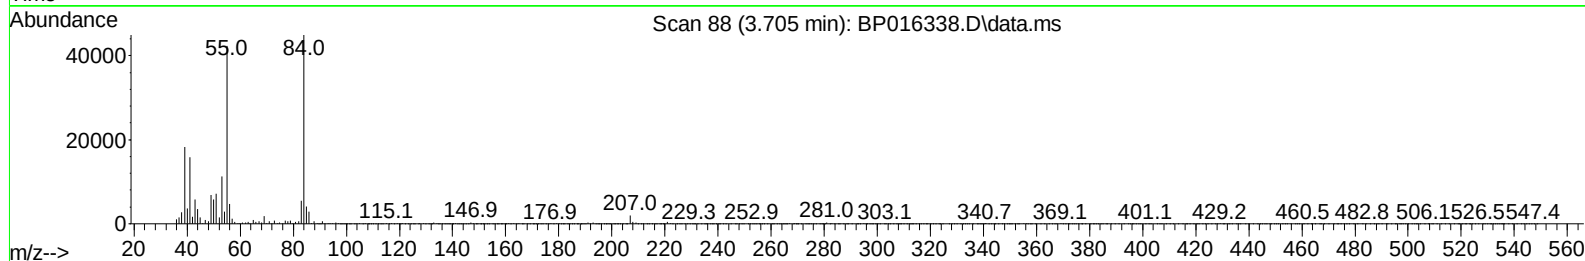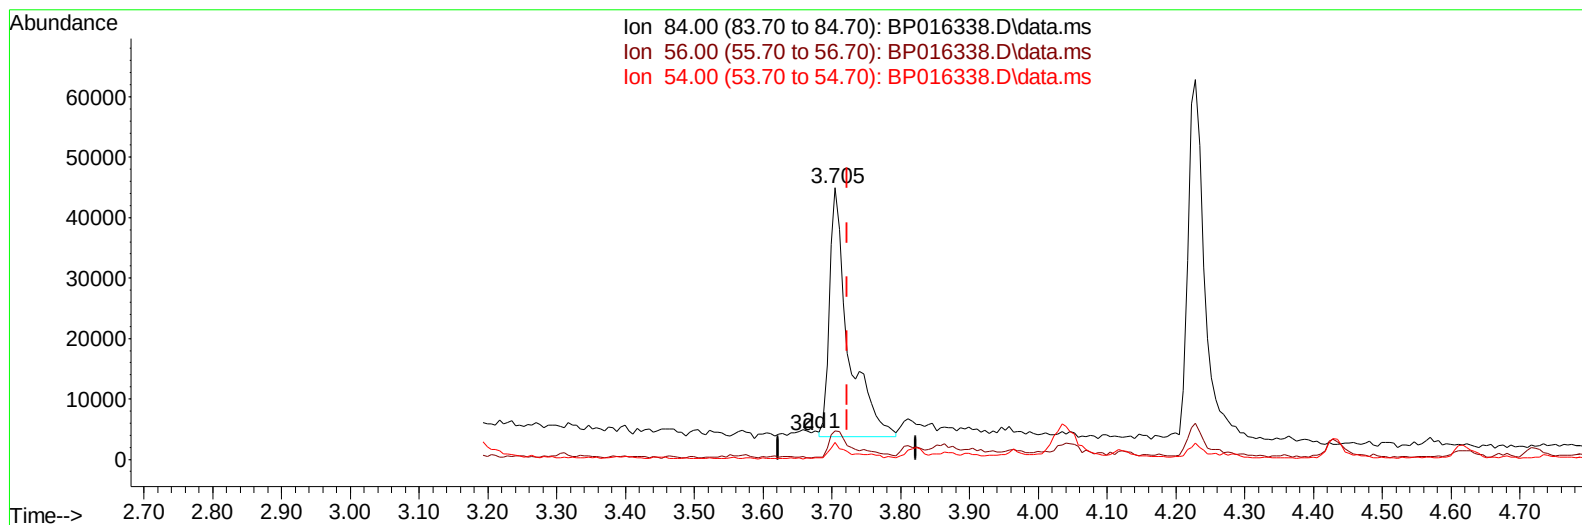

TIC: BP016338.D\data.ms

(4) Pyridine-d5 (S)

3.705min (-0.018) 9.36 ng/ul m

response 78709

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	64.90	10.50#
54.00	32.50	6.31#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071923\
 Data File : BP016338.D
 Acq On : 19 Jul 2023 23:17
 Operator : MA/JU
 Sample : 03472-24
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A46R5

Manual IntegrationsAPPROVED

Quant Time: Jul 20 00:28:33 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jul 19 14:47:57 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/20/2023
 Supervised By :mohammad ahmed 07/20/2023

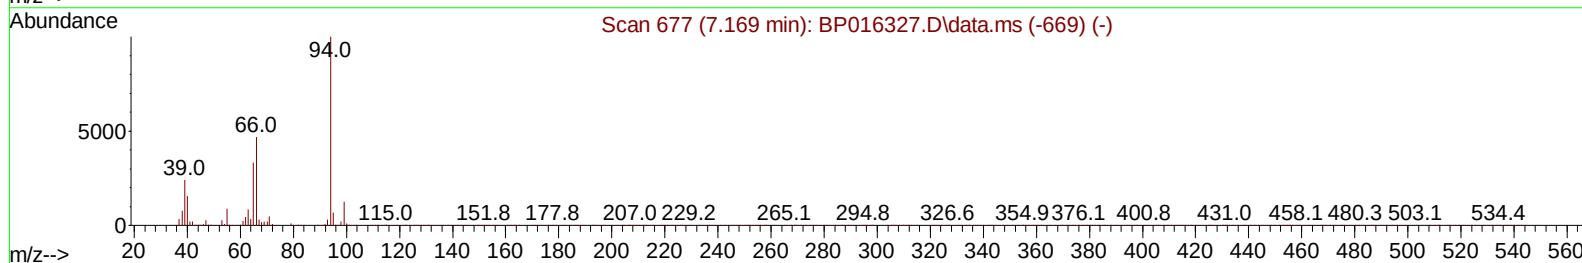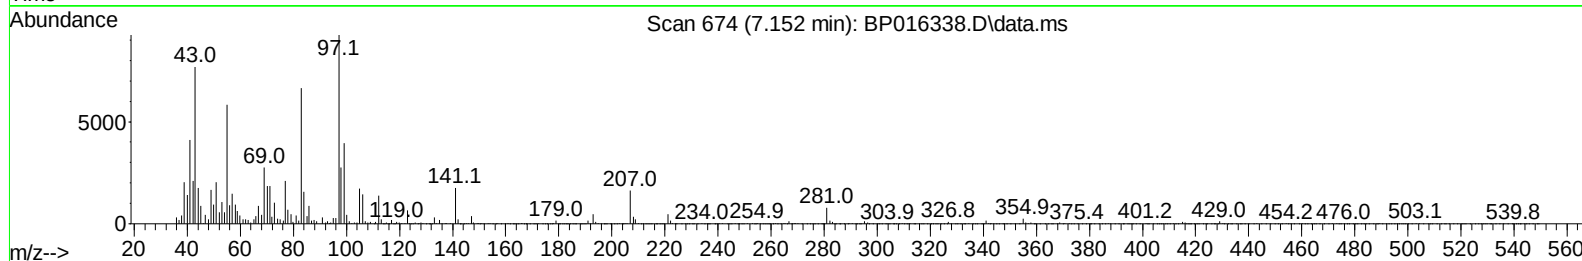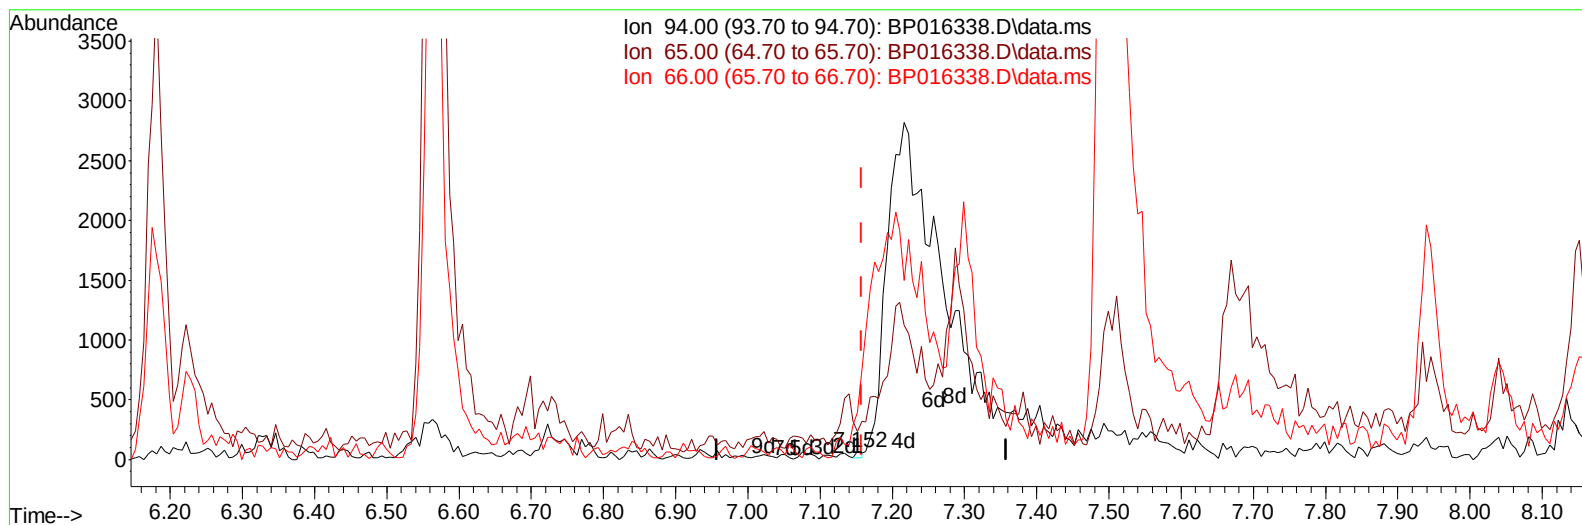

TIC: BP016338.D\data.ms

(8) Phenol

7.152min (-0.006) 0.00 ng/u1

response 31

Ion	Exp%	Act%
94.00	100.00	100.00
65.00	31.90	349.25#
66.00	40.90	585.07#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071923\
 Data File : BP016338.D
 Acq On : 19 Jul 2023 23:17
 Operator : MA/JU
 Sample : 03472-24
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A46R5

Manual IntegrationsAPPROVED

Quant Time: Jul 20 00:28:33 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jul 19 14:47:57 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/20/2023
 Supervised By :mohammad ahmed 07/20/2023

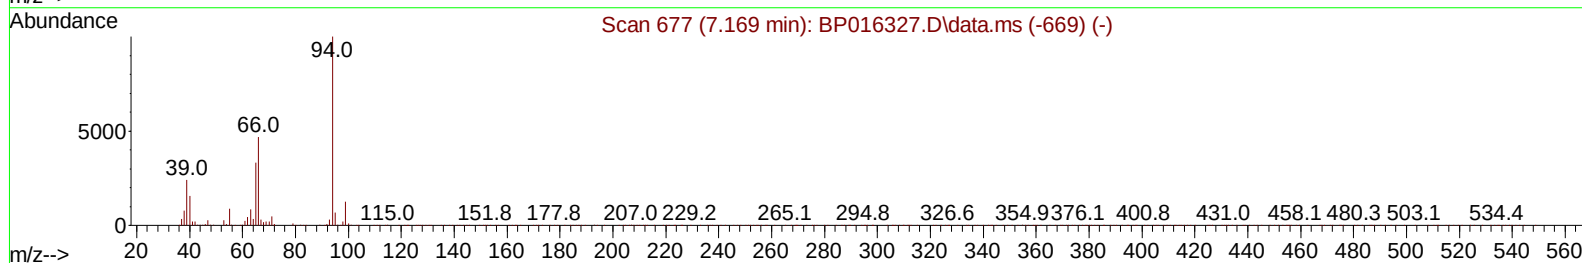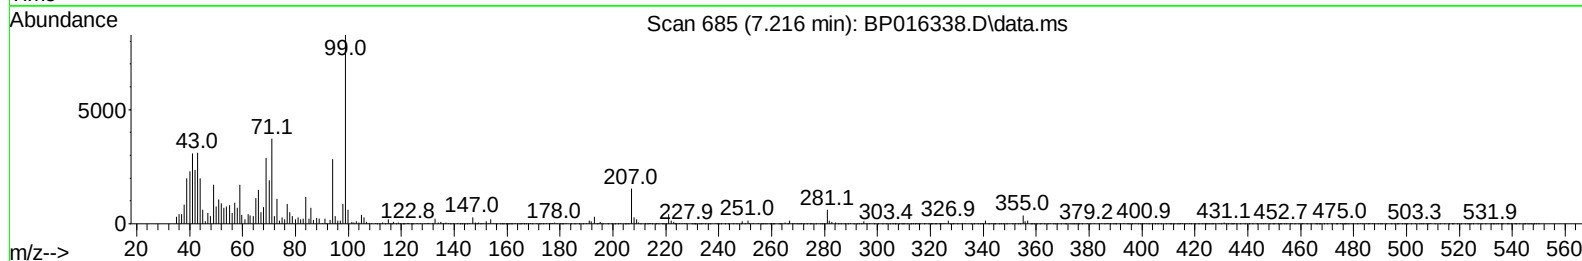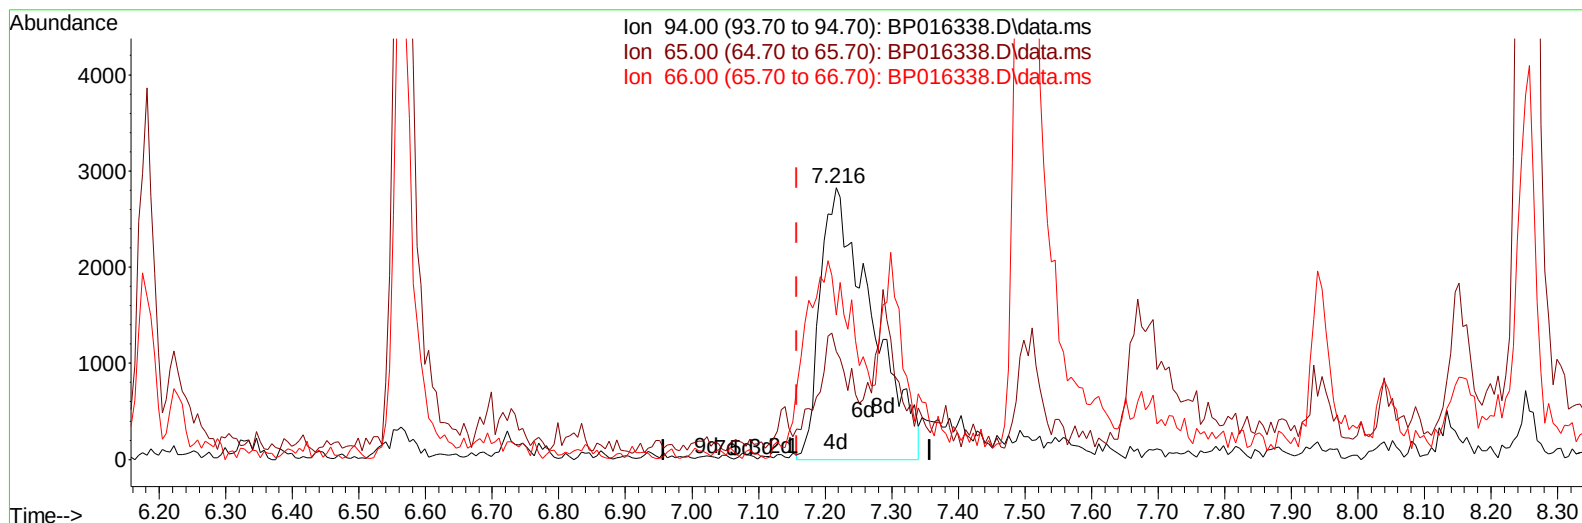

TIC: BP016338.D\data.ms

(8) Phenol

7.216min (+ 0.059) 1.31 ng/ul m

response 15120

Ion	Exp%	Act%
94.00	100.00	100.00
65.00	31.90	39.71#
66.00	40.90	53.10#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071923\
 Data File : BP016338.D
 Acq On : 19 Jul 2023 23:17
 Operator : MA/JU
 Sample : 03472-24
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A46R5

Manual IntegrationsAPPROVED

Quant Time: Jul 20 00:28:33 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jul 19 14:47:57 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/20/2023
 Supervised By :mohammad ahmed 07/20/2023

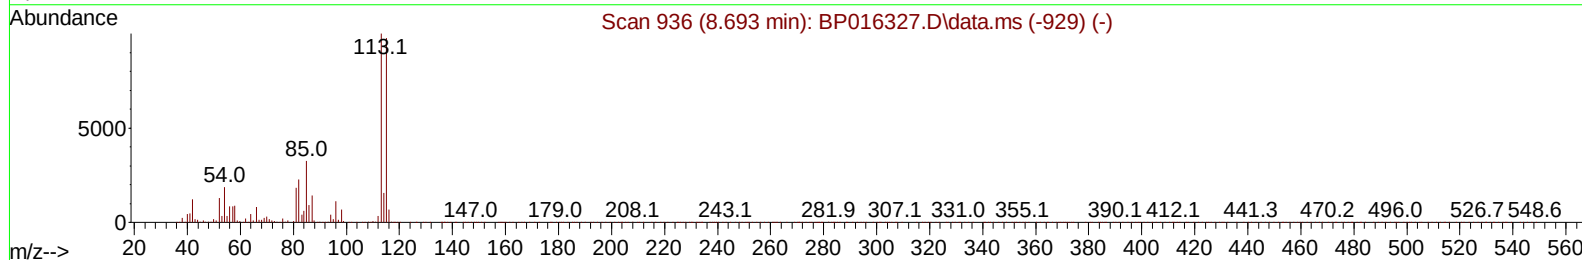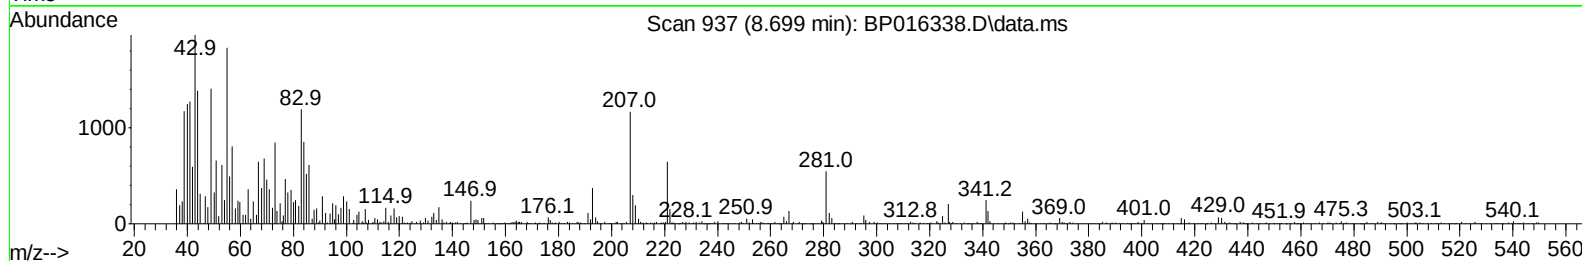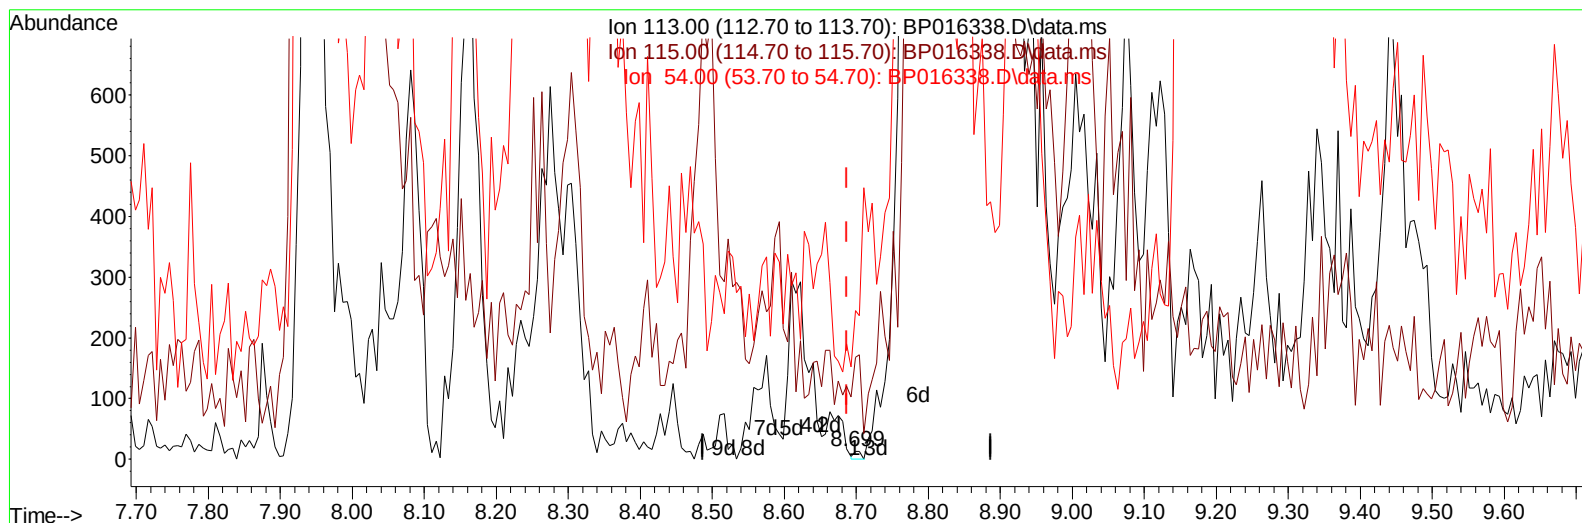

TIC: BP016338.D\data.ms

(15) 4-Methylphenol-d8 (S)

8.699min (+ 0.012) 0.00 ng/ul

response 9

Ion	Exp%	Act%
113.00	100.00	100.00
115.00	90.20	1292.31#
54.00	16.30	1884.62#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071923\
 Data File : BP016338.D
 Acq On : 19 Jul 2023 23:17
 Operator : MA/JU
 Sample : 03472-24
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A46R5

Manual IntegrationsAPPROVED

Quant Time: Jul 20 00:28:33 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jul 19 14:47:57 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/20/2023
 Supervised By :mohammad ahmed 07/20/2023

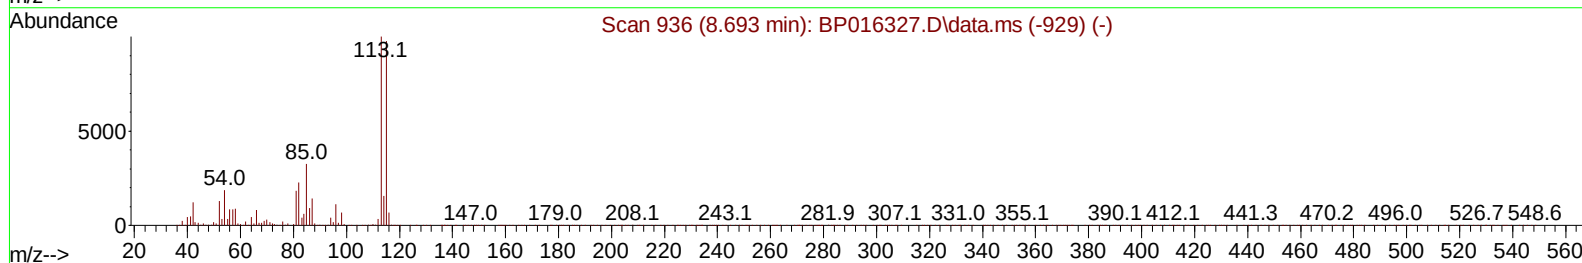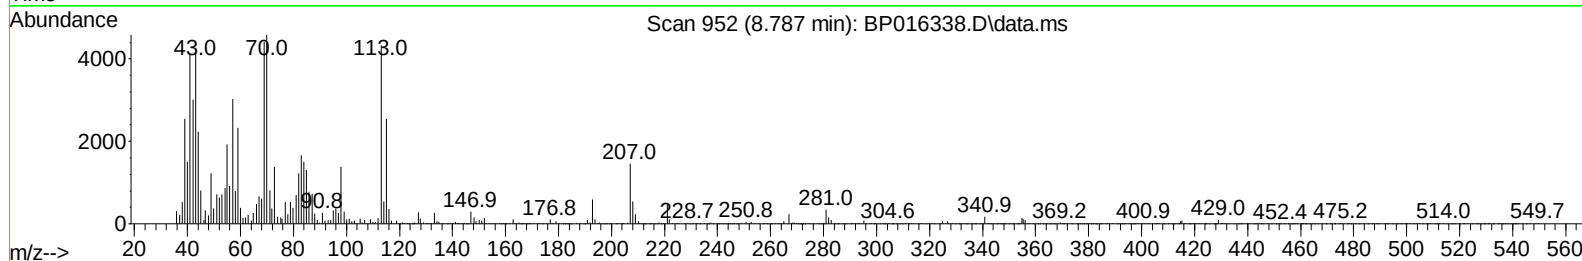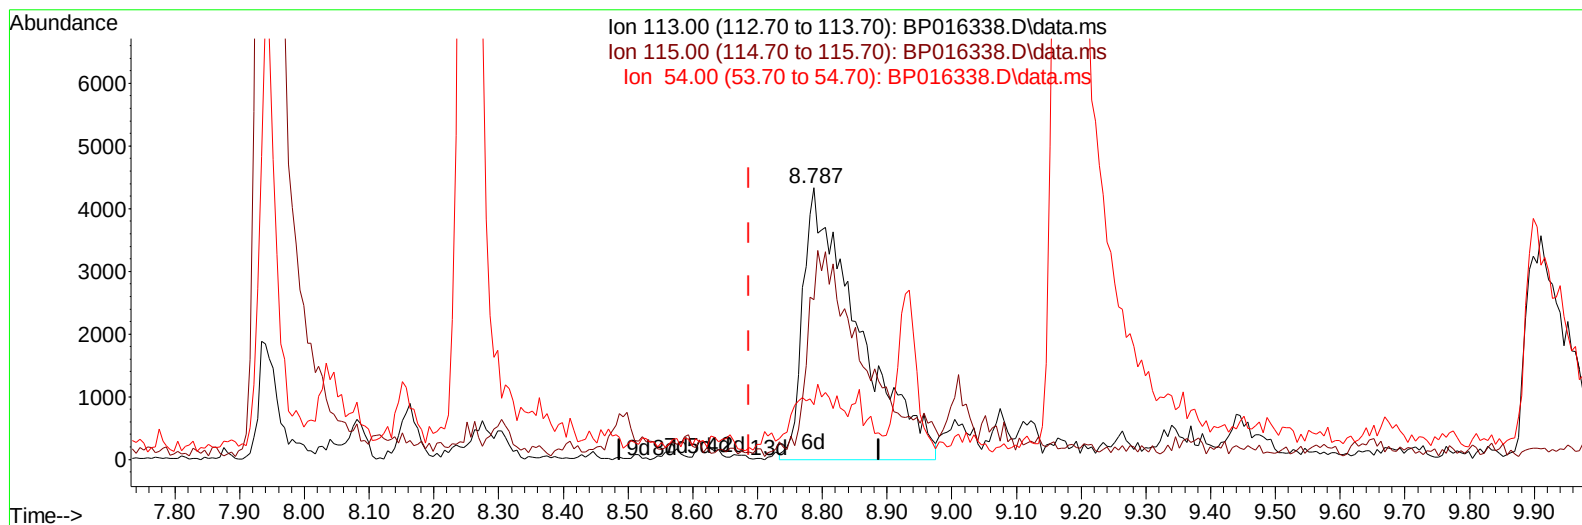

TIC: BP016338.D\data.ms

(15) 4-Methylphenol-d8 (S)

8.787min (+ 0.100) 2.94 ng/ul m

response 25507

Ion	Exp%	Act%
113.00	100.00	100.00
115.00	90.20	58.85#
54.00	16.30	20.09#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071923\
 Data File : BP016338.D
 Acq On : 19 Jul 2023 23:17
 Operator : MA/JU
 Sample : 03472-24
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A46R5

Manual IntegrationsAPPROVED

Quant Time: Jul 20 00:28:33 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jul 19 14:47:57 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/20/2023
 Supervised By :mohammad ahmed 07/20/2023

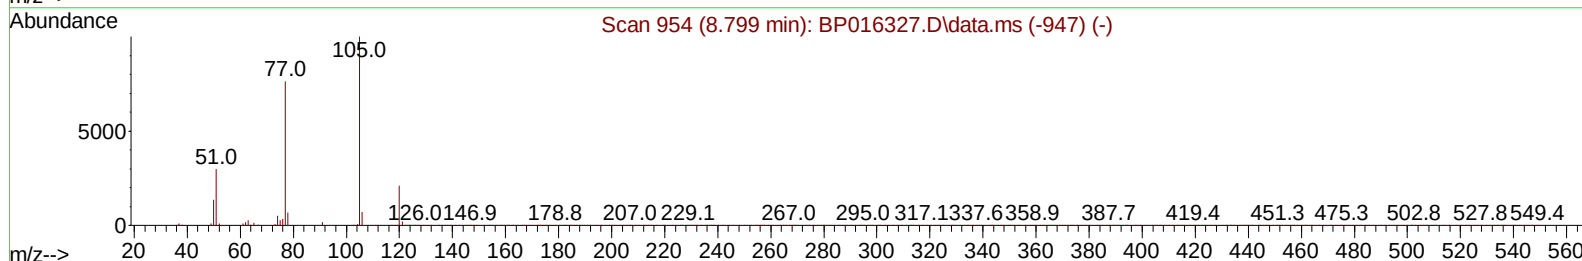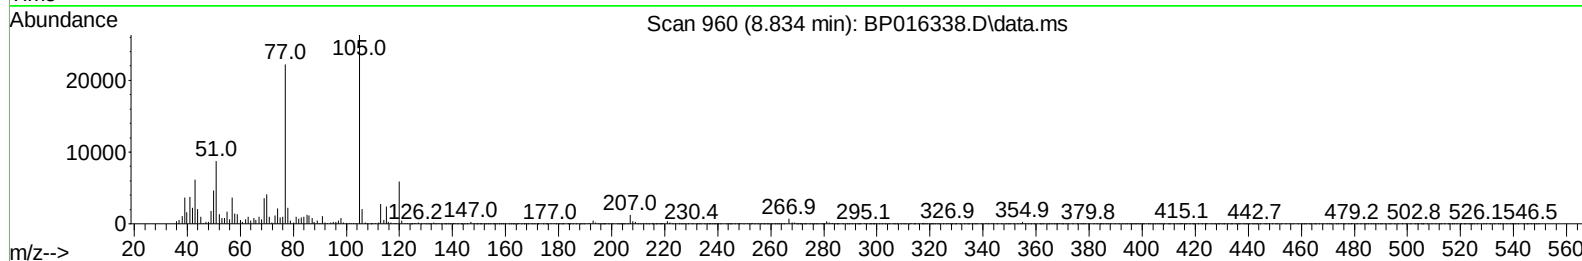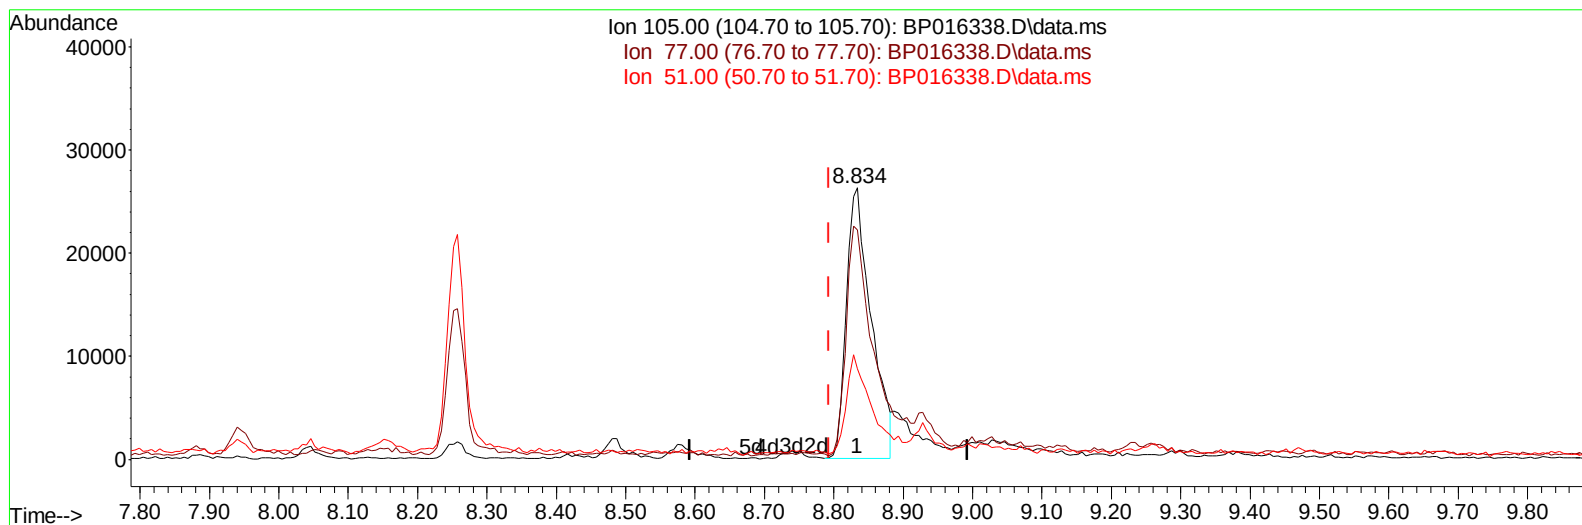

TIC: BP016338.D\data.ms

(16) Acetophenone

8.834min (+ 0.041) 4.52 ng/ul

response 64780

Ion	Exp%	Act%
105.00	100.00	100.00
77.00	87.70	84.56
51.00	32.90	33.39
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071923\
 Data File : BP016338.D
 Acq On : 19 Jul 2023 23:17
 Operator : MA/JU
 Sample : 03472-24
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A46R5

Manual IntegrationsAPPROVED

Quant Time: Jul 20 00:28:33 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jul 19 14:47:57 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/20/2023
 Supervised By :mohammad ahmed 07/20/2023

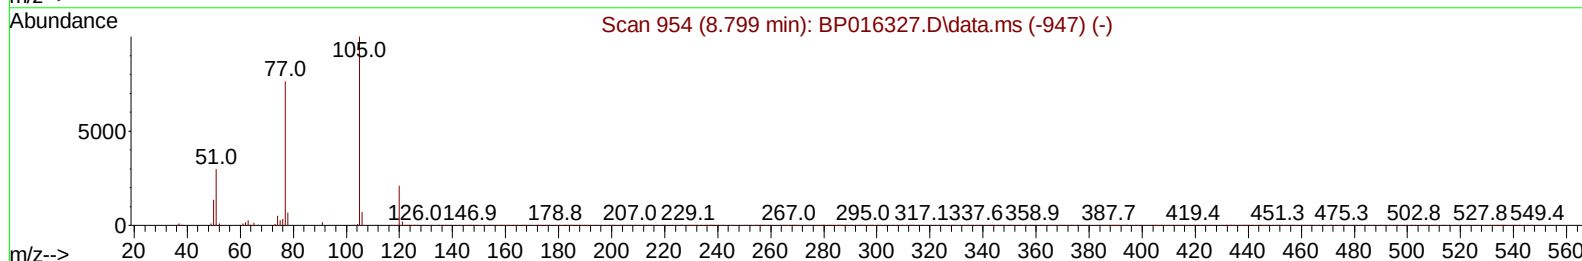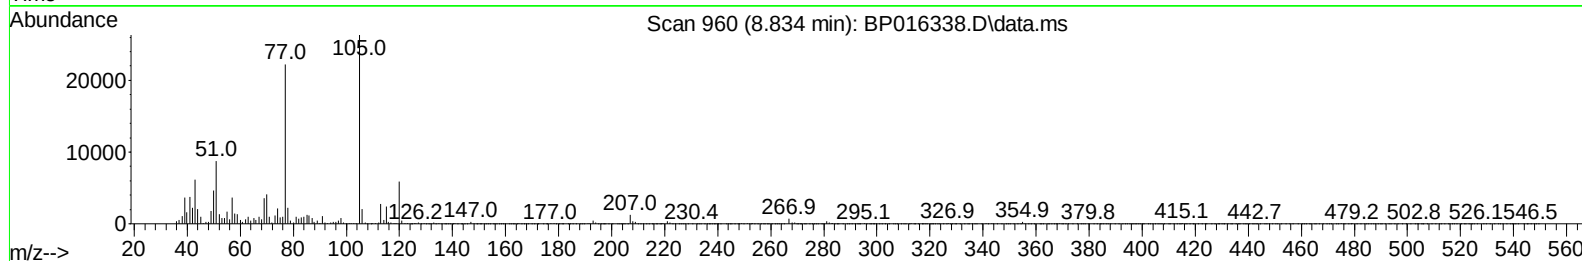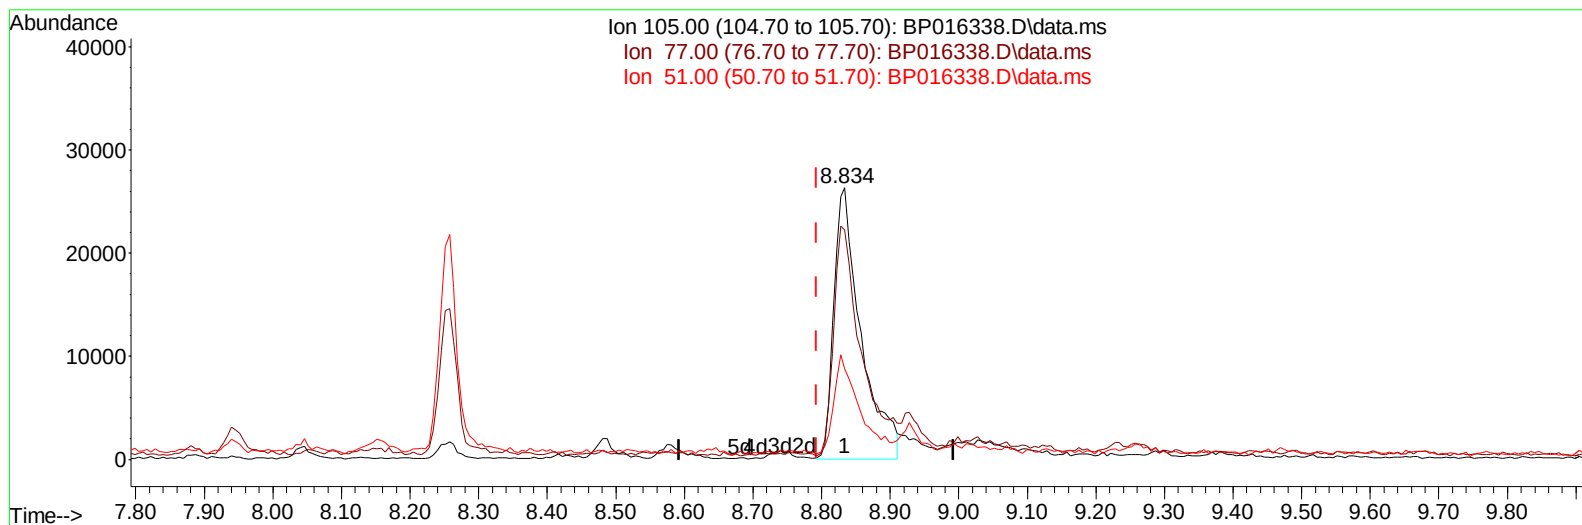

TIC: BP016338.D\data.ms

(16) Acetophenone

8.834min (+ 0.041) 5.02 ng/ul m

response 71915

Ion	Exp%	Act%
105.00	100.00	100.00
77.00	87.70	84.56
51.00	32.90	33.39
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071923\
Data File : BP016338.D
Acq On : 19 Jul 2023 23:17
Operator : MA/JU
Sample : 03472-24
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A46R5

Manual IntegrationsAPPROVED

Quant Time: Jul 20 00:28:33 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jul 19 14:47:57 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/20/2023
Supervised By :mohammad ahmed 07/20/2023

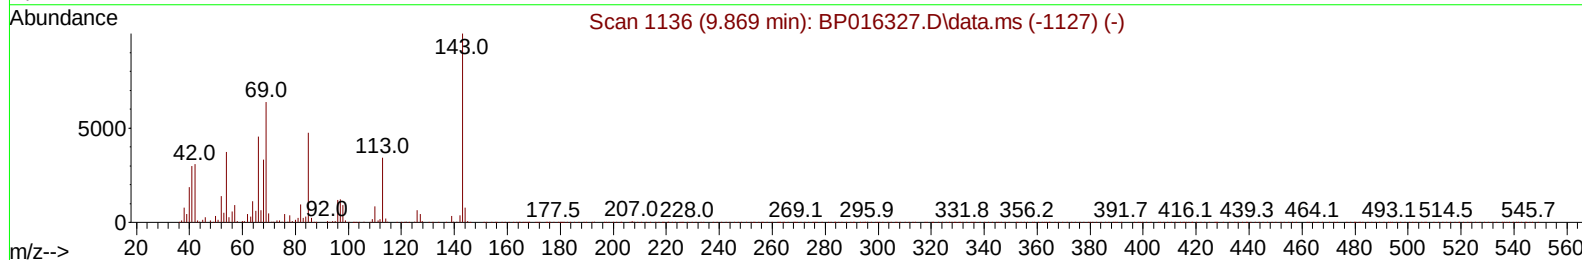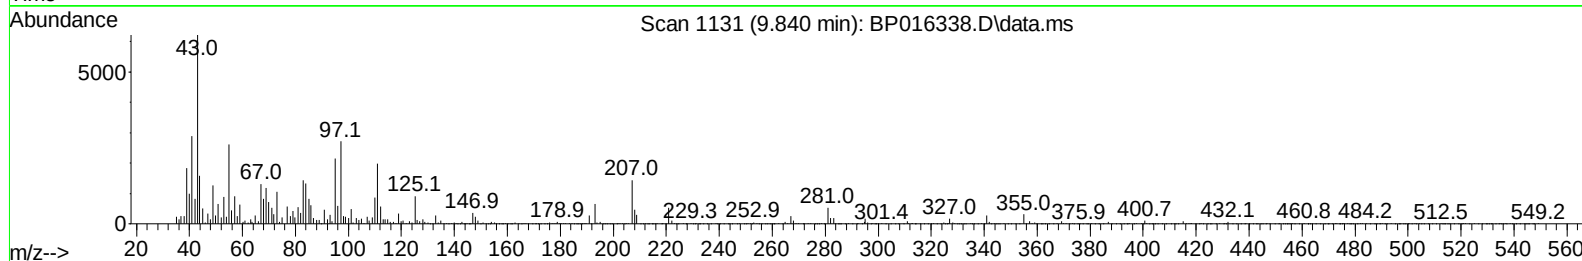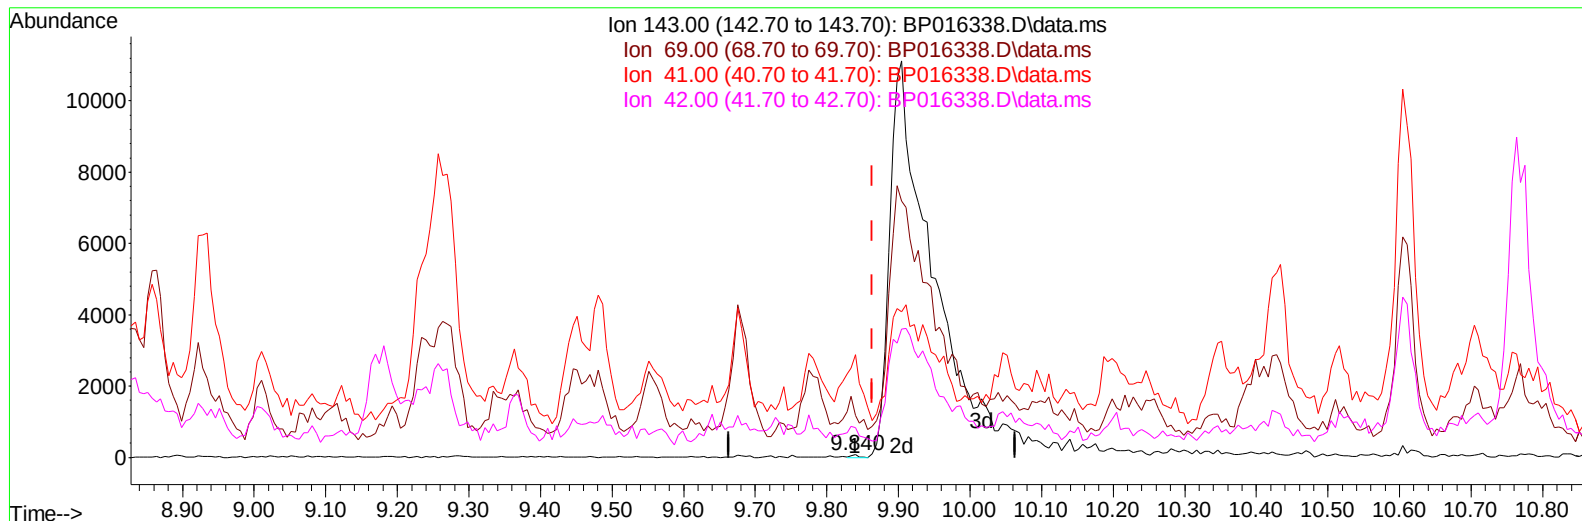

TIC: BP016338.D\data.ms

(24) 2-Nitrophenol-d4 (S)

9.840min (-0.024) 0.01 ng/u1

response 47

Ion	Exp%	Act%
143.00	100.00	100.00
69.00	62.00	1550.00#
41.00	28.60	3803.95#
42.00	29.20	1093.42#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071923\
 Data File : BP016338.D
 Acq On : 19 Jul 2023 23:17
 Operator : MA/JU
 Sample : 03472-24
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A46R5

Manual IntegrationsAPPROVED

Quant Time: Jul 20 00:28:33 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jul 19 14:47:57 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/20/2023
 Supervised By :mohammad ahmed 07/20/2023

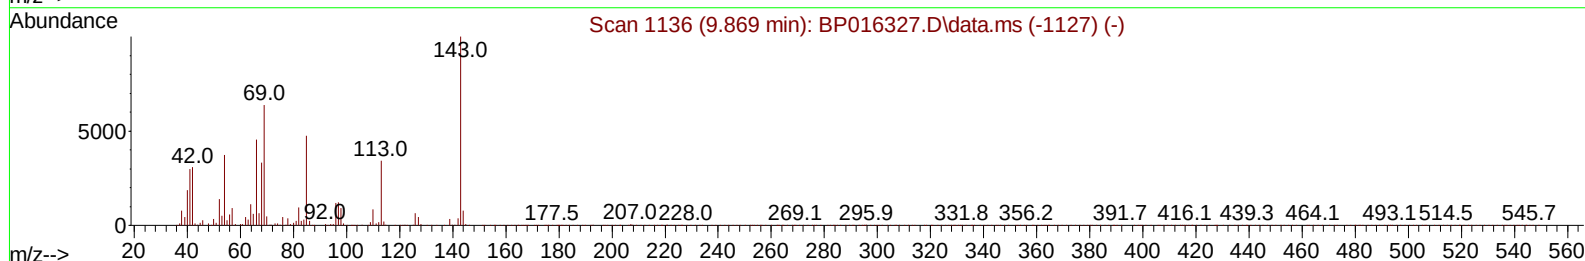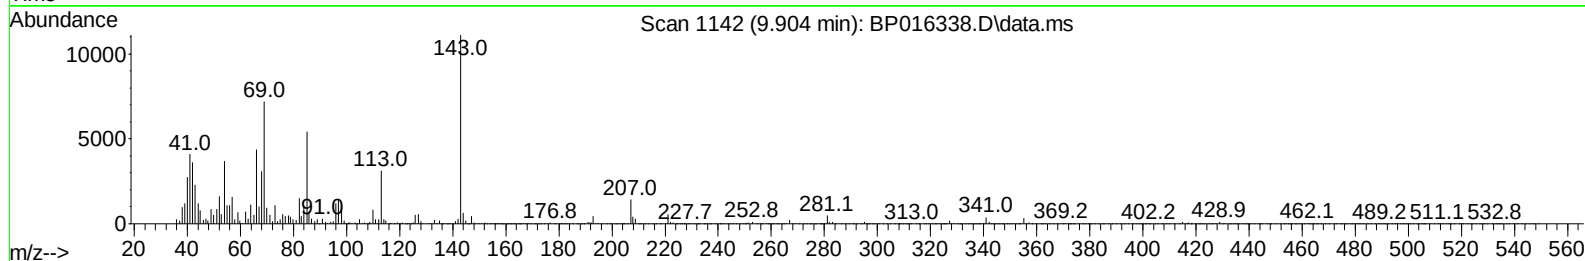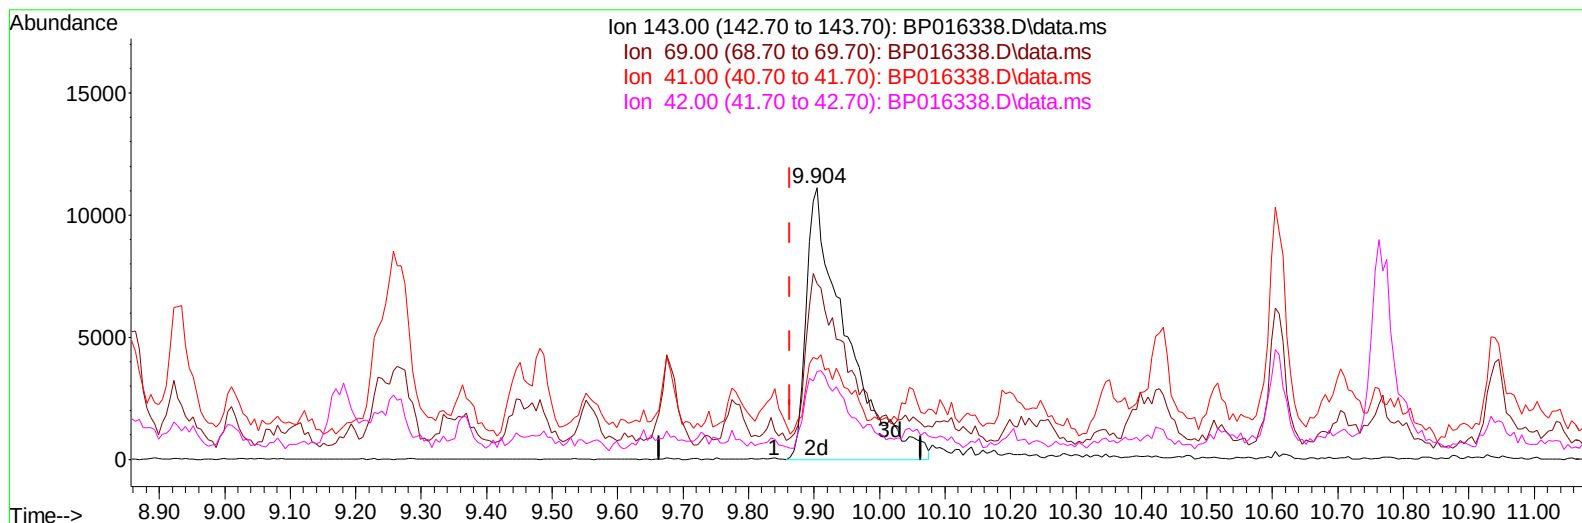

TIC: BP016338.D\data.ms

(24) 2-Nitrophenol-d4 (S)

9.904min (+ 0.041) 10.34 ng/ul m

response 46940

Ion	Exp%	Act%
143.00	100.00	100.00
69.00	62.00	64.63
41.00	28.60	36.80#
42.00	29.20	32.42




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071923\
 Data File : BP016338.D
 Acq On : 19 Jul 2023 23:17
 Operator : MA/JU
 Sample : 03472-24
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A46R5

Manual IntegrationsAPPROVED

Quant Time: Jul 20 00:28:33 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jul 19 14:47:57 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/20/2023
 Supervised By :mohammad ahmed 07/20/2023

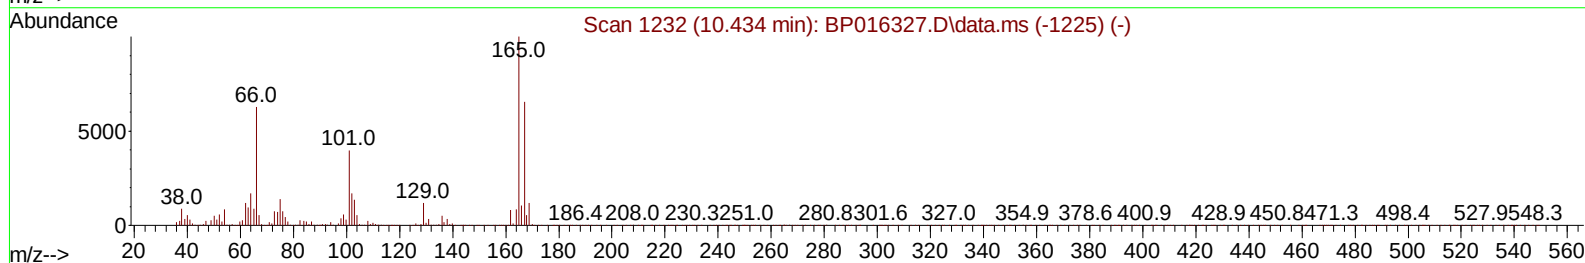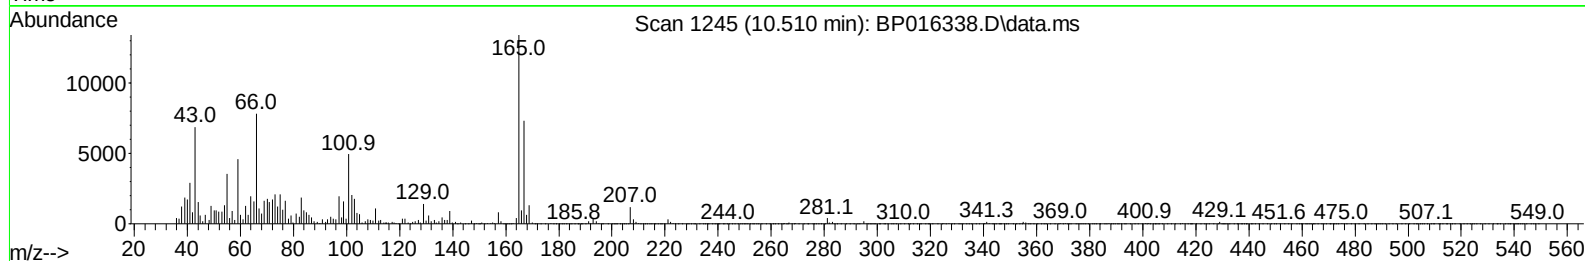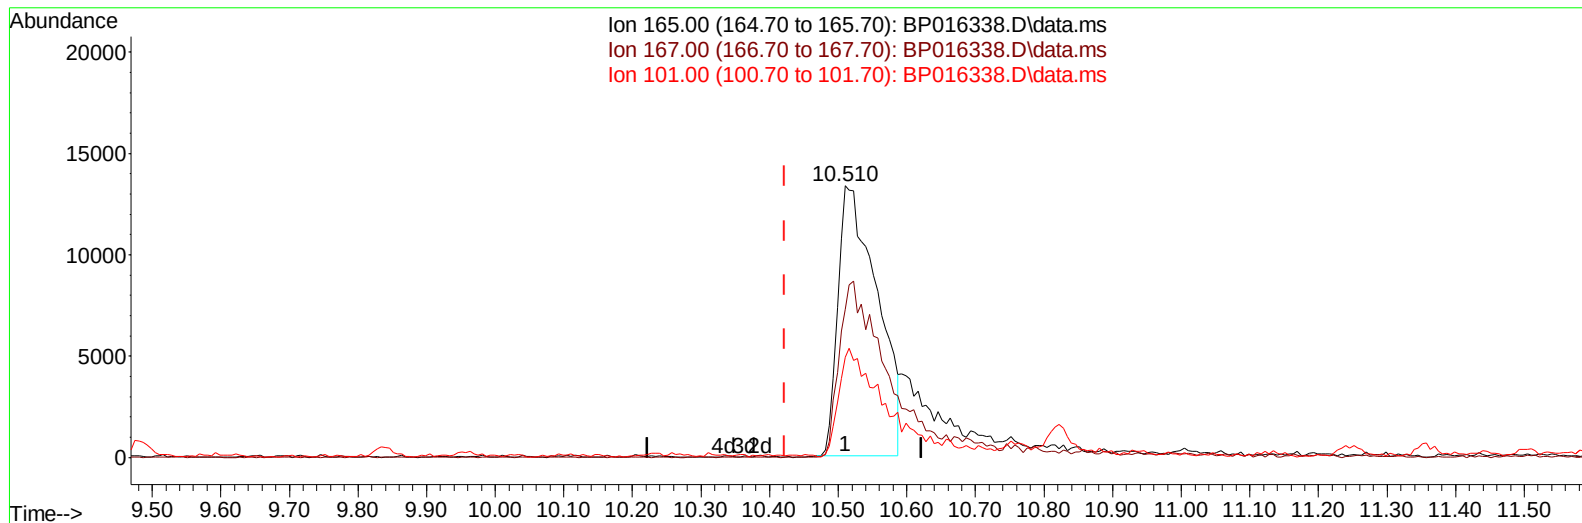

TIC: BP016338.D\data.ms

(28) 2,4-Dichlorophenol-d3 (S)

10.510min (+ 0.088) 6.73 ng/ul

response 52910

Ion	Exp%	Act%
165.00	100.00	100.00
167.00	65.20	54.58
101.00	38.50	36.87
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071923\
Data File : BP016338.D
Acq On : 19 Jul 2023 23:17
Operator : MA/JU
Sample : 03472-24
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A46R5

Manual IntegrationsAPPROVED

Quant Time: Jul 20 00:28:33 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jul 19 14:47:57 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/20/2023
Supervised By :mohammad ahmed 07/20/2023

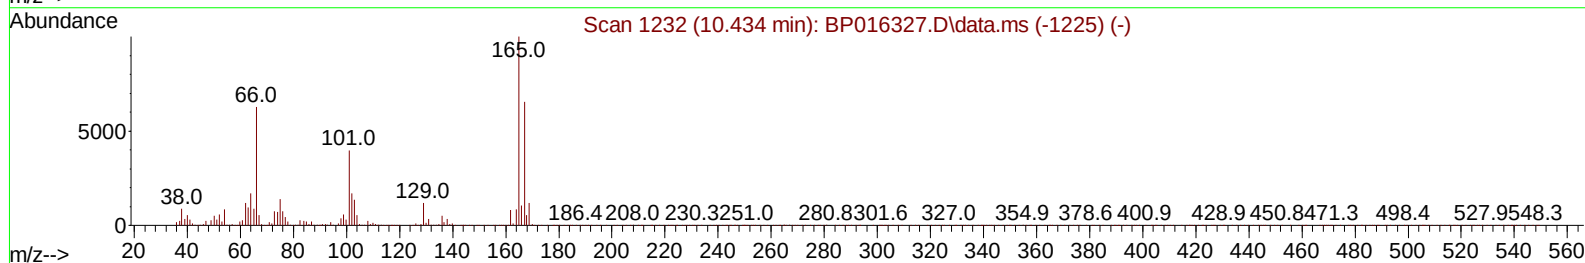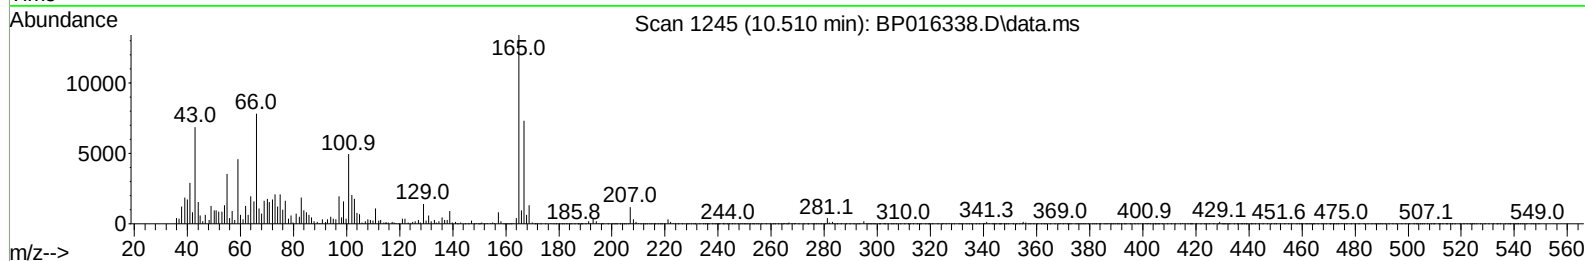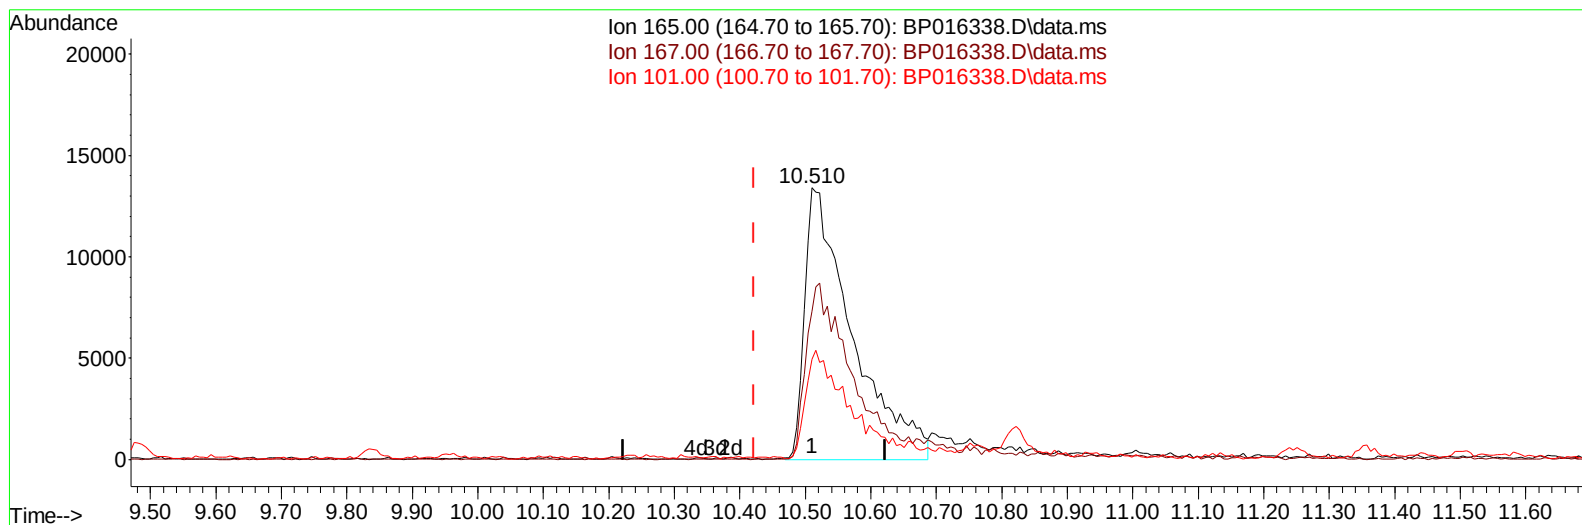

TIC: BP016338.D\data.ms

(28) 2,4-Dichlorophenol-d3 (S)

10.510min (+ 0.088) 8.61 ng/ul m

response 67689

Ion	Exp%	Act%
165.00	100.00	100.00
167.00	65.20	54.58
101.00	38.50	36.87
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071923\
Data File : BP016338.D
Acq On : 19 Jul 2023 23:17
Operator : MA/JU
Sample : 03472-24
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A46R5

Manual IntegrationsAPPROVED

Quant Time: Jul 20 00:28:33 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jul 19 14:47:57 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/20/2023
Supervised By :mohammad ahmed 07/20/2023

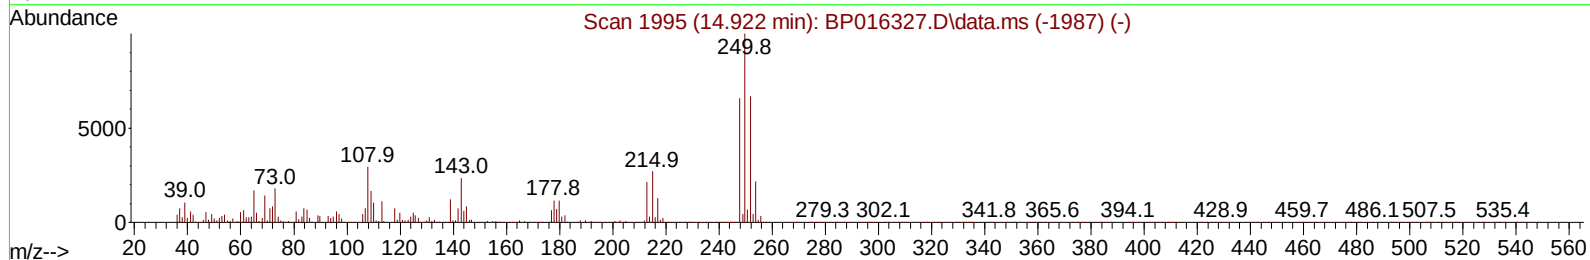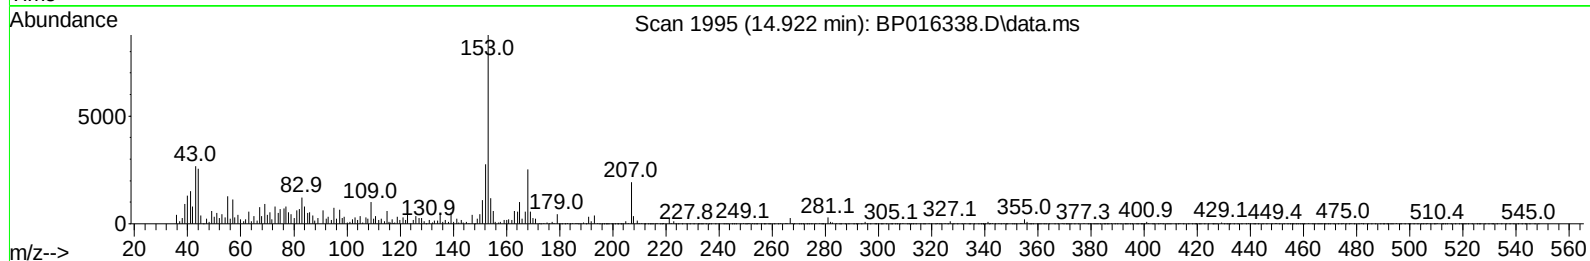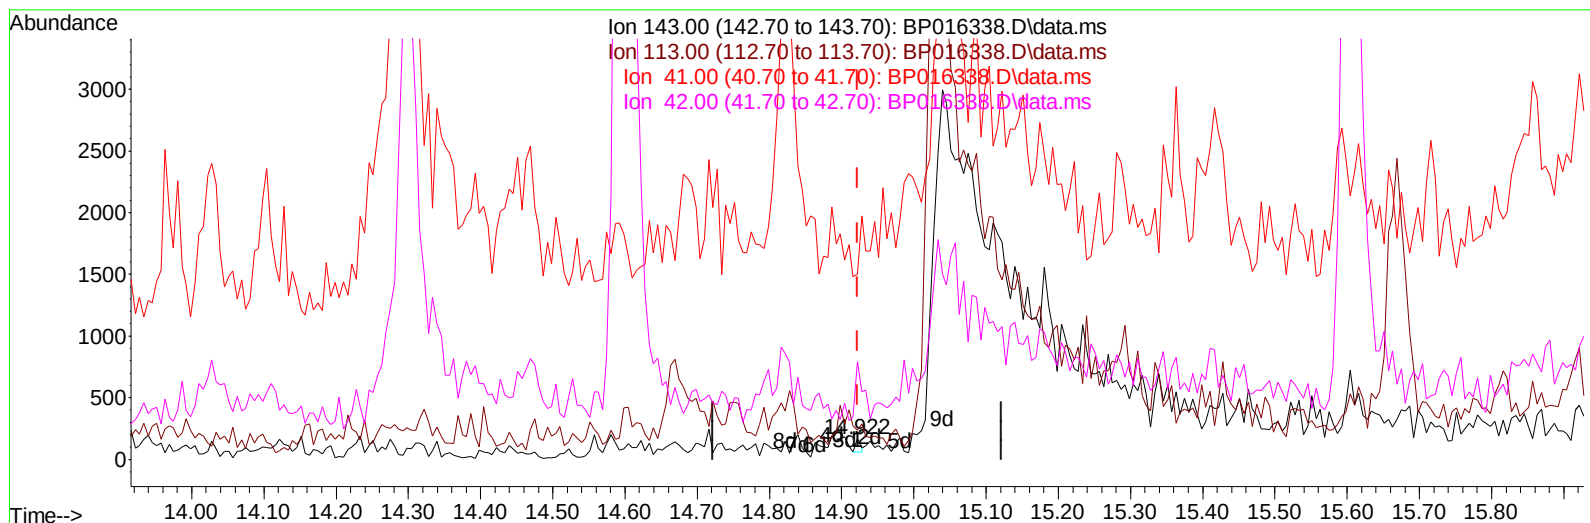

TIC: BP016338.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.922min (+ 0.000) 0.01 ng/u1

response 48

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	79.50	143.11#
41.00	49.30	899.40#
42.00	32.70	473.65#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071923\
Data File : BP016338.D
Acq On : 19 Jul 2023 23:17
Operator : MA/JU
Sample : 03472-24
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A46R5

Manual IntegrationsAPPROVED

Quant Time: Jul 20 00:30:39 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jul 19 14:47:57 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/20/2023
Supervised By :mohammad ahmed 07/20/2023

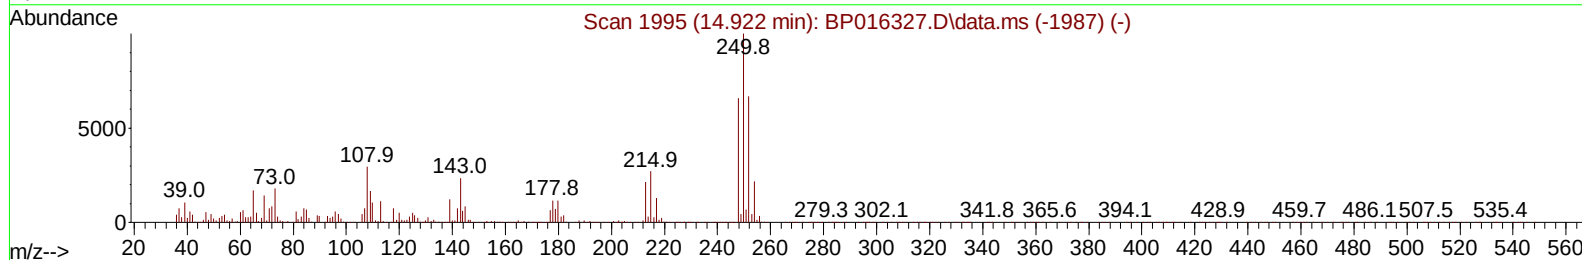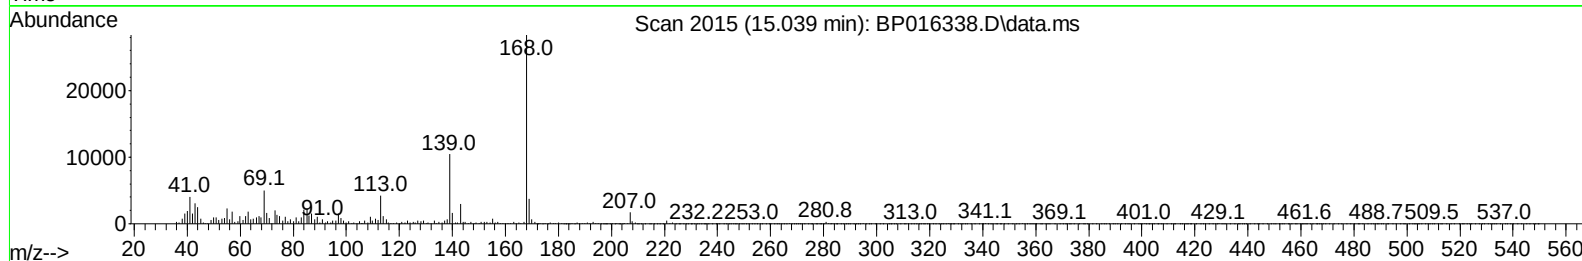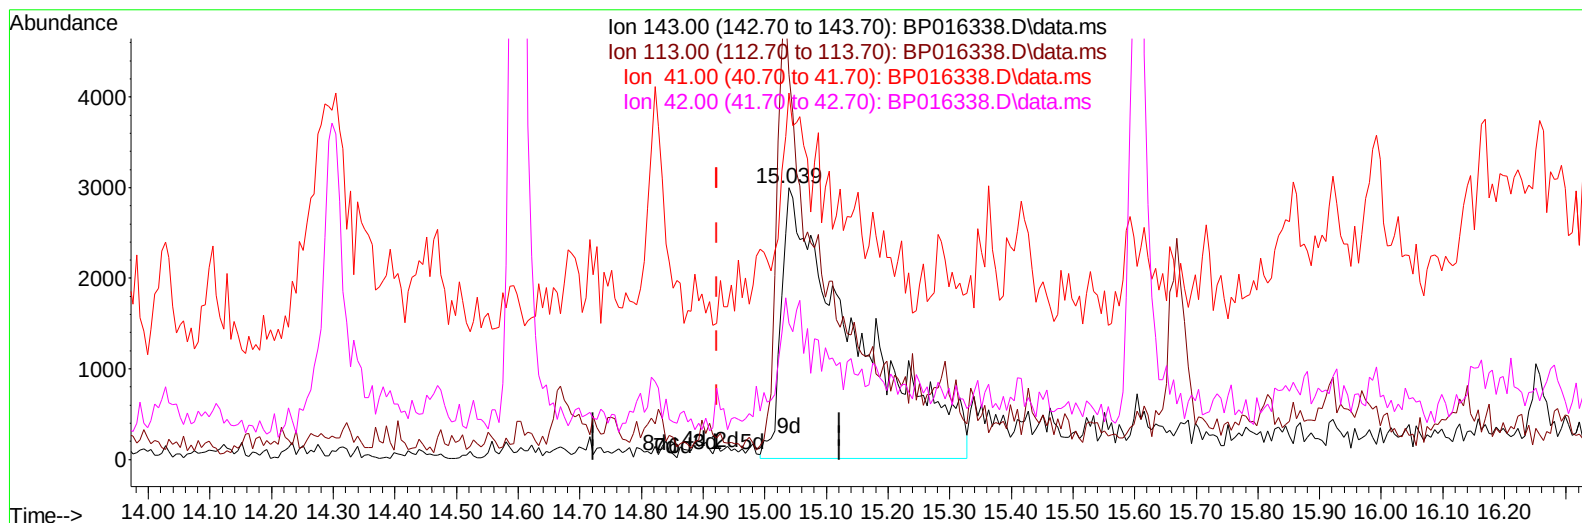

TIC: BP016338.D\data.ms

(54) 4-Nitrophenol-d4 (S)

15.039min (+ 0.118) 4.12 ng/ul m

response 24986

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	79.50	141.74#
41.00	49.30	135.07#
42.00	32.70	50.12#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071923\
Data File : BP016338.D
Acq On : 19 Jul 2023 23:17
Operator : MA/JU
Sample : 03472-24
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A46R5

Manual IntegrationsAPPROVED

Quant Time: Jul 20 00:30:39 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jul 19 14:47:57 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/20/2023
Supervised By :mohammad ahmed 07/20/2023

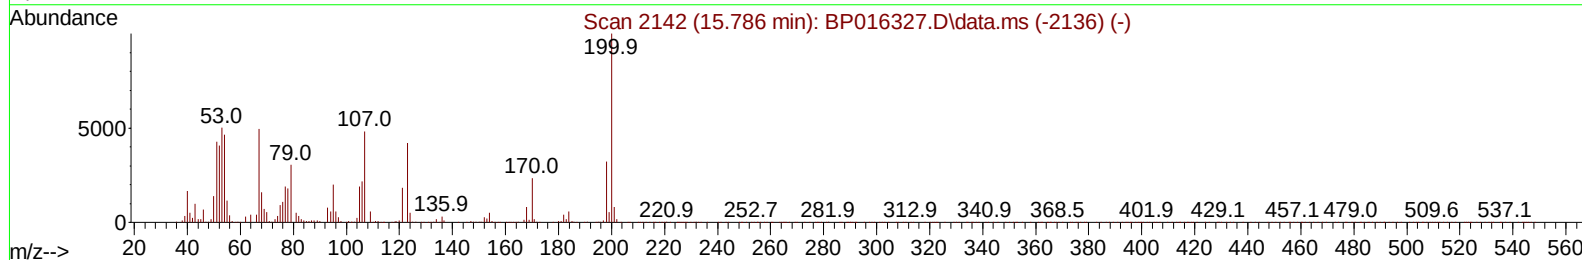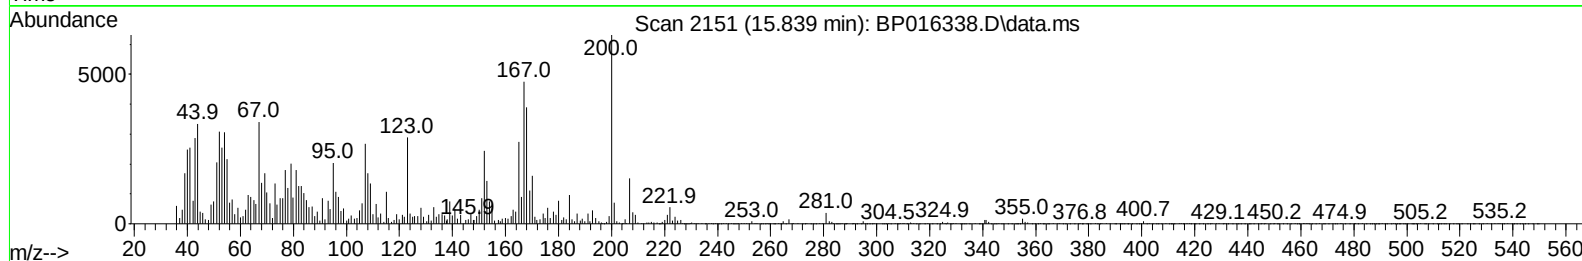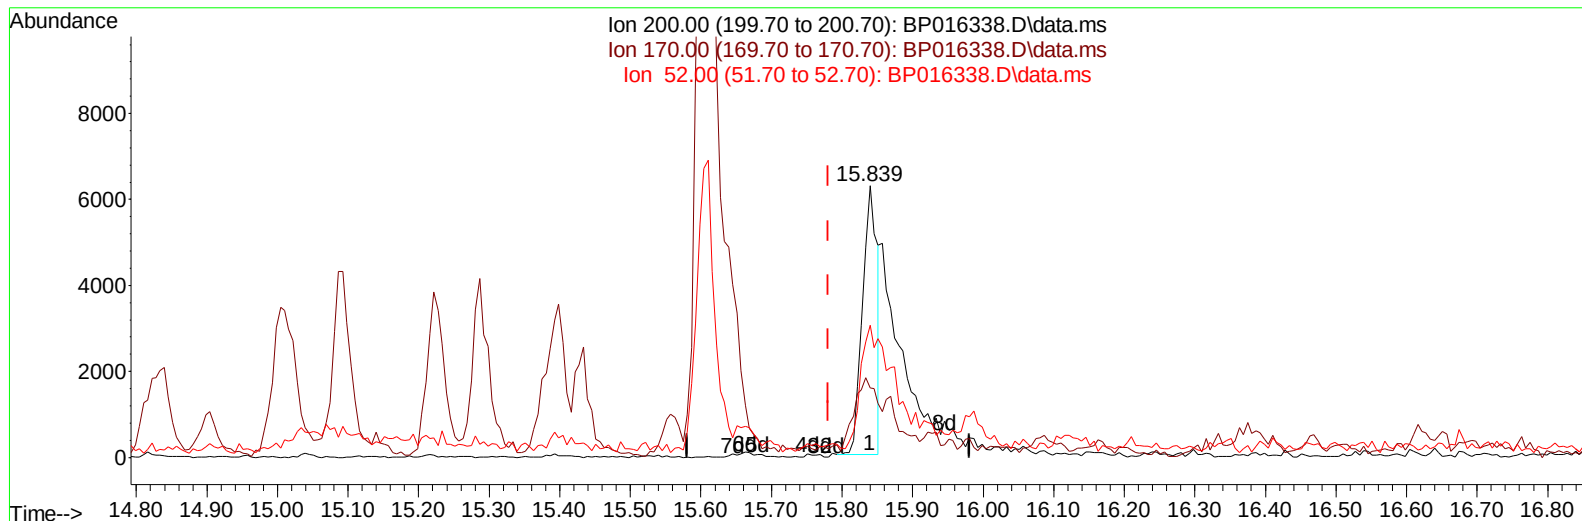

TIC: BP016338.D\data.ms

(65) 4,6-Dinitro-2-methylphenol-d2 (S)

15.839min (+ 0.059) 1.45 ng/ul

response 9203

Ion	Exp%	Act%
200.00	100.00	100.00
170.00	21.90	25.58
52.00	58.00	48.72
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071923\
 Data File : BP016338.D
 Acq On : 19 Jul 2023 23:17
 Operator : MA/JU
 Sample : 03472-24
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A46R5

Manual IntegrationsAPPROVED

Quant Time: Jul 20 00:30:39 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jul 19 14:47:57 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/20/2023
 Supervised By :mohammad ahmed 07/20/2023

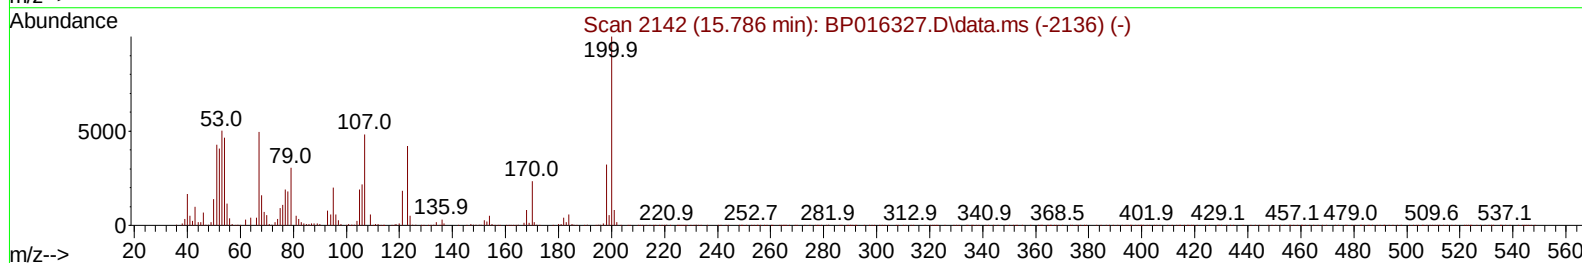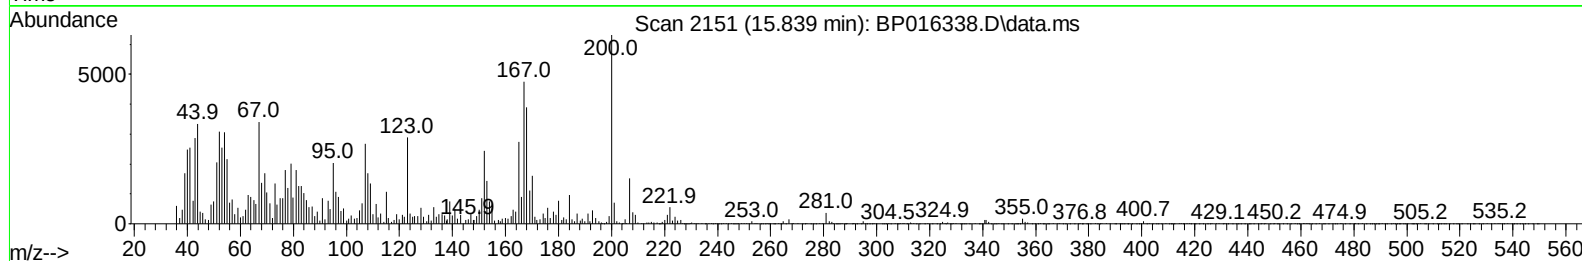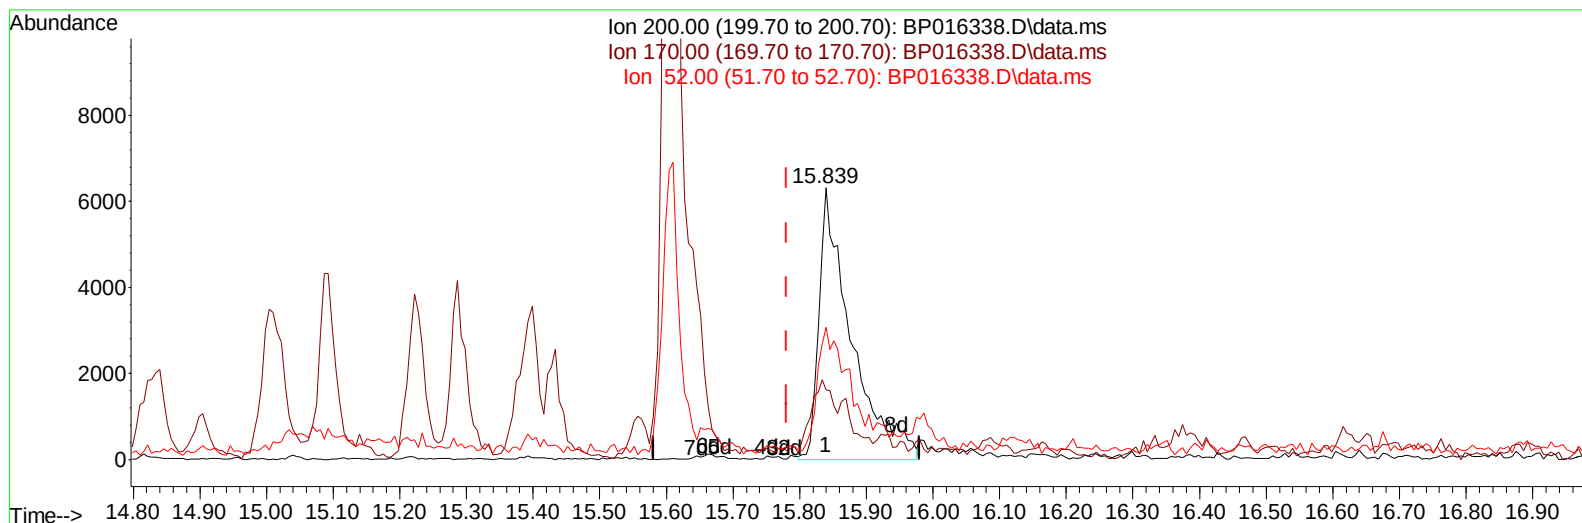

TIC: BP016338.D\data.ms

(65) 4,6-Dinitro-2-methylphenol-d2 (S)

15.839min (+ 0.059) 3.35 ng/ul m

response 21254

Ion	Exp%	Act%
200.00	100.00	100.00
170.00	21.90	25.58
52.00	58.00	48.72
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071923\
Data File : BP016338.D
Acq On : 19 Jul 2023 23:17
Operator : MA/JU
Sample : 03472-24
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A46R5

Manual IntegrationsAPPROVED

Quant Time: Jul 20 00:31:27 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jul 19 14:47:57 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/20/2023
Supervised By :mohammad ahmed 07/20/2023

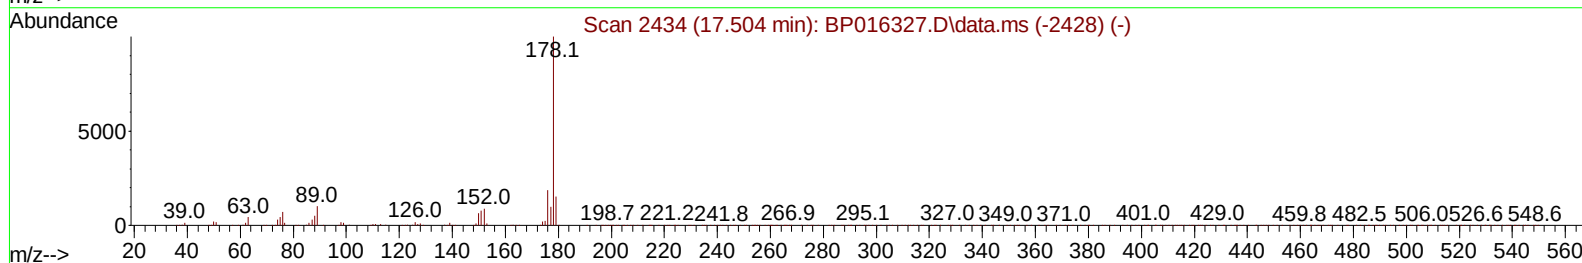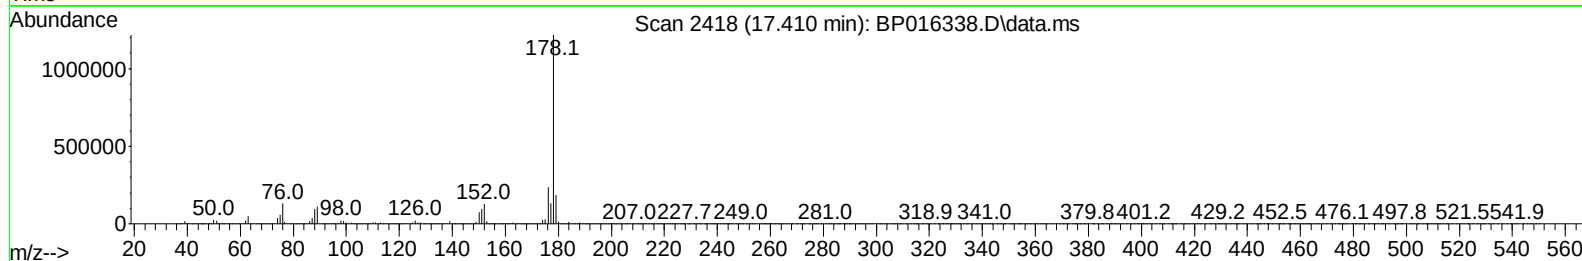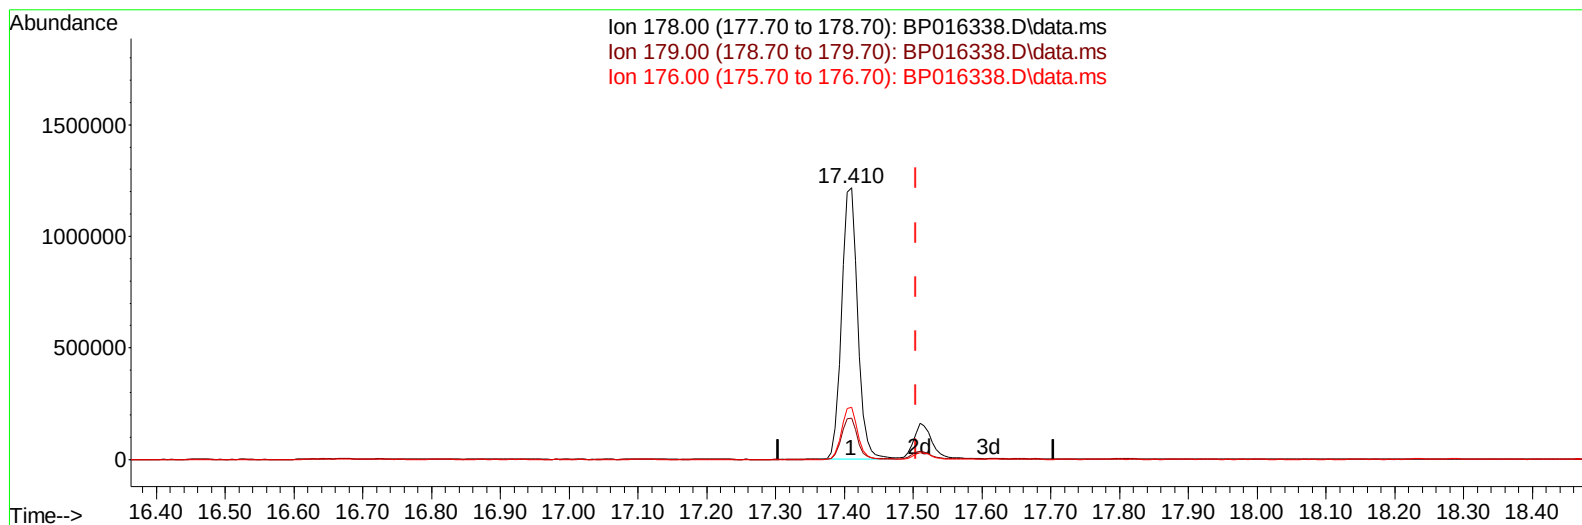

TIC: BP016338.D\data.ms

(74) Anthracene

17.410min (-0.094) 34.58 ng/u1

response 1986999

Ion	Exp%	Act%
178.00	100.00	100.00
179.00	14.90	15.31
176.00	18.70	19.32
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071923\
 Data File : BP016338.D
 Acq On : 19 Jul 2023 23:17
 Operator : MA/JU
 Sample : 03472-24
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A46R5

Manual IntegrationsAPPROVED

Quant Time: Jul 20 00:31:27 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jul 19 14:47:57 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/20/2023
 Supervised By :mohammad ahmed 07/20/2023

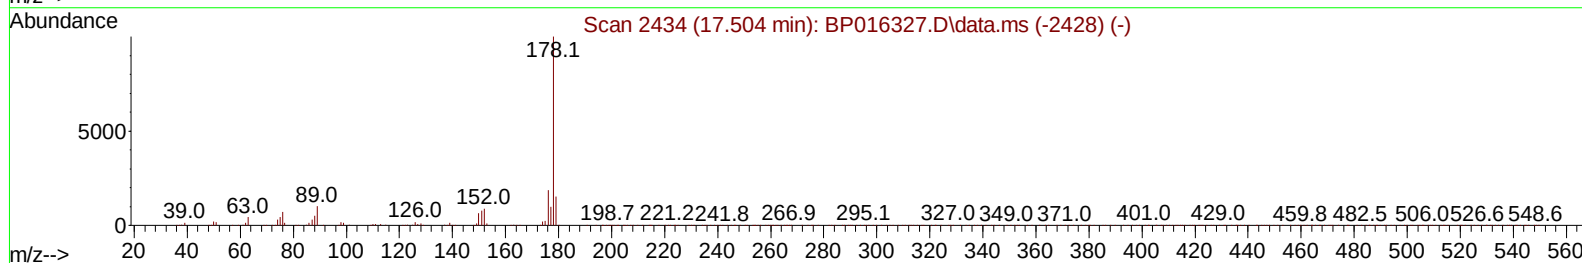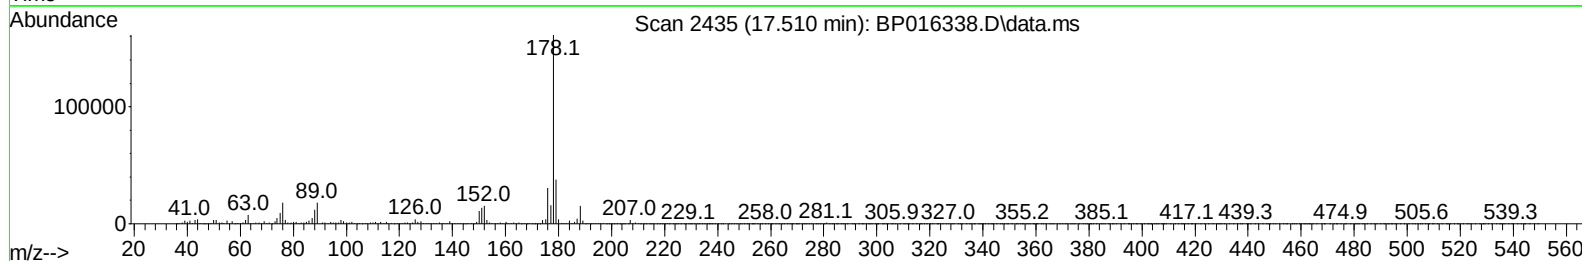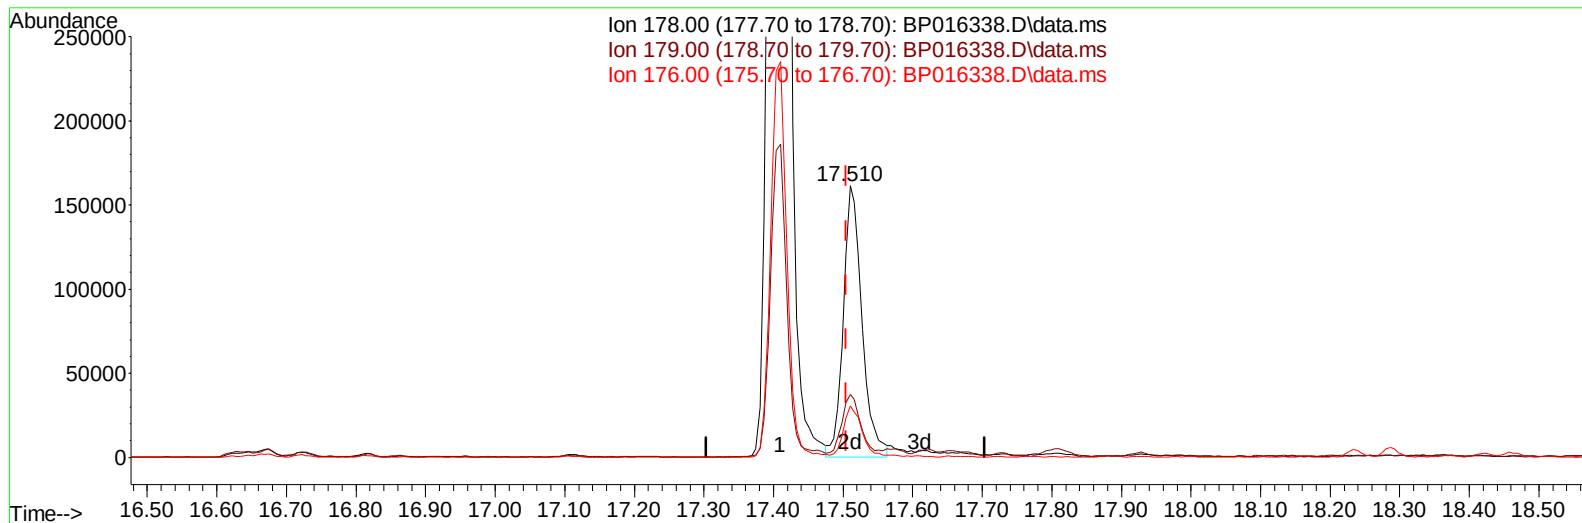

TIC: BP016338.D\data.ms

(74) Anthracene

17.510min (+ 0.006) 5.26 ng/ul m

response 302016

Ion	Exp%	Act%
178.00	100.00	100.00
179.00	14.90	23.25#
176.00	18.70	18.94
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071923\
 Data File : BP016338.D
 Acq On : 19 Jul 2023 23:17
 Operator : MA/JU
 Sample : 03472-24
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A46R5

Manual IntegrationsAPPROVED

Quant Time: Jul 20 00:32:11 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jul 19 14:47:57 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/20/2023
 Supervised By :mohammad ahmed 07/20/2023

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.946	152		119351	20.000	ng/ul	0.00
20) Naphthalene-d8	10.763	136		577242	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.598	164		389459	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.363	188		1097435	20.000	ng/ul	0.00
79) Chrysene-d12	21.457	240		1046372	20.000	ng/ul	0.00
88) Perylene-d12	23.951	264		1041843	20.000	ng/ul	0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.281	96		8040	2.384	ng/uL	0.00
4) Pyridine-d5	3.705	84		78709m	9.357	ng/ul	-0.02
7) Phenol-d5	7.175	99		71195	6.604	ng/ul	0.04
9) Bis-(2-Chloroethyl)eth...	7.287	67		70521	9.674	ng/ul	0.01
11) 2-Chlorophenol-d4	7.499	132		76428	9.821	ng/ul	0.02
15) 4-Methylphenol-d8	8.787	113		25507m	2.937	ng/ul	0.10
21) Nitrobenzene-d5	9.175	128		36235	9.099	ng/ul	0.04
24) 2-Nitrophenol-d4	9.904	143		46940m	10.342	ng/ul	0.04
28) 2,4-Dichlorophenol-d3	10.510	165		67689m	8.612	ng/ul	0.09
31) 4-Chloroaniline-d4	0.000	131		0d	0.000	ng/ul	
46) Dimethylphthalate-d6	14.028	166		339469	11.427	ng/ul	0.02
49) Acenaphthylene-d8	14.298	160		299212	9.190	ng/ul	0.00
54) 4-Nitrophenol-d4	15.039	143		24986m	4.121	ng/ul	0.12
60) Fluorene-d10	15.604	176		312980	12.588	ng/ul	0.01
65) 4,6-Dinitro-2-methylph...	15.839	200		21254m	3.355	ng/ul	0.06
73) Anthracene-d10	17.475	188		456484	9.509	ng/ul	0.00
81) Pyrene-d10	19.704	212		239334	4.408	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.792	264		82111	1.641	ng/ul	0.00
Target Compounds							
							Qvalue
8) Phenol	7.216	94		15120m	1.308	ng/ul	
16) Acetophenone	8.834	105		71915m	5.022	ng/ul	
30) Naphthalene	10.816	128		90557	2.989	ng/ul	98
36) 2-Methylnaphthalene	12.469	142		35114	1.729	ng/ul	95
37) 1-Methylnaphthalene	12.669	142		27078	1.296	ng/ul#	98
52) Acenaphthene	14.669	153		105289	4.163	ng/ul	100
56) Dibenzofuran	15.028	168		91579	2.658	ng/ul	91
61) Fluorene	15.669	166		144243	5.012	ng/ul	99
72) Phenanthrene	17.410	178		1986999	34.749	ng/ul	99
74) Anthracene	17.510	178		302016m	5.256	ng/ul	
80) Fluoranthene	19.375	202		2048848	32.269	ng/ul	100
82) Pyrene	19.733	202		590693	8.714	ng/ul	98
85) Benzo(a)anthracene	21.445	228		762016	11.183	ng/ul	99
86) Bis(2-ethylhexyl)phtha...	21.321	149		110016	2.519	ng/ul	100
87) Chrysene	21.498	228		716609	10.382	ng/ul	99
90) Benzo(b)fluoranthene	23.192	252		646053	10.856	ng/ul	98
91) Benzo(k)fluoranthene	23.239	252		254579	4.204	ng/ul	99
95) Dibenzo(a,h)anthracene	26.604	278		61168	1.027	ng/ul	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071923\
Data File : BP016338.D
Acq On : 19 Jul 2023 23:17
Operator : MA/JU
Sample : 03472-24
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A46R5

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 07/20/2023
Supervised By :mohammad ahmed 07/20/2023

Quant Time: Jul 20 00:32:11 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jul 19 14:47:57 2023
Response via : Initial Calibration

