

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071923\
 Data File : BP016319.D
 Acq On : 19 Jul 2023 11:57
 Operator : MA/JU
 Sample : PB154069BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK069

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP016319.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.276	12	15	22	rVB	47534	68580	1.25%	0.139%
2	3.728	90	92	109	rBV	392252	880777	16.01%	1.789%
3	4.040	143	145	153	rVB7	10544	18902	0.34%	0.038%
4	7.152	664	674	691	rVV	299488	1057534	19.22%	2.148%
5	7.281	691	696	721	rVV	351454	931796	16.94%	1.893%
6	7.487	724	731	759	rVB	410421	1046422	19.02%	2.126%
7	7.952	803	810	834	rBV	278575	844013	15.34%	1.714%
8	8.211	851	854	858	rVB5	4786	6139	0.11%	0.012%
9	8.381	880	883	888	rVB7	5360	8636	0.16%	0.018%
10	8.705	928	938	974	rBV	352611	1319266	23.98%	2.680%
11	9.152	1007	1014	1043	rBV	439550	1319189	23.98%	2.680%
12	9.887	1130	1139	1162	rBV2	290260	1111281	20.20%	2.257%
13	10.475	1232	1239	1253	rBV	264086	1102474	20.04%	2.239%
14	10.775	1283	1290	1309	rVB	578264	1443445	26.24%	2.932%
15	10.981	1317	1325	1358	rBV	284667	1373856	24.97%	2.791%
16	12.457	1569	1576	1583	rBV10	6604	19657	0.36%	0.040%
17	12.516	1583	1586	1593	rVV9	3629	6613	0.12%	0.013%
18	13.493	1746	1752	1759	rBV6	7705	18026	0.33%	0.037%
19	13.610	1767	1772	1777	rVB8	3465	5743	0.10%	0.012%
20	14.028	1833	1843	1872	rBV	1171753	2764766	50.25%	5.616%
21	14.304	1882	1890	1923	rBV	1716292	3114802	56.61%	6.327%
22	14.604	1934	1941	1959	rBV	1188229	2039771	37.07%	4.143%
23	14.969	1994	2003	2025	rBV3	121809	803116	14.60%	1.631%
24	15.616	2106	2113	2134	rBV	1695830	3911392	71.09%	7.945%
25	15.804	2139	2145	2178	rBV	297001	1233220	22.41%	2.505%
26	17.040	2352	2355	2362	rVB8	5216	8980	0.16%	0.018%
27	17.369	2405	2411	2423	rBV	1661037	2575557	46.81%	5.232%
28	17.475	2423	2429	2458	rVB	1799983	4444805	80.79%	9.029%
29	18.251	2557	2561	2571	rBV4	34262	94460	1.72%	0.192%
30	19.292	2734	2738	2742	rBV4	36262	51259	0.93%	0.104%
31	19.369	2748	2751	2756	rBV	28186	40912	0.74%	0.083%
32	19.475	2766	2769	2778	rBV5	26603	60672	1.10%	0.123%
33	19.710	2803	2809	2832	rBV	2703300	5501764	100.00%	11.176%
34	21.480	3105	3110	3125	rBV2	1245789	2612039	47.48%	5.306%
35	23.792	3496	3503	3522	rVB2	1970897	4726873	85.92%	9.602%
36	23.957	3525	3531	3554	rVB	846646	2663582	48.41%	5.410%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071923\
Data File : BP016319.D
Acq On : 19 Jul 2023 11:57
Operator : MA/JU
Sample : PB154069BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK069

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 49230319

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071923\
Data File : BP016319.D
Acq On : 19 Jul 2023 11:57
Operator : MA/JU
Sample : PB154069BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK069

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

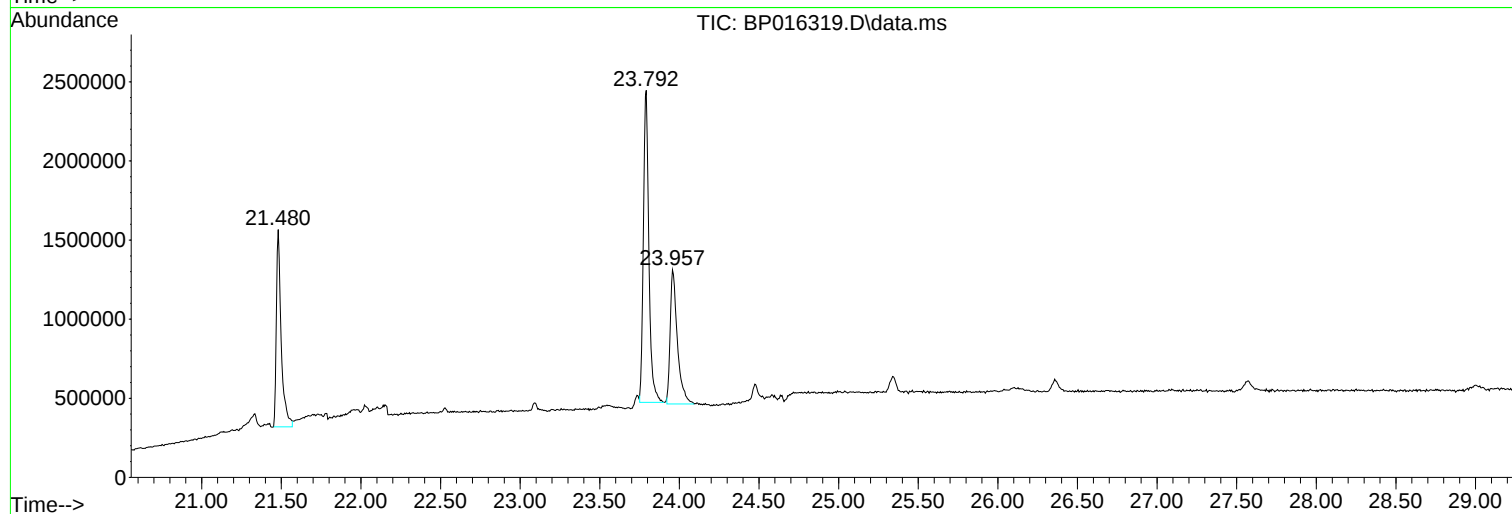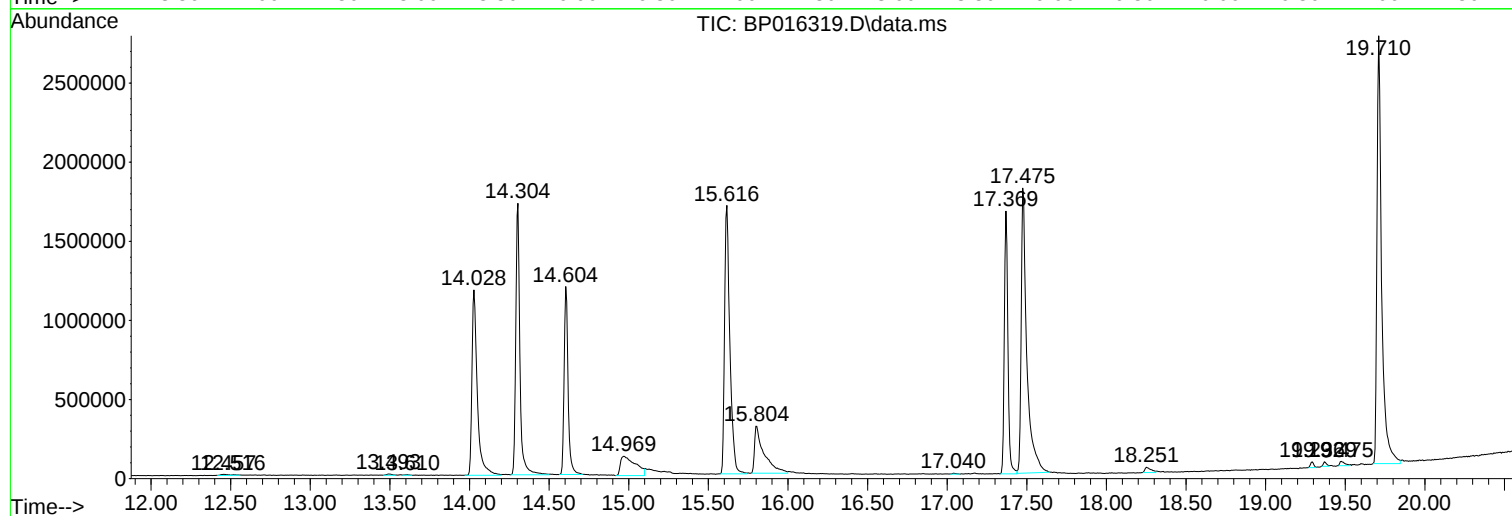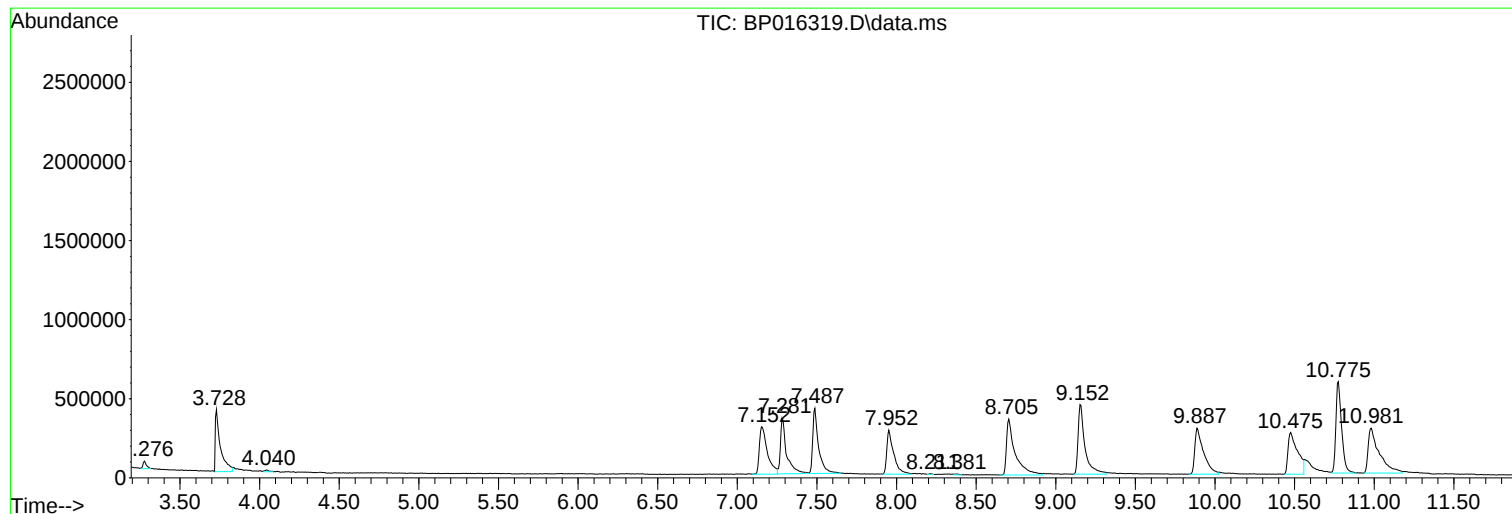

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071923\
Data File : BP016319.D
Acq On : 19 Jul 2023 11:57
Operator : MA/JU
Sample : PB154069BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK069

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071923\
Data File : BP016319.D
Acq On : 19 Jul 2023 11:57
Operator : MA/JU
Sample : PB154069BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK069

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071223.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc