

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP072220\
 Data File : BP002823.D
 Acq On : 22 Jul 2020 13:54
 Operator : CG/JU
 Sample : PB130369BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB130369BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP071020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.175	383	389	414	rBV	1948077	2960295	56.45%	11.366%
2	6.752	650	657	678	rBV	1704382	2937855	56.02%	11.280%
3	7.546	785	792	805	rBV	399013	624041	11.90%	2.396%
4	8.693	980	987	1018	rBV	1085743	1955168	37.28%	7.507%
5	10.316	1254	1263	1285	rBV	436978	832146	15.87%	3.195%
6	12.810	1680	1687	1712	rBV	2353603	3849345	73.40%	14.780%
7	14.198	1915	1923	1941	rBV	628375	1040797	19.85%	3.996%
8	15.704	2173	2179	2211	rBV	1269581	2634604	50.24%	10.116%
9	16.963	2386	2393	2409	rBV	735537	1215366	23.18%	4.667%
10	19.551	2827	2833	2851	rBV	3905532	5244018	100.00%	20.135%
11	20.874	3054	3058	3064	rBV	29726	53157	1.01%	0.204%
12	21.074	3087	3092	3103	rBV	998145	1345955	25.67%	5.168%
13	23.262	3458	3464	3480	rVB2	661219	1351387	25.77%	5.189%


Sum of corrected areas: 26044134

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP072220\
Data File : BP002823.D
Acq On : 22 Jul 2020 13:54
Operator : CG/JU
Sample : PB130369BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB130369BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP071020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

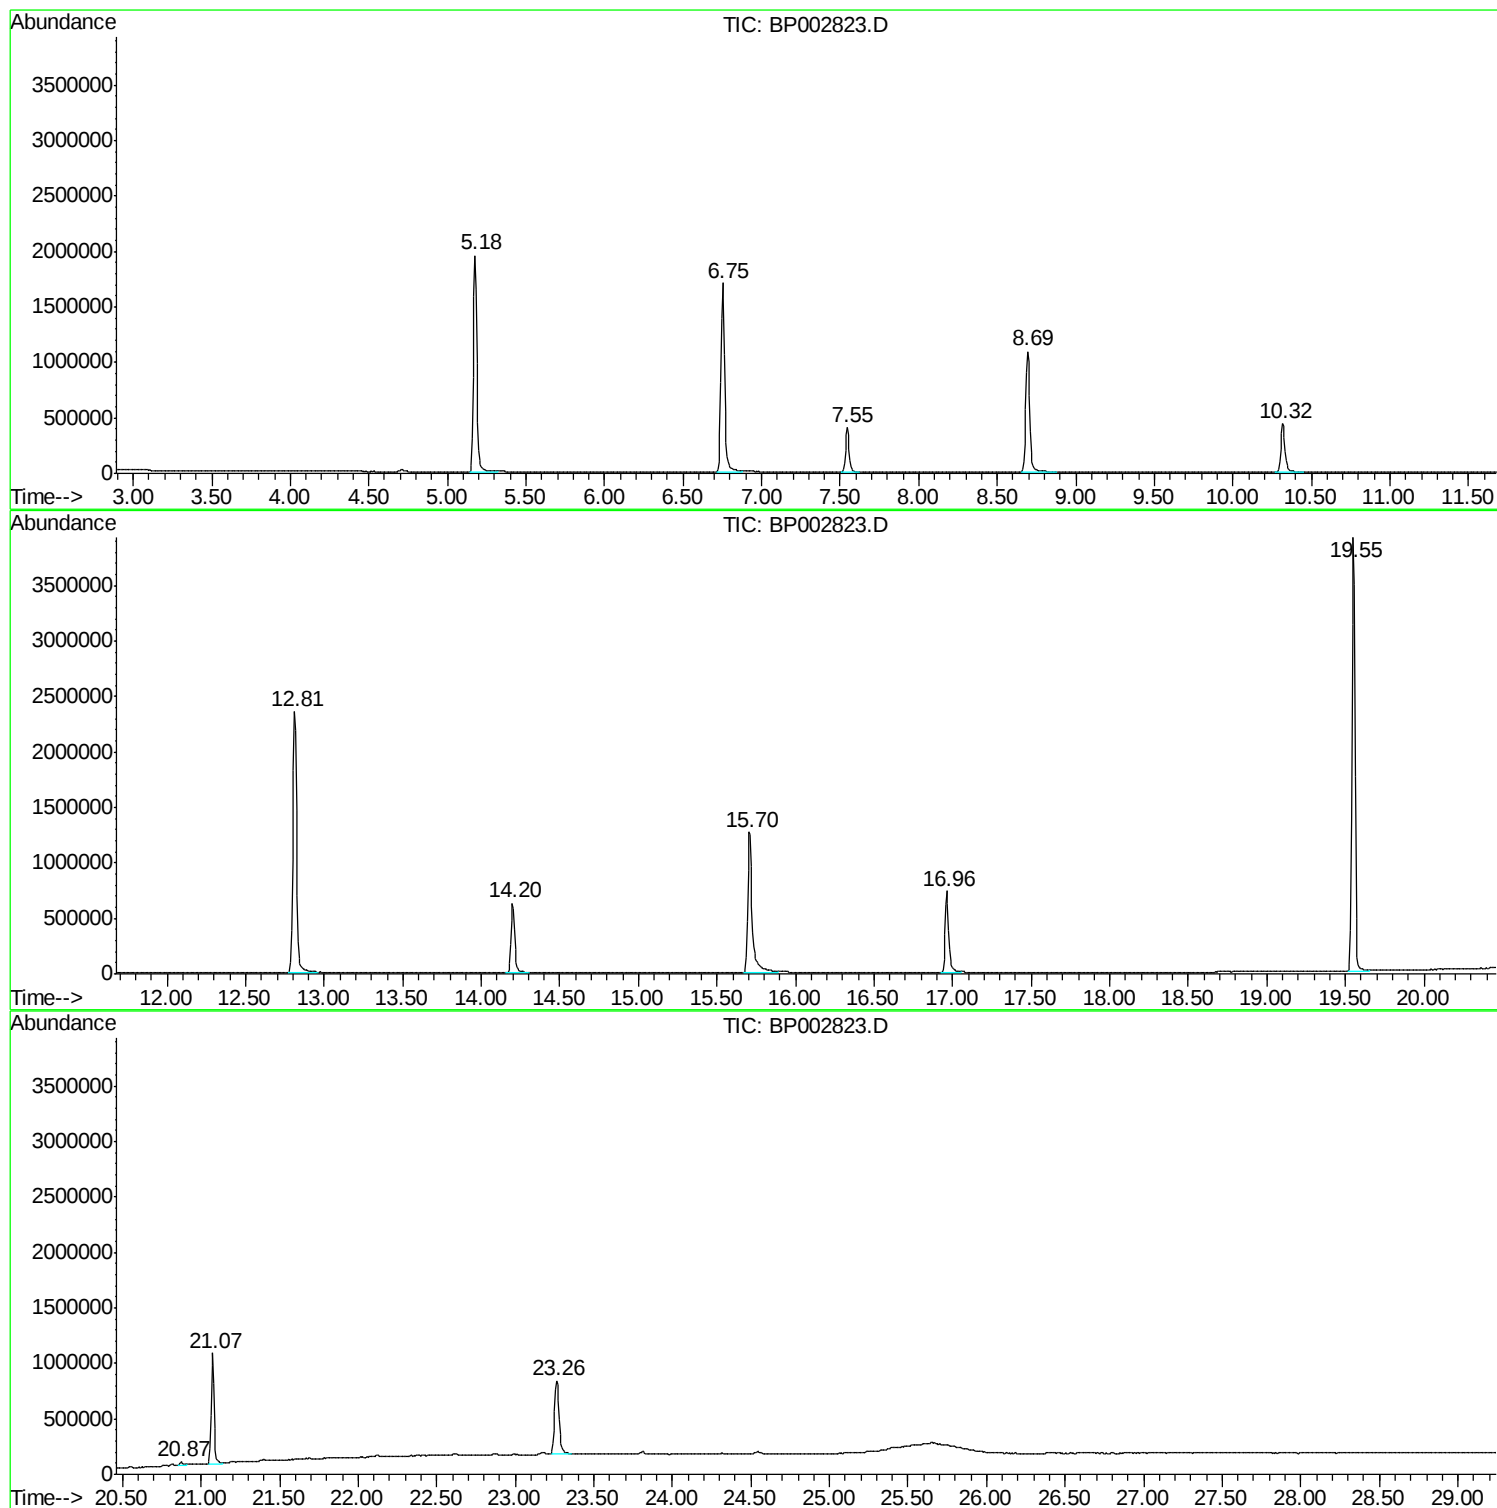

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP072220\
Data File : BP002823.D
Acq On : 22 Jul 2020 13:54
Operator : CG/JU
Sample : PB130369BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB130369BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP071020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP072220\
Data File : BP002823.D
Acq On : 22 Jul 2020 13:54
Operator : CG/JU
Sample : PB130369BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB130369BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP071020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc