

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072523\
 Data File : BP016343.D
 Acq On : 25 Jul 2023 10:44
 Operator : MA/JU
 Sample : SSTD00502
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SSTD005604

Quant Time: Jul 25 23:27:31 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP072523.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jul 25 16:07:21 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.096	152	319960	20.000	ng/ul	0.00
20) Naphthalene-d8	10.931	136	1405782	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.748	164	876356	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.513	188	1938788	20.000	ng/ul	0.00
79) Chrysene-d12	21.607	240	1782521	20.000	ng/ul	0.00
88) Perylene-d12	24.218	264	2034372	20.000	ng/ul	0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.419	96	16456	2.028	ng/uL	-0.01
4) Pyridine-d5	3.849	84	107340	4.662	ng/ul	0.00
7) Phenol-d5	7.219	99	119151	4.450	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.425	67	77223	4.804	ng/ul	-0.01
11) 2-Chlorophenol-d4	7.607	132	92155	4.412	ng/ul	0.00
15) 4-Methylphenol-d8	8.784	113	92431	4.293	ng/ul	-0.01
21) Nitrobenzene-d5	9.290	128	30559	3.530	ng/ul	0.00
24) 2-Nitrophenol-d4	10.007	143	19927	2.791	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.531	165	82376	4.163	ng/ul	0.00
31) 4-Chloroaniline-d4	11.078	131	148166	4.813	ng/ul	0.00
46) Dimethylphthalate-d6	14.154	166	303837	4.737	ng/ul	0.00
49) Acenaphthylene-d8	14.442	160	356961	4.711	ng/ul	0.00
54) 4-Nitrophenol-d4	14.919	143	25673	2.389	ng/ul	0.00
60) Fluorene-d10	15.736	176	263057	4.821	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.848	200	10083	1.579	ng/ul	0.00
73) Anthracene-d10	17.613	188	406522	4.734	ng/ul	0.00
81) Pyrene-d10	19.836	212	464671	4.591	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.042	264	439536	4.478	ng/ul	0.00
Target Compounds						
2) 1,4-Dioxane	3.461	88	16883	1.962	ng/uL#	90
5) Pyridine	3.872	79	113065	4.827	ng/ul	98
6) Benzaldehyde	7.243	77	87686	6.003	ng/ul	93
8) Phenol	7.243	94	127519	4.580	ng/ul	97
10) Bis(2-Chloroethyl)ether	7.525	93	110830	4.859	ng/ul	97
12) 2-Chlorophenol	7.643	128	98732	4.597	ng/ul	98
13) 2-Methylphenol	8.519	108	97794	4.580	ng/ul	98
14) 2,2'-oxybis(1-Chloropr...	8.613	45	91298	3.307	ng/ul	98
16) Acetophenone	8.937	105	174538	5.136	ng/ul	97
17) N-Nitroso-di-n-propyla...	8.907	70	84034	4.749	ng/ul	96
18) 4-Methylphenol	8.849	108	102742	4.504	ng/ul	97
19) Hexachloroethane	9.172	117	42902	4.775	ng/ul	98
22) Nitrobenzene	9.331	77	90104	3.888	ng/ul	97
23) Isophorone	9.843	82	249271	4.775	ng/ul	99
25) 2-Nitrophenol	10.037	139	24218	2.719	ng/ul	93
26) 2,4-Dimethylphenol	10.072	107	116727	4.634	ng/ul	99
27) Bis(2-Chloroethoxy)met...	10.337	93	151410	4.811	ng/ul	99
29) 2,4-Dichlorophenol	10.554	162	84573	4.228	ng/ul	99
30) Naphthalene	10.984	128	354085	4.863	ng/ul	100
32) 4-Chloroaniline	11.101	127	149356	4.949	ng/ul	100
33) Hexachlorobutadiene	11.225	225	62137	4.726	ng/ul	98
34) Caprolactam	11.872	113	29656	4.017	ng/ul	96
35) 4-Chloro-3-methylphenol	12.190	107	96087	4.339	ng/ul	97
36) 2-Methylnaphthalene	12.578	142	238950	4.816	ng/ul	98

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072523\
 Data File : BP016343.D
 Acq On : 25 Jul 2023 10:44
 Operator : MA/JU
 Sample : SSTD00502
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SSTD005604

Quant Time: Jul 25 23:27:31 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP072523.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jul 25 16:07:21 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.795	142	237080	4.779	ng/ul	99
39) 1,2,4,5-Tetrachloroben...	12.925	216	121601	4.697	ng/ul	98
40) Hexachlorocyclopentadiene	12.884	237	58559	3.168	ng/ul#	97
41) 2,4,6-Trichlorophenol	13.172	196	59881	3.925	ng/ul	99
42) 2,4,5-Trichlorophenol	13.237	196	61555	3.771	ng/ul	99
43) 1,1'-Biphenyl	13.584	154	320761	4.847	ng/ul	100
44) 2-Chloronaphthalene	13.631	162	248305	4.797	ng/ul	99
45) 2-Nitroaniline	13.842	65	30967	2.859	ng/ul	91
47) Dimethylphthalate	14.201	163	316829	4.898	ng/ul	100
48) 2,6-Dinitrotoluene	14.337	165	24946	2.676	ng/ul#	91
50) Acenaphthylene	14.472	152	420127	4.867	ng/ul	99
51) 3-Nitroaniline	14.666	138	29194	2.677	ng/ul#	81
52) Acenaphthene	14.807	153	271947	4.886	ng/ul	99
53) 2,4-Dinitrophenol	14.860	184	6573	1.649	ng/ul	91
55) 4-Nitrophenol	14.937	109	28139	3.248	ng/ul	94
56) Dibenzofuran	15.148	168	380907	4.999	ng/ul	98
57) 2,4-Dinitrotoluene	15.113	165	31659	2.382	ng/ul	92
58) 2,3,4,6-Tetrachlorophenol	15.354	232	48752	3.743	ng/ul	95
59) Diethylphthalate	15.560	149	314798	4.832	ng/ul	100
61) Fluorene	15.795	166	312776	5.053	ng/ul	99
62) 4-Chlorophenyl-phenyle...	15.789	204	150239	4.979	ng/ul	94
63) 4-Nitroaniline	15.831	138	28342	2.834	ng/ul#	78
66) 4,6-Dinitro-2-methylph...	15.860	198	11351	1.487	ng/ul#	76
67) N-Nitrosodiphenylamine	16.007	169	258604	4.757	ng/ul	99
68) 4-Bromophenyl-phenylether	16.695	248	85080	4.627	ng/ul	99
69) Hexachlorobenzene	16.772	284	104795	4.753	ng/ul	98
70) Atrazine	16.960	200	86747	4.374	ng/ul	99
71) Pentachlorophenol	17.131	266	36272	2.919	ng/ul	98
72) Phenanthrene	17.554	178	495000	4.906	ng/ul	99
74) Anthracene	17.648	178	508948	4.952	ng/ul	99
75) 1,2,3,4-Tetrachloroben...	13.537	216	125674	4.491	ng/ul	97
76) Pentachlorobenzene	15.037	250	114894	4.646	ng/ul	99
77) Carbazole	17.919	167	445109	5.032	ng/ul	99
78) Di-n-butylphthalate	18.448	149	525741	4.667	ng/ul	99
80) Fluoranthene	19.507	202	567158	4.675	ng/ul	97
82) Pyrene	19.866	202	599251	4.781	ng/ul	100
83) Butylbenzylphthalate	20.736	149	184051	3.879	ng/ul	95
84) 3,3'-Dichlorobenzidine	21.519	252	151928	3.878	ng/ul	100
85) Benzo(a)anthracene	21.589	228	580645	4.809	ng/ul	99
86) Bis(2-ethylhexyl)phtha...	21.495	149	312898	4.323	ng/ul	100
87) Chrysene	21.642	228	538469	4.816	ng/ul	100
89) Di-n-octyl phthalate	22.501	149	505156	3.950	ng/ul	100
90) Benzo(b)fluoranthene	23.401	252	566770	4.652	ng/ul	99
91) Benzo(k)fluoranthene	23.454	252	548581	4.525	ng/ul	99
93) Benzo(a)pyrene	24.095	252	526393	4.588	ng/ul	98
94) Indeno(1,2,3-cd)pyrene	26.995	276	609967	4.604	ng/ul	99
95) Dibenzo(a,h)anthracene	27.036	278	499913	4.562	ng/ul	100
96) Benzo(g,h,i)perylene	27.859	276	500178	4.768	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072523\
 Data File : BP016343.D
 Acq On : 25 Jul 2023 10:44
 Operator : MA/JU
 Sample : SST00502
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SST005604

Quant Time: Jul 25 23:27:31 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP072523.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jul 25 16:07:21 2023
 Response via : Initial Calibration




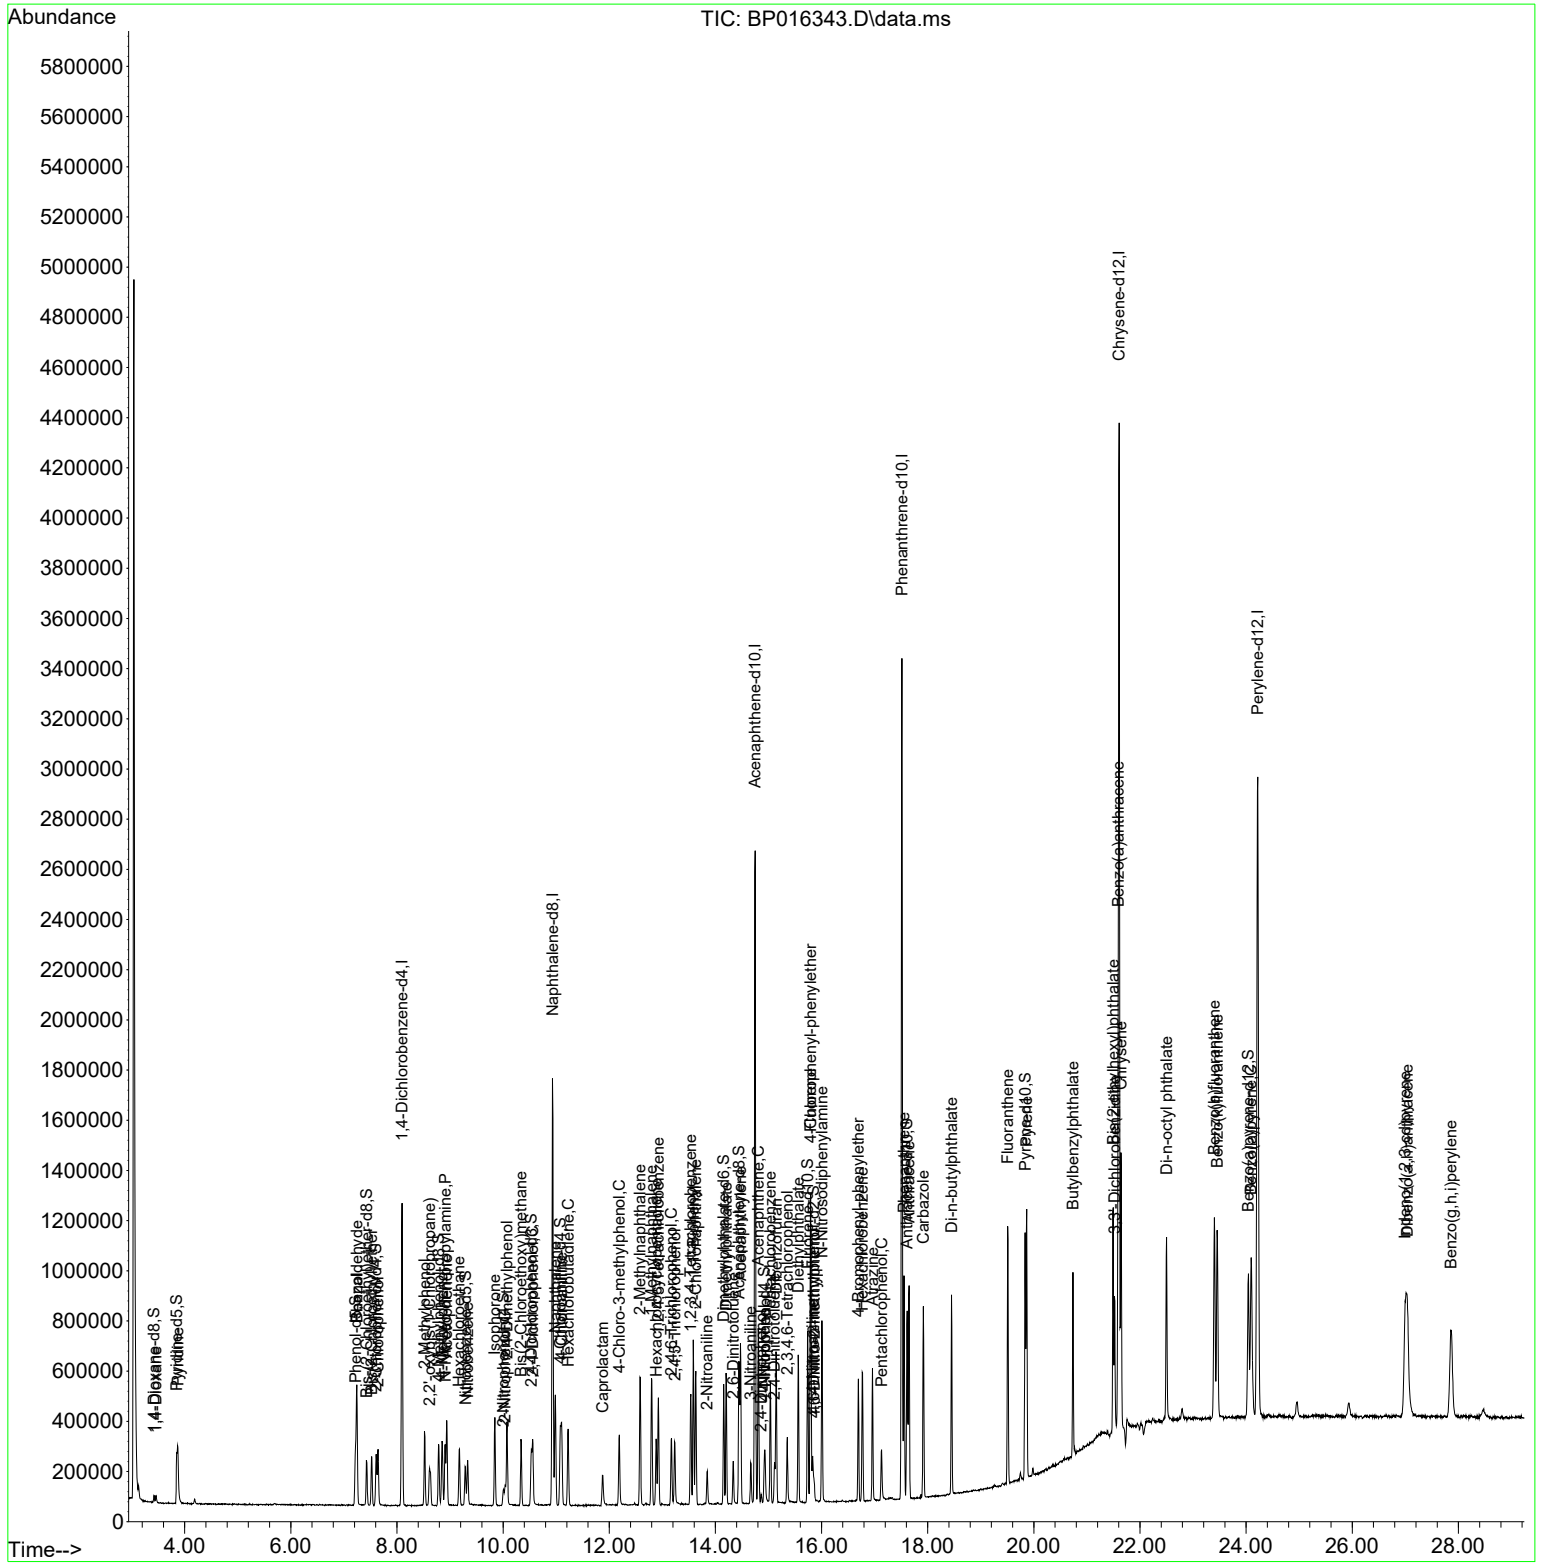




#2
 1,4-Dioxane
 Concen: 1.962 ng/uL
 RT: 3.461 min Scan# 89
 Delta R.T. -0.006 min
 Lab File: BP016343.D
 Acq: 25 Jul 2023 10:44




Instrument :
 BNA_P
 ClientSampleId :
 SSTD005604


Tgt Ion: 88 Resp: 16883
 Ion Ratio Lower Upper
 88 100
 43 33.4 21.8 32.8#
 58 73.6 53.1 79.7

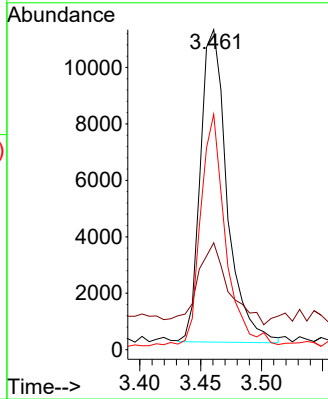

#5
 Pyridine
 Concen: 4.827 ng/uL
 RT: 3.872 min Scan# 159
 Delta R.T. -0.006 min
 Lab File: BP016343.D
 Acq: 25 Jul 2023 10:44

Tgt Ion: 79 Resp: 113065
 Ion Ratio Lower Upper
 79 100
 52 65.2 51.0 76.4
 51 33.0 25.4 38.2


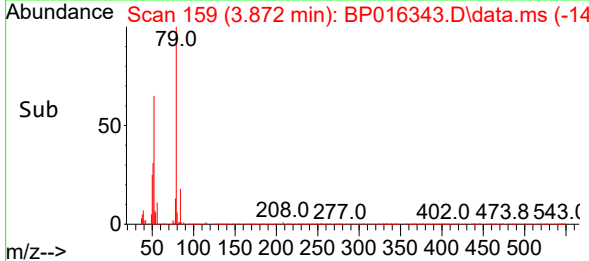
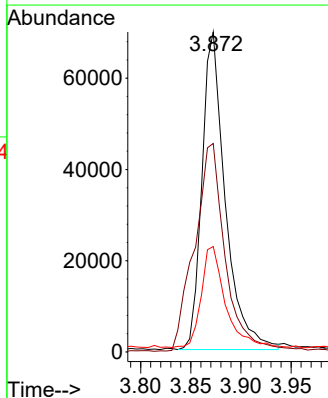



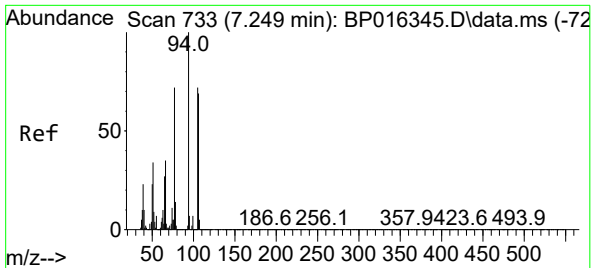

#6
 Benzaldehyde
 Concen: 6.003 ng/u1
 RT: 7.243 min Scan# 71
 Delta R.T. -0.006 min
 Lab File: BP016343.D
 Acq: 25 Jul 2023 10:44




Instrument : BNA_P
 ClientSampleId : SSTD005604


Tgt Ion	Resp	Lower	Upper
77	87686		
77	100		
105	94.5	80.2	120.2
106	88.4	76.5	114.7

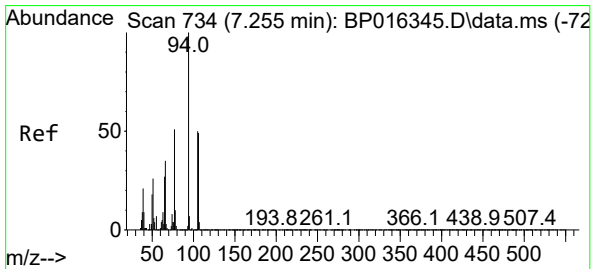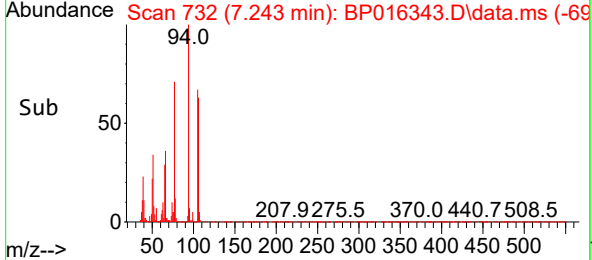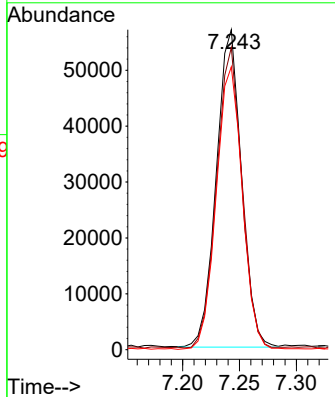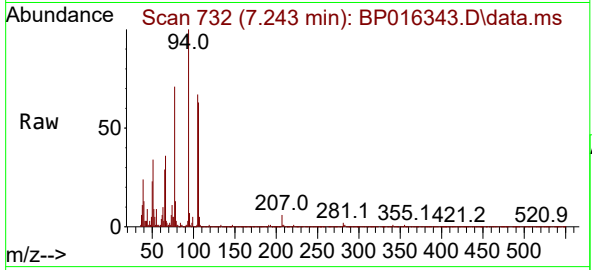

#8
 Phenol
 Concen: 4.580 ng/u1
 RT: 7.243 min Scan# 732
 Delta R.T. -0.012 min
 Lab File: BP016343.D
 Acq: 25 Jul 2023 10:44

Tgt Ion	Resp	Lower	Upper
94	127519		
94	100		
65	29.4	21.4	32.2
66	35.9	28.2	42.4

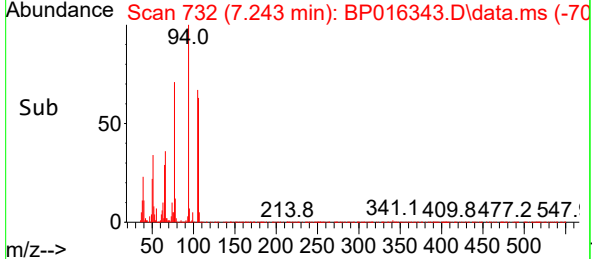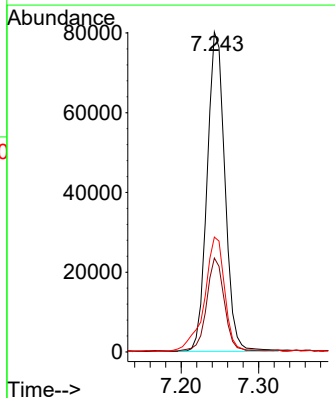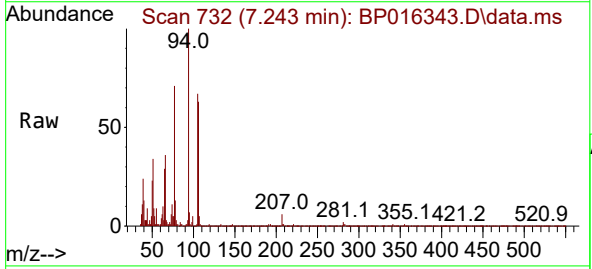




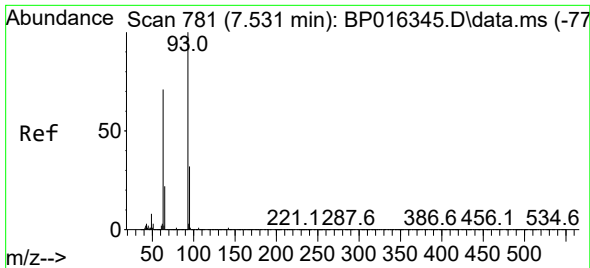


#10
 Bis(2-Chloroethyl)ether
 Concen: 4.859 ng/ul
 RT: 7.525 min Scan# 781
 Delta R.T. -0.006 min
 Lab File: BP016343.D
 Acq: 25 Jul 2023 10:44

Instrument :
 BNA_P
 ClientSampleId :
 SSTD005604

Tgt Ion: 93 Resp: 110830




Ion	Ratio	Lower	Upper
93	100		
63	68.3	57.0	85.4
95	32.9	25.8	38.6

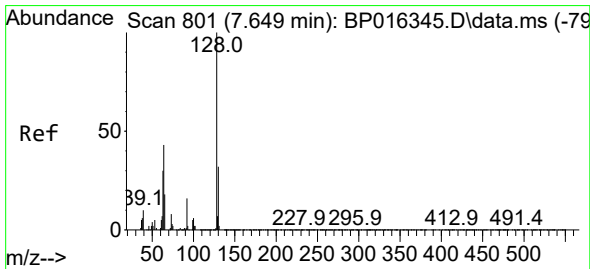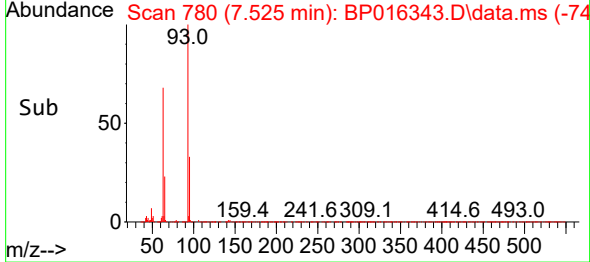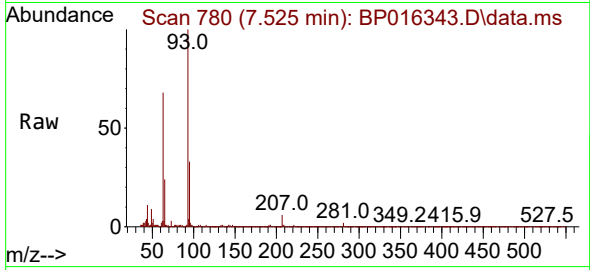


#12
 2-Chlorophenol
 Concen: 4.597 ng/ul
 RT: 7.643 min Scan# 800
 Delta R.T. -0.006 min
 Lab File: BP016343.D
 Acq: 25 Jul 2023 10:44

Tgt Ion: 128 Resp: 98732

Ion	Ratio	Lower	Upper
128	100		
64	45.0	36.4	54.6
130	33.9	25.6	38.4


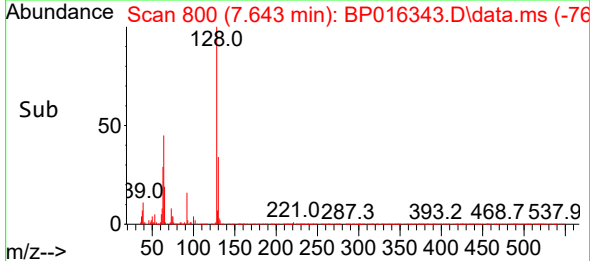

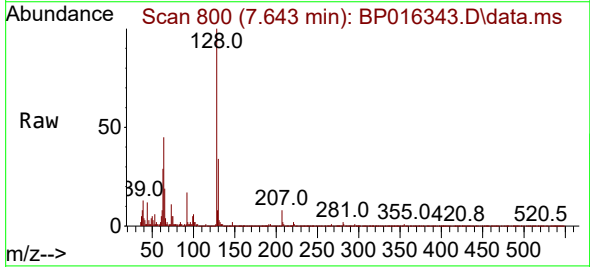


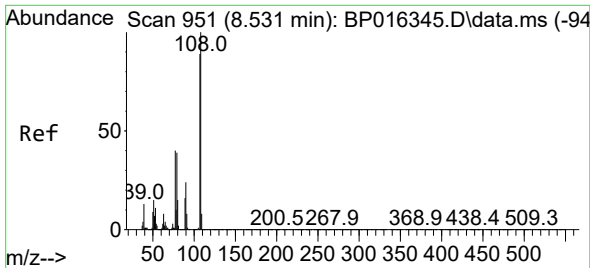

#13
 2-Methylphenol
 Concen: 4.580 ng/ul
 RT: 8.519 min Scan# 949
 Delta R.T. -0.012 min
 Lab File: BP016343.D
 Acq: 25 Jul 2023 10:44




Instrument :
 BNA_P
 ClientSampleId :
 SSTD005604


Tgt Ion:108 Resp: 97794
 Ion Ratio Lower Upper
 108 100
 107 91.1 71.3 106.9

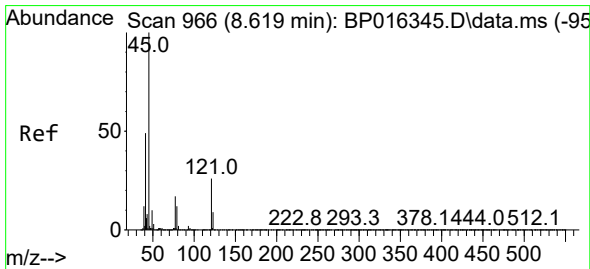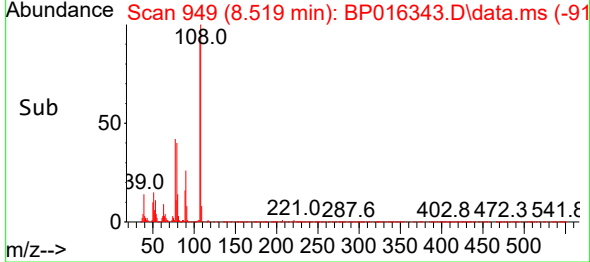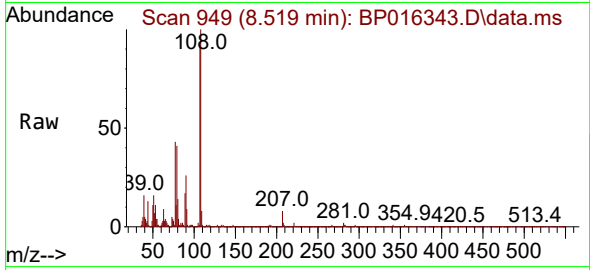

#14
 2,2'-oxybis(1-Chloropropane)
 Concen: 3.307 ng/ul
 RT: 8.613 min Scan# 965
 Delta R.T. -0.006 min
 Lab File: BP016343.D
 Acq: 25 Jul 2023 10:44


Tgt Ion: 45 Resp: 91298
 Ion Ratio Lower Upper
 45 100
 77 17.8 13.7 20.5
 79 13.3 9.6 14.4

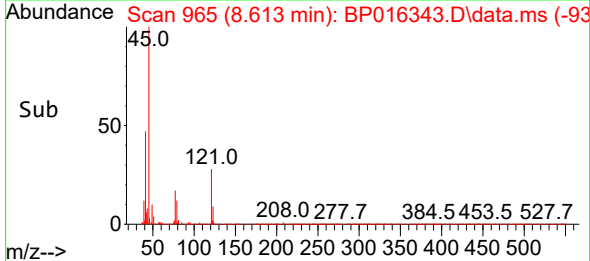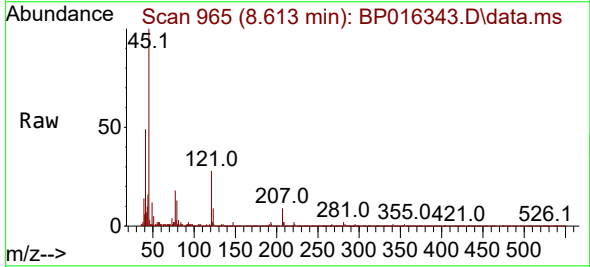



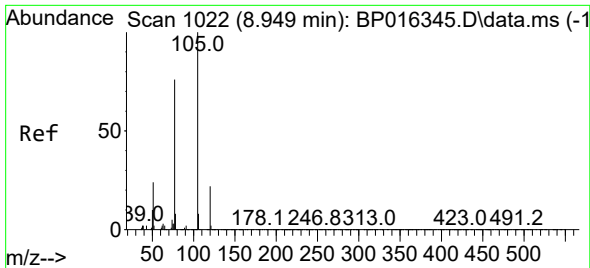


#16
 Acetophenone
 Concen: 5.136 ng/ul
 RT: 8.937 min Scan# 1020
 Delta R.T. -0.012 min
 Lab File: BP016343.D
 Acq: 25 Jul 2023 10:44


Instrument : BNA_P
 ClientSampleId : SSTD005604

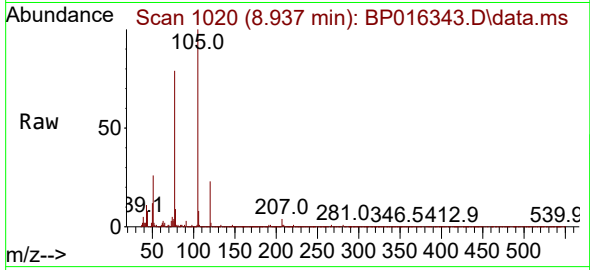



Tgt Ion: 105 Resp: 174538
 Ion Ratio Lower Upper
 105 100
 77 78.8 61.2 91.8
 51 26.0 19.1 28.7

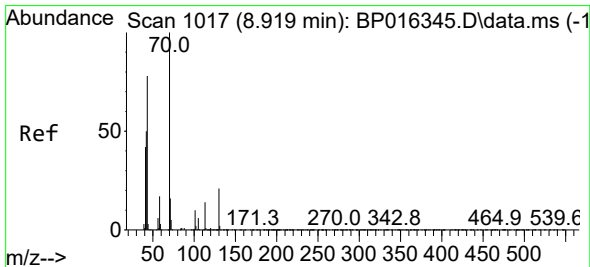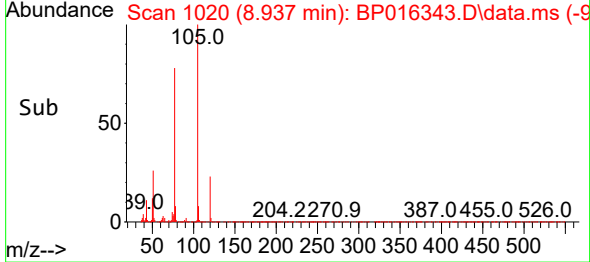


#17
 N-Nitroso-di-n-propylamine
 Concen: 4.749 ng/ul
 RT: 8.907 min Scan# 1015
 Delta R.T. -0.012 min
 Lab File: BP016343.D
 Acq: 25 Jul 2023 10:44

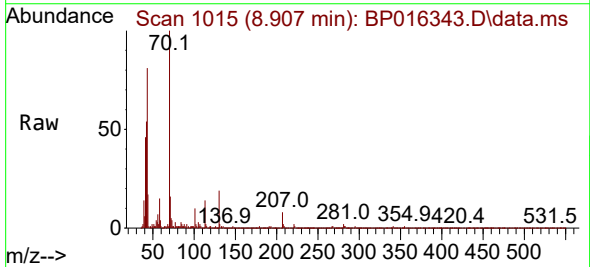

Tgt Ion: 70 Resp: 84034
 Ion Ratio Lower Upper
 70 100
 42 53.5 40.3 60.5
 101 10.3 7.8 11.8
 130 19.4 17.1 25.7



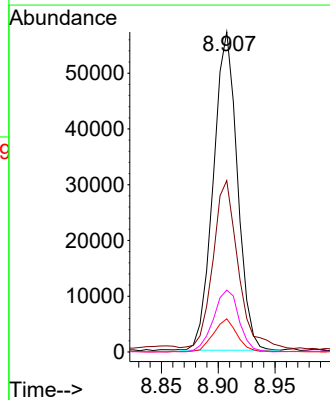
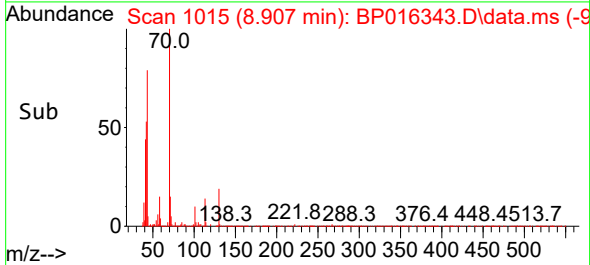


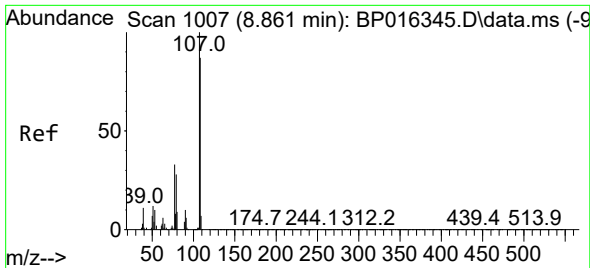

#18
 4-Methylphenol
 Concen: 4.504 ng/ul
 RT: 8.849 min Scan# 1005
 Delta R.T. -0.012 min
 Lab File: BP016343.D
 Acq: 25 Jul 2023 10:44




Instrument :
 BNA_P
 ClientSampleId :
 SSTD005604


Tgt Ion:108 Resp: 102742
 Ion Ratio Lower Upper
 108 100
 107 111.0 91.6 137.4

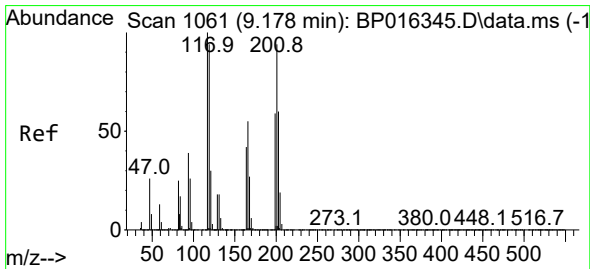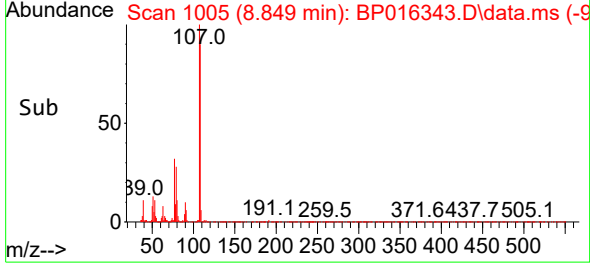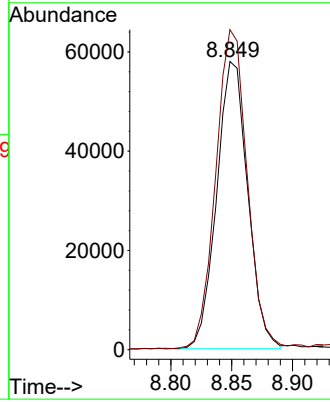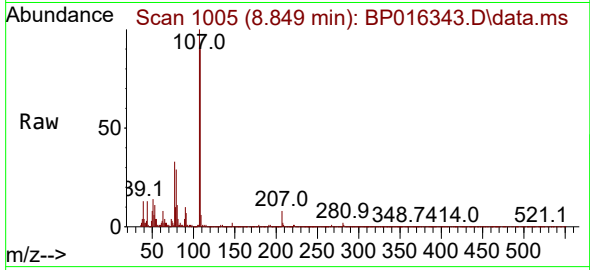

#19
 Hexachloroethane
 Concen: 4.775 ng/ul
 RT: 9.172 min Scan# 1060
 Delta R.T. -0.006 min
 Lab File: BP016343.D
 Acq: 25 Jul 2023 10:44

Tgt Ion:117 Resp: 42902
 Ion Ratio Lower Upper
 117 100
 201 92.2 75.0 112.6
 199 56.4 47.4 71.0

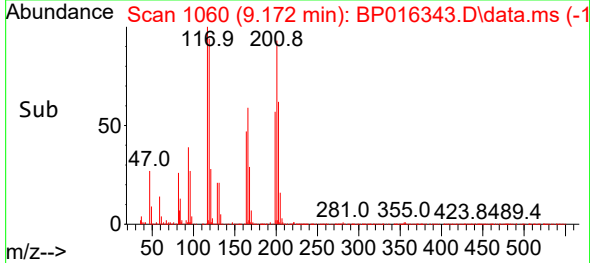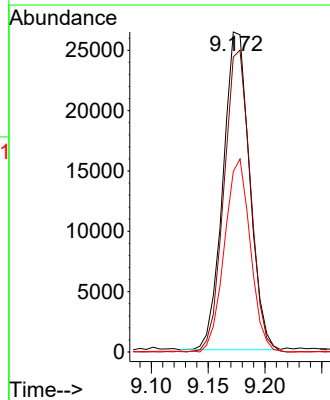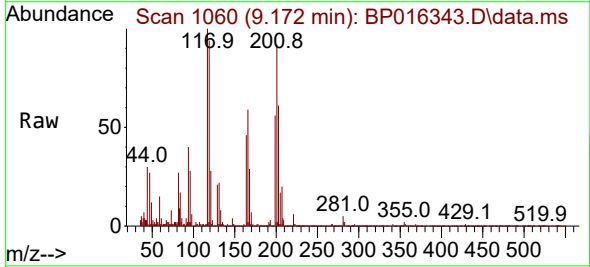




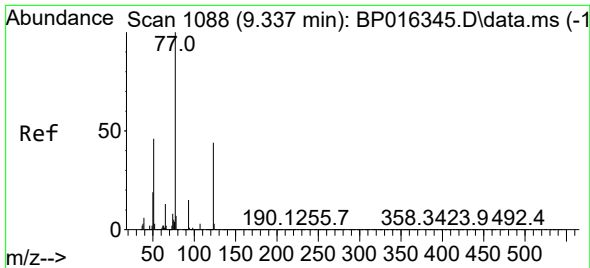


#22
 Nitrobenzene
 Concen: 3.888 ng/ul
 RT: 9.331 min Scan# 1087
 Delta R.T. -0.006 min
 Lab File: BP016343.D
 Acq: 25 Jul 2023 10:44

Instrument :
 BNA_P
 ClientSampleId :
 SSTD005604

Tgt Ion: 77 Resp: 90104




Ion	Ratio	Lower	Upper
77	100		
123	42.4	35.3	52.9
65	13.7	10.2	15.2

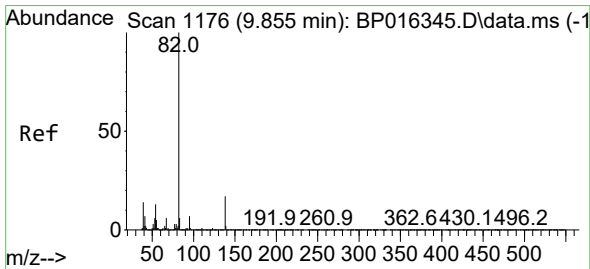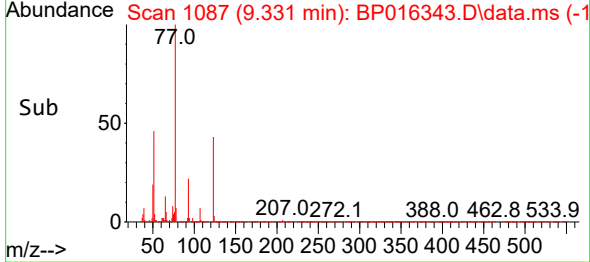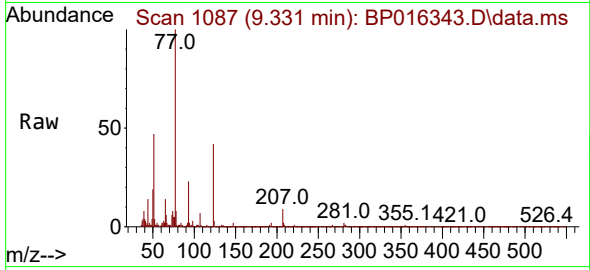


#23
 Isophorone
 Concen: 4.775 ng/ul
 RT: 9.843 min Scan# 1174
 Delta R.T. -0.012 min
 Lab File: BP016343.D
 Acq: 25 Jul 2023 10:44

Tgt Ion: 82 Resp: 249271

Ion	Ratio	Lower	Upper
82	100		
95	7.0	5.6	8.4
138	18.2	14.0	21.0


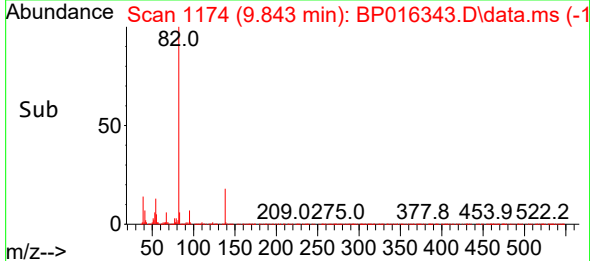

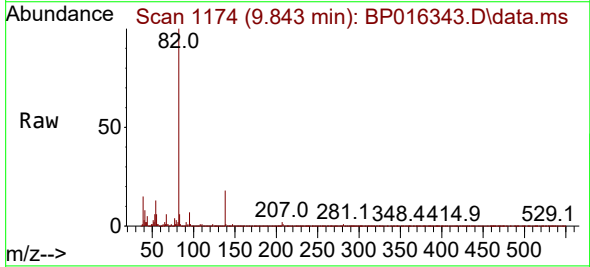




#25
 2-Nitrophenol
 Concen: 2.719 ng/ul
 RT: 10.037 min Scan# 111
 Delta R.T. -0.006 min
 Lab File: BP016343.D
 Acq: 25 Jul 2023 10:44




Instrument : BNA_P
 ClientSampleId : SSTD005604


Tgt Ion	Resp	Lower	Upper
139	24218	100	100
65	55.4	38.7	58.1
109	30.0	25.3	37.9



#26
 2,4-Dimethylphenol
 Concen: 4.634 ng/ul
 RT: 10.072 min Scan# 1213
 Delta R.T. -0.006 min
 Lab File: BP016343.D
 Acq: 25 Jul 2023 10:44

Tgt Ion	Resp	Lower	Upper
107	116727	100	100
121	50.7	39.8	59.6
122	87.3	69.0	103.4

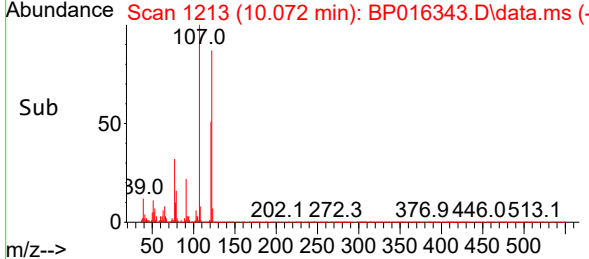







#27
 Bis(2-Chloroethoxy)methane
 Concen: 4.811 ng/ul
 RT: 10.337 min Scan# 11
 Delta R.T. -0.006 min
 Lab File: BP016343.D
 Acq: 25 Jul 2023 10:44

Instrument :
 BNA_P
 ClientSampleId :
 SSTD005604

Tgt Ion: 93 Resp: 151410




Ion	Ratio	Lower	Upper
93	100		
95	31.7	25.9	38.9
123	10.7	8.8	13.2




#29
 2,4-Dichlorophenol
 Concen: 4.228 ng/ul
 RT: 10.554 min Scan# 1295
 Delta R.T. -0.006 min
 Lab File: BP016343.D
 Acq: 25 Jul 2023 10:44

Tgt Ion: 162 Resp: 84573

Ion	Ratio	Lower	Upper
162	100		
164	63.2	51.4	77.0
98	37.1	30.6	46.0


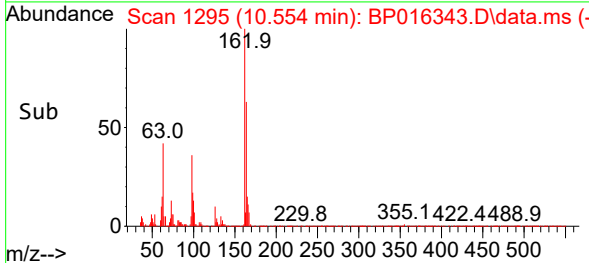




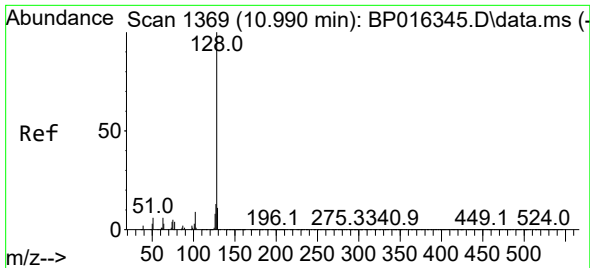

#30
 Naphthalene
 Concen: 4.863 ng/uI
 RT: 10.984 min Scan# 1368
 Delta R.T. -0.006 min
 Lab File: BP016343.D
 Acq: 25 Jul 2023 10:44




Instrument : BNA_P
 Client Sample Id : SSTD005604


Tgt Ion	Resp	Lower	Upper
128	354085		
129	11.1	8.7	13.1
127	13.3	10.6	15.8

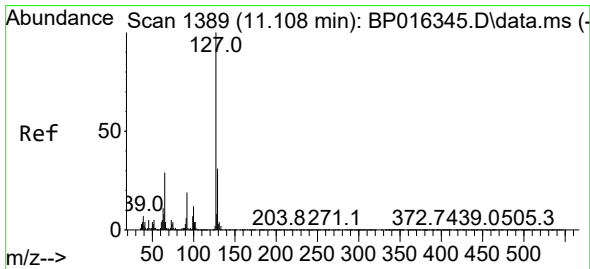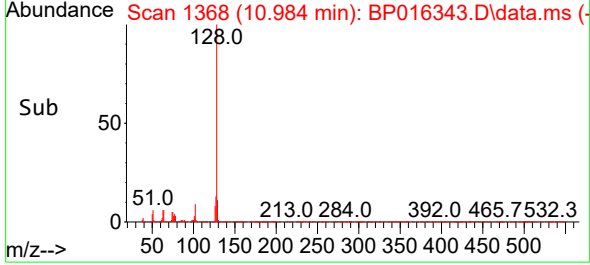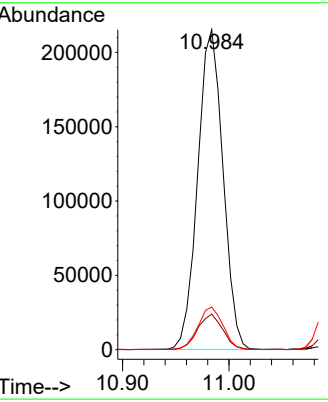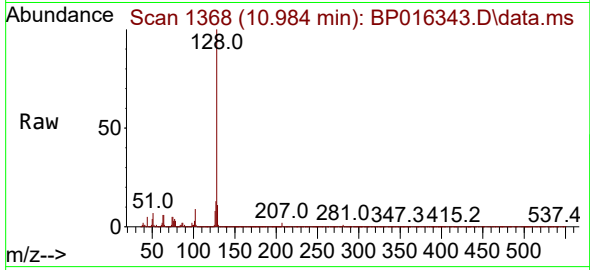

#32
 4-Chloroaniline
 Concen: 4.949 ng/uI
 RT: 11.101 min Scan# 1388
 Delta R.T. -0.006 min
 Lab File: BP016343.D
 Acq: 25 Jul 2023 10:44


Tgt Ion	Resp	Lower	Upper
127	149356		
129	31.3	25.2	37.8

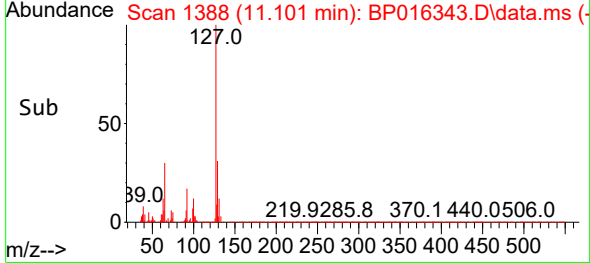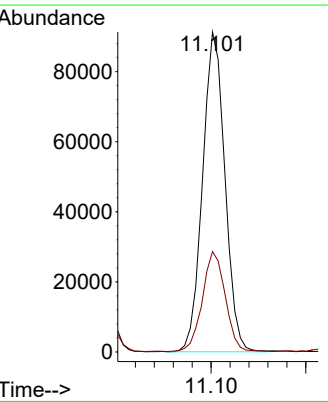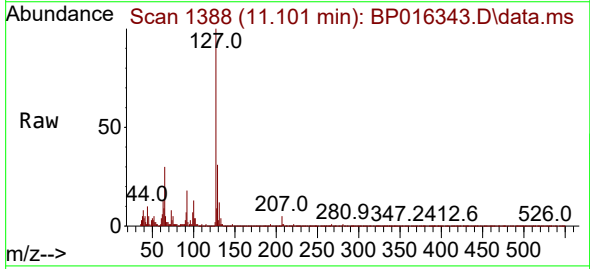






#33
 Hexachlorobutadiene
 Concen: 4.726 ng/uI
 RT: 11.225 min Scan# 1409
 Delta R.T. -0.000 min
 Lab File: BP016343.D
 Acq: 25 Jul 2023 10:44


Instrument :
 BNA_P
 ClientSampleId :
 SSTD005604





Tgt Ion:225 Resp: 62137
 Ion Ratio Lower Upper
 225 100
 223 61.3 50.1 75.1
 227 63.1 51.5 77.3

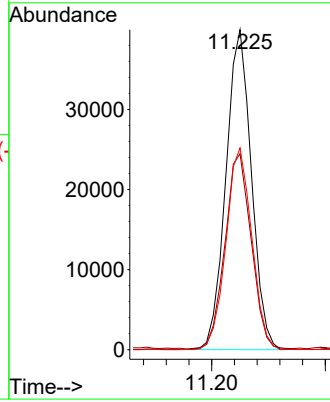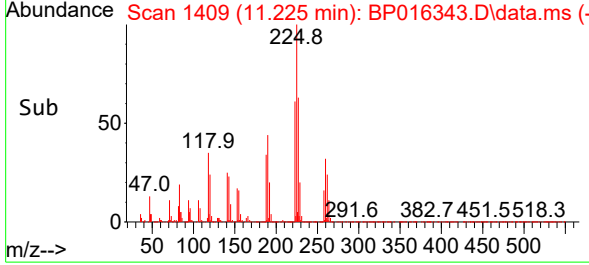


#34
 Caprolactam
 Concen: 4.017 ng/uI
 RT: 11.872 min Scan# 1519
 Delta R.T. -0.018 min
 Lab File: BP016343.D
 Acq: 25 Jul 2023 10:44



Tgt Ion:113 Resp: 29656
 Ion Ratio Lower Upper
 113 100
 55 158.4 122.2 183.4
 56 121.2 93.8 140.8



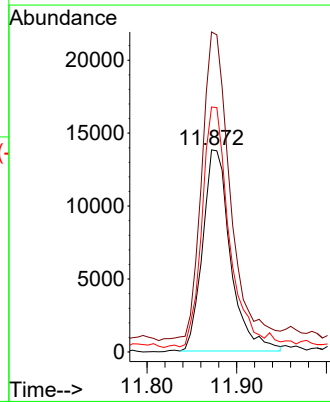
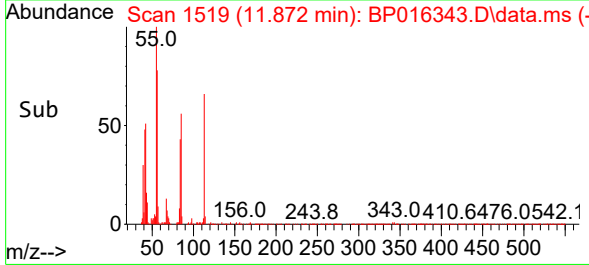




#35
 4-Chloro-3-methylphenol
 Concen: 4.339 ng/ul
 RT: 12.190 min Scan# 11
 Delta R.T. -0.000 min
 Lab File: BP016343.D
 Acq: 25 Jul 2023 10:44




Instrument :
 BNA_P
 ClientSampleId :
 SSTD005604


Tgt Ion	Resp	Lower	Upper
107	96087		
107	100		
144	24.6	20.2	30.2
142	80.9	62.6	93.8

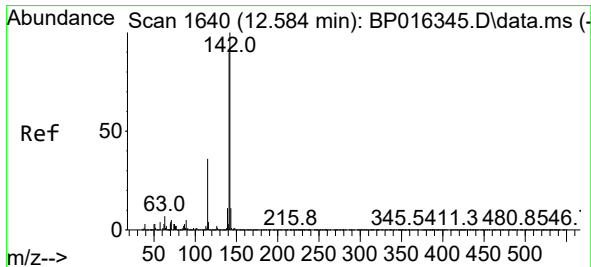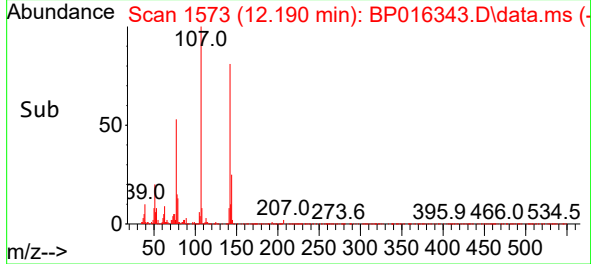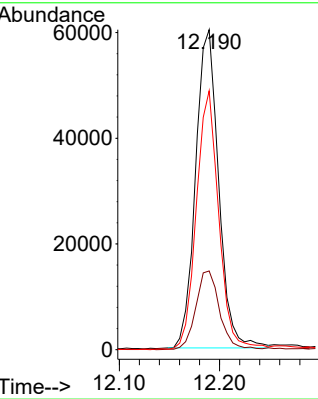

#36
 2-Methylnaphthalene
 Concen: 4.816 ng/ul
 RT: 12.578 min Scan# 1639
 Delta R.T. -0.006 min
 Lab File: BP016343.D
 Acq: 25 Jul 2023 10:44

Tgt Ion	Resp	Lower	Upper
142	238950		
142	100		
141	87.8	71.9	107.9

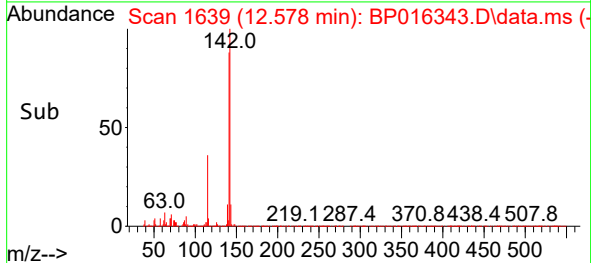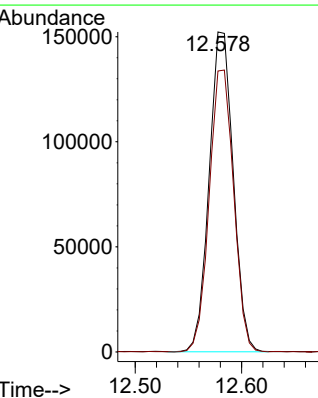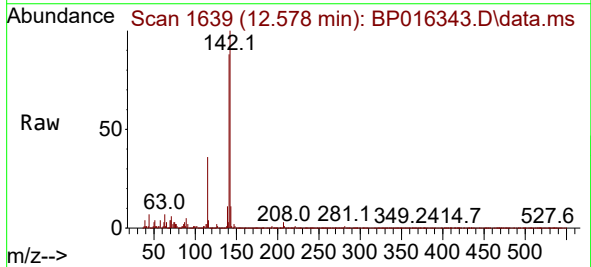







#37
 1-Methylnaphthalene
 Concen: 4.779 ng/ul
 RT: 12.795 min Scan# 1676
 Delta R.T. -0.006 min
 Lab File: BP016343.D
 Acq: 25 Jul 2023 10:44

Instrument : BNA_P
 ClientSampleId : SSTD005604

Tgt Ion:142 Resp: 237080




Ion	Ratio	Lower	Upper
142	100		
141	92.0	73.2	109.8
116	3.9	3.0	4.6




#39
 1,2,4,5-Tetrachlorobenzene
 Concen: 4.697 ng/ul
 RT: 12.925 min Scan# 1698
 Delta R.T. -0.000 min
 Lab File: BP016343.D
 Acq: 25 Jul 2023 10:44

Tgt Ion:216 Resp: 121601

Ion	Ratio	Lower	Upper
216	100		
214	77.9	63.6	95.4
179	21.4	17.4	26.0
108	19.4	14.6	21.8


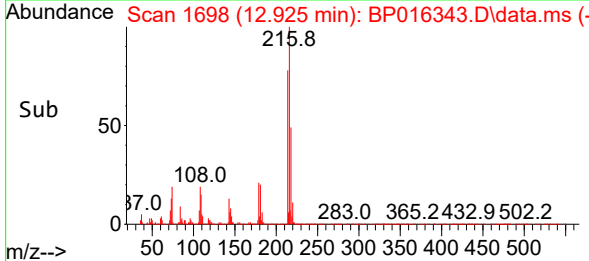




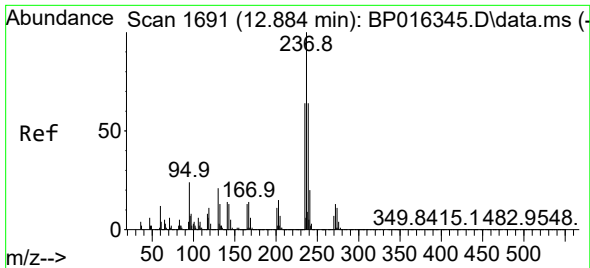

#40
 Hexachlorocyclopentadiene
 Concen: 3.168 ng/ul
 RT: 12.884 min Scan# 1691
 Delta R.T. -0.000 min
 Lab File: BP016343.D
 Acq: 25 Jul 2023 10:44




Instrument : BNA_P
 ClientSampleId : SSTD005604


Tgt Ion	Resp	Lower	Upper
237	100		
235	66.0	51.2	76.8
272	10.1	10.3	15.5#

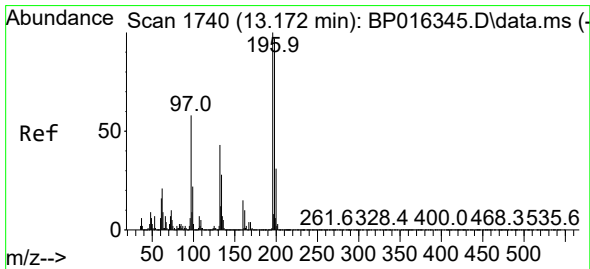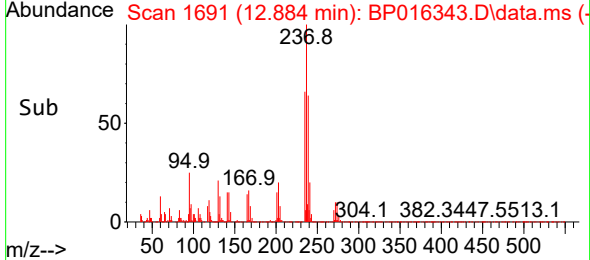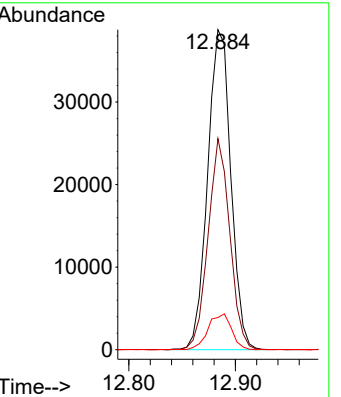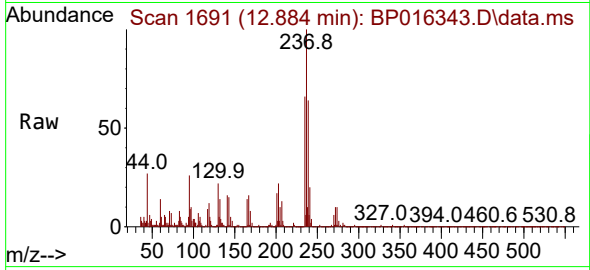

#41
 2,4,6-Trichlorophenol
 Concen: 3.925 ng/ul
 RT: 13.172 min Scan# 1740
 Delta R.T. -0.000 min
 Lab File: BP016343.D
 Acq: 25 Jul 2023 10:44

Tgt Ion	Resp	Lower	Upper
196	100		
198	96.1	77.7	116.5
200	32.2	25.0	37.6


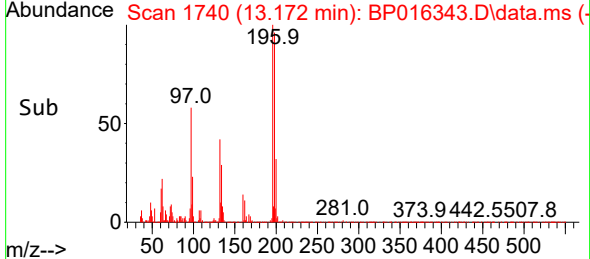
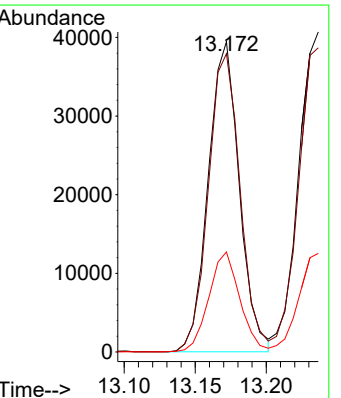
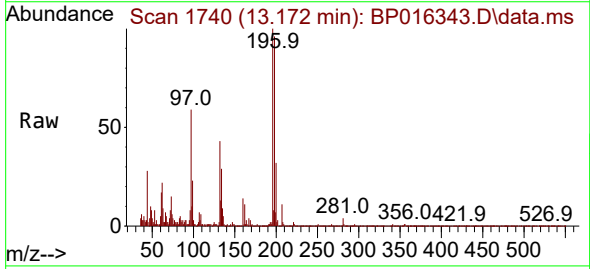


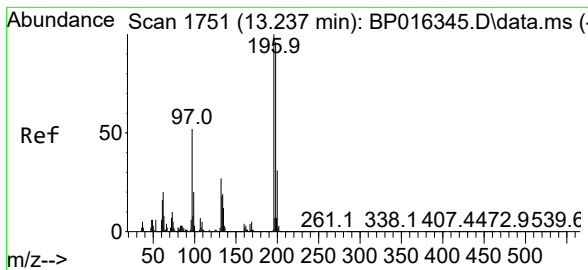

#42
 2,4,5-Trichlorophenol
 Concen: 3.771 ng/ul
 RT: 13.237 min Scan# 1751
 Delta R.T. -0.000 min
 Lab File: BP016343.D
 Acq: 25 Jul 2023 10:44




Instrument : BNA_P
 ClientSampleId : SSTD005604


Tgt Ion	Resp	Lower	Upper
196	100		
198	95.1	77.0	115.4
200	30.8	24.8	37.2

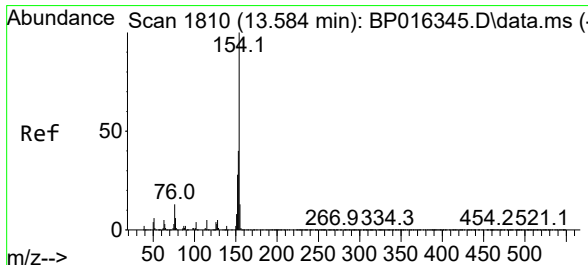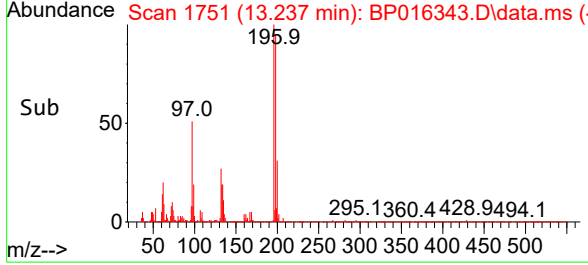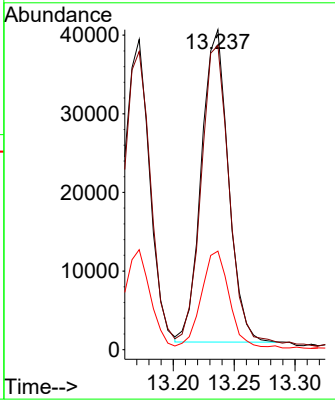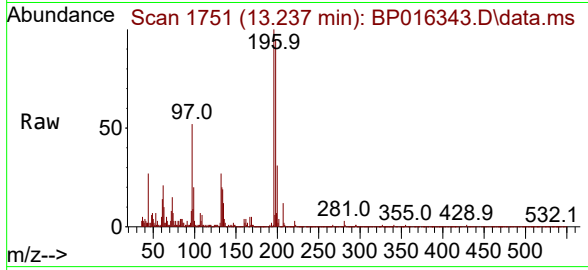

#43
 1,1'-Biphenyl
 Concen: 4.847 ng/ul
 RT: 13.584 min Scan# 1810
 Delta R.T. -0.000 min
 Lab File: BP016343.D
 Acq: 25 Jul 2023 10:44

Tgt Ion	Resp	Lower	Upper
154	100		
153	40.5	32.3	48.5
76	13.9	10.7	16.1


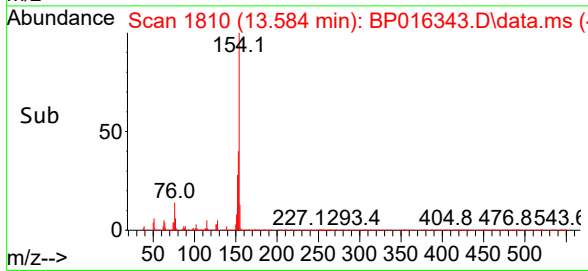
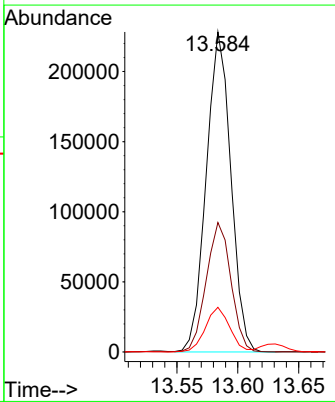
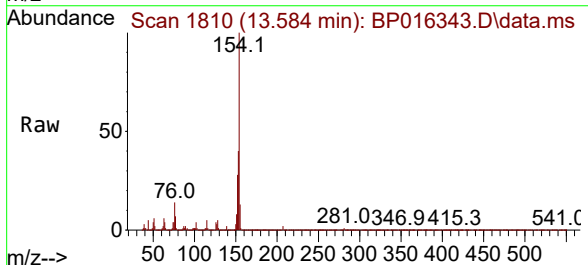




#44
 2-Chloronaphthalene
 Concen: 4.797 ng/ul
 RT: 13.631 min Scan# 1818
 Delta R.T. -0.000 min
 Lab File: BP016343.D
 Acq: 25 Jul 2023 10:44




Instrument : BNA_P
 Client Sample Id : SSTD005604


Tgt Ion	Resp	Lower	Upper
162	248305		
162	100		
164	32.9	26.6	40.0
127	39.4	31.0	46.4

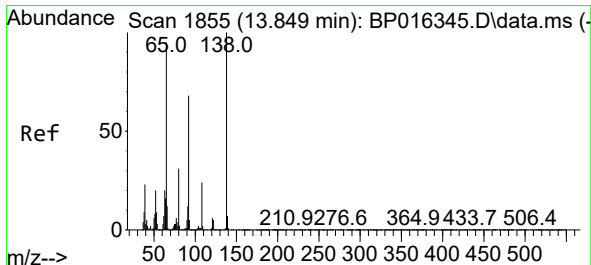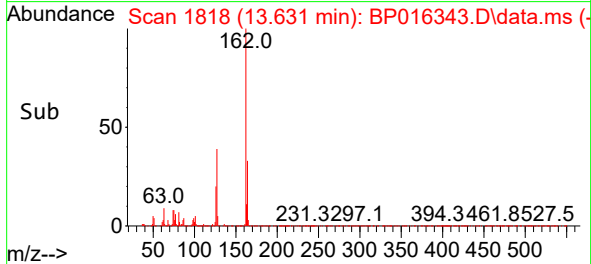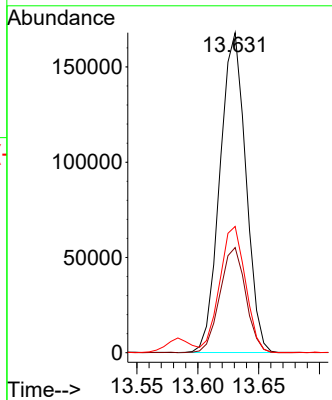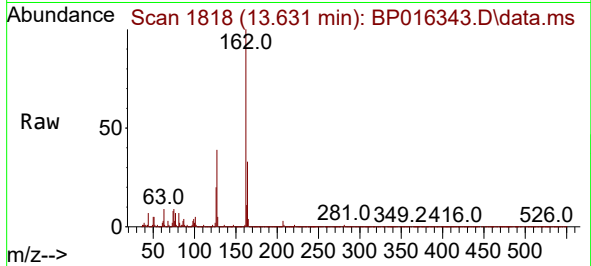

#45
 2-Nitroaniline
 Concen: 2.859 ng/ul
 RT: 13.842 min Scan# 1854
 Delta R.T. -0.006 min
 Lab File: BP016343.D
 Acq: 25 Jul 2023 10:44

Tgt Ion	Resp	Lower	Upper
65	30967		
65	100		
92	68.7	56.8	85.2
138	91.5	83.9	125.9


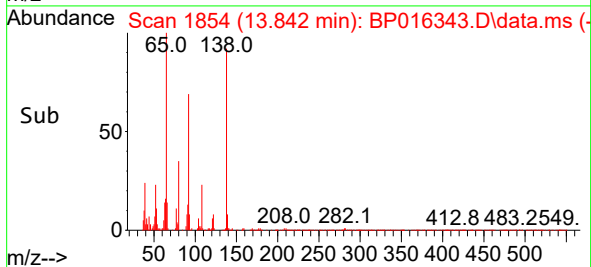
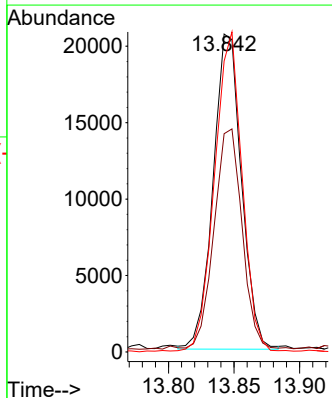
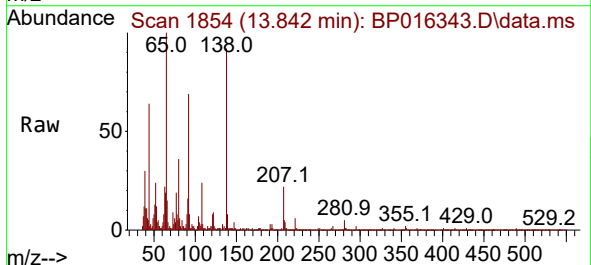




#47
 Dimethylphthalate
 Concen: 4.898 ng/ul
 RT: 14.201 min Scan# 1915
 Delta R.T. -0.006 min
 Lab File: BP016343.D
 Acq: 25 Jul 2023 10:44




Instrument :
 BNA_P
 ClientSampleId :
 SSTD005604


Tgt Ion:163 Resp: 316829
 Ion Ratio Lower Upper
 163 100
 194 4.3 3.3 4.9
 164 9.9 7.9 11.9

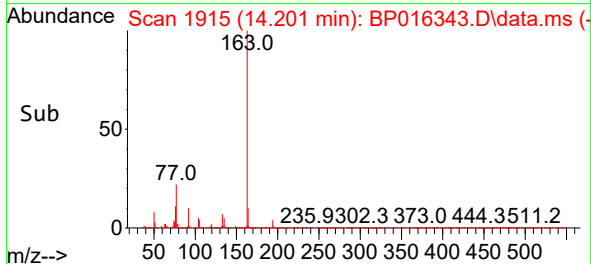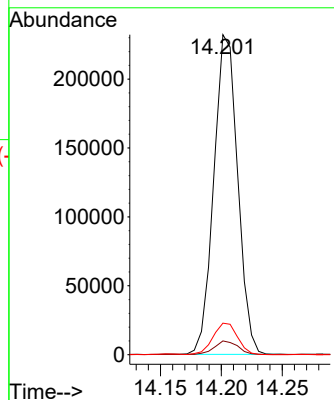

#48
 2,6-Dinitrotoluene
 Concen: 2.676 ng/ul
 RT: 14.337 min Scan# 1938
 Delta R.T. -0.000 min
 Lab File: BP016343.D
 Acq: 25 Jul 2023 10:44

Tgt Ion:165 Resp: 24946
 Ion Ratio Lower Upper
 165 100
 89 73.4 53.8 80.6
 121 31.4 20.0 30.0#

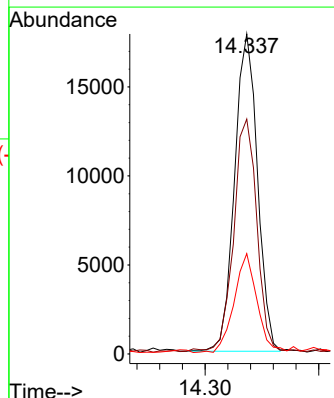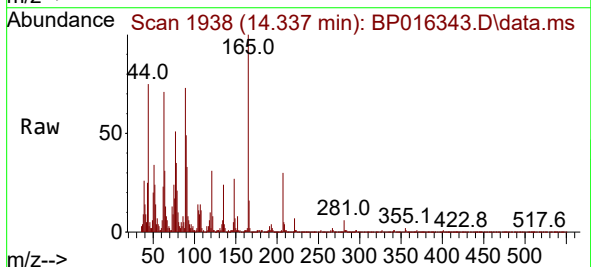

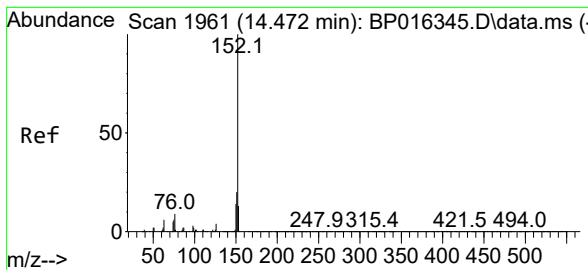

#50
 Acenaphthylene
 Concen: 4.867 ng/ul
 RT: 14.472 min Scan# 1961
 Delta R.T. -0.000 min
 Lab File: BP016343.D
 Acq: 25 Jul 2023 10:44

Instrument :





BNA_P

ClientSampleId :

SSTD005604

Tgt Ion:152 Resp: 420127




Ion	Ratio	Lower	Upper
152	100		
151	20.3	16.0	24.0
153	13.9	10.6	16.0

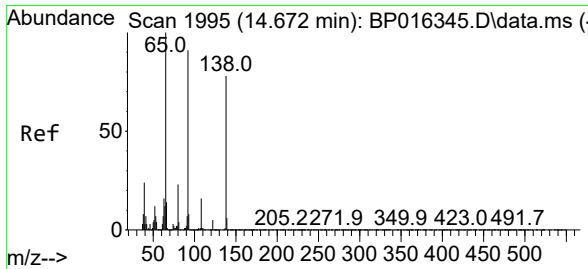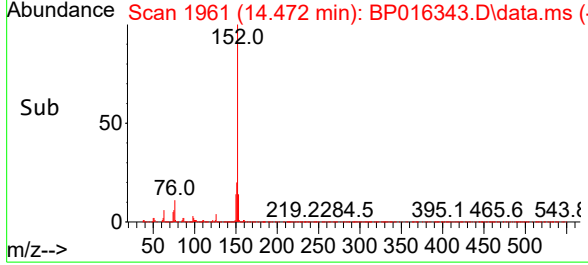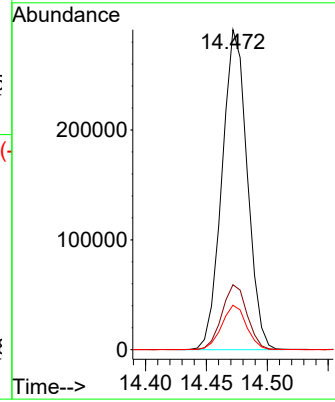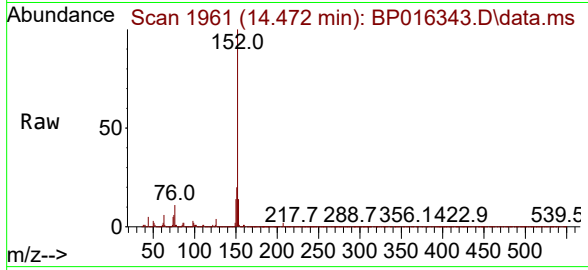


#51
 3-Nitroaniline
 Concen: 2.677 ng/ul
 RT: 14.666 min Scan# 1994
 Delta R.T. -0.006 min
 Lab File: BP016343.D
 Acq: 25 Jul 2023 10:44

Tgt Ion:138 Resp: 29194

Ion	Ratio	Lower	Upper
138	100		
108	48.3	16.6	24.8
92	131.6	94.3	141.5

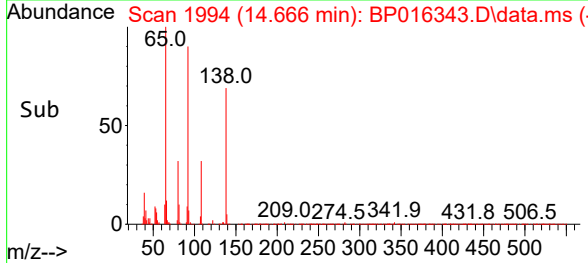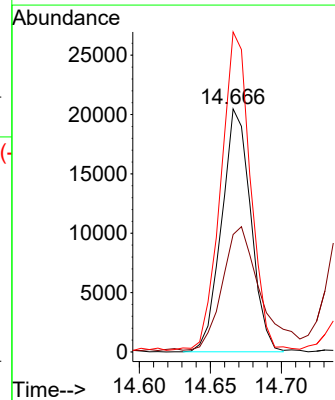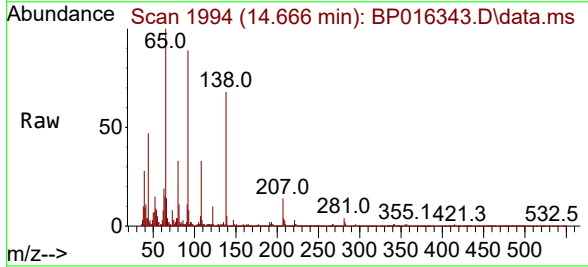







#52
 Acenaphthene
 Concen: 4.886 ng/ul
 RT: 14.807 min Scan# 2018
 Delta R.T. -0.000 min
 Lab File: BP016343.D
 Acq: 25 Jul 2023 10:44

Instrument :
 BNA_P
 ClientSampleId :
 SSTD005604

Tgt Ion:153 Resp: 271947




Ion	Ratio	Lower	Upper
153	100		
152	49.1	38.8	58.2
154	90.5	71.7	107.5

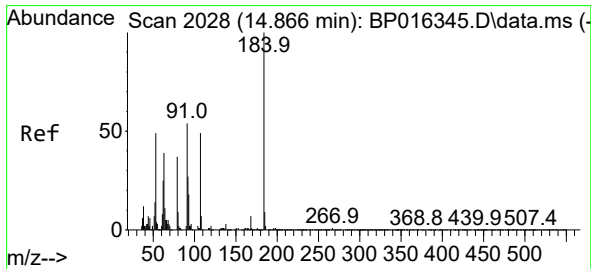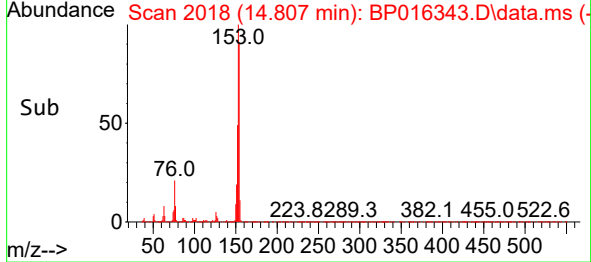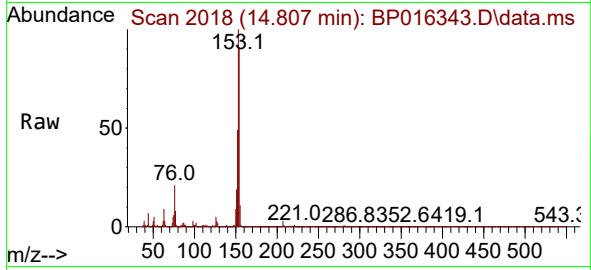


#53
 2,4-Dinitrophenol
 Concen: 1.649 ng/ul
 RT: 14.860 min Scan# 2027
 Delta R.T. -0.006 min
 Lab File: BP016343.D
 Acq: 25 Jul 2023 10:44

Tgt Ion:184 Resp: 6573

Ion	Ratio	Lower	Upper
184	100		
63	86.8	60.0	90.0
154	65.2	55.2	82.8


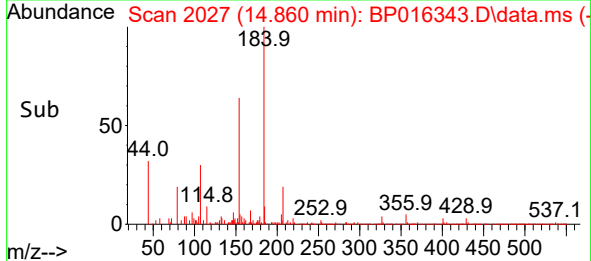

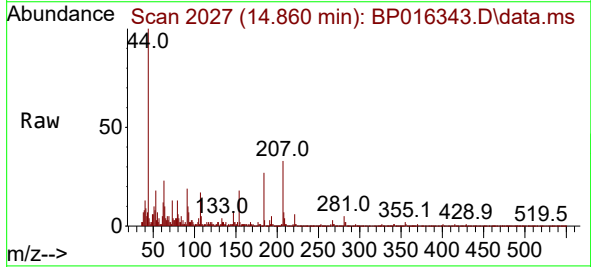




#55
 4-Nitrophenol
 Concen: 3.248 ng/ul
 RT: 14.937 min Scan# 2056
 Delta R.T. -0.006 min
 Lab File: BP016343.D
 Acq: 25 Jul 2023 10:44




Instrument : BNA_P
 ClientSampleId : SSTD005604


Tgt Ion	Resp	Ion Ratio	Lower	Upper
109	28139	100		
139	117.7	103.5	155.3	
65	122.2	98.6	148.0	

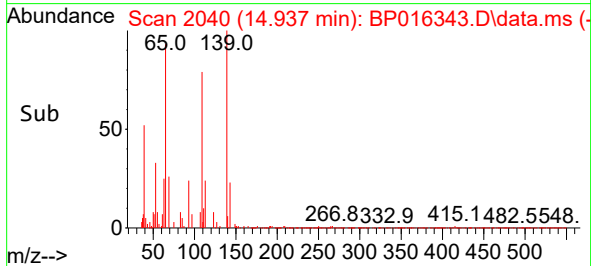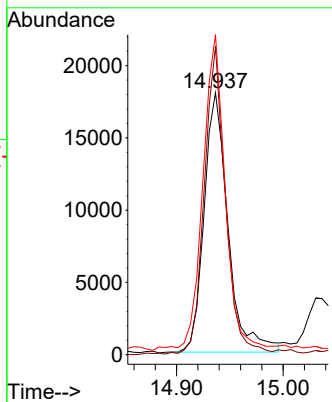

#56
 Dibenzofuran
 Concen: 4.999 ng/ul
 RT: 15.148 min Scan# 2076
 Delta R.T. 0.006 min
 Lab File: BP016343.D
 Acq: 25 Jul 2023 10:44

Tgt Ion	Resp	Ion Ratio	Lower	Upper
168	380907	100		
139	36.5	30.0	45.0	

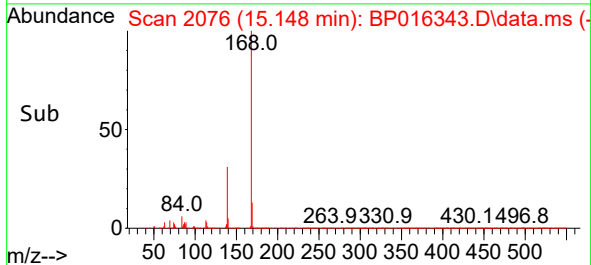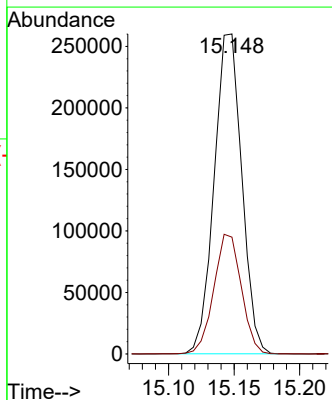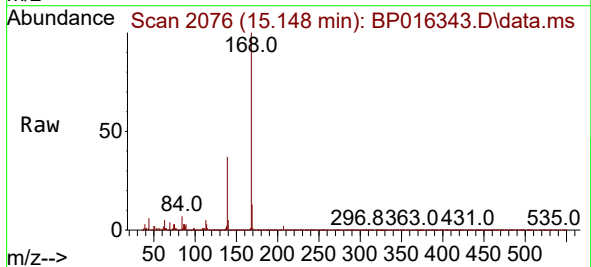







#57
 2,4-Dinitrotoluene
 Concen: 2.382 ng/ul
 RT: 15.113 min Scan# 2070
 Delta R.T. -0.000 min
 Lab File: BP016343.D
 Acq: 25 Jul 2023 10:44

Instrument : BNA_P
 ClientSampleId : SSTD005604

Tgt Ion:165 Resp: 31659




Ion	Ratio	Lower	Upper
165	100		
63	52.7	37.4	56.2
182	2.9	2.2	3.4

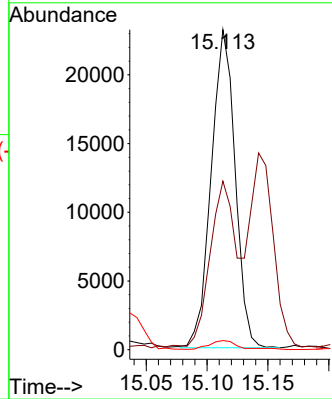


#58
 2,3,4,6-Tetrachlorophenol
 Concen: 3.743 ng/ul
 RT: 15.354 min Scan# 2111
 Delta R.T. -0.000 min
 Lab File: BP016343.D
 Acq: 25 Jul 2023 10:44

Tgt Ion:232 Resp: 48752

Ion	Ratio	Lower	Upper
232	100		
131	47.6	35.1	52.7
130	2.2	2.1	3.1
166	32.8	24.2	36.2

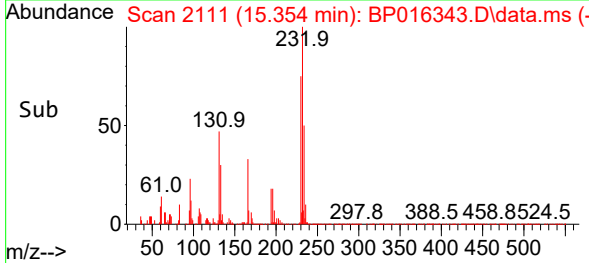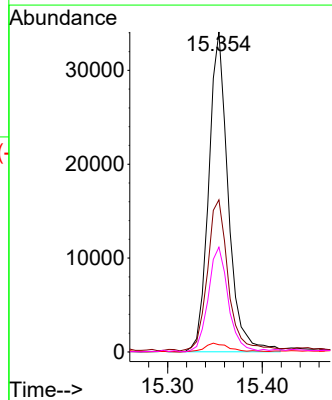



#59
 Diethylphthalate
 Concen: 4.832 ng/u1
 RT: 15.560 min Scan# 2146
 Delta R.T. -0.000 min
 Lab File: BP016343.D
 Acq: 25 Jul 2023 10:44





Instrument :

BNA_P

ClientSampleId :




SSTD005604


Tgt Ion:149 Resp: 314798
 Ion Ratio Lower Upper
 149 100
 177 22.3 17.9 26.9
 150 12.8 9.9 14.9

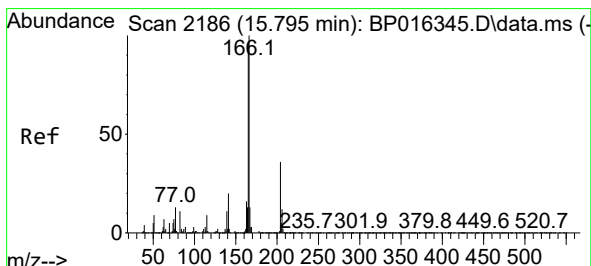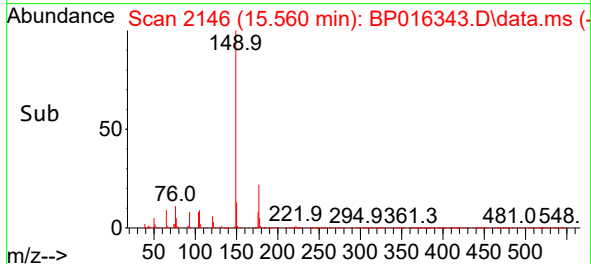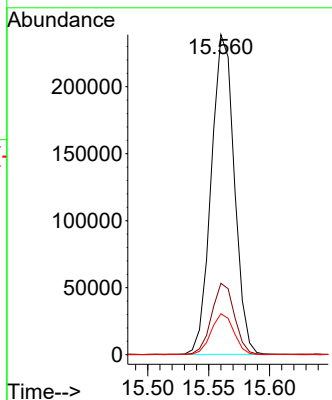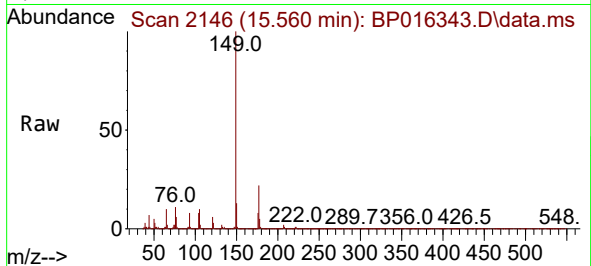

#61
 Fluorene
 Concen: 5.053 ng/u1
 RT: 15.795 min Scan# 2186
 Delta R.T. -0.000 min
 Lab File: BP016343.D
 Acq: 25 Jul 2023 10:44

Tgt Ion:166 Resp: 312776
 Ion Ratio Lower Upper
 166 100
 165 96.8 77.0 115.4
 167 13.4 10.6 15.8



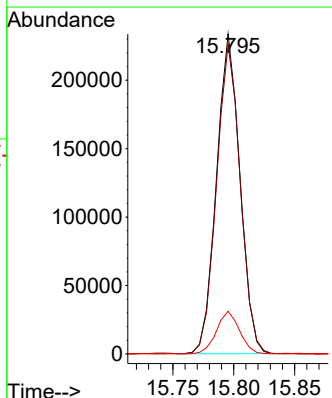
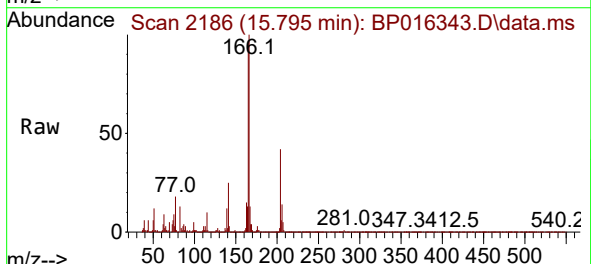




#62
 4-Chlorophenyl-phenylether
 Concen: 4.979 ng/ul
 RT: 15.789 min Scan# 2185
 Delta R.T. -0.000 min
 Lab File: BP016343.D
 Acq: 25 Jul 2023 10:44




Instrument :
 BNA_P
 ClientSampleId :
 SSTD005604


Tgt Ion:204 Resp: 150239
 Ion Ratio Lower Upper
 204 100
 206 34.2 26.5 39.7
 141 63.7 46.2 69.4

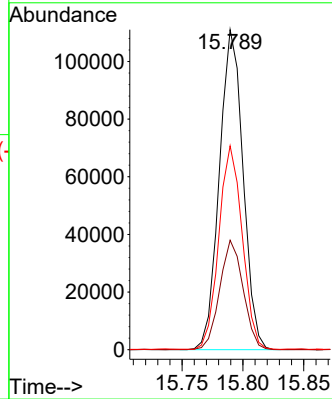

#63
 4-Nitroaniline
 Concen: 2.834 ng/ul
 RT: 15.831 min Scan# 2192
 Delta R.T. -0.006 min
 Lab File: BP016343.D
 Acq: 25 Jul 2023 10:44

Tgt Ion:138 Resp: 28342
 Ion Ratio Lower Upper
 138 100
 92 63.9 45.3 67.9
 108 123.1 76.4 114.6#


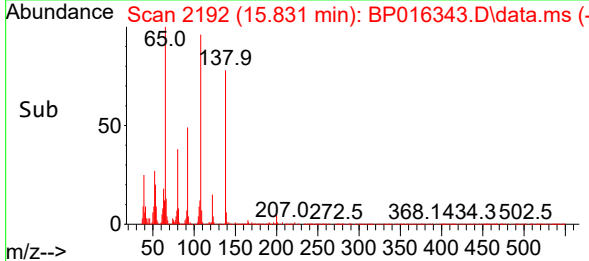
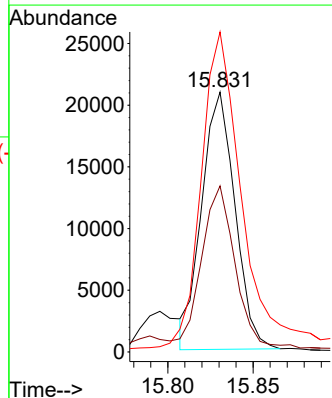





#66
 4,6-Dinitro-2-methylphenol
 Concen: 1.487 ng/ul
 RT: 15.860 min Scan# 2198
 Delta R.T. -0.006 min
 Lab File: BP016343.D
 Acq: 25 Jul 2023 10:44




Instrument : BNA_P
 ClientSampleId : SSTD005604


Tgt Ion	Resp	Lower	Upper
198	11351		
198	100		
182	6.9	3.8	5.8#
77	41.1	21.6	32.4#

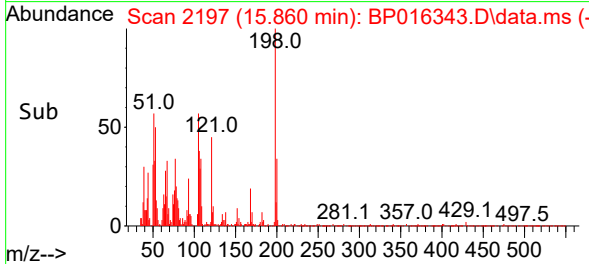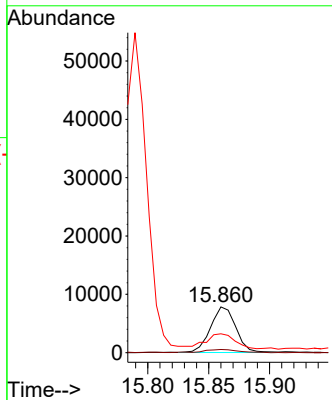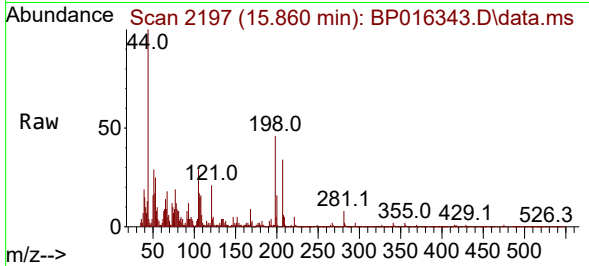

#67
 N-Nitrosodiphenylamine
 Concen: 4.757 ng/ul
 RT: 16.007 min Scan# 2222
 Delta R.T. -0.000 min
 Lab File: BP016343.D
 Acq: 25 Jul 2023 10:44

Tgt Ion	Resp	Lower	Upper
169	258604		
169	100		
168	66.6	54.0	81.0
167	37.1	29.4	44.2

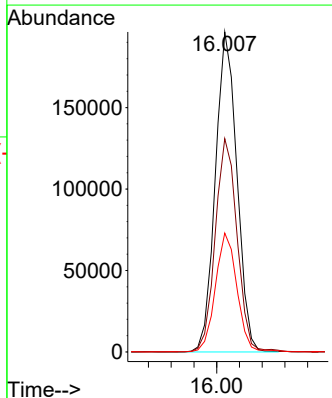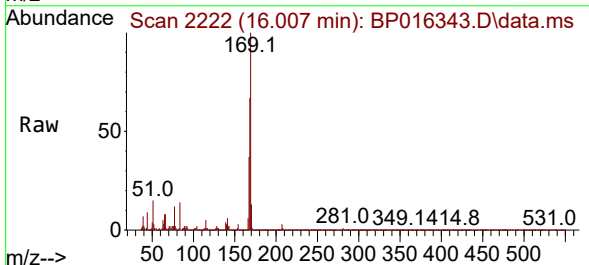







#68
 4-Bromophenyl-phenylether
 Concen: 4.627 ng/ul
 RT: 16.695 min Scan# 21
 Delta R.T. 0.006 min
 Lab File: BP016343.D
 Acq: 25 Jul 2023 10:44

Instrument :
 BNA_P
 ClientSampleId :
 SSTD005604

Tgt Ion:248 Resp: 85080




Ion	Ratio	Lower	Upper
248	100		
250	98.7	78.1	117.1
141	76.3	61.2	91.8

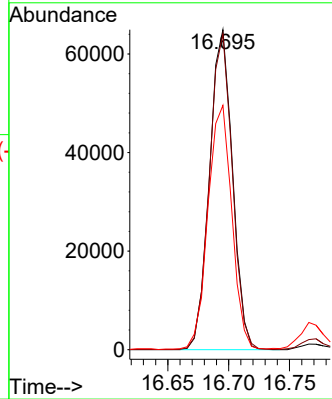


#69
 Hexachlorobenzene
 Concen: 4.753 ng/ul
 RT: 16.772 min Scan# 2352
 Delta R.T. 0.006 min
 Lab File: BP016343.D
 Acq: 25 Jul 2023 10:44

Tgt Ion:284 Resp: 104795

Ion	Ratio	Lower	Upper
284	100		
142	36.6	29.7	44.5
249	29.6	24.8	37.2


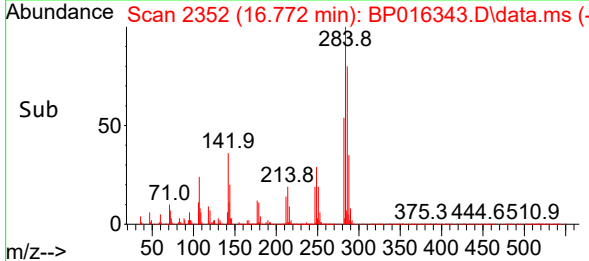
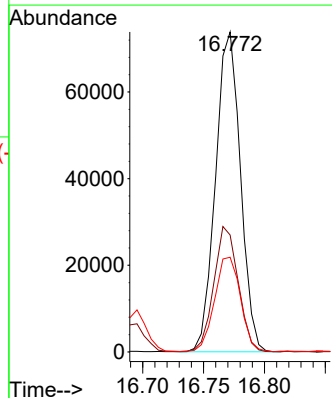





#70
 Atrazine
 Concen: 4.374 ng/uI
 RT: 16.960 min Scan# 21
 Delta R.T. -0.000 min
 Lab File: BP016343.D
 Acq: 25 Jul 2023 10:44




Instrument :
 BNA_P
 ClientSampleId :
 SSTD005604


Tgt Ion	Resp	Lower	Upper
200	100		
173	28.5	21.7	32.5
215	47.7	38.5	57.7

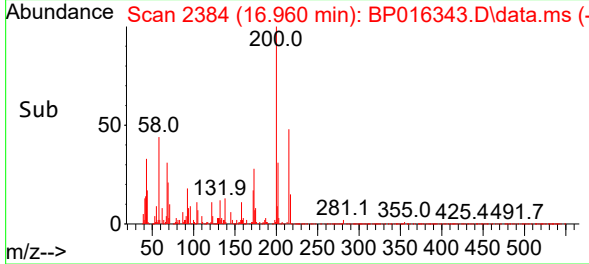

#71
 Pentachlorophenol
 Concen: 2.919 ng/uI
 RT: 17.131 min Scan# 2413
 Delta R.T. 0.006 min
 Lab File: BP016343.D
 Acq: 25 Jul 2023 10:44

Tgt Ion	Resp	Lower	Upper
266	100		
264	65.4	50.9	76.3
268	66.3	51.5	77.3


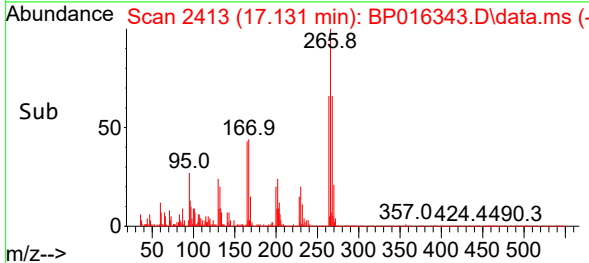




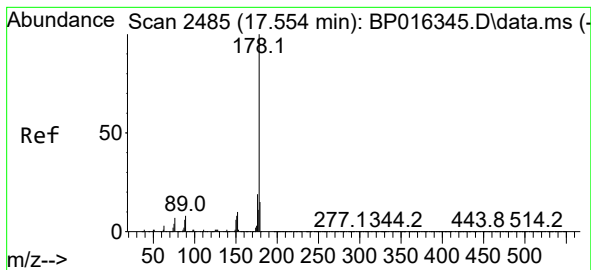

#72
 Phenanthrene
 Concen: 4.906 ng/uI
 RT: 17.554 min Scan# 2485
 Delta R.T. -0.000 min
 Lab File: BP016343.D
 Acq: 25 Jul 2023 10:44




Instrument :
 BNA_P
 ClientSampleId :
 SSTD005604


Tgt Ion	Resp	Ion Ratio	Lower	Upper
178	495000	100		
179	16.0	12.3	12.3	18.5
176	19.1	15.4	15.4	23.0

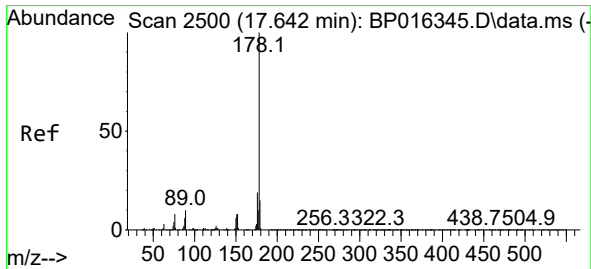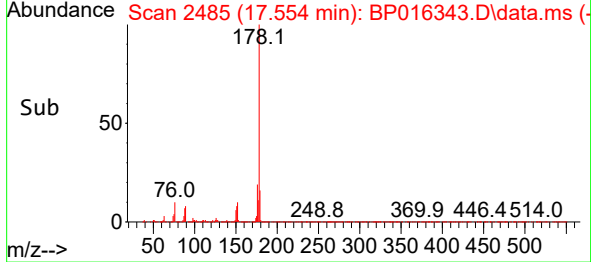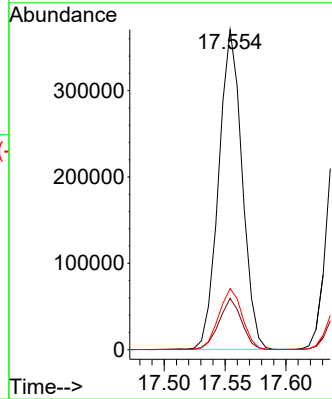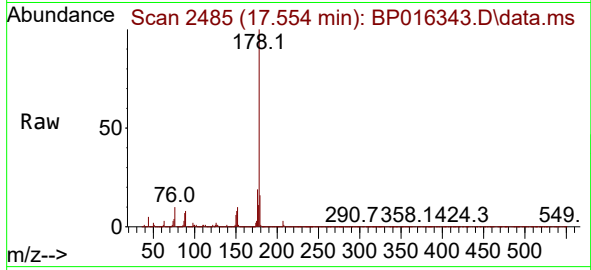

#74
 Anthracene
 Concen: 4.952 ng/uI
 RT: 17.648 min Scan# 2501
 Delta R.T. 0.006 min
 Lab File: BP016343.D
 Acq: 25 Jul 2023 10:44

Tgt Ion	Resp	Ion Ratio	Lower	Upper
178	508948	100		
179	14.8	12.3	12.3	18.5
176	18.6	15.1	15.1	22.7

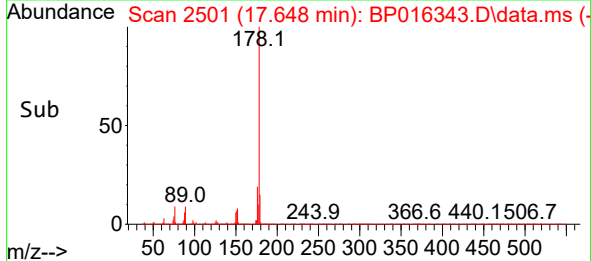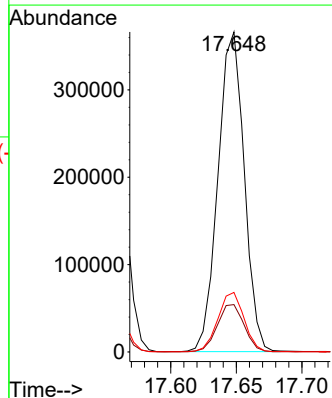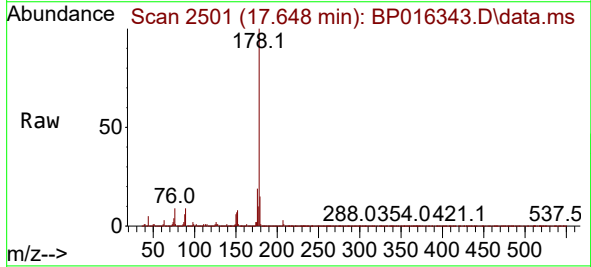







#75
 1,2,3,4-Tetrachlorobenzene
 Concen: 4.491 ng/uL
 RT: 13.537 min Scan# 1802
 Delta R.T. -0.000 min
 Lab File: BP016343.D
 Acq: 25 Jul 2023 10:44

Instrument :
 BNA_P
 ClientSampleId :
 SSTD005604

Tgt Ion: 216 Resp: 125674




Ion	Ratio	Lower	Upper
216	100		
214	81.6	62.8	94.2
218	49.6	38.6	58.0

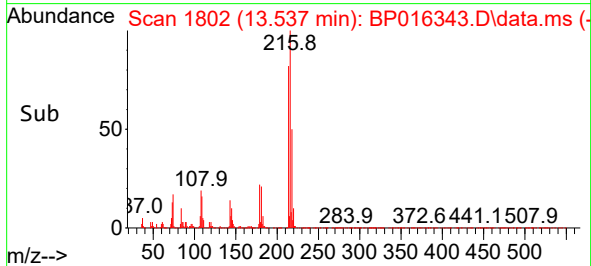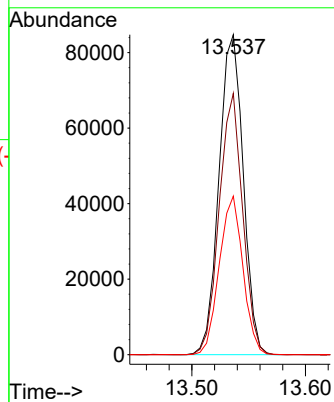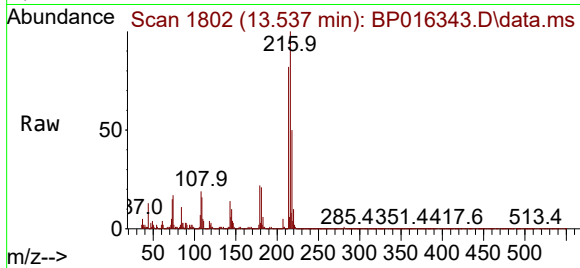


#76
 Pentachlorobenzene
 Concen: 4.646 ng/uL
 RT: 15.037 min Scan# 2057
 Delta R.T. -0.000 min
 Lab File: BP016343.D
 Acq: 25 Jul 2023 10:44

Tgt Ion: 250 Resp: 114894

Ion	Ratio	Lower	Upper
250	100		
248	62.2	50.1	75.1
252	64.9	51.0	76.6

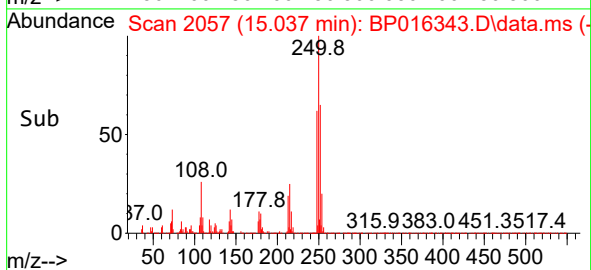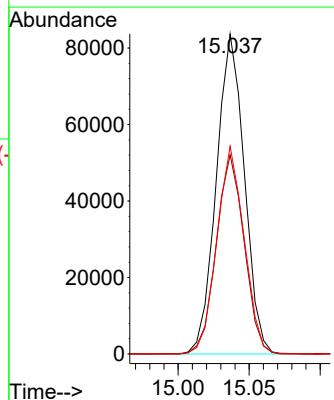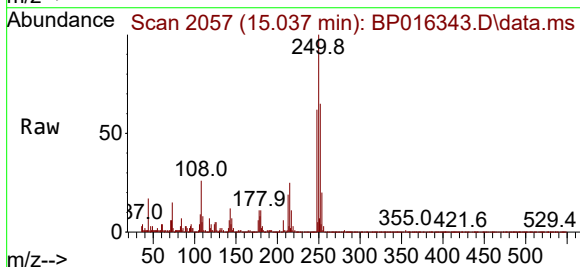







#77
 Carbazole
 Concen: 5.032 ng/ul
 RT: 17.919 min Scan# 21
 Delta R.T. -0.000 min
 Lab File: BP016343.D
 Acq: 25 Jul 2023 10:44

Instrument :
 BNA_P
 Client Sample Id :
 SSTD005604

Tgt Ion:167 Resp: 445109




Ion	Ratio	Lower	Upper
167	100		
166	22.0	17.3	25.9
139	13.1	10.4	15.6

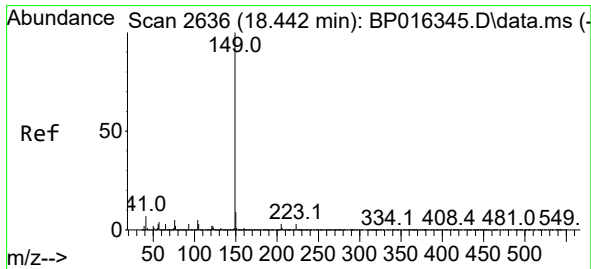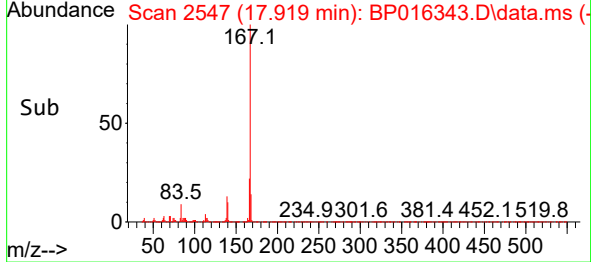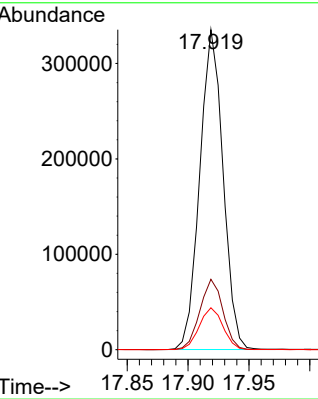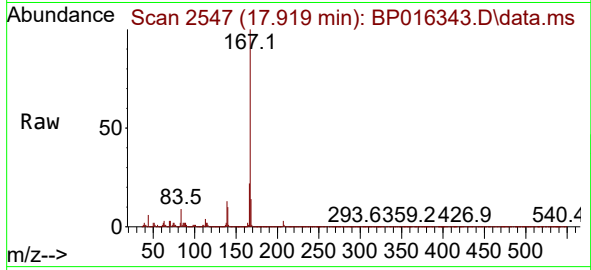


#78
 Di-n-butylphthalate
 Concen: 4.667 ng/ul
 RT: 18.448 min Scan# 2637
 Delta R.T. 0.006 min
 Lab File: BP016343.D
 Acq: 25 Jul 2023 10:44

Tgt Ion:149 Resp: 525741

Ion	Ratio	Lower	Upper
149	100		
150	9.7	7.5	11.3
104	6.1	4.3	6.5


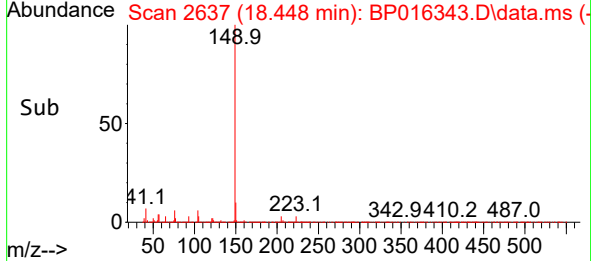
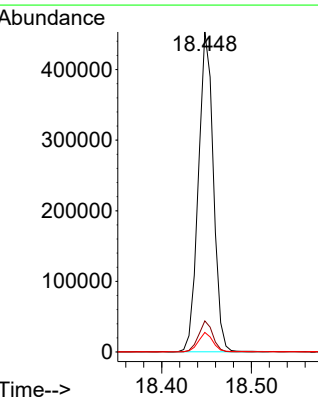
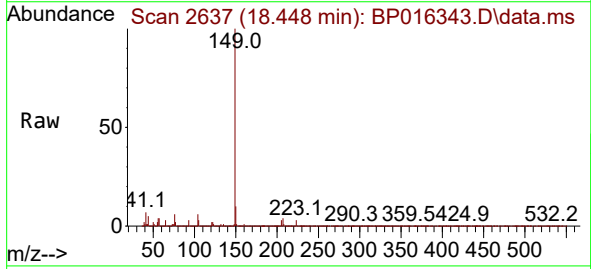


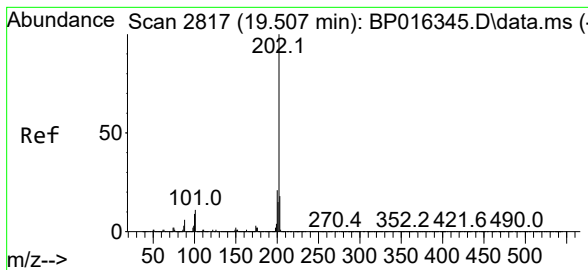

#80
 Fluoranthene
 Concen: 4.675 ng/u1
 RT: 19.507 min Scan# 2817
 Delta R.T. -0.000 min
 Lab File: BP016343.D
 Acq: 25 Jul 2023 10:44




Instrument : BNA_P
 ClientSampleId : SSTD005604


Tgt Ion	Resp	Lower	Upper
202	100		
101	12.5	9.1	13.7
100	9.9	7.1	10.7

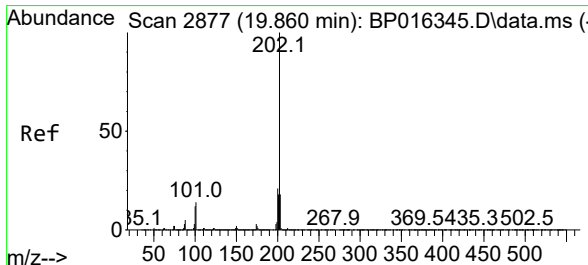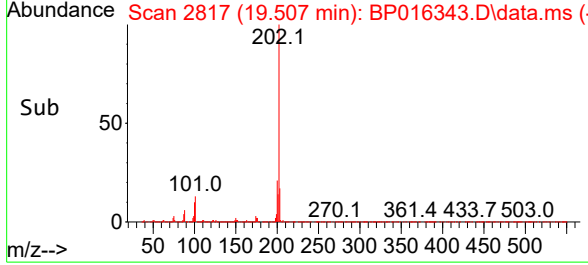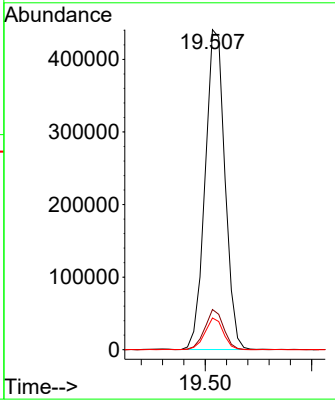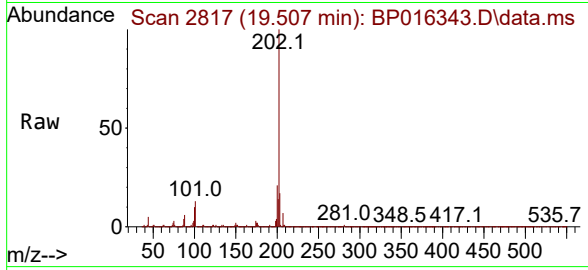

#82
 Pyrene
 Concen: 4.781 ng/u1
 RT: 19.866 min Scan# 2878
 Delta R.T. 0.006 min
 Lab File: BP016343.D
 Acq: 25 Jul 2023 10:44

Tgt Ion	Resp	Lower	Upper
202	100		
101	14.1	11.2	16.8
100	11.6	9.4	14.0


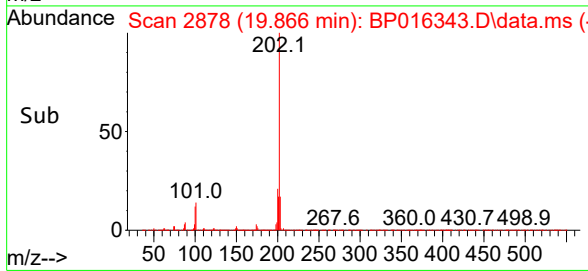
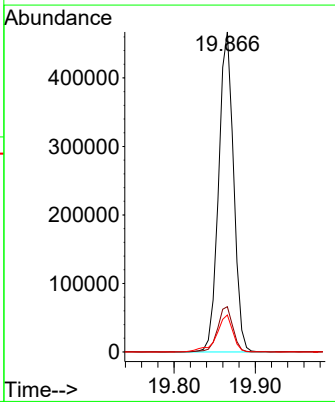
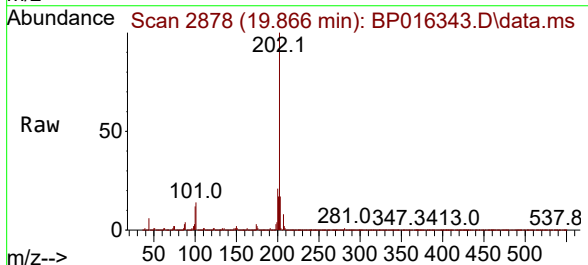




#83
 Butylbenzylphthalate
 Concen: 3.879 ng/ul
 RT: 20.736 min Scan# 3025
 Delta R.T. 0.006 min
 Lab File: BP016343.D
 Acq: 25 Jul 2023 10:44




Instrument : BNA_P
 ClientSampleId : SSTD005604


Tgt Ion	Resp	Lower	Upper
149	184051		
149	100		
91	77.4	58.5	87.7
206	19.9	17.0	25.4



#84
 3,3'-Dichlorobenzidine
 Concen: 3.878 ng/ul
 RT: 21.519 min Scan# 3159
 Delta R.T. 0.006 min
 Lab File: BP016343.D
 Acq: 25 Jul 2023 10:44


Tgt Ion	Resp	Lower	Upper
252	151928		
252	100		
254	63.9	51.4	77.0
126	12.8	10.3	15.5

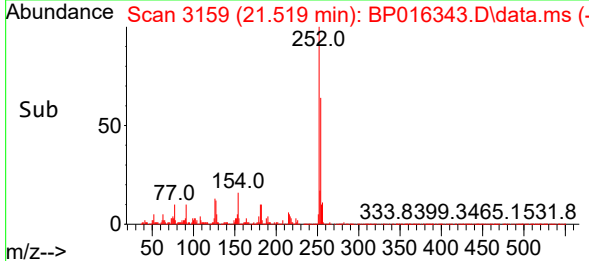






#85
 Benzo(a)anthracene
 Concen: 4.809 ng/ul
 RT: 21.589 min Scan# 3171
 Delta R.T. 0.006 min
 Lab File: BP016343.D
 Acq: 25 Jul 2023 10:44


Instrument : BNA_P
 ClientSampleId : SSTD005604





Tgt Ion:228 Resp: 580645
 Ion Ratio Lower Upper
 228 100
 229 20.0 15.9 23.9
 226 26.9 22.0 33.0

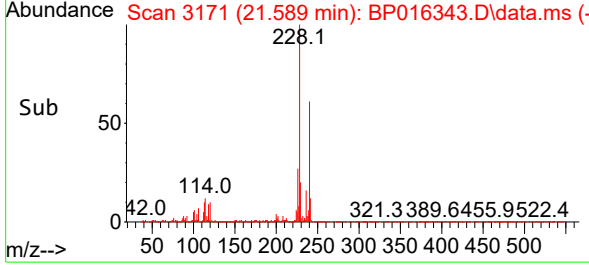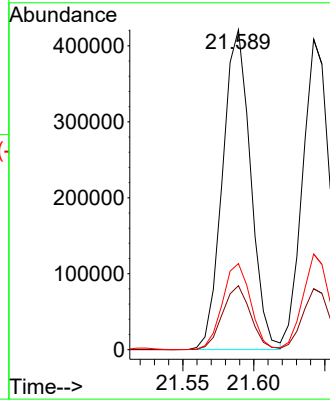


#86
 Bis(2-ethylhexyl)phthalate
 Concen: 4.323 ng/ul
 RT: 21.495 min Scan# 3155
 Delta R.T. 0.012 min
 Lab File: BP016343.D
 Acq: 25 Jul 2023 10:44



Tgt Ion:149 Resp: 312898
 Ion Ratio Lower Upper
 149 100
 167 27.0 21.7 32.5
 279 3.8 3.0 4.4



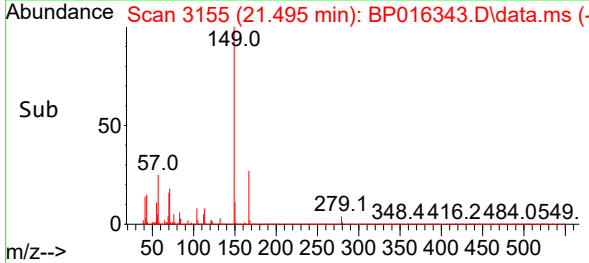
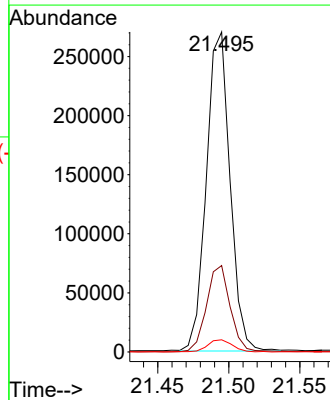




#87
 Chrysene
 Concen: 4.816 ng/ul
 RT: 21.642 min Scan# 3180
 Delta R.T. -0.000 min
 Lab File: BP016343.D
 Acq: 25 Jul 2023 10:44




Instrument : BNA_P
 ClientSampleId : SSTD005604


Tgt Ion	Resp	Lower	Upper
228	100		
226	30.8	24.5	36.7
229	19.6	15.6	23.4



#89
 Di-n-octyl phthalate
 Concen: 3.950 ng/ul
 RT: 22.501 min Scan# 3326
 Delta R.T. 0.012 min
 Lab File: BP016343.D
 Acq: 25 Jul 2023 10:44

Tgt Ion:149 Resp: 505156

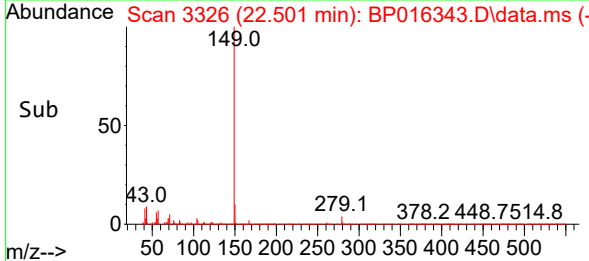







#90
 Benzo(b)fluoranthene
 Concen: 4.652 ng/u1
 RT: 23.401 min Scan# 3479
 Delta R.T. 0.006 min
 Lab File: BP016343.D
 Acq: 25 Jul 2023 10:44

Instrument :
 BNA_P
 ClientSampleId :
 SSTD005604

Tgt Ion:252 Resp: 566770




Ion	Ratio	Lower	Upper
252	100		
253	22.7	17.9	26.9
125	10.7	8.8	13.2

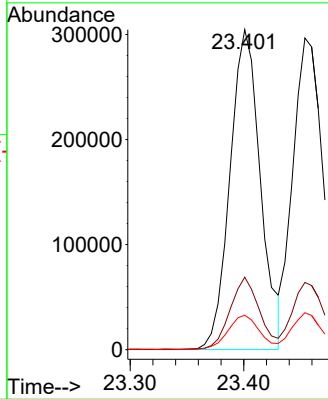


#91
 Benzo(k)fluoranthene
 Concen: 4.525 ng/u1
 RT: 23.454 min Scan# 3488
 Delta R.T. 0.006 min
 Lab File: BP016343.D
 Acq: 25 Jul 2023 10:44

Tgt Ion:252 Resp: 548581


Ion	Ratio	Lower	Upper
252	100		
253	21.6	17.7	26.5
125	11.9	9.0	13.6

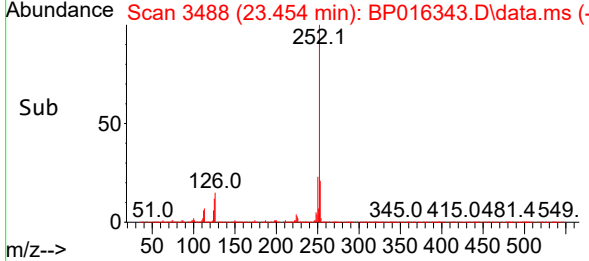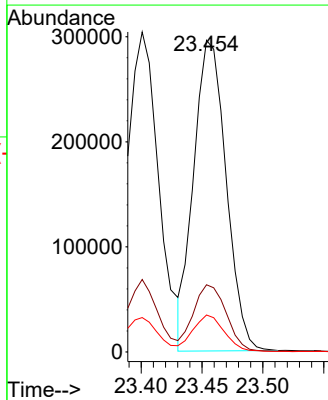






#93
 Benzo(a)pyrene
 Concen: 4.588 ng/u1
 RT: 24.095 min Scan# 31
 Delta R.T. 0.006 min
 Lab File: BP016343.D
 Acq: 25 Jul 2023 10:44


Instrument :
 BNA_P
 ClientSampleId :
 SSTD005604





Tgt Ion:252 Resp: 526393
 Ion Ratio Lower Upper
 252 100
 253 22.1 18.0 27.0
 125 12.9 9.4 14.0




#94
 Indeno(1,2,3-cd)pyrene
 Concen: 4.604 ng/u1
 RT: 26.995 min Scan# 4090
 Delta R.T. 0.006 min
 Lab File: BP016343.D
 Acq: 25 Jul 2023 10:44



Tgt Ion:276 Resp: 609967
 Ion Ratio Lower Upper
 276 100
 138 22.2 18.1 27.1
 277 23.3 19.0 28.4

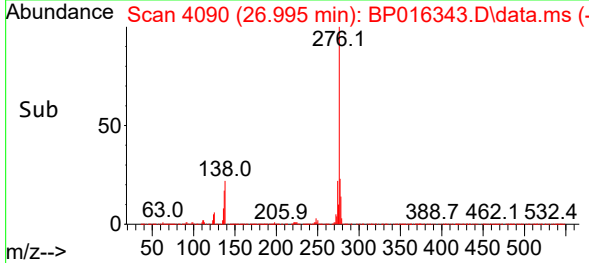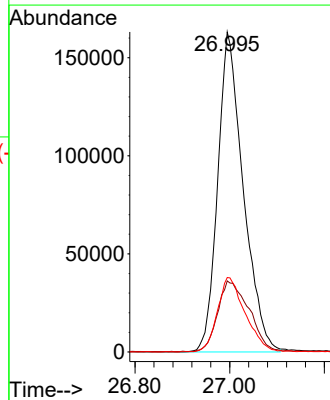







#95
 Dibenzo(a,h)anthracene
 Concen: 4.562 ng/ul
 RT: 27.036 min Scan# 4095
 Delta R.T. 0.012 min
 Lab File: BP016343.D
 Acq: 25 Jul 2023 10:44

Instrument : BNA_P
 ClientSampleId : SSTD005604

Tgt Ion: 278 Resp: 499913

Ion	Ratio	Lower	Upper
278	100		
139	17.6	14.2	21.2
279	24.0	19.4	29.2



#96
 Benzo(g,h,i)perylene
 Concen: 4.768 ng/ul
 RT: 27.859 min Scan# 4237
 Delta R.T. -0.000 min
 Lab File: BP016343.D
 Acq: 25 Jul 2023 10:44

Tgt Ion: 276 Resp: 500178

Ion	Ratio	Lower	Upper
276	100		
138	23.1	17.8	26.6
277	22.8	19.0	28.4

