

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072523\
 Data File : BP016363.D
 Acq On : 26 Jul 2023 01:02
 Operator : MA/JU
 Sample : 03534-11
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A4723

Quant Time: Jul 26 03:05:48 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP072523.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jul 25 23:56:16 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.099	152	356744	20.000	ng/ul	0.00
20) Naphthalene-d8	10.928	136	1561329	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.740	164	958718	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.498	188	2060675	20.000	ng/ul	0.00
79) Chrysene-d12	21.586	240	1831523	20.000	ng/ul	-0.01
88) Perylene-d12	24.192	264	2017199	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.423	96	40712	4.500	ng/uL	0.00
4) Pyridine-d5	3.852	84	618341	24.088	ng/ul	0.00
7) Phenol-d5	7.222	99	833940	27.935	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.428	67	475375	26.523	ng/ul	0.00
11) 2-Chlorophenol-d4	7.611	132	615111	26.411	ng/ul	0.00
15) 4-Methylphenol-d8	8.787	113	669951	27.905	ng/ul	0.00
21) Nitrobenzene-d5	9.287	128	294623	30.644	ng/ul	0.00
24) 2-Nitrophenol-d4	10.005	143	260691	32.877	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.528	165	612247	27.856	ng/ul	0.00
31) 4-Chloroaniline-d4	11.075	131	929088	27.172	ng/ul	0.00
46) Dimethylphthalate-d6	14.151	166	1998073	28.477	ng/ul	0.00
49) Acenaphthylene-d8	14.440	160	2350115	28.351	ng/ul	0.00
54) 4-Nitrophenol-d4	14.916	143	260977	22.198	ng/ul	0.00
60) Fluorene-d10	15.728	176	1760739	29.497	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.840	200	69177	10.192	ng/ul	0.00
73) Anthracene-d10	17.598	188	2605036	28.539	ng/ul	0.00
81) Pyrene-d10	19.822	212	3054918	29.375	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.022	264	2952593	30.338	ng/ul	-0.01
Target Compounds						
47) Dimethylphthalate	14.193	163	233368	3.298	ng/ul	Qvalue 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072523\
Data File : BP016363.D
Acq On : 26 Jul 2023 01:02
Operator : MA/JU
Sample : 03534-11
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A4723


Quant Time: Jul 26 03:05:48 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP072523.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jul 25 23:56:16 2023
Response via : Initial Calibration

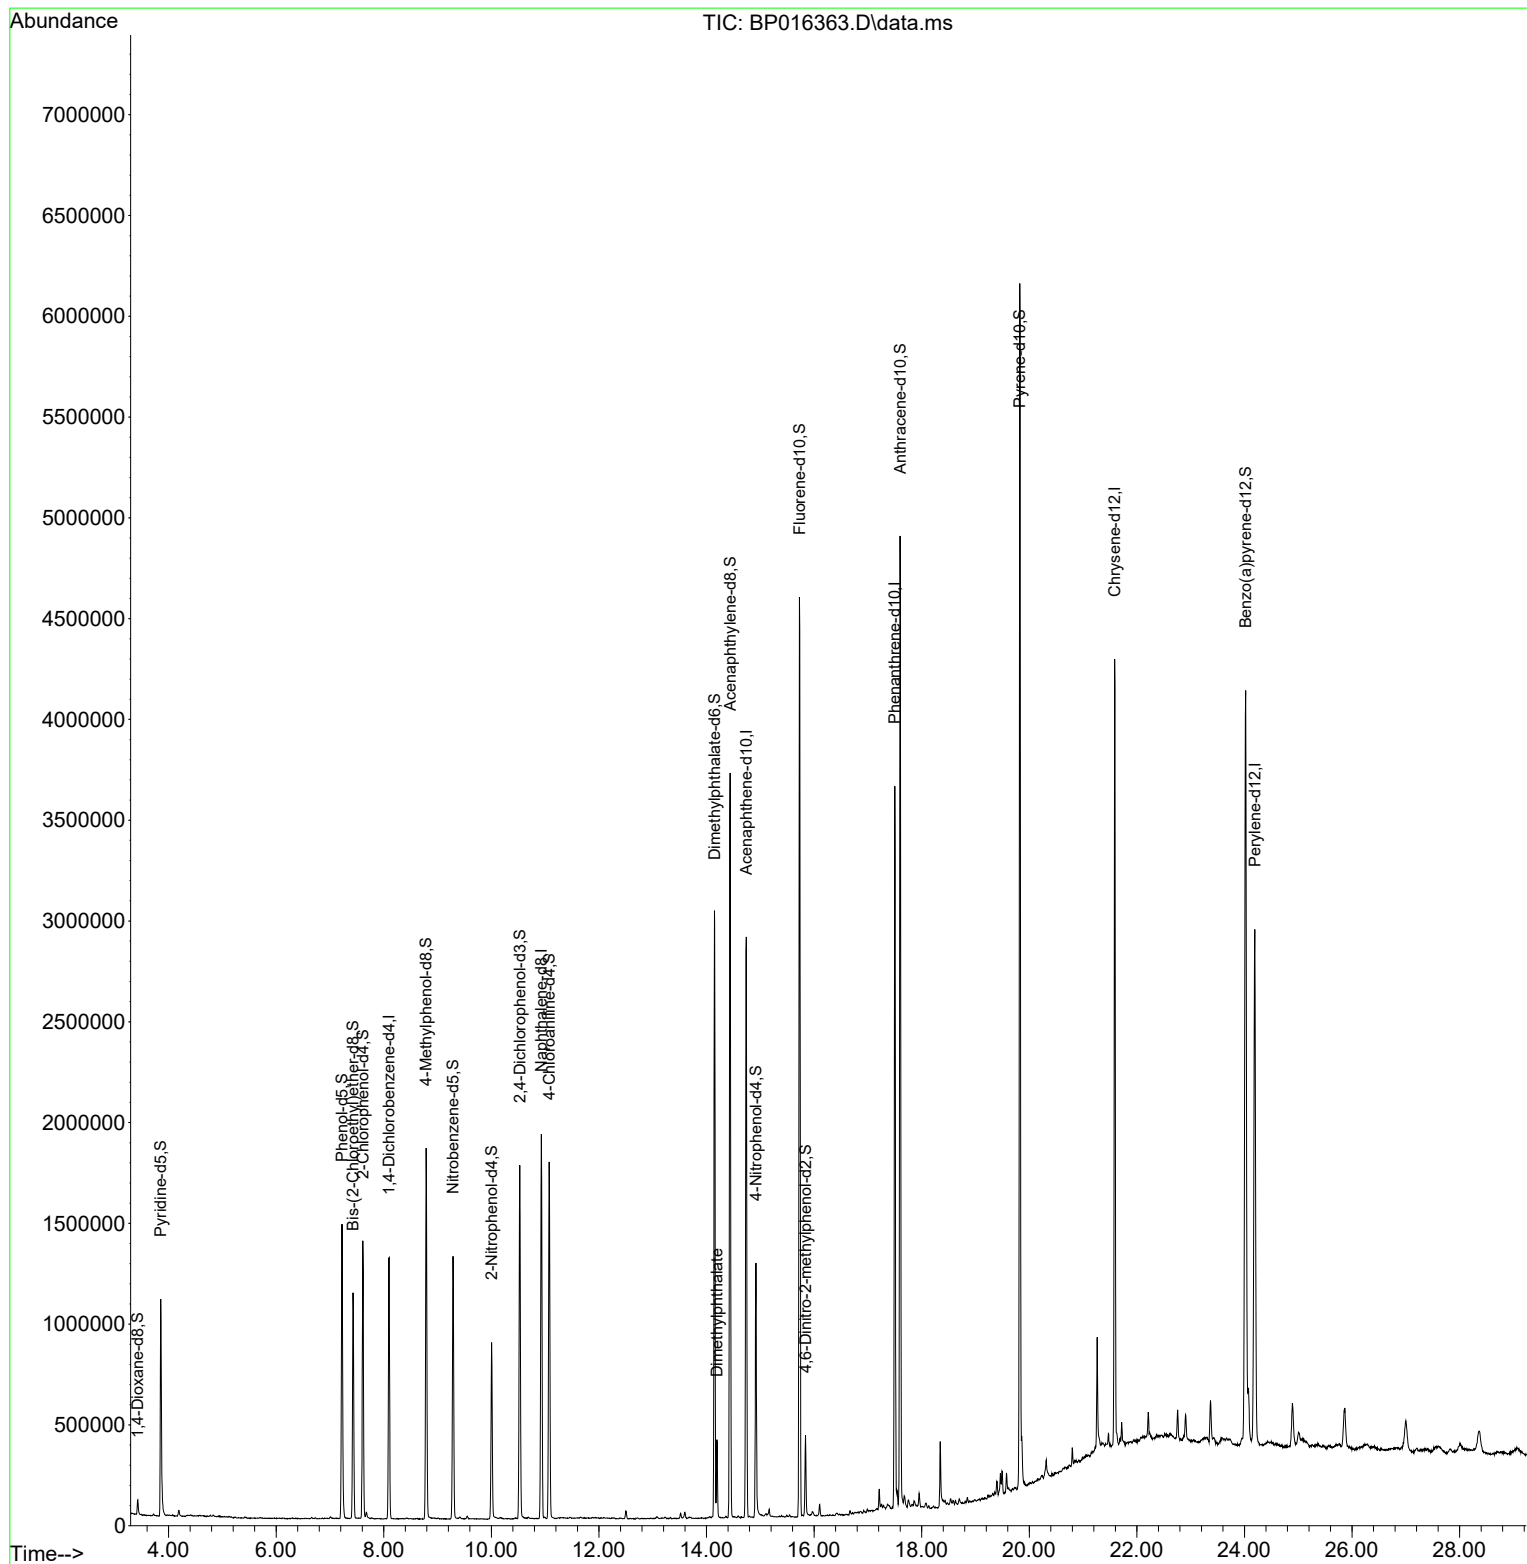

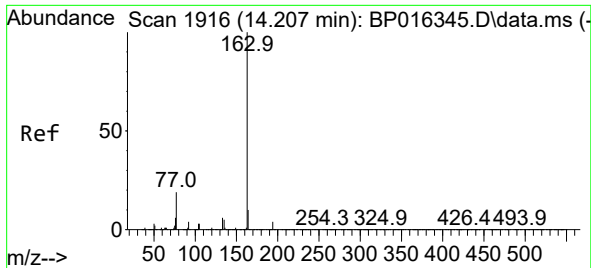

#47
 Dimethylphthalate
 Concen: 3.298 ng/ul
 RT: 14.193 min Scan# 1854
 Delta R.T. -0.015 min
 Lab File: BP016363.D
 Acq: 26 Jul 2023 01:02

Instrument :
 BNA_P
 ClientSampleId :
 A4723

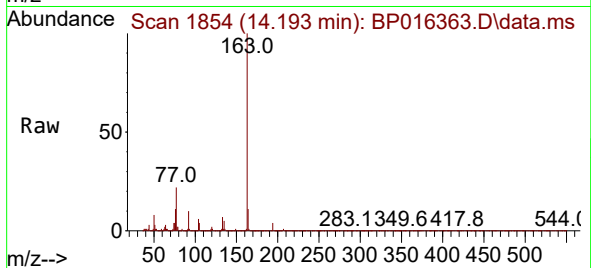

Tgt Ion:163 Resp: 233368
 Ion Ratio Lower Upper
 163 100
 194 3.8 3.3 4.9
 164 10.8 7.9 11.9

