

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072523\
Data File : BP016358.D
Acq On : 25 Jul 2023 22:13
Operator : MA/JU
Sample : 03534-06
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A4718

Manual IntegrationsAPPROVED

Quant Time: Jul 26 00:45:05 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP072523.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jul 25 23:56:16 2023
Response via : Initial Calibration

Reviewed By :Yogesh




Patel

07/26/2023

Supervised By :mohammad

ahmed

07/26/2023

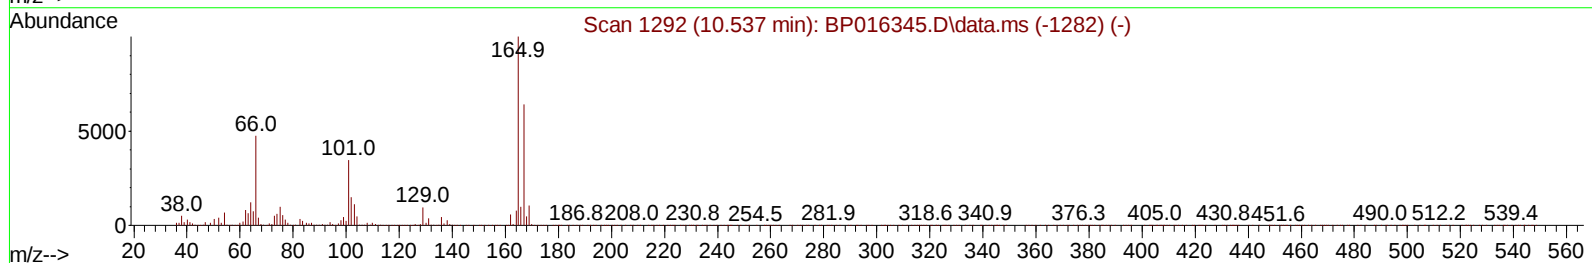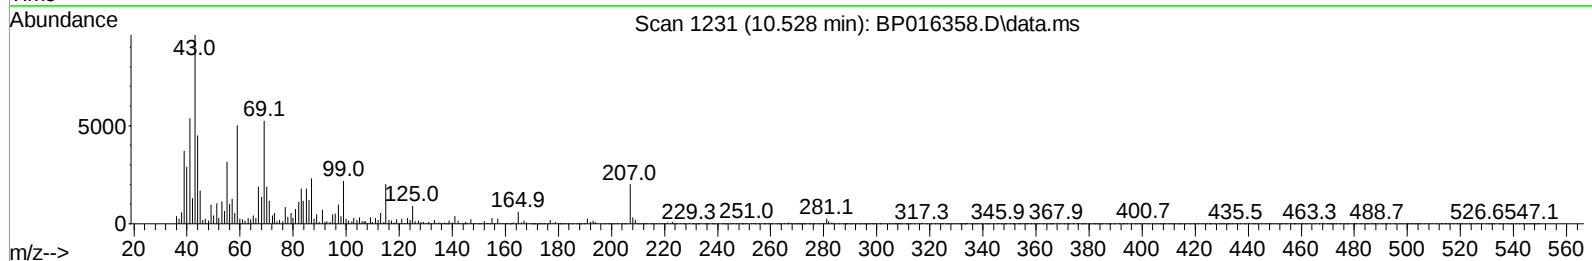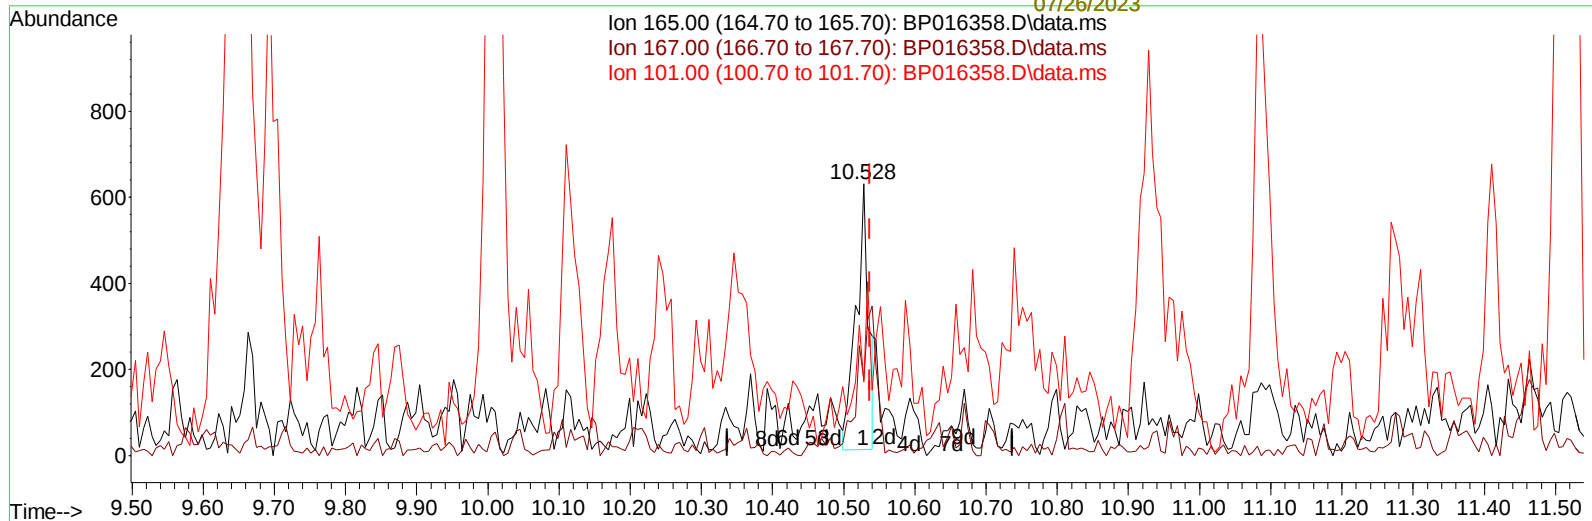

TIC: BP016358.D\data.ms

(28) 2,4-Dichlorophenol-d3 (S)

10.528min (-0.009) 0.04 ng/u1

response 749

Ion	Exp%	Act%
165.00	100.00	100.00
167.00	64.00	28.05#
101.00	34.60	27.10#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072523\
Data File : BP016358.D
Acq On : 25 Jul 2023 22:13
Operator : MA/JU
Sample : 03534-06
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A4718

Manual IntegrationsAPPROVED

Quant Time: Jul 26 00:45:05 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP072523.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jul 25 23:56:16 2023
Response via : Initial Calibration




Reviewed By :Yogesh

Patel

07/26/2023

Supervised By :mohammad
ahmed

07/26/2023

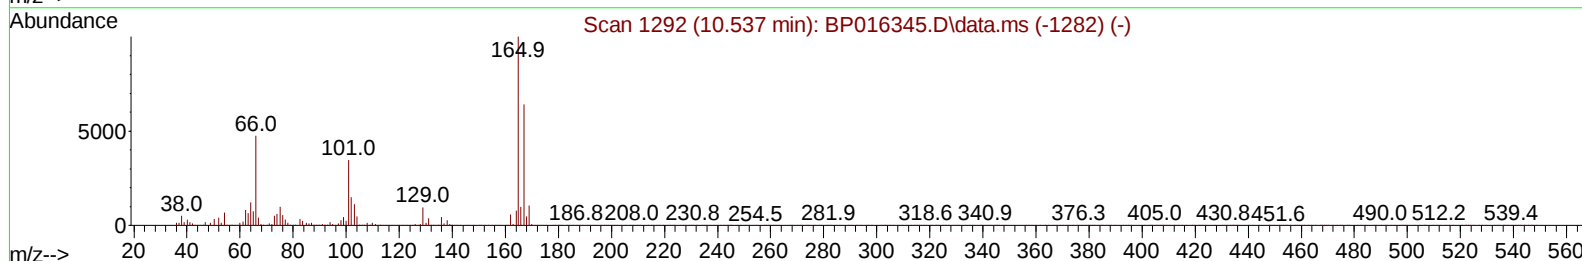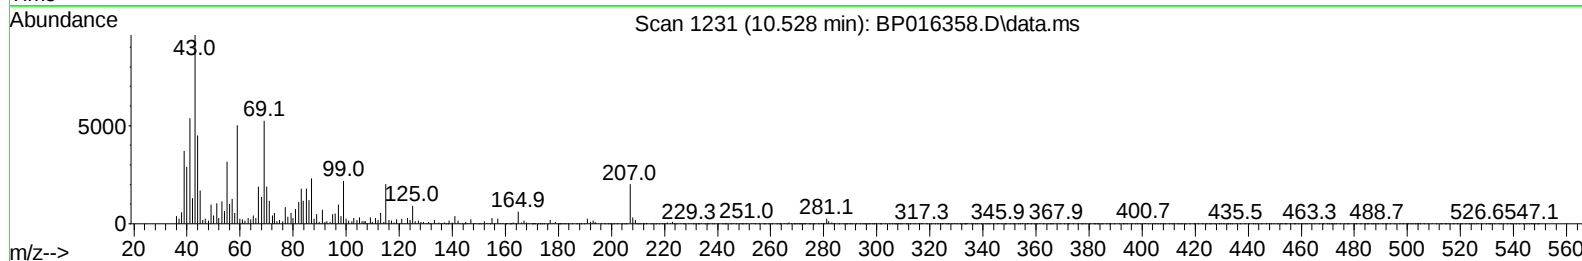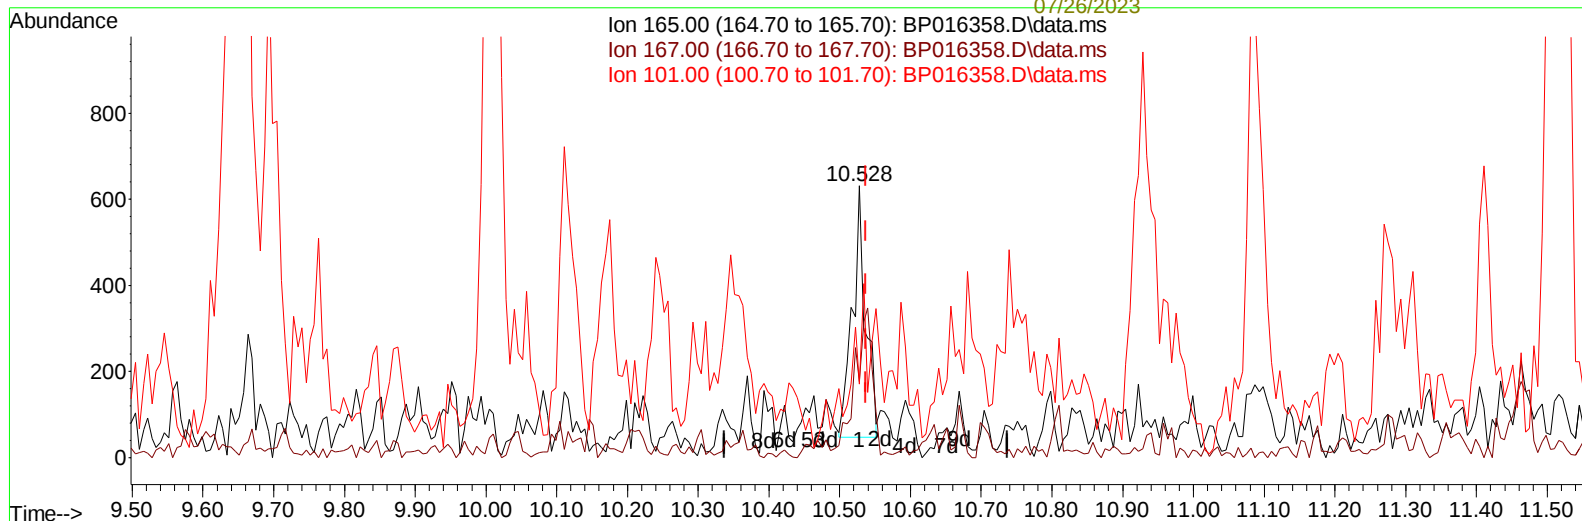

TIC: BP016358.D\data.ms

(28) 2,4-Dichlorophenol-d3 (S)

10.528min (-0.009) 0.04 ng/ul m

response 755

Ion	Exp%	Act%
165.00	100.00	100.00
167.00	64.00	28.05#
101.00	34.60	27.10#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072523\
 Data File : BP016358.D
 Acq On : 25 Jul 2023 22:13
 Operator : MA/JU
 Sample : 03534-06
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A4718

Manual IntegrationsAPPROVED

Reviewed By :Yogesh

Patel

07/26/2023

Supervised By :mohammad

ahmed

07/26/2023

Quant Time: Jul 26 00:46:24 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP072523.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jul 25 23:56:16 2023
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	8.099	152		354831	20.000	ng/ul	0.00
20) Naphthalene-d8	10.928	136		1510275	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.740	164		935461	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.498	188		2045808	20.000	ng/ul	0.00
79) Chrysene-d12	21.592	240		1736971	20.000	ng/ul	0.00
88) Perylene-d12	24.192	264		1471772	20.000	ng/ul	-0.01
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.428	96		8277	0.920	ng/uL	0.00
4) Pyridine-d5	3.852	84		258779	10.135	ng/ul	0.00
7) Phenol-d5	7.222	99		6898	0.232	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.428	67		96189	5.396	ng/ul	0.00
11) 2-Chlorophenol-d4	7.616	132		9162	0.396	ng/ul	0.00
15) 4-Methylphenol-d8	8.787	113		28586	1.197	ng/ul	0.00
21) Nitrobenzene-d5	9.287	128		47017	5.056	ng/ul	0.00
24) 2-Nitrophenol-d4	10.005	143		34122	4.449	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.528	165		755m	0.036	ng/ul	0.00
31) 4-Chloroaniline-d4	11.069	131		164	0.005	ng/ul	-0.01
46) Dimethylphthalate-d6	14.146	166		368633	5.384	ng/ul	-0.01
49) Acenaphthylene-d8	14.434	160		324694	4.014	ng/ul	0.00
54) 4-Nitrophenol-d4	14.916	143		24996	2.179	ng/ul	0.00
60) Fluorene-d10	15.728	176		314082	5.393	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.840	200		9679	1.436	ng/ul	0.00
73) Anthracene-d10	17.598	188		76412	0.843	ng/ul	0.00
81) Pyrene-d10	19.822	212		482681	4.894	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.016	264		23253	0.327	ng/ul	-0.02
Target Compounds							
16) Acetophenone	8.940	105		47380	1.257	ng/ul	95
86) Bis(2-ethylhexyl)phtha...	21.475	149		100071	1.419	ng/ul	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072523\
Data File : BP016358.D
Acq On : 25 Jul 2023 22:13
Operator : MA/JU
Sample : 03534-06
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A4718

Manual IntegrationsAPPROVED

Quant Time: Jul 26 00:46:24 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP072523.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jul 25 23:56:16 2023
Response via : Initial Calibration

Reviewed By :Yogesh

Patel

07/26/2023

Supervised By :mohammad

ahmed

07/26/2023

