

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072523\
 Data File : BP016367.D
 Acq On : 26 Jul 2023 03:17
 Operator : MA/JU
 Sample : 03534-15
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A4729

Quant Time: Jul 26 03:49:26 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP072523.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jul 25 23:56:16 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.099	152	413649	20.000	ng/u1	0.00
20) Naphthalene-d8	10.928	136	1809385	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.740	164	1116937	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.498	188	2399393	20.000	ng/u1	0.00
79) Chrysene-d12	21.592	240	1953764	20.000	ng/u1	0.00
88) Perylene-d12	24.186	264	1629462	20.000	ng/u1	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.428	96	23635	2.253	ng/uL	0.00
4) Pyridine-d5	3.852	84	296359	9.957	ng/u1	0.00
7) Phenol-d5	7.222	99	133099	3.845	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.428	67	264876	12.745	ng/u1	0.00
11) 2-Chlorophenol-d4	7.611	132	130392	4.828	ng/u1	0.00
15) 4-Methylphenol-d8	8.787	113	95956	3.447	ng/u1	0.00
21) Nitrobenzene-d5	9.287	128	159834	14.345	ng/u1	0.00
24) 2-Nitrophenol-d4	10.005	143	143205	15.584	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.528	165	35492	1.393	ng/u1	0.00
31) 4-Chloroaniline-d4	11.093	131	809	0.020	ng/u1	0.00
46) Dimethylphthalate-d6	14.151	166	1111532	13.598	ng/u1	0.00
49) Acenaphthylene-d8	14.434	160	1049372	10.866	ng/u1	0.00
54) 4-Nitrophenol-d4	14.916	143	127859	9.335	ng/u1	0.00
60) Fluorene-d10	15.728	176	948417	13.638	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.839	200	42928	5.432	ng/u1	0.00
73) Anthracene-d10	17.598	188	369335	3.475	ng/u1	0.00
81) Pyrene-d10	19.822	212	1351544	12.183	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.010	264	119312	1.518	ng/u1	-0.03
Target Compounds						
					Qvalue	
16) Acetophenone	8.940	105	69327	1.578	ng/u1	99
47) Dimethylphthalate	14.193	163	125074	1.517	ng/u1	99
86) Bis(2-ethylhexyl)phtha...	21.469	149	147049	1.853	ng/u1	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072523\
Data File : BP016367.D
Acq On : 26 Jul 2023 03:17
Operator : MA/JU
Sample : 03534-15
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A4729

Quant Time: Jul 26 03:49:26 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP072523.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jul 25 23:56:16 2023
Response via : Initial Calibration




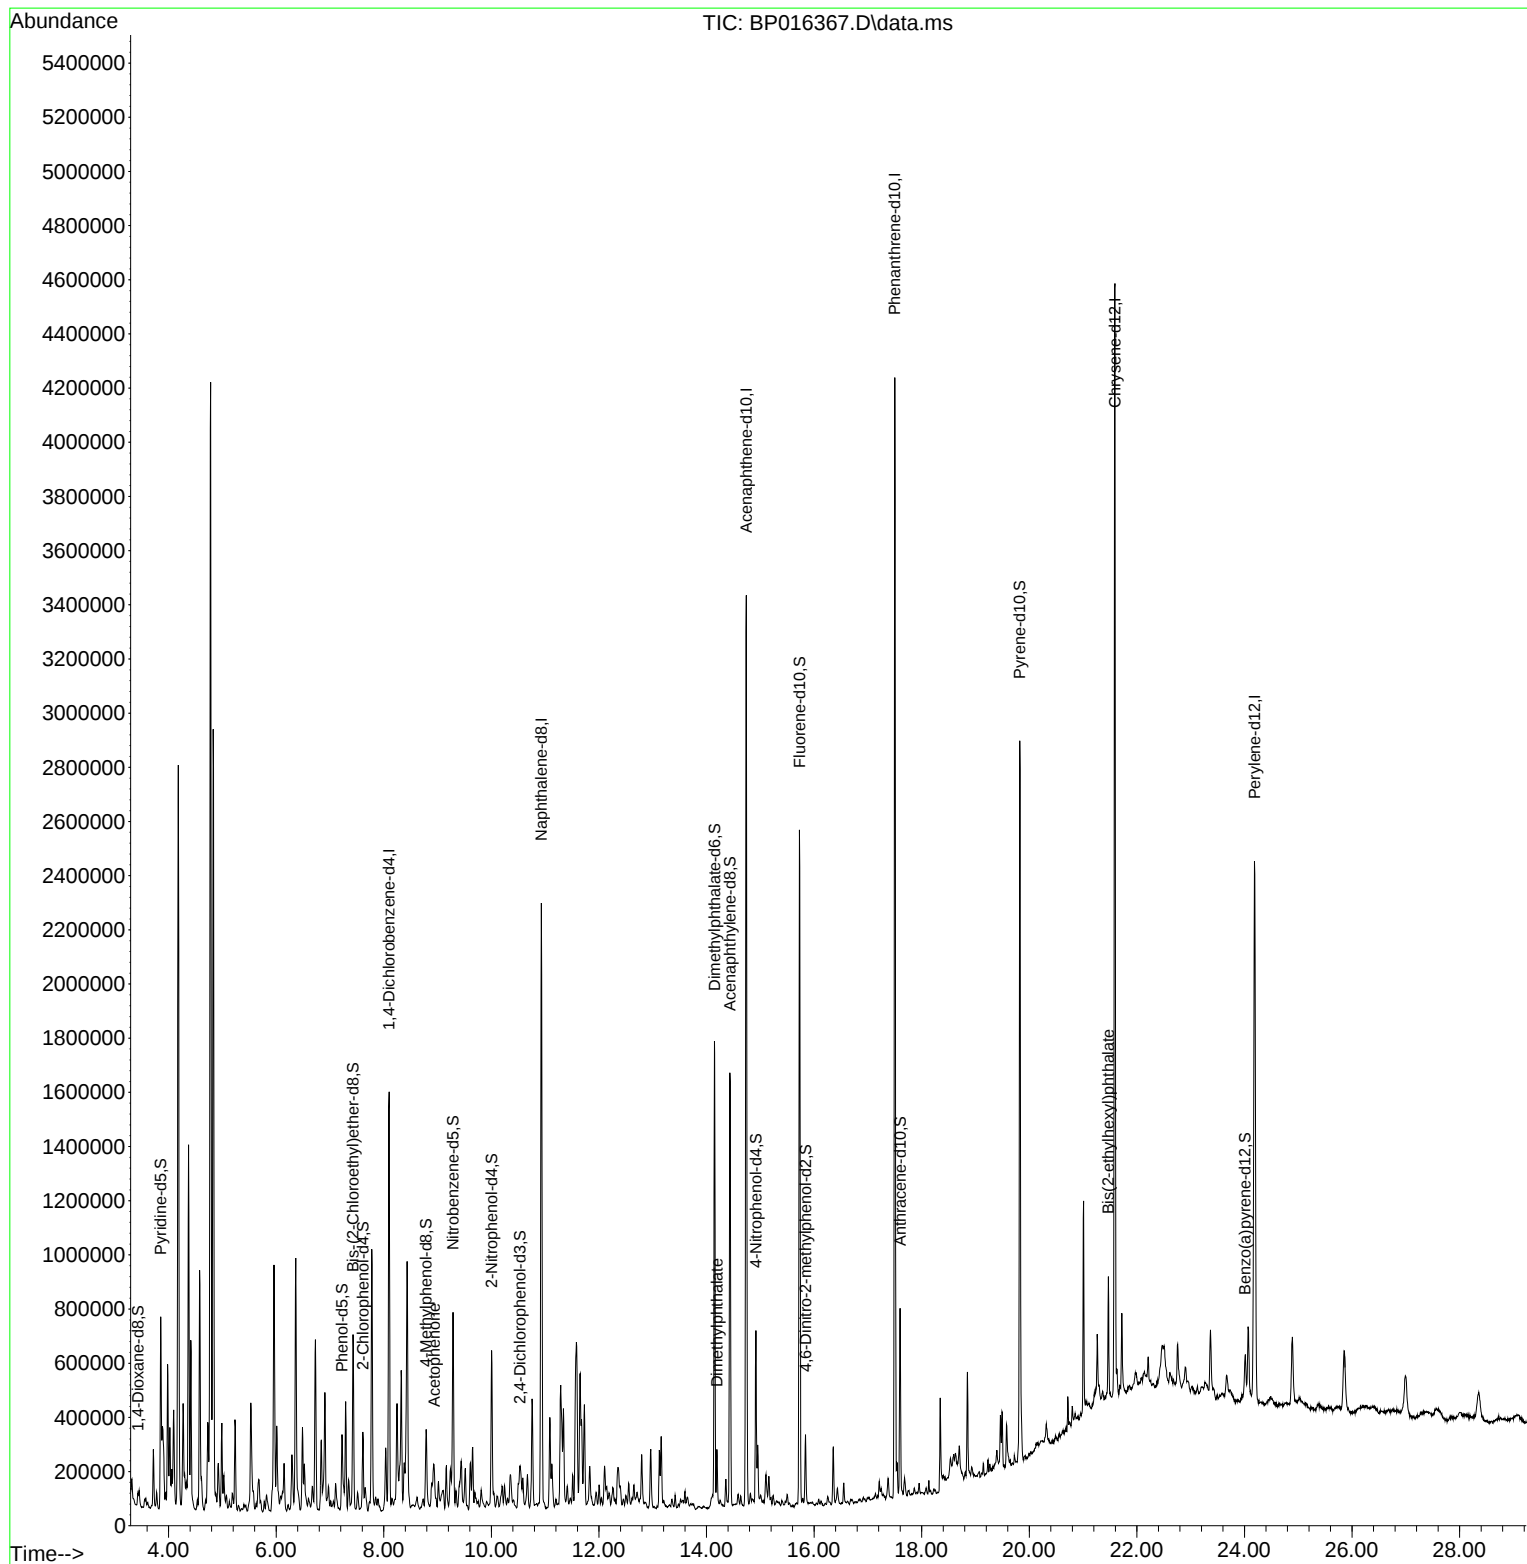


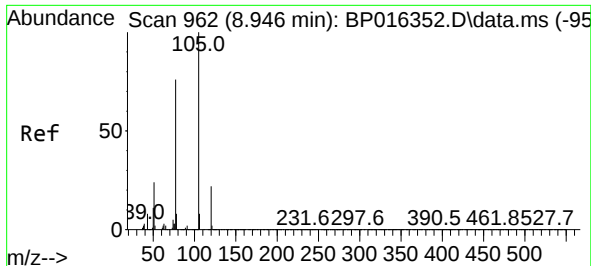

#16
Acetophenone
Concen: 1.578 ng/ul
RT: 8.940 min Scan# 90
Delta R.T. -0.009 min
Lab File: BP016367.D
Acq: 26 Jul 2023 03:17




Instrument :
BNA_P
ClientSampleId :
A4729


Tgt Ion:105 Resp: 69327
Ion Ratio Lower Upper
105 100
77 76.1 61.2 91.8
51 24.4 19.1 28.7

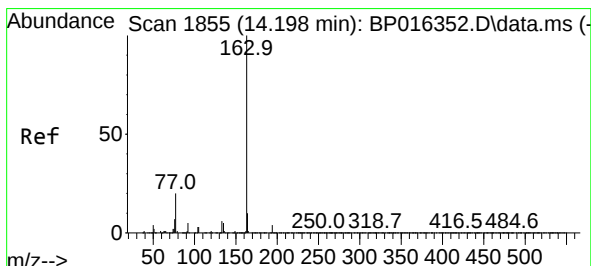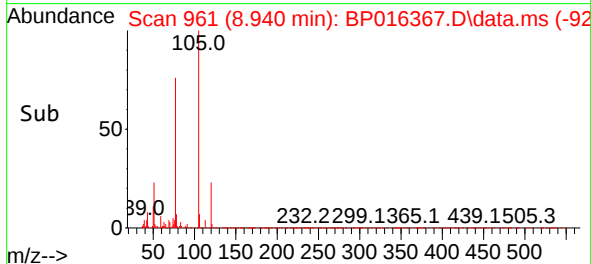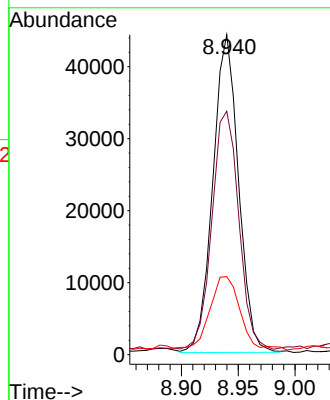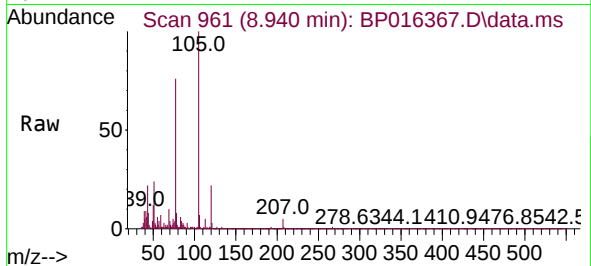

#47
Dimethylphthalate
Concen: 1.517 ng/ul
RT: 14.193 min Scan# 1854
Delta R.T. -0.015 min
Lab File: BP016367.D
Acq: 26 Jul 2023 03:17

Tgt Ion:163 Resp: 125074
Ion Ratio Lower Upper
163 100
194 3.5 3.3 4.9
164 9.6 7.9 11.9

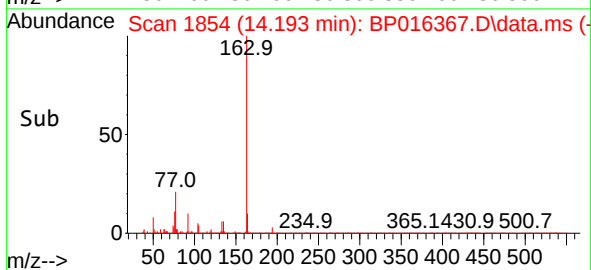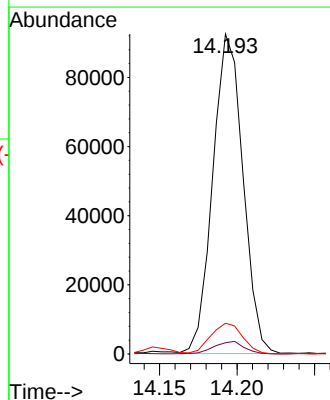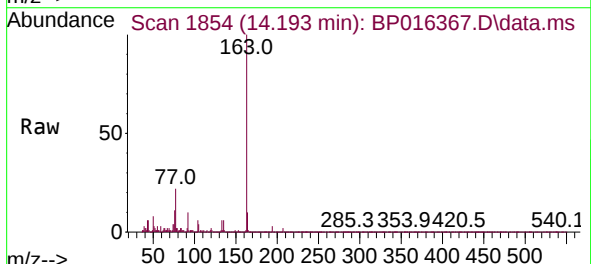

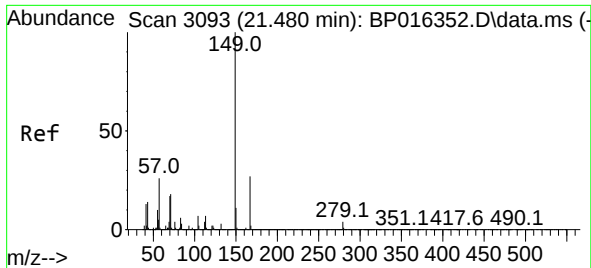

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 1.853 ng/ul
 RT: 21.469 min Scan# 3091
 Delta R.T. -0.015 min
 Lab File: BP016367.D
 Acq: 26 Jul 2023 03:17

Instrument :
 BNA_P
 ClientSampleId :
 A4729

Tgt Ion:149 Resp: 147049
 Ion Ratio Lower Upper
 149 100
 167 26.6 21.7 32.5
 279 3.9 3.0 4.4

