

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP072523\  
 Data File : BP016368.D  
 Acq On : 26 Jul 2023 03:51  
 Operator : MA/JU  
 Sample : 03534-16  
 Misc :  
 ALS Vial : 20 Sample Multiplier: 1

Instrument :  
 BNA\_P  
 ClientSampleId :  
 A4731

Quant Time: Jul 26 06:28:53 2023  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\SFAM-EPA-BP072523.MA.M  
 Quant Title : SVOA CALIBRATION  
 QLast Update : Tue Jul 25 23:56:16 2023  
 Response via : Initial Calibration


| Compound                      | R.T.   | QIon | Response | Conc   | Units | Dev(Min)      |
|-------------------------------|--------|------|----------|--------|-------|---------------|
| -----                         |        |      |          |        |       |               |
| Internal Standards            |        |      |          |        |       |               |
| 1) 1,4-Dichlorobenzene-d4     | 8.098  | 152  | 448996   | 20.000 | ng/u1 | 0.00          |
| 20) Naphthalene-d8            | 10.928 | 136  | 1991428  | 20.000 | ng/u1 | 0.00          |
| 38) Acenaphthene-d10          | 14.739 | 164  | 1237282  | 20.000 | ng/u1 | 0.00          |
| 64) Phenanthrene-d10          | 17.498 | 188  | 2687250  | 20.000 | ng/u1 | 0.00          |
| 79) Chrysene-d12              | 21.592 | 240  | 2275207  | 20.000 | ng/u1 | 0.00          |
| 88) Perylene-d12              | 24.192 | 264  | 2194447  | 20.000 | ng/u1 | -0.02         |
| System Monitoring Compounds   |        |      |          |        |       |               |
| 3) 1,4-Dioxane-d8             | 3.428  | 96   | 53283    | 4.679  | ng/uL | 0.00          |
| 4) Pyridine-d5                | 3.857  | 84   | 788879   | 24.417 | ng/u1 | 0.00          |
| 7) Phenol-d5                  | 7.222  | 99   | 1093580  | 29.105 | ng/u1 | 0.00          |
| 9) Bis-(2-Chloroethyl)eth...  | 7.428  | 67   | 623970   | 27.661 | ng/u1 | 0.00          |
| 11) 2-Chlorophenol-d4         | 7.610  | 132  | 814948   | 27.802 | ng/u1 | 0.00          |
| 15) 4-Methylphenol-d8         | 8.787  | 113  | 850249   | 28.139 | ng/u1 | 0.00          |
| 21) Nitrobenzene-d5           | 9.287  | 128  | 405260   | 33.048 | ng/u1 | 0.00          |
| 24) 2-Nitrophenol-d4          | 10.004 | 143  | 379330   | 37.507 | ng/u1 | 0.00          |
| 28) 2,4-Dichlorophenol-d3     | 10.528 | 165  | 828760   | 29.564 | ng/u1 | 0.00          |
| 31) 4-Chloroaniline-d4        | 11.075 | 131  | 1156736  | 26.524 | ng/u1 | 0.00          |
| 46) Dimethylphthalate-d6      | 14.151 | 166  | 2635299  | 29.102 | ng/u1 | 0.00          |
| 49) Acenaphthylene-d8         | 14.439 | 160  | 3086998  | 28.856 | ng/u1 | 0.00          |
| 54) 4-Nitrophenol-d4          | 14.916 | 143  | 367440   | 24.217 | ng/u1 | 0.00          |
| 60) Fluorene-d10              | 15.727 | 176  | 2298454  | 29.836 | ng/u1 | 0.00          |
| 65) 4,6-Dinitro-2-methylph... | 15.839 | 200  | 119908   | 13.547 | ng/u1 | 0.00          |
| 73) Anthracene-d10            | 17.598 | 188  | 3373262  | 28.338 | ng/u1 | 0.00          |
| 81) Pyrene-d10                | 19.827 | 212  | 3929426  | 30.416 | ng/u1 | 0.00          |
| 92) Benzo(a)pyrene-d12        | 24.021 | 264  | 3249594  | 30.693 | ng/u1 | -0.02         |
| Target Compounds              |        |      |          |        |       |               |
| 47) Dimethylphthalate         | 14.192 | 163  | 257707   | 2.822  | ng/u1 | Qvalue<br>100 |
| -----                         |        |      |          |        |       |               |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP072523\  
Data File : BP016368.D  
Acq On : 26 Jul 2023 03:51  
Operator : MA/JU  
Sample : 03534-16  
Misc :  
ALS Vial : 20 Sample Multiplier: 1

Instrument :  
BNA\_P  
ClientSampleId :  
A4731

Quant Time: Jul 26 06:28:53 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\SFAM-EPA-BP072523.MA.M  
Quant Title : SVOA CALIBRATION  
QLast Update : Tue Jul 25 23:56:16 2023  
Response via : Initial Calibration

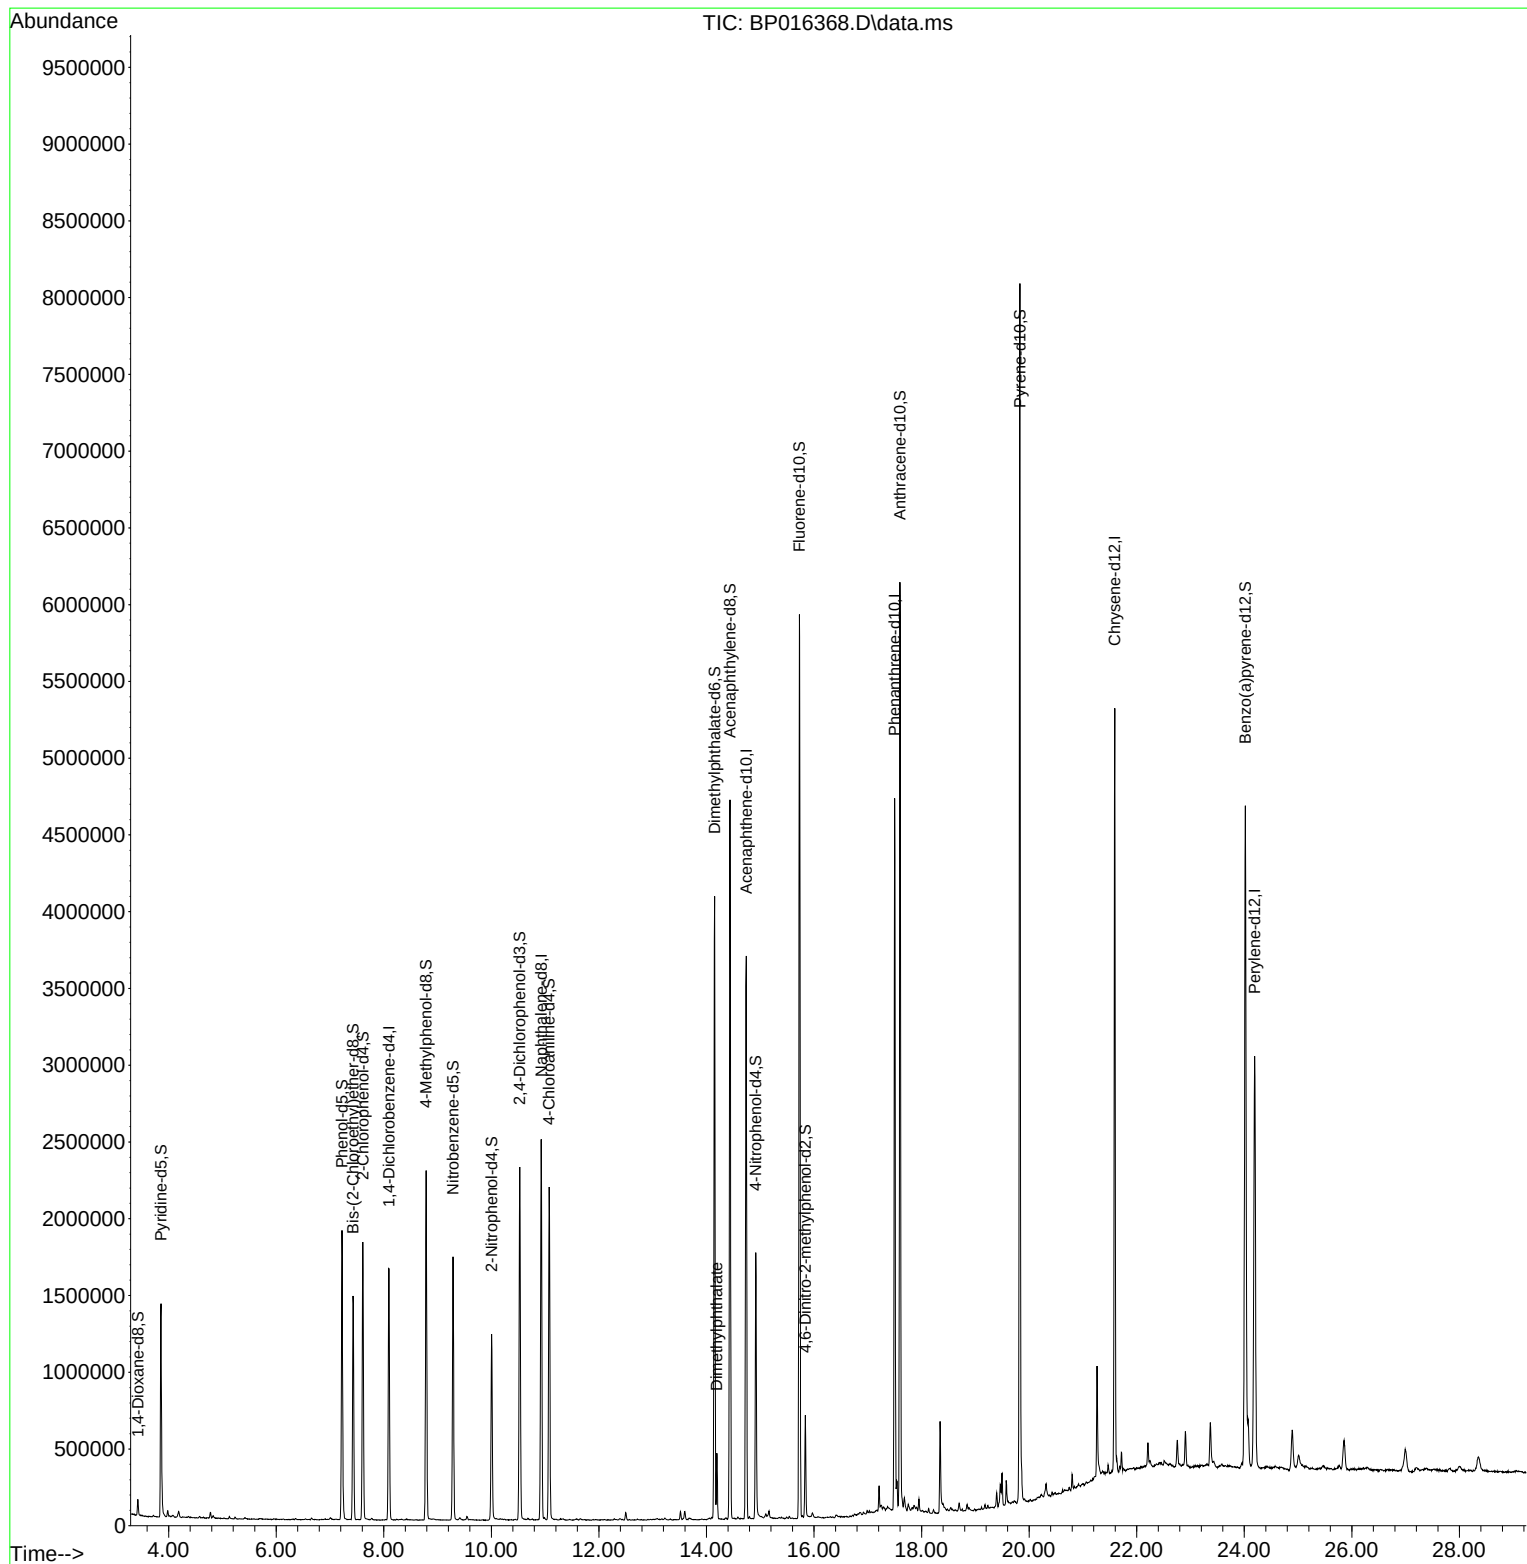

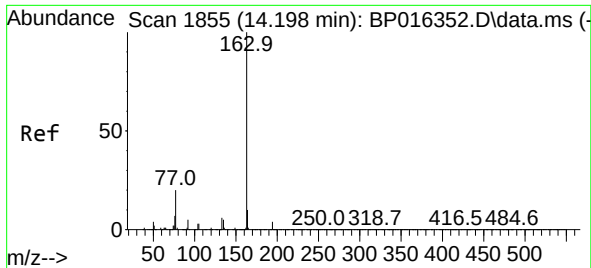

#47  
 Dimethylphthalate  
 Concen: 2.822 ng/ul  
 RT: 14.192 min Scan# 1854  
 Delta R.T. -0.015 min  
 Lab File: BP016368.D  
 Acq: 26 Jul 2023 03:51

Instrument :  
 BNA\_P  
 ClientSampleId :  
 A4731

Tgt Ion:163 Resp: 257707  
 Ion Ratio Lower Upper  
 163 100  
 194 4.1 3.3 4.9  
 164 10.0 7.9 11.9

