

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072623\
 Data File : BG058487.D
 Acq On : 26 Jul 2023 20:37
 Operator : MA/JU
 Sample : 03553-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :

Quant Time: Jul 27 02:17:59 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG071723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jul 26 17:43:09 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.813	152	49978	20.000	ng/ul	0.00
20) Naphthalene-d8	10.616	136	213670	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.458	164	150329	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.208	188	373747	20.000	ng/ul	0.00
79) Chrysene-d12	21.444	240	341054	20.000	ng/ul	0.00
88) Perylene-d12	24.517	264	391245	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.236	96	6486	4.777	ng/uL	0.00
4) Pyridine-d5	3.659	84	37905	9.405	ng/ul	0.00
7) Phenol-d5	6.985	99	26285	5.544	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.143	67	84914	28.655	ng/ul	0.00
11) 2-Chlorophenol-d4	7.349	132	73548	22.161	ng/ul	0.00
15) 4-Methylphenol-d8	8.524	113	46634	12.895	ng/ul	0.00
21) Nitrobenzene-d5	8.976	128	47547	29.688	ng/ul	0.00
24) 2-Nitrophenol-d4	9.699	143	51820	29.637	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.240	165	86440	25.789	ng/ul	0.00
31) 4-Chloroaniline-d4	10.757	131	120744	24.849	ng/ul	0.00
46) Dimethylphthalate-d6	13.865	166	337020	29.073	ng/ul	0.00
49) Acenaphthylene-d8	14.153	160	379812	31.265	ng/ul	0.00
54) 4-Nitrophenol-d4	14.693	143	685	0.391	ng/ul	0.01
60) Fluorene-d10	15.457	176	305987	31.882	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.580	200	39134	20.552	ng/ul	0.00
73) Anthracene-d10	17.302	188	566557	35.083	ng/ul	0.00
81) Pyrene-d10	19.599	212	717425	35.615	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.305	264	738081	39.031	ng/ul	0.00
Target Compounds						
78) Di-n-butylphthalate	18.166	149	56610	2.882	ng/ul#	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072623\
Data File : BG058487.D
Acq On : 26 Jul 2023 20:37
Operator : MA/JU
Sample : 03553-01
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :


Quant Time: Jul 27 02:17:59 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG071723.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jul 26 17:43:09 2023
Response via : Initial Calibration

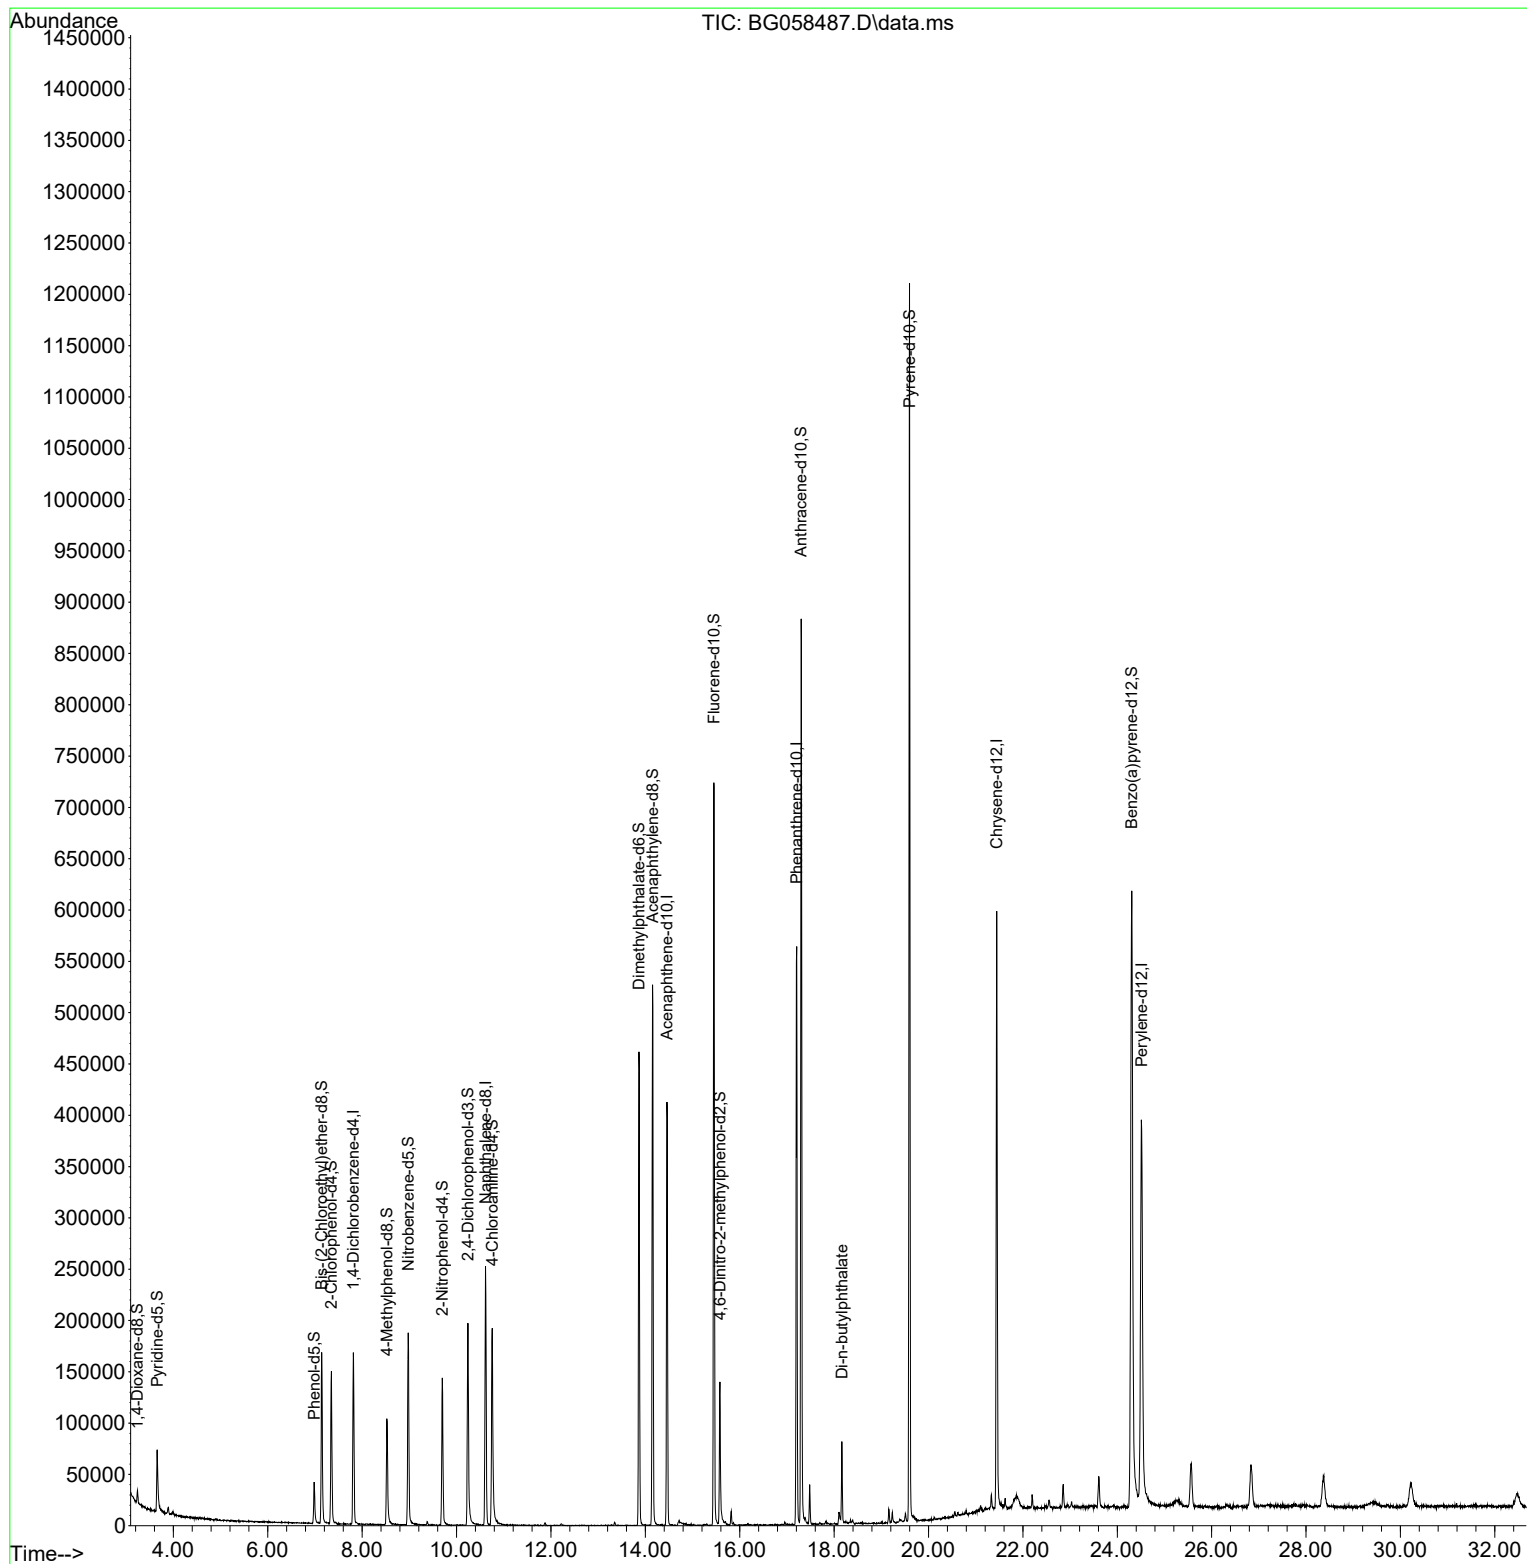

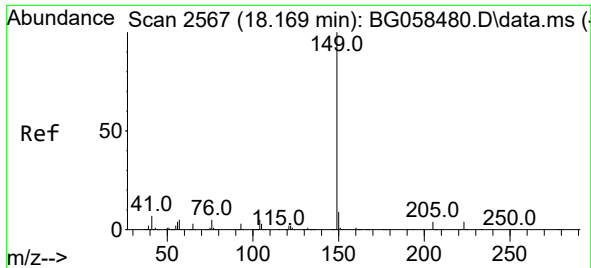

#78
 Di-n-butylphthalate
 Concen: 2.882 ng/ul
 RT: 18.166 min Scan# 21
 Delta R.T. -0.005 min
 Lab File: BG058487.D
 Acq: 26 Jul 2023 20:37

Instrument :
 BNA_P
 ClientSampleId :

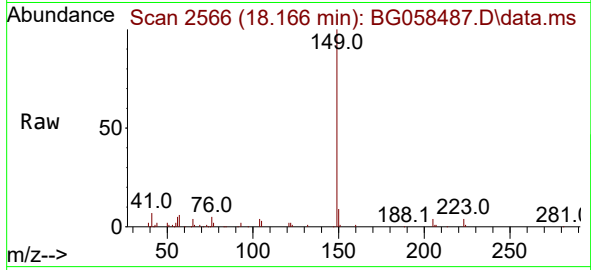

Tgt Ion:149 Resp: 56610
 Ion Ratio Lower Upper
 149 100
 150 8.9 7.2 10.8
 104 3.9 3.9 5.9#

