

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072623\
 Data File : BG058489.D
 Acq On : 26 Jul 2023 22:00
 Operator : MA/JU
 Sample : 03553-03
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :

Quant Time: Jul 27 02:18:16 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG071723.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jul 26 17:43:09 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.815	152	42612	20.000	ng/ul	0.00
20) Naphthalene-d8	10.618	136	194625	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.460	164	141519	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.204	188	338235	20.000	ng/ul	0.00
79) Chrysene-d12	21.446	240	297689	20.000	ng/ul	0.00
88) Perylene-d12	24.513	264	346568	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.238	96	6456	5.576	ng/uL	0.00
4) Pyridine-d5	3.655	84	47981	13.963	ng/ul	0.00
7) Phenol-d5	6.987	99	30295	7.494	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.145	67	98984	39.178	ng/ul	0.00
11) 2-Chlorophenol-d4	7.345	132	87697	30.993	ng/ul	0.00
15) 4-Methylphenol-d8	8.526	113	55599	18.032	ng/ul	0.00
21) Nitrobenzene-d5	8.979	128	58670	40.217	ng/ul	0.00
24) 2-Nitrophenol-d4	9.701	143	64226	40.327	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.242	165	102464	33.561	ng/ul	0.00
31) 4-Chloroaniline-d4	10.753	131	144023	32.541	ng/ul	0.00
46) Dimethylphthalate-d6	13.867	166	416331	38.150	ng/ul	0.00
49) Acenaphthylene-d8	14.155	160	466043	40.751	ng/ul	0.00
54) 4-Nitrophenol-d4	14.701	143	1033	0.627	ng/ul	0.02
60) Fluorene-d10	15.453	176	375587	41.570	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.577	200	39420	22.875	ng/ul	0.00
73) Anthracene-d10	17.304	188	632641	43.288	ng/ul	0.00
81) Pyrene-d10	19.595	212	756119	43.004	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.308	264	786894	46.977	ng/ul	0.00
Target Compounds						
					Qvalue	
78) Di-n-butylphthalate	18.162	149	104589	5.884	ng/ul	99
86) Bis(2-ethylhexyl)phtha...	21.335	149	11608	1.015	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072623\
Data File : BG058489.D
Acq On : 26 Jul 2023 22:00
Operator : MA/JU
Sample : 03553-03
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :

Quant Time: Jul 27 02:18:16 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG071723.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jul 26 17:43:09 2023
Response via : Initial Calibration

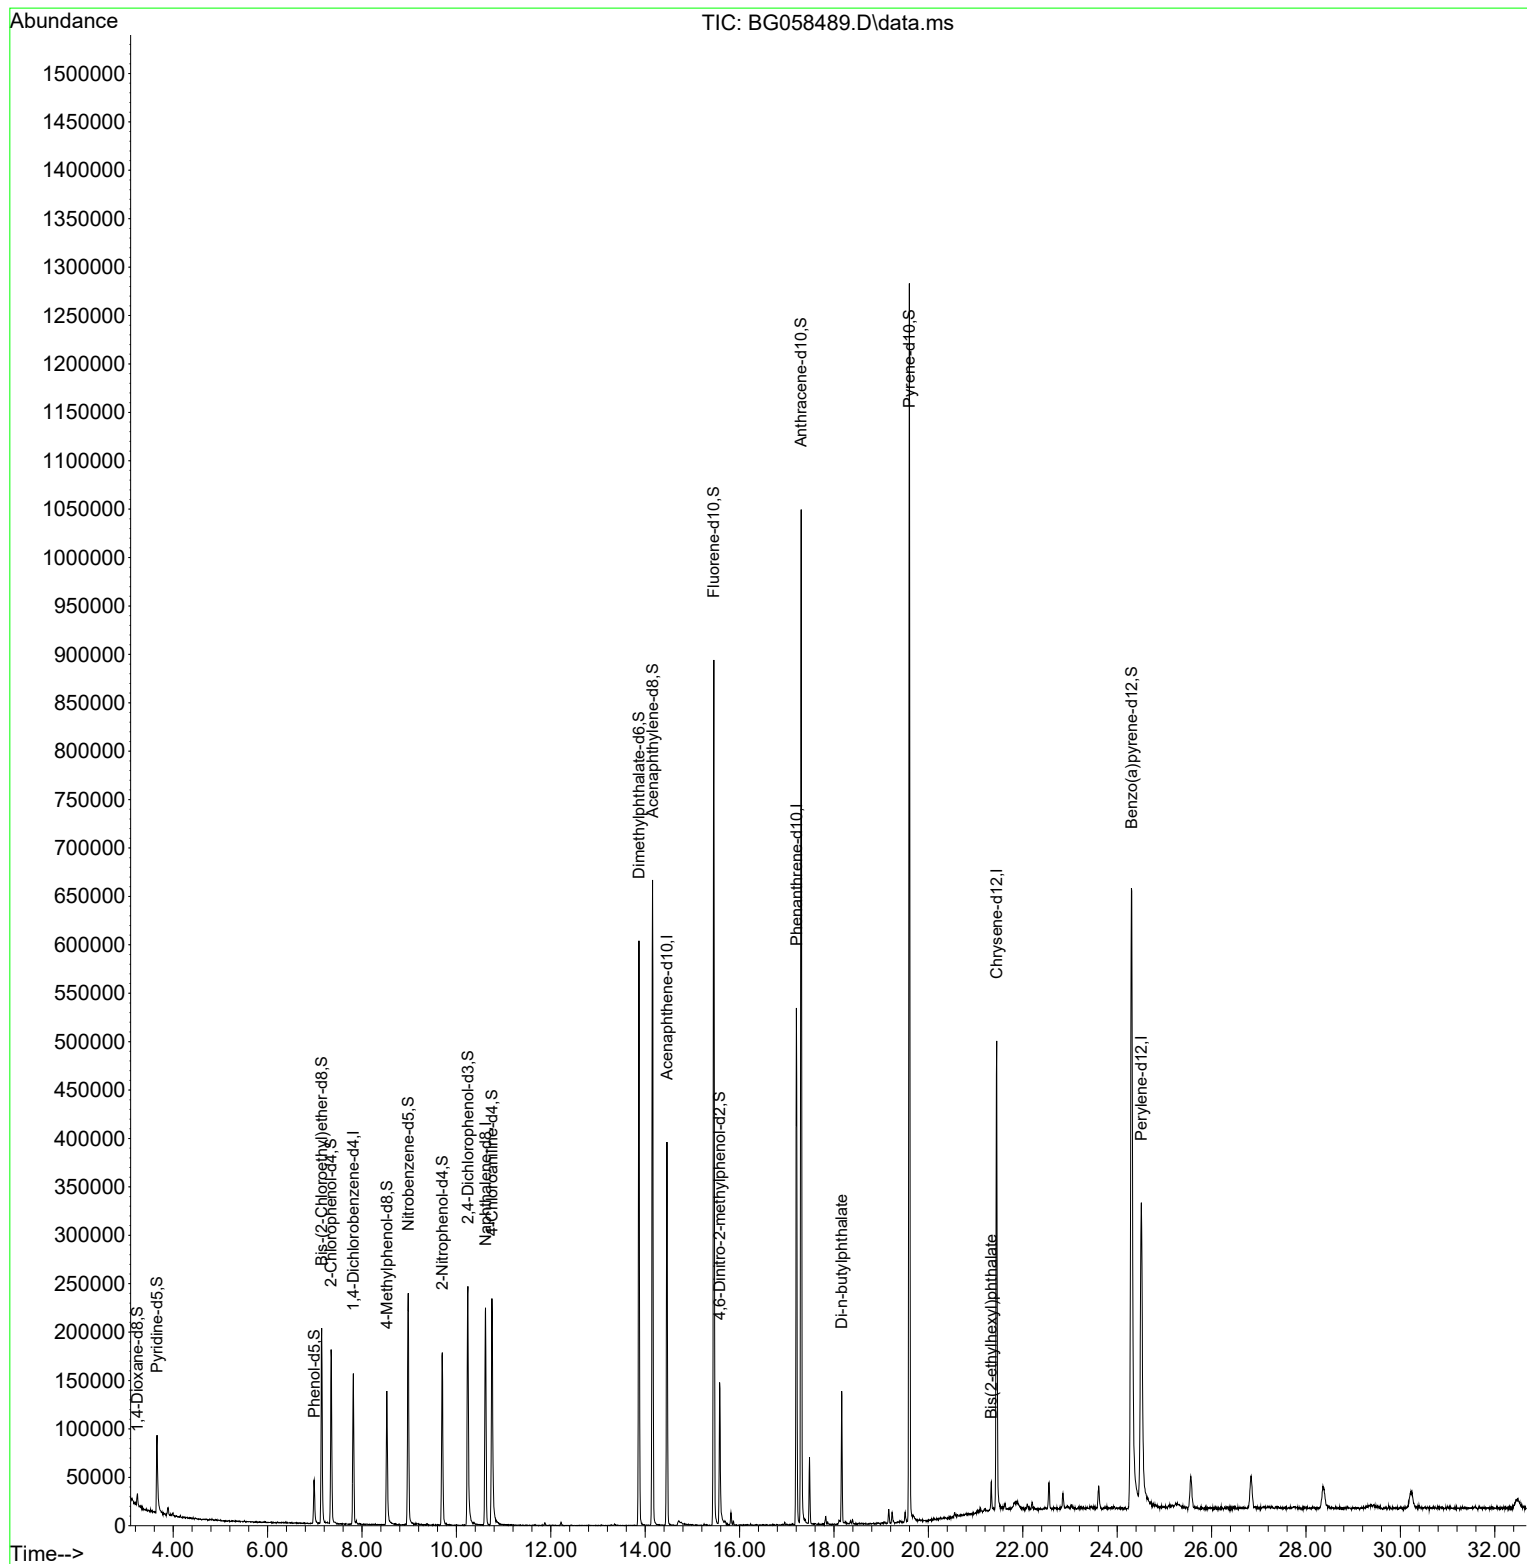

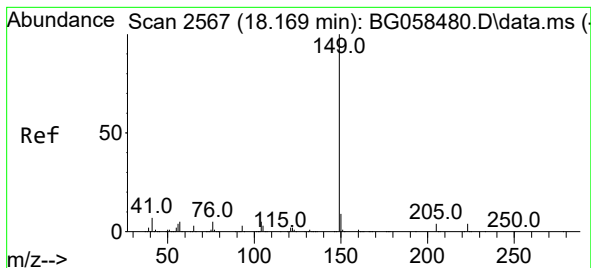

#78

Di-n-butylphthalate

Concen: 5.884 ng/ul

RT: 18.162 min Scan# 21

Delta R.T. -0.009 min

Lab File: BG058489.D

Acq: 26 Jul 2023 22:00

Instrument :

BNA_P

ClientSampleId :





Tgt Ion:149 Resp: 104589

Ion Ratio Lower Upper

149 100

150 9.2 7.2 10.8

104 5.0 3.9 5.9

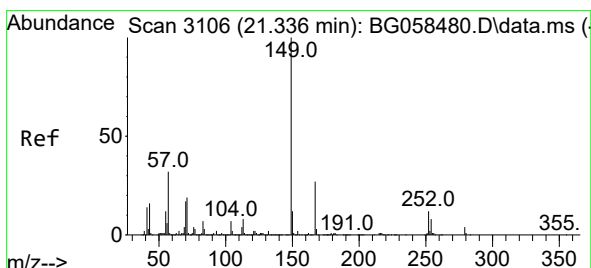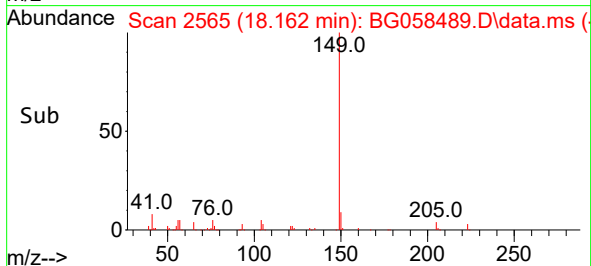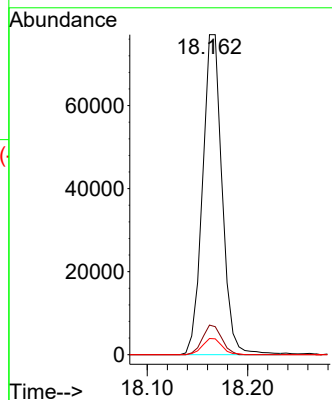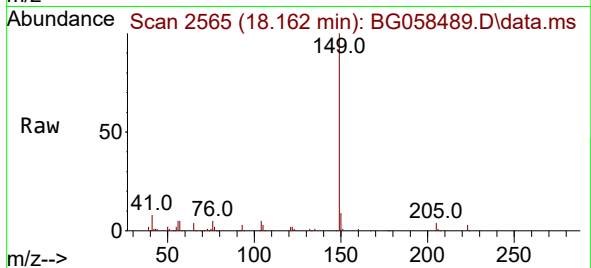

#86

Bis(2-ethylhexyl)phthalate

Concen: 1.015 ng/ul

RT: 21.335 min Scan# 3105

Delta R.T. -0.003 min

Lab File: BG058489.D

Acq: 26 Jul 2023 22:00

Tgt Ion:149 Resp: 11608

Ion Ratio Lower Upper

149 100

167 28.3 21.6 32.4

279 3.6 3.0 4.4

