

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072623\
 Data File : BP016378.D
 Acq On : 26 Jul 2023 16:57
 Operator : MA/JU
 Sample : 03575-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCHA0

Quant Time: Jul 26 23:45:35 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP072523.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jul 25 23:56:16 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.099	152	386180	20.000	ng/ul	0.00
20) Naphthalene-d8	10.928	136	1657148	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.734	164	1000124	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.498	188	2093430	20.000	ng/ul	0.00
79) Chrysene-d12	21.592	240	1756828	20.000	ng/ul	0.00
88) Perylene-d12	24.192	264	1735530	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.422	96	48780	4.981	ng/uL	0.00
4) Pyridine-d5	3.852	84	718233	25.847	ng/ul	0.00
7) Phenol-d5	7.222	99	1172052	36.268	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.428	67	679895	35.042	ng/ul	0.00
11) 2-Chlorophenol-d4	7.611	132	889801	35.293	ng/ul	0.00
15) 4-Methylphenol-d8	8.787	113	920418	35.415	ng/ul	0.00
21) Nitrobenzene-d5	9.287	128	430003	42.139	ng/ul	0.00
24) 2-Nitrophenol-d4	10.005	143	400598	47.600	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.528	165	850807	36.472	ng/ul	0.00
31) 4-Chloroaniline-d4	11.075	131	1164262	32.082	ng/ul	0.00
46) Dimethylphthalate-d6	14.151	166	2521557	34.449	ng/ul	0.00
49) Acenaphthylene-d8	14.440	160	3050083	35.271	ng/ul	0.00
54) 4-Nitrophenol-d4	14.916	143	369169	30.101	ng/ul	0.00
60) Fluorene-d10	15.728	176	2220677	35.662	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.839	200	153128	22.208	ng/ul	0.00
73) Anthracene-d10	17.598	188	3216281	34.684	ng/ul	0.00
81) Pyrene-d10	19.828	212	3615936	36.248	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.027	264	3054798	36.482	ng/ul	0.00
Target Compounds						
						Qvalue
47) Dimethylphthalate	14.193	163	1260087	17.071	ng/ul	99
71) Pentachlorophenol	17.122	266	680602	50.731	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072623\
Data File : BP016378.D
Acq On : 26 Jul 2023 16:57
Operator : MA/JU
Sample : 03575-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCHA0

Quant Time: Jul 26 23:45:35 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP072523.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jul 25 23:56:16 2023
Response via : Initial Calibration




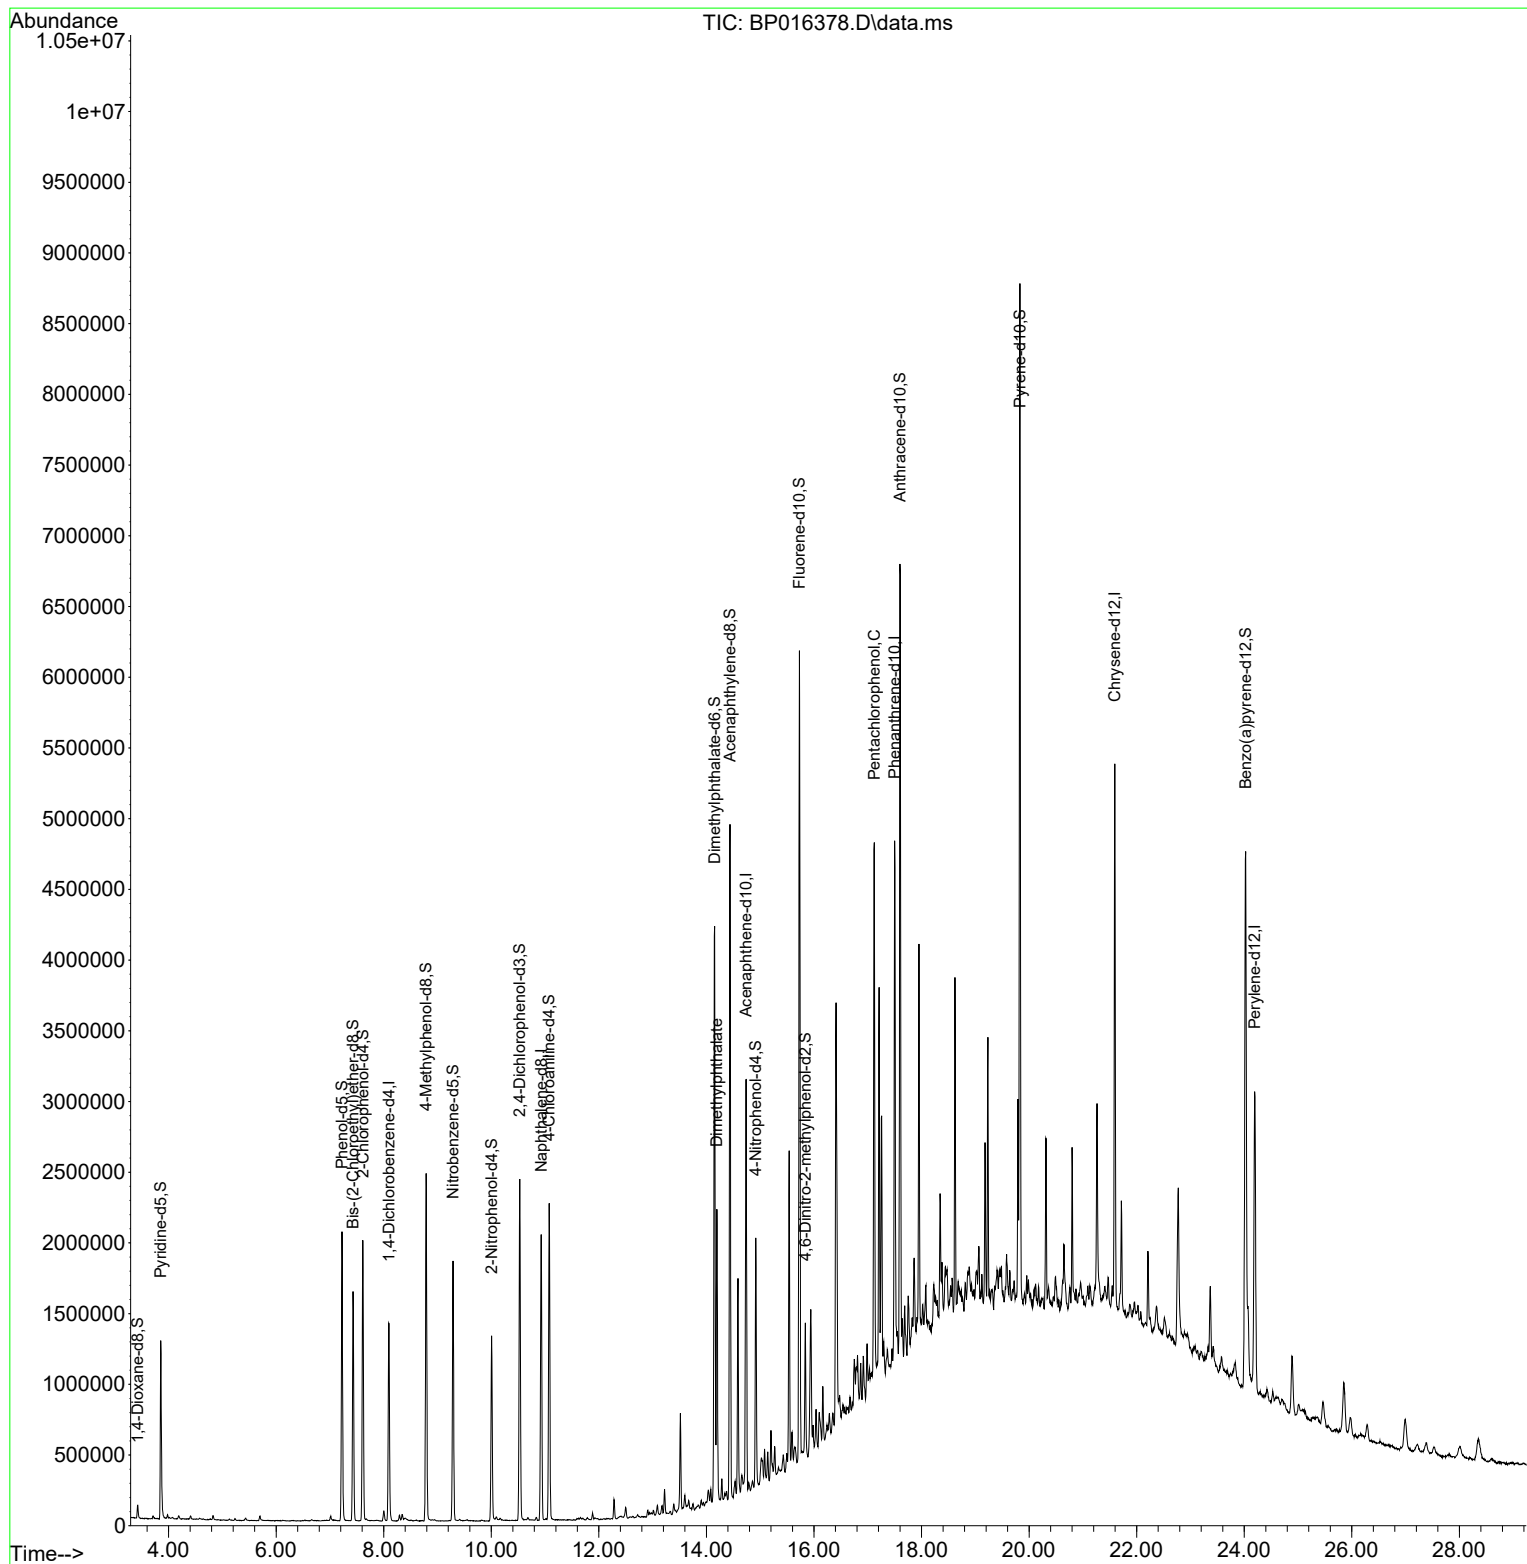


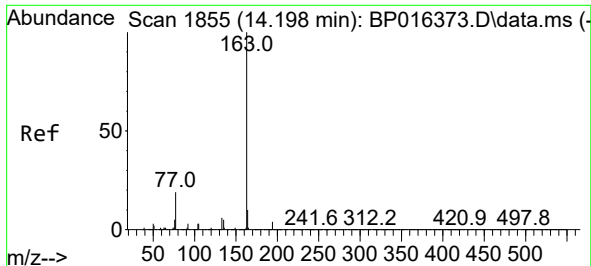

#47
Dimethylphthalate
Concen: 17.071 ng/ul
RT: 14.193 min Scan# 1855
Delta R.T. -0.015 min
Lab File: BP016378.D
Acq: 26 Jul 2023 16:57

Instrument :
BNA_P
ClientSampleId :
DCHA0

Tgt Ion:163 Resp: 1260087
Ion Ratio Lower Upper
163 100
194 3.9 3.3 4.9
164 10.5 7.9 11.9

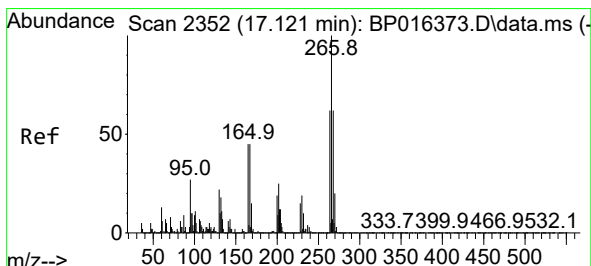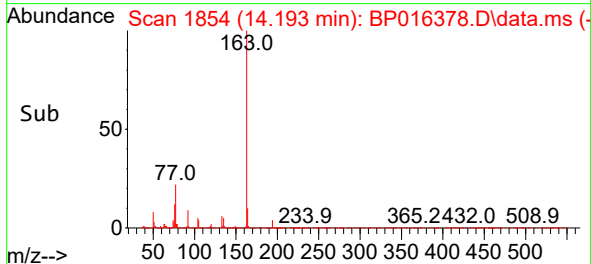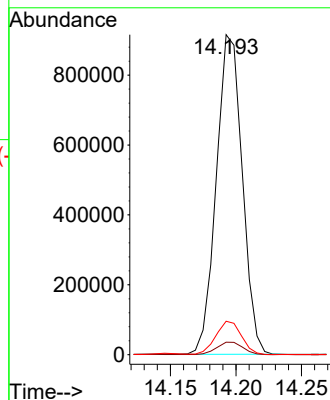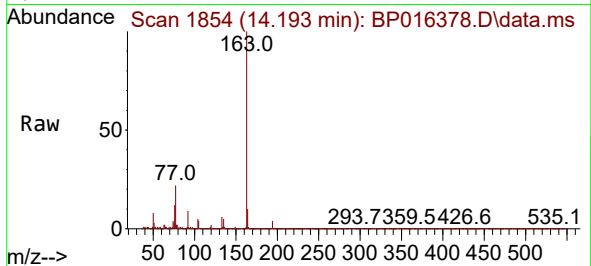

#71
Pentachlorophenol
Concen: 50.731 ng/ul
RT: 17.122 min Scan# 2352
Delta R.T. -0.003 min
Lab File: BP016378.D
Acq: 26 Jul 2023 16:57

Tgt Ion:266 Resp: 680602
Ion Ratio Lower Upper
266 100
264 63.1 50.9 76.3
268 64.0 51.5 77.3

