

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072623\
 Data File : BP016379.D
 Acq On : 26 Jul 2023 17:31
 Operator : MA/JU
 Sample : 03575-02
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DCHA1

Quant Time: Jul 26 23:45:46 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP072523.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jul 25 23:56:16 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.099	152	288616	20.000	ng/ul	0.00
20) Naphthalene-d8	10.928	136	1278962	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.739	164	794119	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.498	188	1730277	20.000	ng/ul	0.00
79) Chrysene-d12	21.586	240	1422053	20.000	ng/ul	-0.01
88) Perylene-d12	24.192	264	1363940	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.422	96	76010	10.384	ng/uL	0.00
4) Pyridine-d5	3.852	84	1160134	55.862	ng/ul	0.00
7) Phenol-d5	7.222	99	1676161	69.400	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.428	67	949691	65.494	ng/ul	0.00
11) 2-Chlorophenol-d4	7.610	132	1247308	66.197	ng/ul	0.00
15) 4-Methylphenol-d8	8.793	113	1346054	69.301	ng/ul	0.00
21) Nitrobenzene-d5	9.287	128	636551	80.826	ng/ul	0.00
24) 2-Nitrophenol-d4	10.004	143	633924	97.598	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.528	165	1257545	69.849	ng/ul	0.00
31) 4-Chloroaniline-d4	11.075	131	1847228	65.952	ng/ul	0.00
46) Dimethylphthalate-d6	14.151	166	3892721	66.978	ng/ul	0.00
49) Acenaphthylene-d8	14.440	160	4578481	66.681	ng/ul	0.00
54) 4-Nitrophenol-d4	14.922	143	631105	64.807	ng/ul	0.00
60) Fluorene-d10	15.734	176	3365059	68.059	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.839	200	319612	56.081	ng/ul	0.00
73) Anthracene-d10	17.604	188	5121734	66.825	ng/ul	0.00
81) Pyrene-d10	19.827	212	5655792	70.045	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.021	264	4712518	71.613	ng/ul	-0.01
Target Compounds						Qvalue
47) Dimethylphthalate	14.198	163	1293755	22.074	ng/ul	100
71) Pentachlorophenol	17.116	266	69119	6.233	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072623\
Data File : BP016379.D
Acq On : 26 Jul 2023 17:31
Operator : MA/JU
Sample : 03575-02
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DCHA1

Quant Time: Jul 26 23:45:46 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP072523.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jul 25 23:56:16 2023
Response via : Initial Calibration




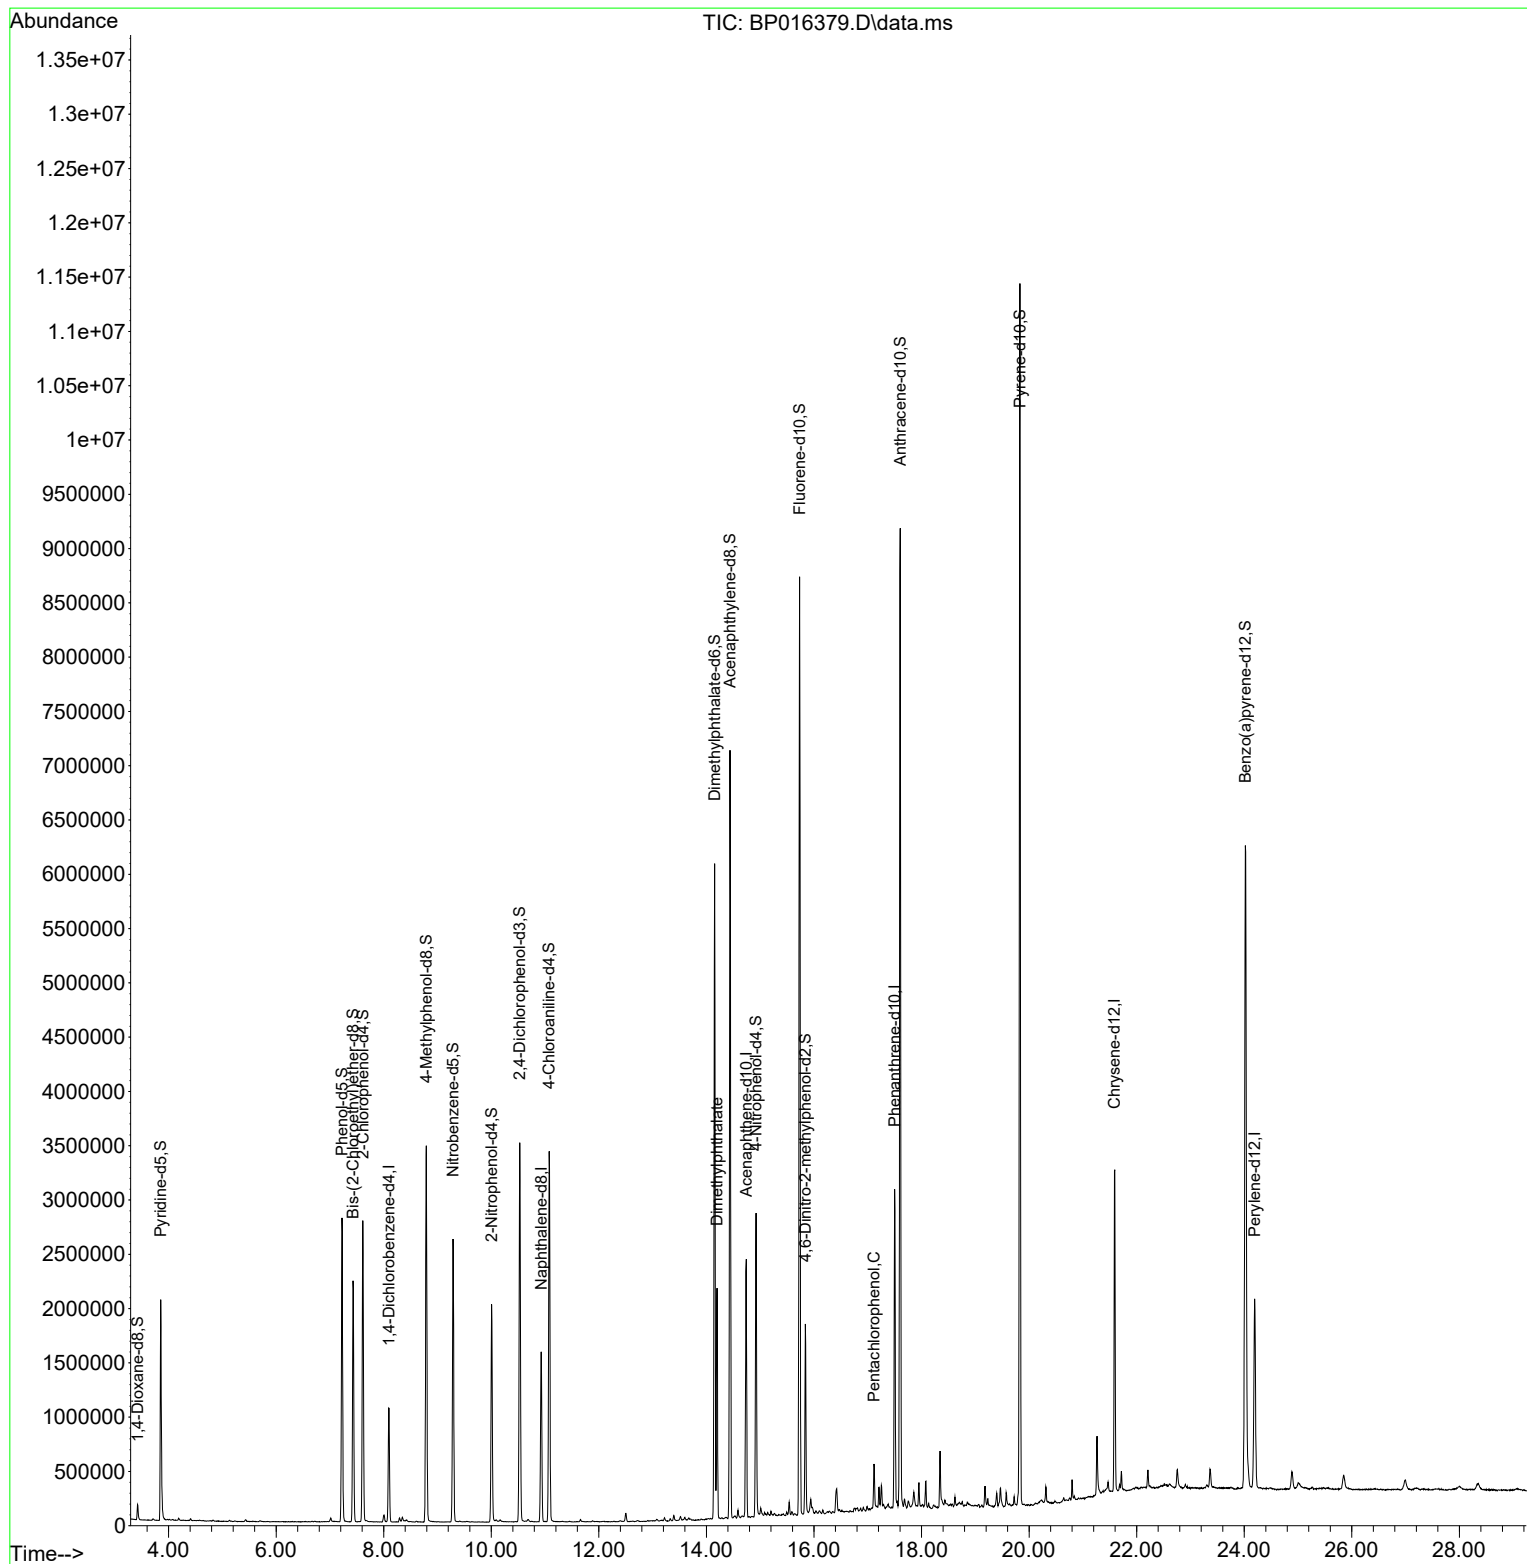


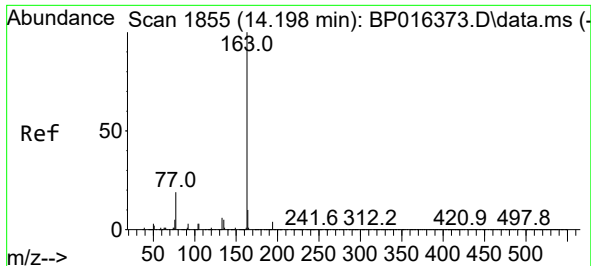

#47
Dimethylphthalate
Concen: 22.074 ng/ul
RT: 14.198 min Scan# 1855
Delta R.T. -0.009 min
Lab File: BP016379.D
Acq: 26 Jul 2023 17:31

Instrument :
BNA_P
ClientSampleId :
DCHA1

Tgt Ion:163 Resp: 1293755
Ion Ratio Lower Upper
163 100
194 4.1 3.3 4.9
164 10.1 7.9 11.9

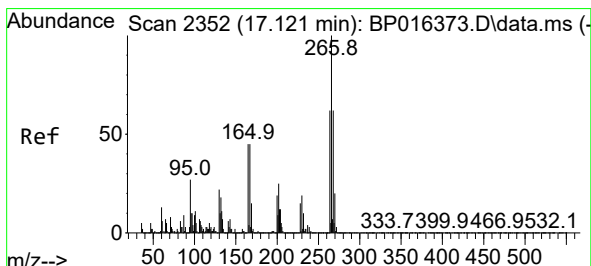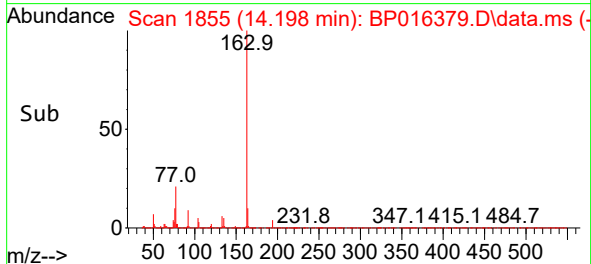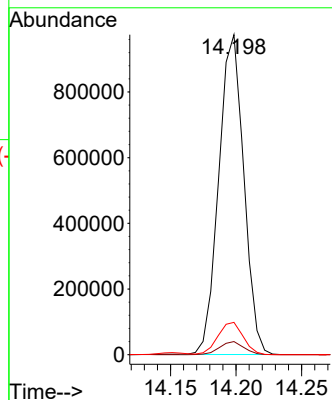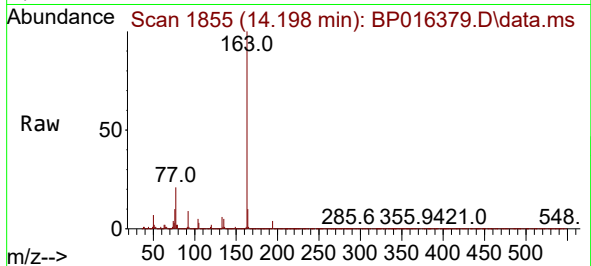

#71
Pentachlorophenol
Concen: 6.233 ng/ul
RT: 17.116 min Scan# 2351
Delta R.T. -0.009 min
Lab File: BP016379.D
Acq: 26 Jul 2023 17:31

Tgt Ion:266 Resp: 69119
Ion Ratio Lower Upper
266 100
264 60.4 50.9 76.3
268 64.5 51.5 77.3

