

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072623\
 Data File : BP016389.D
 Acq On : 26 Jul 2023 23:13
 Operator : MA/JU
 Sample : 03534-15
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A4729

Quant Time: Jul 27 00:51:00 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP072523.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jul 25 23:56:16 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.093	152	462653	20.000	ng/u1	0.00
20) Naphthalene-d8	10.928	136	2035311	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.734	164	1248760	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.498	188	2758904	20.000	ng/u1	0.00
79) Chrysene-d12	21.586	240	2313296	20.000	ng/u1	-0.01
88) Perylene-d12	24.186	264	1779106	20.000	ng/u1	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.428	96	26372	2.248	ng/uL	0.00
4) Pyridine-d5	3.852	84	322424	9.685	ng/u1	0.00
7) Phenol-d5	7.222	99	318307	8.222	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.428	67	404033	17.382	ng/u1	0.00
11) 2-Chlorophenol-d4	7.611	132	273126	9.043	ng/u1	0.00
15) 4-Methylphenol-d8	8.787	113	192550	6.184	ng/u1	0.00
21) Nitrobenzene-d5	9.287	128	258326	20.612	ng/u1	0.00
24) 2-Nitrophenol-d4	10.005	143	238390	23.063	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.528	165	169778	5.926	ng/u1	0.00
31) 4-Chloroaniline-d4	11.087	131	22210	0.498	ng/u1	0.00
46) Dimethylphthalate-d6	14.145	166	1682468	18.409	ng/u1	-0.01
49) Acenaphthylene-d8	14.434	160	1675754	15.520	ng/u1	0.00
54) 4-Nitrophenol-d4	14.916	143	226722	14.805	ng/u1	0.00
60) Fluorene-d10	15.728	176	1461003	18.791	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.839	200	79072	8.701	ng/u1	0.00
73) Anthracene-d10	17.598	188	833363	6.819	ng/u1	0.00
81) Pyrene-d10	19.822	212	2182421	16.615	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.010	264	565176	6.584	ng/u1	-0.03
Target Compounds						
16) Acetophenone	8.940	105	80978	1.648	ng/u1	96
47) Dimethylphthalate	14.193	163	140071	1.520	ng/u1	99
86) Bis(2-ethylhexyl)phtha...	21.463	149	166671	1.774	ng/u1	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072623\
Data File : BP016389.D
Acq On : 26 Jul 2023 23:13
Operator : MA/JU
Sample : 03534-15
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A4729

Quant Time: Jul 27 00:51:00 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP072523.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jul 25 23:56:16 2023
Response via : Initial Calibration




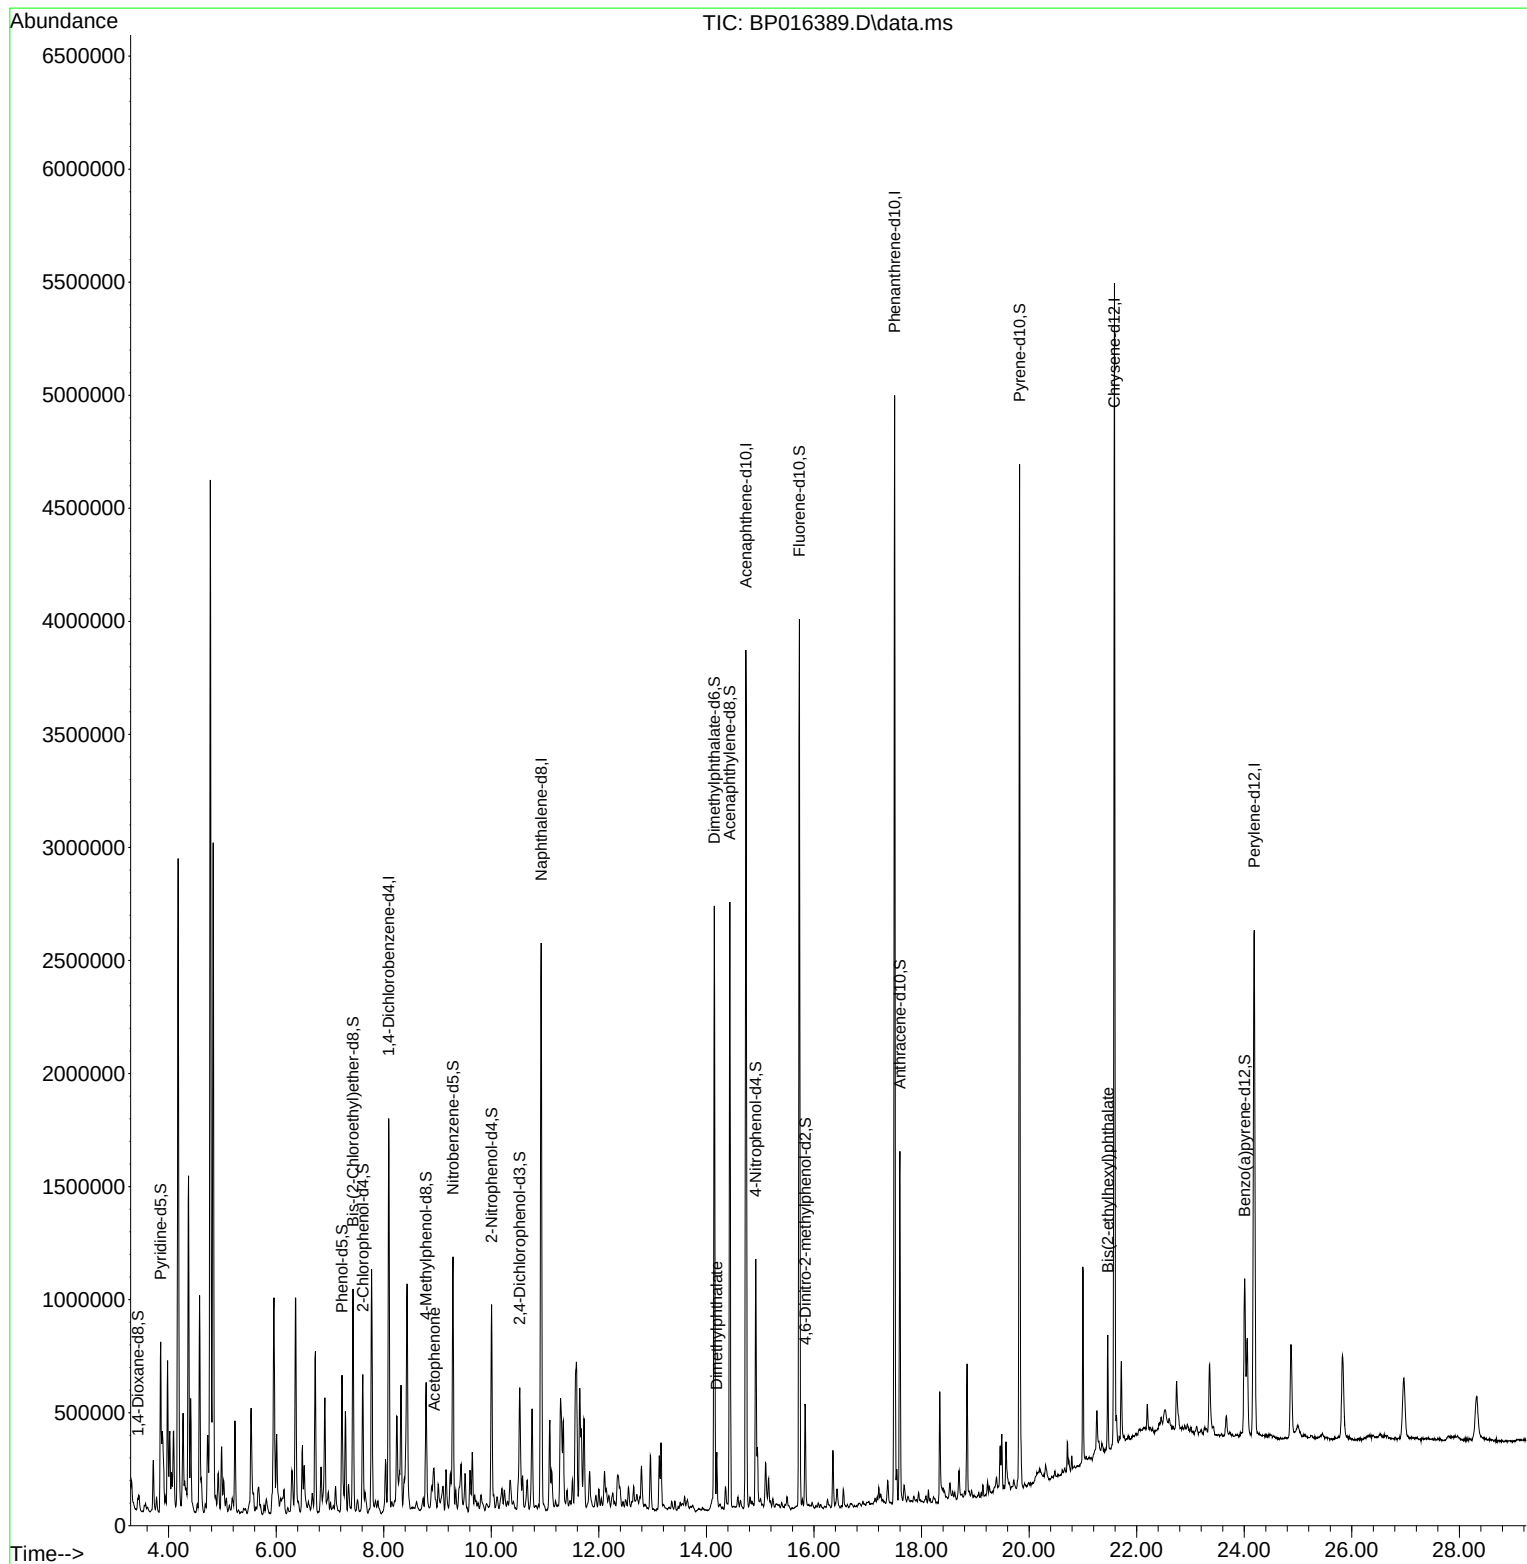


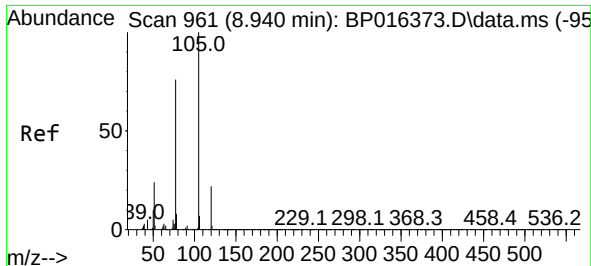

#16
Acetophenone
Concen: 1.648 ng/ul
RT: 8.940 min Scan# 90
Delta R.T. -0.009 min
Lab File: BP016389.D
Acq: 26 Jul 2023 23:13




Instrument :
BNA_P
ClientSampleId :
A4729


Tgt Ion:105 Resp: 80978
Ion Ratio Lower Upper
105 100
77 79.8 61.2 91.8
51 26.4 19.1 28.7

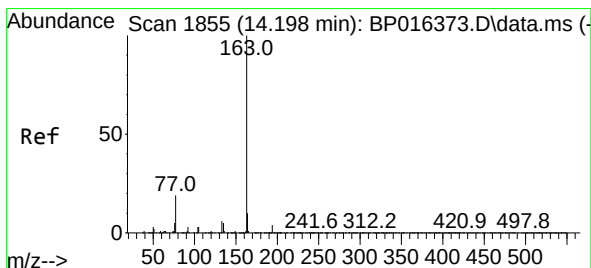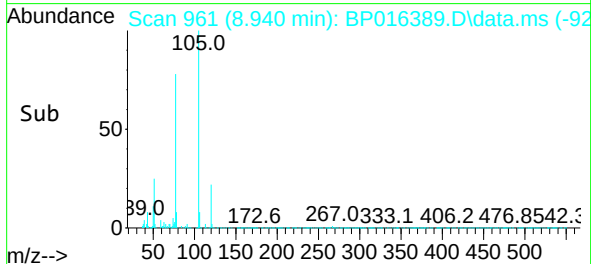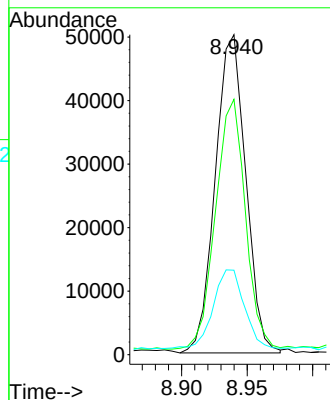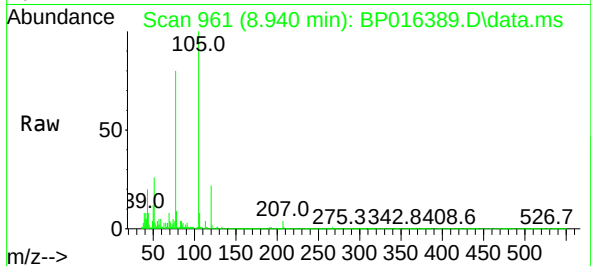

#47
Dimethylphthalate
Concen: 1.520 ng/ul
RT: 14.193 min Scan# 1854
Delta R.T. -0.015 min
Lab File: BP016389.D
Acq: 26 Jul 2023 23:13

Tgt Ion:163 Resp: 140071
Ion Ratio Lower Upper
163 100
194 3.9 3.3 4.9
164 10.3 7.9 11.9

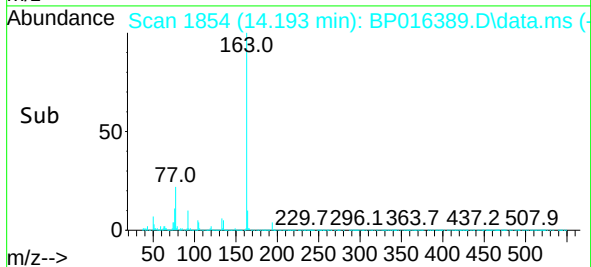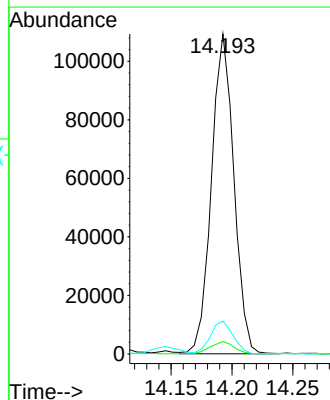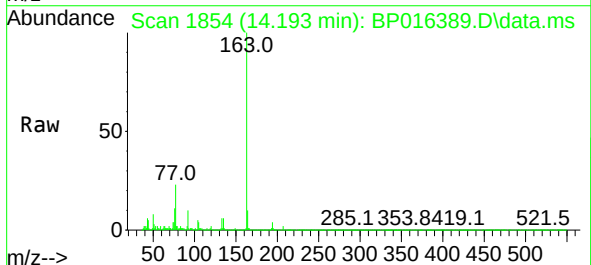

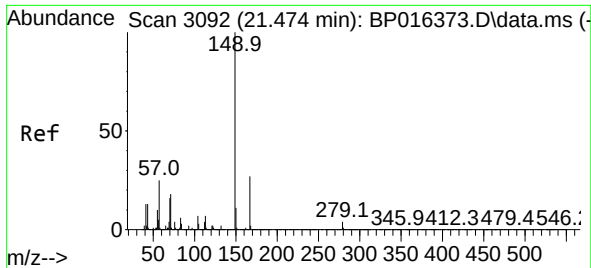

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 1.774 ng/ul
 RT: 21.463 min Scan# 3090
 Delta R.T. -0.021 min
 Lab File: BP016389.D
 Acq: 26 Jul 2023 23:13

Instrument :
 BNA_P
 ClientSampleId :
 A4729

Tgt Ion:149 Resp: 166671
 Ion Ratio Lower Upper
 149 100
 167 27.0 21.7 32.5
 279 4.2 3.0 4.4

