

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072623\
 Data File : BP016374.D
 Acq On : 26 Jul 2023 14:40
 Operator : MA/JU
 Sample : PB154224BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK224

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP072523.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP016374.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.428	20	24	31	rVB	155533	191730	1.94%	0.163%
2	3.857	92	97	110	rBV	2096924	3003836	30.36%	2.553%
3	4.193	149	154	161	rVB	29579	48681	0.49%	0.041%
4	7.222	661	669	683	rBV	2314589	3612632	36.51%	3.070%
5	7.428	696	704	714	rBV	1864275	2892893	29.24%	2.459%
6	7.610	728	735	746	rBV	2253650	3525094	35.63%	2.996%
7	8.093	810	817	830	rBV	1783844	2851803	28.82%	2.424%
8	8.787	928	935	947	rBV	2789979	4469283	45.17%	3.798%
9	9.287	1011	1020	1033	rBV	2120833	3437491	34.74%	2.922%
10	10.004	1130	1142	1151	rBV	1451066	2374401	24.00%	2.018%
11	10.528	1223	1231	1247	rBV	2712299	4424558	44.72%	3.760%
12	10.928	1291	1299	1306	rBV	2565223	4298440	43.44%	3.653%
13	11.075	1313	1324	1338	rBV	2873597	4743629	47.94%	4.032%
14	11.863	1452	1458	1462	rBV9	5968	13003	0.13%	0.011%
15	12.498	1561	1566	1572	rBV	52049	85506	0.86%	0.073%
16	13.592	1745	1752	1762	rVV	59286	101570	1.03%	0.086%
17	13.704	1766	1771	1776	rVB3	9355	14084	0.14%	0.012%
18	14.145	1840	1846	1857	rBV	4519428	6442876	65.12%	5.476%
19	14.433	1886	1895	1903	rBV	5325486	8090284	81.77%	6.876%
20	14.739	1939	1947	1956	rBV	3877591	5700951	57.62%	4.845%
21	14.916	1969	1977	2002	rBV	1768354	2701322	27.30%	2.296%
22	15.733	2109	2116	2123	rBV	6513560	9568790	96.71%	8.133%
23	15.839	2126	2134	2149	rVV	920259	1287330	13.01%	1.094%
24	15.969	2152	2156	2164	rVB	33106	49585	0.50%	0.042%
25	16.304	2209	2213	2218	rVB6	6789	12220	0.12%	0.010%
26	17.169	2354	2360	2365	rVB10	10167	15801	0.16%	0.013%
27	17.280	2376	2379	2383	rBV3	11254	16431	0.17%	0.014%
28	17.498	2408	2416	2425	rBV	4397942	6414252	64.83%	5.452%
29	17.604	2427	2434	2444	rVV	6694802	9780650	98.85%	8.313%
30	19.398	2735	2739	2745	rBV2	77963	106399	1.08%	0.090%
31	19.468	2745	2751	2760	rBV	77120	122404	1.24%	0.104%
32	19.721	2791	2794	2798	rBV5	13394	16874	0.17%	0.014%
33	19.827	2806	2812	2823	rBV	7735437	9894052	100.00%	8.409%
34	21.592	3106	3112	3121	rBV	3656899	4770302	48.21%	4.054%
35	24.027	3517	3526	3544	rBV2	3626192	7927603	80.12%	6.738%
36	24.198	3547	3555	3566	rVB	2163860	4653331	47.03%	3.955%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072623\
Data File : BP016374.D
Acq On : 26 Jul 2023 14:40
Operator : MA/JU
Sample : PB154224BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK224

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP072523.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 117660091

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072623\
Data File : BP016374.D
Acq On : 26 Jul 2023 14:40
Operator : MA/JU
Sample : PB154224BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK224

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP072523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

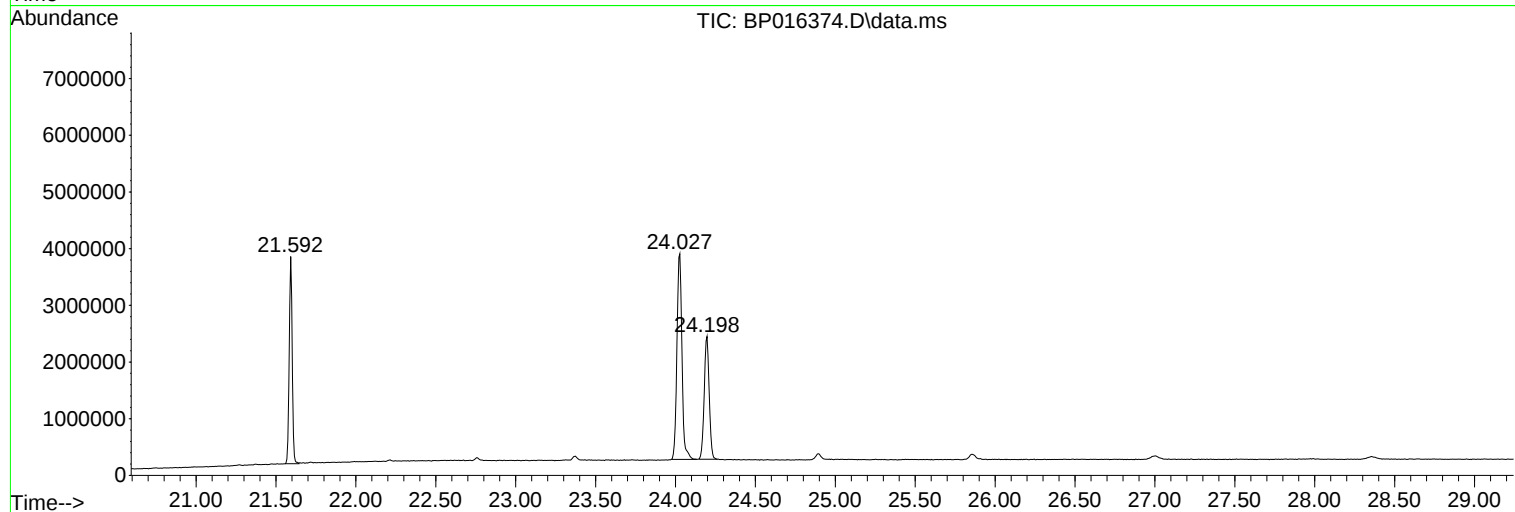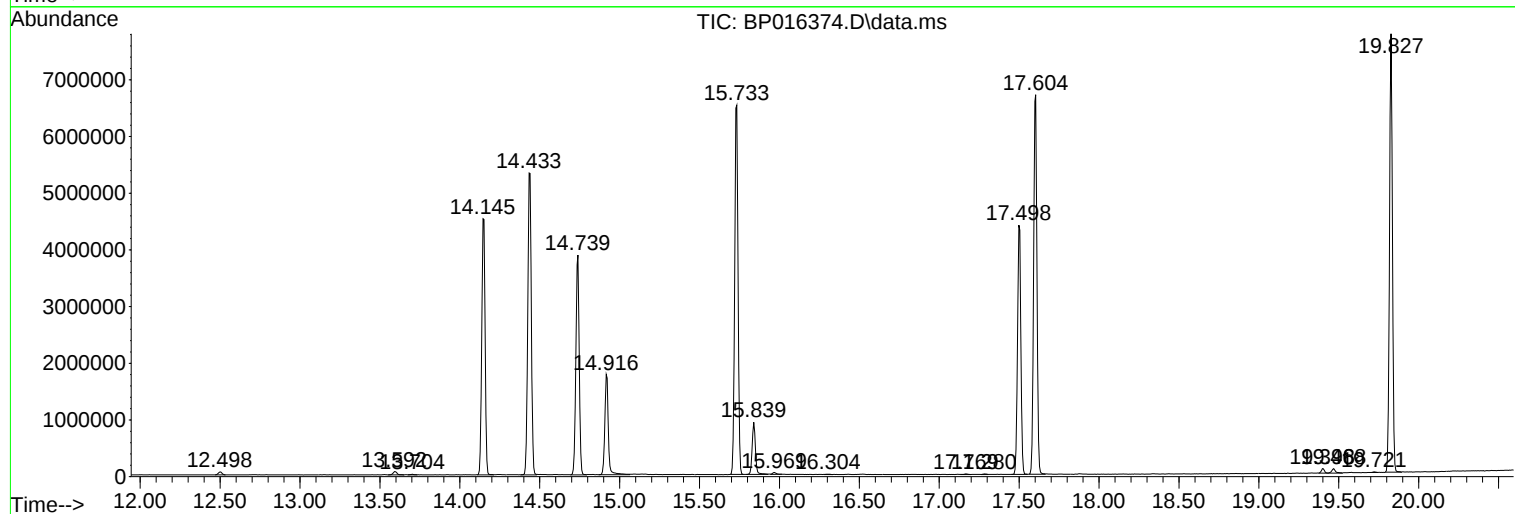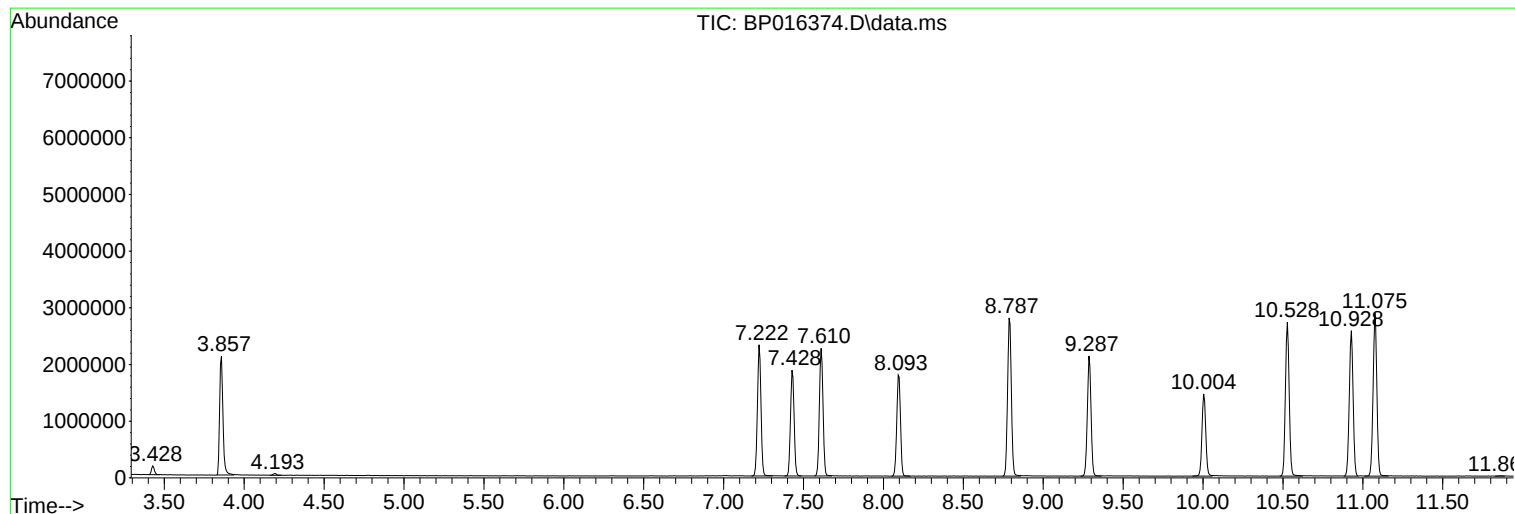

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072623\
Data File : BP016374.D
Acq On : 26 Jul 2023 14:40
Operator : MA/JU
Sample : PB154224BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK224

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP072523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072623\
Data File : BP016374.D
Acq On : 26 Jul 2023 14:40
Operator : MA/JU
Sample : PB154224BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK224

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP072523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------