
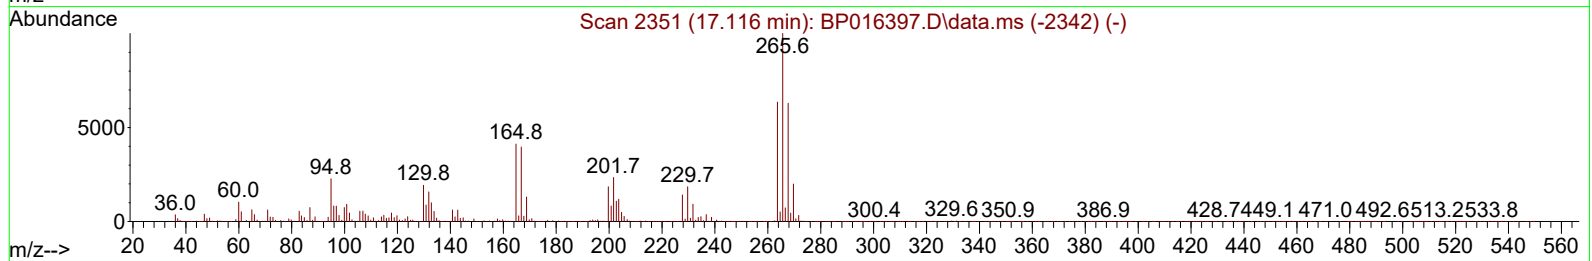
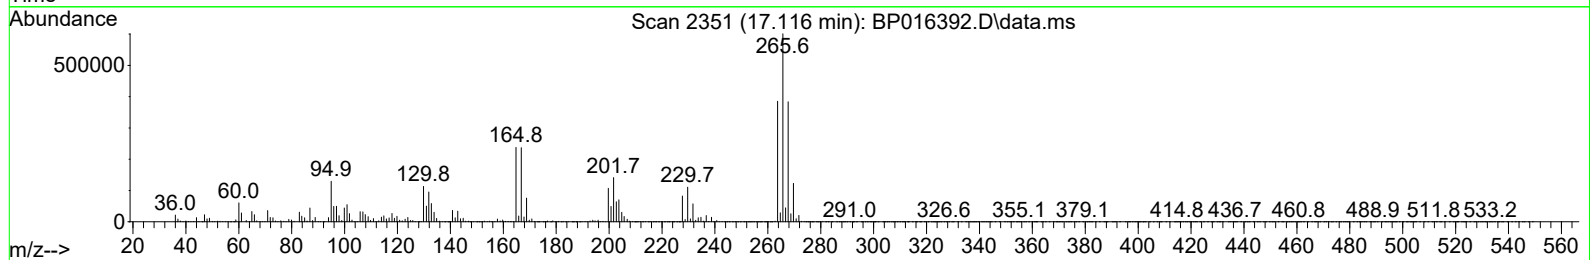


Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP072723\  
Data File : BP016392.D  
Acq On : 27 Jul 2023 09:55  
Operator : MA/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 28 04:44:53 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP072723.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Jul 28 01:48:25 2023  
Response via : Initial Calibration

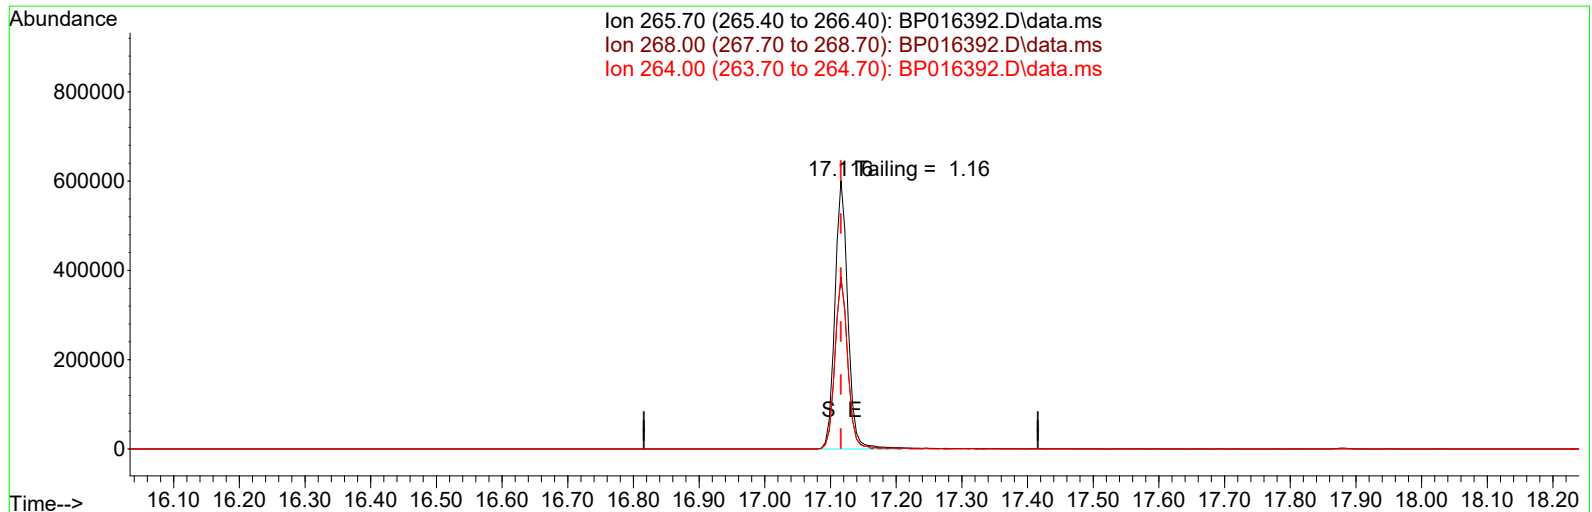

TIC: BP016392.D\data.ms

**(70) Pentachlorophenol (C)**




17.116min (-0.000) 104614.76 ng

response 830934

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 67.40  | 68.10  |
| 264.00 | 68.60  | 68.84  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP072723\  
Data File : BP016392.D  
Acq On : 27 Jul 2023 09:55  
Operator : MA/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 28 04:44:53 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP072723.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Jul 28 01:48:25 2023  
Response via : Initial Calibration

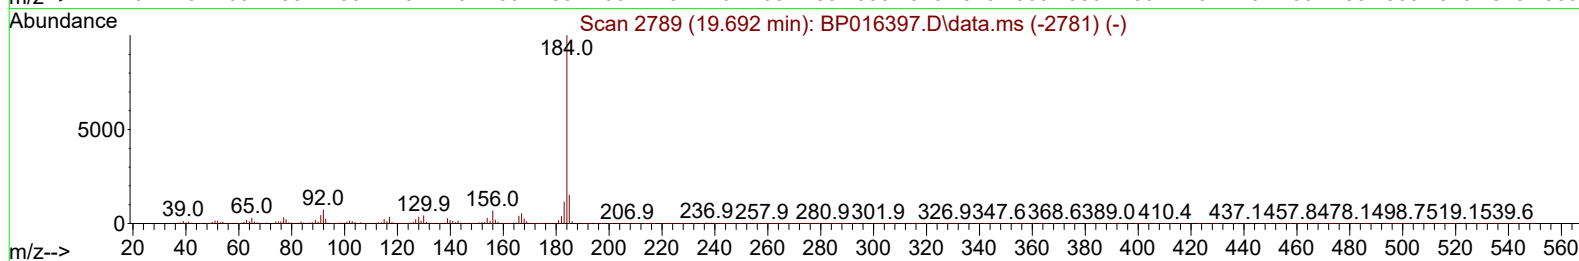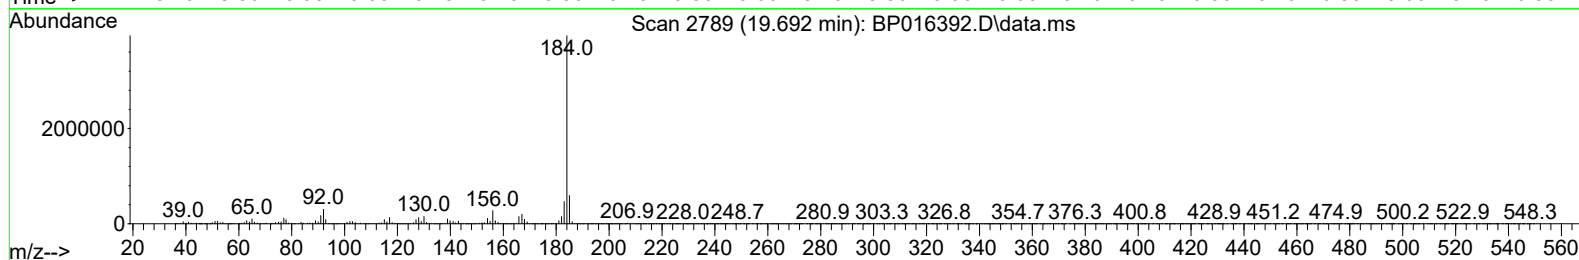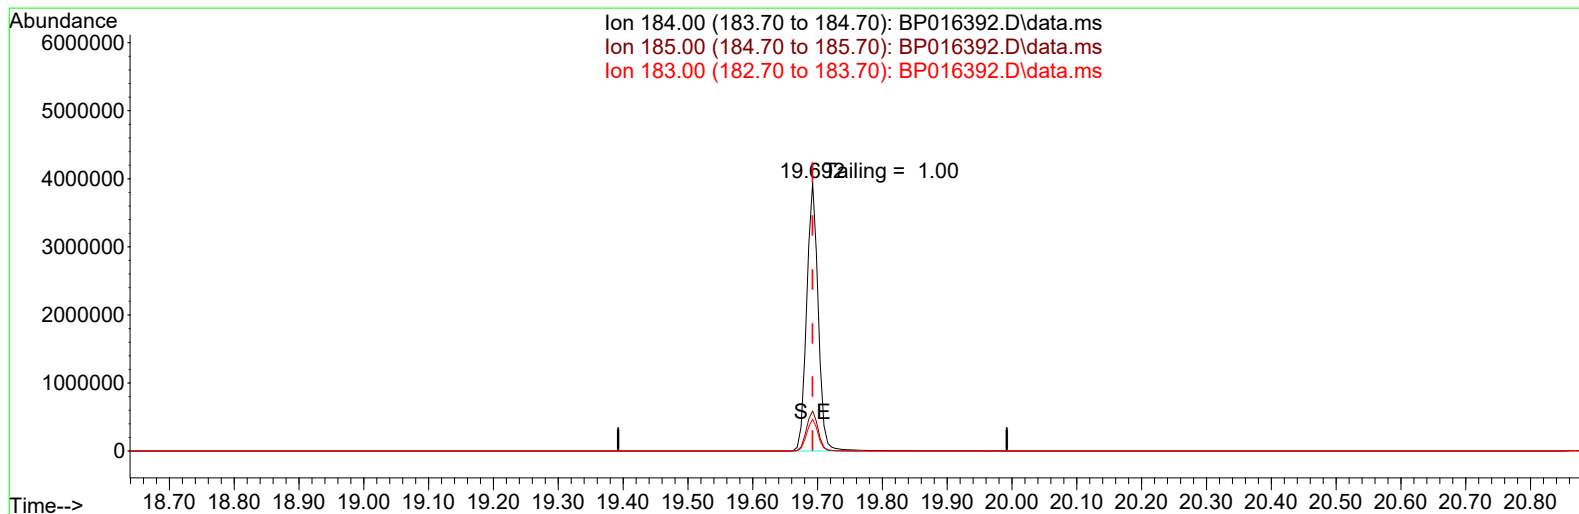

TIC: BP016392.D\data.ms

**(77) Benzidine****19.692min (-0.000) 180967.88 ng****response 4885195**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 15.00  | 14.97  |
| 183.00 | 11.50  | 11.81  |
| 0.00   | 0.00   | 0.00   |