

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072723\
 Data File : BP016404.D
 Acq On : 27 Jul 2023 17:21
 Operator : MA/JU
 Sample : 03706-08
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 B-P21B

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072723.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP016404.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.605	386	394	406	rBV	4702758	6911230	49.44%	8.758%
2	7.222	662	669	680	rBV	4496339	7173922	51.32%	9.091%
3	8.093	807	817	825	rBV	1576399	2451839	17.54%	3.107%
4	9.287	1011	1020	1034	rBV	2794664	4446887	31.81%	5.635%
5	10.922	1290	1298	1307	rBV	2009040	3380034	24.18%	4.283%
6	13.363	1701	1713	1721	rBV	6713273	9920085	70.97%	12.570%
7	14.734	1936	1946	1953	rBV	2976069	4335002	31.01%	5.493%
8	16.228	2192	2200	2213	rBV	4845185	7315240	52.33%	9.270%
9	17.498	2409	2416	2422	rBV	3781072	5292013	37.86%	6.706%
10	17.604	2429	2434	2443	rVB2	106260	169134	1.21%	0.214%
11	18.339	2554	2559	2571	rBV	247481	380501	2.72%	0.482%
12	19.475	2748	2752	2758	rBV	139659	190007	1.36%	0.241%
13	19.569	2764	2768	2777	rBV4	102327	155441	1.11%	0.197%
14	19.716	2789	2793	2803	rBV	379840	454226	3.25%	0.576%
15	20.039	2841	2848	2857	rBV	11527400	13977830	100.00%	17.712%
16	21.257	3051	3055	3066	rBV3	256047	458766	3.28%	0.581%
17	21.586	3106	3111	3121	rBV	4436660	5780094	41.35%	7.324%
18	24.186	3545	3553	3564	rBV	2795379	6124071	43.81%	7.760%




Sum of corrected areas: 78916322

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072723\
Data File : BP016404.D
Acq On : 27 Jul 2023 17:21
Operator : MA/JU
Sample : 03706-08
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
B-P21B

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

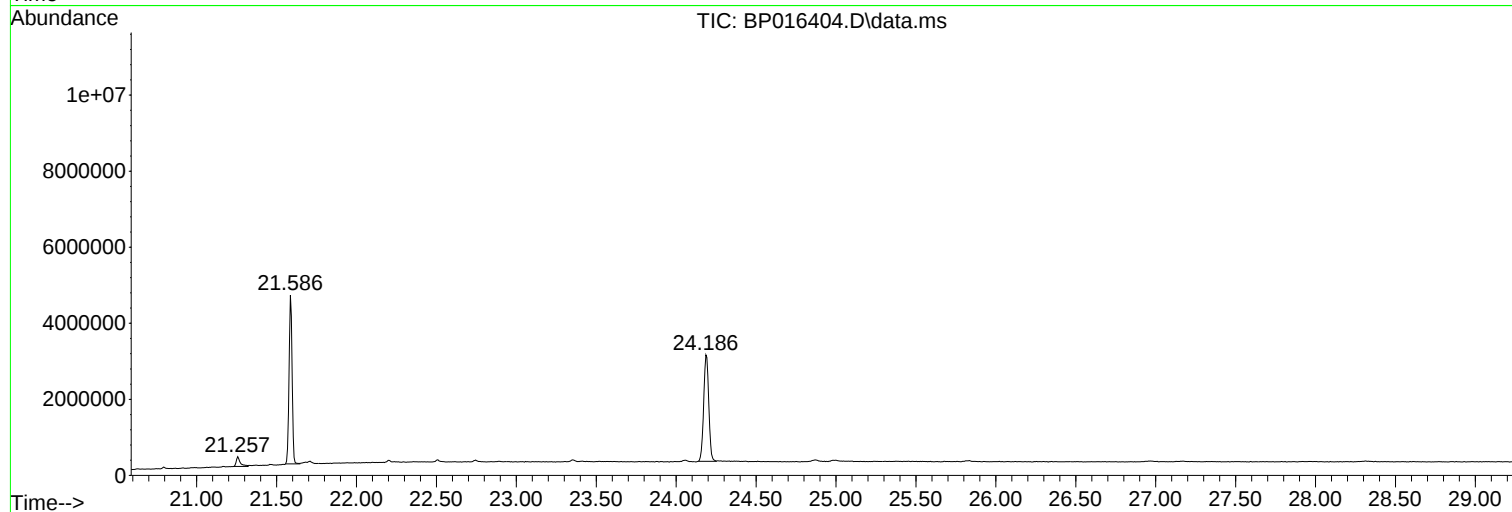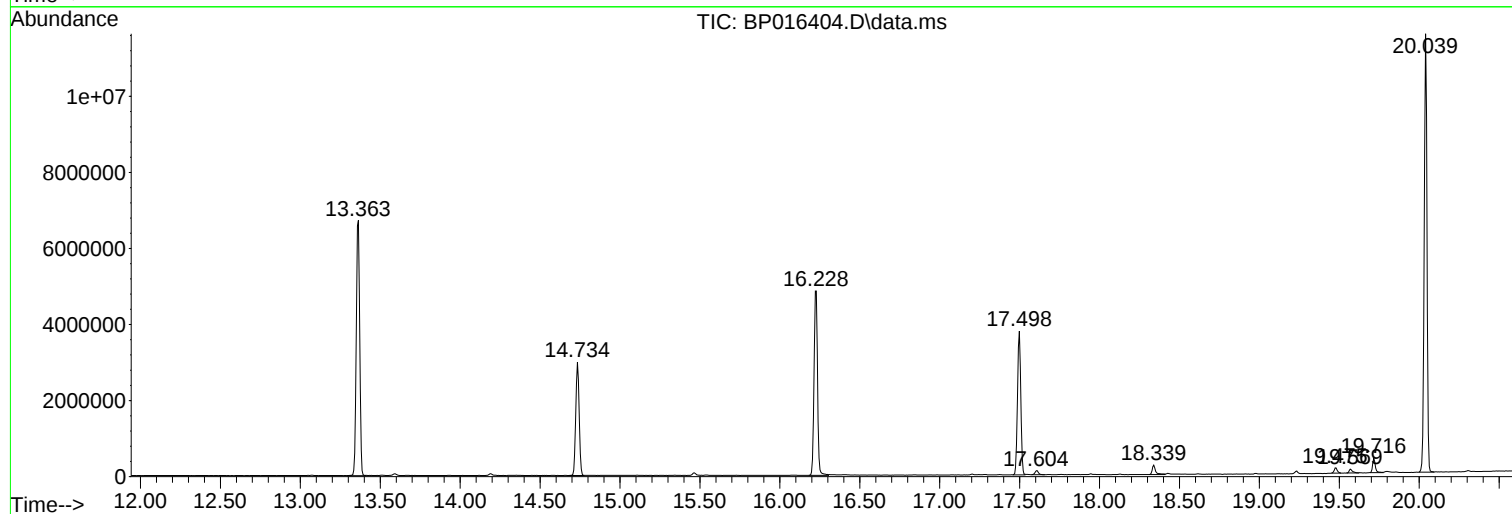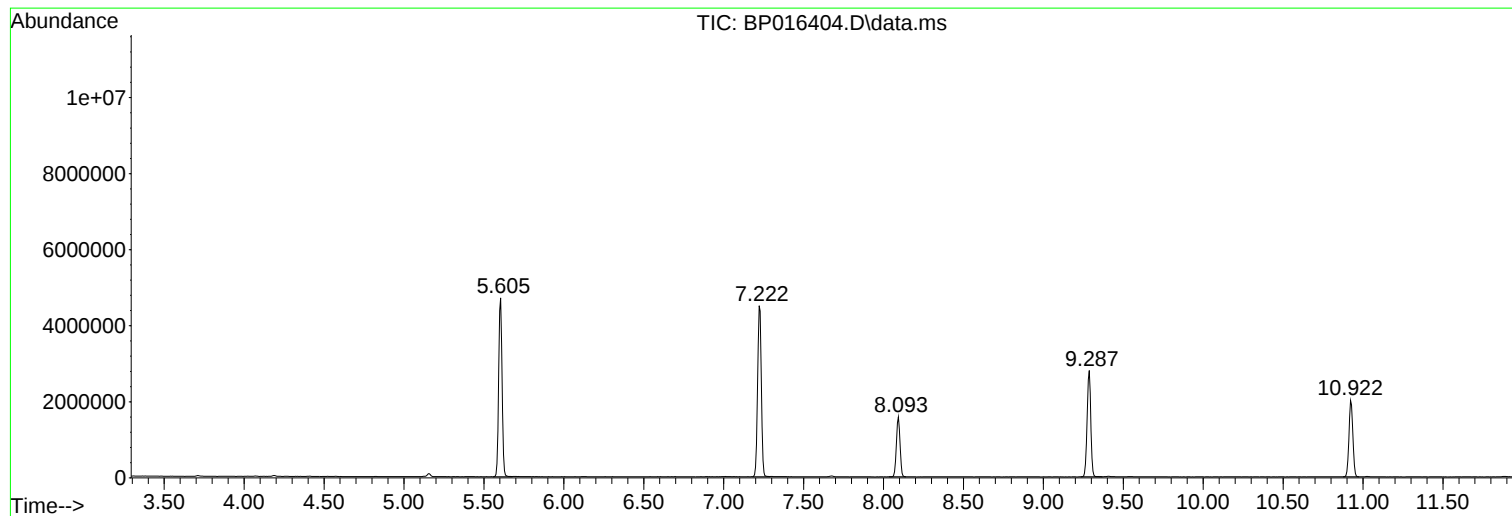

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072723\
Data File : BP016404.D
Acq On : 27 Jul 2023 17:21
Operator : MA/JU
Sample : 03706-08
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
B-P21B

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072723\
Data File : BP016404.D
Acq On : 27 Jul 2023 17:21
Operator : MA/JU
Sample : 03706-08
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
B-P21B

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------