

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072723\
 Data File : BP016408.D
 Acq On : 27 Jul 2023 19:39
 Operator : MA/JU
 Sample : 03719-06
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 B-P23B

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072723.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP016408.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.605	387	394	407	rBV	5068681	7291724	46.68%	9.349%
2	7.222	662	669	686	rBV	4759056	7612259	48.73%	9.760%
3	8.093	810	817	827	rVB	1349504	2113312	13.53%	2.710%
4	9.287	1012	1020	1031	rBV	2837798	4587628	29.37%	5.882%
5	10.922	1288	1298	1306	rBV	1716952	2911036	18.63%	3.732%
6	13.363	1702	1713	1721	rBV	7238953	10607727	67.90%	13.601%
7	14.734	1938	1946	1955	rBV	2615624	3715699	23.78%	4.764%
8	16.222	2192	2199	2222	rBV	5155567	7541853	48.28%	9.670%
9	17.498	2409	2416	2428	rVB	3195758	4556582	29.17%	5.842%
10	17.604	2428	2434	2442	rBV2	135326	190368	1.22%	0.244%
11	18.339	2554	2559	2565	rBV	235149	337362	2.16%	0.433%
12	20.039	2842	2848	2858	rBV	12896299	15622058	100.00%	20.030%
13	21.251	3050	3054	3065	rBV2	364180	660454	4.23%	0.847%
14	21.586	3105	3111	3120	rBV	3754153	4995769	31.98%	6.405%
15	24.180	3544	3552	3566	rVB	2451249	5248960	33.60%	6.730%




Sum of corrected areas: 77992791

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072723\
Data File : BP016408.D
Acq On : 27 Jul 2023 19:39
Operator : MA/JU
Sample : 03719-06
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
B-P23B

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

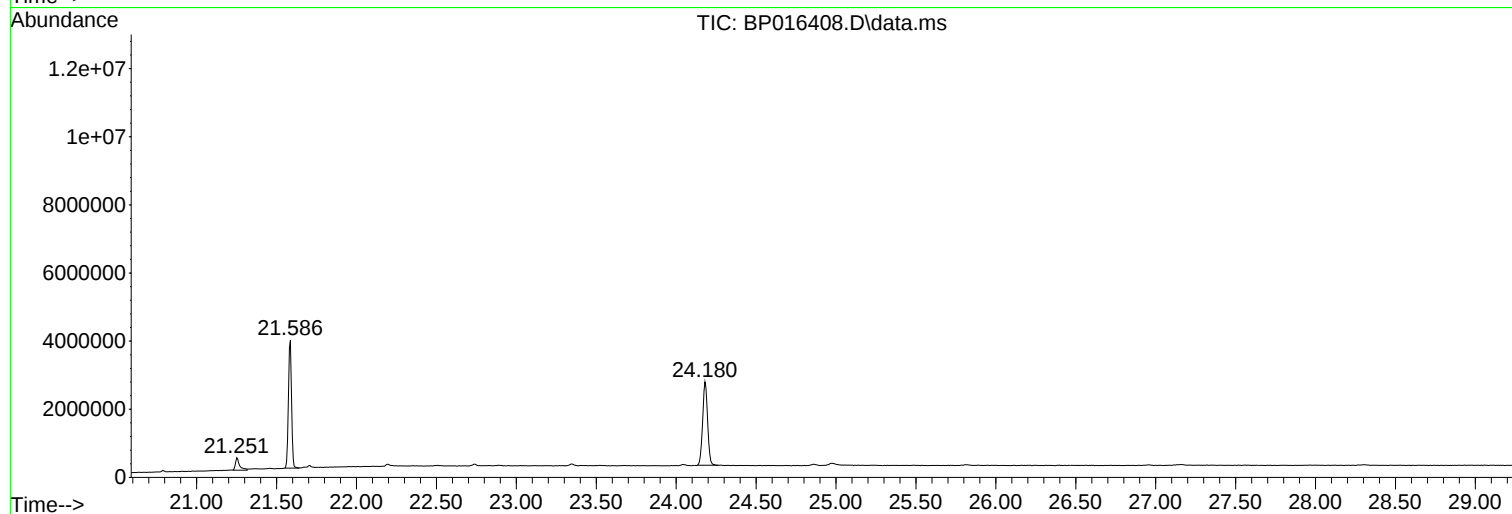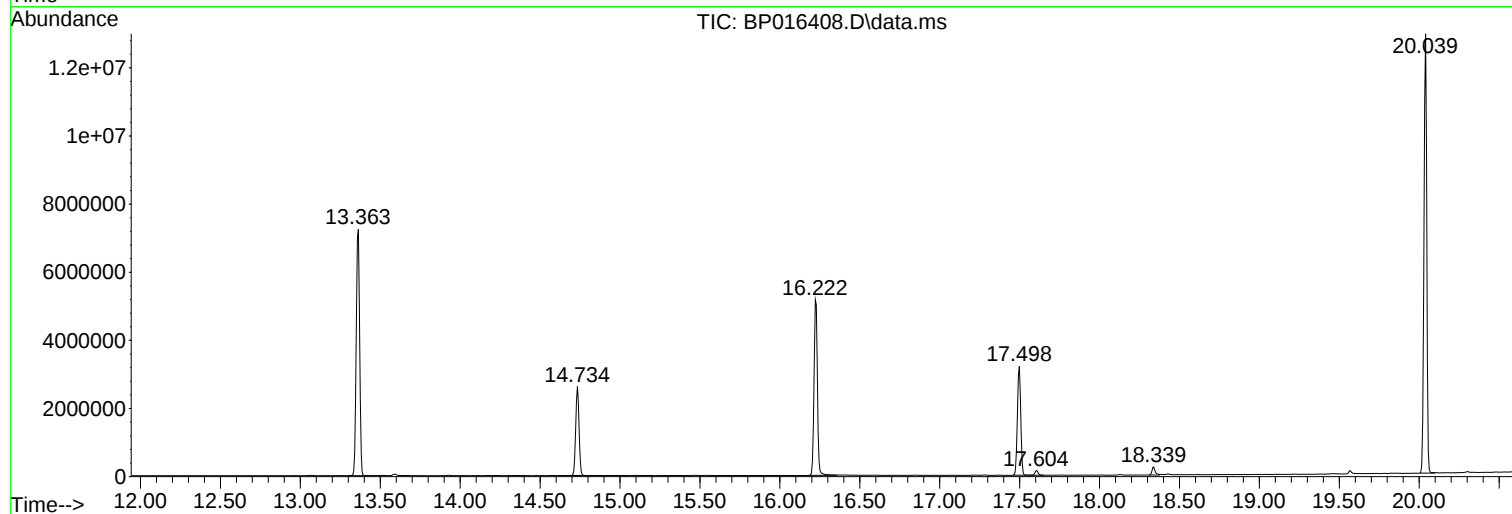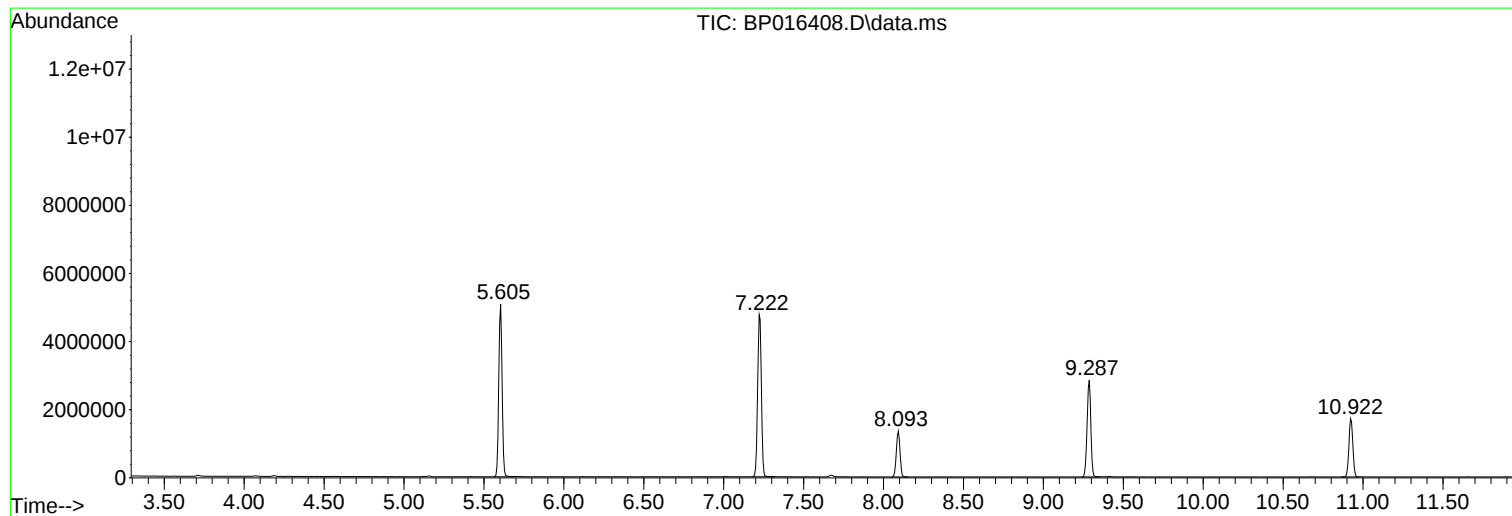

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072723\
Data File : BP016408.D
Acq On : 27 Jul 2023 19:39
Operator : MA/JU
Sample : 03719-06
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
B-P23B










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Cyclotetracosane Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
21.251	2.64 ng	660454	Chrysene-d12	21.586

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Cyclotetracosane	336	C24H48	000297-03-0	97
2			Ethanol, 2-(tetradecyloxy)-	258	C16H34O2	002136-70-1	93
3			Pentadecafluorooctanoic acid, oc...	666	C26H37F15O2	1000406-04-8	93
4			Nonadecyl trifluoroacetate	380	C21H39F3O2	1000351-76-3	90
5			Nonadecyl pentafluoropropionate	430	C22H39F5O2	1000351-88-8	90

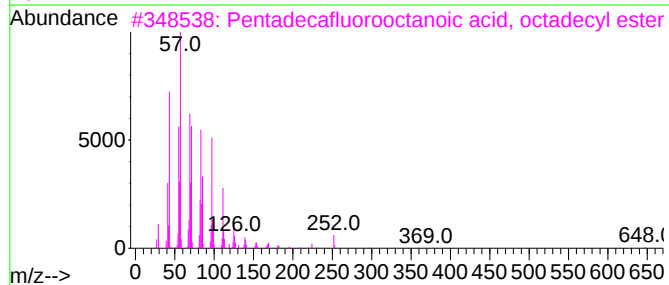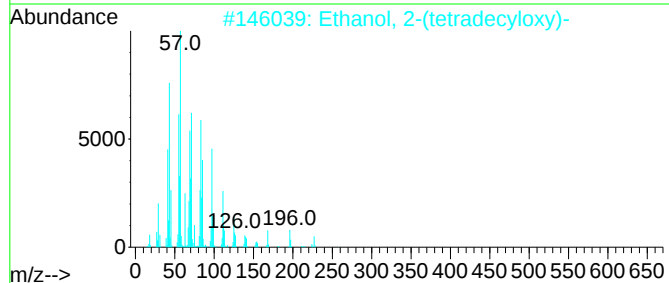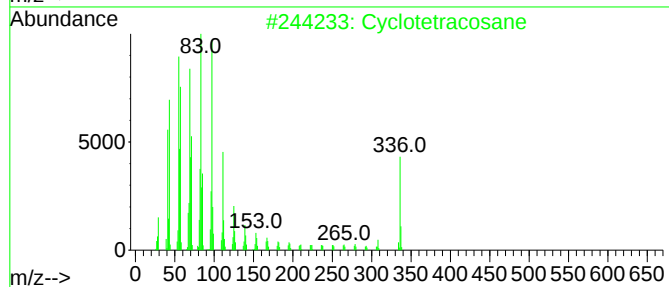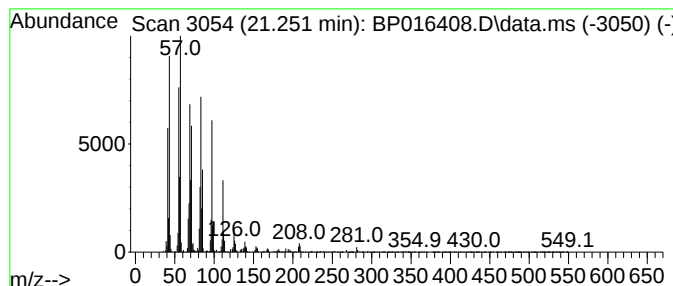

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072723\
Data File : BP016408.D
Acq On : 27 Jul 2023 19:39
Operator : MA/JU
Sample : 03719-06
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
B-P23B

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Cyclotetracosane	21.251	2.6	ng	660454	5	21.586	4995770	20.0