
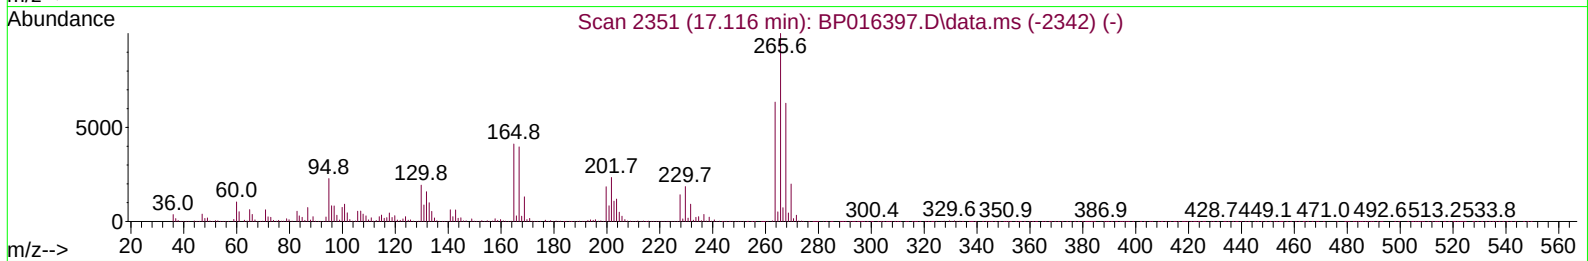
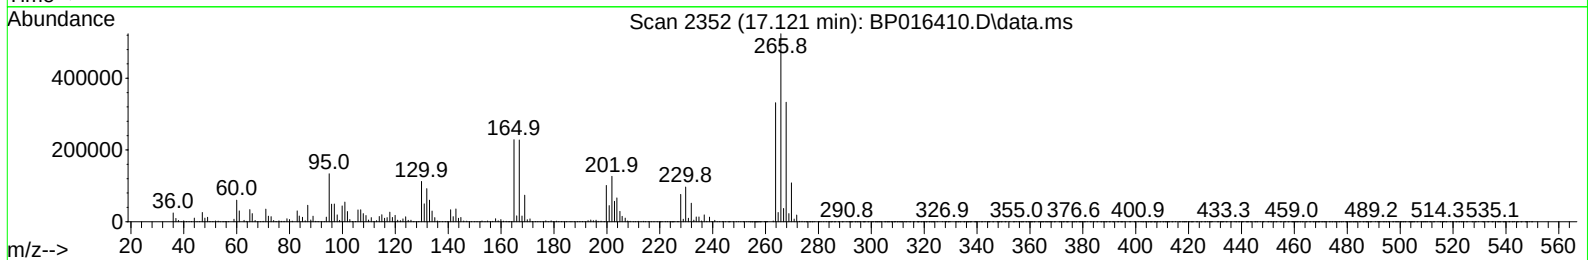


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072823\
 Data File : BP016410.D
 Acq On : 28 Jul 2023 07:30
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 29 05:07:41 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072723.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 28 01:48:25 2023
 Response via : Initial Calibration

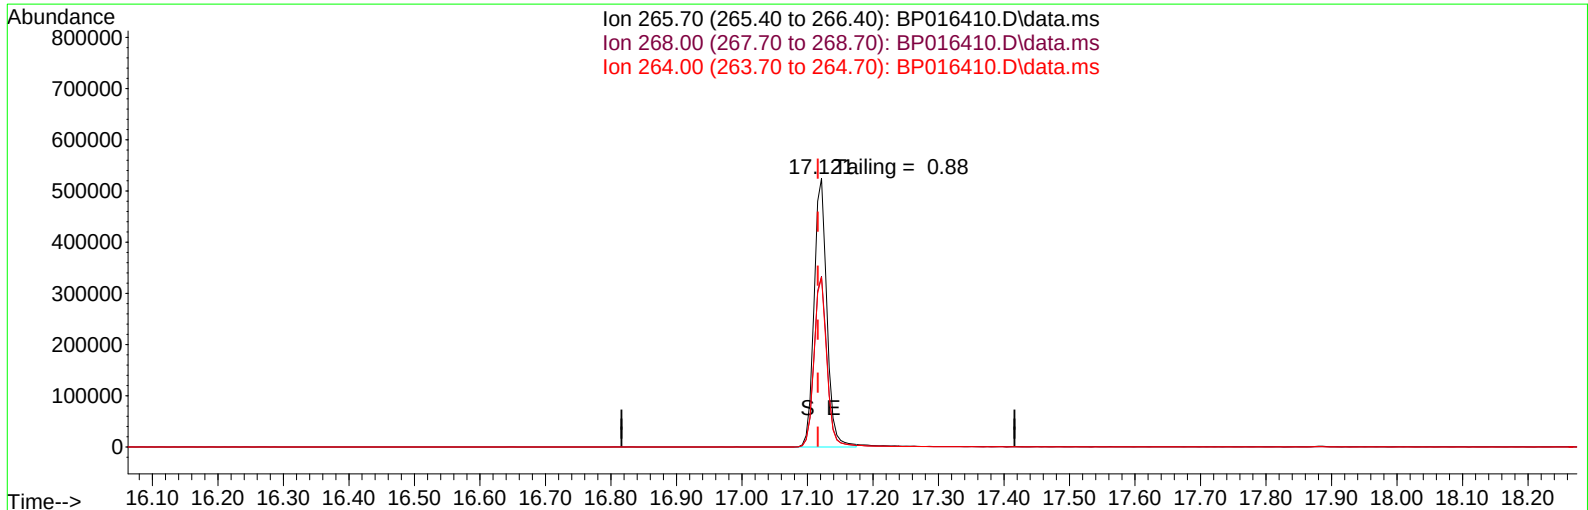

TIC: BP016410.D\data.ms

(70) Pentachlorophenol (C)




17.121min (+ 0.005) 229486.64 ng

response 725731

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	67.40	63.56
264.00	68.60	63.25
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072823\
Data File : BP016410.D
Acq On : 28 Jul 2023 07:30
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 29 05:07:41 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 28 01:48:25 2023
Response via : Initial Calibration

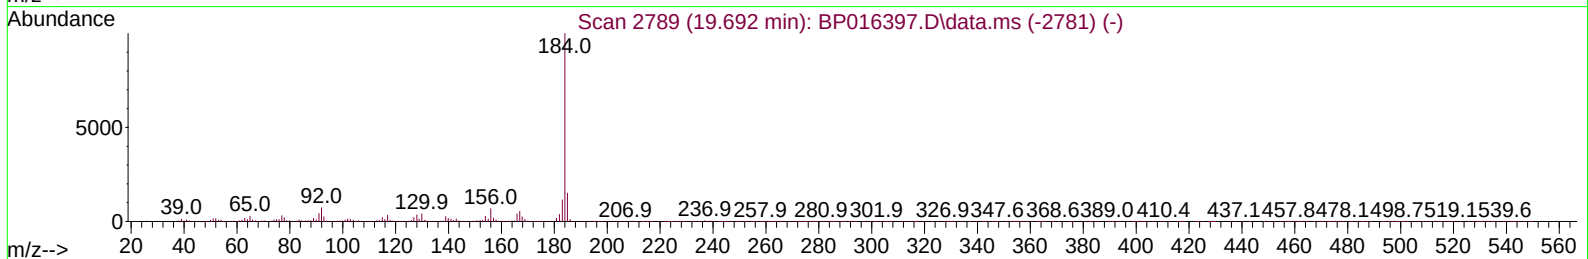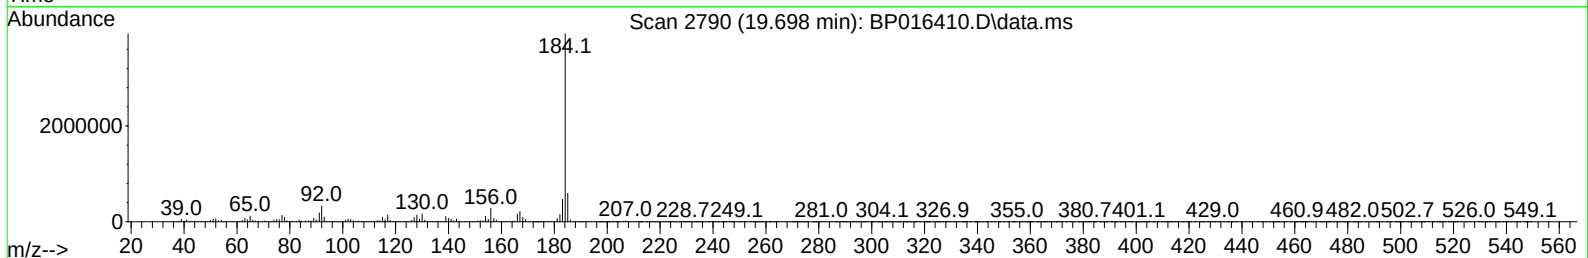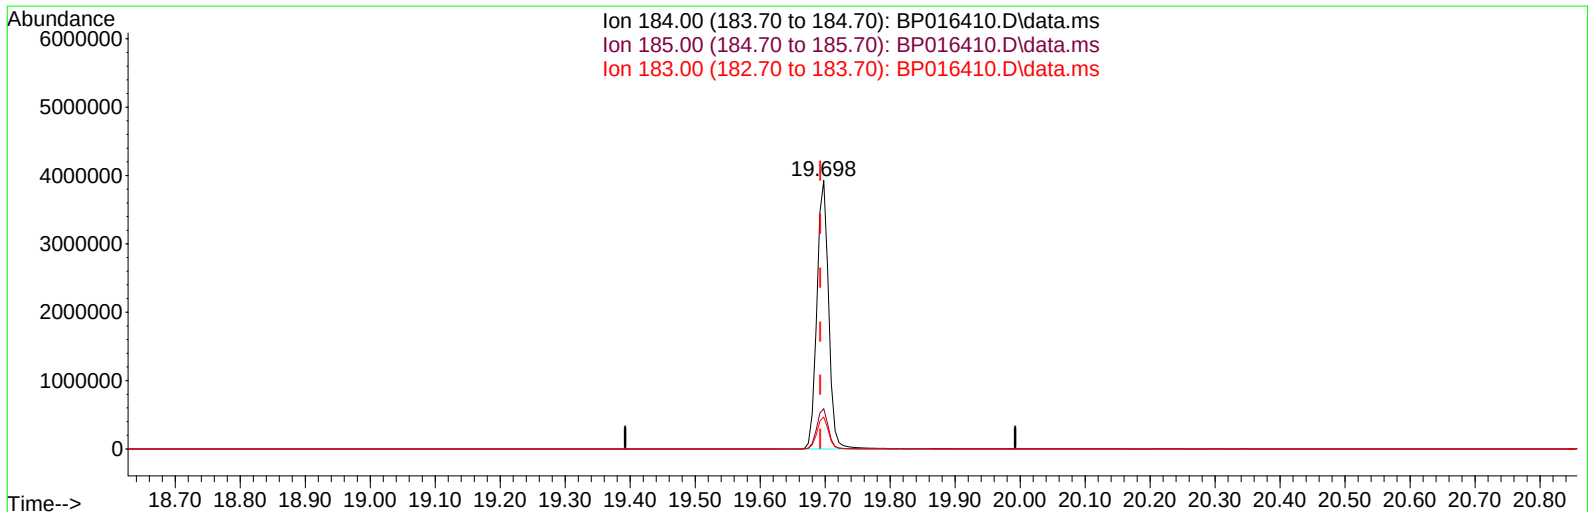

TIC: BP016410.D\data.ms

(77) Benzidine**19.698min (+ 0.005) 35107.37 ng****response 4943102**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	15.00
183.00	11.50	11.89
0.00	0.00	0.00