

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072823\
 Data File : BP016417.D
 Acq On : 28 Jul 2023 11:38
 Operator : MA/JU
 Sample : PB192316BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB154180BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072723.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP016417.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.599	384	393	406	rBV	7656479	11152326	43.72%	9.997%
2	7.222	660	669	681	rBV	7301430	11604304	45.49%	10.402%
3	8.087	806	816	823	rBV	1430321	2249081	8.82%	2.016%
4	9.281	1011	1019	1031	rBV	4428008	7272838	28.51%	6.519%
5	10.922	1288	1298	1308	rVB	1880128	3168880	12.42%	2.840%
6	13.357	1705	1712	1719	rBV	11216726	16873576	66.15%	15.125%
7	14.734	1938	1946	1954	rBV	2857721	4170186	16.35%	3.738%
8	16.222	2190	2199	2226	rBV	8167972	12203218	47.84%	10.939%
9	17.498	2409	2416	2426	rBV	3727143	5275811	20.68%	4.729%
10	20.045	2843	2849	2862	rVB	19078841	25508690	100.00%	22.865%
11	21.586	3106	3111	3119	rBV	4462220	5874743	23.03%	5.266%
12	24.186	3545	3553	3565	rBV	2926080	6207672	24.34%	5.564%




Sum of corrected areas: 111561325

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072823\
Data File : BP016417.D
Acq On : 28 Jul 2023 11:38
Operator : MA/JU
Sample : PB192316BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB154180BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

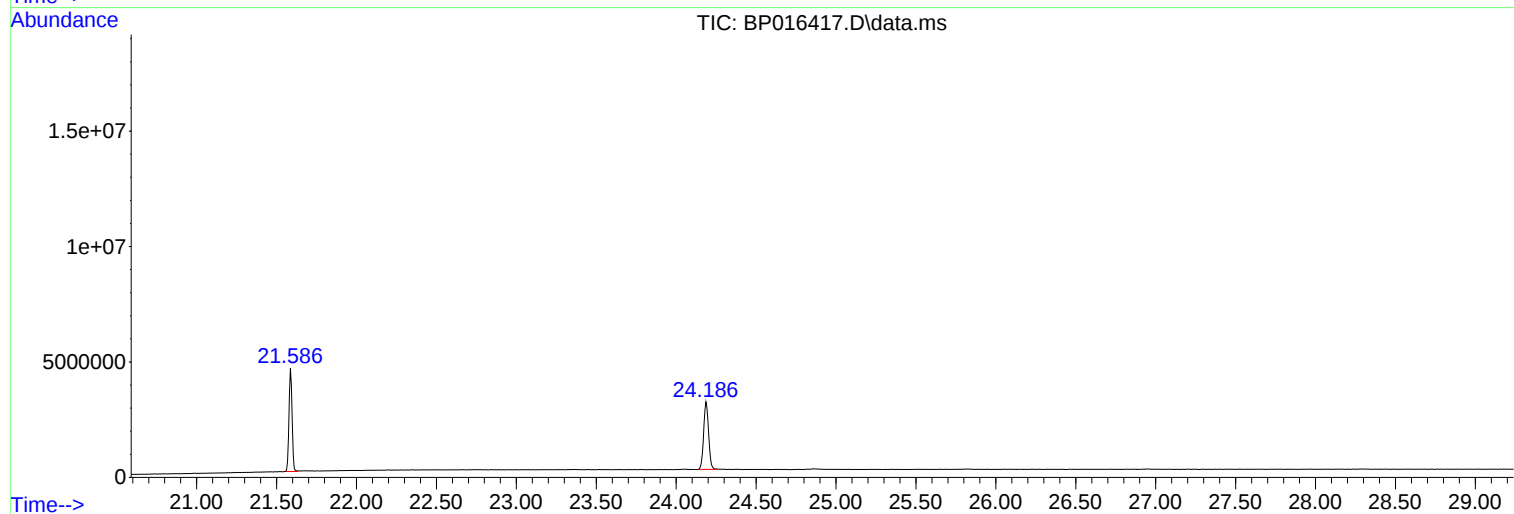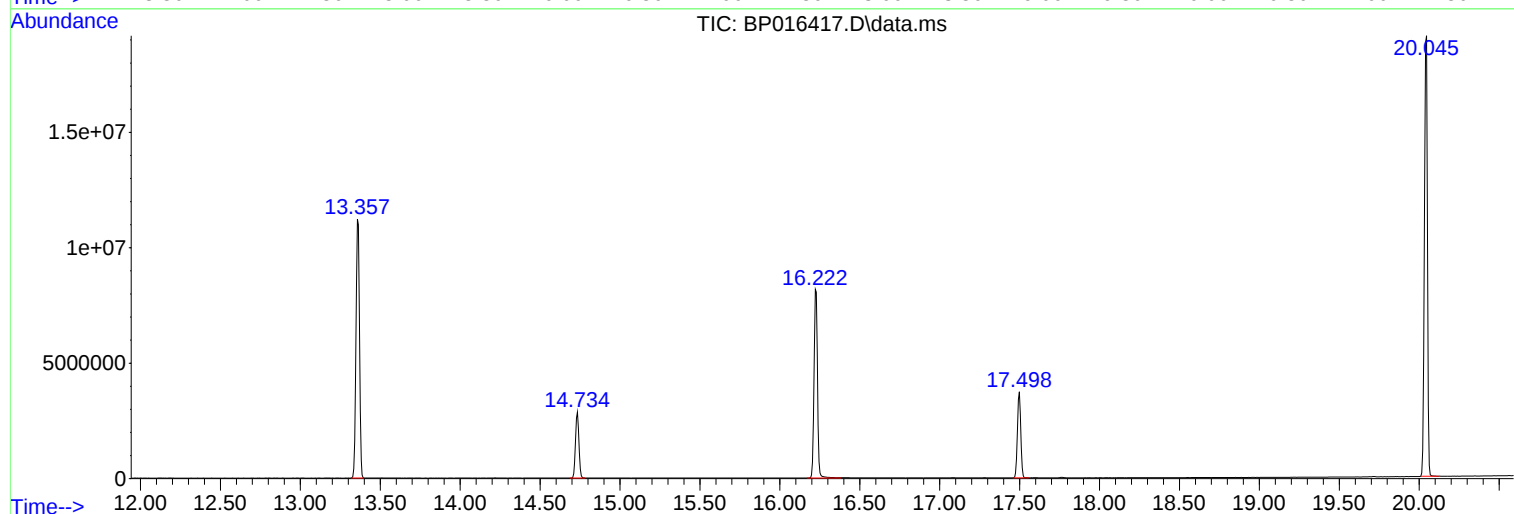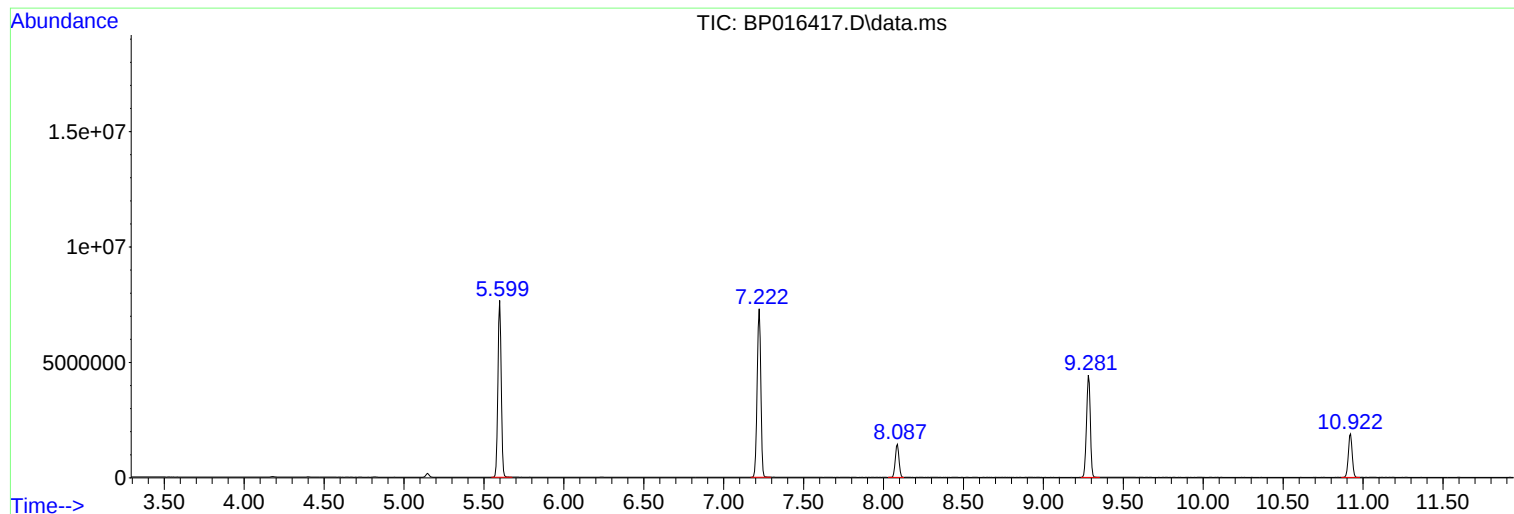

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072823\
Data File : BP016417.D
Acq On : 28 Jul 2023 11:38
Operator : MA/JU
Sample : PB192316BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB154180BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072823\
Data File : BP016417.D
Acq On : 28 Jul 2023 11:38
Operator : MA/JU
Sample : PB192316BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB154180BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------