

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072823\
Data File : BP016427.D
Acq On : 28 Jul 2023 17:23
Operator : MA/JU
Sample : PB154510BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB154510BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072723.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP016427.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.605	386	394	404	rBV	7722007	11207947	48.50%	10.588%
2	7.228	661	670	681	rBV	7230762	11676324	50.52%	11.030%
3	8.087	809	816	824	rBV	1350235	2148221	9.30%	2.029%
4	9.287	1011	1020	1030	rBV	4407990	7228353	31.28%	6.828%
5	10.922	1291	1298	1305	rBV	1870025	3064437	13.26%	2.895%
6	13.357	1705	1712	1725	rBV	11158420	16583830	71.76%	15.666%
7	14.734	1939	1946	1956	rBV	2719734	3988517	17.26%	3.768%
8	16.222	2192	2199	2219	rBV	8171297	12232572	52.93%	11.556%
9	17.498	2409	2416	2425	rBV	3475918	4937822	21.37%	4.665%
10	20.039	2842	2848	2853	rBV	18645552	23110321	100.00%	21.831%
11	21.586	3105	3111	3117	rBV	3652722	4895226	21.18%	4.624%
12	24.180	3545	3552	3569	rVB2	2238258	4784210	20.70%	4.519%




Sum of corrected areas: 105857780

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072823\
Data File : BP016427.D
Acq On : 28 Jul 2023 17:23
Operator : MA/JU
Sample : PB154510BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB154510BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

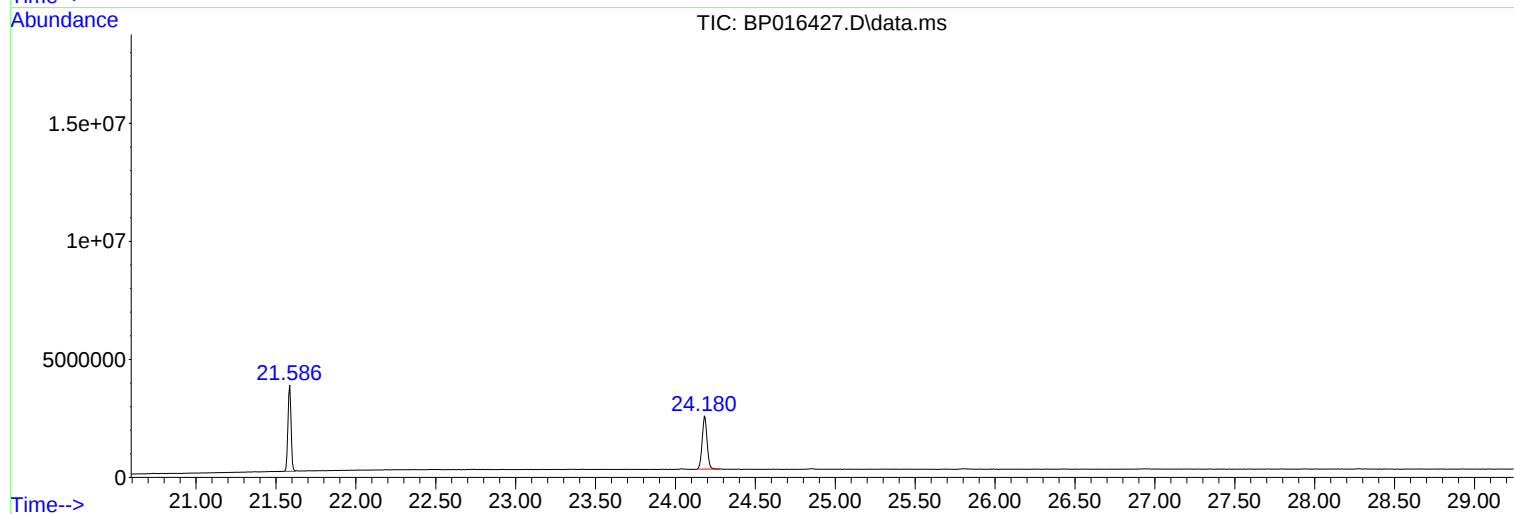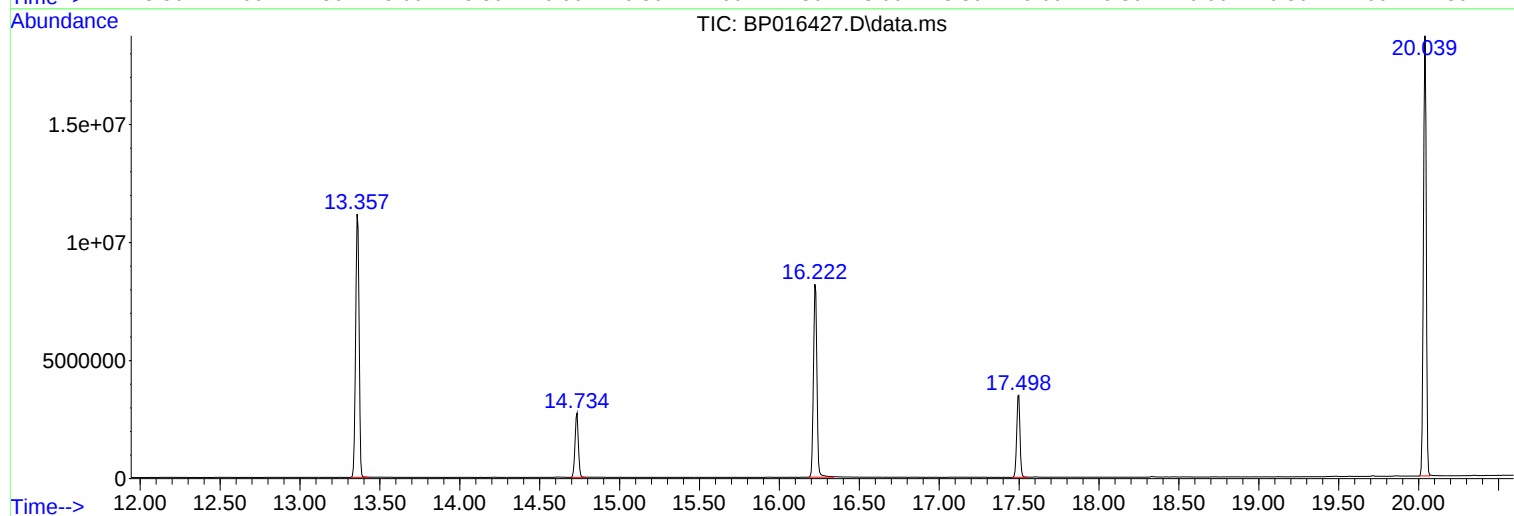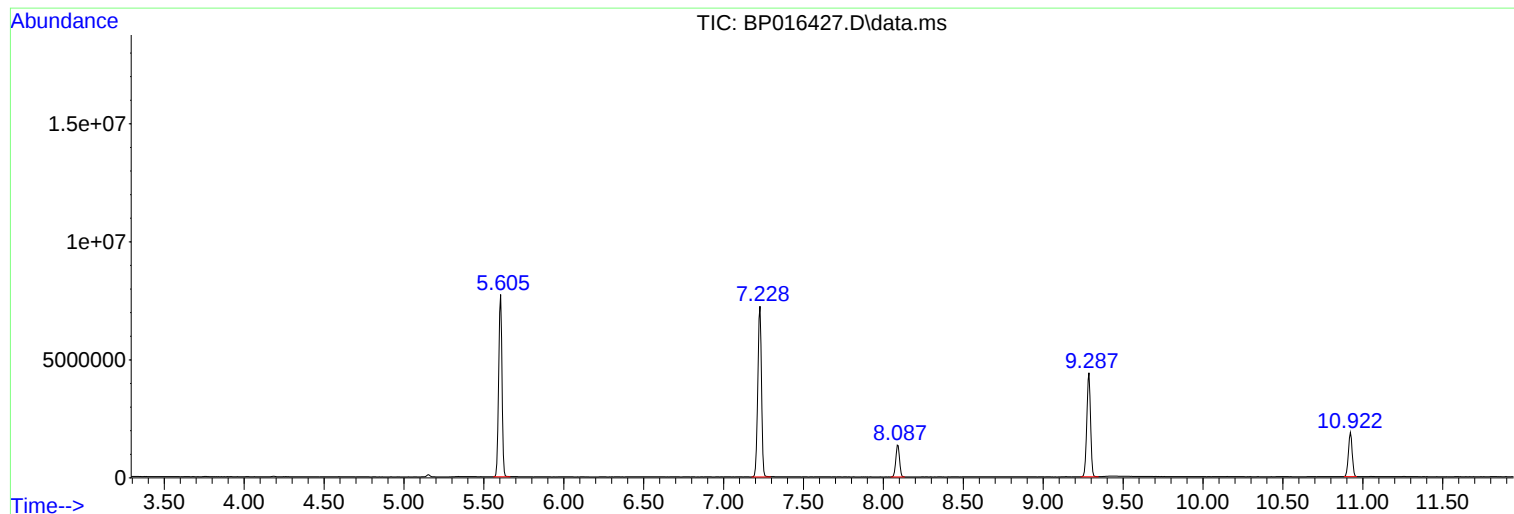

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072823\
Data File : BP016427.D
Acq On : 28 Jul 2023 17:23
Operator : MA/JU
Sample : PB154510BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB154510BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072823\
Data File : BP016427.D
Acq On : 28 Jul 2023 17:23
Operator : MA/JU
Sample : PB154510BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB154510BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------