
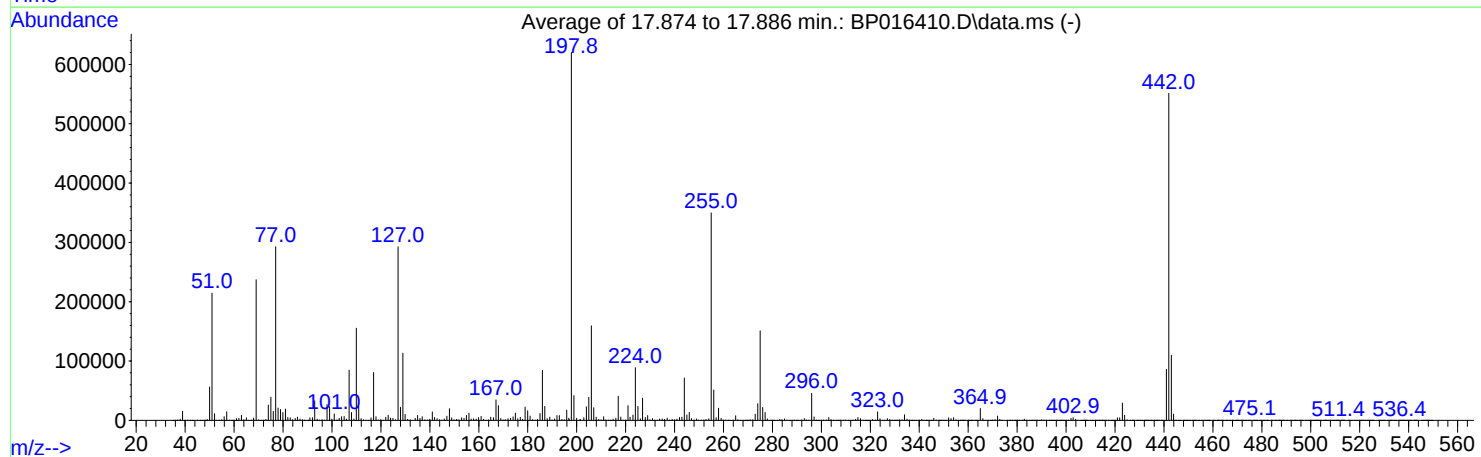


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072823\
Data File : BP016410.D
Acq On : 28 Jul 2023 07:30
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072723.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Jul 28 01:48:25 2023

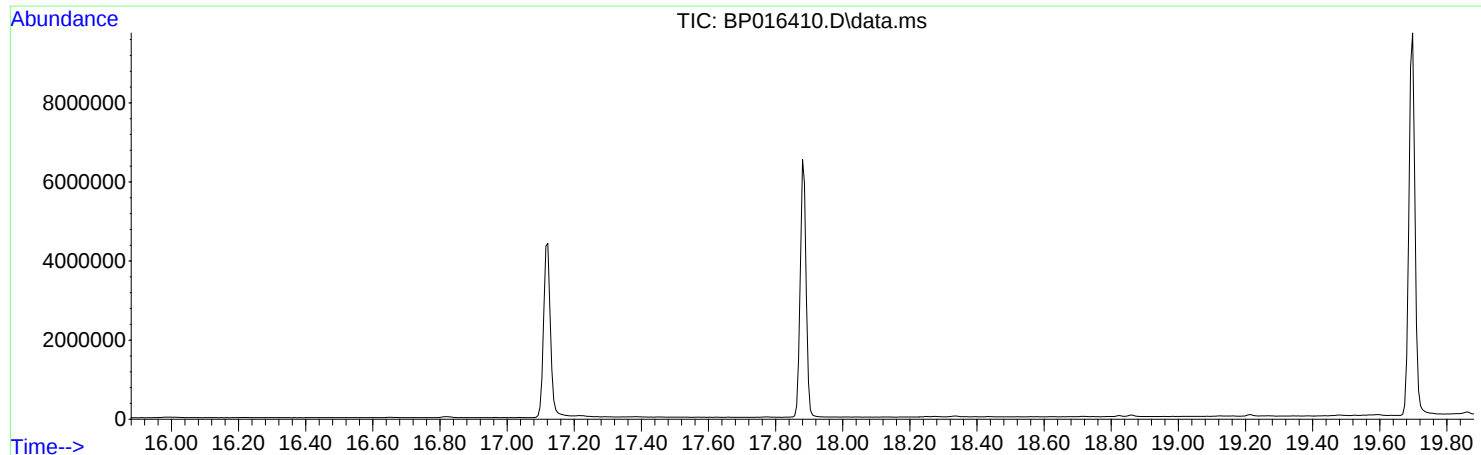




AutoFind: Scans 2480, 2481, 2482; Background Corrected with Scan 2467

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.6	214512	PASS
68	69	0.00	2	1.6	3909	PASS
69	198	0.00	100	38.2	237067	PASS
70	69	0.00	2	0.5	1179	PASS
127	198	10	80	47.2	292596	PASS
197	198	0.00	2	0.6	3496	PASS
198	198	100	100	100.0	620143	PASS
199	198	5	9	6.7	41813	PASS
275	198	10	60	24.4	151165	PASS
365	198	1	100	3.2	19862	PASS
441	198	0.01	100	13.9	85952	PASS
442	442	100	100	100.0	551251	PASS
443	442	15	24	19.9	109755	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072823\
 Data File : BP016410.D
 Acq On : 28 Jul 2023 07:30
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Jul 29 05:07:41 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072723.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 28 01:48:25 2023
 Response via : Initial Calibration

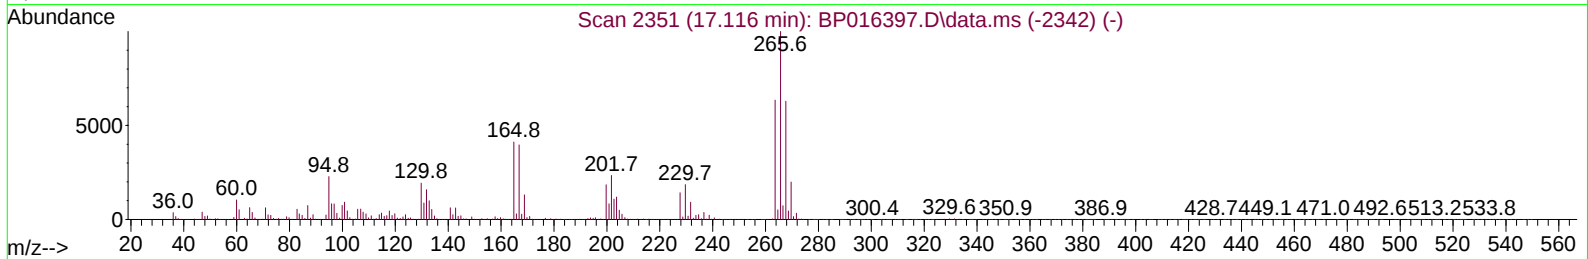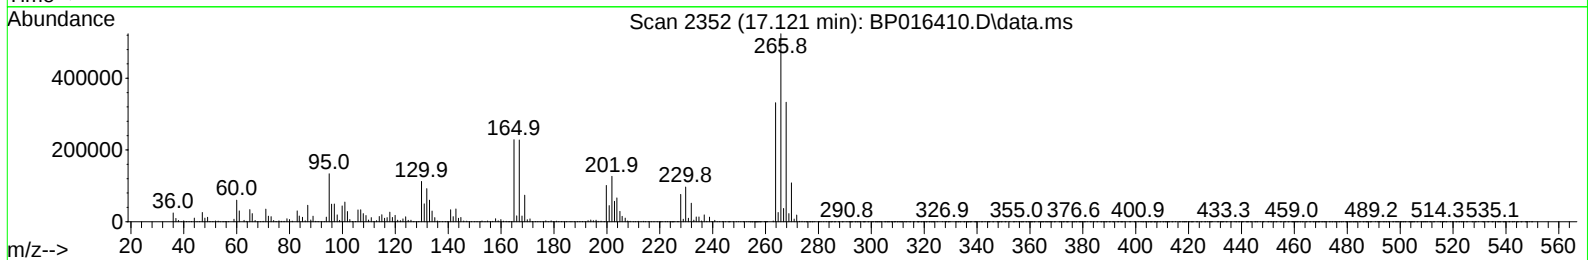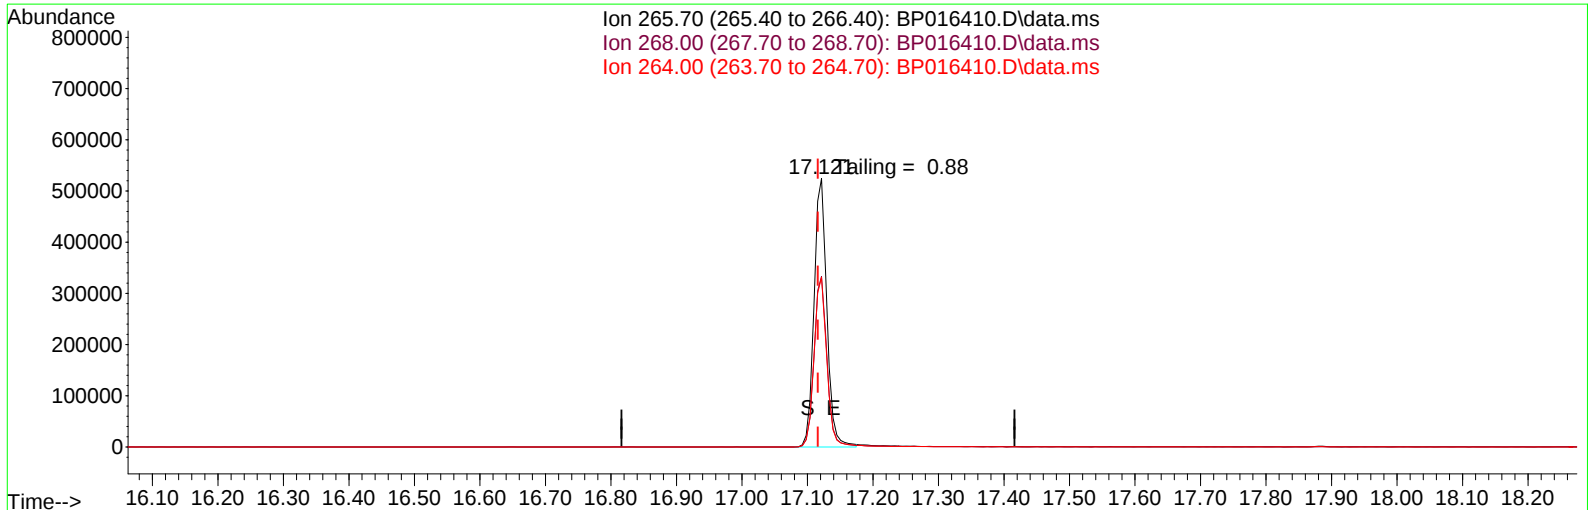

TIC: BP016410.D\data.ms

(70) Pentachlorophenol (C)

17.121min (+ 0.005) 229486.64 ng




response 725731

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	67.40	63.56
264.00	68.60	63.25
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072823\
Data File : BP016410.D
Acq On : 28 Jul 2023 07:30
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Jul 29 05:07:41 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 28 01:48:25 2023
Response via : Initial Calibration

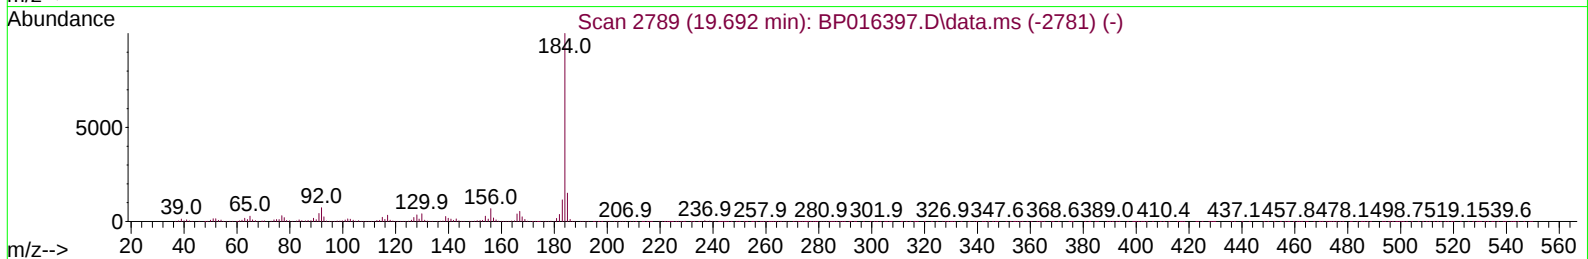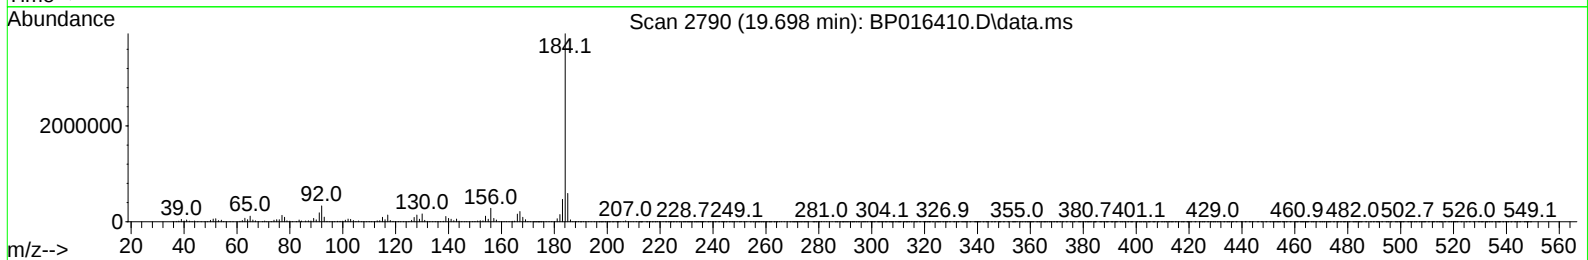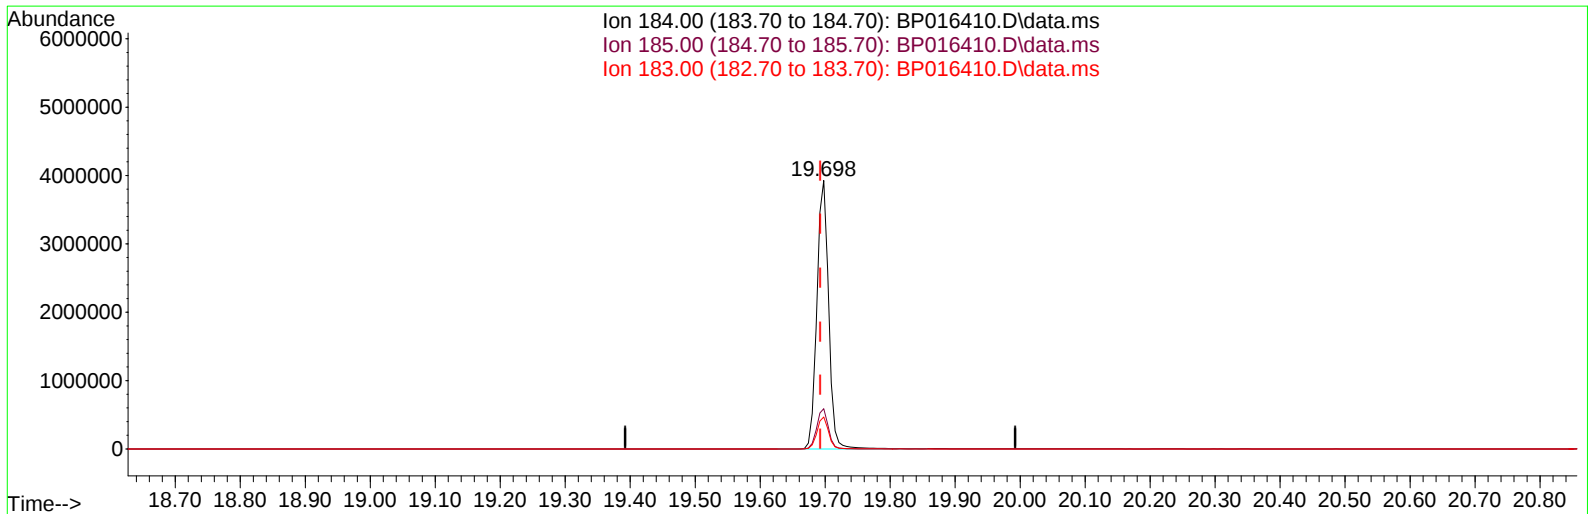

TIC: BP016410.D\data.ms

(77) Benzidine

19.698min (+ 0.005) 35107.37 ng

response 4943102

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	15.00
183.00	11.50	11.89
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/28/2023	BNA_P	<u>BP016410.D</u>
Compound Name	Response	Retention Time
DDT	1955000	20.874
DDD	41977	20.439
DDE	3142	19.939
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
45119	2000119	2.26

Instrument :
BNA_P
ClientSampleId :
DFTPP