
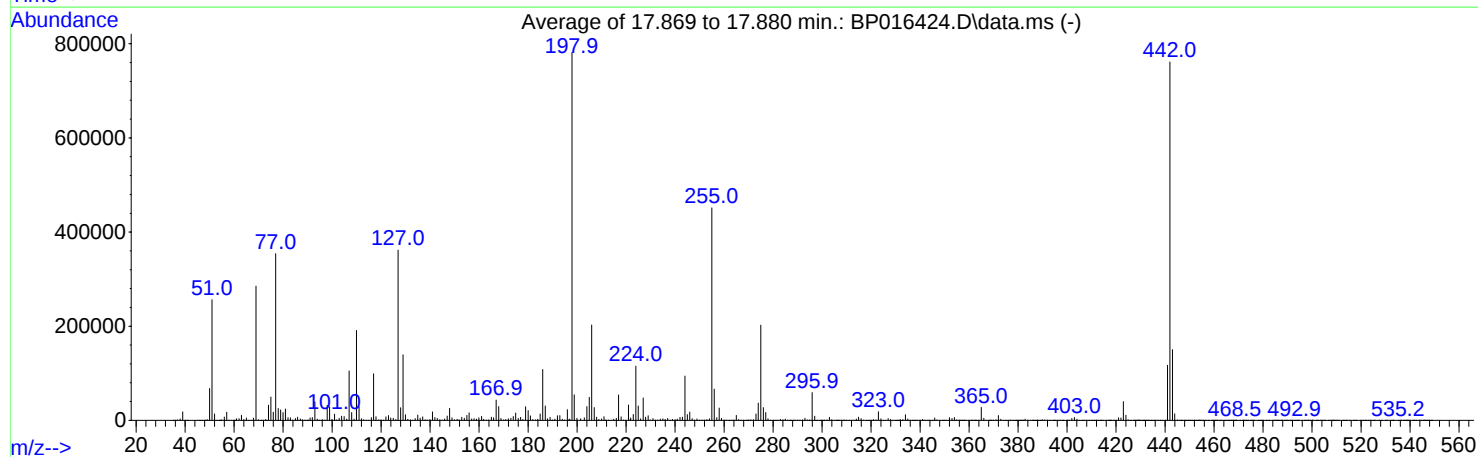


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072823\
 Data File : BP016424.D
 Acq On : 28 Jul 2023 15:39
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072723.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jul 28 01:48:25 2023

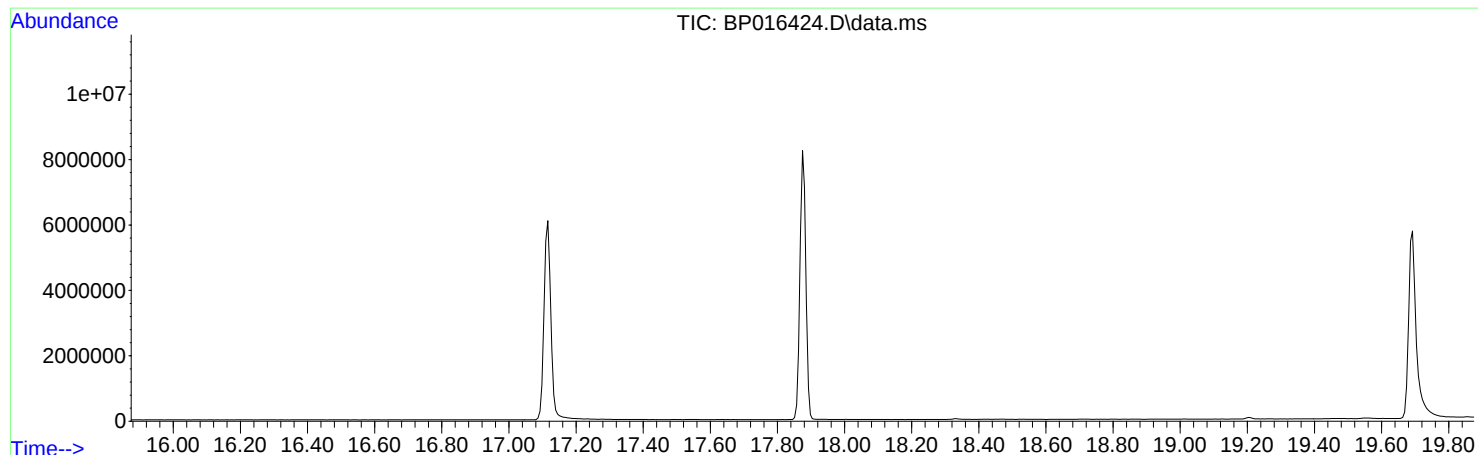




AutoFind: Scans 2479, 2480, 2481; Background Corrected with Scan 2468

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.8	256141	PASS
68	69	0.00	2	1.6	4673	PASS
69	198	0.00	100	36.5	285229	PASS
70	69	0.00	2	0.5	1374	PASS
127	198	10	80	46.3	361608	PASS
197	198	0.00	2	0.3	2730	PASS
198	198	100	100	100.0	781467	PASS
199	198	5	9	7.0	54540	PASS
275	198	10	60	25.9	202261	PASS
365	198	1	100	3.5	27514	PASS
441	198	0.01	100	15.0	117111	PASS
442	442	100	100	100.0	761216	PASS
443	442	15	24	19.7	150128	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072823\
Data File : BP016424.D
Acq On : 28 Jul 2023 15:39
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Jul 29 05:14:31 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 28 01:48:25 2023
Response via : Initial Calibration

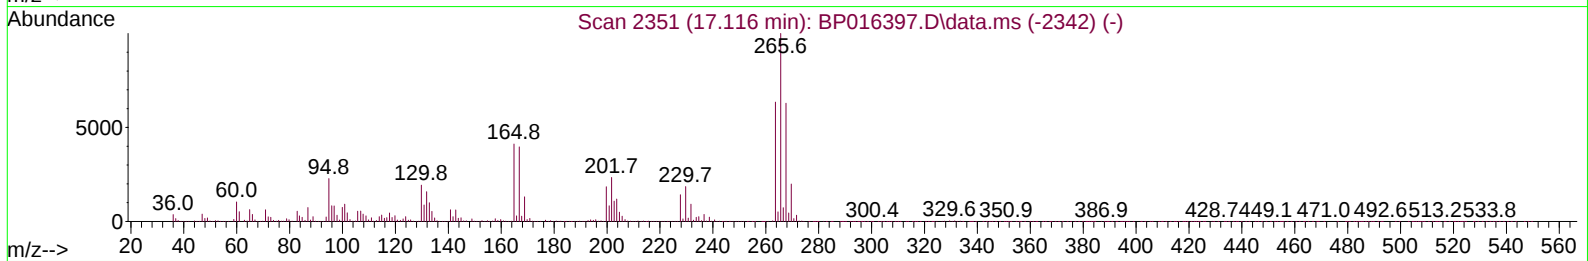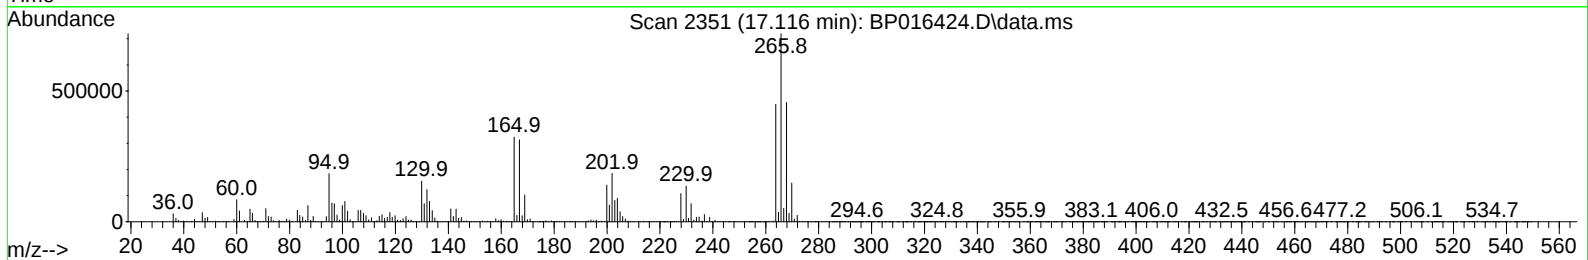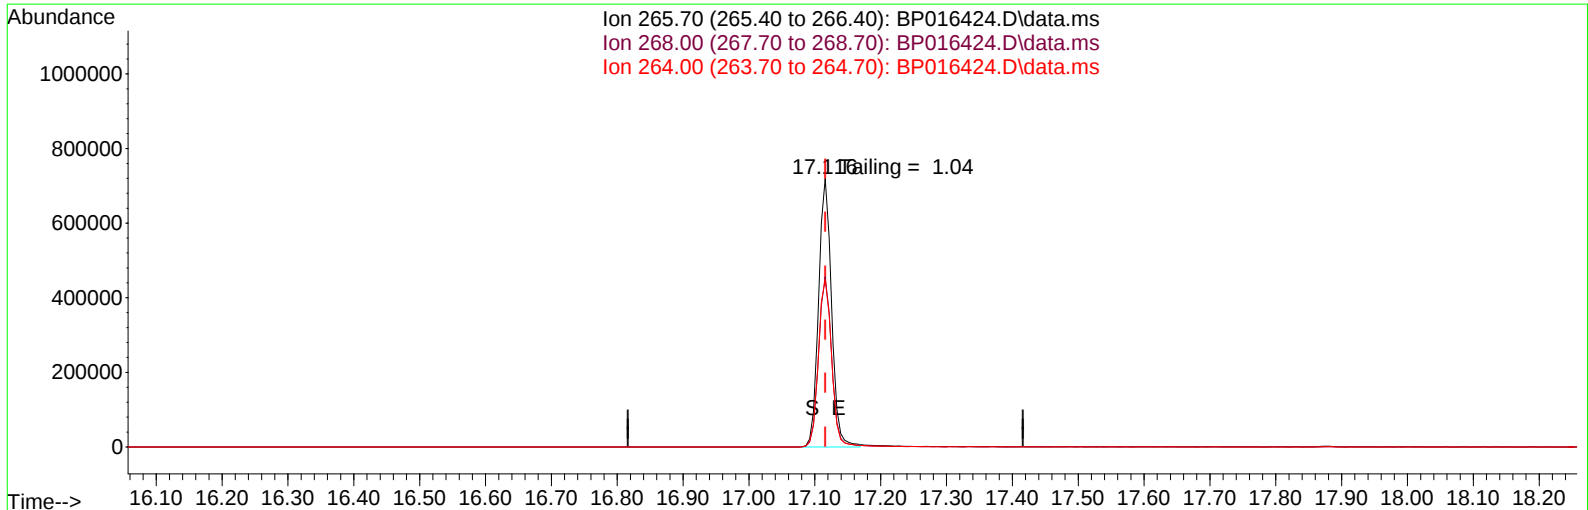

TIC: BP016424.D\data.ms

(70) Pentachlorophenol (C)

17.116min (-0.000) 445195.79 ng




response 996802

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	67.40	63.34
264.00	68.60	62.33
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072823\
Data File : BP016424.D
Acq On : 28 Jul 2023 15:39
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Jul 29 05:14:31 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 28 01:48:25 2023
Response via : Initial Calibration

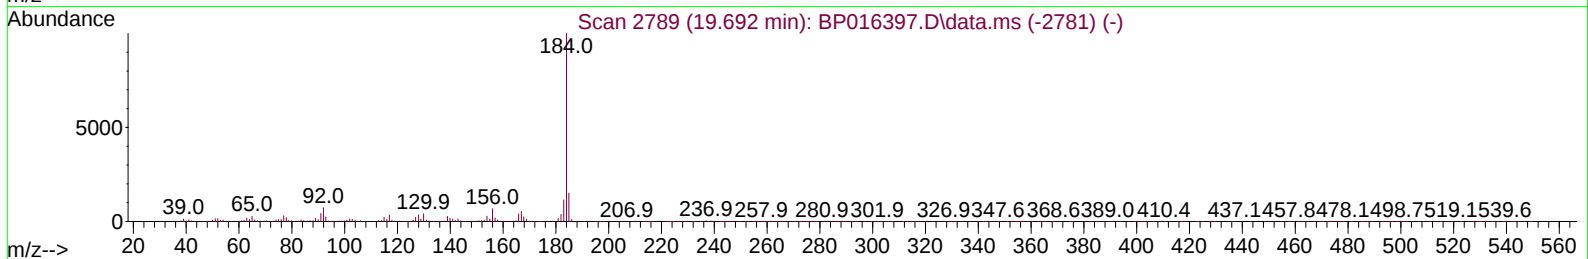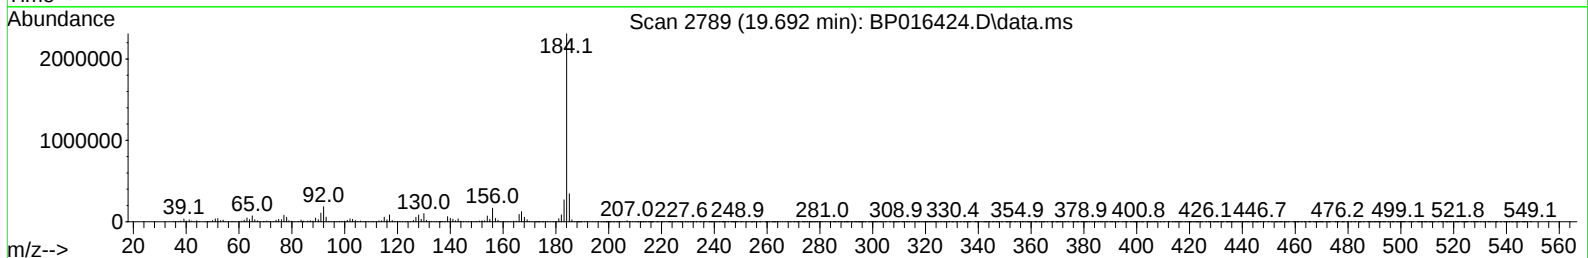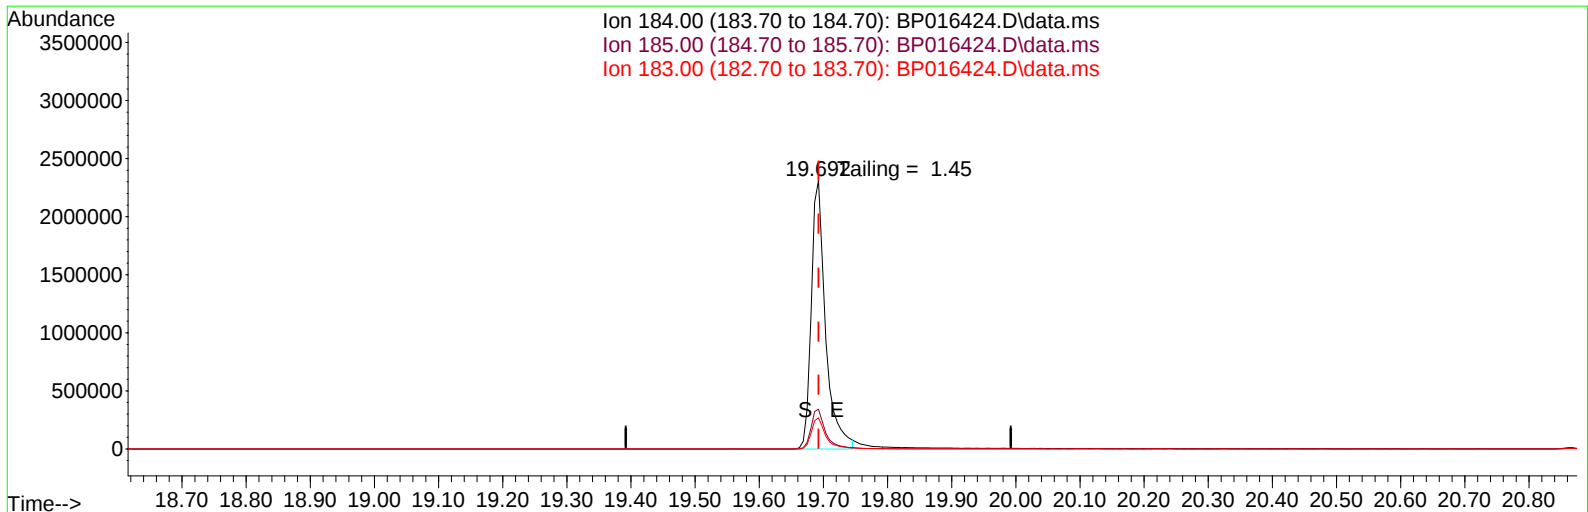

TIC: BP016424.D\data.ms

(77) Benzidine

19.692min (-0.000) 1456011.28 ng

response 3710854

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	14.84
183.00	11.50	11.64
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/28/2023	BNA_P	<u>BP016424.D</u>
Compound Name	Response	Retention Time
DDT	2595413	20.863
DDD	5932	20.651
DDE	0	19.939
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5932	2601345	0.23

Instrument :
BNA_P
ClientSampleId :
DFTPP