

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072924\
 Data File : BM046894.D
 Acq On : 29 Jul 2024 21:37
 Operator : MA/JU
 Sample : P3329-13
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :

Quant Time: Jul 30 00:02:41 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM072424.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 24 15:10:37 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.455	152	3273	0.400	ng/ul	-0.02
4) Naphthalene-d8	10.210	136	10270	0.400	ng/ul	-0.02
9) Acenaphthene-d10	14.104	164	6707	0.400	ng/ul	-0.01
13) Phenanthrene-d10	0.000	188	0	0.000	ng/ul	-16.87
17) Chrysene-d12	21.078	240	7327	0.400	ng/ul	0.00
23) Perylene-d12	23.206	264	8040	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.084	96	8811	3.845	ng/ul	-0.02
6) 2-Methylnaphthalene-d10	11.816	152	4592	0.281	ng/ul	-0.01
18) Fluoranthene-d10	18.904	212	8228	0.345	ng/ul	0.00
Target Compounds						
					Qvalue	
5) Naphthalene	10.260	128	851	0.033	ng/ul#	76
10) Acenaphthylene	13.817	152	953	0.031	ng/ul#	74
19) Fluoranthene	18.937	202	6767	0.210	ng/ul#	97
20) Pyrene	19.299	202	11050	0.332	ng/ul#	96
21) Benzo(a)anthracene	21.061	228	3799	0.124	ng/ul#	90
22) Chrysene	21.113	228	5142	0.166	ng/ul#	92
24) Benzo(b)fluoranthene	22.577	252	11102	0.315	ng/ul#	79
25) Benzo(k)fluoranthene	22.577	252	11102	0.312	ng/ul#	83
26) Benzo(a)pyrene	23.115	252	3345	0.132	ng/ul#	70
27) Indeno(1,2,3-cd)pyrene	25.306	276	2975	0.076	ng/ul#	69
28) Dibenzo(a,h)anthracene	25.319	278	772	0.027	ng/ul#	1
29) Benzo(g,h,i)perylene	25.950	276	2631	0.077	ng/ul#	68


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072924\
Data File : BM046894.D
Acq On : 29 Jul 2024 21:37
Operator : MA/JU
Sample : P3329-13
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :


Quant Time: Jul 30 00:02:41 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM072424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 24 15:10:37 2024
Response via : Initial Calibration

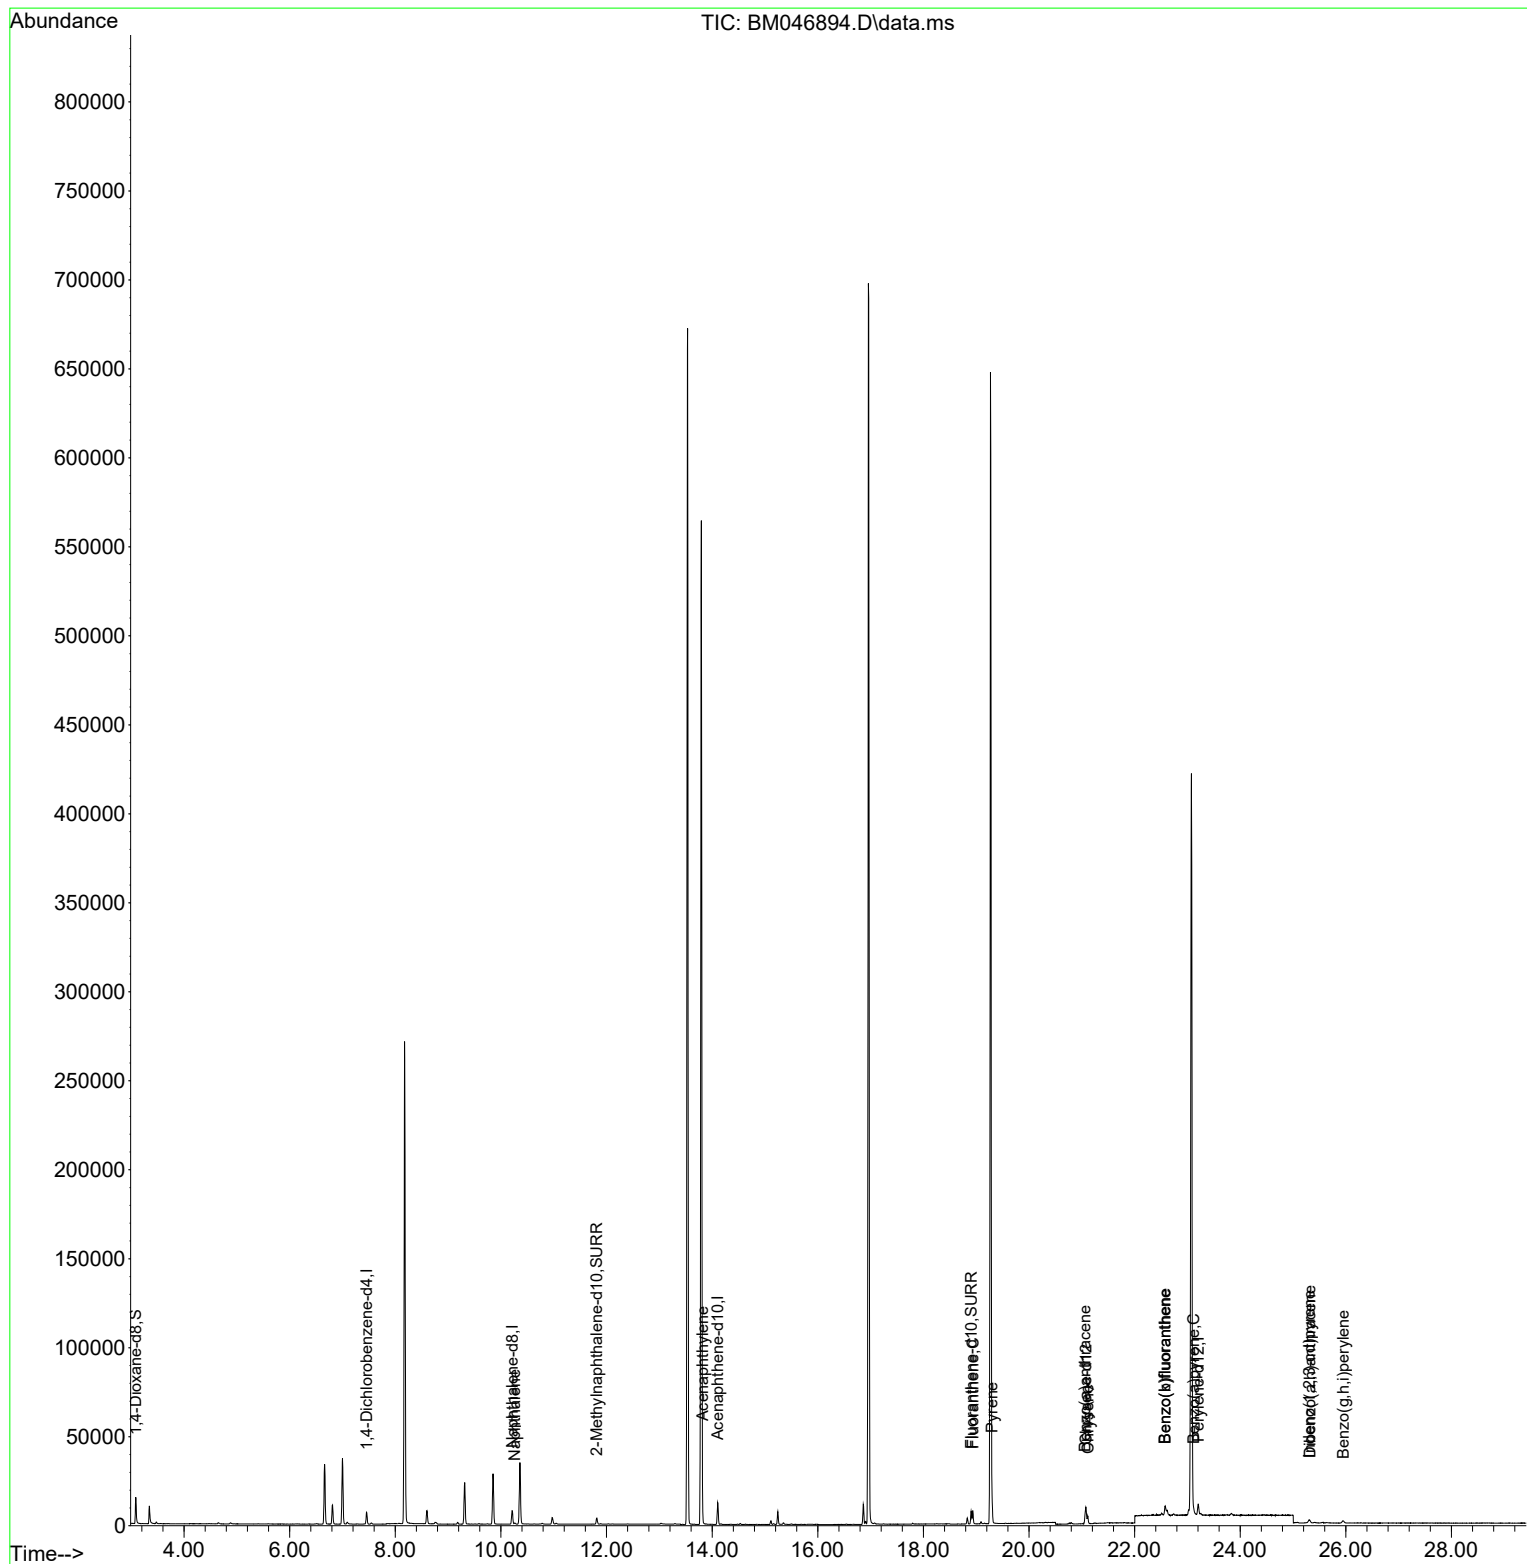



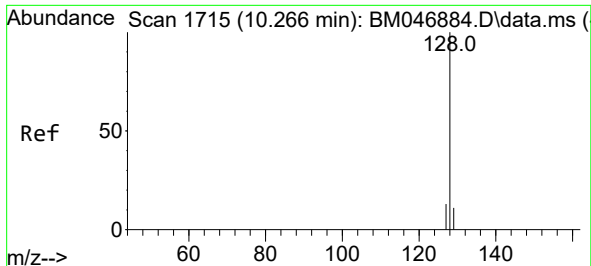


#5
Naphthalene
Concen: 0.033 ng/ul
RT: 10.260 min Scan# 1714
Delta R.T. -0.017 min
Lab File: BM046894.D
Acq: 29 Jul 2024 21:37

Instrument :
BNA_P
ClientSampleId :







Tgt Ion:128 Resp: 851
Ion Ratio Lower Upper
128 100
129 23.4 10.1 15.1#
127 22.8 11.5 17.3#

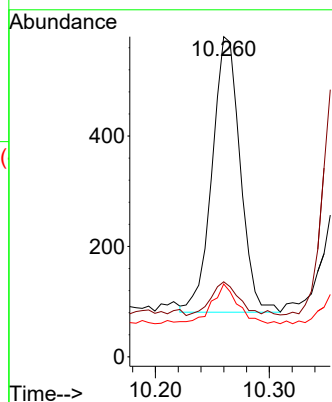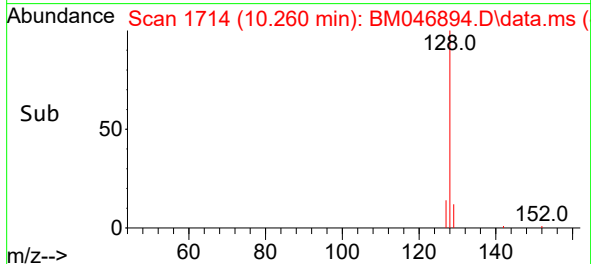

#10
Acenaphthylene
Concen: 0.031 ng/ul
RT: 13.817 min Scan# 2375
Delta R.T. -0.014 min
Lab File: BM046894.D
Acq: 29 Jul 2024 21:37

Tgt Ion:152 Resp: 953
Ion Ratio Lower Upper
152 100
151 29.6 16.8 25.2#
153 28.8 11.0 16.6#


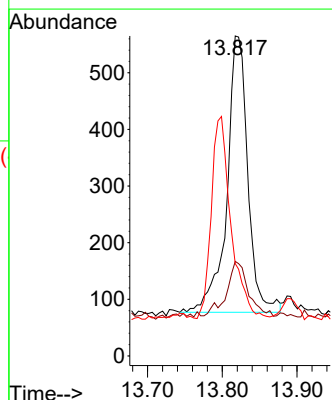
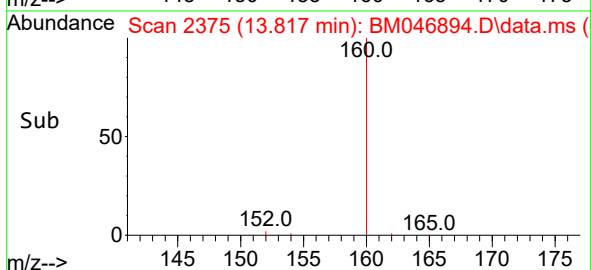
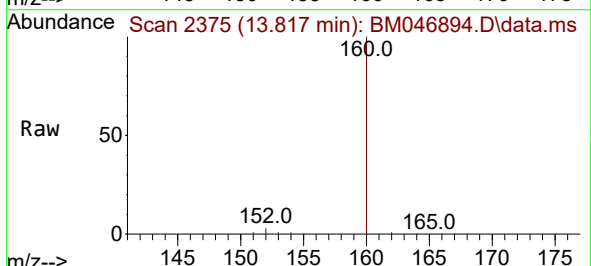


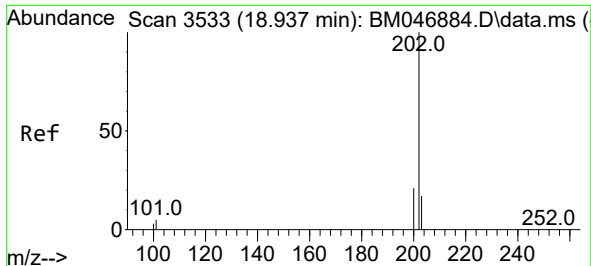

#19
Fluoranthene
Concen: 0.210 ng/ul
RT: 18.937 min Scan# 3533
Delta R.T. -0.005 min
Lab File: BM046894.D
Acq: 29 Jul 2024 21:37




Instrument :
BNA_P
ClientSampleId :


Tgt Ion:202 Resp: 6767
Ion Ratio Lower Upper
202 100
101 7.0 4.7 7.1
100 5.2 3.4 5.2#

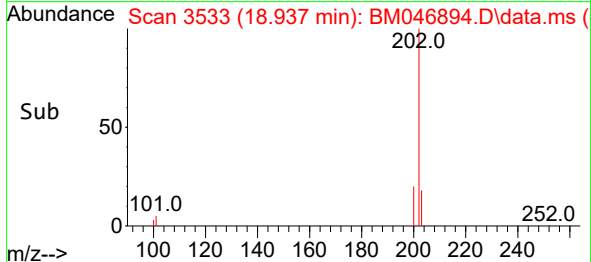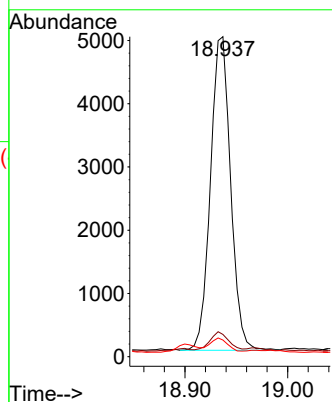

#20
Pyrene
Concen: 0.332 ng/ul
RT: 19.299 min Scan# 3611
Delta R.T. -0.005 min
Lab File: BM046894.D
Acq: 29 Jul 2024 21:37

Tgt Ion:202 Resp: 11050
Ion Ratio Lower Upper
202 100
101 7.8 5.2 7.8#
100 6.6 4.3 6.5#

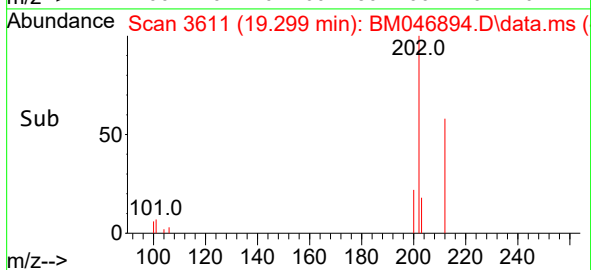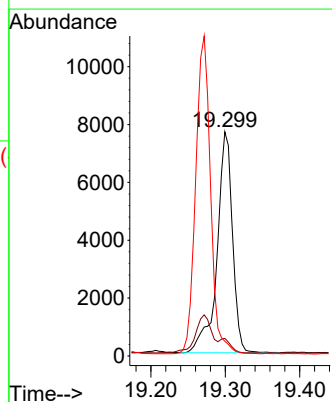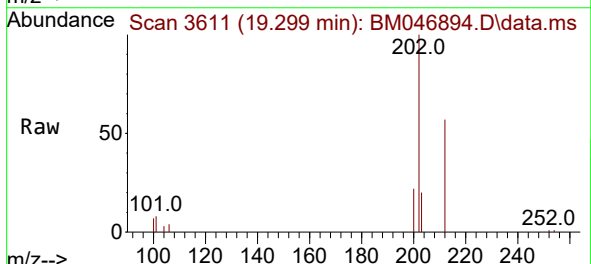



#21

Benzo(a)anthracene

Concen: 0.124 ng/ul

RT: 21.061 min Scan# 4062

Delta R.T. -0.003 min


Lab File: BM046894.D

Acq: 29 Jul 2024 21:37

Instrument :

BNA_P

ClientSampleId :






Tgt Ion:228 Resp: 3799

Ion Ratio Lower Upper

228 100

229 24.9 16.3 24.5#

226 32.9 22.3 33.5

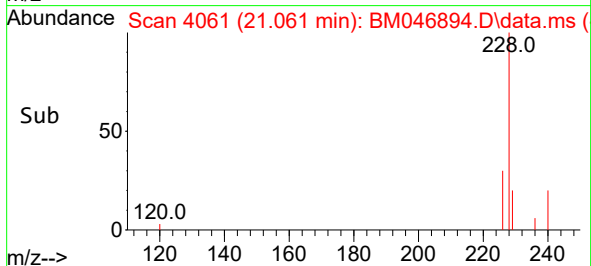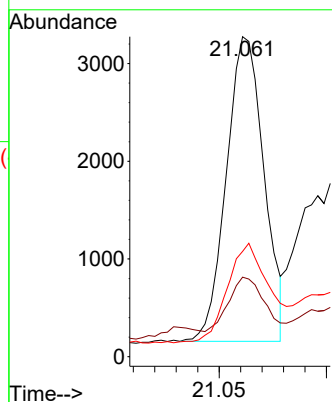

#22

Chrysene

Concen: 0.166 ng/ul

RT: 21.113 min Scan# 4079

Delta R.T. -0.003 min

Lab File: BM046894.D

Acq: 29 Jul 2024 21:37




Tgt Ion:228 Resp: 5142


Ion Ratio Lower Upper

228 100

226 34.1 24.5 36.7

229 25.5 16.2 24.2#


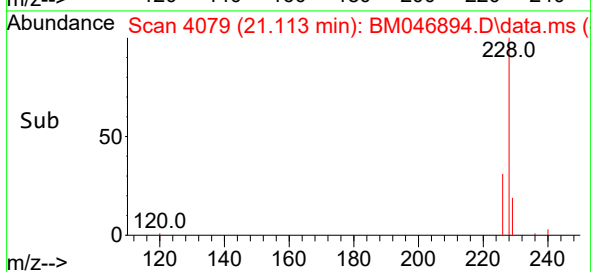
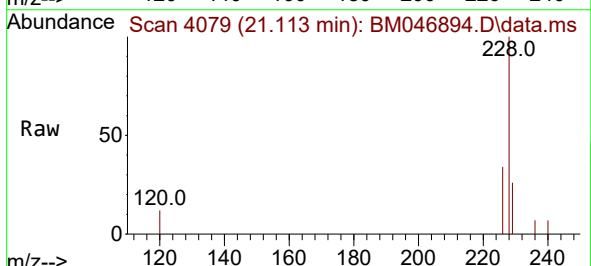
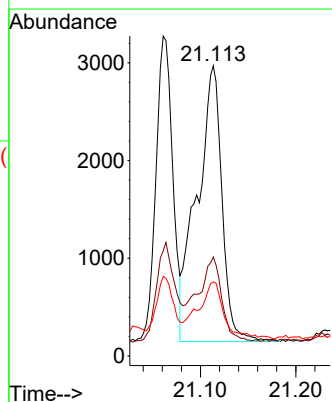




#24
Benzo(b)fluoranthene
Concen: 0.315 ng/ul
RT: 22.577 min Scan# 4580
Delta R.T. -0.003 min
Lab File: BM046894.D
Acq: 29 Jul 2024 21:37




Instrument :
BNA_P
ClientSampleId :


Tgt Ion	Ratio	Lower	Upper
252	100		
253	38.1	0.0	56.4
125	18.6	0.0	15.8#

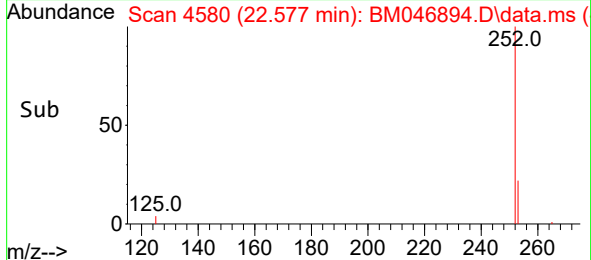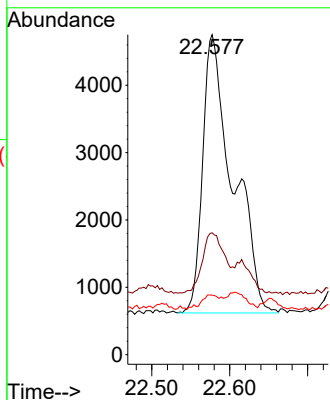

#25
Benzo(k)fluoranthene
Concen: 0.312 ng/ul
RT: 22.577 min Scan# 4580
Delta R.T. -0.044 min
Lab File: BM046894.D
Acq: 29 Jul 2024 21:37

Tgt Ion	Ratio	Lower	Upper
252	100		
253	38.1	23.5	35.3#
125	18.6	8.6	13.0#

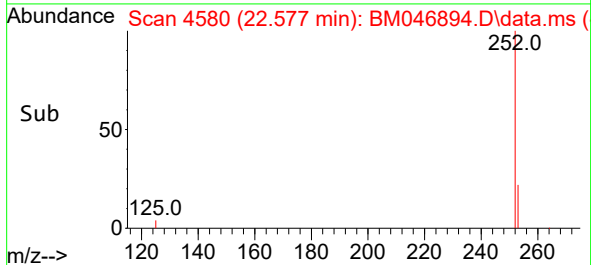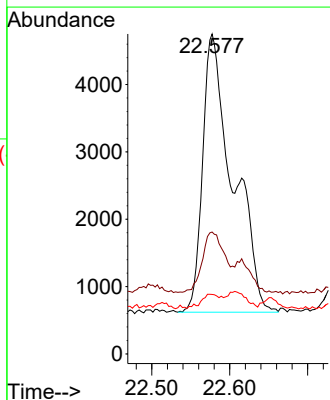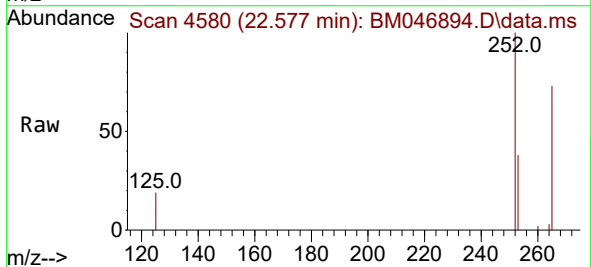

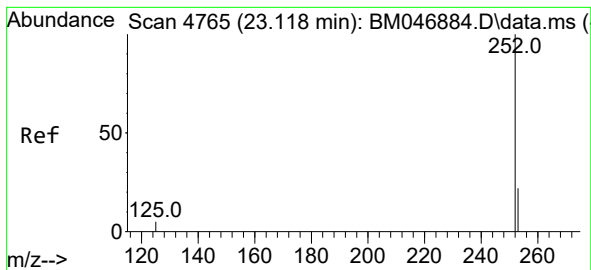

#26

Benzo(a)pyrene

Concen: 0.132 ng/ul

RT: 23.115 min Scan# 4765

Delta R.T. -0.003 min


Lab File: BM046894.D

Acq: 29 Jul 2024 21:37

Instrument :

BNA_P

ClientSampleId :

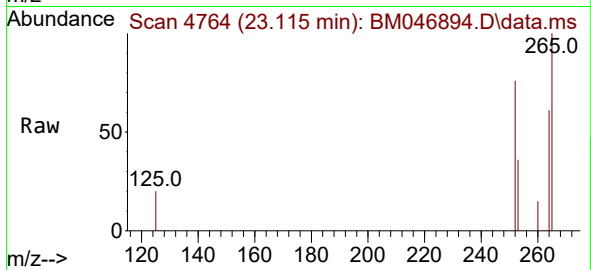




Tgt Ion:252 Resp: 3345

Ion Ratio Lower Upper

252 100

253 46.9 26.0 39.0#

125 26.1 7.8 11.8#

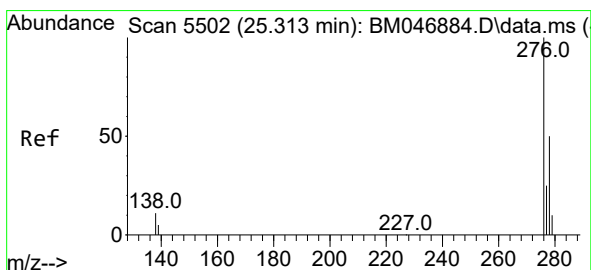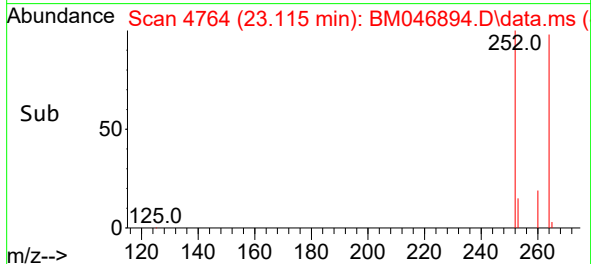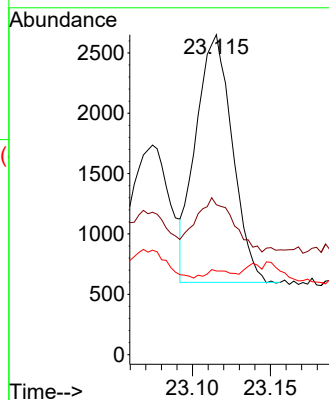

#27

Indeno(1,2,3-cd)pyrene

Concen: 0.076 ng/ul

RT: 25.306 min Scan# 5500

Delta R.T. -0.010 min

Lab File: BM046894.D

Acq: 29 Jul 2024 21:37




Tgt Ion:276 Resp: 2975


Ion Ratio Lower Upper

276 100

138 0.0 9.7 14.5#

227 0.4 0.2 0.2#

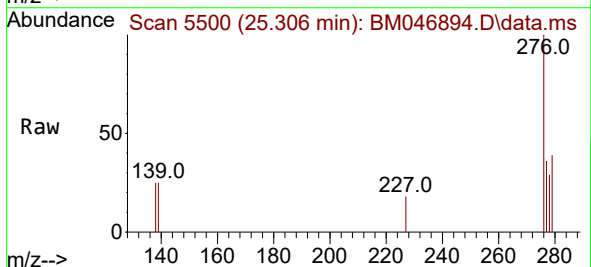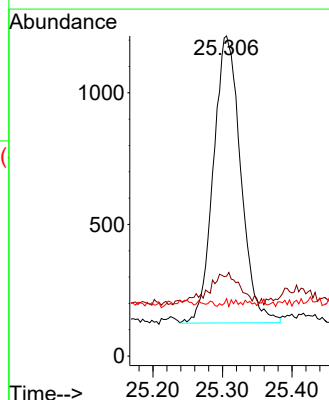

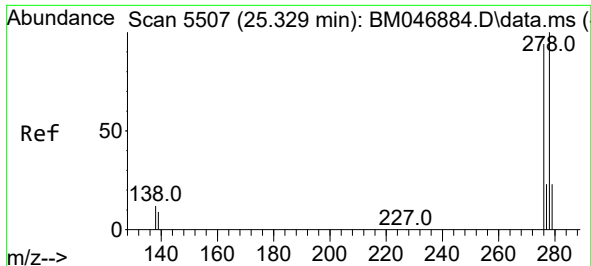

#28

Dibenzo(a,h)anthracene

Concen: 0.027 ng/ul

RT: 25.319 min Scan# 5

Delta R.T. -0.014 min


Lab File: BM046894.D

Acq: 29 Jul 2024 21:37

Instrument :

BNA_P

ClientSampleId :






Tgt Ion:278 Resp: 772

Ion Ratio Lower Upper

278 100

139 86.5 9.8 14.8#

279 136.2 25.2 37.8#

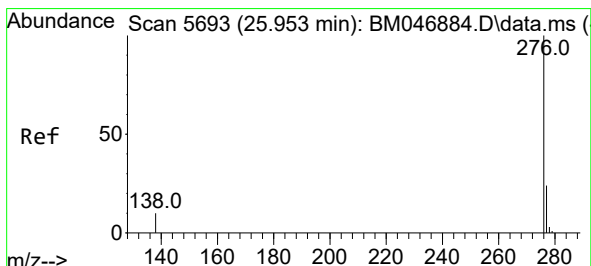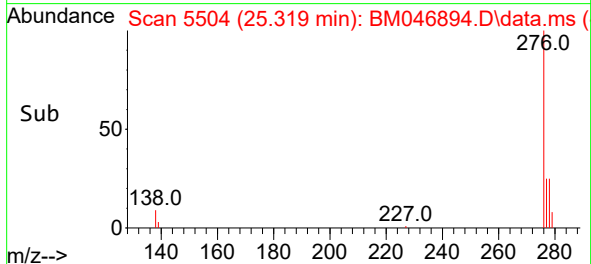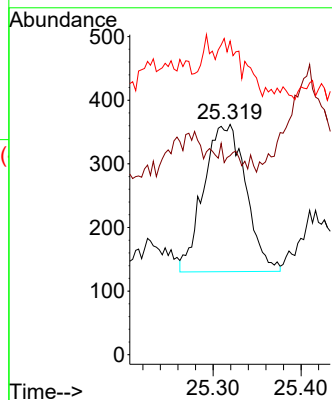

#29

Benzo(g,h,i)perylene

Concen: 0.077 ng/ul

RT: 25.950 min Scan# 5692

Delta R.T. -0.003 min

Lab File: BM046894.D

Acq: 29 Jul 2024 21:37

Tgt Ion:276 Resp: 2631

Ion Ratio Lower Upper

276 100

138 28.8 9.5 14.3#

277 39.5 20.9 31.3#

