




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072924\
Data File : BP021212.D
Acq On : 29 Jul 2024 16:21
Operator : MA/JU
Sample : P3301-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
F7E83

Manual IntegrationsAPPROVED

Quant Time: Jul 30 00:39:44 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jul 29 12:46:18 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/30/2024
Supervised By :mohammad ahmed 09/04/2024

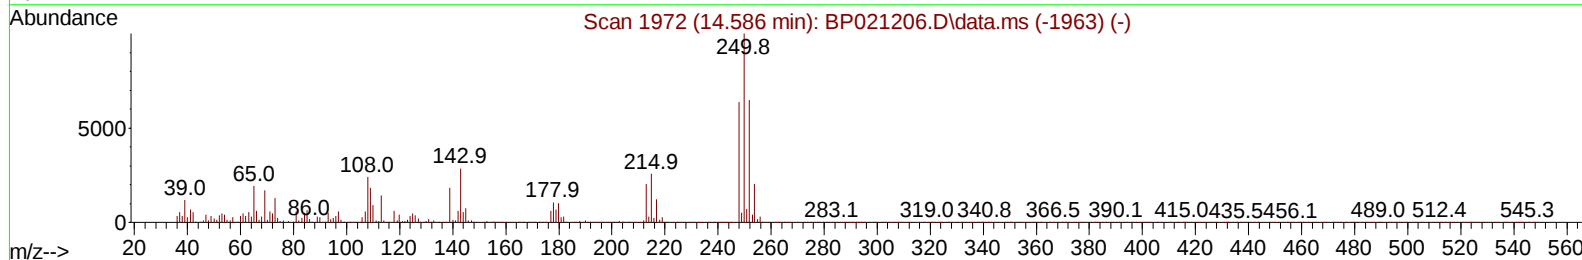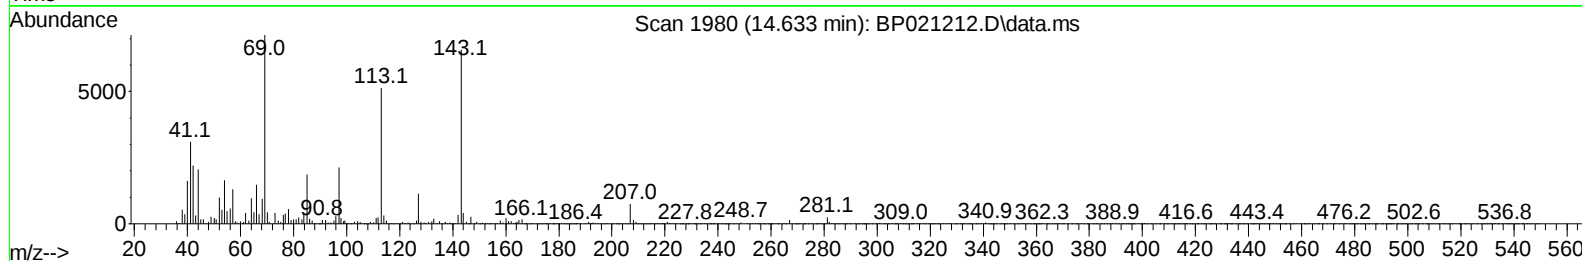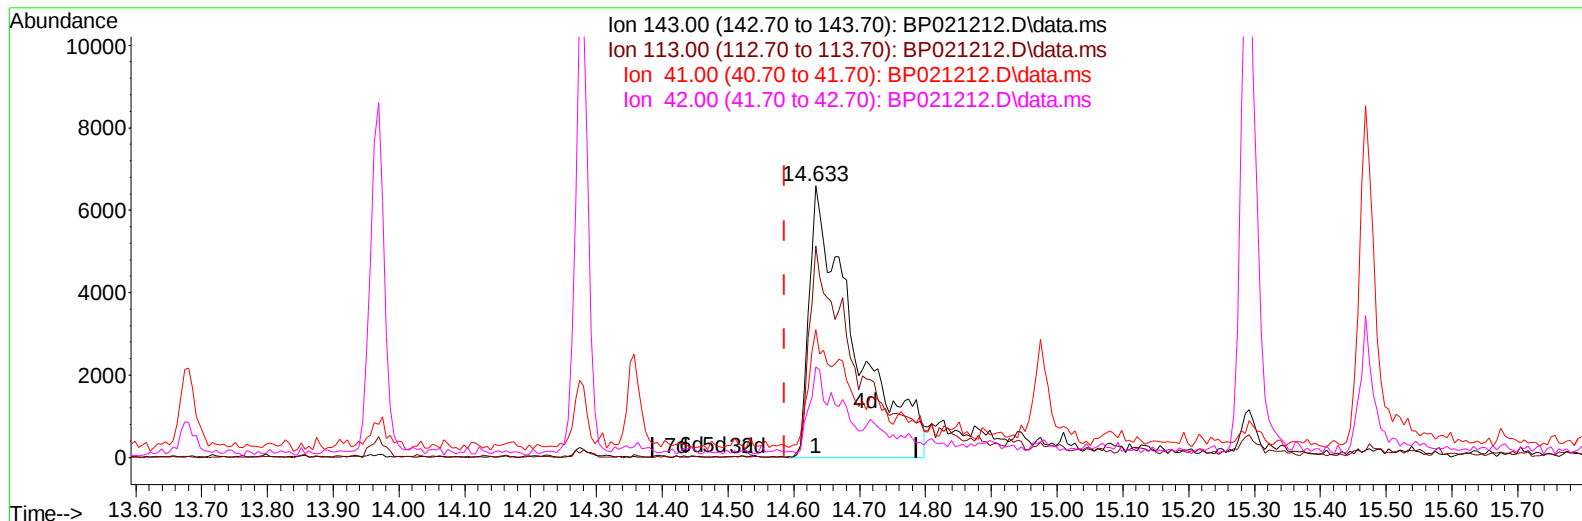

TIC: BP021212.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.633min (+ 0.047) 5.87 ng/ul m

response 31422

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	74.70	77.95
41.00	37.90	47.02#
42.00	27.10	33.42#

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072924\
 Data File : BP021212.D
 Acq On : 29 Jul 2024 16:21
 Operator : MA/JU
 Sample : P3301-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 F7E83

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 07/30/2024
 Supervised By :mohammad ahmed 09/04/2024

Quant Time: Jul 30 00:40:19 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jul 29 12:46:18 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.634	152	199297	20.000	ng/ul	0.00
20) Naphthalene-d8	10.404	136	809218	20.000	ng/ul	0.01
38) Acenaphthene-d10	14.280	164	517142	20.000	ng/ul	0.01
64) Phenanthrene-d10	17.092	188	1128336	20.000	ng/ul	0.00
79) Chrysene-d12	21.551	240	1153721	20.000	ng/ul	0.02
88) Perylene-d12	24.874	264	1376135	20.000	ng/ul	0.04
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.169	96	15706	3.586	ng/uL	0.00
4) Pyridine-d5	3.604	84	74464	5.873	ng/ul	0.01
7) Phenol-d5	6.869	99	99111	6.100	ng/ul	0.02
9) Bis-(2-Chloroethyl)eth...	6.987	67	234648	23.830	ng/ul	0.00
11) 2-Chlorophenol-d4	7.192	132	283837	21.202	ng/ul	0.01
15) 4-Methylphenol-d8	8.369	113	191036	14.156	ng/ul	0.00
21) Nitrobenzene-d5	8.792	128	149530	23.790	ng/ul	0.00
24) 2-Nitrophenol-d4	9.504	143	170485	23.699	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.063	165	277995	21.371	ng/ul	0.01
31) 4-Chloroaniline-d4	10.563	131	367590	21.331	ng/ul	0.00
46) Dimethylphthalate-d6	13.680	166	1003339	26.689	ng/ul	0.00
49) Acenaphthylene-d8	13.969	160	1060035	25.112	ng/ul	0.00
54) 4-Nitrophenol-d4	14.633	143	31422m	5.875	ng/ul	0.05
60) Fluorene-d10	15.292	176	868145	28.149	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.474	200	174599	25.575	ng/ul	0.01
73) Anthracene-d10	17.198	188	1543193	30.793	ng/ul	0.00
81) Pyrene-d10	19.592	212	1963181	27.523	ng/ul	0.02
92) Benzo(a)pyrene-d12	24.627	264	2233399	32.907	ng/ul	0.03

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072924\
Data File : BP021212.D
Acq On : 29 Jul 2024 16:21
Operator : MA/JU
Sample : P3301-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
F7E83

Manual IntegrationsAPPROVED

Quant Time: Jul 30 00:40:19 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jul 29 12:46:18 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/30/2024
Supervised By :mohammad ahmed 09/04/2024

