




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072924\
Data File : BP021229.D
Acq On : 30 Jul 2024 05:28
Operator : MA/JU
Sample : P3336-01
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
F7E87

Manual IntegrationsAPPROVED

Quant Time: Jul 30 05:53:27 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jul 29 12:46:18 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/30/2024
Supervised By :mohammad ahmed 09/04/2024

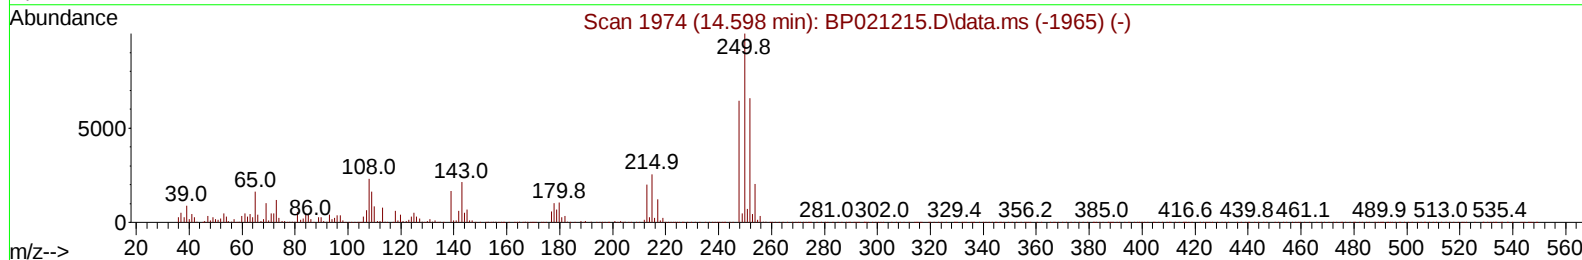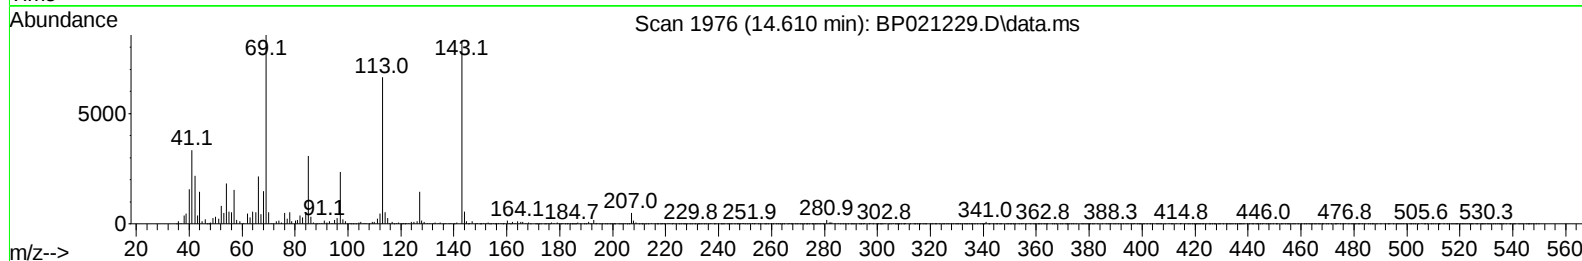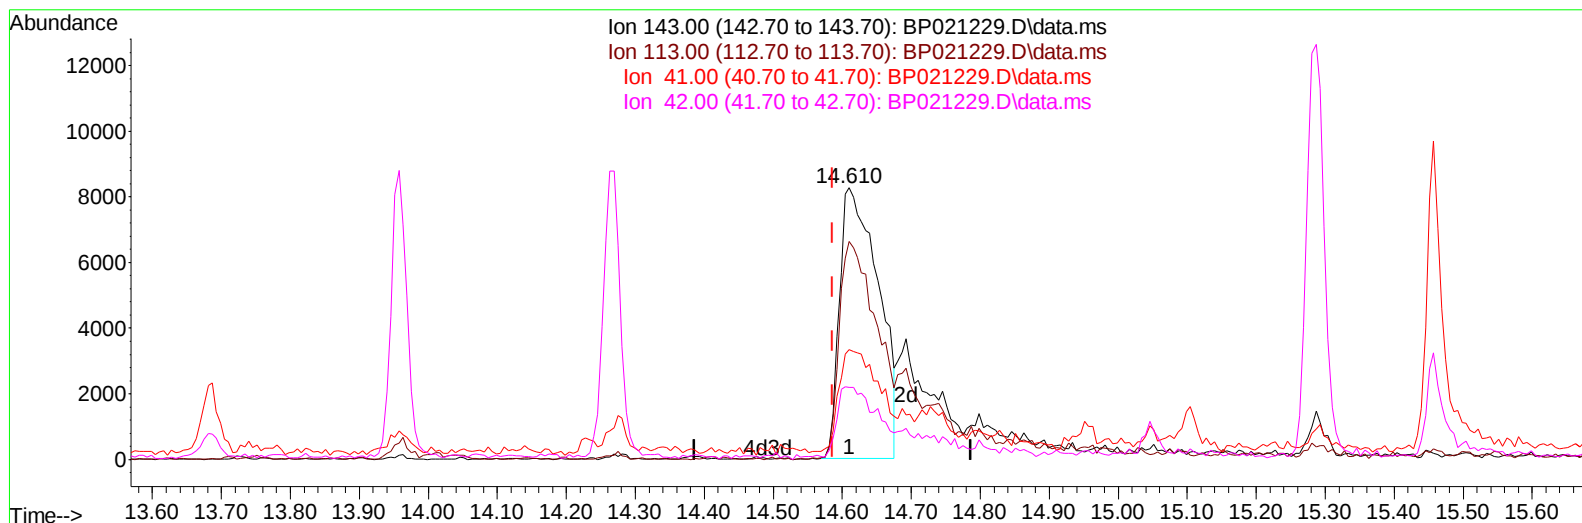

TIC: BP021229.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.610min (+ 0.024) 5.03 ng/u1

response 32167

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	74.70	80.27
41.00	37.90	40.47
42.00	27.10	26.48




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072924\
Data File : BP021229.D
Acq On : 30 Jul 2024 05:28
Operator : MA/JU
Sample : P3336-01
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
F7E87

Manual IntegrationsAPPROVED

Quant Time: Jul 30 05:53:27 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jul 29 12:46:18 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/30/2024
Supervised By :mohammad ahmed 09/04/2024

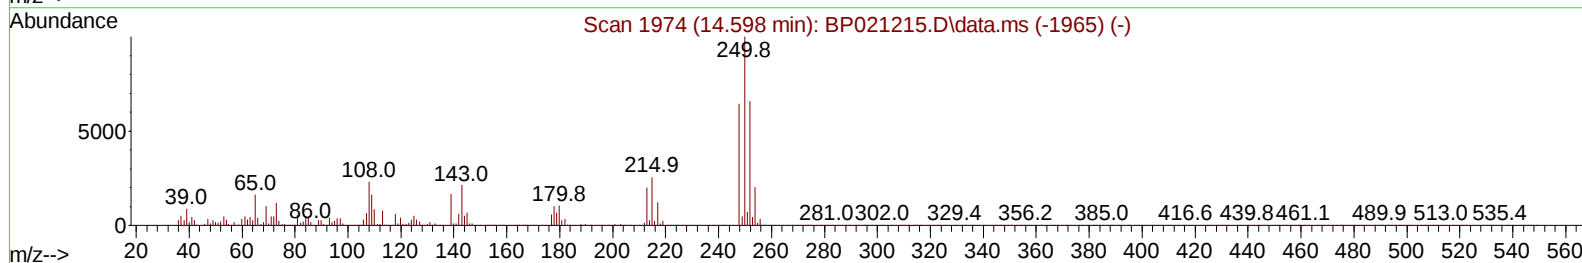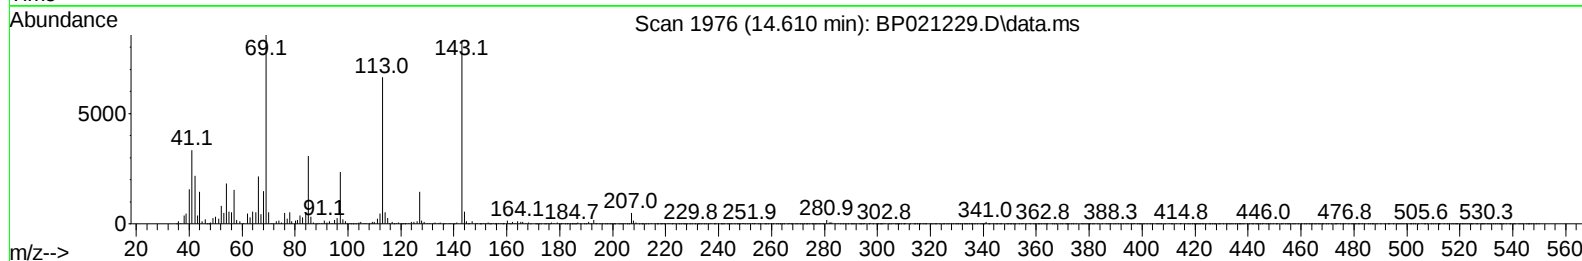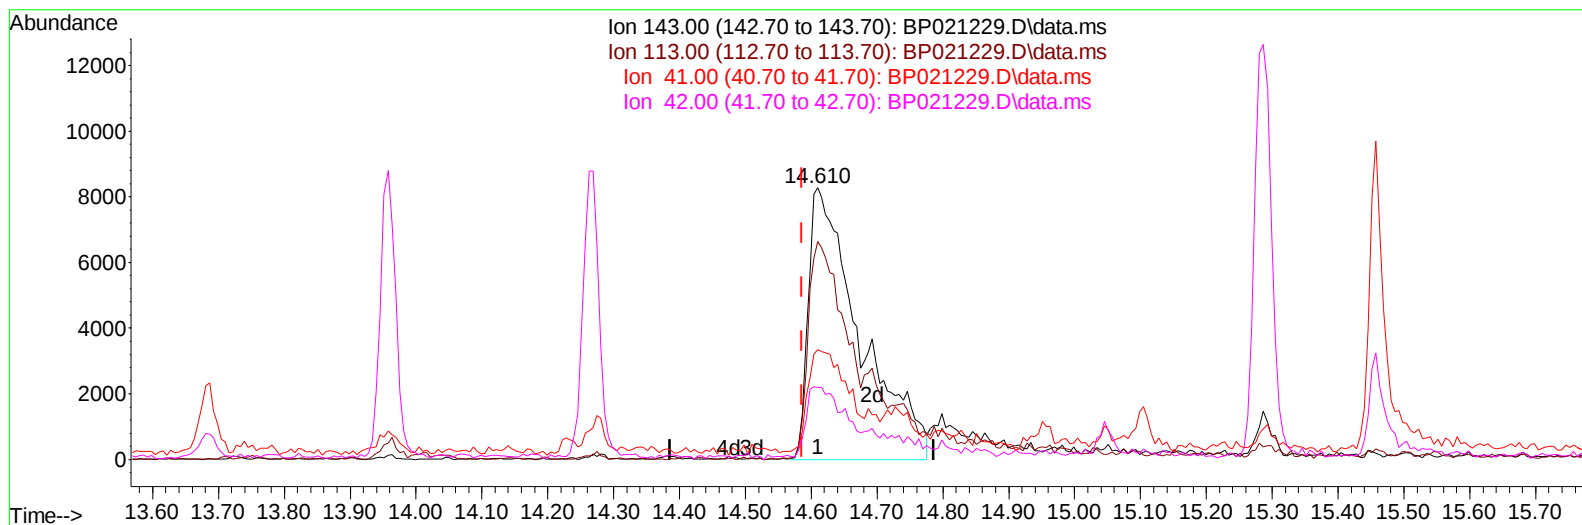

TIC: BP021229.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.610min (+ 0.024) 7.01 ng/ul m

response 44769

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	74.70	80.27
41.00	37.90	40.47
42.00	27.10	26.48

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072924\
 Data File : BP021229.D
 Acq On : 30 Jul 2024 05:28
 Operator : MA/JU
 Sample : P3336-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 F7E87

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 07/30/2024
 Supervised By :mohammad ahmed 09/04/2024

Quant Time: Jul 30 05:54:24 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jul 29 12:46:18 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.640	152	234772	20.000	ng/ul	0.00
20) Naphthalene-d8	10.393	136	934956	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.269	164	617906	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.087	188	1349814	20.000	ng/ul	0.00
79) Chrysene-d12	21.533	240	1412245	20.000	ng/ul	0.00
88) Perylene-d12	24.827	264	1727194	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.175	96	20915	4.054	ng/uL	0.00
4) Pyridine-d5	3.599	84	76791	5.141	ng/ul	0.00
7) Phenol-d5	6.858	99	124668	6.513	ng/ul	0.01
9) Bis-(2-Chloroethyl)eth...	6.987	67	260260	22.437	ng/ul	0.00
11) 2-Chlorophenol-d4	7.187	132	356014	22.575	ng/ul	0.00
15) 4-Methylphenol-d8	8.369	113	230084	14.473	ng/ul	0.00
21) Nitrobenzene-d5	8.793	128	190037	26.169	ng/ul	0.00
24) 2-Nitrophenol-d4	9.505	143	216676	26.069	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.052	165	363468	24.184	ng/ul	0.00
31) 4-Chloroaniline-d4	10.563	131	319763	16.060	ng/ul	0.00
46) Dimethylphthalate-d6	13.687	166	1276884	28.427	ng/ul	0.00
49) Acenaphthylene-d8	13.957	160	1368055	27.124	ng/ul	0.00
54) 4-Nitrophenol-d4	14.610	143	44769m	7.005	ng/ul	0.02
60) Fluorene-d10	15.287	176	1095423	29.726	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.457	200	243397	29.802	ng/ul	0.00
73) Anthracene-d10	17.192	188	1965120	32.778	ng/ul	0.00
81) Pyrene-d10	19.581	212	2480492	28.410	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.598	264	2958942	34.735	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072924\
Data File : BP021229.D
Acq On : 30 Jul 2024 05:28
Operator : MA/JU
Sample : P3336-01
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
F7E87

Manual IntegrationsAPPROVED

Quant Time: Jul 30 05:54:24 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jul 29 12:46:18 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/30/2024
Supervised By :mohammad ahmed 09/04/2024

