




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072924\
Data File : BP021242.D
Acq On : 30 Jul 2024 19:58
Operator : MA/JU
Sample : P3347-05
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AY9

Manual IntegrationsAPPROVED

Quant Time: Jul 30 22:55:20 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jul 29 12:46:18 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/31/2024
Supervised By :mohammad ahmed 09/04/2024

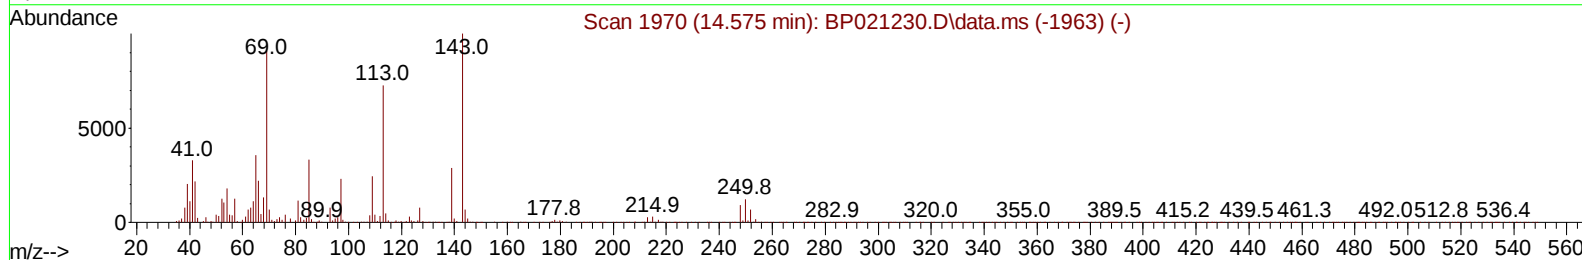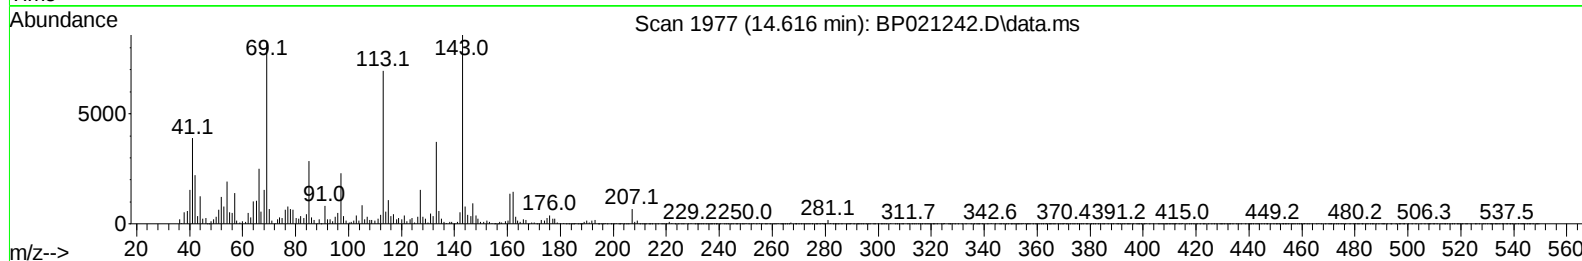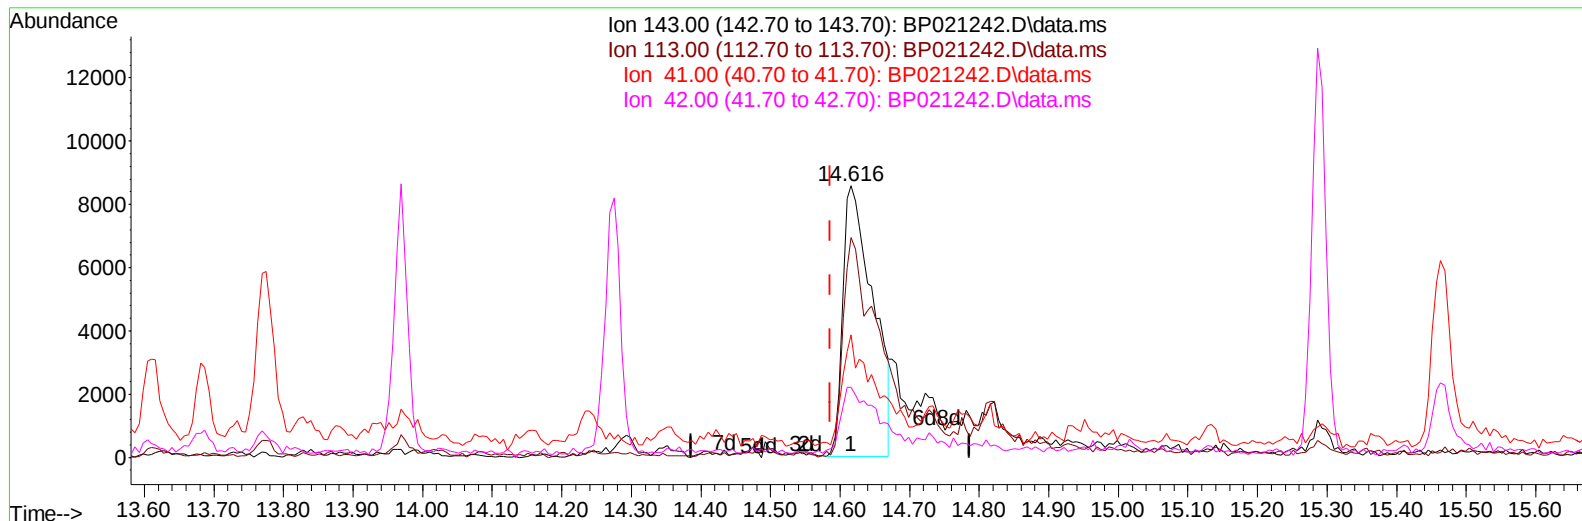

TIC: BP021242.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.616min (+ 0.030) 5.01 ng/u1

response 25589

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	74.70	80.94
41.00	37.90	45.28
42.00	27.10	25.93




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072924\
Data File : BP021242.D
Acq On : 30 Jul 2024 19:58
Operator : MA/JU
Sample : P3347-05
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AY9

Manual IntegrationsAPPROVED

Quant Time: Jul 30 22:55:20 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jul 29 12:46:18 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/31/2024
Supervised By :mohammad ahmed 09/04/2024

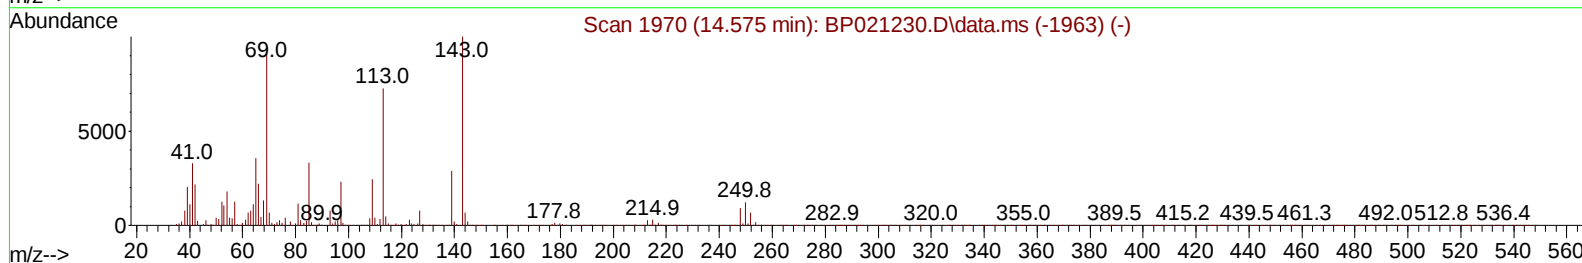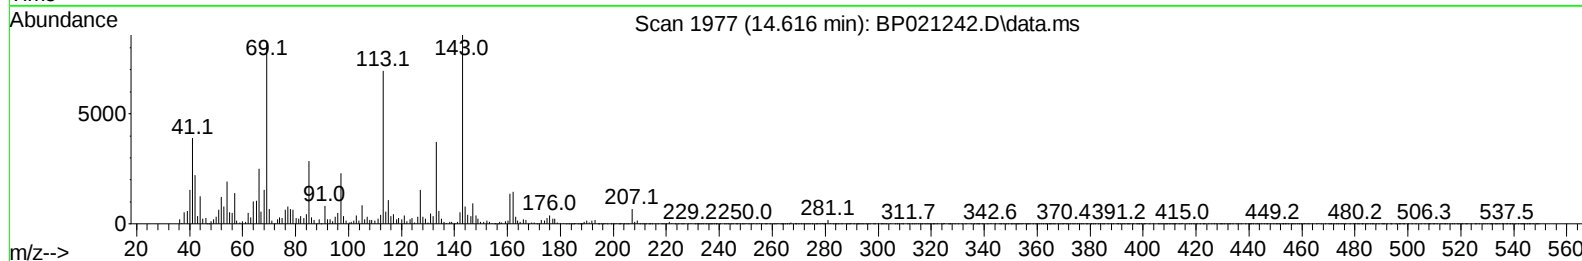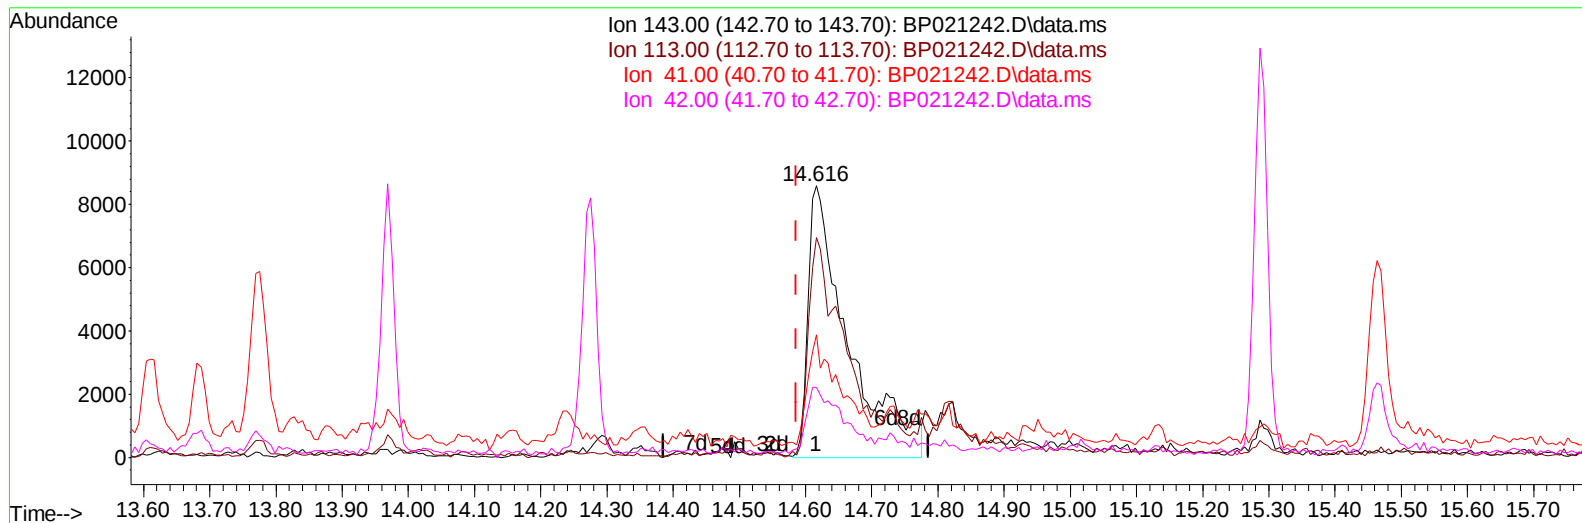

TIC: BP021242.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.616min (+ 0.030) 7.10 ng/ul m

response 36272

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	74.70	80.94
41.00	37.90	45.28
42.00	27.10	25.93

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072924\
 Data File : BP021242.D
 Acq On : 30 Jul 2024 19:58
 Operator : MA/JU
 Sample : P3347-05
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AY9

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 07/31/2024
 Supervised By :mohammad ahmed 09/04/2024

Quant Time: Jul 30 23:29:55 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jul 29 12:46:18 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.622	152	181958	20.000	ng/ul	-0.01
20) Naphthalene-d8	10.393	136	725795	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.275	164	493598	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.092	188	1106767	20.000	ng/ul	0.00
79) Chrysene-d12	21.539	240	1264226	20.000	ng/ul	0.00
88) Perylene-d12	24.845	264	1395369	20.000	ng/ul	0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.170	96	13585	3.397	ng/uL	0.00
4) Pyridine-d5	3.593	84	81087	7.005	ng/ul	0.00
7) Phenol-d5	6.852	99	147259	9.927	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.975	67	206412	22.960	ng/ul	0.00
11) 2-Chlorophenol-d4	7.181	132	293697	24.029	ng/ul	0.00
15) 4-Methylphenol-d8	8.358	113	237551	19.280	ng/ul	0.00
21) Nitrobenzene-d5	8.787	128	147875	26.231	ng/ul	0.00
24) 2-Nitrophenol-d4	9.499	143	169805	26.317	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.057	165	302884	25.960	ng/ul	0.00
31) 4-Chloroaniline-d4	10.557	131	332339	21.502	ng/ul	0.00
46) Dimethylphthalate-d6	13.681	166	1028588	28.666	ng/ul	0.00
49) Acenaphthylene-d8	13.969	160	1103564	27.390	ng/ul	0.00
54) 4-Nitrophenol-d4	14.616	143	36272m	7.105	ng/ul	0.03
60) Fluorene-d10	15.287	176	883979	30.029	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.469	200	171321	25.584	ng/ul	0.00
73) Anthracene-d10	17.192	188	1478827	30.084	ng/ul	0.00
81) Pyrene-d10	19.581	212	1954693	25.009	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.610	264	2101489	30.536	ng/ul	0.01

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072924\
Data File : BP021242.D
Acq On : 30 Jul 2024 19:58
Operator : MA/JU
Sample : P3347-05
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AY9

Manual IntegrationsAPPROVED

Quant Time: Jul 30 23:29:55 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jul 29 12:46:18 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/31/2024
Supervised By :mohammad ahmed 09/04/2024

